

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030723\
 Data File : BM038916.D
 Acq On : 08 Mar 2023 04:25
 Operator : CG/JU
 Sample : PB151197BL
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK197

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022823.M
 Title : SVOA CALIBRATION

Signal : TIC: BM038916.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.375	11	15	27	rVB	66606	112133	1.52%	0.152%
2	3.799	84	87	115	rBV	889163	1512892	20.52%	2.051%
3	4.140	141	145	150	rBV	21157	34532	0.47%	0.047%
4	7.151	650	657	672	rVB	1164382	1802700	24.45%	2.443%
5	7.328	680	687	695	rBV	950648	1518538	20.60%	2.058%
6	7.528	713	721	731	rBV	1141432	1823218	24.73%	2.471%
7	7.998	794	801	810	rBV	1044938	1661479	22.54%	2.252%
8	8.704	913	921	935	rBV	1453645	2259009	30.64%	3.062%
9	9.163	992	999	1009	rBV	1101149	1772965	24.05%	2.403%
10	9.892	1112	1123	1130	rBV	831516	1373588	18.63%	1.862%
11	10.428	1205	1214	1225	rBV	1402659	2245707	30.46%	3.044%
12	10.816	1272	1280	1291	rVB	1529471	2518675	34.16%	3.414%
13	10.945	1291	1302	1318	rBV	1467278	2458096	33.34%	3.332%
14	12.398	1543	1549	1557	rVB2	22826	40699	0.55%	0.055%
15	14.045	1822	1829	1839	rBV	2583533	3404925	46.18%	4.615%
16	14.327	1871	1877	1885	rBV	2848856	4109128	55.74%	5.570%
17	14.633	1923	1929	1940	rBV	2261645	3383654	45.90%	4.586%
18	14.816	1953	1960	1973	rBV	1293888	1822204	24.72%	2.470%
19	15.045	1996	1999	2005	rVB8	10208	11553	0.16%	0.016%
20	15.627	2091	2098	2108	rBV	3699567	5155029	69.92%	6.987%
21	15.733	2110	2116	2128	rBV	991525	1302413	17.67%	1.765%
22	15.868	2134	2139	2144	rVB4	16911	27160	0.37%	0.037%
23	17.057	2336	2341	2344	rBV7	6426	9385	0.13%	0.013%
24	17.162	2355	2359	2362	rBV4	4391	7744	0.11%	0.010%
25	17.380	2389	2396	2405	rBV	2866358	4009913	54.39%	5.435%
26	17.474	2406	2412	2428	rBV	3920796	5637225	76.46%	7.641%
27	19.333	2724	2728	2732	rBV3	43259	58787	0.80%	0.080%
28	19.398	2735	2739	2744	rBV2	44811	65260	0.89%	0.088%
29	19.762	2795	2801	2809	rBV	5099004	6817706	92.48%	9.241%
30	21.556	3100	3106	3116	rBV	3297539	4491954	60.93%	6.088%
31	23.844	3488	3495	3503	rBV2	3825345	7372373	100.00%	9.993%
32	24.003	3515	3522	3534	rVB2	2425995	4957197	67.24%	6.719%




Sum of corrected areas: 73777841

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030723\
Data File : BM038916.D
Acq On : 08 Mar 2023 04:25
Operator : CG/JU
Sample : PB151197BL
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK197

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

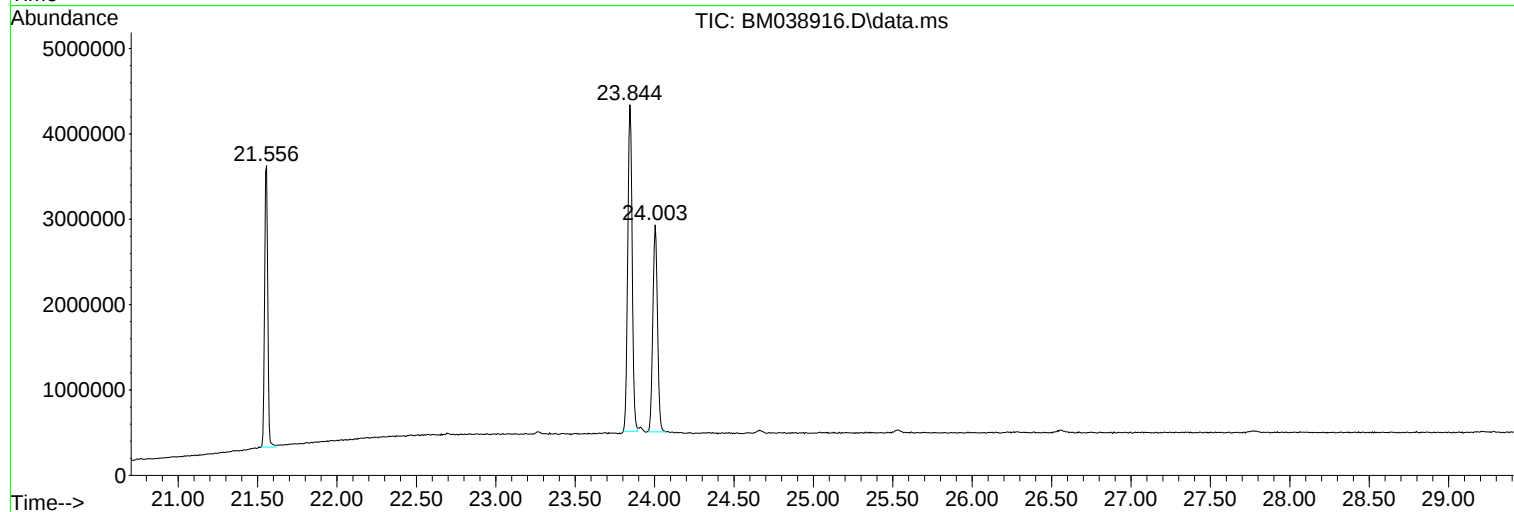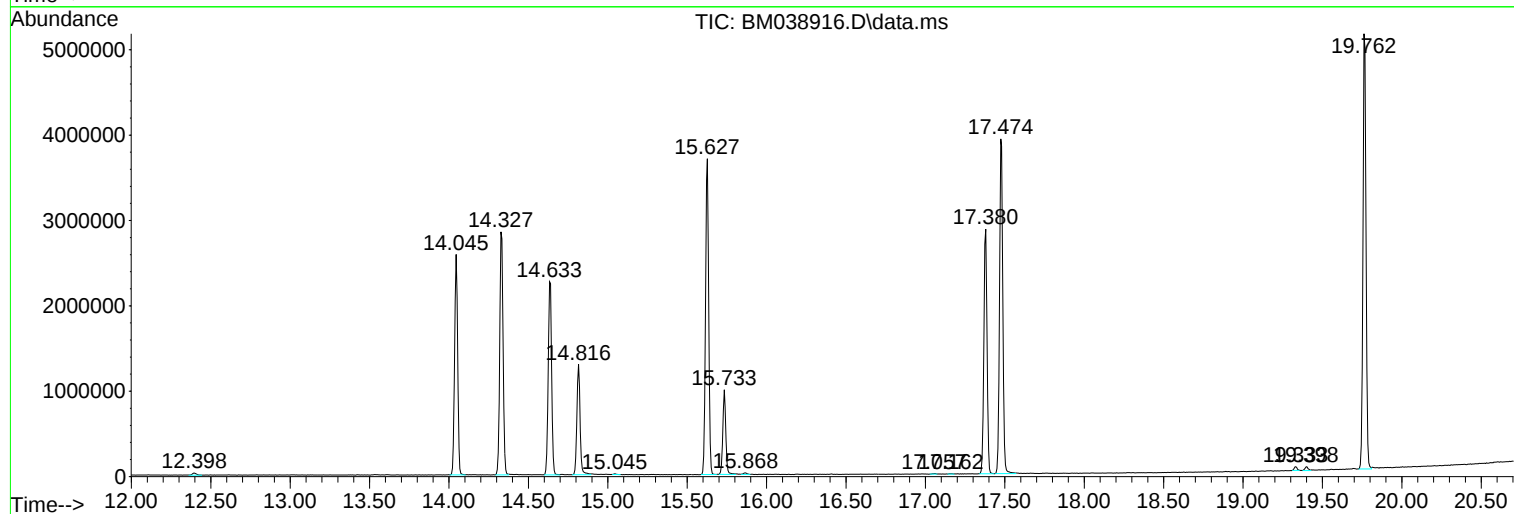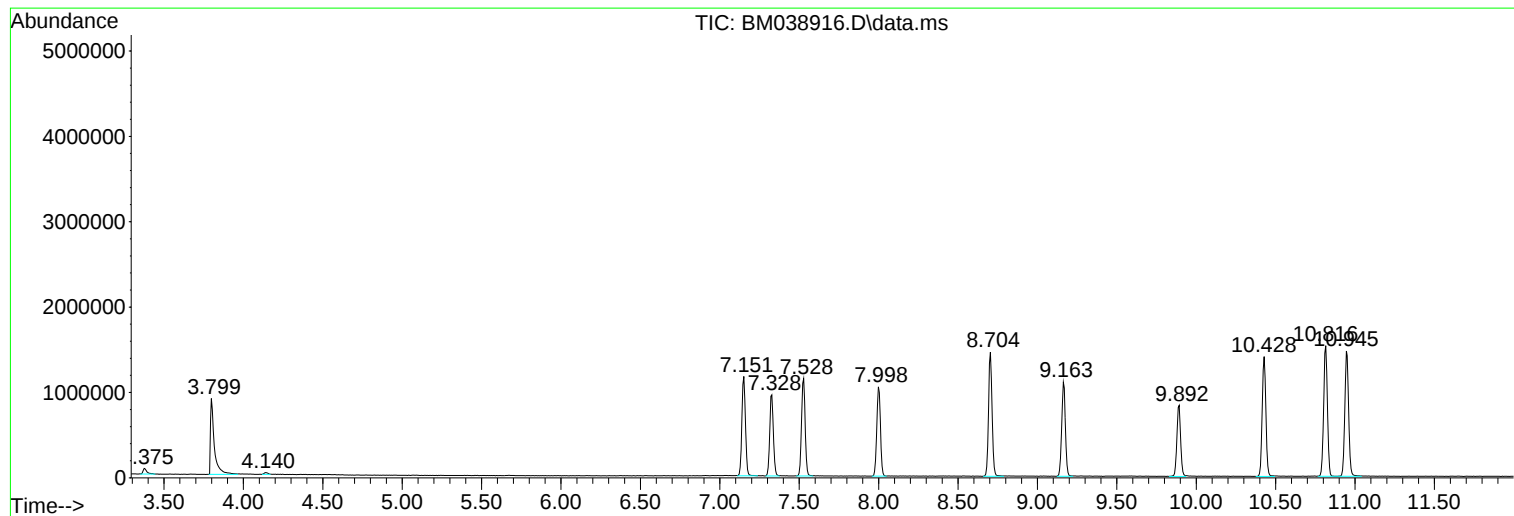

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030723\
Data File : BM038916.D
Acq On : 08 Mar 2023 04:25
Operator : CG/JU
Sample : PB151197BL
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK197

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030723\
Data File : BM038916.D
Acq On : 08 Mar 2023 04:25
Operator : CG/JU
Sample : PB151197BL
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK197

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc