

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030723\
 Data File : BM038921.D
 Acq On : 08 Mar 2023 07:30
 Operator : CG/JU
 Sample : 01746-15
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DCAF1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022823.M
 Title : SVOA CALIBRATION

Signal : TIC: BM038921.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.375	12	15	22	rBV	60572	84493	0.77%	0.094%
2	3.663	62	64	74	rVB8	10735	27703	0.25%	0.031%
3	3.804	87	88	97	rBV	163888	248114	2.26%	0.276%
4	4.046	124	129	134	rBV	33749	56107	0.51%	0.062%
5	4.140	142	145	152	rVB	21456	31788	0.29%	0.035%
6	4.246	159	163	169	rVB4	21090	33357	0.30%	0.037%
7	5.075	299	304	312	rVB	17208	31002	0.28%	0.034%
8	6.375	519	525	529	rBV3	20443	34411	0.31%	0.038%
9	7.151	650	657	667	rVB	282201	457271	4.16%	0.508%
10	7.322	680	686	696	rVB	1212614	1916791	17.43%	2.132%
11	7.522	713	720	731	rBV	1071509	1722178	15.66%	1.915%
12	7.998	792	801	810	rBV	1144511	1799748	16.37%	2.001%
13	8.704	914	921	932	rBV	837703	1350522	12.28%	1.502%
14	9.163	991	999	1012	rBV	1451866	2326042	21.15%	2.587%
15	9.275	1012	1018	1024	rBV	81152	129660	1.18%	0.144%
16	9.592	1066	1072	1078	rVB5	12441	21687	0.20%	0.024%
17	9.886	1112	1122	1136	rBV	1069224	1771583	16.11%	1.970%
18	10.428	1206	1214	1227	rBV	1621978	2609063	23.73%	2.901%
19	10.816	1272	1280	1289	rVB	1656824	2772391	25.21%	3.083%
20	10.945	1293	1302	1312	rBV	1507952	2526398	22.97%	2.809%
21	11.592	1406	1412	1416	rBV6	15707	30472	0.28%	0.034%
22	12.092	1491	1497	1502	rBV2	13789	20245	0.18%	0.023%
23	12.398	1539	1549	1556	rVB	32229	54627	0.50%	0.061%
24	13.533	1739	1742	1747	rVB7	7634	11487	0.10%	0.013%
25	13.610	1747	1755	1758	rBV8	5515	11121	0.10%	0.012%
26	14.045	1822	1829	1846	rBV	3574857	4669799	42.46%	5.193%
27	14.327	1870	1877	1884	rBV	3897626	5575784	50.70%	6.200%
28	14.633	1922	1929	1938	rBV	2595739	3803840	34.59%	4.230%
29	14.815	1954	1960	1973	rBV	286784	452278	4.11%	0.503%
30	15.004	1987	1992	1995	rVV4	10503	15198	0.14%	0.017%
31	15.045	1995	1999	2004	rVB6	24656	34250	0.31%	0.038%
32	15.445	2061	2067	2072	rBV5	8519	16512	0.15%	0.018%
33	15.627	2091	2098	2110	rBV	5030718	7269680	66.11%	8.084%
34	15.733	2110	2116	2126	rBV	1602741	2095407	19.05%	2.330%
35	15.862	2134	2138	2144	rVB2	26889	41580	0.38%	0.046%
36	15.986	2154	2159	2166	rBV	265700	357340	3.25%	0.397%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030723\
 Data File : BM038921.D
 Acq On : 08 Mar 2023 07:30
 Operator : CG/JU
 Sample : 01746-15
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DCAF1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022823.M
 Title : SVOA CALIBRATION

37	16.409	2228	2231	2236	rVB7	6923	11229	0.10%	0.012%
38	16.562	2253	2257	2263	rVB9	6501	13604	0.12%	0.015%
39	17.051	2338	2340	2345	rBV5	7969	13200	0.12%	0.015%
40	17.298	2378	2382	2385	rBV6	8235	12397	0.11%	0.014%
41	17.380	2389	2396	2405	rBV	3155227	4514375	41.05%	5.020%
42	17.480	2406	2413	2423	rBV	6016982	8563754	77.87%	9.523%
43	18.045	2507	2509	2515	rVB6	15244	18926	0.17%	0.021%
44	18.268	2543	2547	2553	rBV	80297	110536	1.01%	0.123%
45	18.345	2557	2560	2564	rVV	23886	30212	0.27%	0.034%
46	19.333	2723	2728	2734	rBV	77072	120453	1.10%	0.134%
47	19.398	2735	2739	2742	rBV	65175	87952	0.80%	0.098%
48	19.545	2761	2764	2770	rBV5	39943	49488	0.45%	0.055%
49	19.768	2796	2802	2809	rBV	7774820	10173319	92.51%	11.313%
50	21.262	3054	3056	3063	rVB5	74896	88417	0.80%	0.098%
51	21.556	3101	3106	3114	rBV	4041214	5112928	46.49%	5.686%
52	23.850	3488	3496	3504	rBV2	5551741	10997075	100.00%	12.229%
53	24.009	3516	3523	3536	rVB2	2734515	5598671	50.91%	6.226%




Sum of corrected areas: 89926465

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030723\
Data File : BM038921.D
Acq On : 08 Mar 2023 07:30
Operator : CG/JU
Sample : 01746-15
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DCAF1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

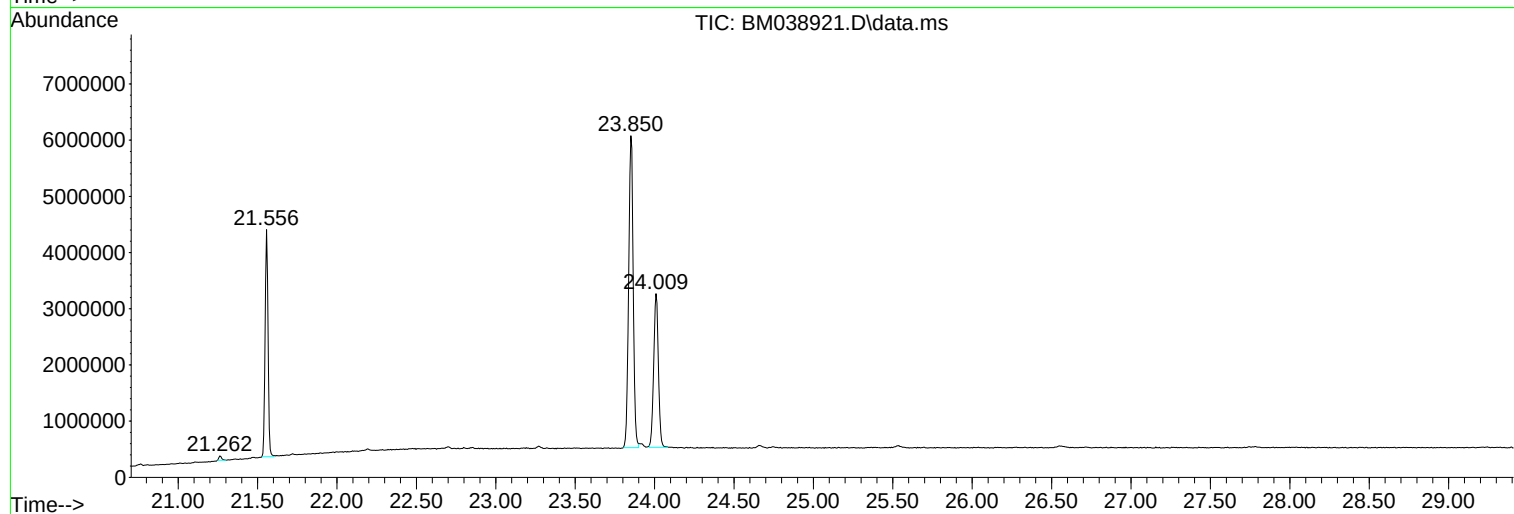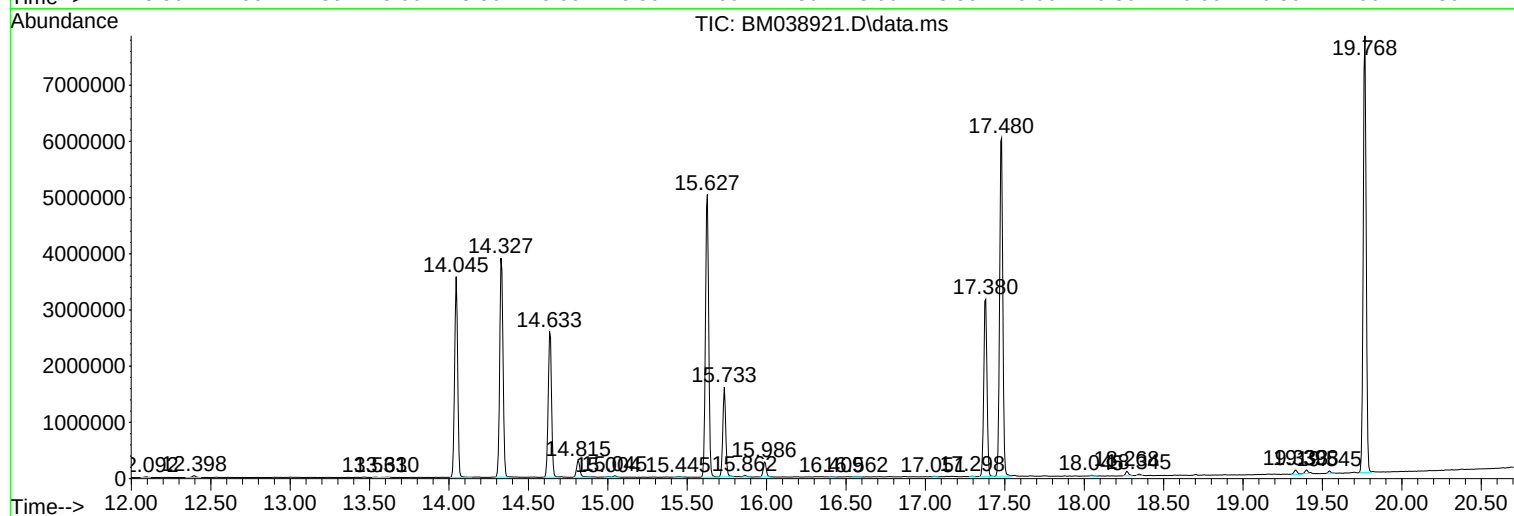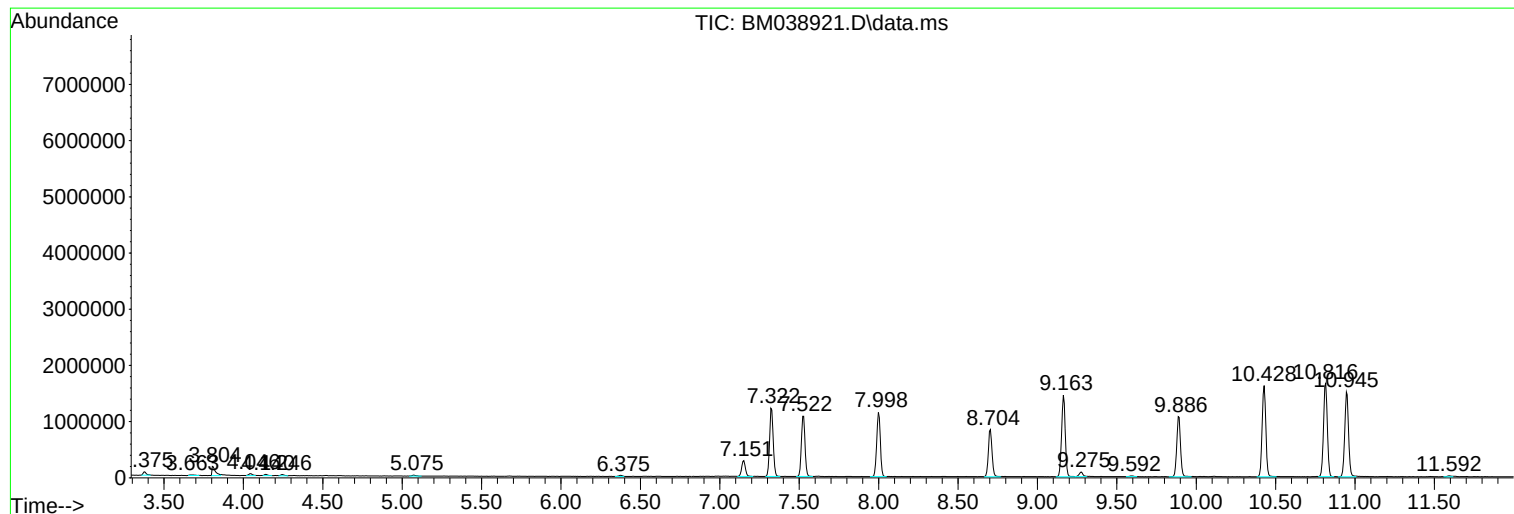

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030723\
Data File : BM038921.D
Acq On : 08 Mar 2023 07:30
Operator : CG/JU
Sample : 01746-15
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DCAF1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030723\
Data File : BM038921.D
Acq On : 08 Mar 2023 07:30
Operator : CG/JU
Sample : 01746-15
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DCAF1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc