

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030723\
 Data File : BM038922.D
 Acq On : 08 Mar 2023 08:07
 Operator : CG/JU
 Sample : 01746-04
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DCAC8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022823.M
 Title : SVOA CALIBRATION

Signal : TIC: BM038922.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.375	12	15	30	rVB	64287	99831	1.00%	0.113%
2	3.669	60	65	70	rBV7	9068	21602	0.22%	0.024%
3	3.804	85	88	105	rBV	287379	501323	5.04%	0.568%
4	4.046	124	129	136	rVB	31285	51739	0.52%	0.059%
5	4.140	141	145	153	rVB2	22185	37961	0.38%	0.043%
6	4.246	159	163	171	rVB4	19975	34641	0.35%	0.039%
7	5.075	298	304	308	rBV4	16631	30936	0.31%	0.035%
8	6.375	520	525	531	rBV2	18407	32456	0.33%	0.037%
9	7.151	650	657	668	rVB	270652	437292	4.40%	0.495%
10	7.322	680	686	695	rVB	1216272	1893659	19.05%	2.144%
11	7.528	713	721	730	rBV	1058209	1698540	17.09%	1.923%
12	7.998	791	801	809	rBV	1269913	1964257	19.76%	2.224%
13	8.704	913	921	933	rBV	831606	1310953	13.19%	1.484%
14	9.163	991	999	1008	rBV	1404777	2284169	22.98%	2.586%
15	9.269	1011	1017	1025	rBV	49982	86936	0.87%	0.098%
16	9.592	1065	1072	1077	rVB5	7996	17185	0.17%	0.019%
17	9.886	1113	1122	1131	rBV	1046913	1745784	17.56%	1.976%
18	10.428	1205	1214	1223	rBV	1595755	2614915	26.31%	2.960%
19	10.816	1271	1280	1287	rBV	1816231	3027835	30.46%	3.428%
20	10.945	1295	1302	1312	rBV	1617459	2644904	26.61%	2.994%
21	11.598	1406	1413	1418	rBV7	8698	20590	0.21%	0.023%
22	12.092	1491	1497	1501	rBV4	8033	13309	0.13%	0.015%
23	12.392	1543	1548	1556	rVB	30981	51717	0.52%	0.059%
24	12.533	1567	1572	1579	rVB	20553	33952	0.34%	0.038%
25	13.539	1737	1743	1747	rVV5	11414	17616	0.18%	0.020%
26	13.604	1751	1754	1763	rVB8	5964	12640	0.13%	0.014%
27	14.045	1822	1829	1843	rBV	3394236	4475925	45.03%	5.067%
28	14.327	1870	1877	1893	rBV	3837163	5481574	55.15%	6.205%
29	14.633	1922	1929	1937	rBV	2775783	4098763	41.24%	4.640%
30	14.816	1953	1960	1973	rBV	249517	392146	3.95%	0.444%
31	15.045	1994	1999	2003	rBV7	20337	29007	0.29%	0.033%
32	15.433	2061	2065	2071	rBV2	10534	18609	0.19%	0.021%
33	15.627	2091	2098	2109	rBV	5038668	7005536	70.48%	7.930%
34	15.733	2109	2116	2131	rVV	1532386	2008828	20.21%	2.274%
35	15.862	2134	2138	2148	rVB2	26325	48224	0.49%	0.055%
36	16.174	2187	2191	2198	rBV8	13303	23352	0.23%	0.026%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030723\
 Data File : BM038922.D
 Acq On : 08 Mar 2023 08:07
 Operator : CG/JU
 Sample : 01746-04
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DCAC8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022823.M
 Title : SVOA CALIBRATION

37	17.015	2329	2334	2338	rBV3	34016	52021	0.52%	0.059%
38	17.380	2389	2396	2404	rBV	3539256	4846417	48.76%	5.486%
39	17.480	2406	2413	2424	rBV	5738219	8166851	82.17%	9.245%
40	18.268	2543	2547	2554	rBV3	38472	58715	0.59%	0.066%
41	18.345	2557	2560	2564	rVB	17567	21921	0.22%	0.025%
42	18.703	2618	2621	2626	rVB7	15862	16982	0.17%	0.019%
43	19.333	2724	2728	2732	rBV2	65333	83088	0.84%	0.094%
44	19.398	2735	2739	2743	rBV	67356	90532	0.91%	0.102%
45	19.545	2761	2764	2771	rBV6	28680	41044	0.41%	0.046%
46	19.768	2796	2802	2809	rBV	7561049	9617820	96.76%	10.888%
47	21.556	3101	3106	3114	rBV	4136667	5361710	53.94%	6.070%
48	23.850	3489	3496	3505	rBV2	4989848	9939453	100.00%	11.252%
49	24.009	3516	3523	3534	rVB2	2880401	5771577	58.07%	6.534%




Sum of corrected areas: 88336837

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030723\
Data File : BM038922.D
Acq On : 08 Mar 2023 08:07
Operator : CG/JU
Sample : 01746-04
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DCAC8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

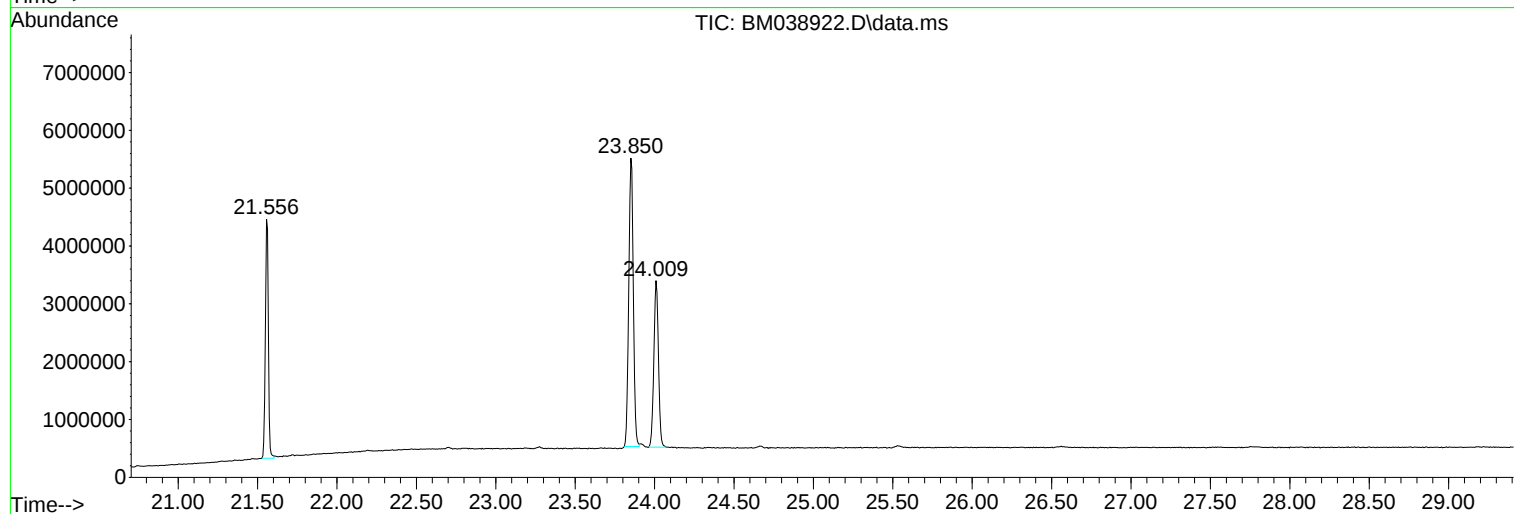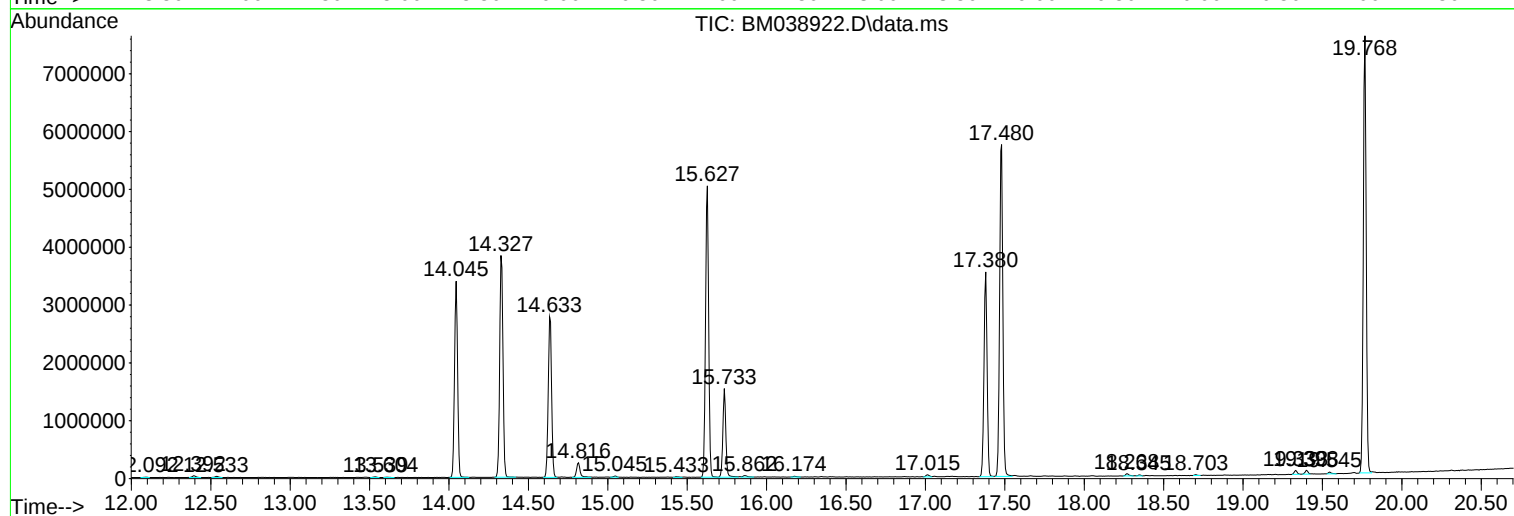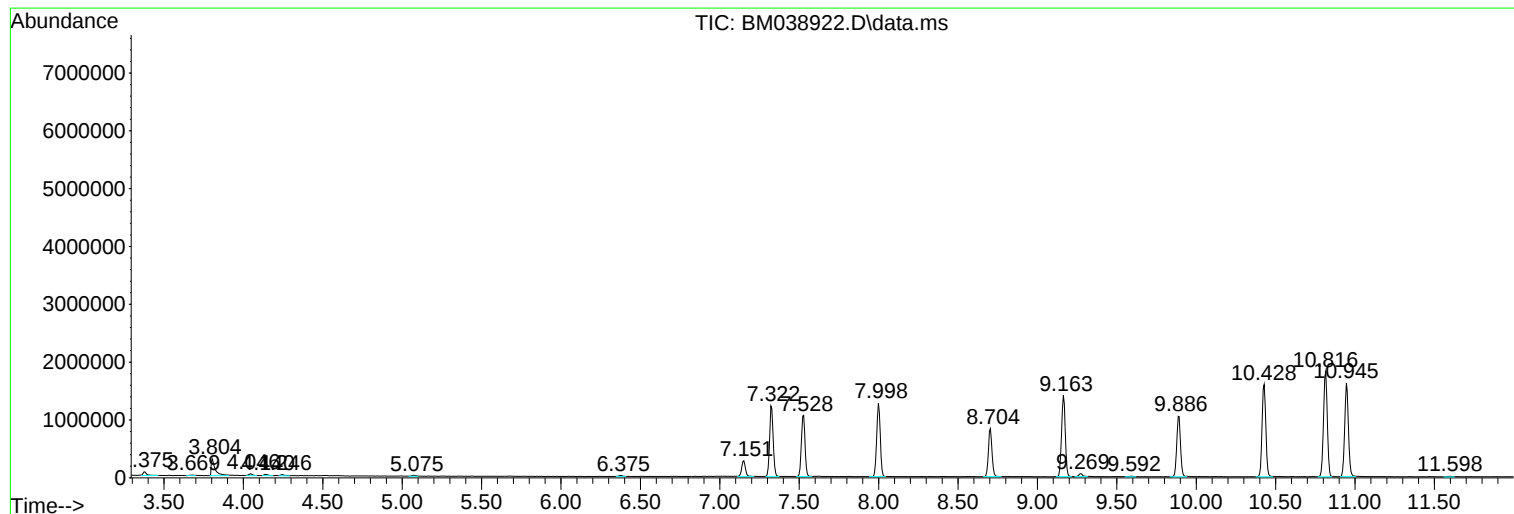

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030723\
Data File : BM038922.D
Acq On : 08 Mar 2023 08:07
Operator : CG/JU
Sample : 01746-04
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DCAC8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030723\
Data File : BM038922.D
Acq On : 08 Mar 2023 08:07
Operator : CG/JU
Sample : 01746-04
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DCAC8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc