

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM030816\
 Data File : BM004575.D
 Acq On : 08 Mar 2016 11:33
 Operator : SJ/UM
 Sample : SSTDICC0.8
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SSTDICC0.8

Quant Time: Mar 08 14:08:49 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\8270-SIM-BM030816.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Mar 08 13:49:28 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.29	152	37107	5.00	ng	-0.02
6) Naphthalene-d8	10.05	136	139569	5.00	ng	-0.02
10) Acenaphthene-d10	13.96	164	81696	5.00	ng	-0.02
16) Phenanthrene-d10	16.74	188	162919	5.00	ng	0.00
22) Chrysene-d12	20.97	240	157246	5.00	ng	-0.01
28) Perylene-d12	23.08	264	125970	5.00	ng	0.00

System Monitoring Compounds						
4) 2-Fluorophenol	5.04	112	5081	0.59	ng	-0.05
5) Phenol-d6	6.64	99	6531	0.67	ng	-0.03
7) Nitrobenzene-d5	8.49	82	5069	0.71	ng	-0.02
11) 2,4,6-Tribromophenol	15.51	330	1702	0.54	ng	-0.01
12) 2-Fluorobiphenyl	12.59	172	19361	0.77	ng	-0.01
24) Terphenyl-d14	19.42	244	15184	0.75	ng	0.00


Target Compounds				Qvalue		
2) 1,4-Dioxane	2.87	88	2711	0.63	ng	94
3) n-Nitrosodimethylamine	3.20	42	2380	0.63	ng	# 98
8) Naphthalene	10.10	128	31815	0.72	ng	100
9) 2-Methylnaphthalene	11.75	142	20220	0.83	ng	97
13) Acenaphthylene	13.69	152	34169	0.73	ng	# 71
14) Acenaphthene	14.02	154	23778	0.78	ng	98
15) Fluorene	15.05	166	27941	0.75	ng	99
17) Hexachlorobenzene	16.05	284	8176	0.81	ng	# 70
18) Pentachlorophenol	16.48	266	400	0.16	ng	93
19) Phenanthrene	16.76	178	45229	0.79	ng	98
20) Anthracene	16.87	178	38862	0.80	ng	97
21) Fluoranthene	18.82	202	46971	0.76	ng	99
23) Pyrene	19.20	202	48382	0.78	ng	99
25) Benzo(a)anthracene	20.95	228	45430	0.78	ng	97
26) Chrysene	21.01	228	38037	0.32	ng	96
27) Indeno(1,2,3-cd)pyrene	25.16	276	34995	0.65	ng	99
29) Benzo(b)fluoranthene	22.47	252	73834	1.50	ng	# 57
30) Benzo(k)fluoranthene	22.47	252	75108	1.55	ng	# 57
31) Benzo(a)pyrene	22.98	252	34658	0.78	ng	99
32) Dibenzo(a,h)anthracene	25.16	278	27091	0.70	ng	98
33) Benzo(g,h,i)perylene	25.79	276	30709	0.72	ng	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM030816\
Data File : BM004575.D
Acq On : 08 Mar 2016 11:33
Operator : SJ/UM
Sample : SSTDICC0.8
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SSTDICC0.8

Quant Time: Mar 08 14:08:49 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\8270-SIM-BM030816.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 08 13:49:28 2016
Response via : Initial Calibration

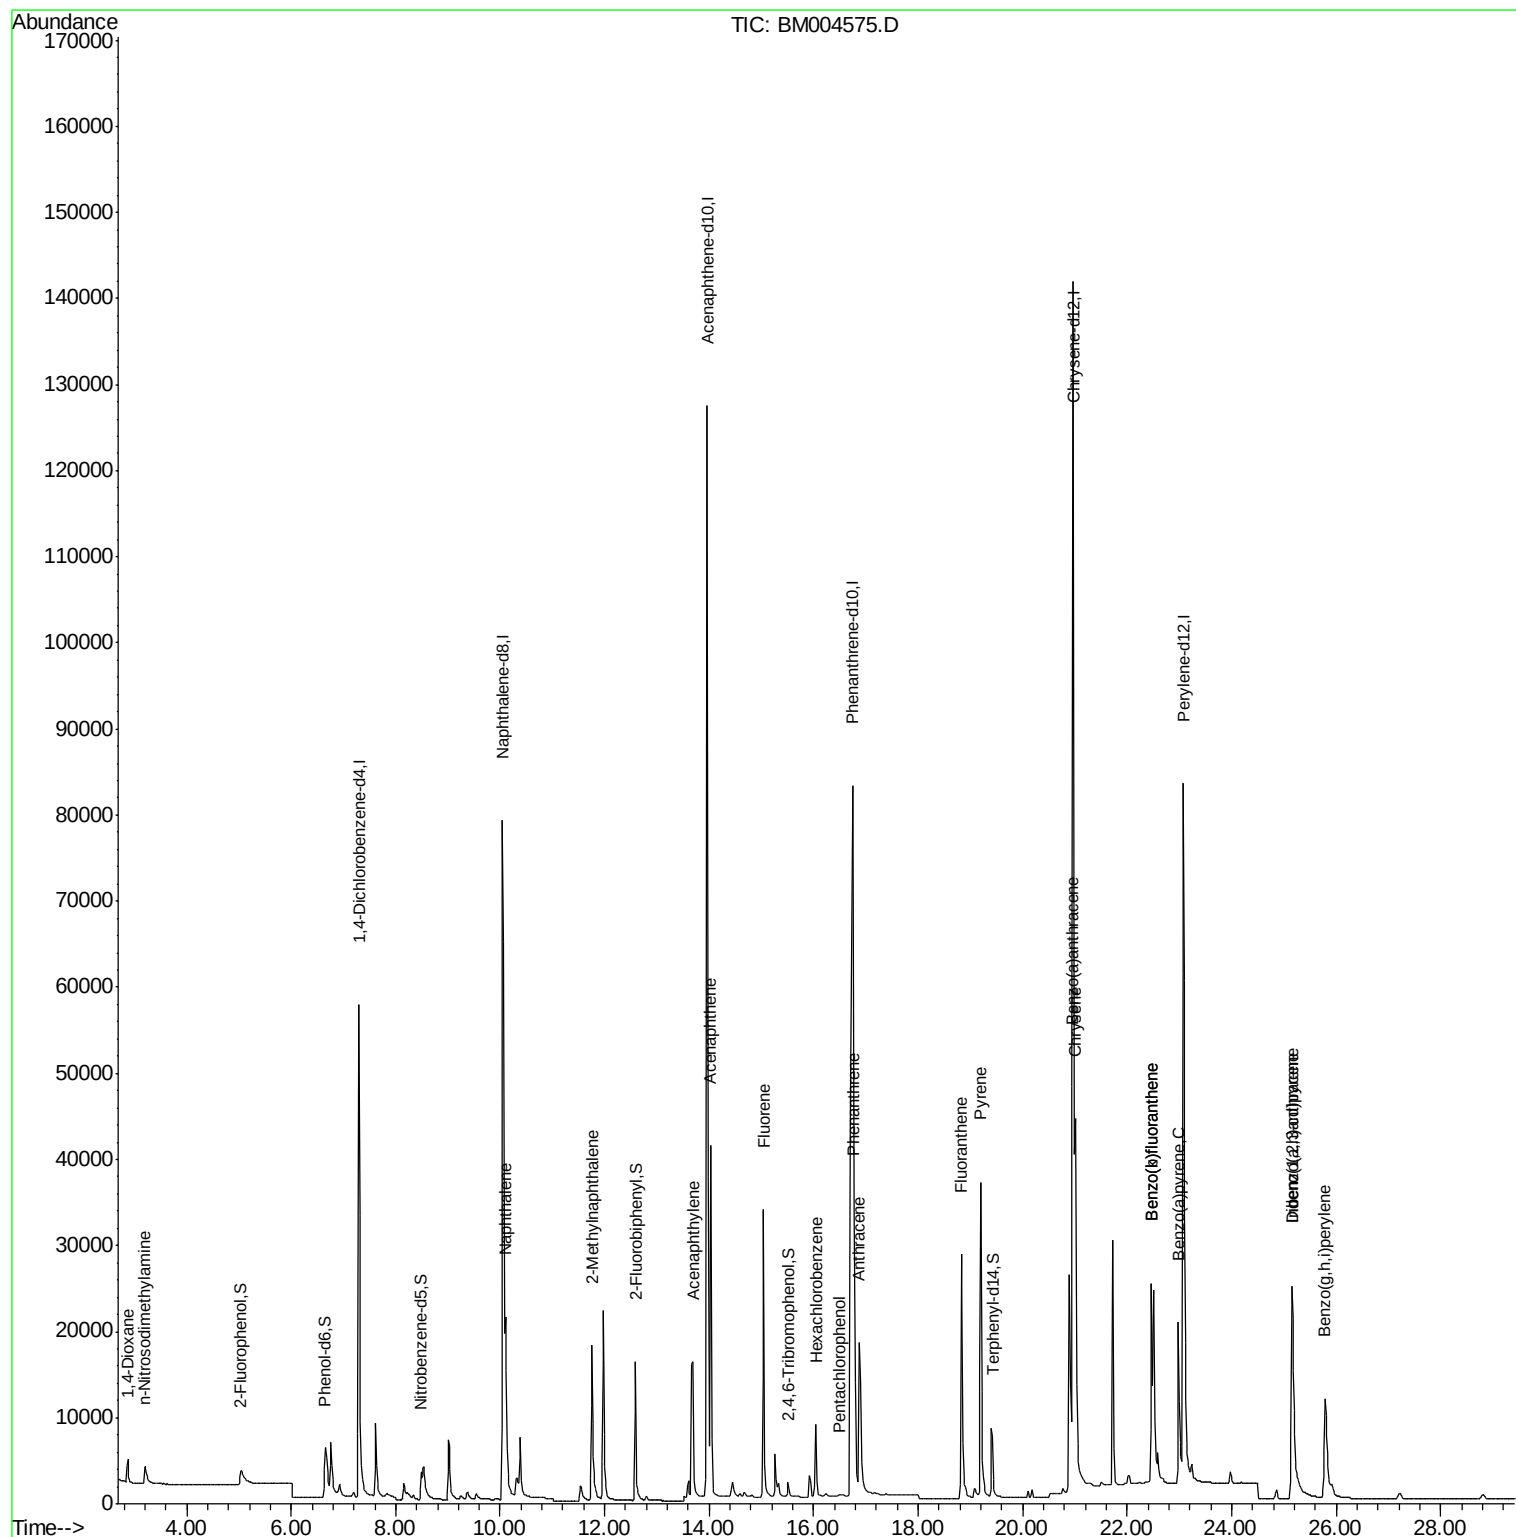



#1

1,4-Dichlorobenzene-d4

Concen: 5.00 ng

RT: 7.29 min Scan# 291

Delta R.T. -0.02 min

Lab File: BM004575.D

Acq: 08 Mar 2016 11:33

Instrument :

BNA_M

ClientSampleId :

SSTDIC0.8


Tgt Ion:152 Resp: 37107

Ion Ratio Lower Upper

152 100

150 166.2 111.9 167.9




115 63.5 37.7 56.5#

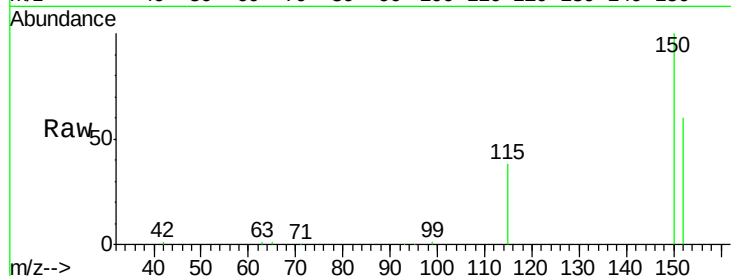

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

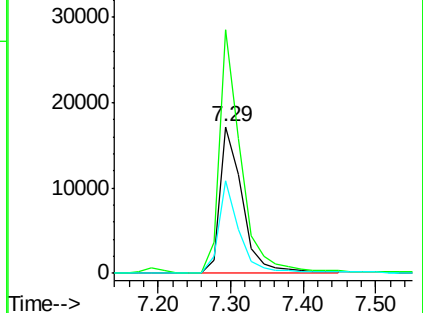

#2

1,4-Dioxane

Concen: 0.63 ng

RT: 2.87 min Scan# 13

Delta R.T. -0.00 min

Lab File: BM004575.D

Acq: 08 Mar 2016 11:33


Tgt Ion: 88 Resp: 2711

Ion Ratio Lower Upper

88 100

58 61.0 45.4 68.0



43 26.4 19.3 28.9




Abundance Ion 88.00 (87.70 to 88.70): BM0

Ion 58.00 (57.70 to 58.70): BM0

Ion 43.00 (42.70 to 43.70): BM0

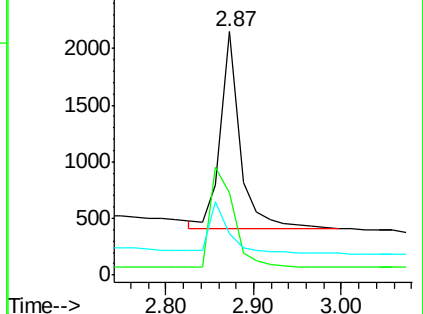

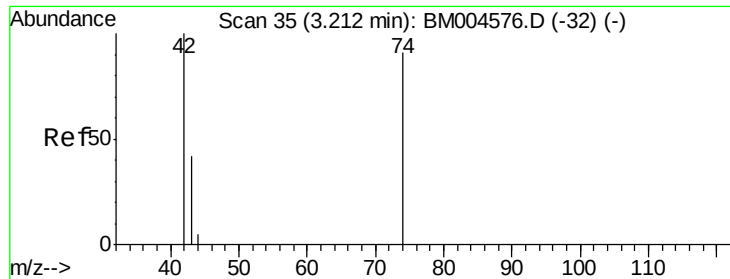

#3

n-Nitrosodimethylamine

Concen: 0.63 ng

RT: 3.20 min Scan# 34

Delta R.T. -0.02 min

Lab File: BM004575.D

Acq: 08 Mar 2016 11:33

Instrument :

BNA_M

ClientSampleId :

SSTDICC0.8


Tgt Ion: 42 Resp: 2380

Ion Ratio Lower Upper

42 100

74 149.4 117.8 176.8




44 9.2 6.1 9.1#

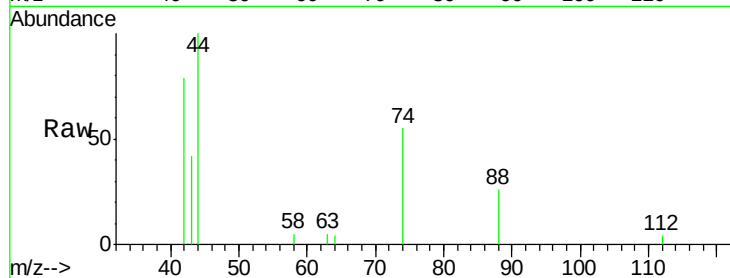

Abundance Ion 42.00 (41.70 to 42.70): BM004575.D (-32) (-)

Ion 74.00 (73.70 to 74.70): BM004575.D (-32) (-)

Ion 44.00 (43.70 to 44.70): BM004575.D (-32) (-)

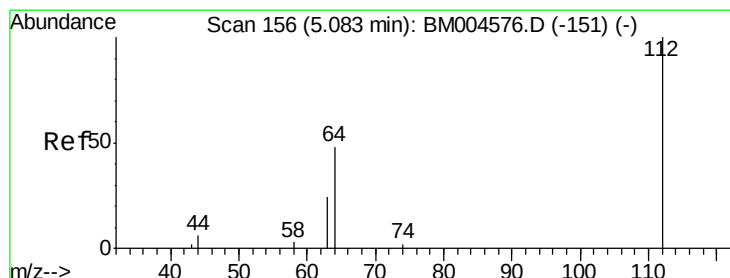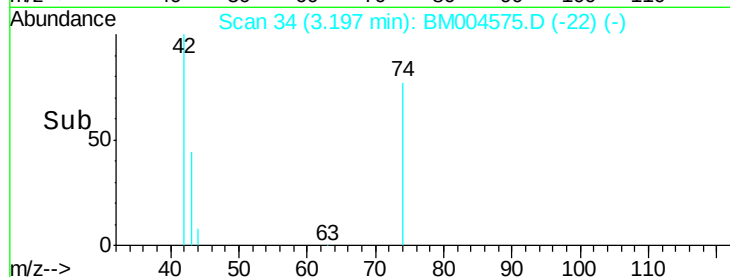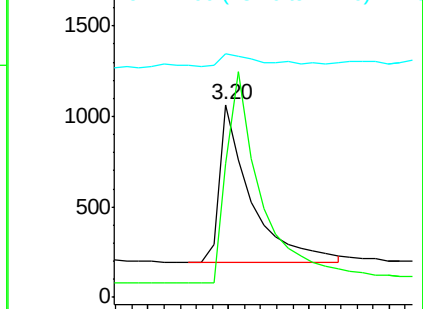

#4

2-Fluorophenol

Concen: 0.59 ng

RT: 5.04 min Scan# 153

Delta R.T. -0.05 min

Lab File: BM004575.D

Acq: 08 Mar 2016 11:33


Tgt Ion: 112 Resp: 5081

Ion Ratio Lower Upper

112 100

64 49.6 39.6 59.4



63 25.0 20.0 30.0

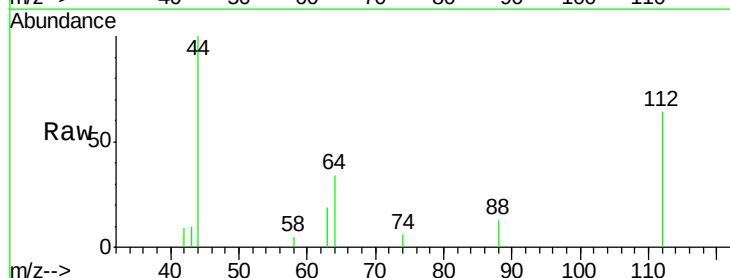


Abundance Ion 112.00 (111.70 to 112.70): BM004575.D (-151) (-)

Ion 64.00 (63.70 to 64.70): BM004575.D (-151) (-)

Ion 63.00 (62.70 to 63.70): BM004575.D (-151) (-)

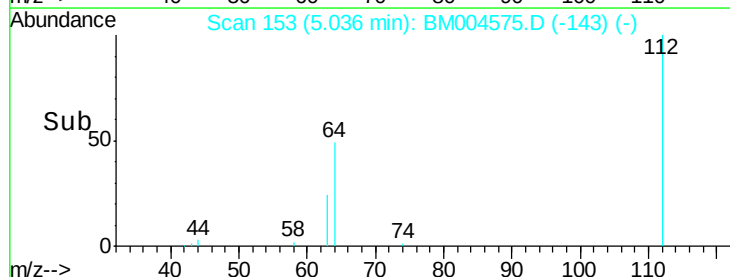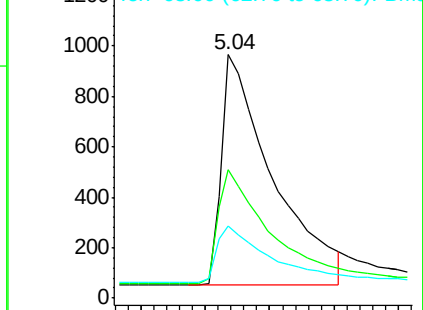



#5

Phenol-d6

Concen: 0.67 ng

RT: 6.64 min Scan# 253

Delta R.T. -0.03 min

Lab File: BM004575.D

Acq: 08 Mar 2016 11:33

Instrument :

BNA_M

ClientSampleId :

SSTDIC0.8


Tgt Ion: 99 Resp: 6531

Ion Ratio Lower Upper

99 100

42 16.2 12.2 18.2

71 28.3 23.4 35.2





Abundance Ion 99.00 (98.70 to 99.70): BM004575.D (-251) (-)

Ion 42.00 (41.70 to 42.70): BM004575.D (-251) (-)

Ion 71.00 (70.70 to 71.70): BM004575.D (-251) (-)

6.64

Time-->

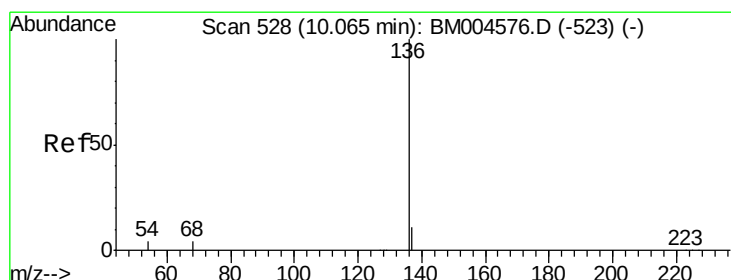

#6

Naphthalene-d8

Concen: 5.00 ng

RT: 10.05 min Scan# 527

Delta R.T. -0.02 min

Lab File: BM004575.D

Acq: 08 Mar 2016 11:33

Tgt Ion: 136 Resp: 139569


Ion Ratio Lower Upper

136 100

137 10.0 8.2 12.2

54 8.9 6.4 9.6

68 7.2 5.0 7.4



Abundance Ion 136.00 (135.70 to 136.70): BM004575.D (-523) (-)


Ion 137.00 (136.70 to 137.70): BM004575.D (-523) (-)


Ion 54.00 (53.70 to 54.70): BM004575.D (-523) (-)

Ion 68.00 (67.70 to 68.70): BM004575.D (-523) (-)

10.05

Time-->





#7

Nitrobenzene-d5

Concen: 0.71 ng

RT: 8.49 min Scan# 379

Delta R.T. -0.02 min

Lab File: BM004575.D

Acq: 08 Mar 2016 11:33

Instrument :

BNA_M

ClientSampleId :

SSTDIC0.8


Tgt Ion: 82 Resp: 5069

Ion Ratio Lower Upper

82 100

128 54.6 43.7 65.5




54 43.7 33.5 50.3



Abundance Ion 82.00 (81.70 to 82.70): BM004576.D (-373) (-)

Ion 128.00 (127.70 to 128.70): BM004576.D (-373) (-)

Ion 54.00 (53.70 to 54.70): BM004576.D (-373) (-)

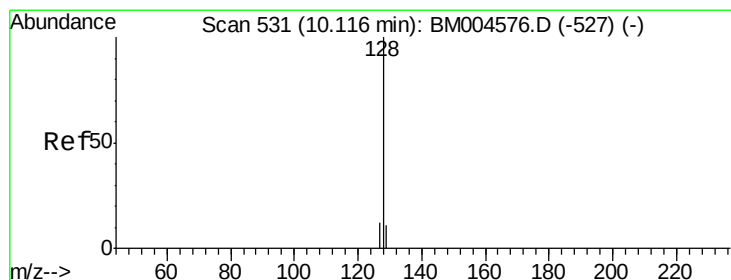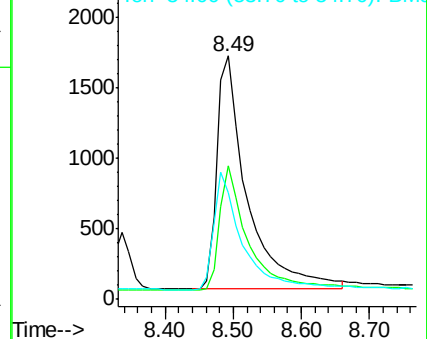

#8

Naphthalene

Concen: 0.72 ng

RT: 10.10 min Scan# 530

Delta R.T. -0.02 min

Lab File: BM004575.D

Acq: 08 Mar 2016 11:33


Tgt Ion: 128 Resp: 31815

Ion Ratio Lower Upper

128 100

129 10.9 8.9 13.3



127 13.7 10.9 16.3

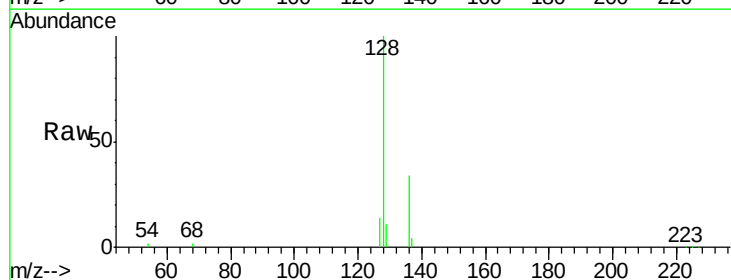


Abundance Ion 128.00 (127.70 to 128.70): BM004576.D (-527) (-)

Ion 129.00 (128.70 to 129.70): BM004576.D (-527) (-)

Ion 127.00 (126.70 to 127.70): BM004576.D (-527) (-)

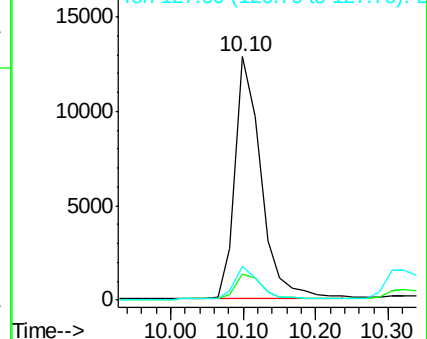

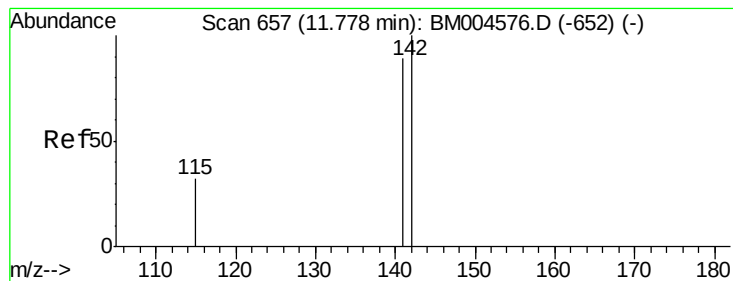

#9

2-Methylnaphthalene

Concen: 0.83 ng

RT: 11.75 min Scan# 654

Delta R.T. -0.02 min

Lab File: BM004575.D

Acq: 08 Mar 2016 11:33

Instrument :

BNA_M

ClientSampleId :

SSTDICC0.8


Tgt Ion:142 Resp: 20220

Ion Ratio Lower Upper

142 100

141 90.6 70.2 105.2




115 33.1 25.8 38.6

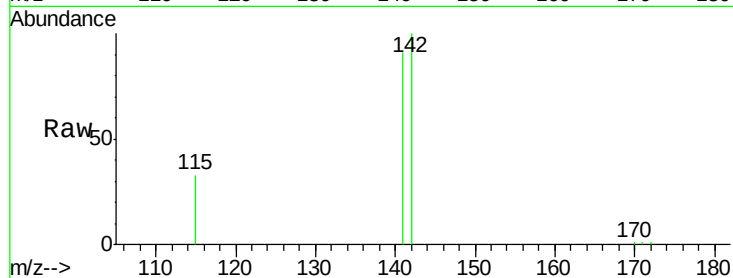

Abundance Ion 142.00 (141.70 to 142.70): E

Ion 141.00 (140.70 to 141.70): E

Ion 115.00 (114.70 to 115.70): E

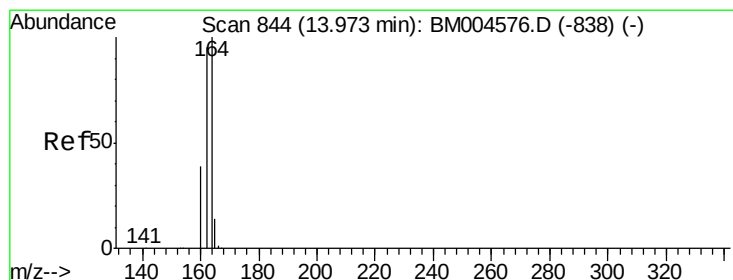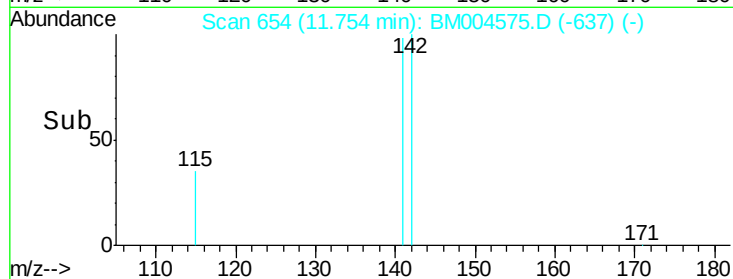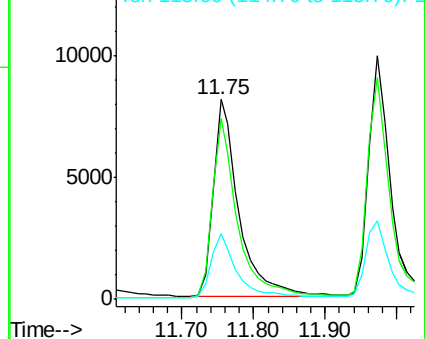

#10

Acenaphthene-d10

Concen: 5.00 ng

RT: 13.96 min Scan# 843

Delta R.T. -0.02 min

Lab File: BM004575.D

Acq: 08 Mar 2016 11:33


Tgt Ion:164 Resp: 81696

Ion Ratio Lower Upper

164 100

162 117.6 84.2 126.4



160 57.2 37.4 56.2#

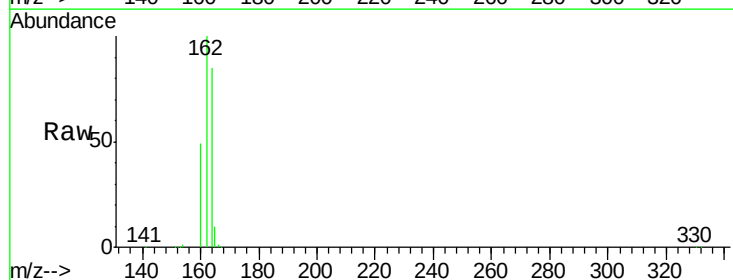


Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E



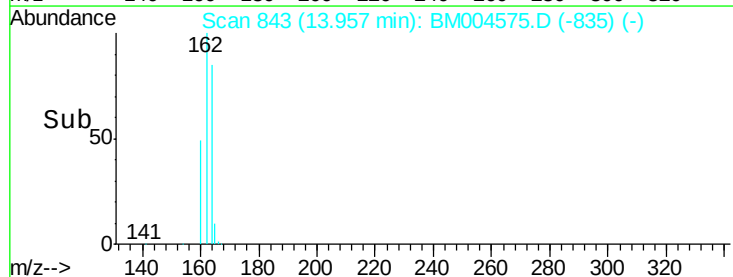
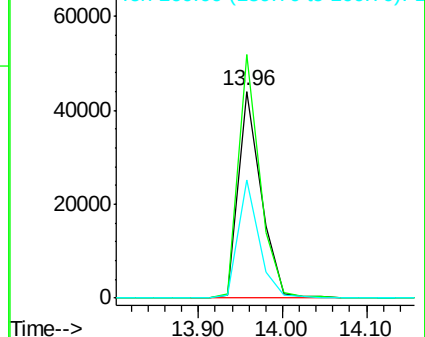




#11
 2,4,6-Tribromophenol
 Concen: 0.54 ng
 RT: 15.51 min Scan# 913
 Delta R.T. -0.01 min
 Lab File: BM004575.D
 Acq: 08 Mar 2016 11:33




Instrument :
 BNA_M
 ClientSampleId :
 SSTDICC0.8


Tgt Ion:330 Resp: 1702
 Ion Ratio Lower Upper
 330 100
 332 94.9 76.1 114.1
 141 0.0 16.0 24.0#

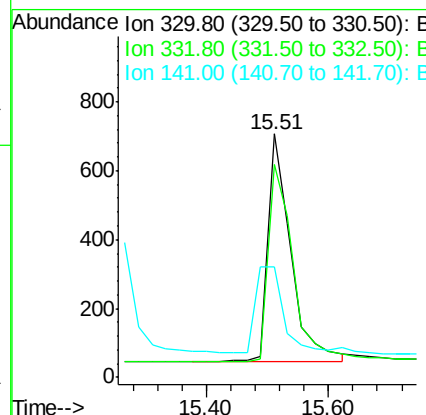

#12
 2-Fluorobiphenyl
 Concen: 0.77 ng
 RT: 12.59 min Scan# 734
 Delta R.T. -0.01 min
 Lab File: BM004575.D
 Acq: 08 Mar 2016 11:33

Tgt Ion:172 Resp: 19361
 Ion Ratio Lower Upper
 172 100
 171 34.6 29.2 43.8
 170 22.2 19.7 29.5

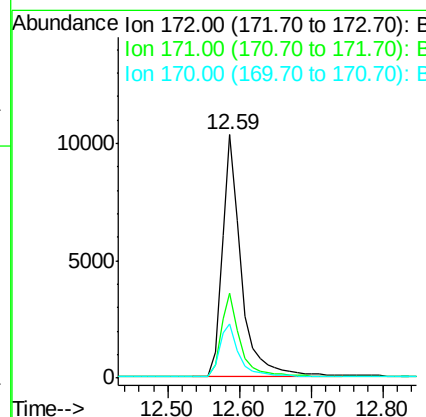

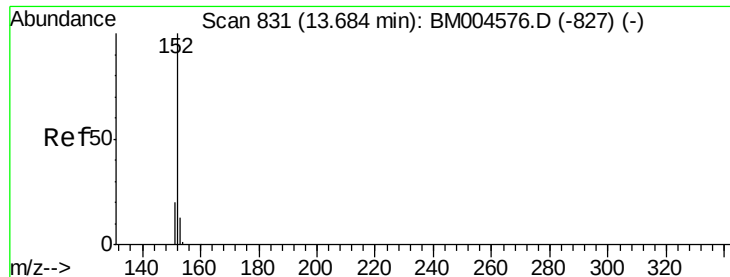

#13

Acenaphthylene

Concen: 0.73 ng

RT: 13.69 min Scan# 831

Delta R.T. 0.01 min

Lab File: BM004575.D

Acq: 08 Mar 2016 11:33

Instrument :

BNA_M

ClientSampleId :

SSTDIC0.8


Tgt Ion:152 Resp: 34169

Ion Ratio Lower Upper

152 100

151 0.0 15.8 23.6#

153 15.3 10.2 15.4

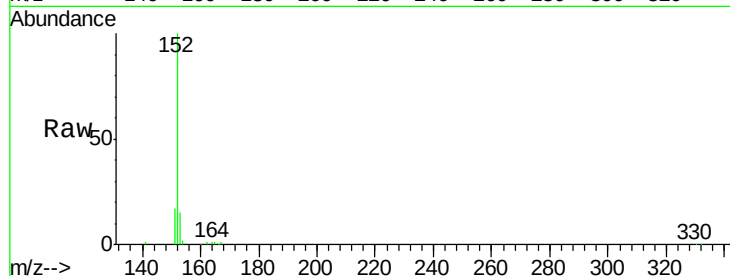

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 151.00 (150.70 to 151.70): E

Ion 153.00 (152.70 to 153.70): E



13.69

10000

5000

0

Time--> 13.40 13.60 13.80

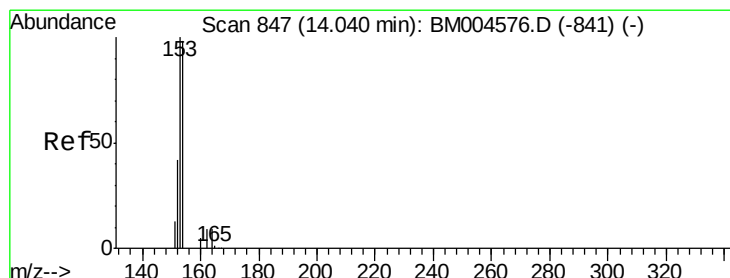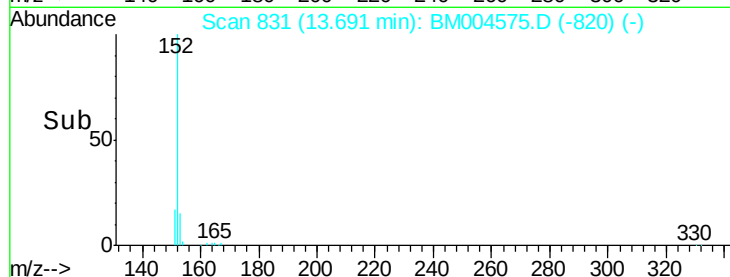

#14

Acenaphthene

Concen: 0.78 ng

RT: 14.02 min Scan# 846

Delta R.T. -0.02 min

Lab File: BM004575.D

Acq: 08 Mar 2016 11:33


Tgt Ion:154 Resp: 23778

Ion Ratio Lower Upper

154 100

153 111.7 88.0 132.0

152 52.3 41.1 61.7

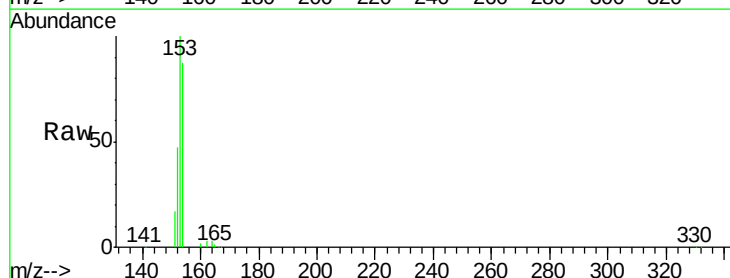

Abundance Ion 154.00 (153.70 to 154.70): E

Ion 153.00 (152.70 to 153.70): E

Ion 152.00 (151.70 to 152.70): E

14.02

20000


15000


10000

5000

0

Time--> 13.80 14.00 14.20




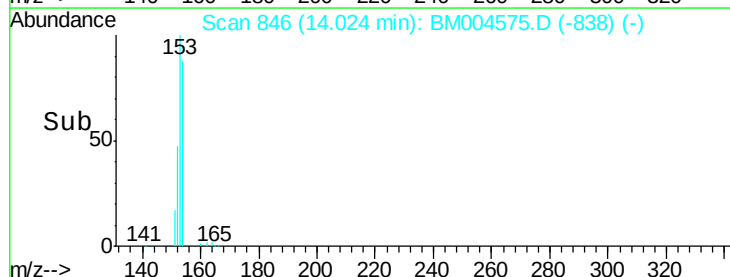




#15
Fluorene
 Concen: 0.75 ng
 RT: 15.05 min Scan# 892
 Delta R.T. -0.02 min
 Lab File: BM004575.D
 Acq: 08 Mar 2016 11:33




Instrument :
 BNA_M
 ClientSampleId :
 SSTDICC0.8


Tgt Ion:166 Resp: 27941
 Ion Ratio Lower Upper
 166 100
 165 95.2 77.2 115.8
 167 13.7 10.9 16.3

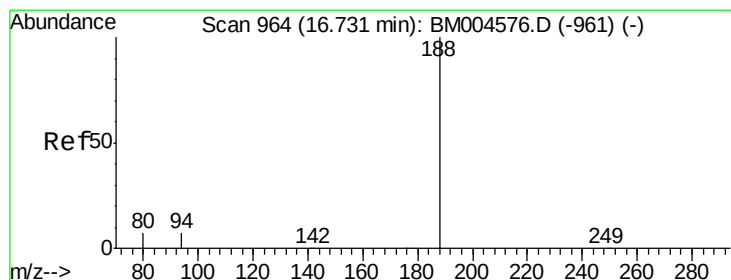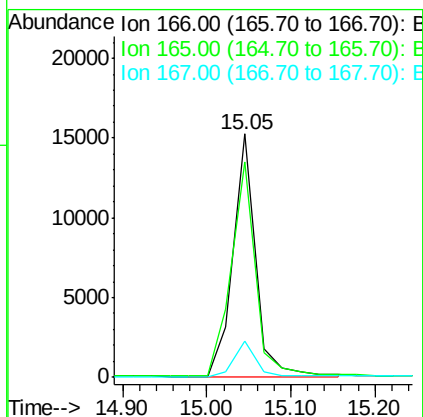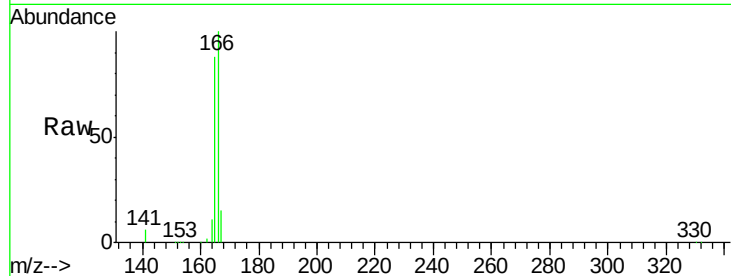

#16
Phenanthrene-d10
 Concen: 5.00 ng
 RT: 16.74 min Scan# 964
 Delta R.T. 0.01 min
 Lab File: BM004575.D
 Acq: 08 Mar 2016 11:33

Tgt Ion:188 Resp: 162919
 Ion Ratio Lower Upper
 188 100
 94 3.7 7.4 11.0#
 80 3.2 6.9 10.3#

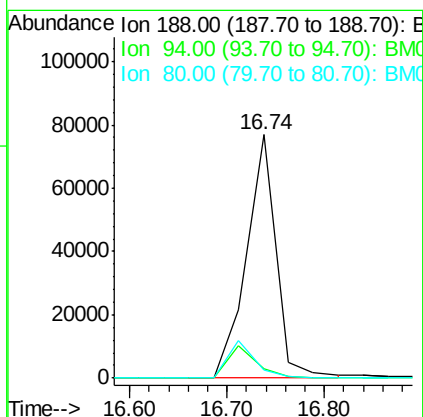







#17
Hexachlorobenzene
Concen: 0.81 ng
RT: 16.05 min Scan# 937
Delta R.T. -0.02 min
Lab File: BM004575.D
Acq: 08 Mar 2016 11:33

Instrument :
BNA_M
ClientSampleId :
SSTDIC0.8

Tgt Ion:284 Resp: 8176
Ion Ratio Lower Upper
284 100
142 43.4 20.8 31.2#
249 44.6 24.0 36.0#

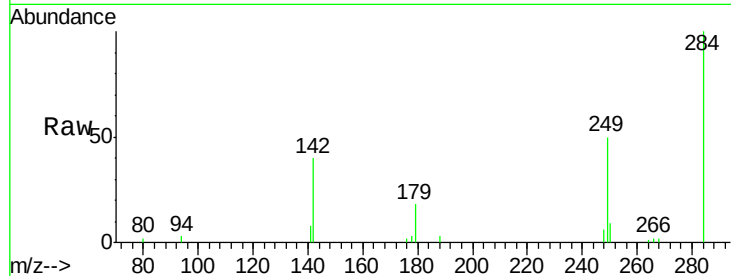


Abundance Ion 283.80 (283.50 to 284.50): E
Ion 142.00 (141.70 to 142.70): E
Ion 249.00 (248.70 to 249.70): E


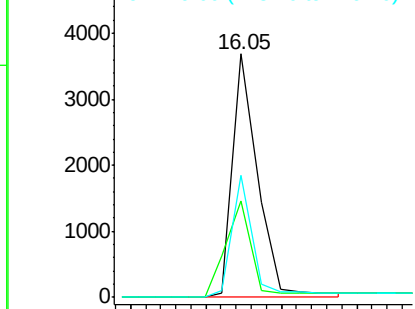



#18
Pentachlorophenol
Concen: 0.16 ng
RT: 16.48 min Scan# 954
Delta R.T. -0.04 min
Lab File: BM004575.D
Acq: 08 Mar 2016 11:33

Tgt Ion:266 Resp: 400
Ion Ratio Lower Upper
266 100
268 83.9 60.7 91.1
264 75.0 57.1 85.7



Abundance Ion 265.70 (265.40 to 266.40): E
Ion 268.00 (267.70 to 268.70): E
Ion 264.00 (263.70 to 264.70): E

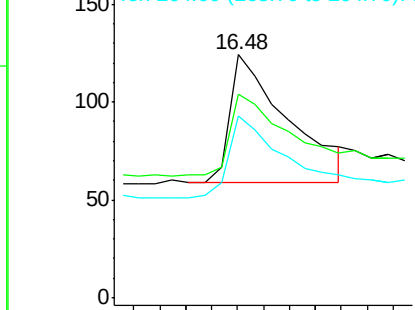

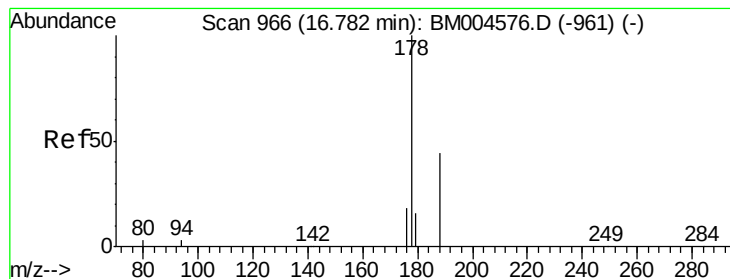

#19

Phenanthrene

Concen: 0.79 ng

RT: 16.76 min Scan# 965

Delta R.T. -0.02 min

Lab File: BM004575.D

Acq: 08 Mar 2016 11:33

Instrument :

BNA_M

ClientSampleId :

SSTDIC0.8


Tgt Ion:178 Resp: 45229

Ion Ratio Lower Upper

178 100

176 19.5 14.7 22.1




179 15.2 12.9 19.3

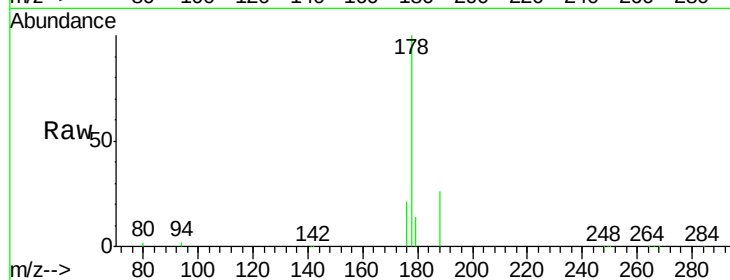

Abundance Ion 178.00 (177.70 to 178.70): E

Ion 176.00 (175.70 to 176.70): E

Ion 179.00 (178.70 to 179.70): E

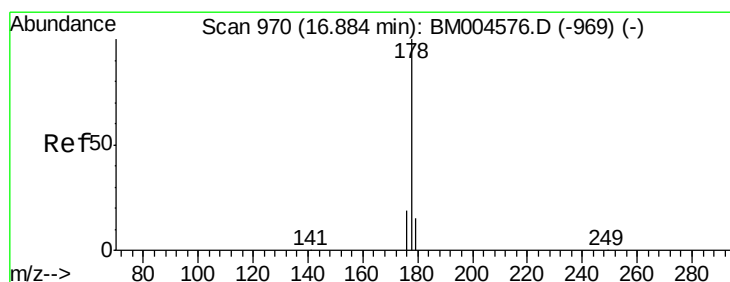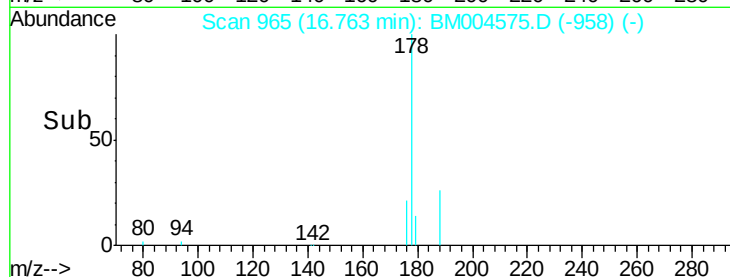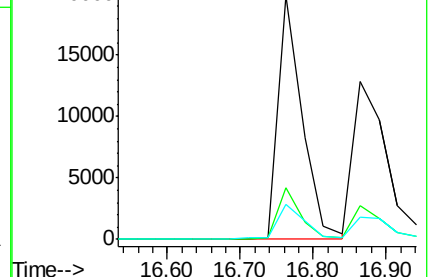

#20

Anthracene

Concen: 0.80 ng

RT: 16.87 min Scan# 969

Delta R.T. -0.02 min

Lab File: BM004575.D

Acq: 08 Mar 2016 11:33


Tgt Ion:178 Resp: 38862

Ion Ratio Lower Upper

178 100

176 18.9 15.6 23.4



179 14.5 13.6 20.4

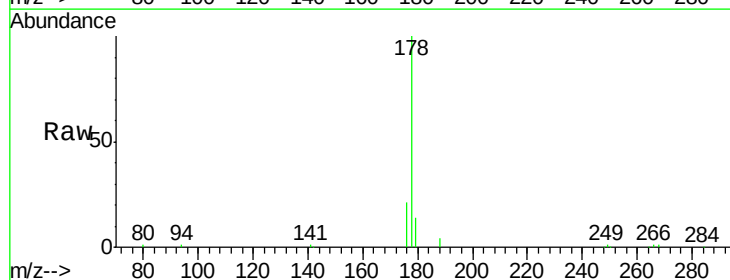


Abundance Ion 178.00 (177.70 to 178.70): E

Ion 176.00 (175.70 to 176.70): E

Ion 179.00 (178.70 to 179.70): E



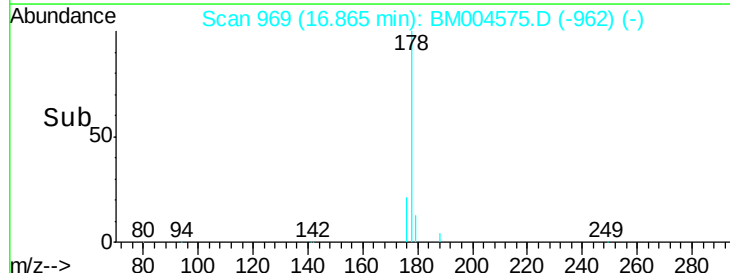
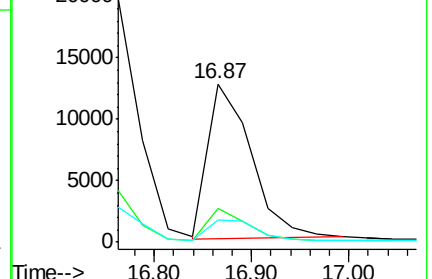




#21
Fluoranthene
Concen: 0.76 ng
RT: 18.82 min Scan# 1061
Delta R.T. -0.03 min
Lab File: BM004575.D
Acq: 08 Mar 2016 11:33




Instrument :
BNA_M
ClientSampleId :
SSTDIC0.8


Tgt Ion: 202 Resp: 46971
Ion Ratio Lower Upper
202 100
101 12.7 9.4 14.2
203 17.2 13.9 20.9

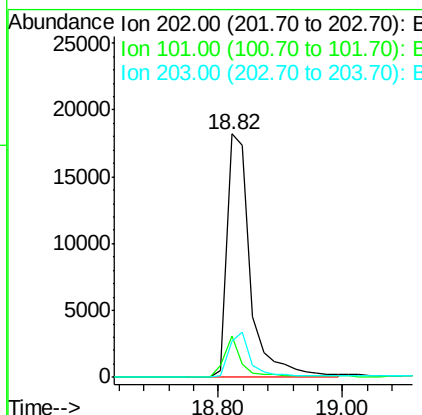

#22
Chrysene-d12
Concen: 5.00 ng
RT: 20.97 min Scan# 1182
Delta R.T. -0.01 min
Lab File: BM004575.D
Acq: 08 Mar 2016 11:33

Tgt Ion: 240 Resp: 157246
Ion Ratio Lower Upper
240 100
120 10.7 6.1 9.1#
236 29.3 22.6 34.0



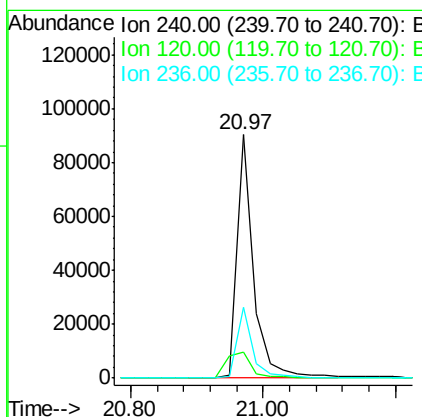





#23
 Pyrene
 Concen: 0.78 ng
 RT: 19.20 min Scan# 1083
 Delta R.T. -0.01 min
 Lab File: BM004575.D
 Acq: 08 Mar 2016 11:33




Instrument :
 BNA_M
 ClientSampleId :
 SSTDICC0.8


Tgt Ion: 202 Resp: 48382
 Ion Ratio Lower Upper
 202 100
 200 21.1 16.6 24.8
 203 17.4 14.1 21.1

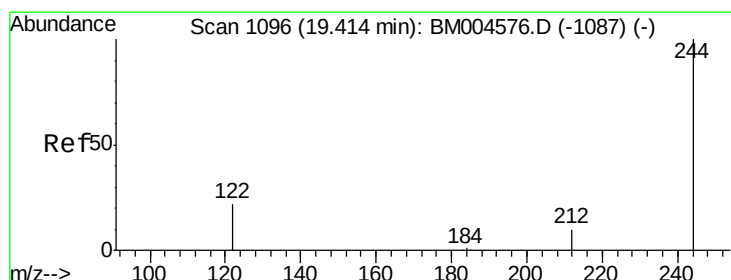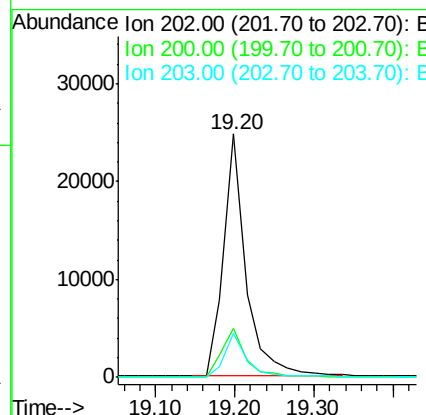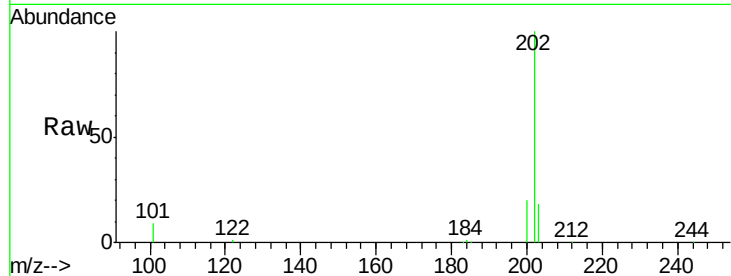

#24
 Terphenyl-d14
 Concen: 0.75 ng
 RT: 19.42 min Scan# 1096
 Delta R.T. 0.01 min
 Lab File: BM004575.D
 Acq: 08 Mar 2016 11:33

Tgt Ion: 244 Resp: 15184
 Ion Ratio Lower Upper
 244 100
 212 8.8 7.5 11.3
 122 7.9 4.2 6.2#

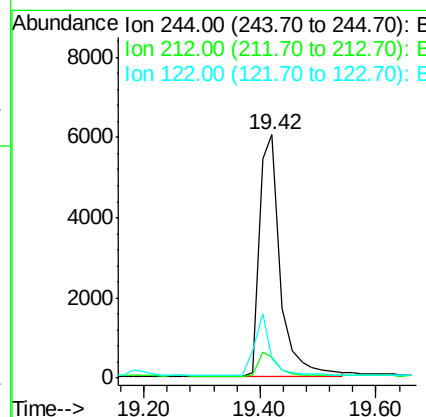

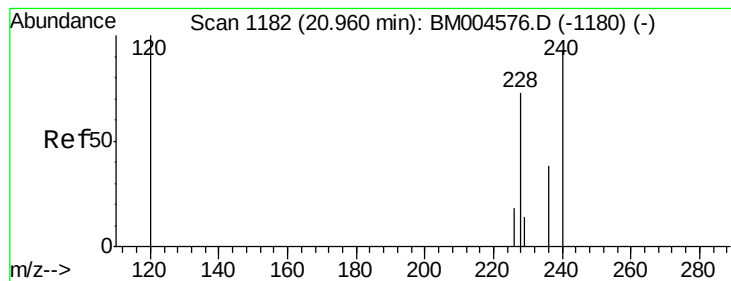

#25

Benzo(a)anthracene

Concen: 0.78 ng

RT: 20.95 min Scan# 1181

Delta R.T. -0.01 min

Lab File: BM004575.D

Acq: 08 Mar 2016 11:33

Instrument :

BNA_M

ClientSampleId :

SSTDICC0.8





Tgt Ion:228 Resp: 45430

Ion Ratio Lower Upper

228 100

226 30.1 22.8 34.2

229 17.1 14.6 22.0

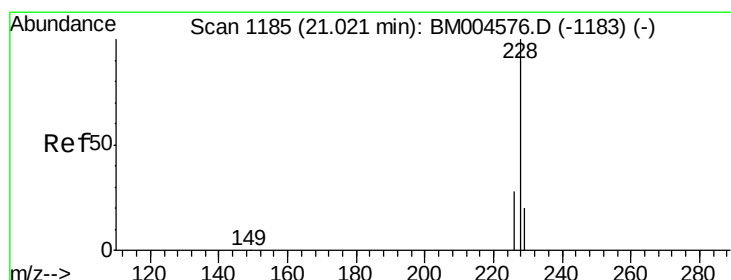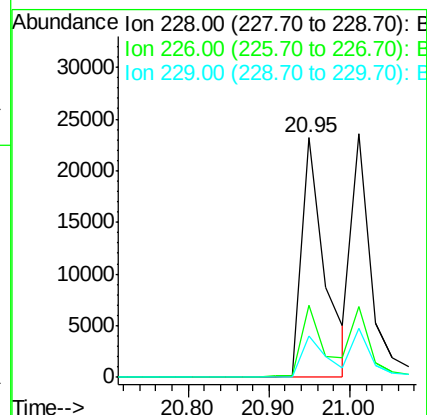

#26

Chrysene

Concen: 0.32 ng

RT: 21.01 min Scan# 1184

Delta R.T. -0.01 min

Lab File: BM004575.D

Acq: 08 Mar 2016 11:33




Tgt Ion:228 Resp: 38037


Ion Ratio Lower Upper

228 100

226 29.1 21.4 32.2

229 20.2 17.1 25.7



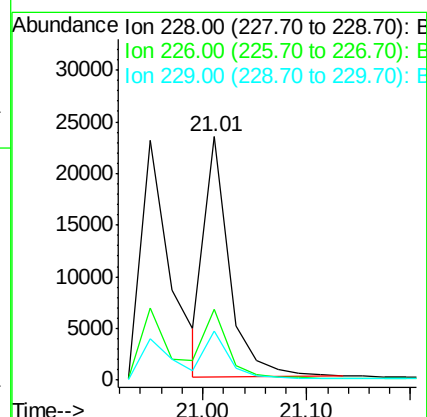
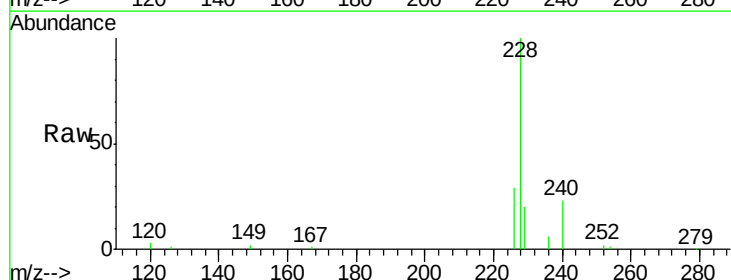




#27
 Indeno(1,2,3-cd)pyrene
 Concen: 0.65 ng
 RT: 25.16 min Scan# 1502
 Delta R.T. -0.02 min
 Lab File: BM004575.D
 Acq: 08 Mar 2016 11:33




Instrument :
 BNA_M
 ClientSampleId :
 SSTDICC0.8


Tgt Ion: 276 Resp: 34995
 Ion Ratio Lower Upper
 276 100
 138 39.2 30.4 45.6
 277 24.7 19.8 29.8

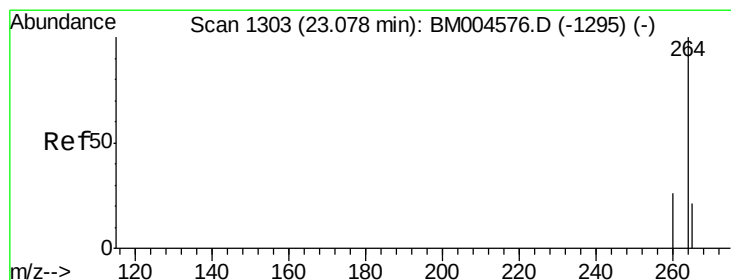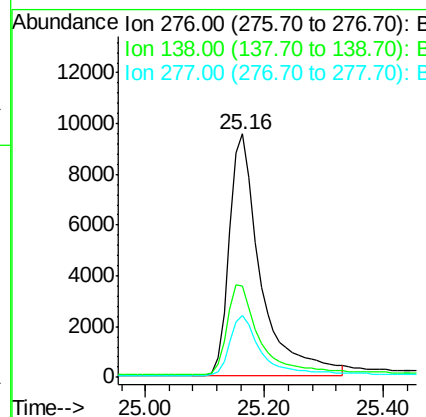

#28
 Perylene-d12
 Concen: 5.00 ng
 RT: 23.08 min Scan# 1302
 Delta R.T. -0.00 min
 Lab File: BM004575.D
 Acq: 08 Mar 2016 11:33

Tgt Ion: 264 Resp: 125970
 Ion Ratio Lower Upper
 264 100
 260 25.5 19.8 29.6
 265 23.3 18.9 28.3

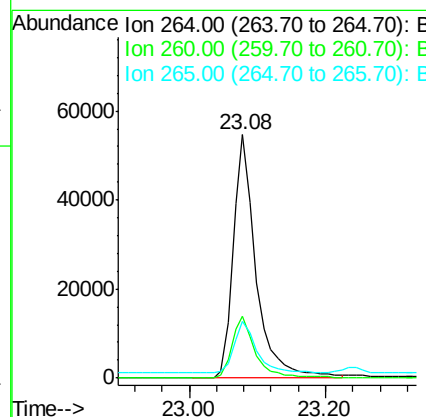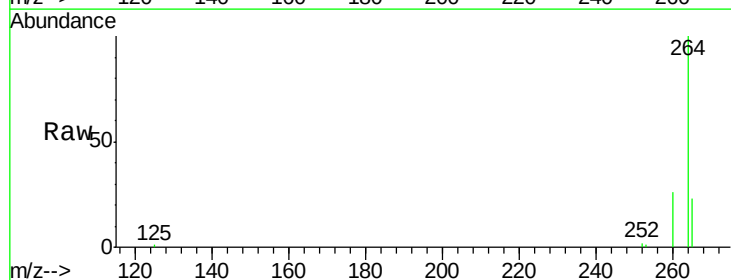

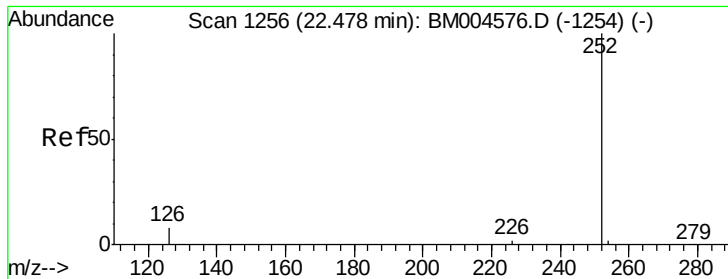

#29

Benzo(b)fluoranthene

Concen: 1.50 ng

RT: 22.47 min Scan# 1255

Delta R.T. -0.01 min

Lab File: BM004575.D

Acq: 08 Mar 2016 11:33

Instrument :

BNA_M

ClientSampleId :

SSTDIC0.8


Tgt Ion:252 Resp: 73834

Ion Ratio Lower Upper

252 100

253 0.0 18.8 28.2#




125 0.0 11.8 17.8#

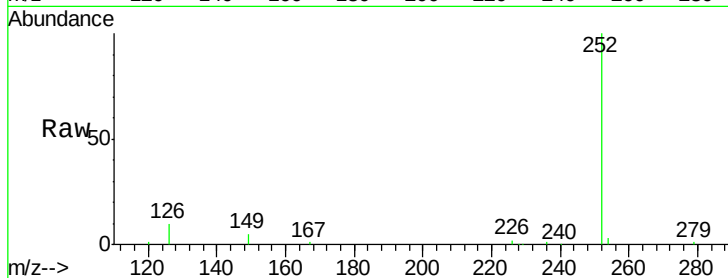

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

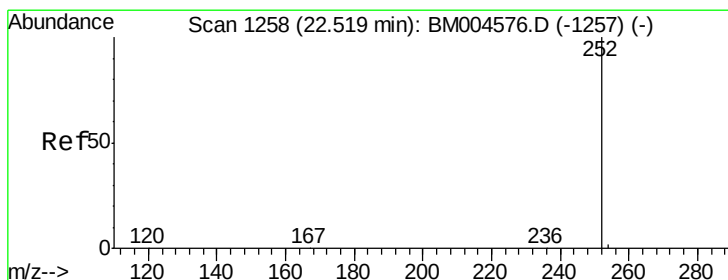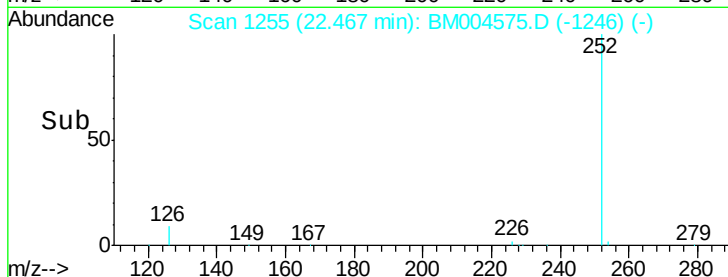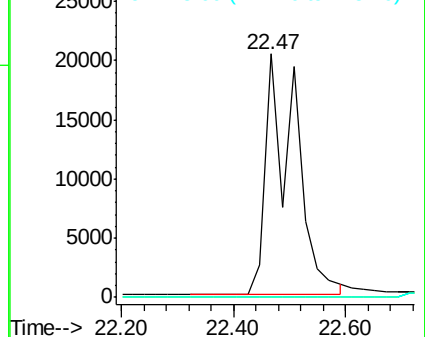

#30

Benzo(k)fluoranthene

Concen: 1.55 ng

RT: 22.47 min Scan# 1255

Delta R.T. -0.05 min

Lab File: BM004575.D

Acq: 08 Mar 2016 11:33


Tgt Ion:252 Resp: 75108

Ion Ratio Lower Upper

252 100

253 0.0 18.3 27.5#



125 0.0 12.2 18.4#

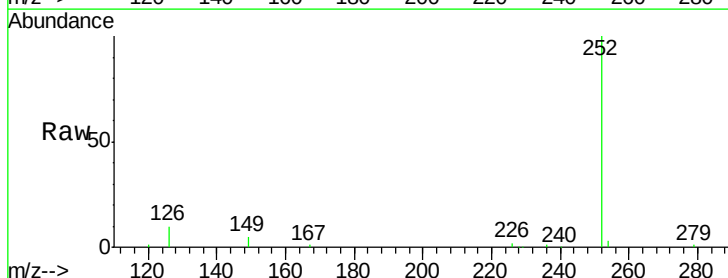


Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

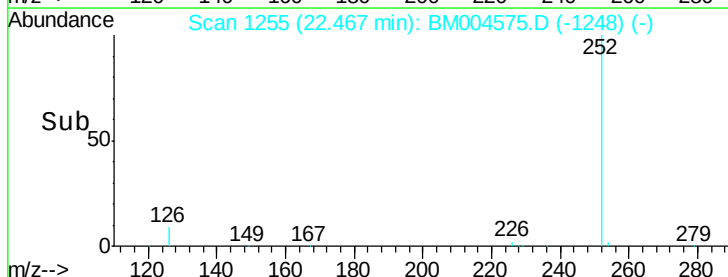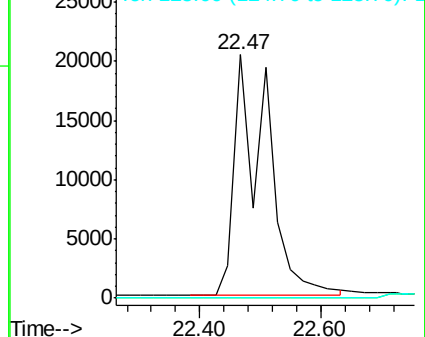







#31
Benzo(a)pyrene
Concen: 0.78 ng
RT: 22.98 min Scan# 1293
Delta R.T. -0.01 min
Lab File: BM004575.D
Acq: 08 Mar 2016 11:33

Instrument :
BNA_M
ClientSampleId :
SSTDIC0.8

Tgt Ion: 252 Resp: 34658
Ion Ratio Lower Upper
252 100
253 22.4 18.0 27.0
125 18.7 14.3 21.5

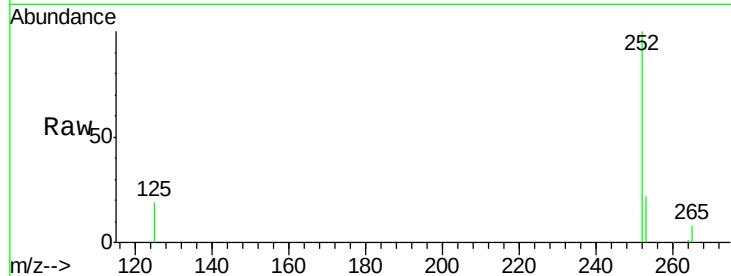


Abundance Ion 252.00 (251.70 to 252.70): E
Ion 253.00 (252.70 to 253.70): E
Ion 125.00 (124.70 to 125.70): E


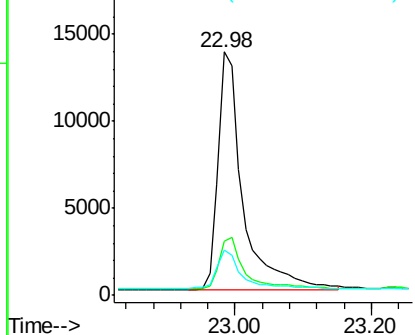



#32
Dibenzo(a,h)anthracene
Concen: 0.70 ng
RT: 25.16 min Scan# 1502
Delta R.T. -0.02 min
Lab File: BM004575.D
Acq: 08 Mar 2016 11:33

Tgt Ion: 278 Resp: 27091
Ion Ratio Lower Upper
278 100
139 27.7 21.2 31.8
279 25.2 19.6 29.4



Abundance Ion 278.00 (277.70 to 278.70): E
Ion 139.00 (138.70 to 139.70): E
Ion 279.00 (278.70 to 279.70): E

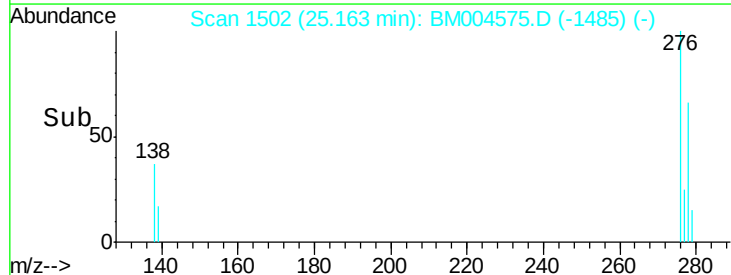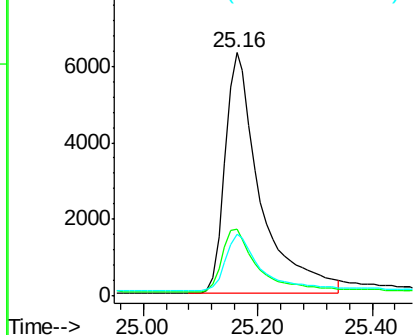

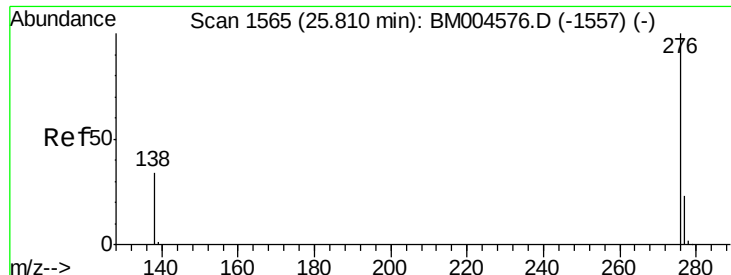

#33

Benzo(g,h,i)perylene

Concen: 0.72 ng

RT: 25.79 min Scan# 1562

Delta R.T. -0.02 min

Lab File: BM004575.D


Acq: 08 Mar 2016 11:33

Instrument :

BNA_M

ClientSampleId :

SSTDIC0.8

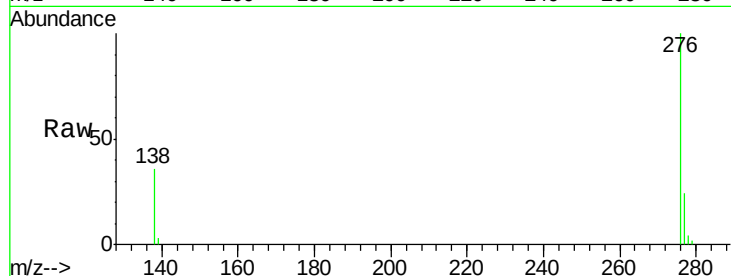

Tgt Ion: 276 Resp: 30709

Ion Ratio Lower Upper

276 100

277 23.6 19.6 29.4

138 35.5 26.2 39.2

