


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM030816\
 Data File : BM004572.D
 Acq On : 08 Mar 2016 09:41
 Operator : SJ/UM
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\8270-SIM-BM030816.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Mar 08 18:22:06 2016

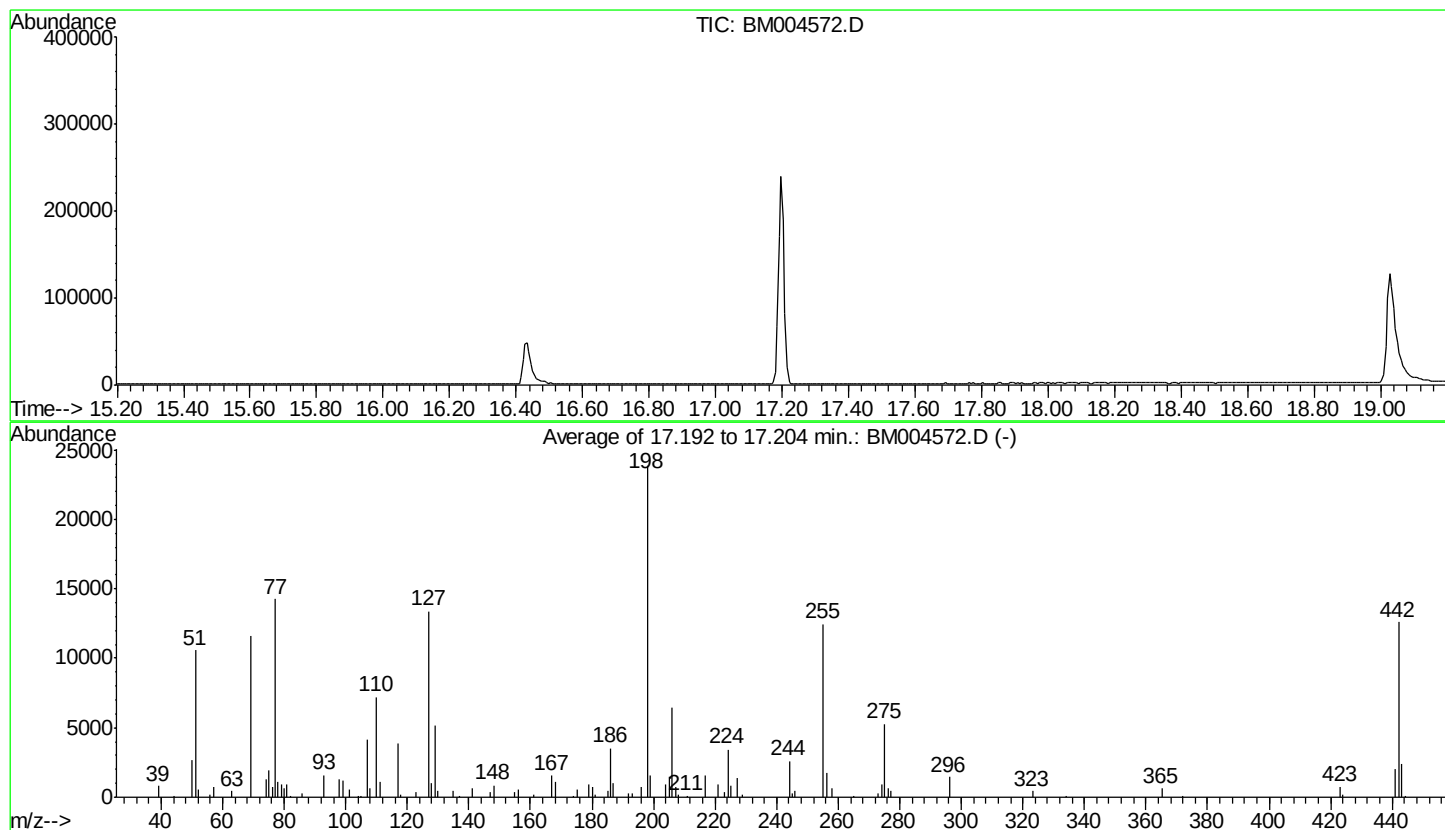

AutoFind: Scans 2466, 2467, 2468; Background Corrected with Scan 2461

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.3	10562	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	48.6	11604	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	56.1	13386	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	23864	PASS
199	198	5	9	6.6	1569	PASS
275	198	10	60	22.2	5294	PASS
365	198	1	100	2.6	618	PASS
441	442	0.01	24	15.9	2000	PASS
442	198	50	100	52.9	12613	PASS
443	442	15	24	19.3	2436	PASS