

Data Path : Z:\HPCHEM1\BNA_M\Data\BM030817\
 Data File : BM009107.D
 Acq On : 08 Mar 2017 13:53
 Operator : SJ/MA
 Sample : PB97370BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK70

Quant Time: Mar 08 15:10:49 2017
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030317.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 08 15:09:59 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.90	152	136	0.40	ng/ul	0.00
2) Naphthalene-d8	10.69	136	390	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.52	164	253	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.36	188	48842	0.40	ng/ul	0.10
16) Chrysene-d12	21.45	240	648	0.40	ng/ul	0.00
20) Perylene-d12	23.64	264	45495	0.40	ng/ul	-0.15
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.28	152	204	0.32	ng/ul	0.00
14) Fluoranthene-d10	19.30	212	559	0.00	ng/ul	0.00
Target Compounds						
17) Pyrene	19.66	202	115	0.05	ng/ul#	Qvalue 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\Data\BM030817\
Data File : BM009107.D
Acq On : 08 Mar 2017 13:53
Operator : SJ/MA
Sample : PB97370BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK70

Quant Time: Mar 08 15:10:49 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 08 15:09:59 2017
Response via : Initial Calibration

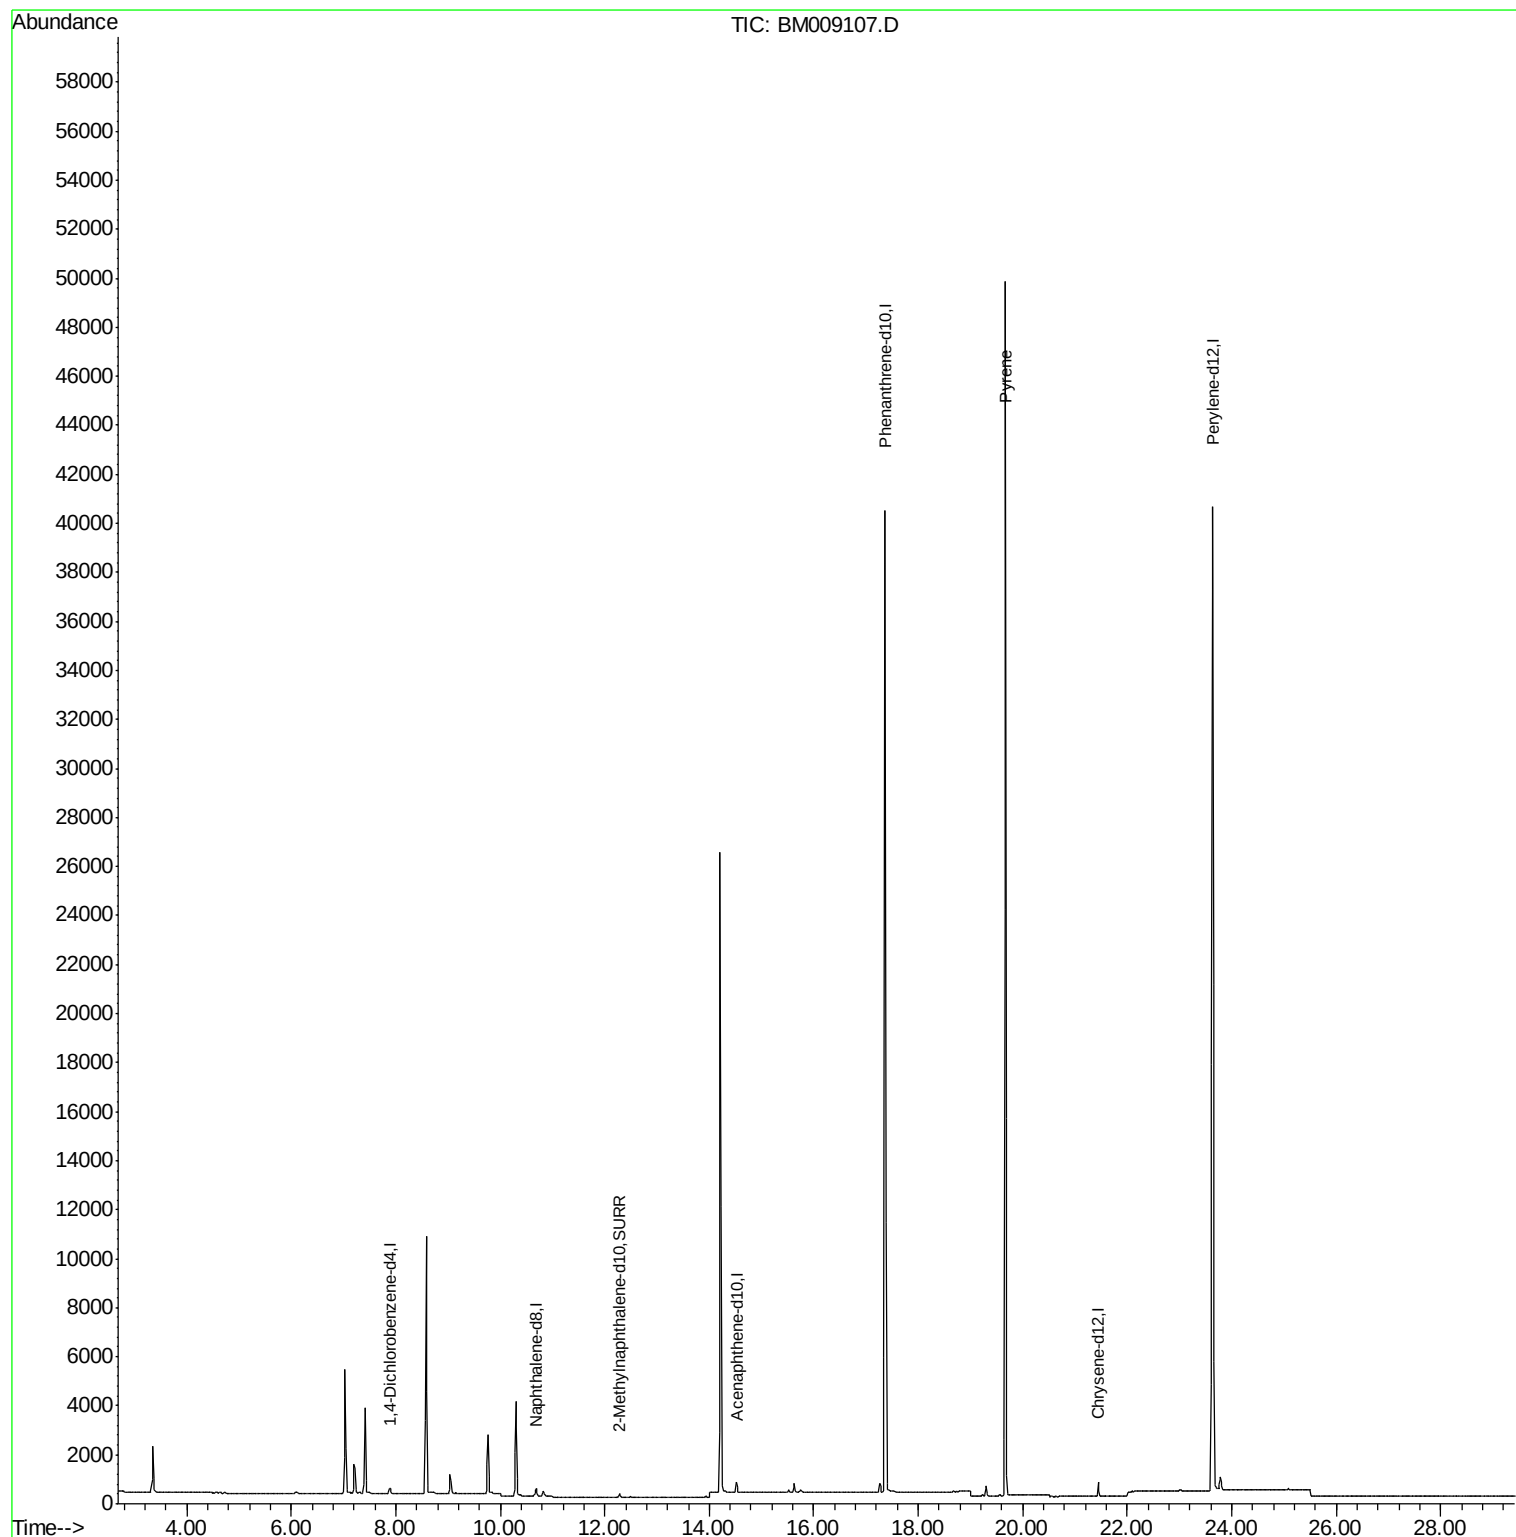


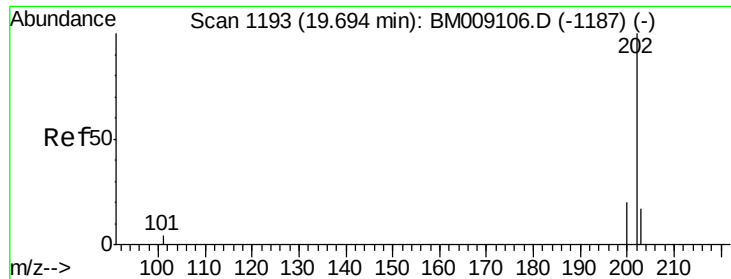

#17
 Pyrene
 Concen: 0.05 ng/ul
 RT: 19.66 min Scan# 1191
 Delta R.T. -0.03 min
 Lab File: BM009107.D
 Acq: 08 Mar 2017 13:53

Instrument :
 BNA_M
 ClientSampleId :
 SBLK70

Tgt Ion: 202 Resp: 115
 Ion Ratio Lower Upper
 202 100
 200 39.3 18.2 27.4#
 203 164.8 15.6 23.4#

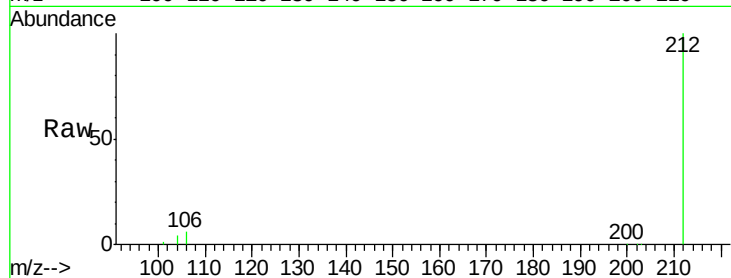

Abundance Ion 202.00 (201.70 to 202.70): E
 Ion 200.00 (199.70 to 200.70): E
 Ion 203.00 (202.70 to 203.70): E

