

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM030817\
 Data File : BM009118.D
 Acq On : 08 Mar 2017 20:29
 Operator : SJ/MA
 Sample : I2062-14
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AD6

Quant Time: Mar 09 01:20:43 2017
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030317.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 09 01:19:41 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.88	152	250	0.40	ng/ul	-0.02
2) Naphthalene-d8	10.68	136	790	0.40	ng/ul	-0.01
6) Acenaphthene-d10	14.52	164	524	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.36	188	112446	0.40	ng/ul	0.10
16) Chrysene-d12	21.45	240	1371	0.40	ng/ul	0.00
20) Perylene-d12	23.64	264	90830	0.40	ng/ul	-0.15
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.27	152	448	0.34	ng/ul	-0.01
14) Fluoranthene-d10	19.30	212	1328	0.00	ng/ul	0.00
Target Compounds						
17) Pyrene	19.67	202	316	0.07	ng/ul#	Qvalue 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM030817\
Data File : BM009118.D
Acq On : 08 Mar 2017 20:29
Operator : SJ/MA
Sample : I2062-14
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AD6

Quant Time: Mar 09 01:20:43 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 09 01:19:41 2017
Response via : Initial Calibration

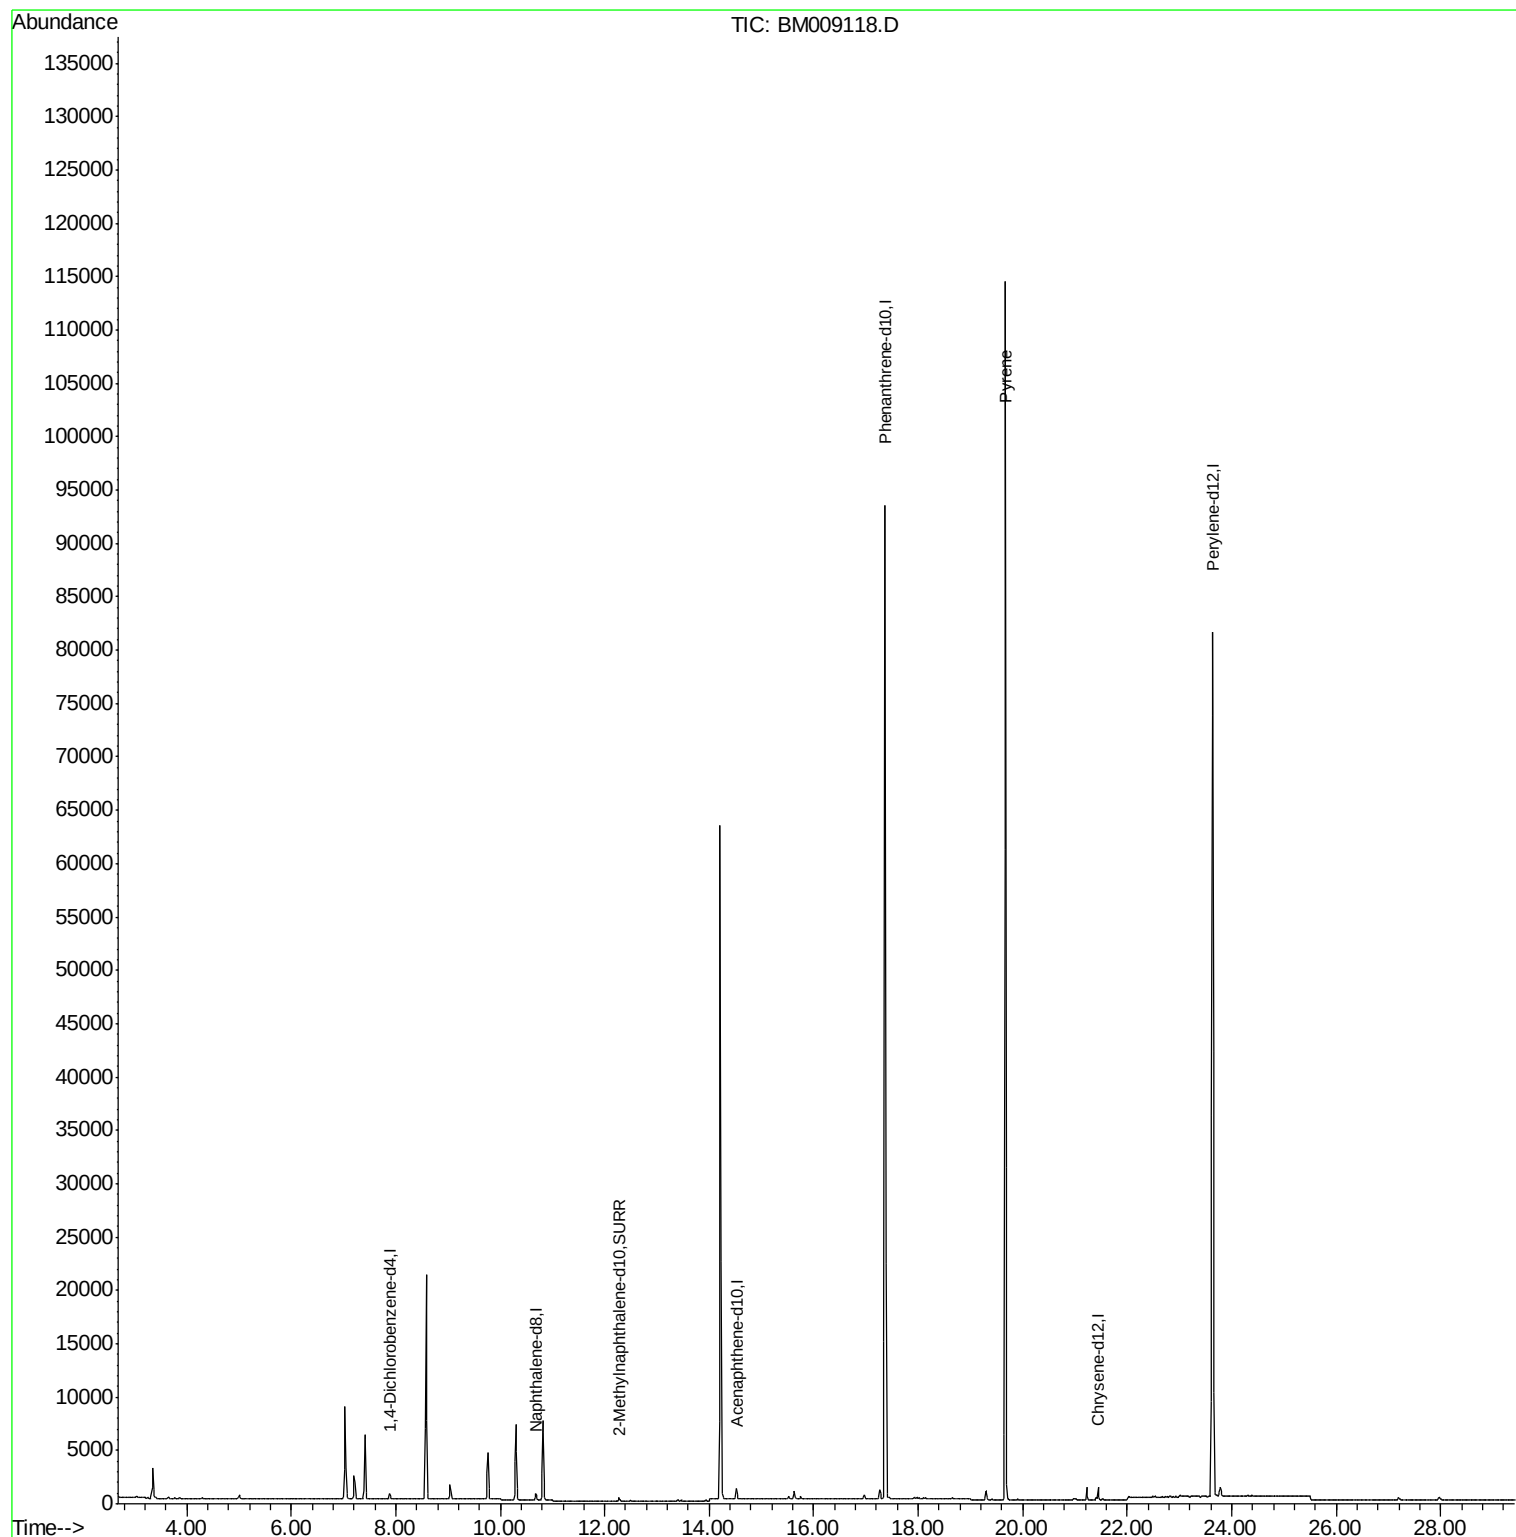

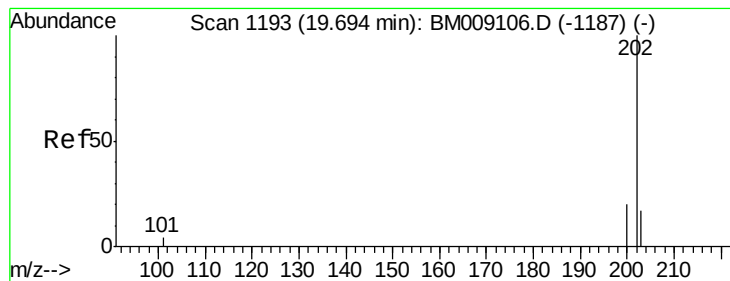

#17
 Pyrene
 Concen: 0.07 ng/ul
 RT: 19.67 min Scan# 1191
 Delta R.T. -0.03 min
 Lab File: BM009118.D
 Acq: 08 Mar 2017 20:29

Instrument :
 BNA_M
 ClientSampleId :
 C0AD6

Tgt Ion: 202 Resp: 316
 Ion Ratio Lower Upper
 202 100
 200 24.7 18.2 27.4
 203 182.8 15.6 23.4#

