

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM030817\
 Data File : BM009119.D
 Acq On : 08 Mar 2017 21:05
 Operator : SJ/MA
 Sample : I2062-15
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AD7

Quant Time: Mar 09 01:20:47 2017
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030317.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 09 01:19:41 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.88	152	282	0.40	ng/ul	-0.02
2) Naphthalene-d8	10.69	136	928	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.52	164	556	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.36	188	109979	0.40	ng/ul	0.10
16) Chrysene-d12	21.45	240	1196	0.40	ng/ul	0.00
20) Perylene-d12	23.64	264	77755	0.40	ng/ul	-0.15
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.27	152	523	0.34	ng/ul	-0.01
14) Fluoranthene-d10	19.30	212	1221	0.00	ng/ul	0.00
Target Compounds						
17) Pyrene	19.69	202	504	0.12	ng/ul#	68
18) Benzo(a)anthracene	21.43	228	308	0.08	ng/ul#	65
19) Chrysene	21.48	228	528	0.14	ng/ul#	82


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM030817\
Data File : BM009119.D
Acq On : 08 Mar 2017 21:05
Operator : SJ/MA
Sample : I2062-15
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AD7

Quant Time: Mar 09 01:20:47 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 09 01:19:41 2017
Response via : Initial Calibration

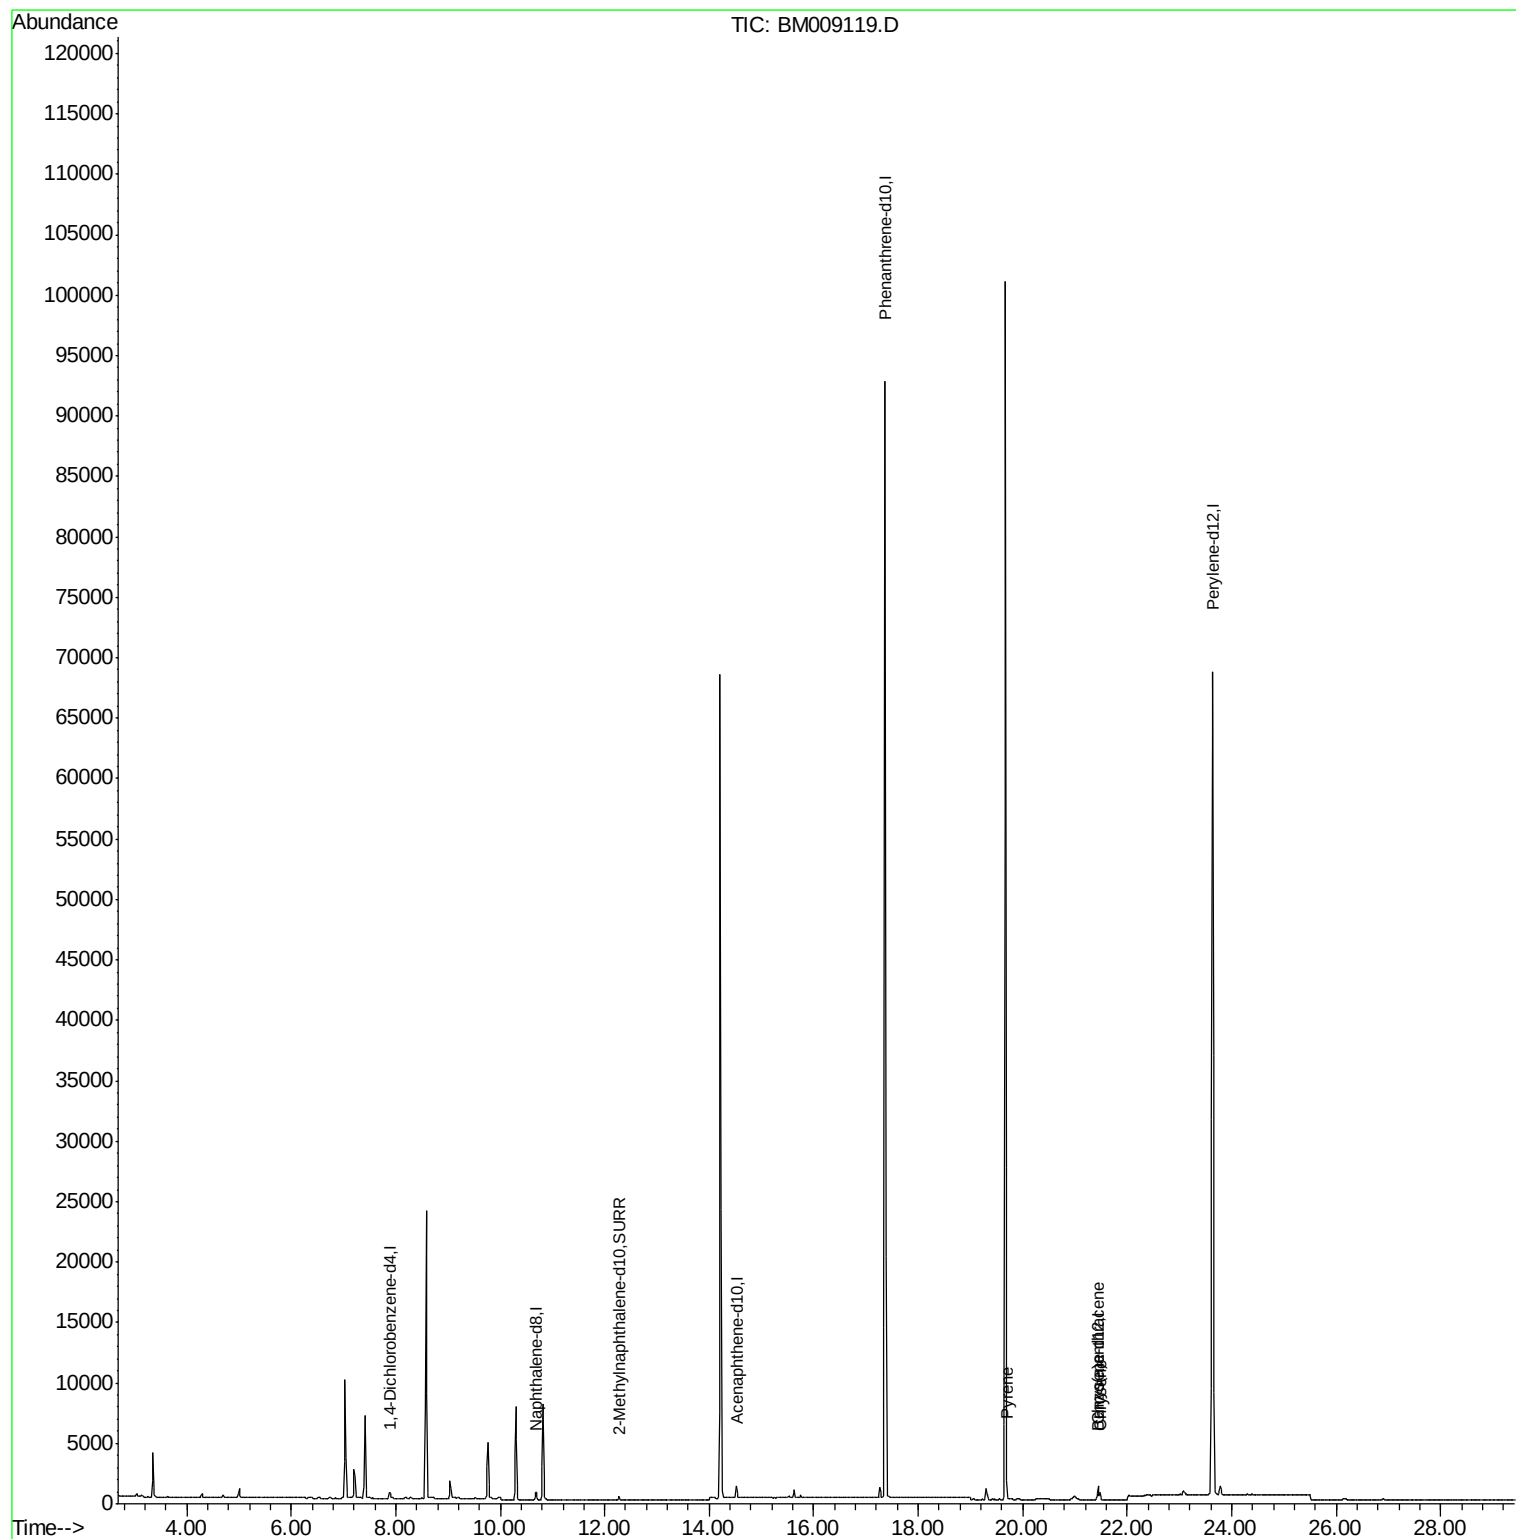

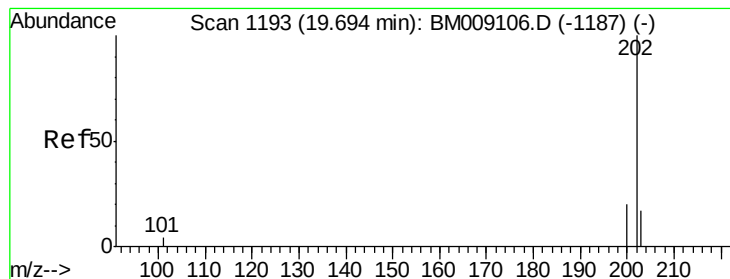

#17

Pyrene

Concen: 0.12 ng/ul

RT: 19.69 min Scan# 1193

Delta R.T. -0.00 min

Lab File: BM009119.D

Acq: 08 Mar 2017 21:05

Instrument :

BNA_M

ClientSampleId :

C0AD7


Tgt Ion:202 Resp: 504

Ion Ratio Lower Upper

202 100

200 36.0 18.2 27.4#




203 36.3 15.6 23.4#

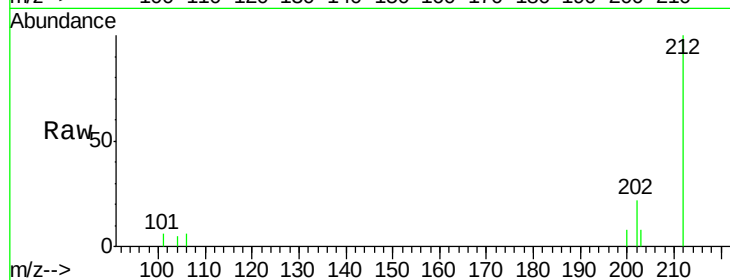

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 200.00 (199.70 to 200.70): E

Ion 203.00 (202.70 to 203.70): E

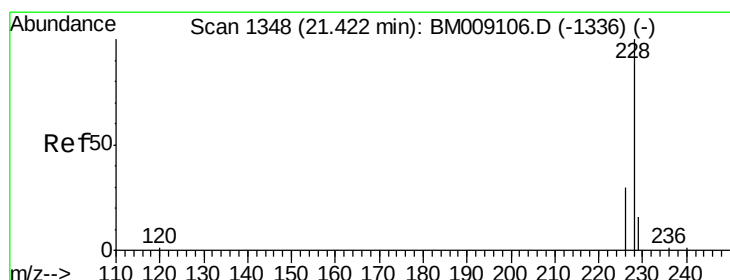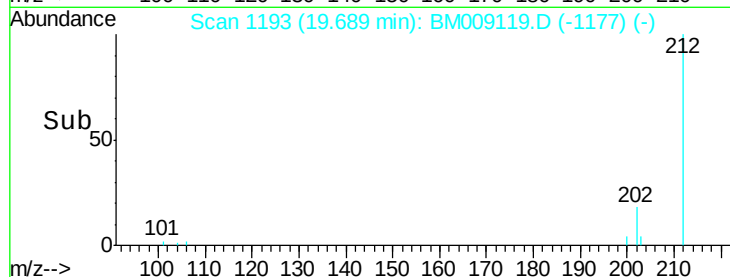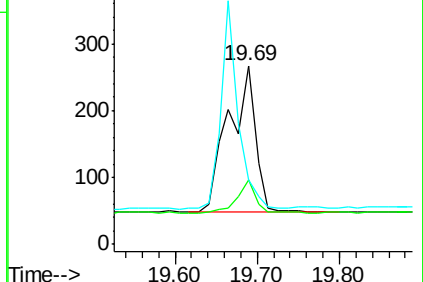

#18

Benzo(a)anthracene

Concen: 0.08 ng/ul

RT: 21.43 min Scan# 1349

Delta R.T. 0.01 min

Lab File: BM009119.D

Acq: 08 Mar 2017 21:05


Tgt Ion:228 Resp: 308

Ion Ratio Lower Upper

228 100

226 42.8 22.8 34.2#



229 42.4 17.0 25.6#



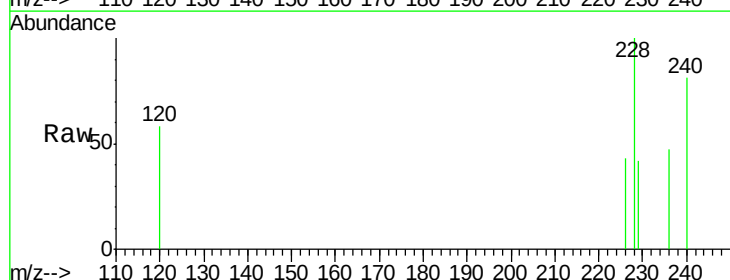


Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

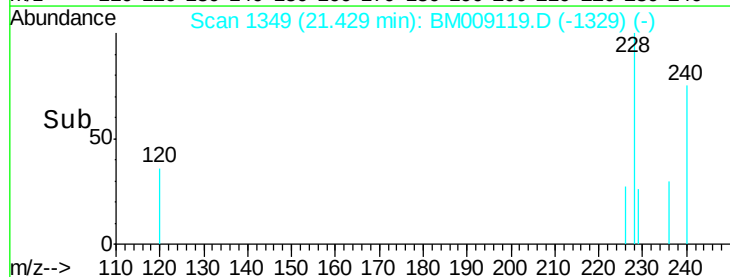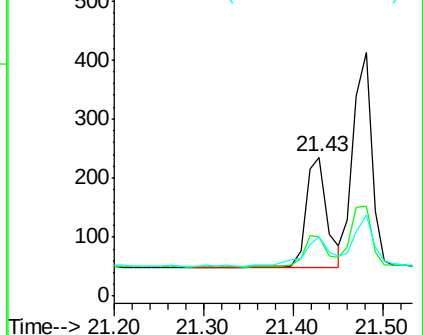

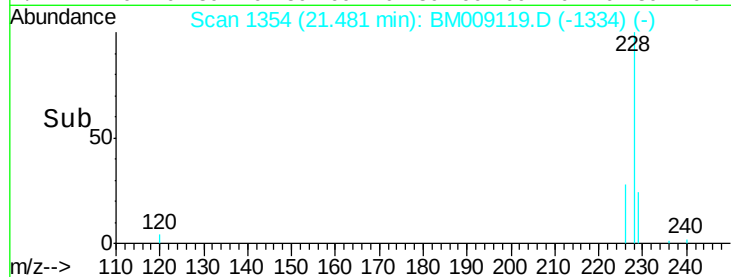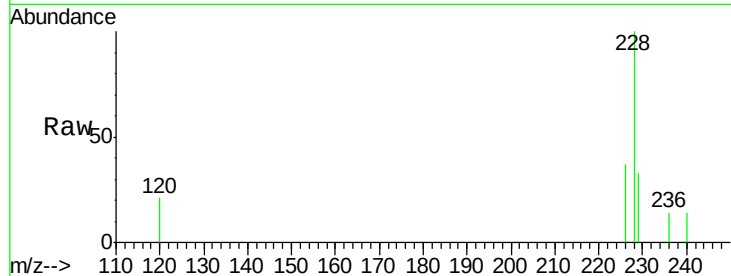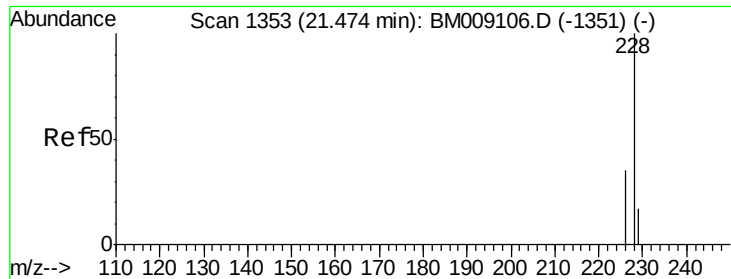

#19

Chrysene

Concen: 0.14 ng/ul

RT: 21.48 min Scan# 1354

Delta R.T. 0.01 min

Lab File: BM009119.D

Acq: 08 Mar 2017 21:05

Instrument :

BNA_M

ClientSampleId :

C0AD7

Tgt Ion: 228 Resp: 528

Ion Ratio Lower Upper

228 100

226 37.1 23.4 35.0#

229 33.3 17.7 26.5#

