

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM030817\
 Data File : BM009129.D
 Acq On : 09 Mar 2017 05:11
 Operator : SJ/MA
 Sample : I2069-02
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AG4

Quant Time: Mar 09 05:59:47 2017
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030317.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 09 02:44:03 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.88	152	282	0.40	ng/ul	0.00
2) Naphthalene-d8	10.68	136	879	0.40	ng/ul	-0.01
6) Acenaphthene-d10	14.52	164	503	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.36	188	64399	0.40	ng/ul	0.10
16) Chrysene-d12	21.44	240	1116	0.40	ng/ul	0.00
20) Perylene-d12	23.63	264	58323	0.40	ng/ul	-0.15
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.27	152	310	0.21	ng/ul	0.00
14) Fluoranthene-d10	19.30	212	725	0.00	ng/ul	0.00
Target Compounds						
8) Acenaphthene	14.59	153	73	0.04	ng/ul#	80
9) Fluorene	15.58	166	120	0.05	ng/ul#	83
17) Pyrene	19.66	202	176	0.05	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM030817\
Data File : BM009129.D
Acq On : 09 Mar 2017 05:11
Operator : SJ/MA
Sample : I2069-02
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AG4

Quant Time: Mar 09 05:59:47 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 09 02:44:03 2017
Response via : Initial Calibration

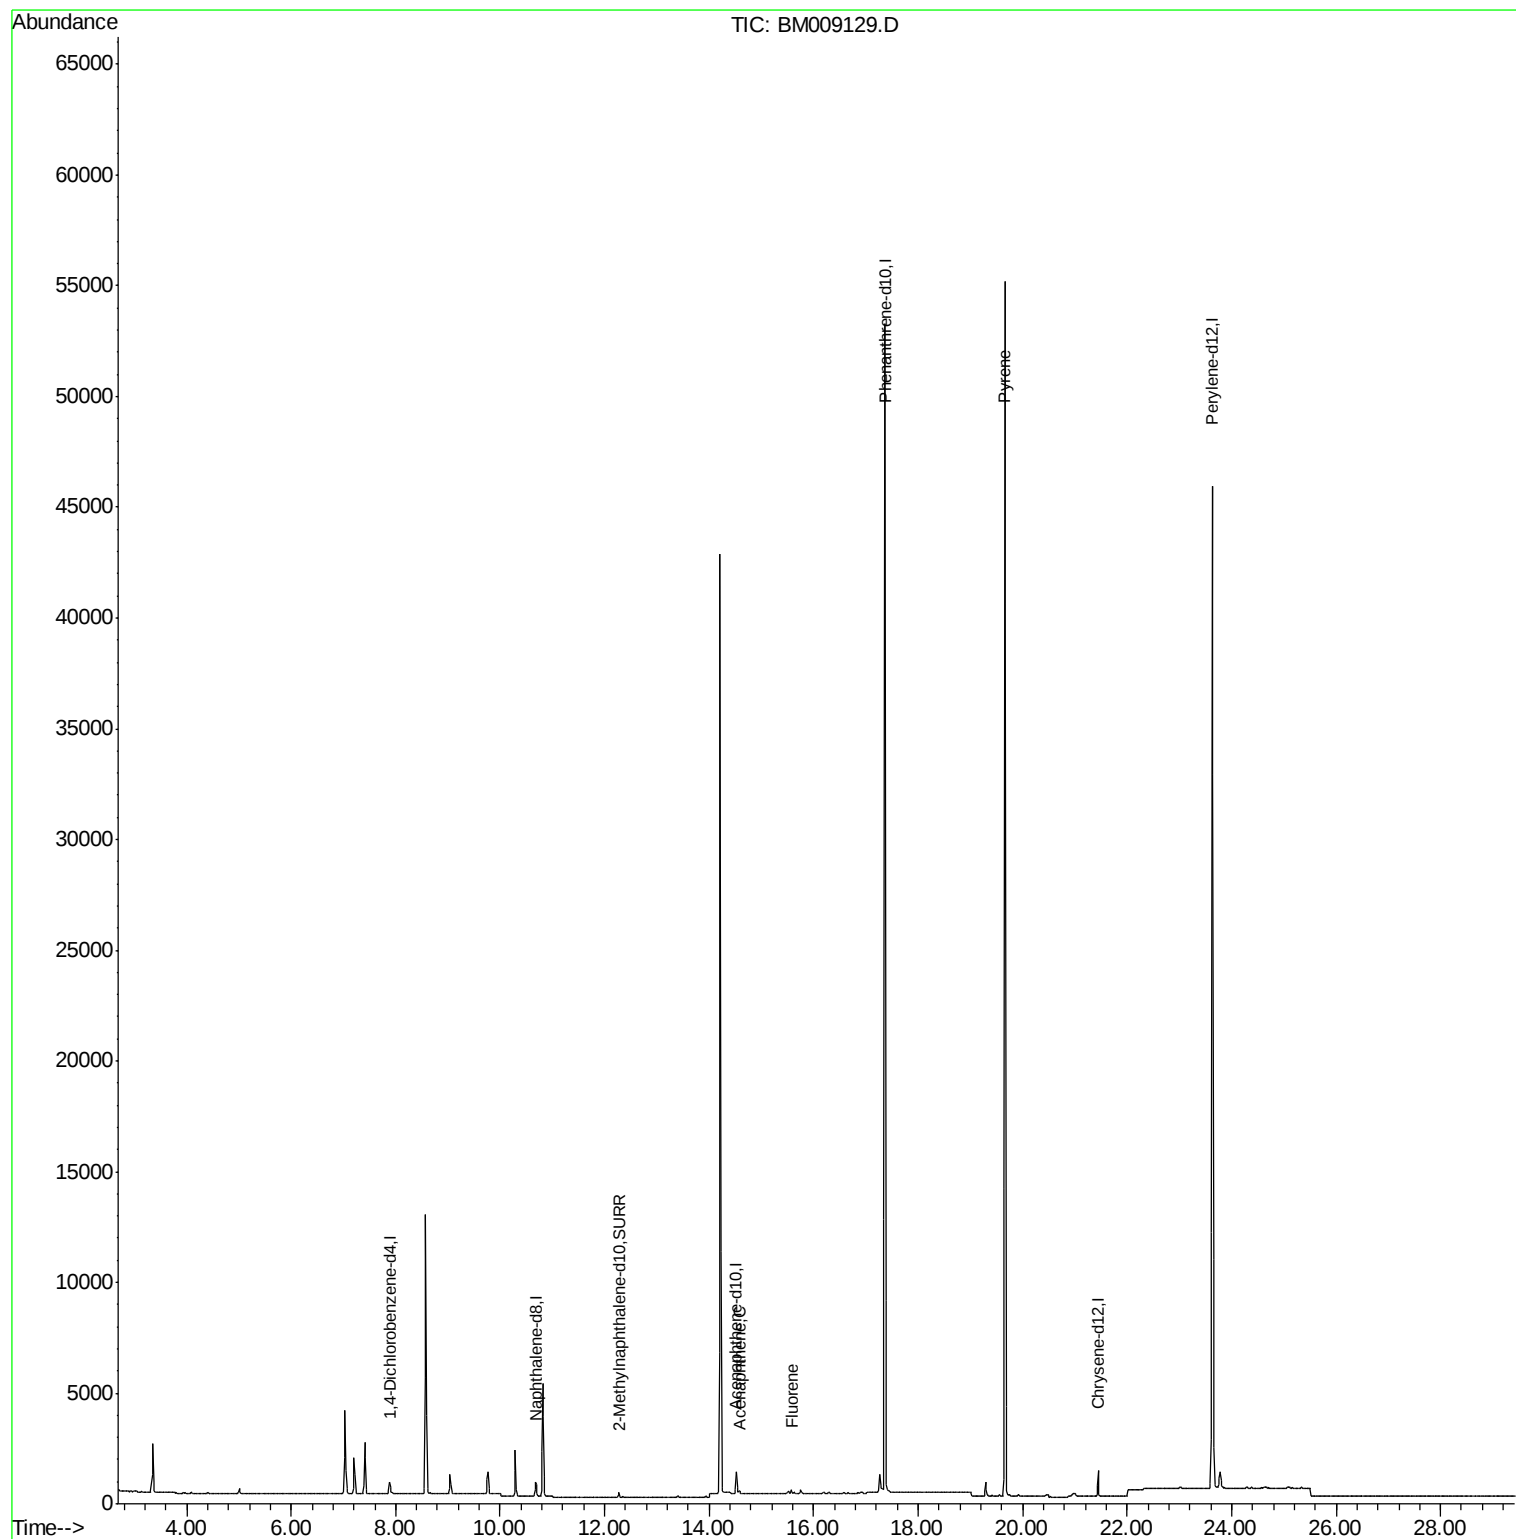

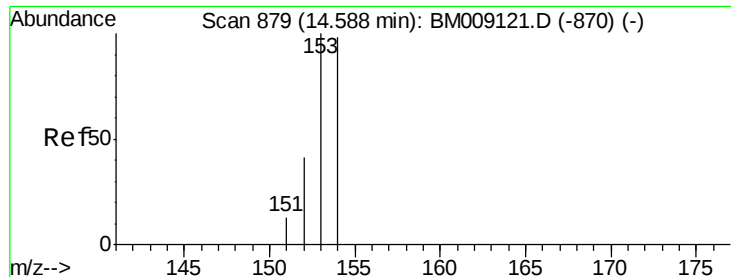

#8

Acenaphthene

Concen: 0.04 ng/ul

RT: 14.59 min Scan# 879

Delta R.T. 0.00 min

Lab File: BM009129.D

Acq: 09 Mar 2017 05:11

Instrument :





BNA_M

ClientSampleId :

C0AG4

Tgt Ion:153 Resp: 73

Ion	Ratio	Lower	Upper
153	100		
152	75.6	40.3	60.5#
154	98.8	71.4	107.2

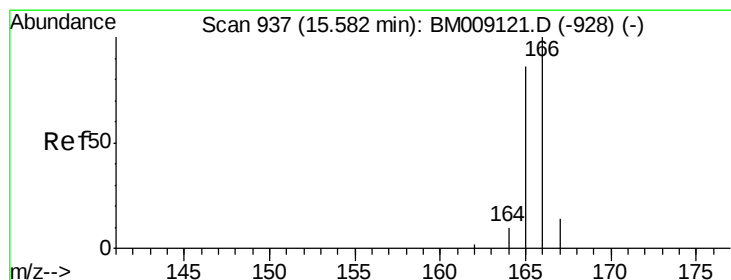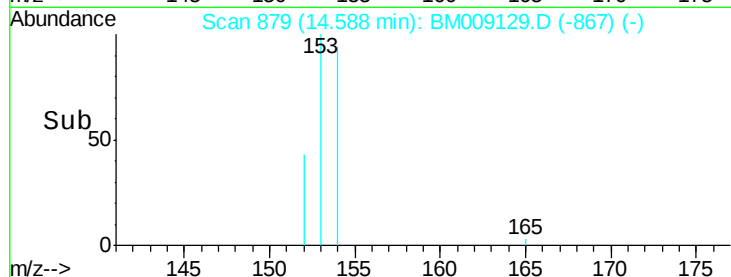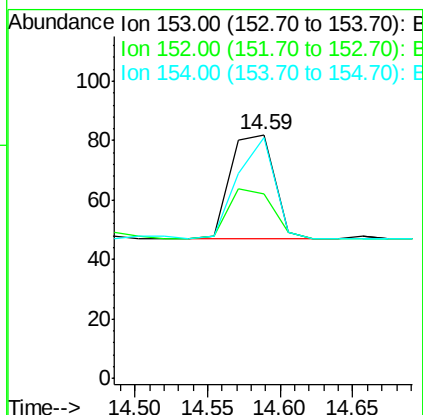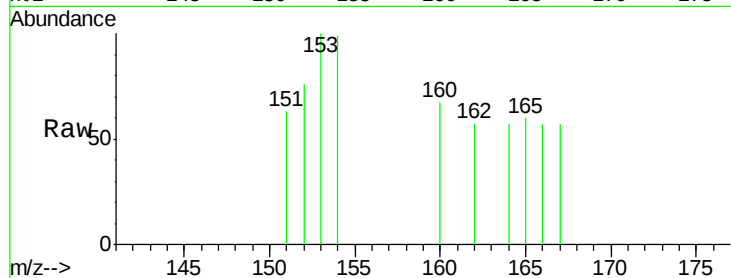

#9

Fluorene

Concen: 0.05 ng/ul

RT: 15.58 min Scan# 937




Delta R.T. 0.00 min




Lab File: BM009129.D

Acq: 09 Mar 2017 05:11

Tgt Ion:166 Resp: 120

Ion	Ratio	Lower	Upper
166	100		
165	95.2	73.4	110.2
167	55.2	14.6	22.0#

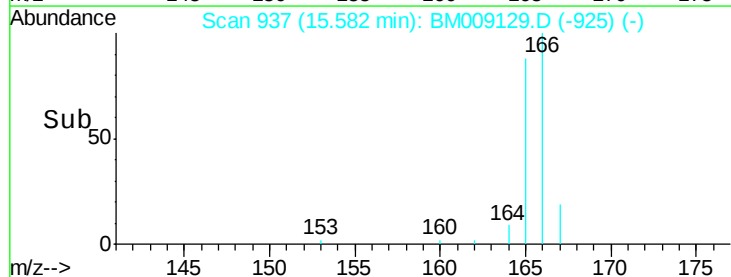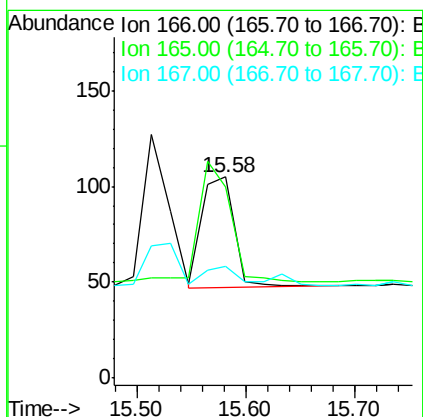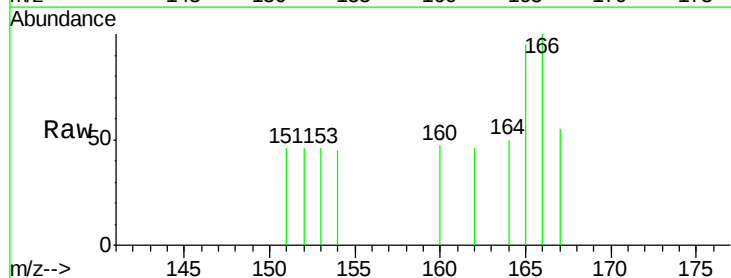

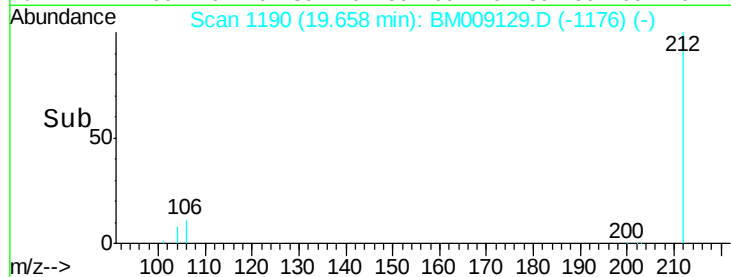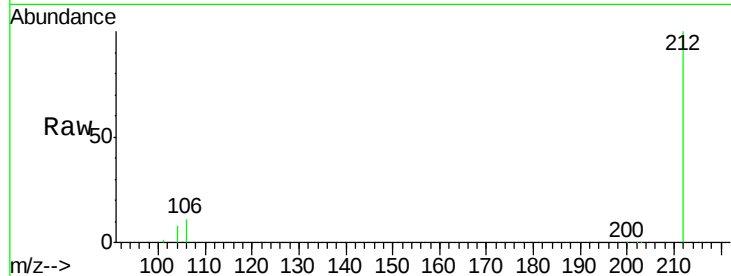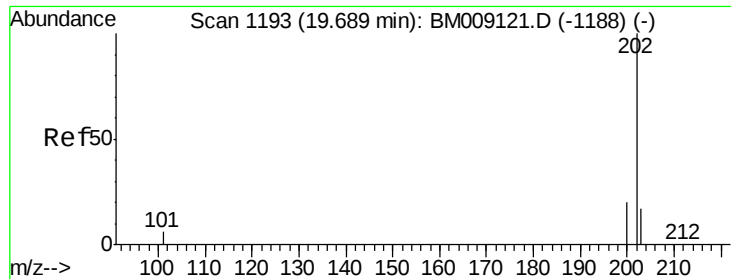

#17

Pyrene

Concen: 0.05 ng/ul

RT: 19.66 min Scan# 1190

Delta R.T. -0.03 min

Lab File: BM009129.D

Acq: 09 Mar 2017 05:11

Instrument :

BNA_M

ClientSampleId :

C0AG4

Tgt Ion: 202 Resp: 176

Ion Ratio Lower Upper

202 100

200 36.2 18.2 27.4#

203 133.3 15.6 23.4#

