

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM030817\
 Data File : BM009130.D
 Acq On : 09 Mar 2017 05:47
 Operator : SJ/MA
 Sample : I2069-03
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AG5

Quant Time: Mar 09 06:23:05 2017
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030317.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 09 02:44:03 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.88	152	278	0.40	ng/ul	0.00
2) Naphthalene-d8	10.68	136	891	0.40	ng/ul	-0.01
6) Acenaphthene-d10	14.52	164	532	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.36	188	76934	0.40	ng/ul	0.10
16) Chrysene-d12	21.44	240	1327	0.40	ng/ul	-0.01
20) Perylene-d12	23.63	264	79597	0.40	ng/ul	-0.16
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.27	152	369	0.25	ng/ul	0.00
14) Fluoranthene-d10	19.54	212	36	0.00	ng/ul	0.24
Target Compounds						
17) Pyrene	19.66	202	224	0.05	ng/ul#	1
18) Benzo(a)anthracene	21.43	228	113	0.03	ng/ul#	13


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM030817\
Data File : BM009130.D
Acq On : 09 Mar 2017 05:47
Operator : SJ/MA
Sample : I2069-03
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AG5

Quant Time: Mar 09 06:23:05 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 09 02:44:03 2017
Response via : Initial Calibration

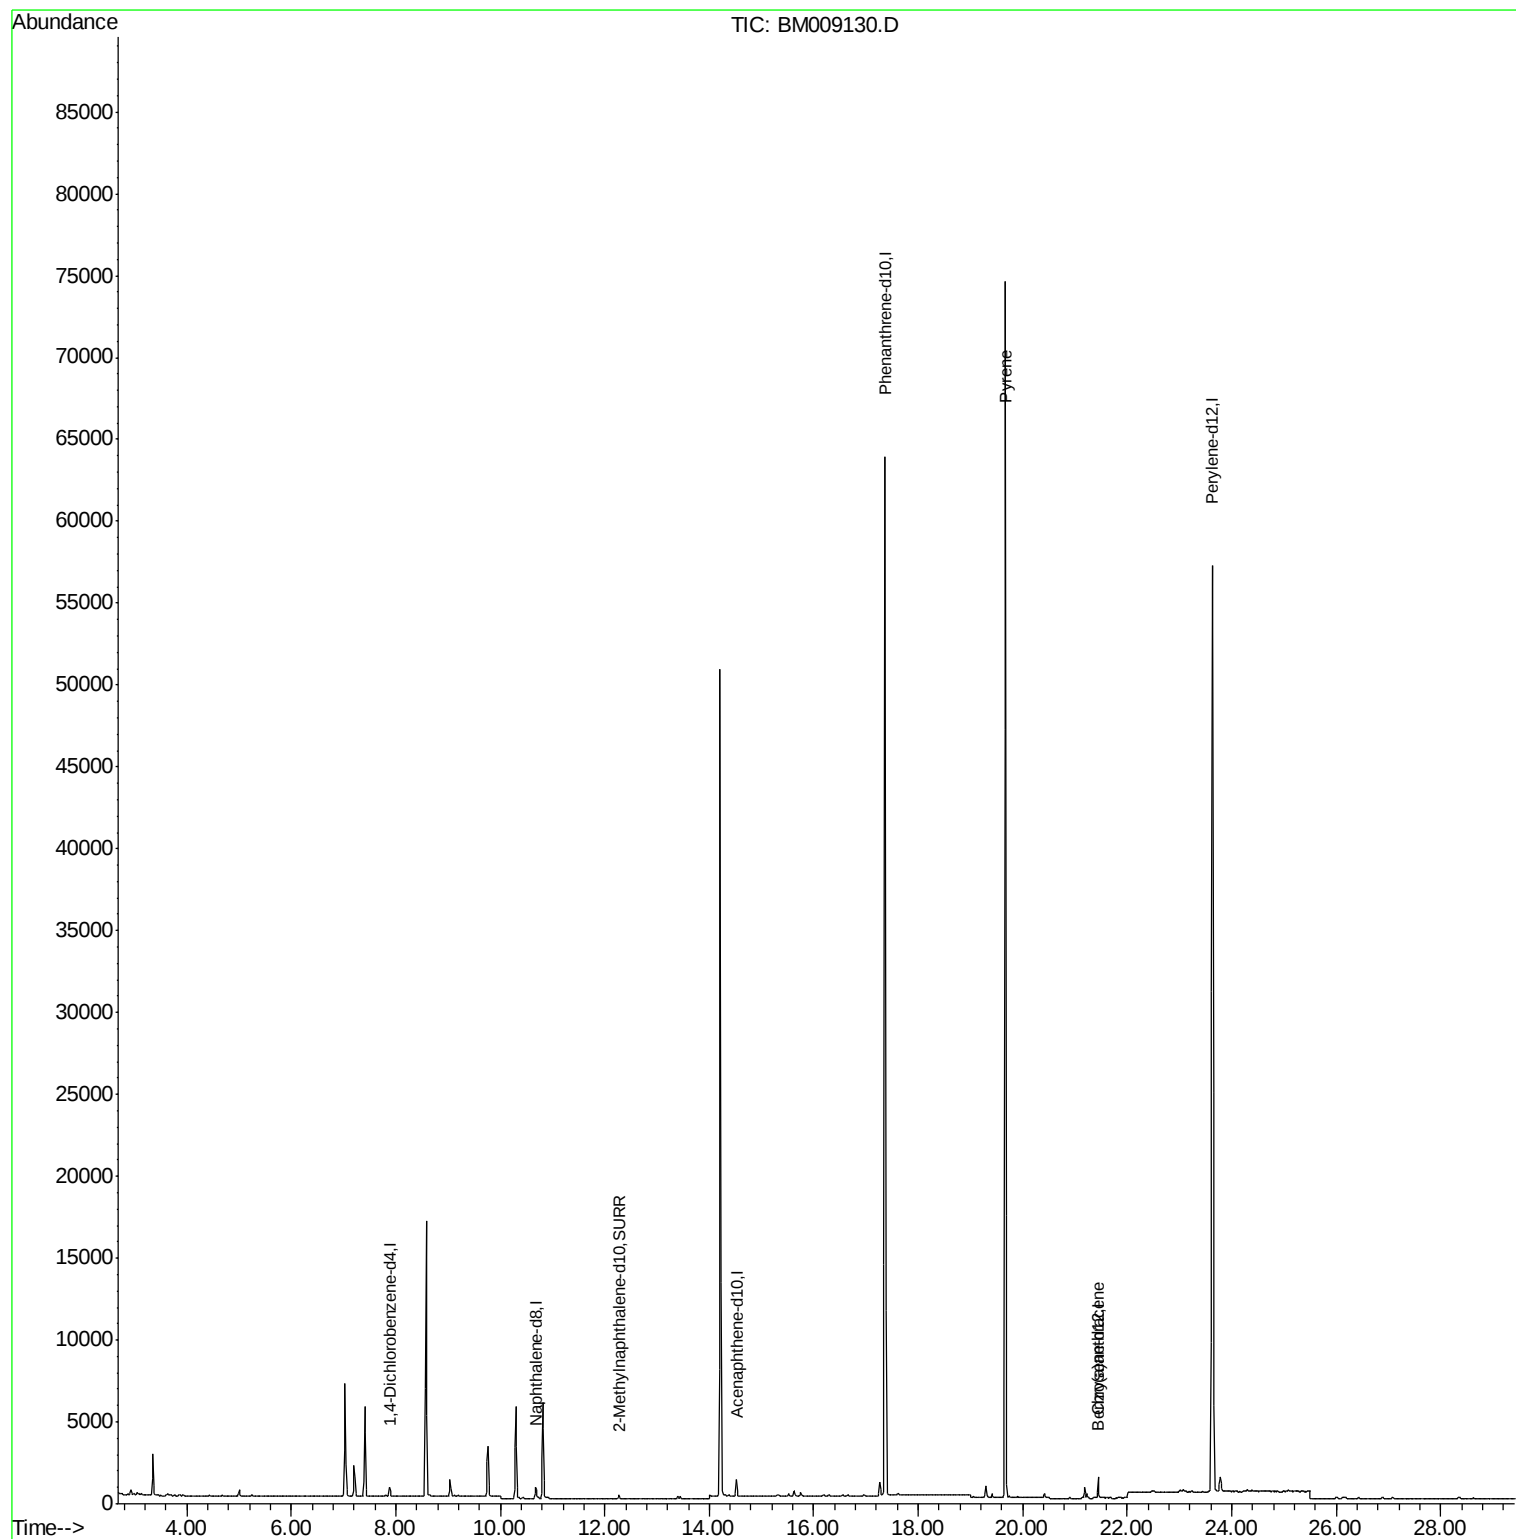

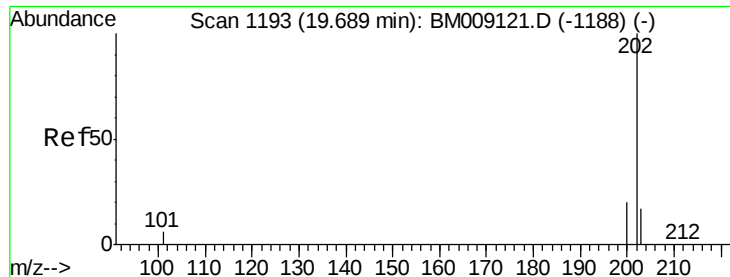

#17

Pyrene

Concen: 0.05 ng/ul

RT: 19.66 min Scan# 1191

Delta R.T. -0.02 min

Lab File: BM009130.D

Acq: 09 Mar 2017 05:47

Instrument :

BNA_M

ClientSampleId :

C0AG5


Tgt Ion:202 Resp: 224

Ion Ratio Lower Upper

202 100

200 34.2 18.2 27.4#




203 173.5 15.6 23.4#

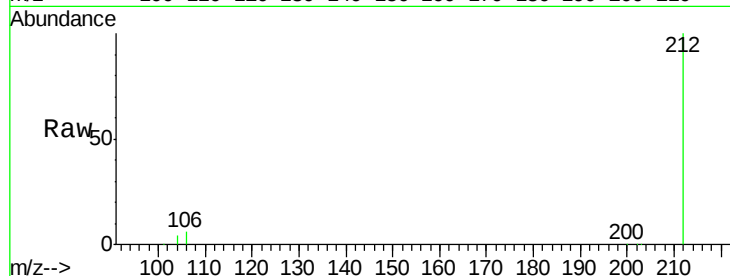

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 200.00 (199.70 to 200.70): E

Ion 203.00 (202.70 to 203.70): E

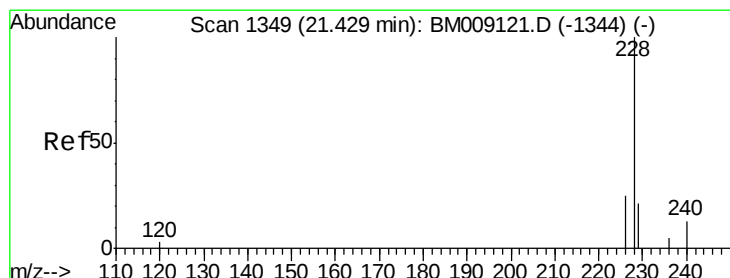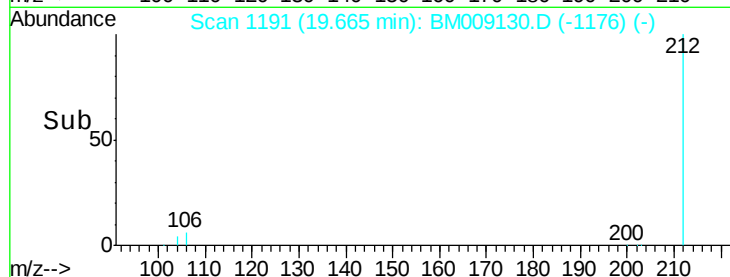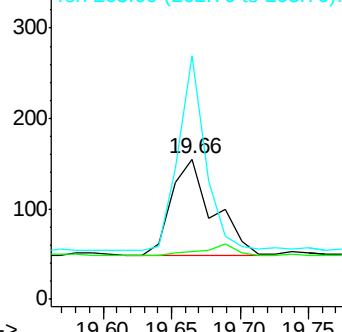

#18

Benzo(a)anthracene

Concen: 0.03 ng/ul

RT: 21.43 min Scan# 1349

Delta R.T. 0.00 min

Lab File: BM009130.D

Acq: 09 Mar 2017 05:47


Tgt Ion:228 Resp: 113

Ion Ratio Lower Upper

228 100

226 67.4 22.8 34.2#

229 70.5 17.0 25.6#

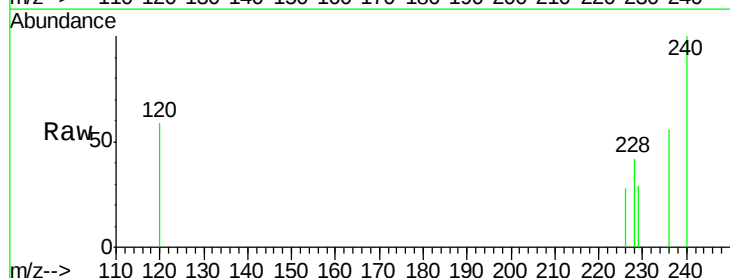

Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

