

Data Path : Z:\HPCHEM1\BNA_M\Data\BM030817\
 Data File : BM009135.D
 Acq On : 09 Mar 2017 08:46
 Operator : SJ/MA
 Sample : I2069-10
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AH3

Quant Time: Mar 09 10:28:59 2017
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030317.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 09 02:44:03 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.88	152	239	0.40	ng/ul	0.00
2) Naphthalene-d8	10.68	136	790	0.40	ng/ul	-0.01
6) Acenaphthene-d10	14.52	164	492	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.36	188	98322	0.40	ng/ul	0.10
16) Chrysene-d12	21.44	240	1289	0.40	ng/ul	-0.01
20) Perylene-d12	23.63	264	101190	0.40	ng/ul	-0.16
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.27	152	428	0.33	ng/ul	0.00
14) Fluoranthene-d10	19.29	212	1190	0.00	ng/ul	-0.01
Target Compounds						
					Qvalue	
17) Pyrene	19.66	202	365	0.08	ng/ul#	1
18) Benzo(a)anthracene	21.43	228	112	0.03	ng/ul#	33
19) Chrysene	21.47	228	93	0.02	ng/ul#	29


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\Data\BM030817\
Data File : BM009135.D
Acq On : 09 Mar 2017 08:46
Operator : SJ/MA
Sample : I2069-10
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AH3

Quant Time: Mar 09 10:28:59 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 09 02:44:03 2017
Response via : Initial Calibration




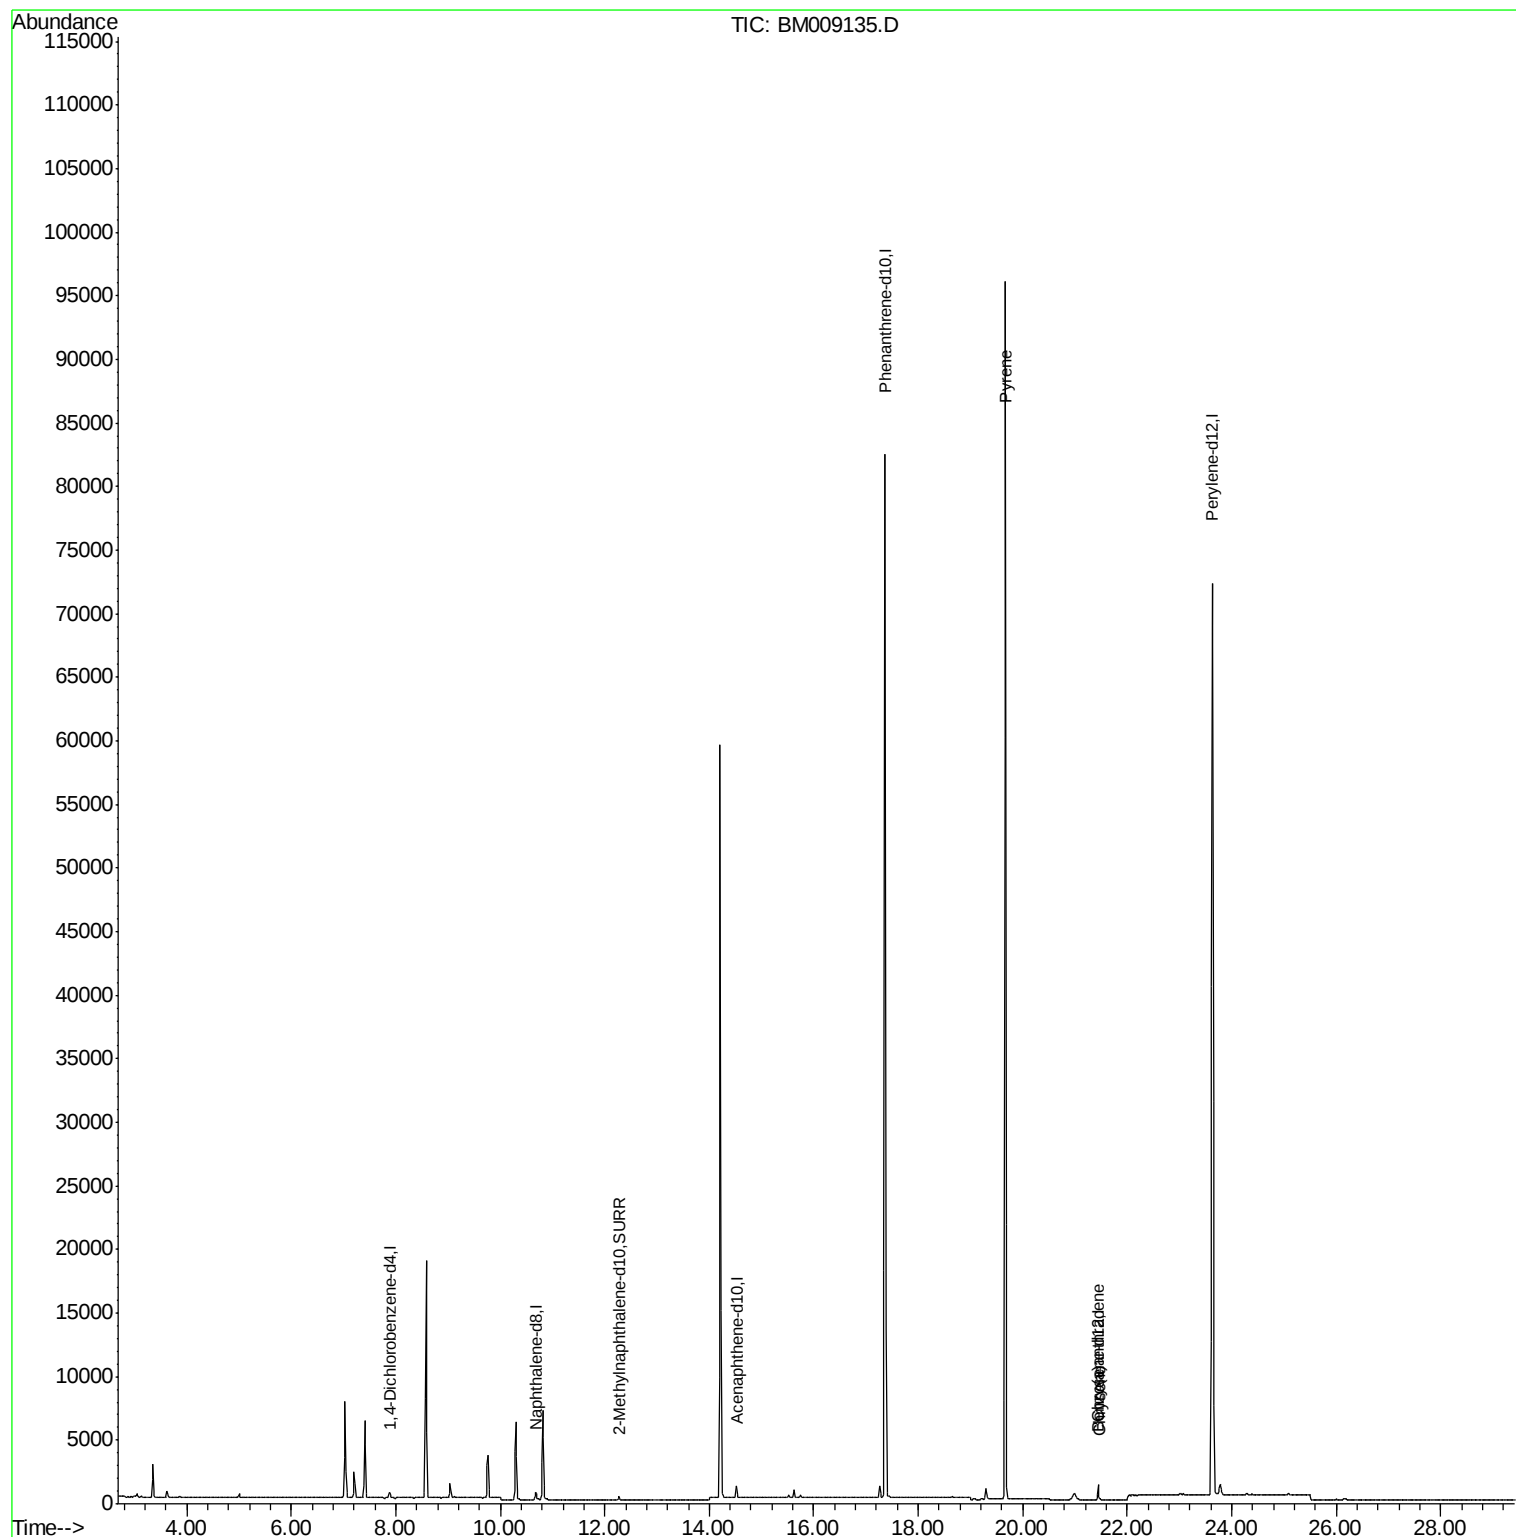


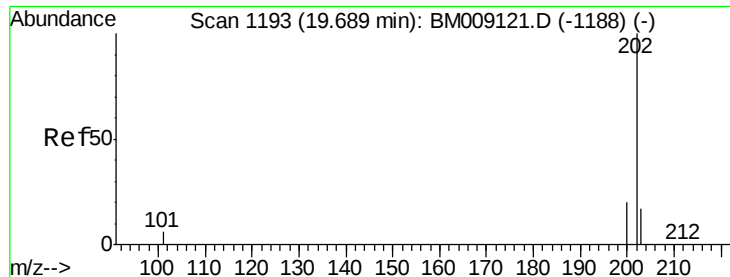

#17
Pyrene
Concen: 0.08 ng/ul
RT: 19.66 min Scan# 1191
Delta R.T. -0.02 min
Lab File: BM009135.D
Acq: 09 Mar 2017 08:46




Instrument :
BNA_M
ClientSampleId :
C0AH3


Tgt Ion: 202 Resp: 365
Ion Ratio Lower Upper
202 100
200 28.6 18.2 27.4#
203 186.2 15.6 23.4#

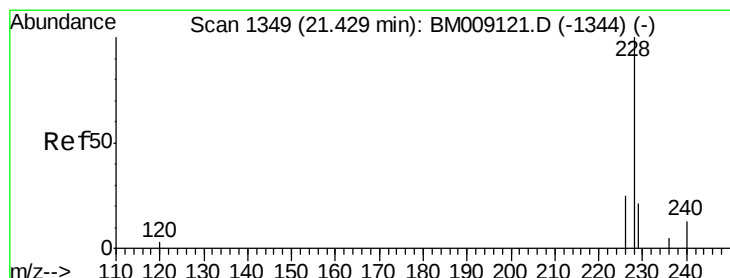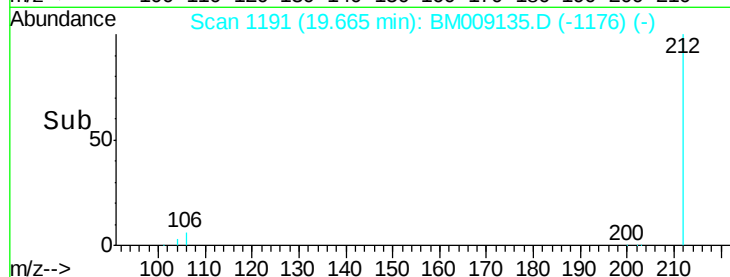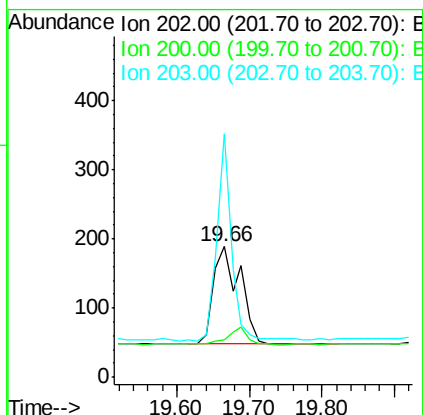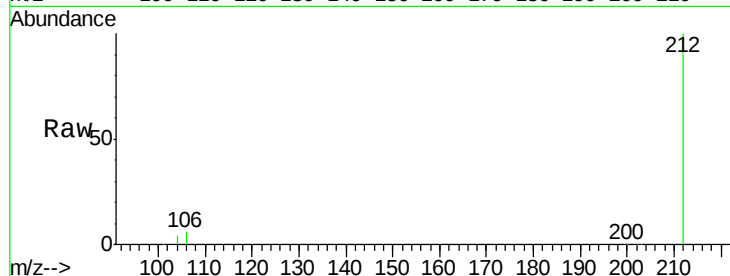

#18
Benzo(a)anthracene
Concen: 0.03 ng/ul
RT: 21.43 min Scan# 1349
Delta R.T. 0.00 min
Lab File: BM009135.D
Acq: 09 Mar 2017 08:46

Tgt Ion: 228 Resp: 112
Ion Ratio Lower Upper
228 100
226 60.5 22.8 34.2#
229 57.0 17.0 25.6#

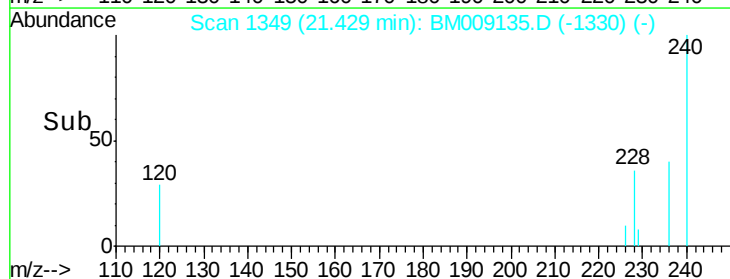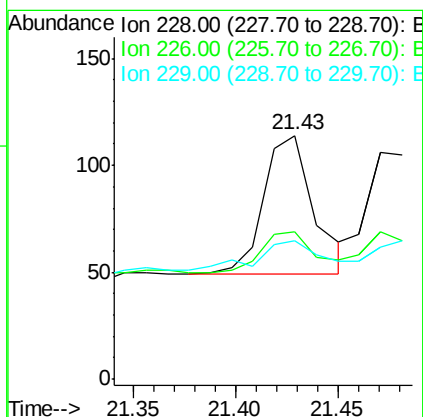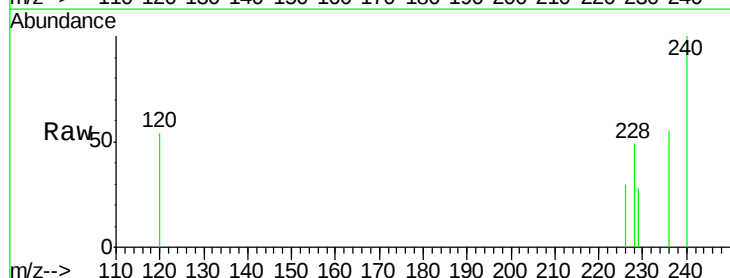

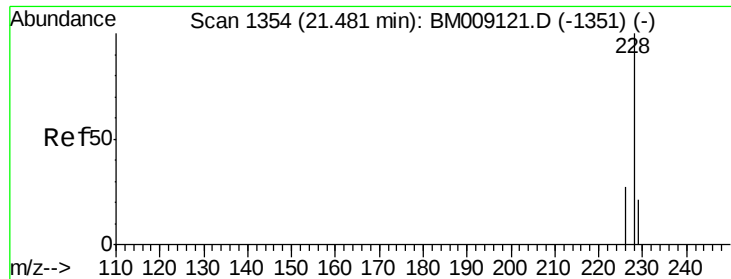

#19

Chrysene

Concen: 0.02 ng/ul

RT: 21.47 min Scan# 1353

Delta R.T. -0.01 min

Lab File: BM009135.D


Acq: 09 Mar 2017 08:46

Instrument :

BNA_M

ClientSampleId :

C0AH3

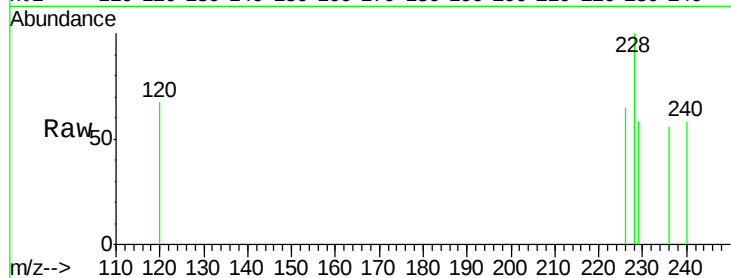

Tgt Ion: 228 Resp: 93

Ion Ratio Lower Upper

228 100

226 65.1 23.4 35.0#

229 58.5 17.7 26.5#

