




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM030817\
Data File : BM009127.D
Acq On : 09 Mar 2017 03:59
Operator : SJ/MA
Sample : I2062-11
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AD0

Manual Integrations
APPROVED

mohammad
3/9/2017 2:02:15 PM

Quant Time: Mar 09 04:52:26 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 09 02:44:03 2017
Response via : Initial Calibration

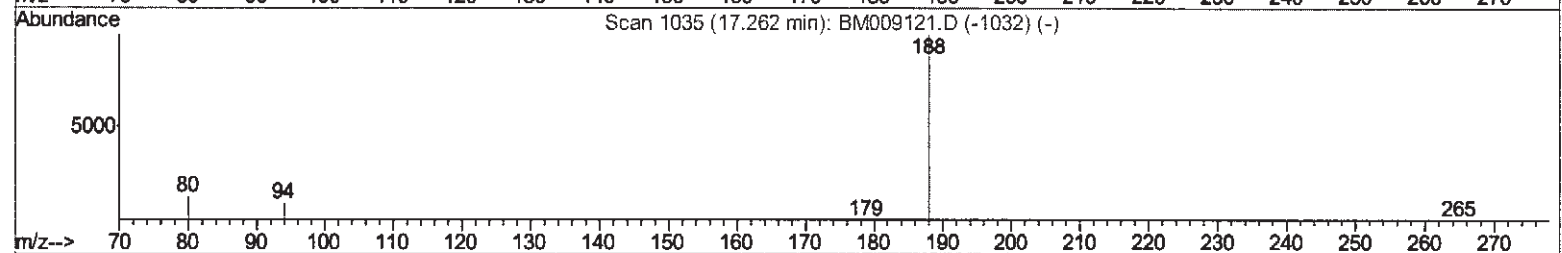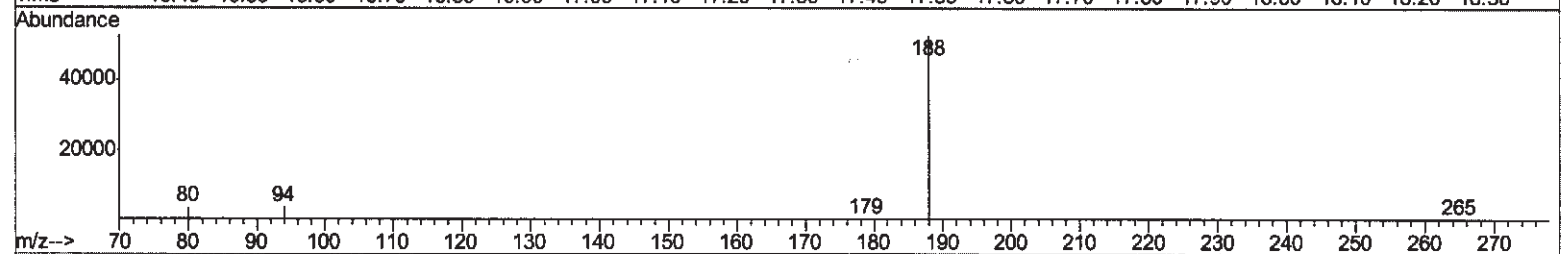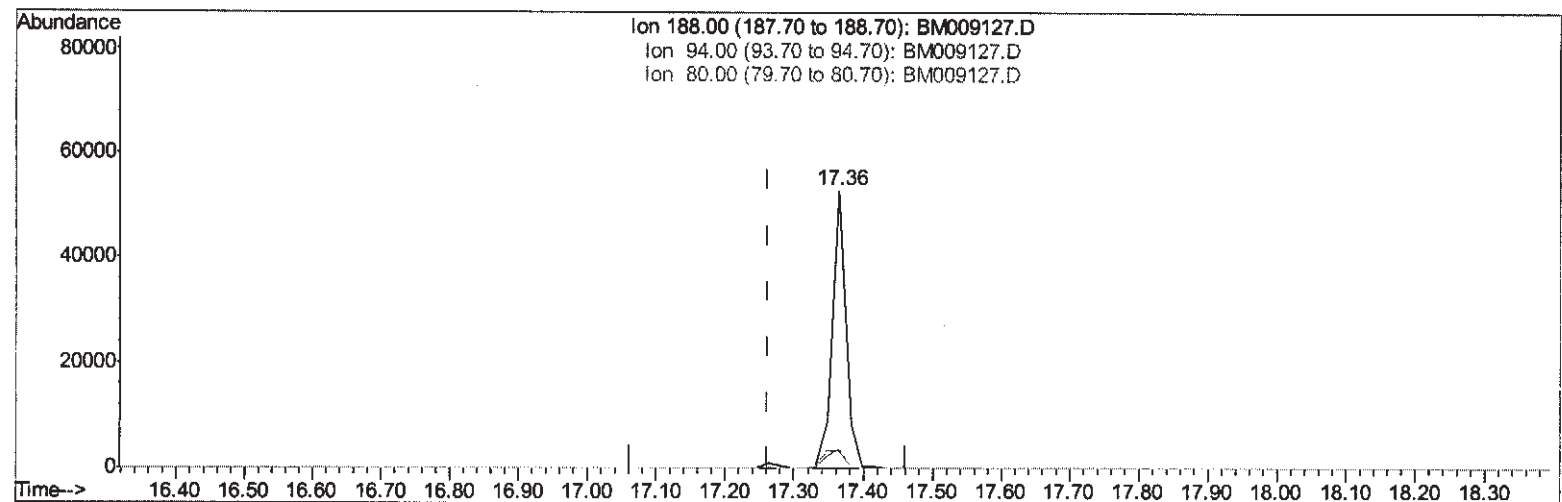

TIC: BM009127.D

(10) Phenanthrene-d10 (I)

17.365min (+0.103) 0.40ng/ul

response 72451

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	6.77#
80.00	11.80	6.58#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM030817\
Data File : BM009127.D
Acq On : 09 Mar 2017 03:59
Operator : SJ/MA
Sample : I2062-11
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleID :
C0AD0

Manual Integrations
APPROVED

mohammad
3/9/2017 2:02:15 PM

Quant Time: Mar 09 04:52:26 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 09 02:44:03 2017
Response via : Initial Calibration

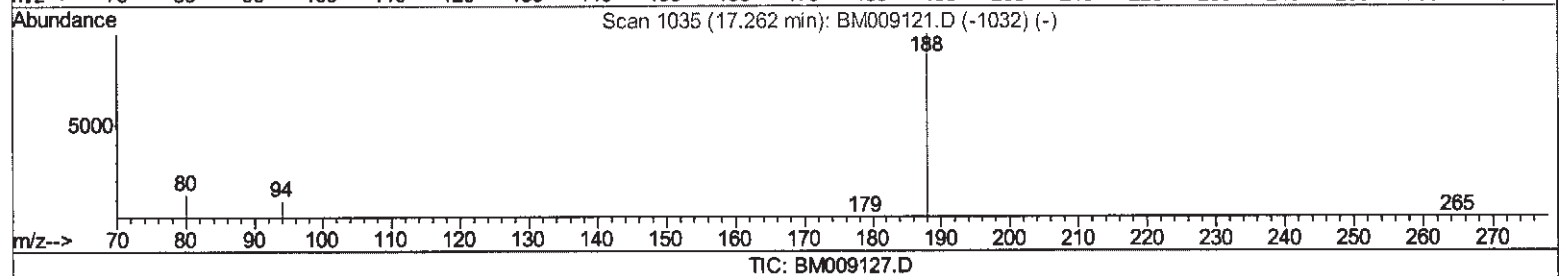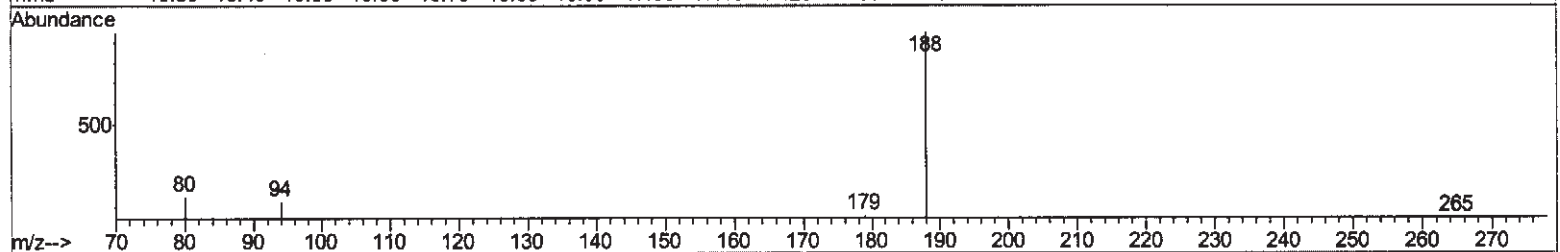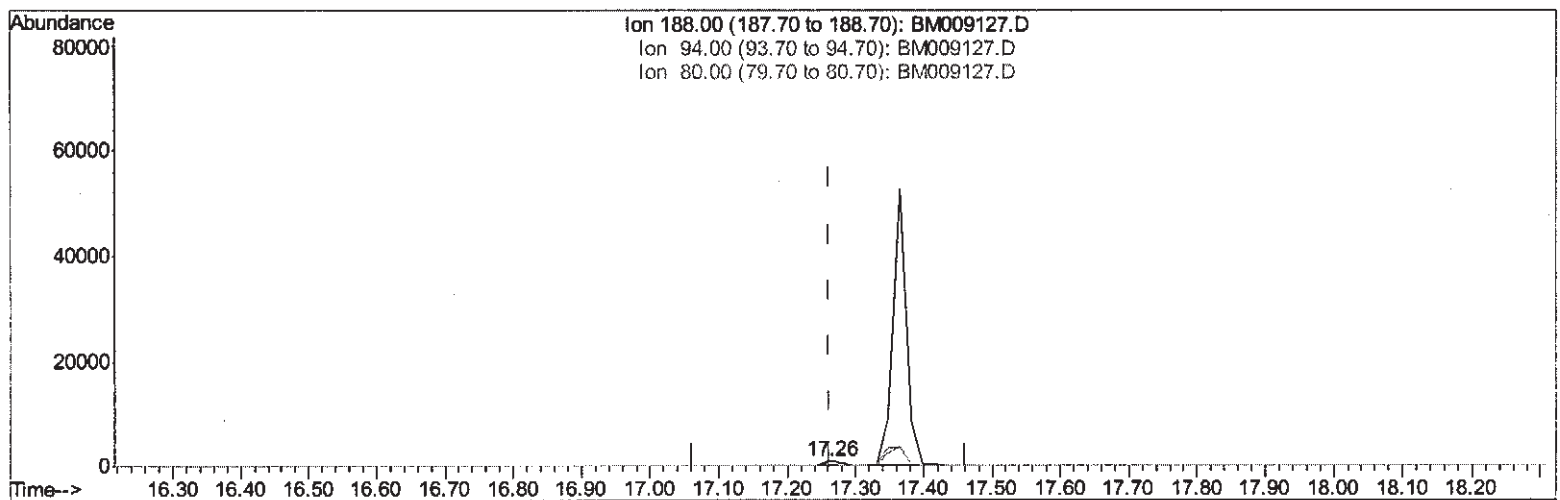

(10) Phenanthrene-d10 (I)

17.262min (+0.000) 0.40ng/ul m

SJ 3/16/17

response 1551

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	13.68#
80.00	11.80	16.21#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM030817\
Data File : BM009127.D
Acq On : 09 Mar 2017 03:59
Operator : SJ/MA
Sample : I2062-11
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AD0

Manual Integrations
APPROVED

mohammad
3/9/2017 2:02:15 PM

Quant Time: Mar 09 04:52:26 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 09 02:44:03 2017
Response via : Initial Calibration

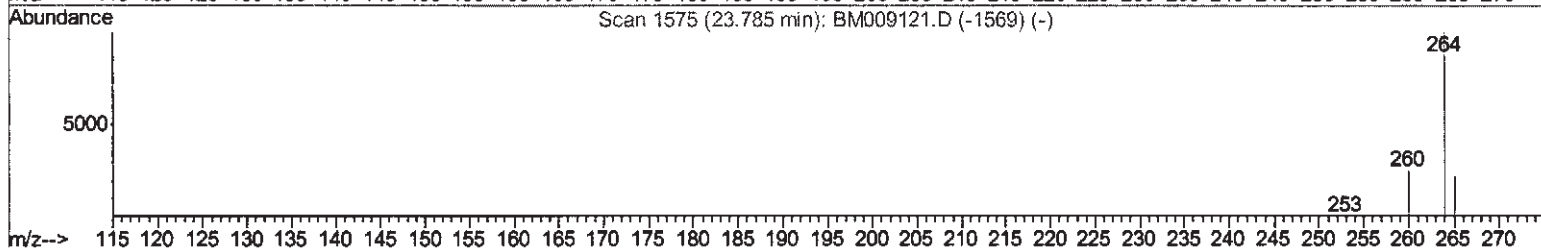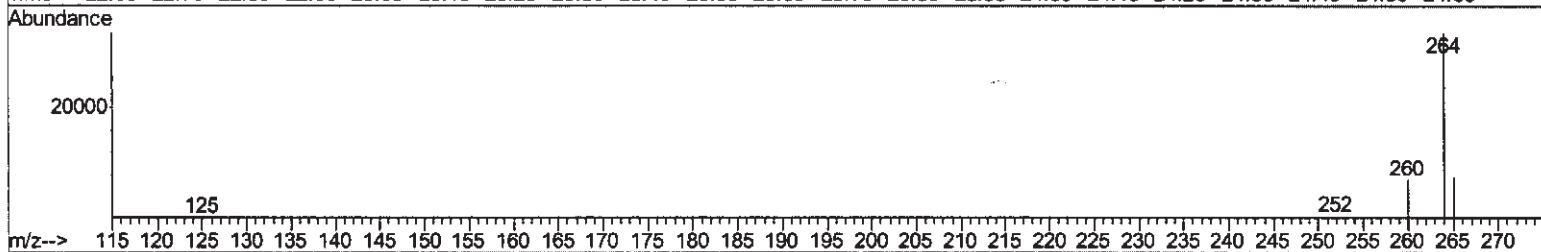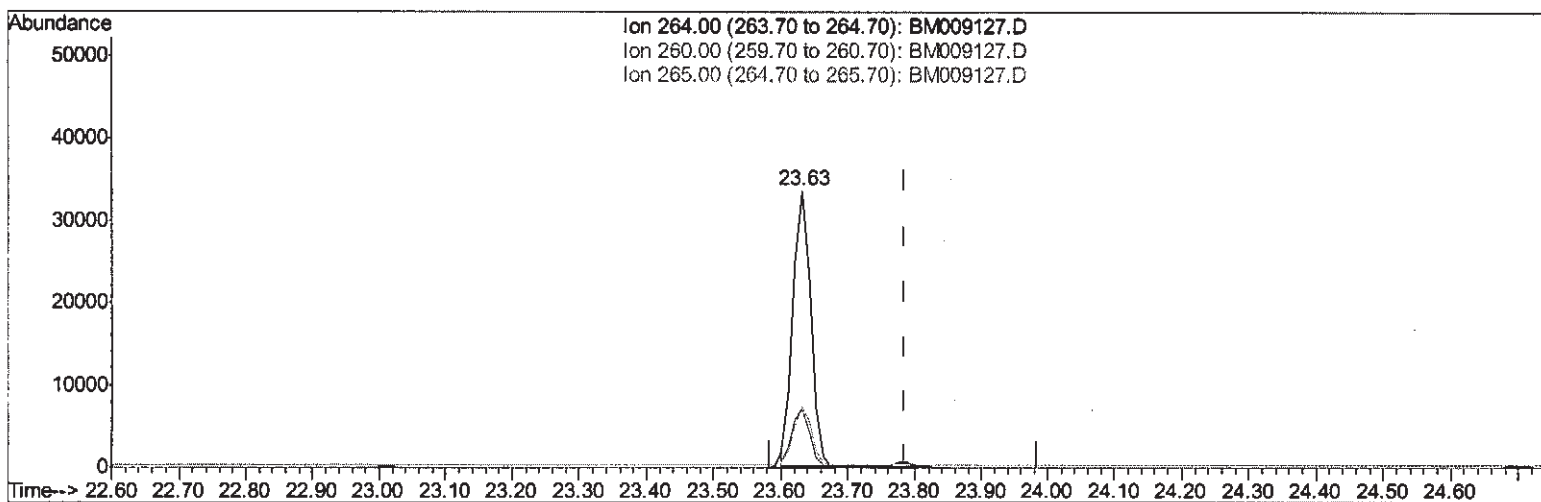

(20) Perylene-d12 (I)

23.632min (-0.153) 0.40ng/ul

response 61779

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	20.94#
265.00	103.50	22.18#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM030817\
Data File : BM009127.D
Acq On : 09 Mar 2017 03:59
Operator : SJ/MA
Sample : I2062-11
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AD0

Manual Integrations
APPROVED

mohammad
3/9/2017 2:02:15 PM

Quant Time: Mar 09 04:52:26 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 09 02:44:03 2017
Response via : Initial Calibration

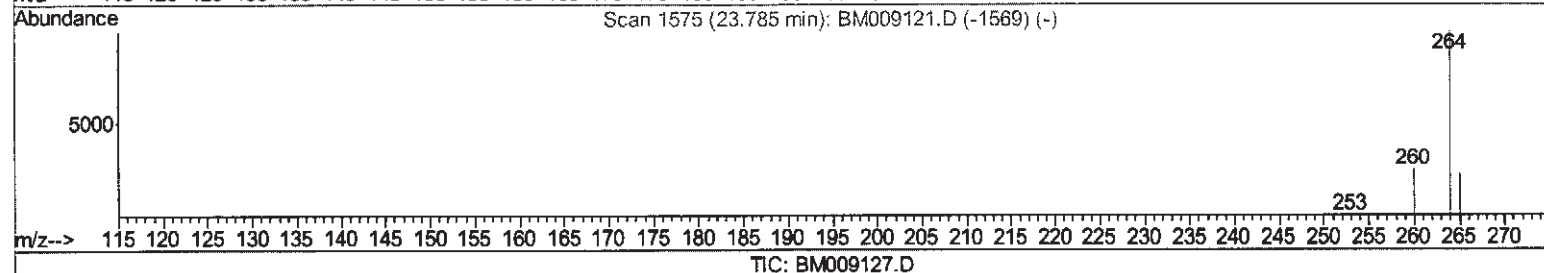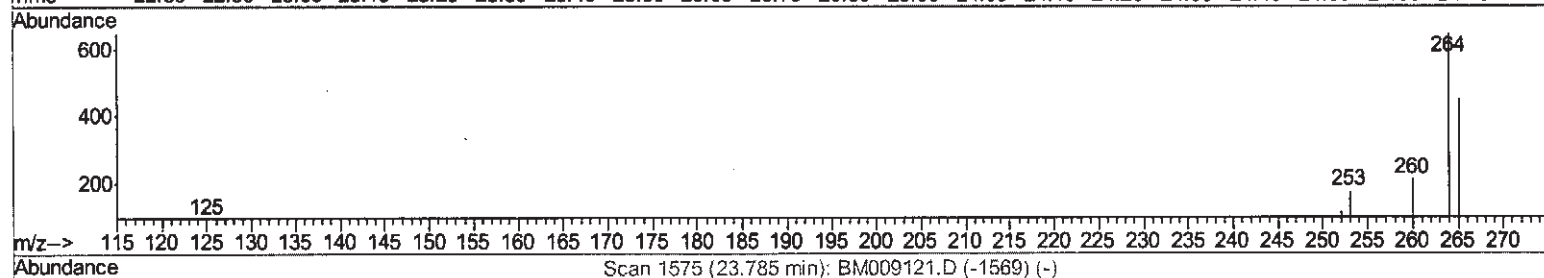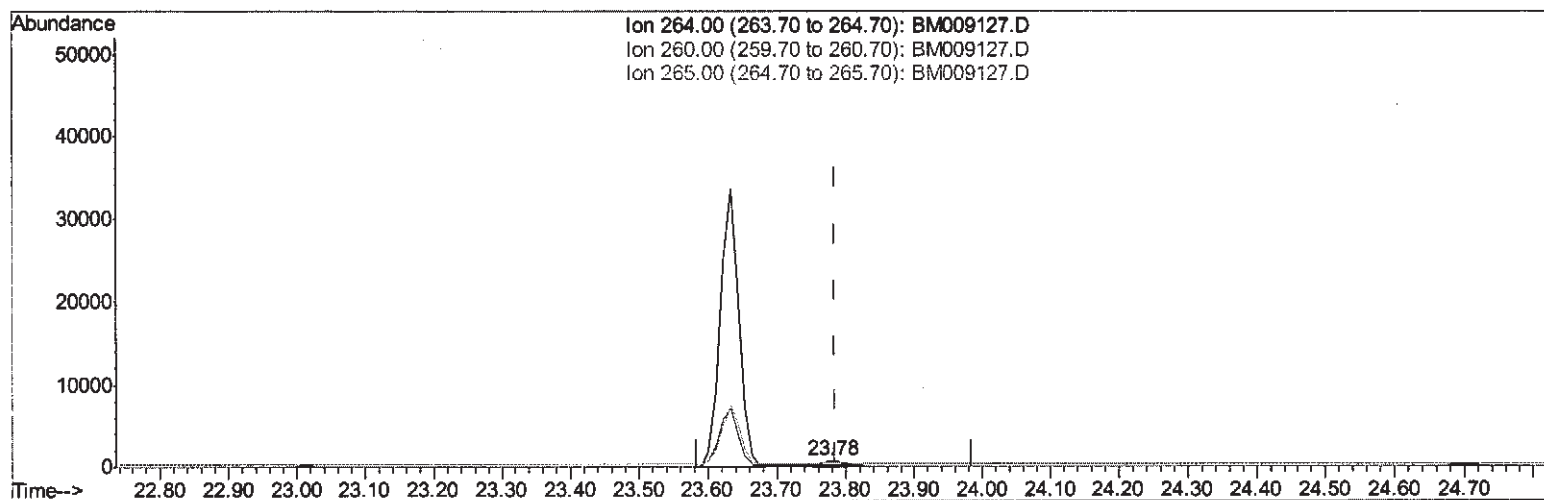

(20) Perylene-d12 (I)

23.778min (-0.007) 0.40ng/ul m

SJ 3/16/17

response 1145

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	32.05
265.00	103.50	69.03#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM030817\
Data File : BM009127.D
Acq On : 09 Mar 2017 03:59
Operator : SJ/MA
Sample : I2062-11
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AD0

Manual Integrations
APPROVED

mohammad
3/9/2017 2:02:15 PM

Quant Time: Mar 09 05:51:30 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 09 02:44:03 2017
Response via : Initial Calibration

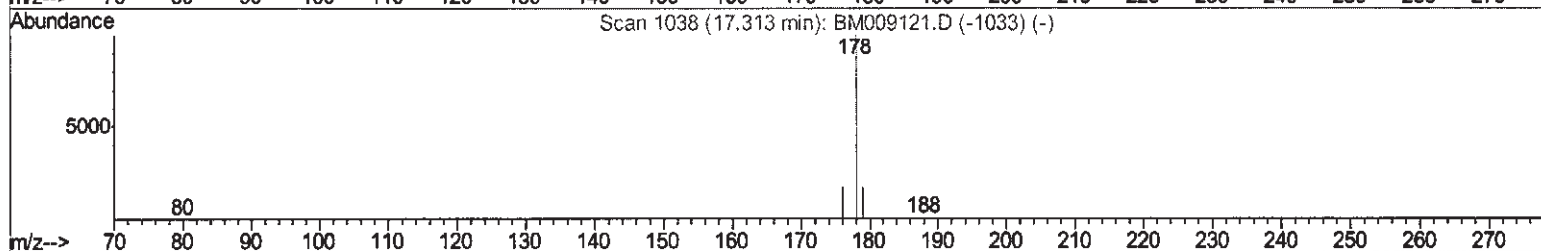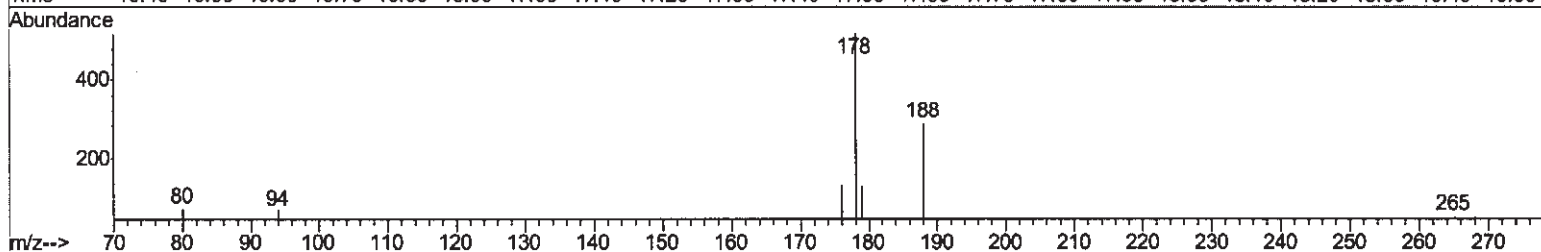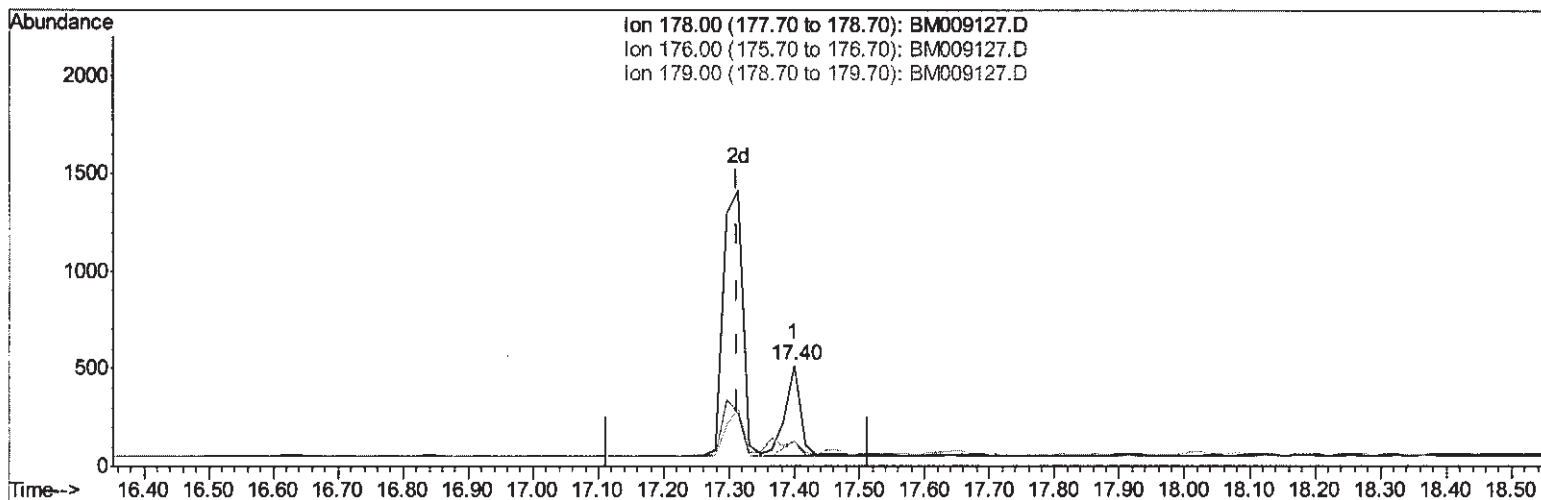

TIC: BM009127.D

(12) Phenanthrene

17.399min (+0.086) 0.16ng/ul

response 767

Ion	Exp%	Act%
178.00	100	100
176.00	23.00	25.53
179.00	17.00	25.15#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM030817\
Data File : BM009127.D
Acq On : 09 Mar 2017 03:59
Operator : SJ/MA
Sample : I2062-11
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AD0

Manual Integrations
APPROVED

mohammad
3/9/2017 2:02:15 PM

Quant Time: Mar 09 05:51:30 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 09 02:44:03 2017
Response via : Initial Calibration

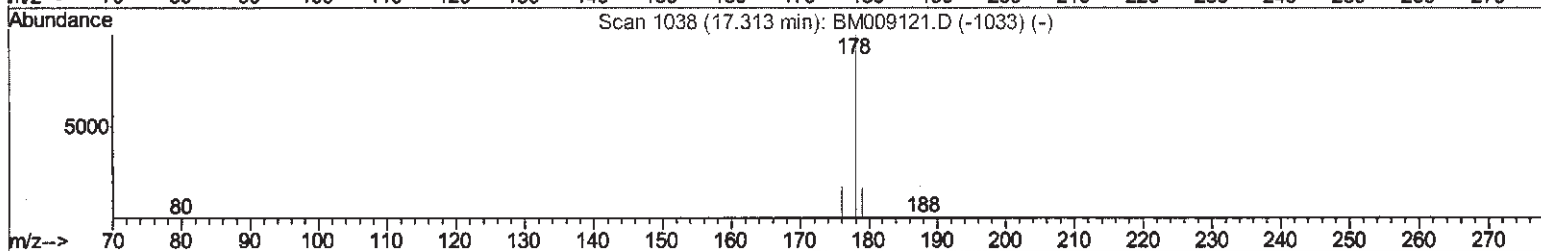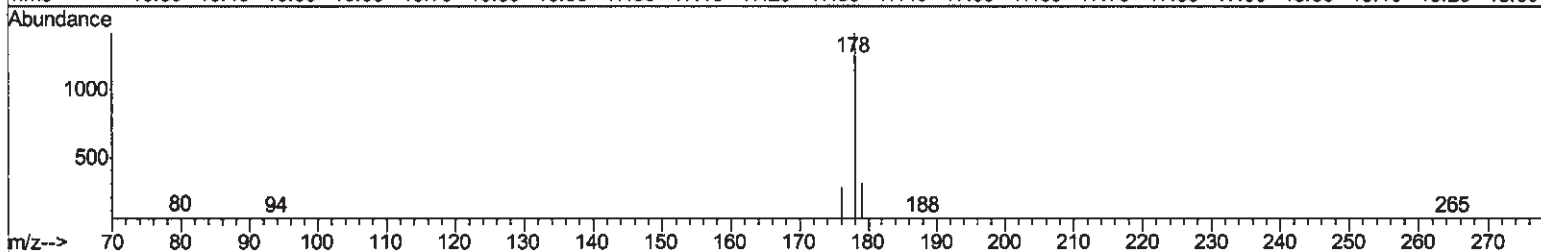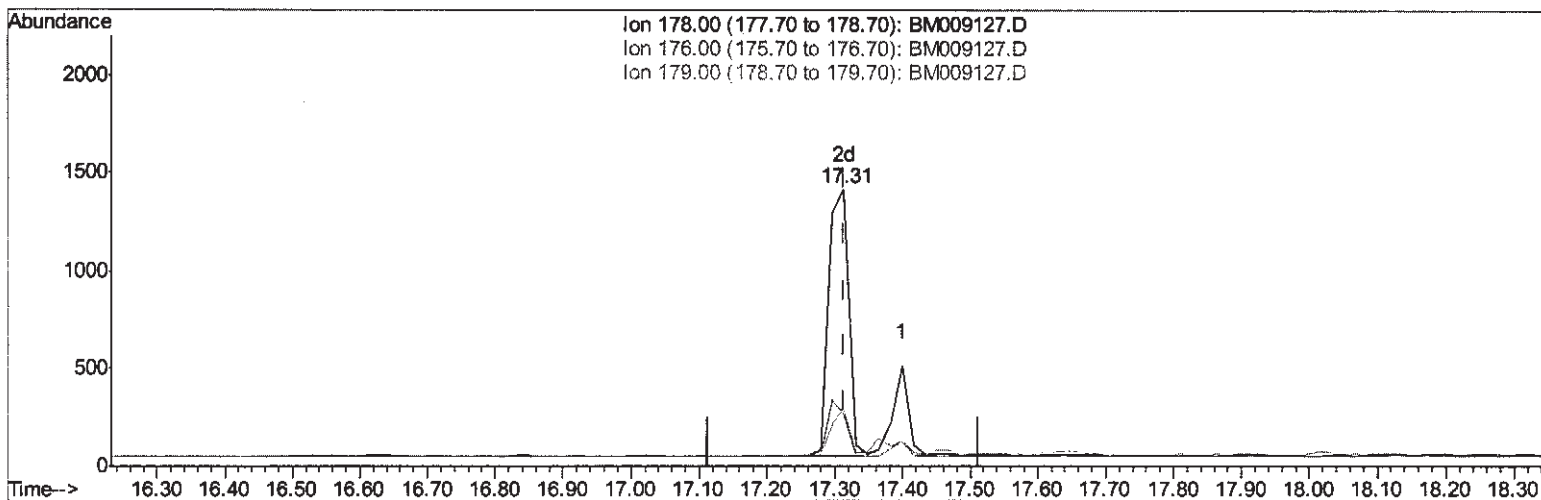

TIC: BM009127.D

(12) Phenanthrene

17.313min (+0.000) 0.58ng/ul m

SJ 3/16/17

response 2814

Ion	Exp%	Act%
178.00	100	100
176.00	23.00	19.31
179.00	17.00	20.93#
0.00	0.00	0.00


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM030817\
Data File : BM009127.D
Acq On : 09 Mar 2017 03:59
Operator : SJ/MA
Sample : I2062-11
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AD0

Manual Integrations
APPROVED

mohammad
3/9/2017 2:02:15 PM

Quant Time: Mar 09 05:55:39 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 09 02:44:03 2017
Response via : Initial Calibration

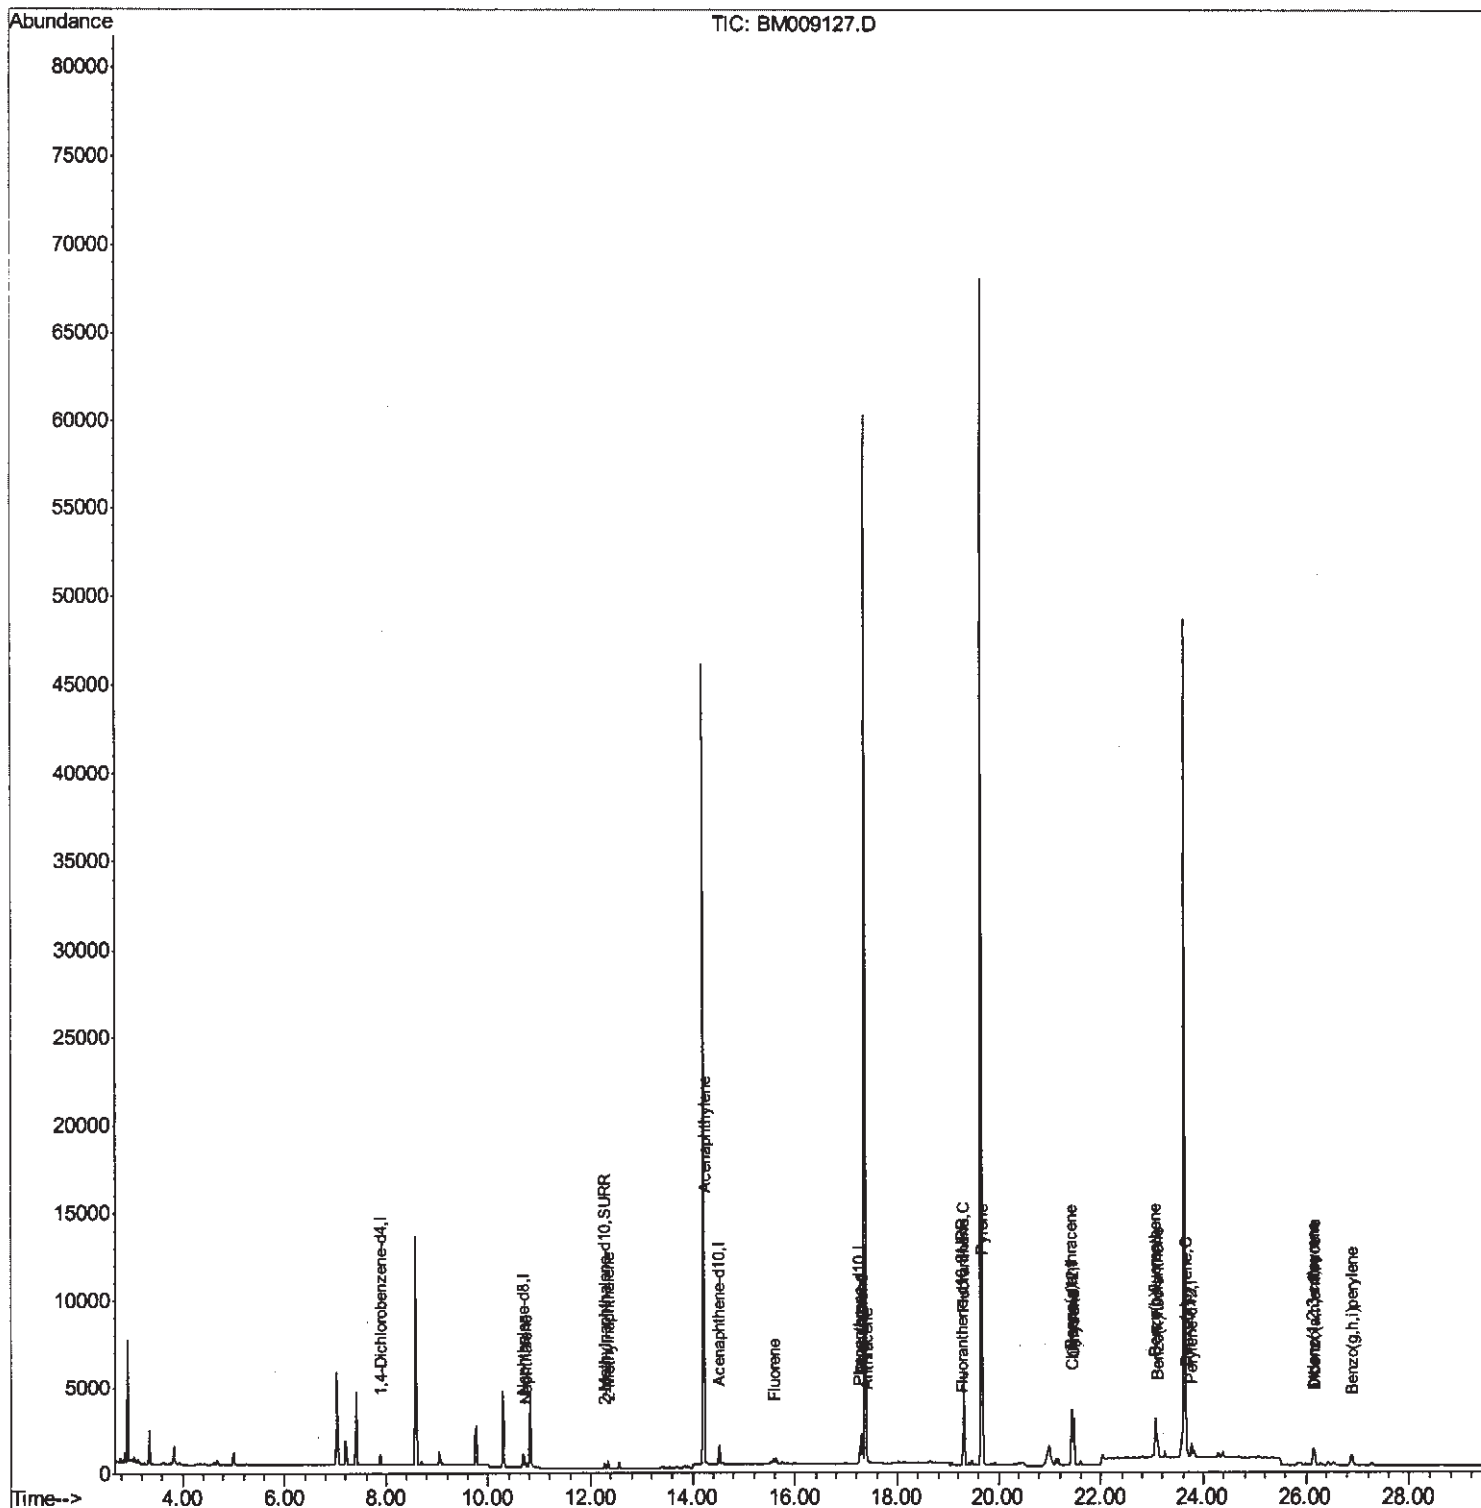




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM030817\
Data File : BM009127.D
Acq On : 09 Mar 2017 03:59
Operator : SJ/MA
Sample : I2062-11
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AD0

Manual Integrations
APPROVED

mohammad
3/9/2017 2:02:15 PM

Quant Time: Mar 09 05:51:30 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 09 02:44:03 2017
Response via : Initial Calibration

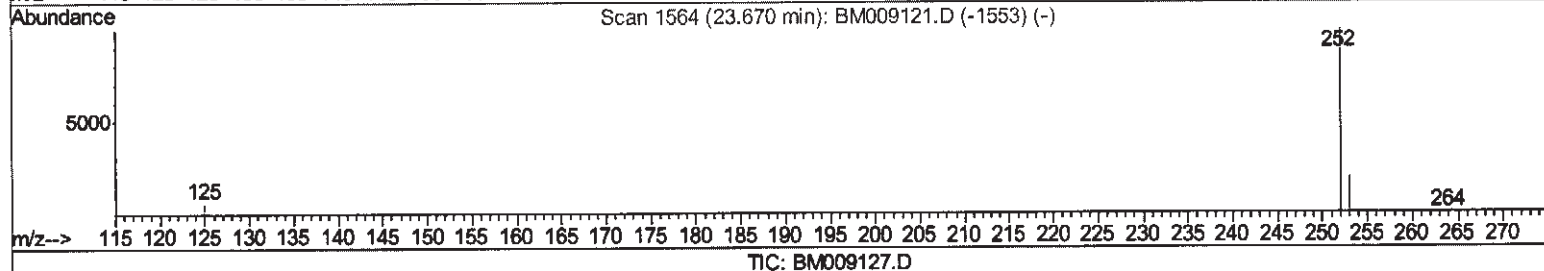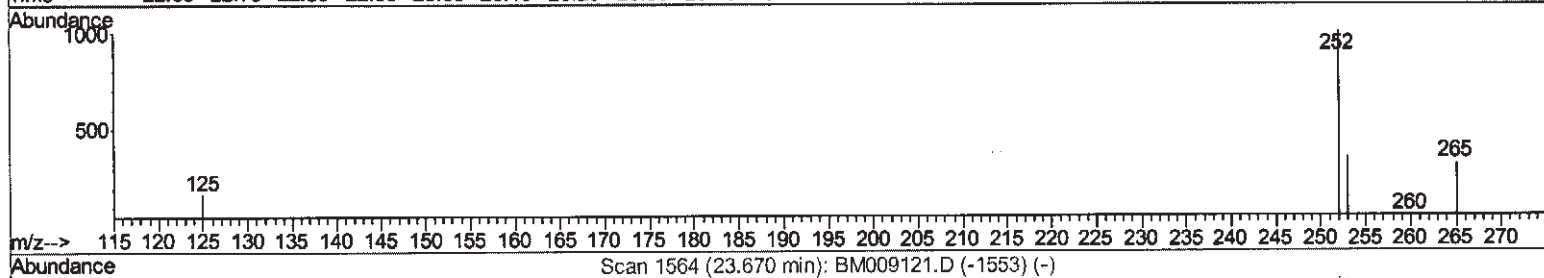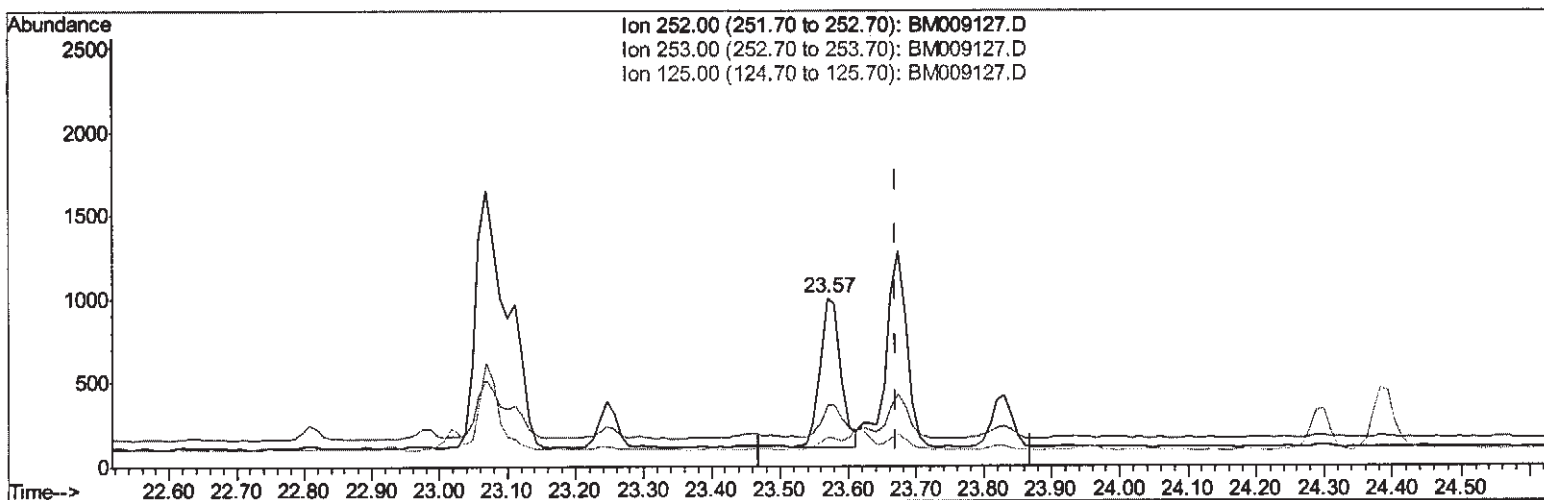

(23) Benzo(a)pyrene (C)

23.569min (-0.101) 0.46ng/ul

response 1860

Ion	Exp%	Act%
252.00	100	100
253.00	35.60	35.86
125.00	22.60	16.98#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM030817\
Data File : BM009127.D
Acq On : 09 Mar 2017 03:59
Operator : SJ/MA
Sample : I2062-11
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AD0

Manual Integrations
APPROVED

mohammad
3/9/2017 2:02:15 PM

Quant Time: Mar 09 05:51:30 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 09 02:44:03 2017
Response via : Initial Calibration

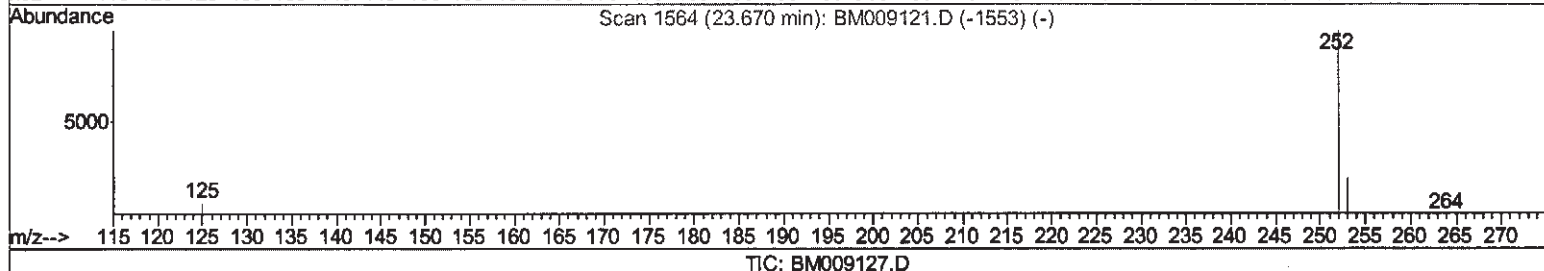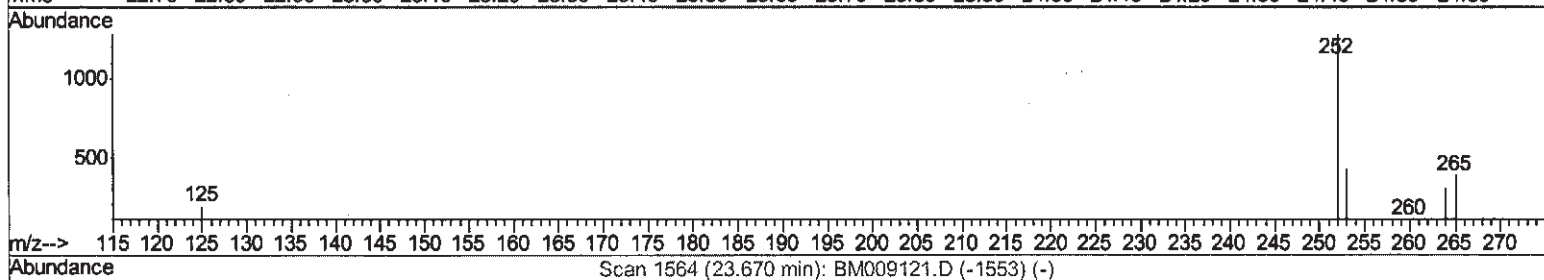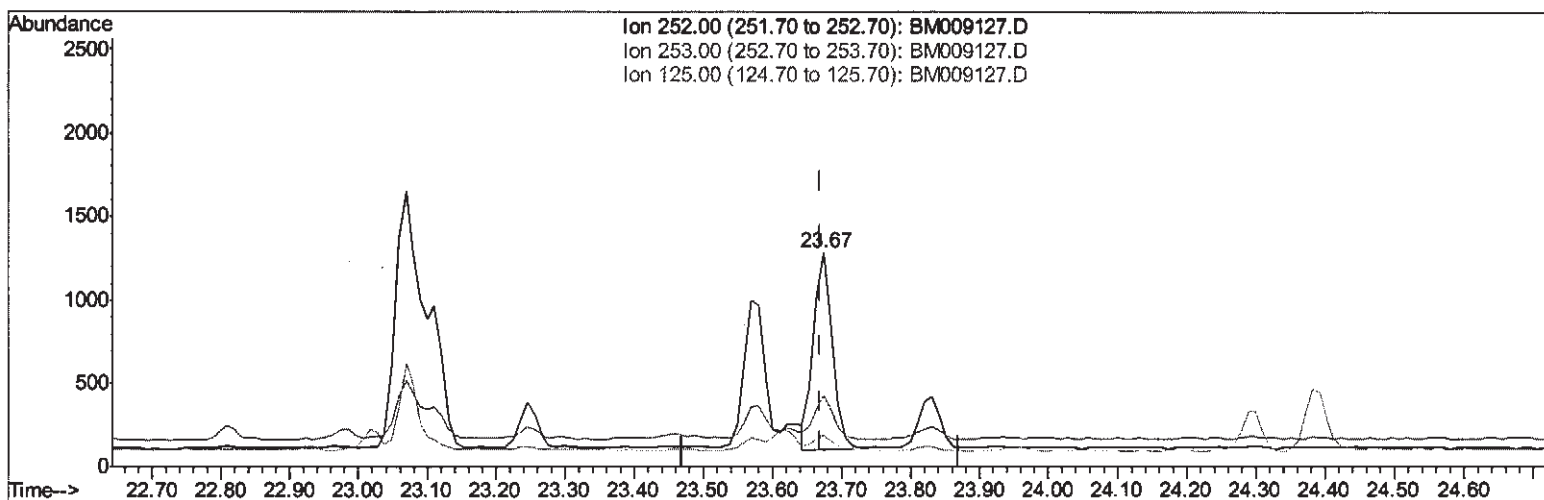

(23) Benzo(a)pyrene (C)

23.674min (+0.003) 0.56ng/ul m

SJ 3/16/17

response 2273

Ion	Exp%	Act%
252.00	100	100
253.00	35.60	33.18
125.00	22.60	14.41#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM030817\
Data File : BM009127.D
Acq On : 09 Mar 2017 03:59
Operator : SJ/MA
Sample : I2062-11
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AD0

Manual Integrations
APPROVED

mohammad
3/9/2017 2:02:15 PM

Quant Time: Mar 09 05:51:30 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 09 02:44:03 2017
Response via : Initial Calibration

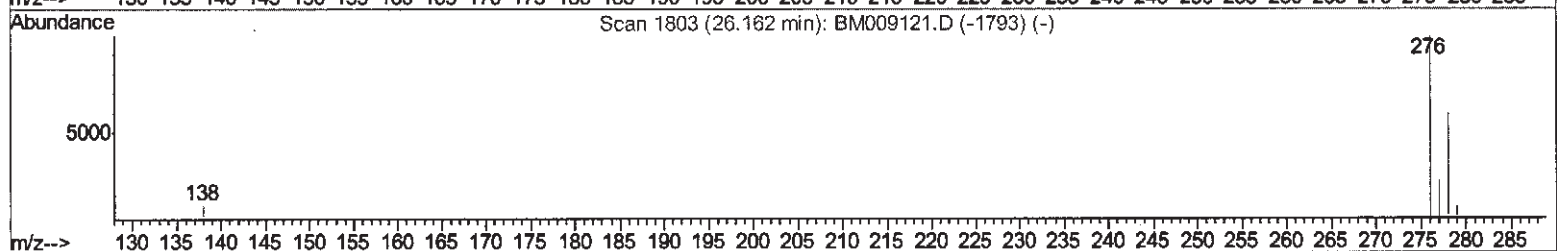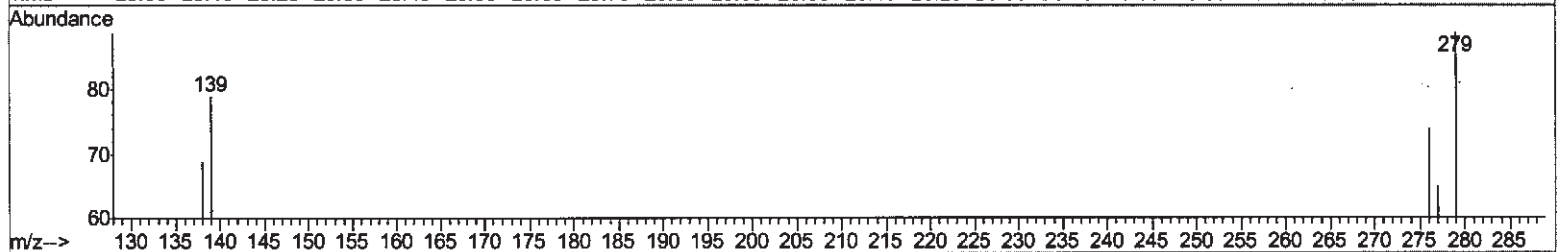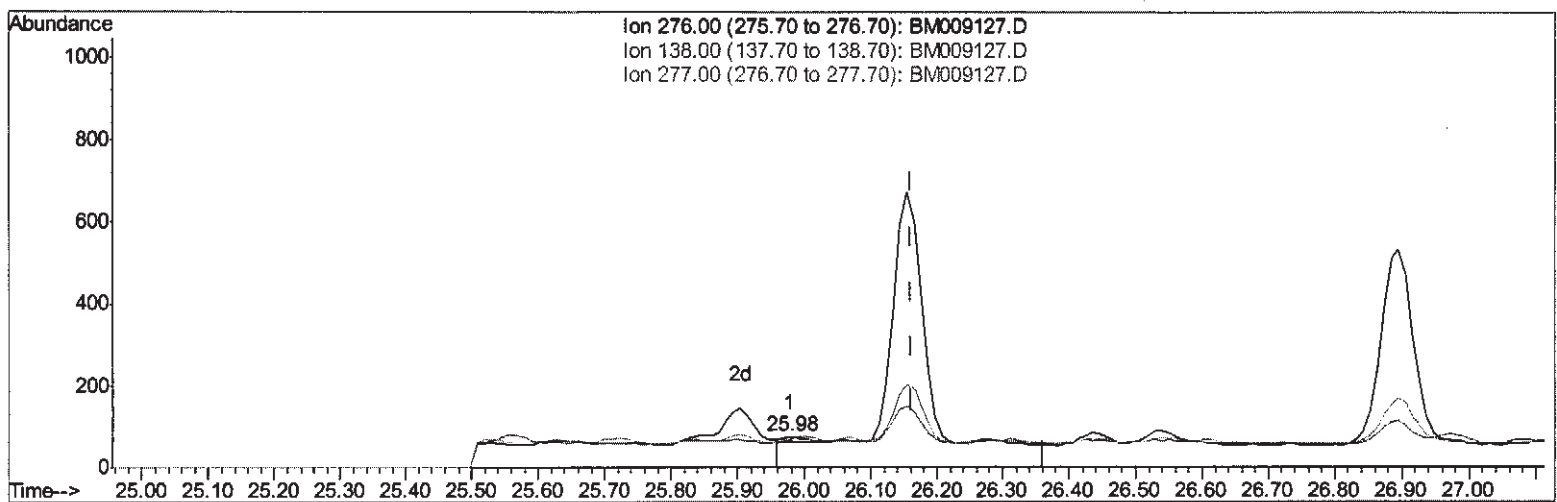

TIC: BM009127.D

(24) Indeno(1,2,3-cd)pyrene

25.977min (-0.184) 0.01ng/ul

response 31

Ion	Exp%	Act%
276.00	100	100
138.00	23.90	0.00#
277.00	24.50	0.00#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM030817\
Data File : BM009127.D
Acq On : 09 Mar 2017 03:59
Operator : SJ/MA
Sample : I2062-11
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AD0

Manual Integrations
APPROVED

mohammad
3/9/2017 2:02:15 PM

Quant Time: Mar 09 05:51:30 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 09 02:44:03 2017
Response via : Initial Calibration

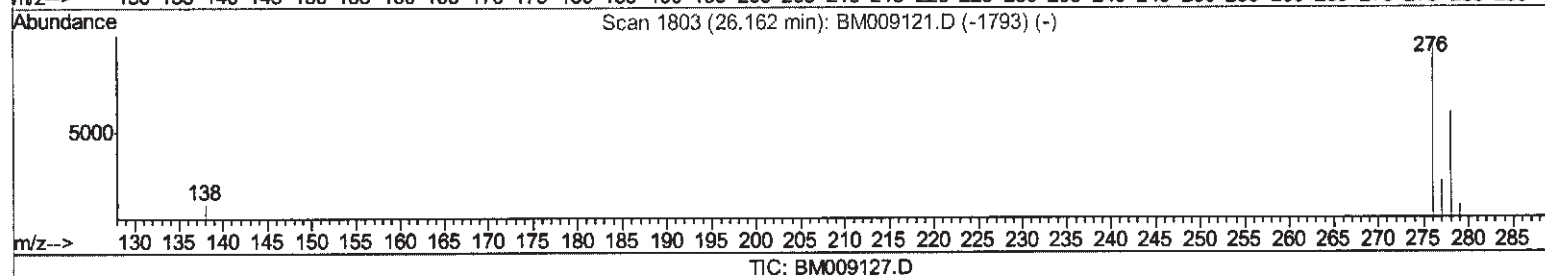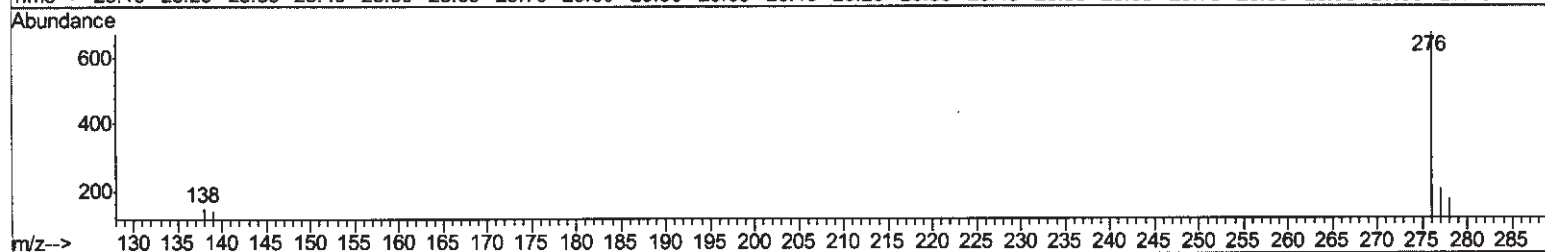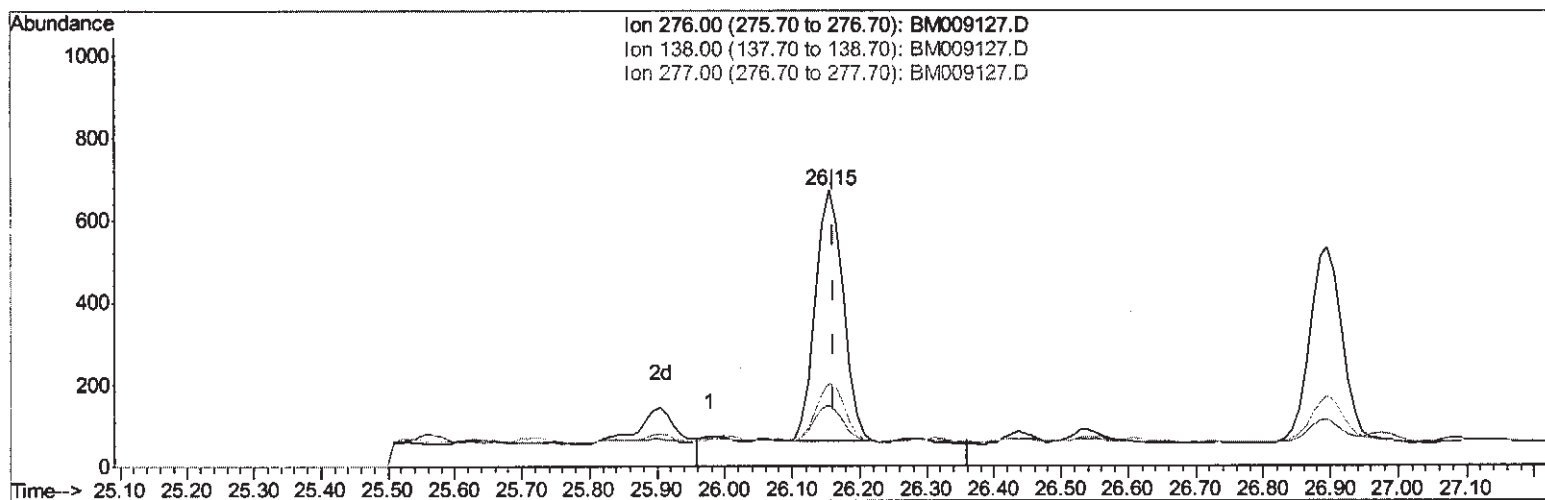

(24) Indeno(1,2,3-cd)pyrene

26.155min (-0.007) 0.34ng/ul m

SJ 3/16/17

response 1771

Ion	Exp%	Act%
276.00	100	100
138.00	23.90	0.00#
277.00	24.50	0.00#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM030817\
Data File : BM009127.D
Acq On : 09 Mar 2017 03:59
Operator : SJ/MA
Sample : I2062-11
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AD0

Manual Integrations
APPROVED

mohammad
3/9/2017 2:02:15 PM

Quant Time: Mar 09 05:51:30 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 09 02:44:03 2017
Response via : Initial Calibration

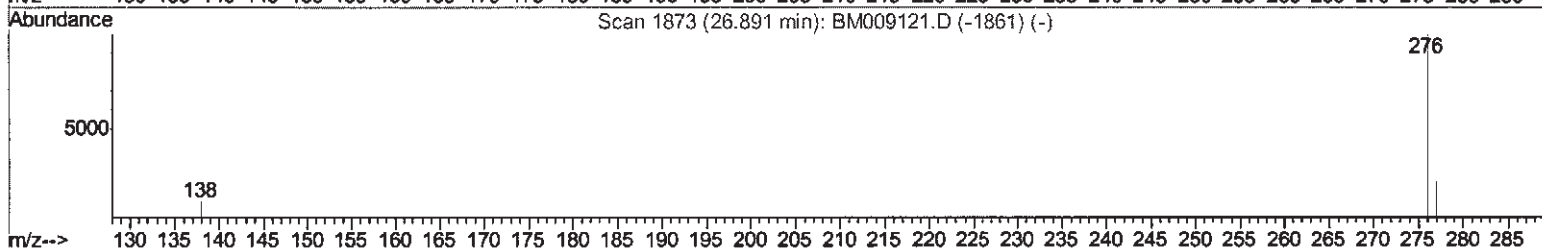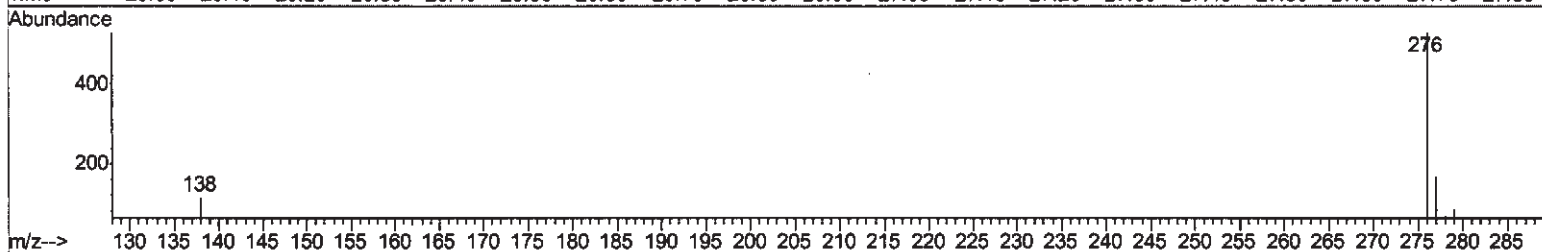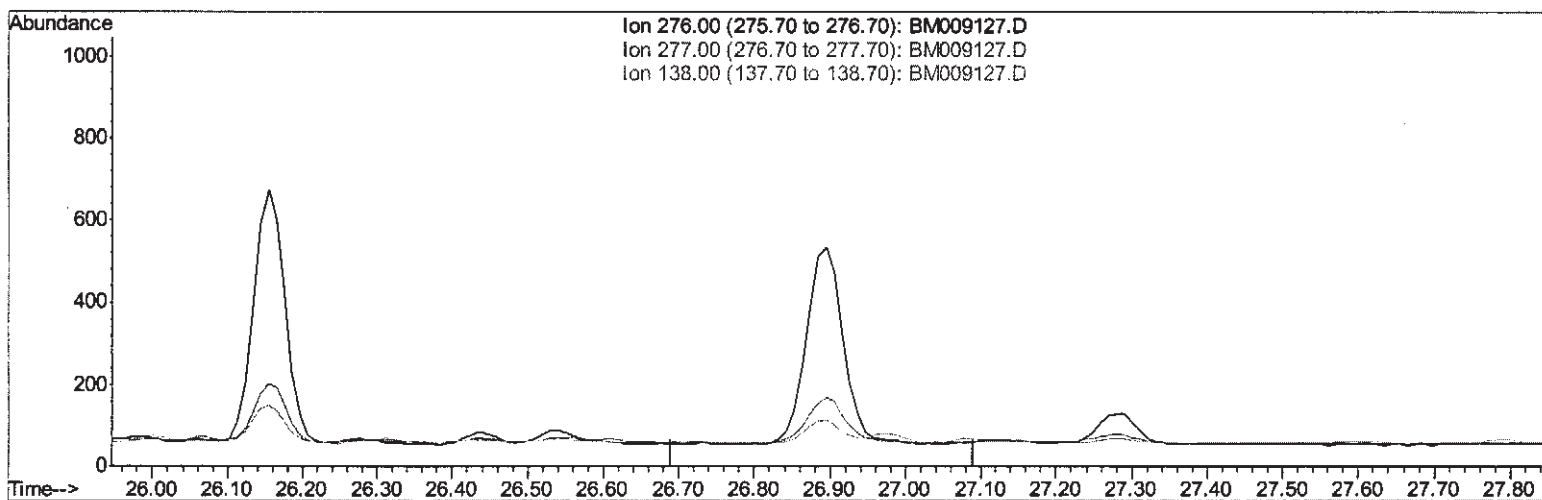

TIC: BM009127.D

(26) Benzo(g,h,i)perylene

26.891min (-26.891) 0.00ng/ul

response 0

Ion	Exp%	Act%
276.00	100	0.00
277.00	27.30	0.00#
138.00	25.60	0.00#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM030817\
Data File : BM009127.D
Acq On : 09 Mar 2017 03:59
Operator : SJ/MA
Sample : I2062-11
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AD0

Manual Integrations
APPROVED

mohammad
3/9/2017 2:02:15 PM

Quant Time: Mar 09 05:51:30 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 09 02:44:03 2017
Response via : Initial Calibration

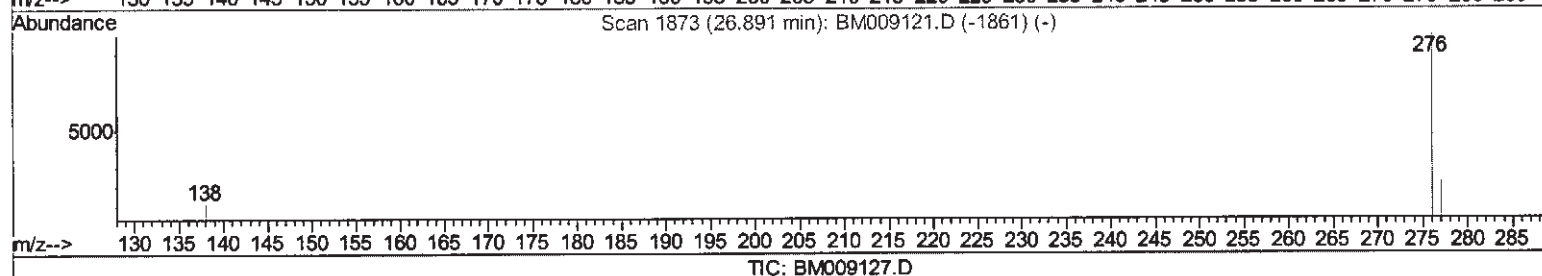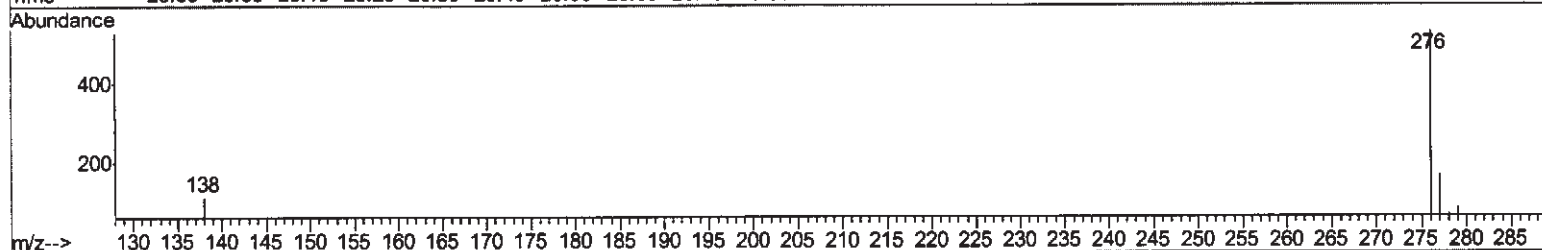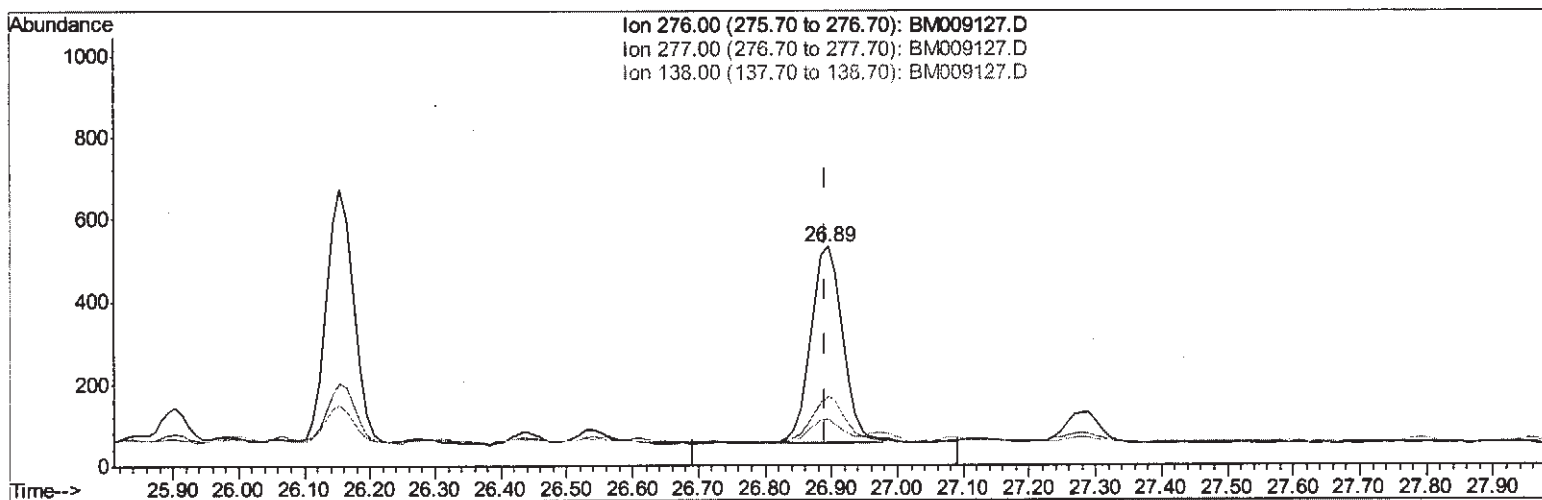

(26) Benzo(g,h,i)perylene

26.895min (+0.003) 0.37ng/ul m

SJ 3/16/17

response 1606

Ion	Exp%	Act%
276.00	100	100
277.00	27.30	31.89
138.00	25.60	21.58
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM030817\
Data File : BM009127.D
Acq On : 09 Mar 2017 03:59
Operator : SJ/MA
Sample : I2062-11
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AD0

Manual Integrations
APPROVED

mohammad
3/9/2017 2:02:15 PM

Quant Time: Mar 09 05:53:14 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 09 02:44:03 2017
Response via : Initial Calibration

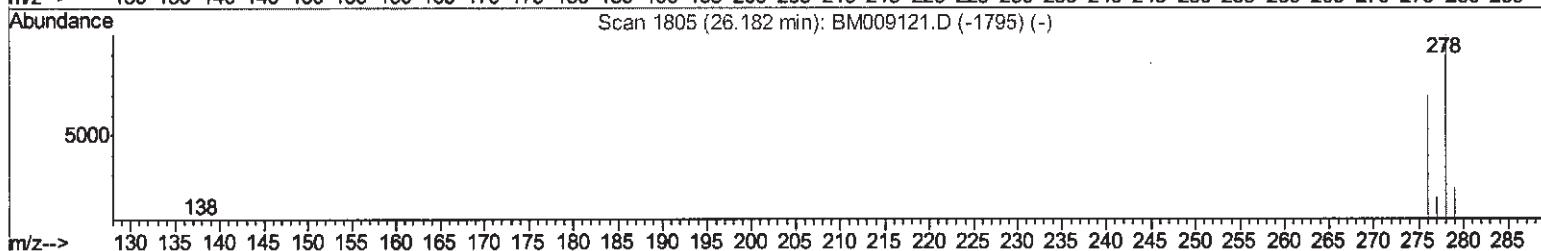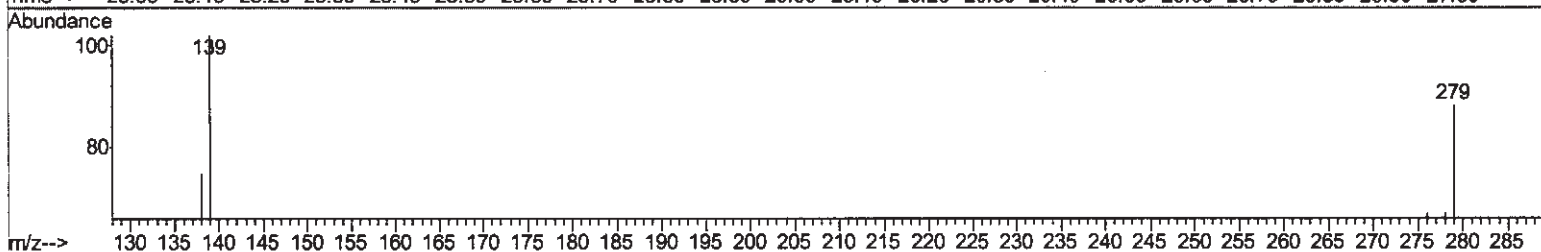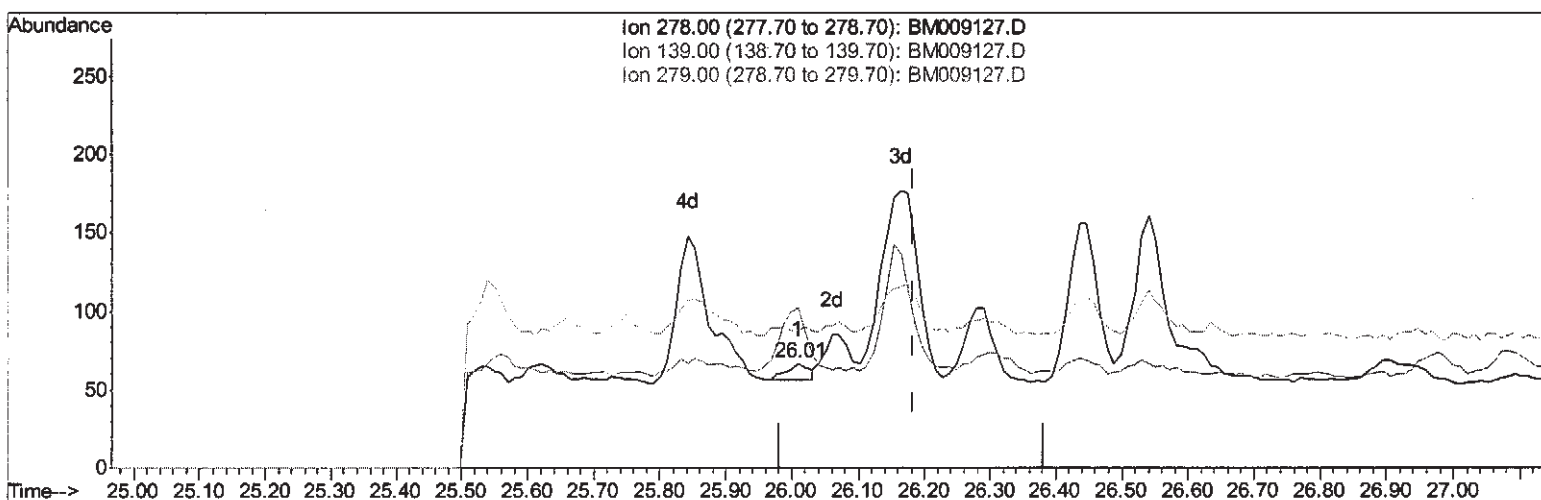

TIC: BM009127.D

(25) Dibenzo(a,h)anthracene

26.009min (-0.174) 0.01ng/ul

response 26

Ion	Exp%	Act%
278.00	100	100
139.00	21.70	152.24#
279.00	32.40	131.34#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM030817\
Data File : BM009127.D
Acq On : 09 Mar 2017 03:59
Operator : SJ/MA
Sample : I2062-11
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AD0

Manual Integrations
APPROVED

mohammad
3/9/2017 2:02:15 PM

Quant Time: Mar 09 05:53:14 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 09 02:44:03 2017
Response via : Initial Calibration

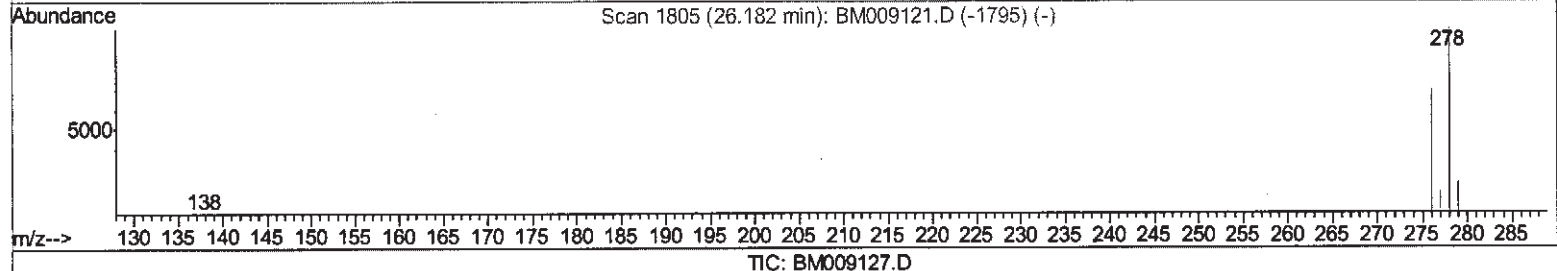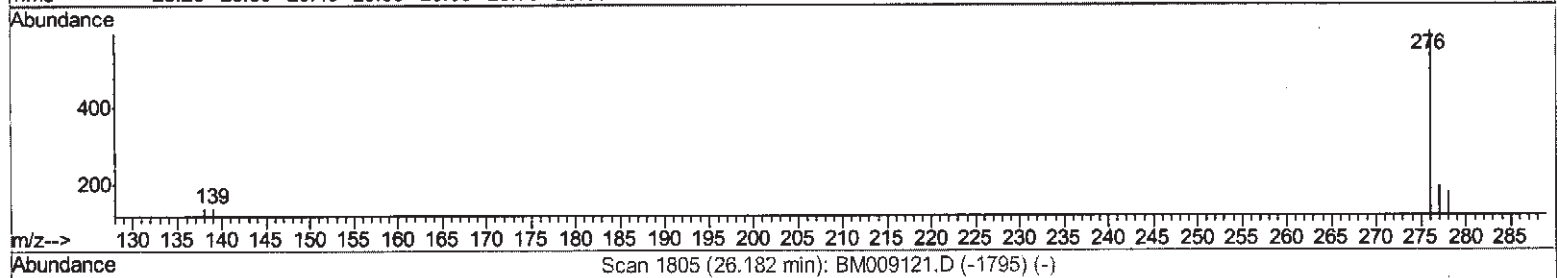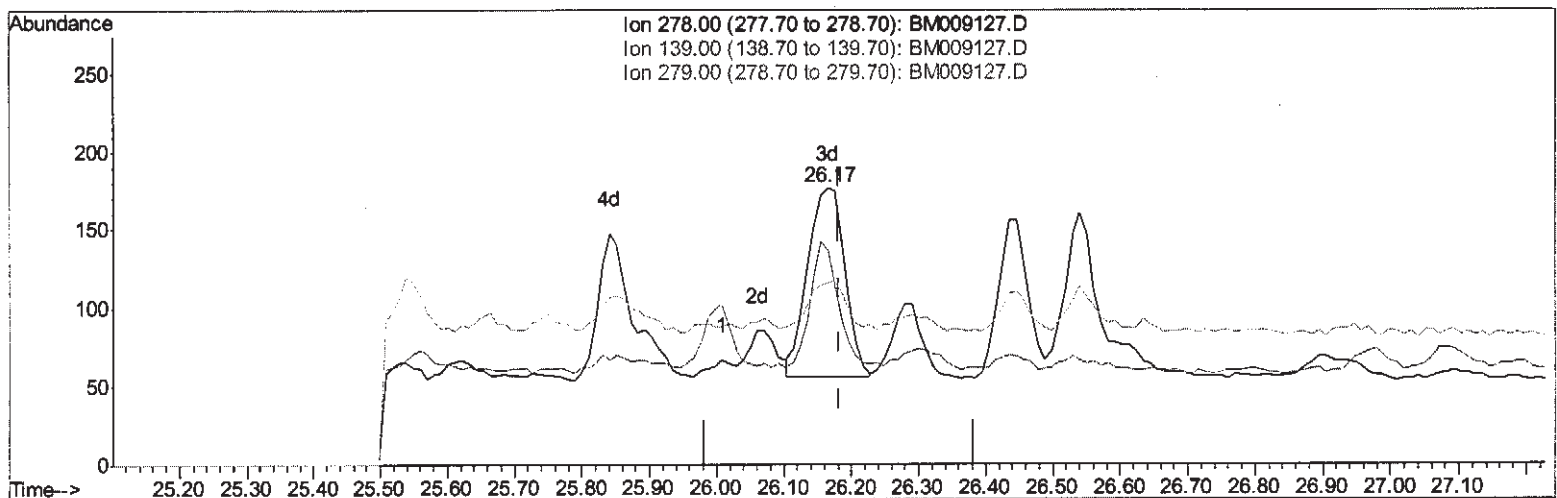

(25) Dibenzo(a,h)anthracene

26.165min (-0.017) 0.11ng/ul m

response 461

Ion	Exp%	Act%
278.00	100	100
139.00	21.70	77.40#
279.00	32.40	65.54#
0.00	0.00	0.00

SJ

3/16/17

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM030817\
 Data File : BM009127.D
 Acq On : 09 Mar 2017 03:59
 Operator : SJ/MA
 Sample : I2062-11
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AD0

Manual Integrations
 APPROVED

mohammad
 3/9/2017 2:02:15 PM

Quant Time: Mar 09 05:55:39 2017
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030317.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 09 02:44:03 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.88	152	323	0.40	ng/ul	0.00
2) Naphthalene-d8	10.68	136	1070	0.40	ng/ul	-0.01
6) Acenaphthene-d10	14.52	164	652	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.26	188	1551m	0.40	ng/ul	0.00
16) Chrysene-d12	21.44	240	1389	0.40	ng/ul	0.00
20) Perylene-d12	23.78	264	1145m	0.40	ng/ul	0.00

SJ 3/16/17

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	12.27	152	347	0.20	ng/ul	0.00
14) Fluoranthene-d10	19.30	212	891	0.18	ng/ul	0.00

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
3) Naphthalene	10.73	128	361	0.12	ng/ul#	65
5) 2-Methylnaphthalene	12.34	142	278	0.13	ng/ul	97
7) Acenaphthylene	14.23	152	300	0.09	ng/ul#	51
9) Fluorene	15.58	166	255	0.08	ng/ul#	90
12) Phenanthrene	17.31	178	2814m	0.58	ng/ul	90
13) Anthracene	17.40	178	773	0.16	ng/ul#	90
15) Fluoranthene	19.32	202	5463m	0.86	ng/ul	96
17) Pyrene	19.68	202	4946	1.04	ng/ul	97
18) Benzo(a)anthracene	21.42	228	2861	0.62	ng/ul	93
19) Chrysene	21.47	228	2837	0.65	ng/ul	93
21) Benzo(b)fluoranthene	23.07	252	3950m	0.88	ng/ul	
22) Benzo(k)fluoranthene	23.11	252	1155m	0.29	ng/ul	
23) Benzo(a)pyrene	23.67	252	2273m	0.56	ng/ul	
24) Indeno(1,2,3-cd)pyrene	26.15	276	1771m	0.34	ng/ul	
25) Dibenzo(a,h)anthracene	26.17	278	461m	0.11	ng/ul	
26) Benzo(g,h,i)perylene	26.89	276	1606m	0.37	ng/ul	

SJ 3/16/17

SJ 3/16/17

(#) = qualifier out of range (m) = manual integration (+) = signals summed




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM030817\
Data File : BM009127.D
Acq On : 09 Mar 2017 03:59
Operator : SJ/MA
Sample : I2062-11
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AD0

Manual Integrations
APPROVED

mohammad
3/9/2017 2:02:15 PM

Quant Time: Mar 09 05:51:30 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 09 02:44:03 2017
Response via : Initial Calibration

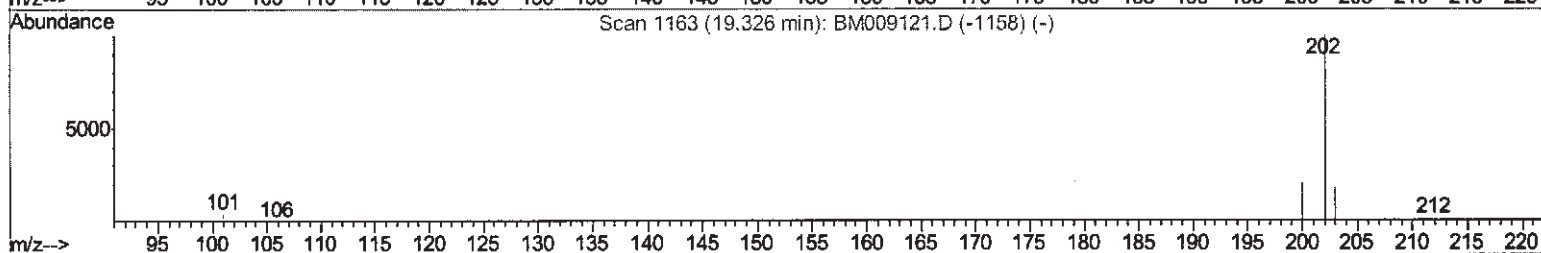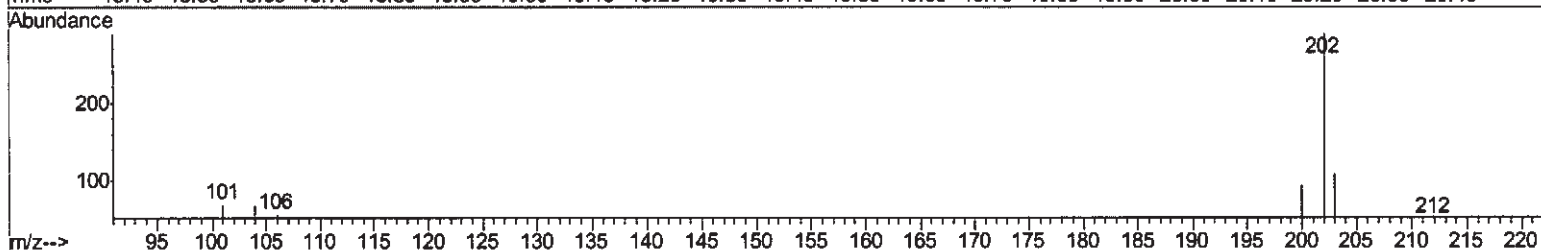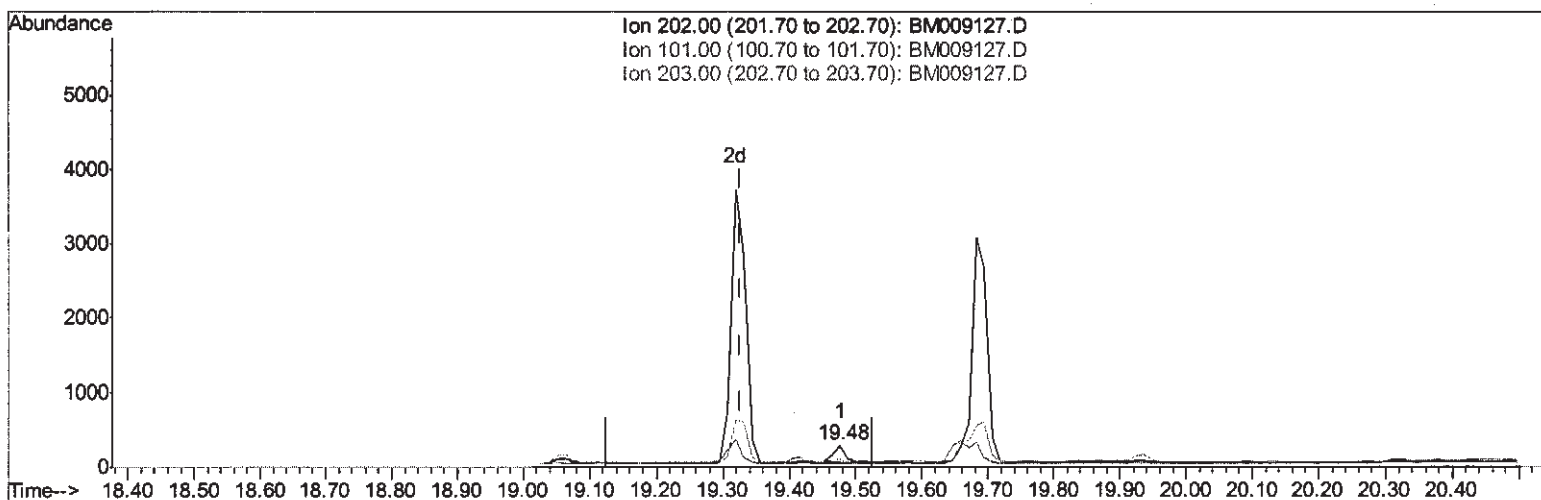

TIC: BM009127.D

(15) Fluoranthene (C)

19.477min (+0.150) 0.05ng/ul

response 325

Ion	Exp%	Act%
202.00	100	100
101.00	10.30	23.88
203.00	19.50	37.37
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM030817\
 Data File : BM009127.D
 Acq On : 09 Mar 2017 03:59
 Operator : SJ/MA
 Sample : I2062-11
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AD0

Manual Integrations
 APPROVED

mohammad
 3/9/2017 2:02:15 PM

Quant Time: Mar 09 05:51:30 2017
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030317.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 09 02:44:03 2017
 Response via : Initial Calibration

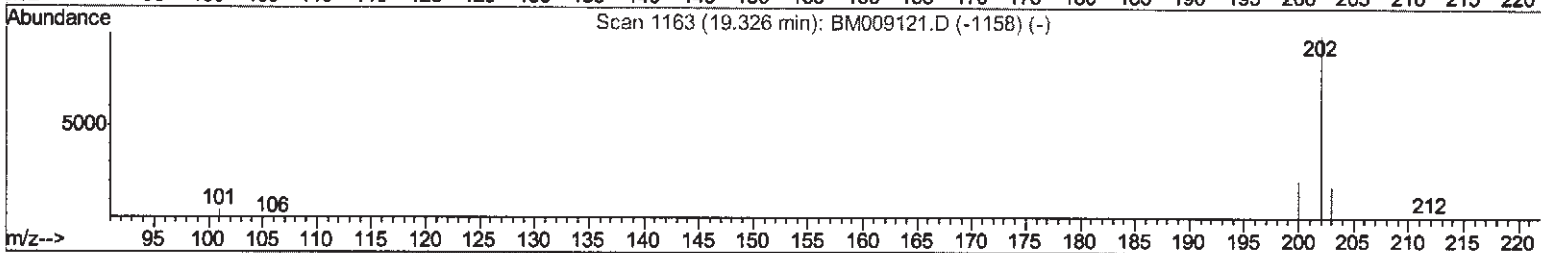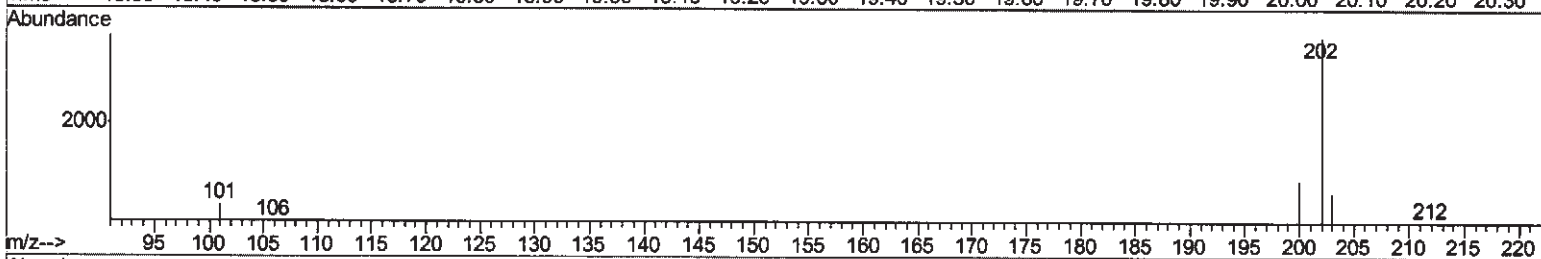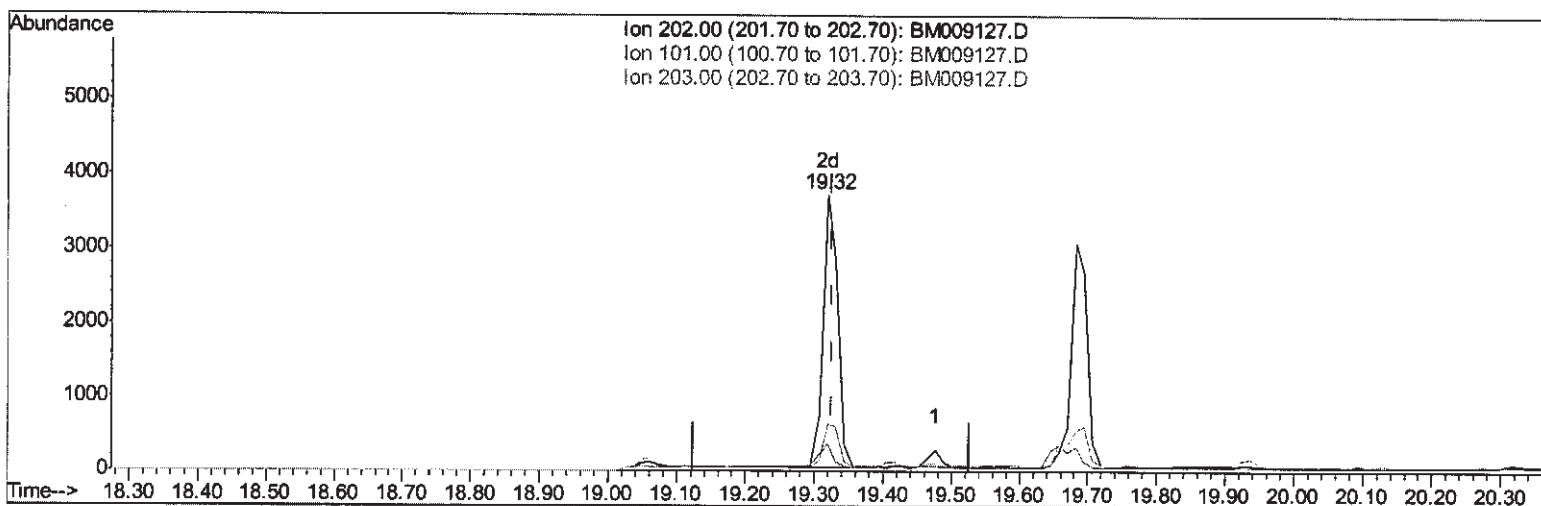

TIC: BM009127.D

(15) Fluoranthene (C)

19.319min (-0.007) 0.86ng/ul m SJ 3/16/17

response 5463

Ion	Exp%	Act%
202.00	100	100
101.00	10.30	10.01
203.00	19.50	17.23
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM030817\
Data File : BM009127.D
Acq On : 09 Mar 2017 03:59
Operator : SJ/MA
Sample : I2062-11
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AD0

Manual Integrations
APPROVED

mohammad
3/9/2017 2:02:15 PM

Quant Time: Mar 09 05:51:30 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 09 02:44:03 2017
Response via : Initial Calibration

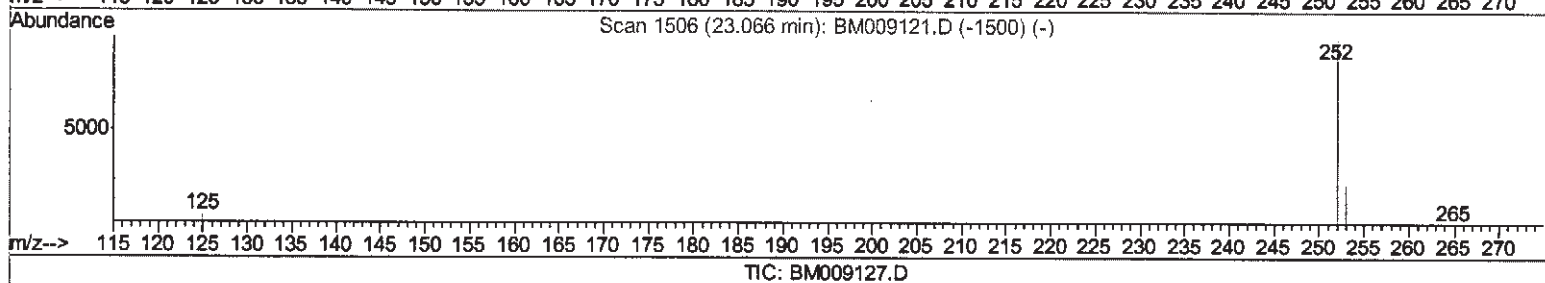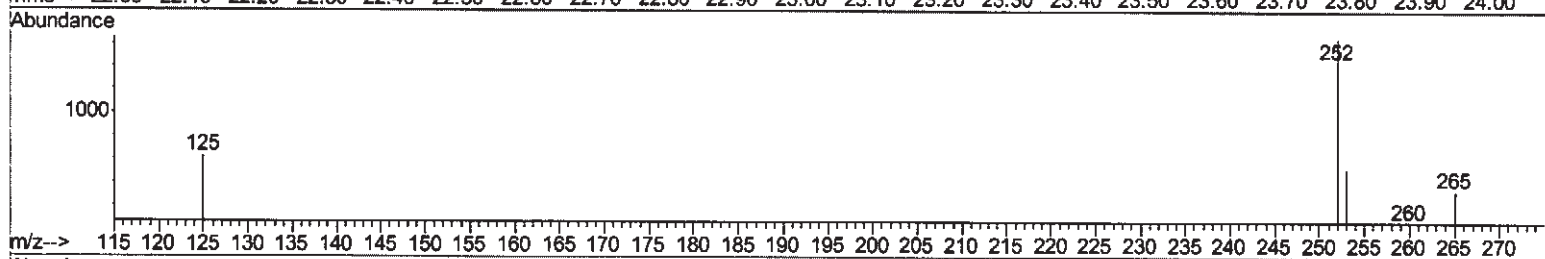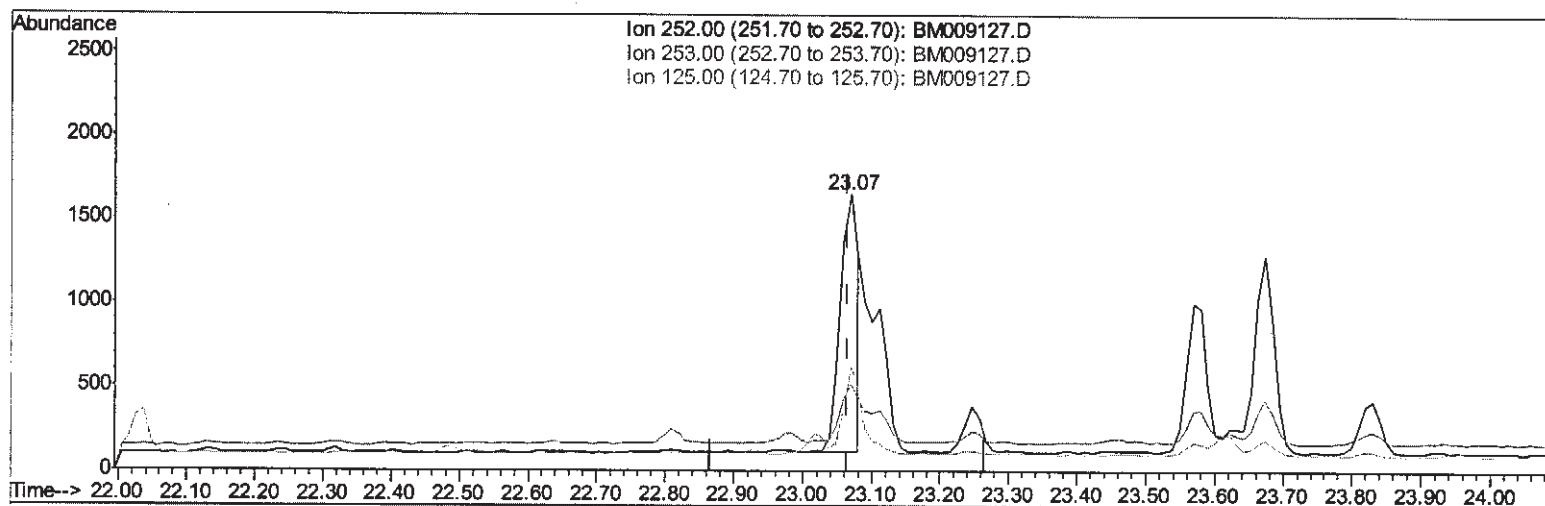

(21) Benzo(b)fluoranthene

23.069min (+0.003) 0.64ng/ul

response 2870

Ion	Exp%	Act%
252.00	100	100
253.00	32.10	31.36
125.00	17.50	37.77#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM030817\
Data File : BM009127.D
Acq On : 09 Mar 2017 03:59
Operator : SJ/MA
Sample : I2062-11
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AD0

Manual Integrations
APPROVED

mohammad
3/9/2017 2:02:15 PM

Quant Time: Mar 09 05:51:30 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 09 02:44:03 2017
Response via : Initial Calibration

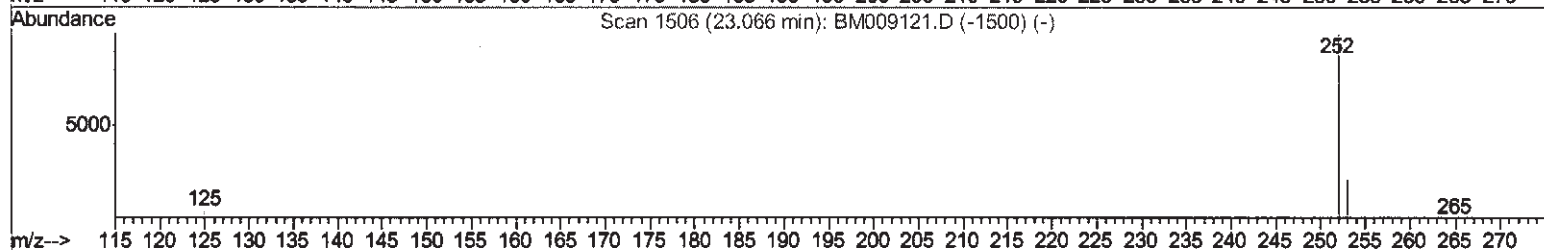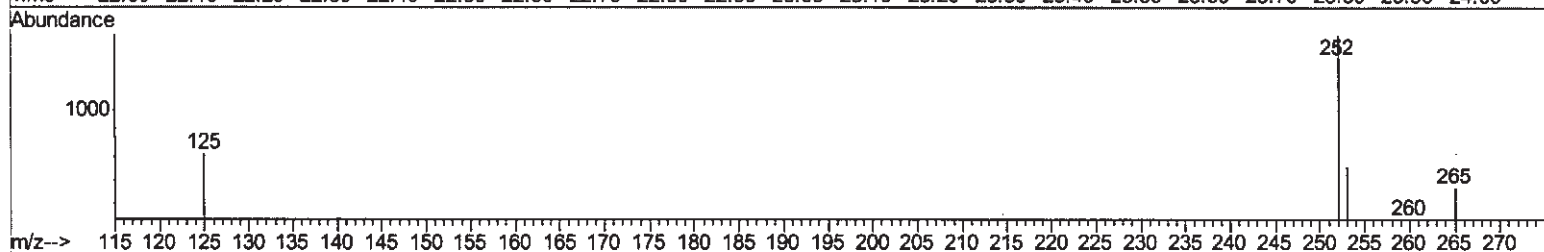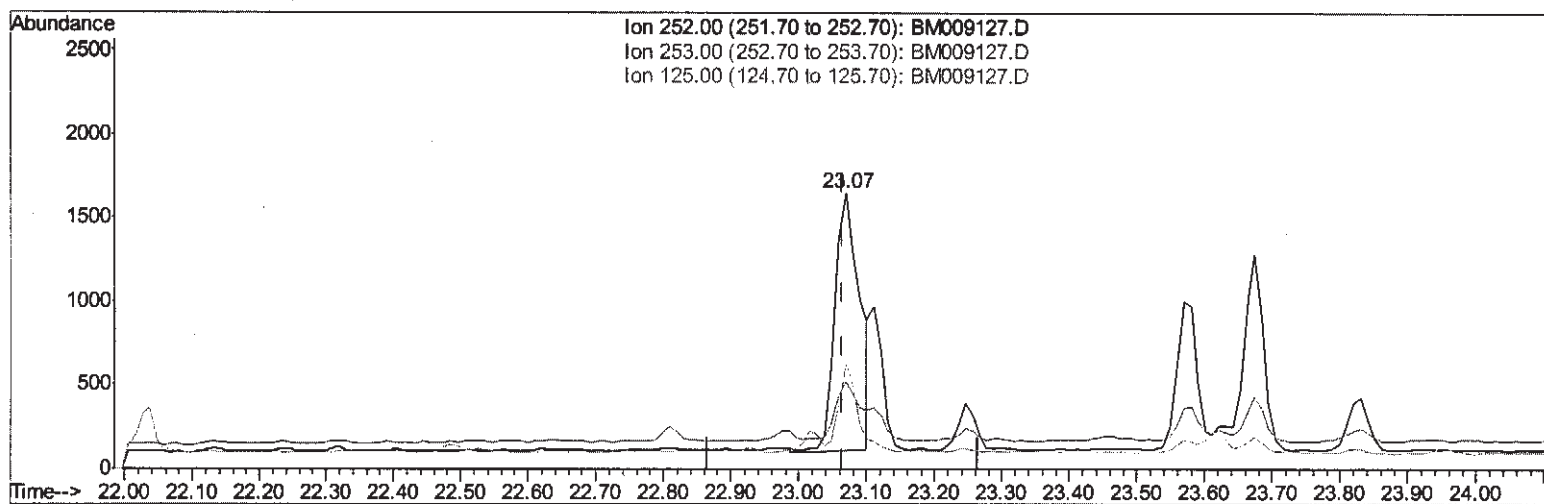

TIC: BM009127.D

(21) Benzo(b)fluoranthene

23.069min (+0.003) 0.88ng/ul m SJ 3/16/17

response 3950

Ion	Exp%	Act%
252.00	100	100
253.00	32.10	31.36
125.00	17.50	37.77#
0.00	0.00	0.00



Data Path : Z:\HPCHEM1\BNA_M\DATA\BM030817\
Data File : BM009127.D
Acq On : 09 Mar 2017 03:59
Operator : SJ/MA
Sample : I2062-11
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AD0


Manual Integrations
APPROVED

mohammad
3/9/2017 2:02:15 PM

Quant Time: Mar 09 05:51:30 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 09 02:44:03 2017
Response via : Initial Calibration

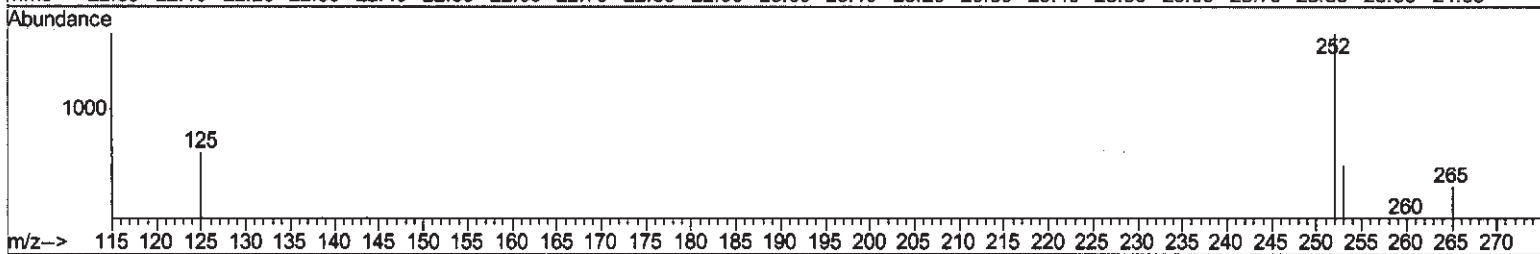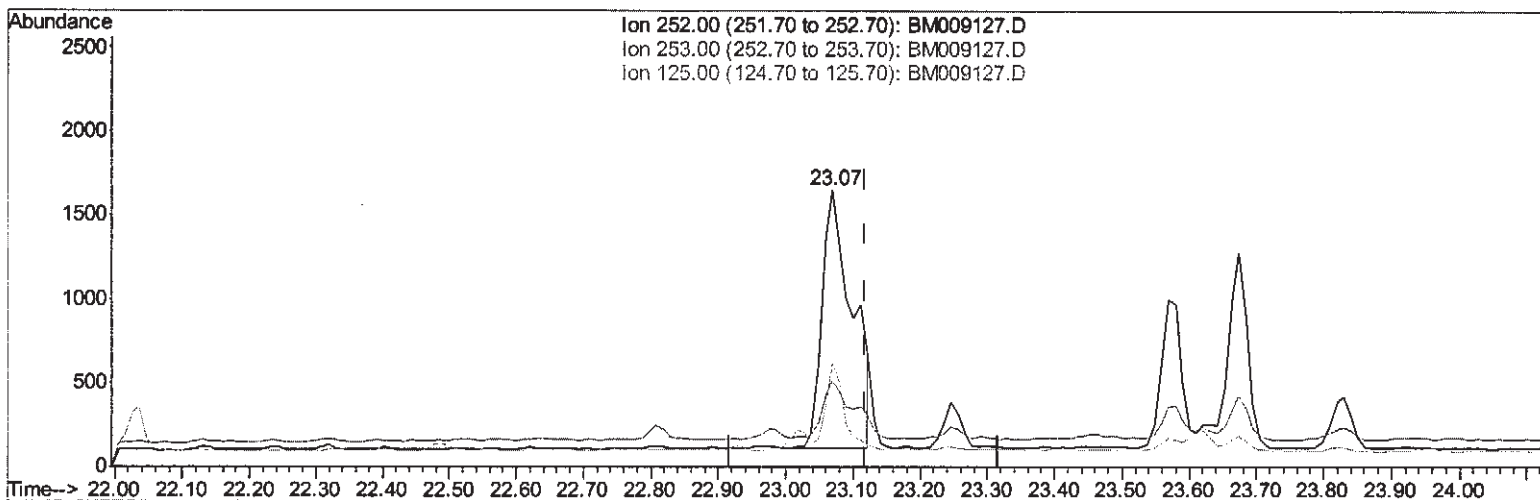

Scan 1511 (23.118 min): BM009121.D (-1508) (-)

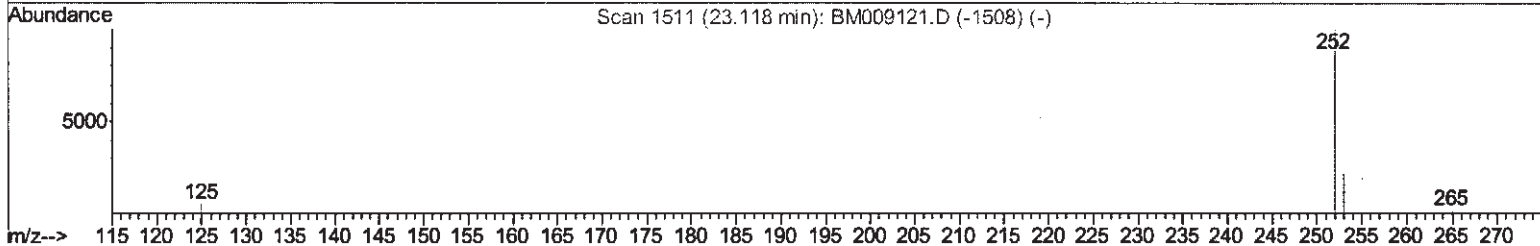

TIC: BM009127.D

(22) Benzo(k)fluoranthene

23.069min (-0.049) 1.21ng/ul

response 4813

Ion	Exp%	Act%
252.00	100	100
253.00	30.60	31.36
125.00	17.10	37.77#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM030817\
Data File : BM009127.D
Acq On : 09 Mar 2017 03:59
Operator : SJ/MA
Sample : I2062-11
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AD0

Manual Integrations
APPROVED

mohammad
3/9/2017 2:02:15 PM

Quant Time: Mar 09 05:51:30 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 09 02:44:03 2017
Response via : Initial Calibration

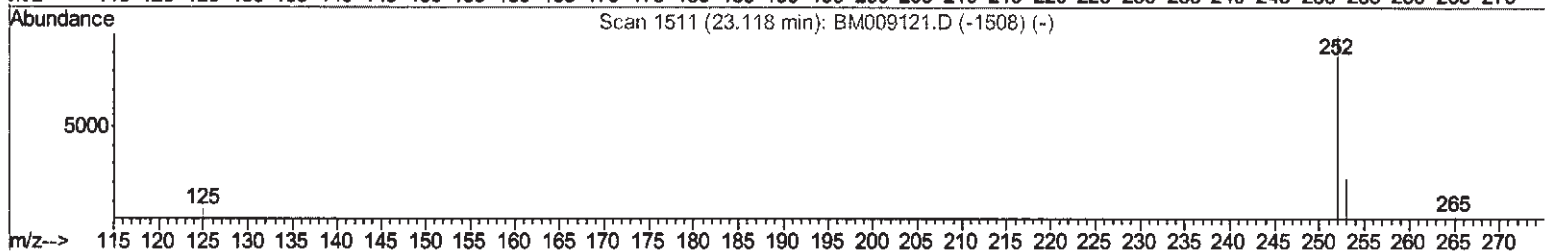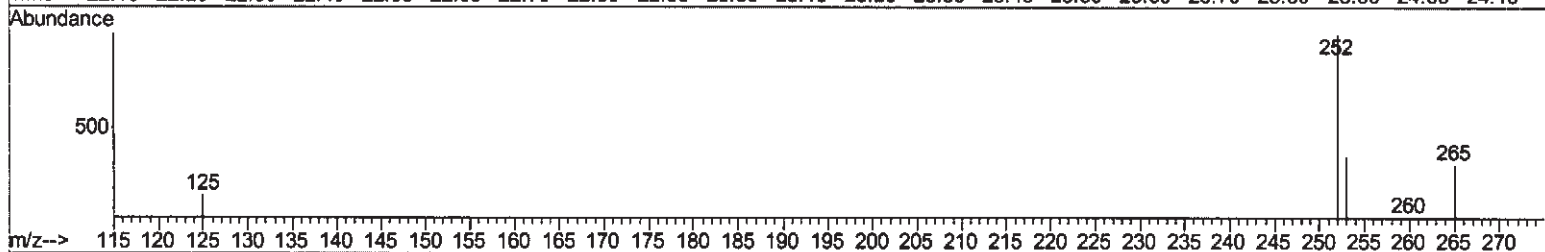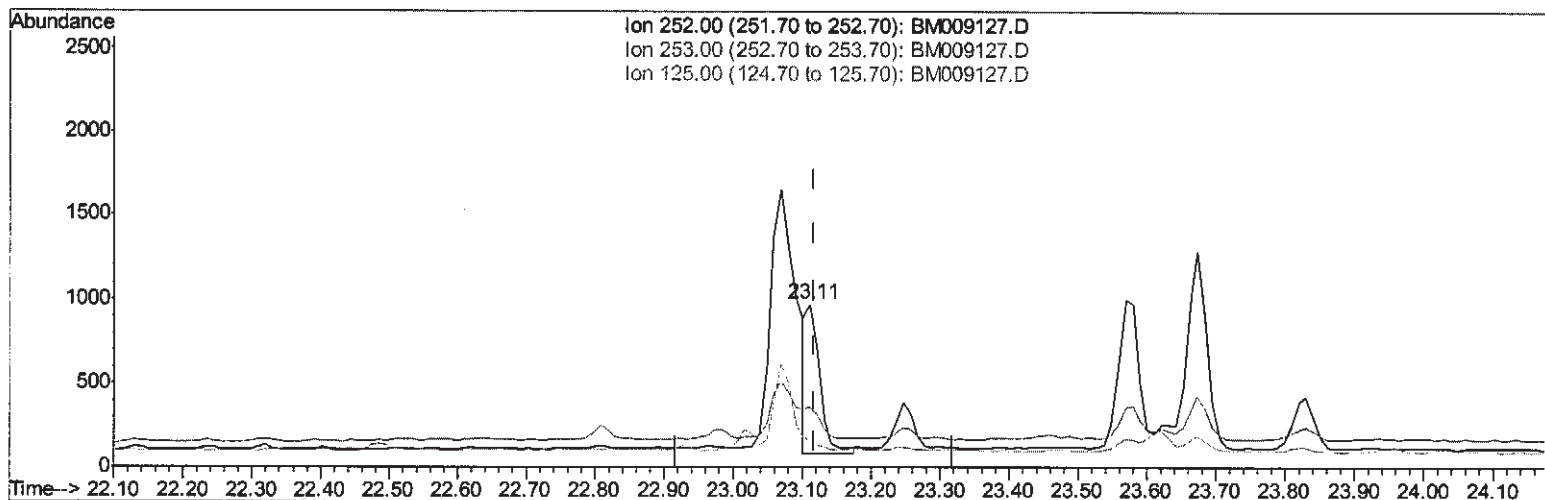

TIC: BM009127.D

(22) Benzo(k)fluoranthene

23.111min (-0.007) 0.29ng/ul m

SJ 3/16/17

response 1155

Ion	Exp%	Act%
252.00	100	100
253.00	30.60	37.46#
125.00	17.10	17.13
0.00	0.00	0.00