


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM030817\
Data File : BM009131.D
Acq On : 09 Mar 2017 06:22
Operator : SJ/MA
Sample : I2069-06
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AG7

Manual Integrations
APPROVED

mohammad
3/9/2017 2:02:46 PM

Quant Time: Mar 09 07:06:52 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 09 02:44:03 2017
Response via : Initial Calibration

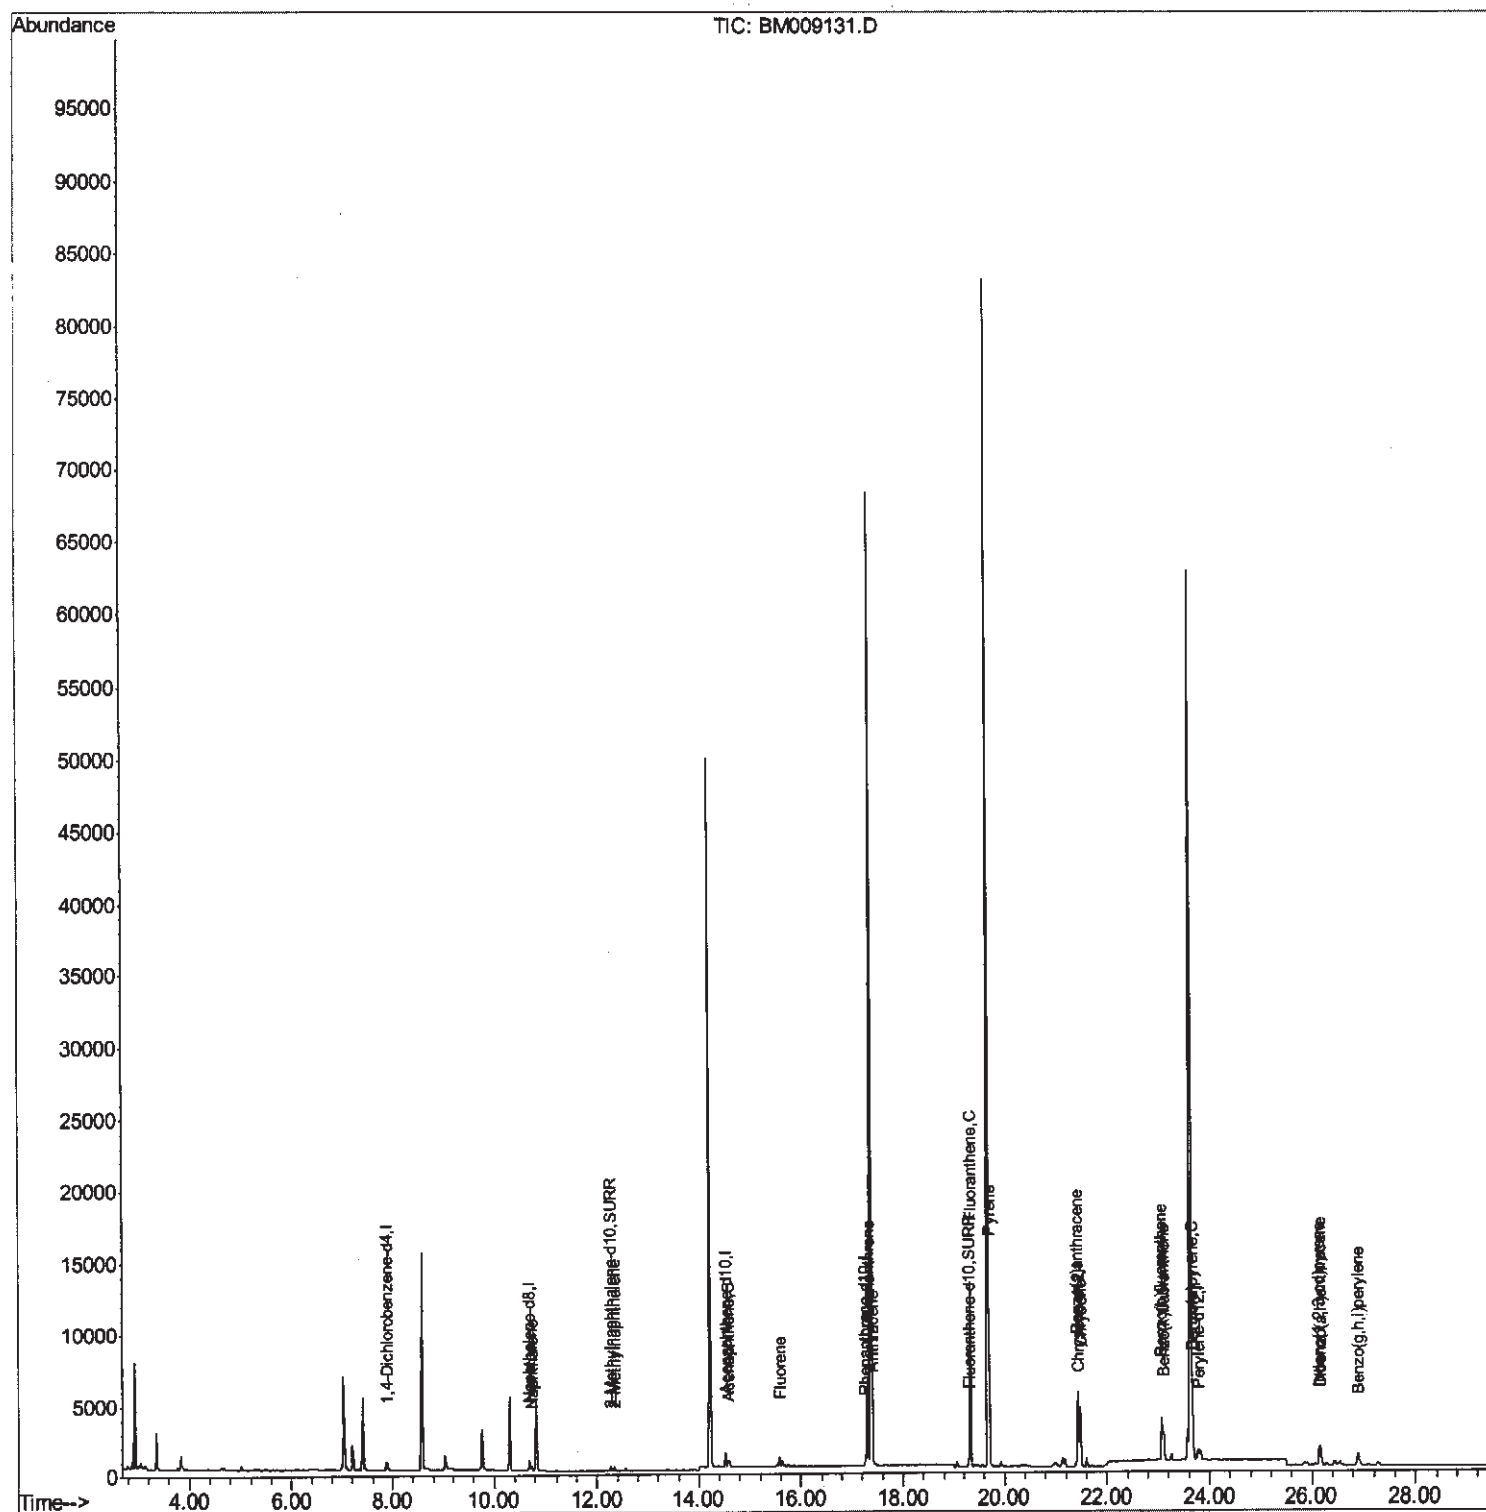




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM030817\
Data File : BM009131.D
Acq On : 09 Mar 2017 06:22
Operator : SJ/MA
Sample : I2069-06
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AG7

Manual Integrations
APPROVED

mohammad
3/9/2017 2:02:46 PM

Quant Time: Mar 09 07:03:20 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 09 02:44:03 2017
Response via : Initial Calibration

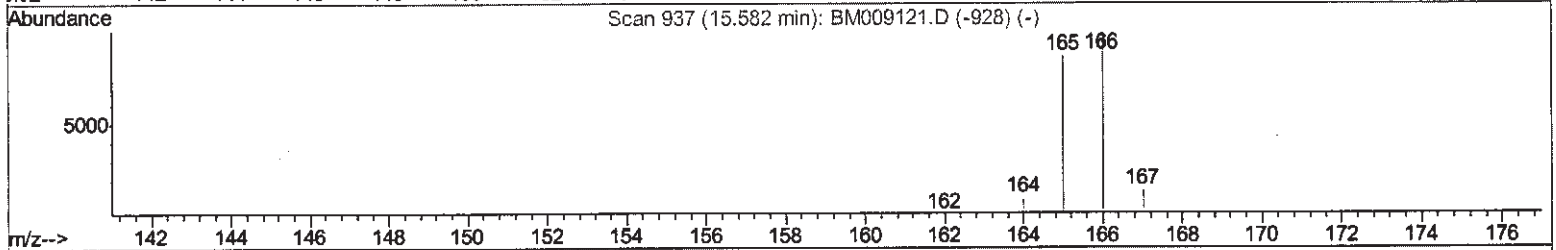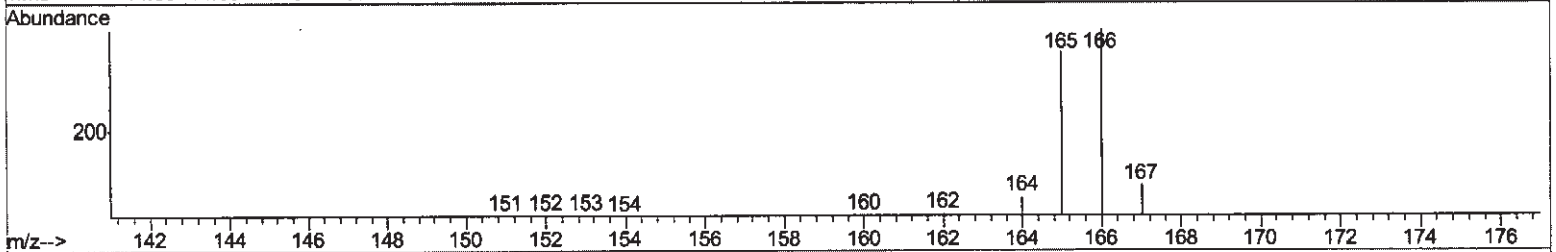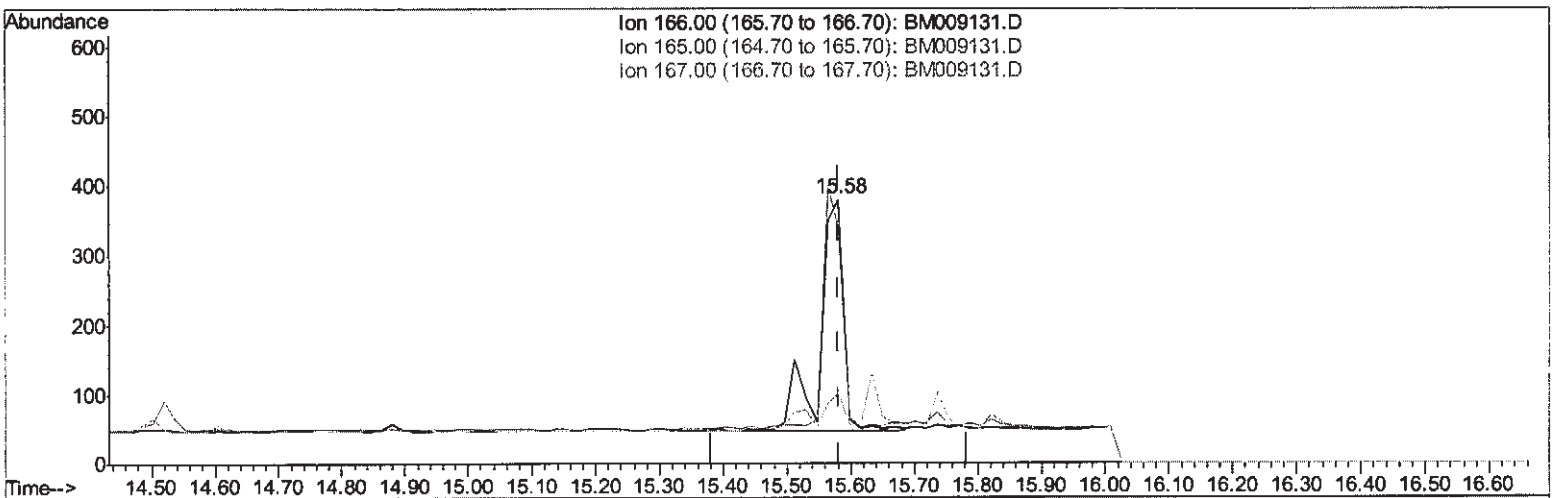

TIC: BM009131.D

(9) Fluorene

15.581min (-0.000) 0.33ng/ul

response 885

Ion	Exp%	Act%
166.00	100	100
165.00	91.80	89.24
167.00	18.30	26.77#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM030817\
Data File : BM009131.D
Acq On : 09 Mar 2017 06:22
Operator : SJ/MA
Sample : I2069-06
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AG7

Manual Integrations
APPROVED

mohammad
3/9/2017 2:02:46 PM

Quant Time: Mar 09 07:03:20 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 09 02:44:03 2017
Response via : Initial Calibration

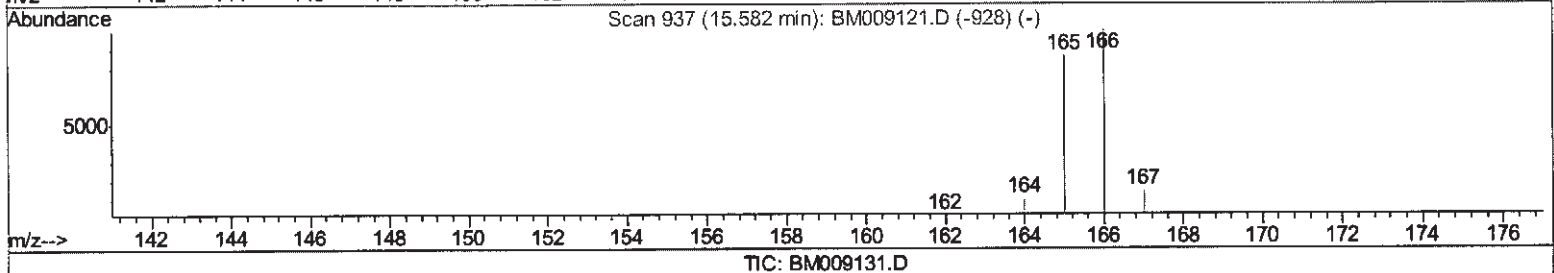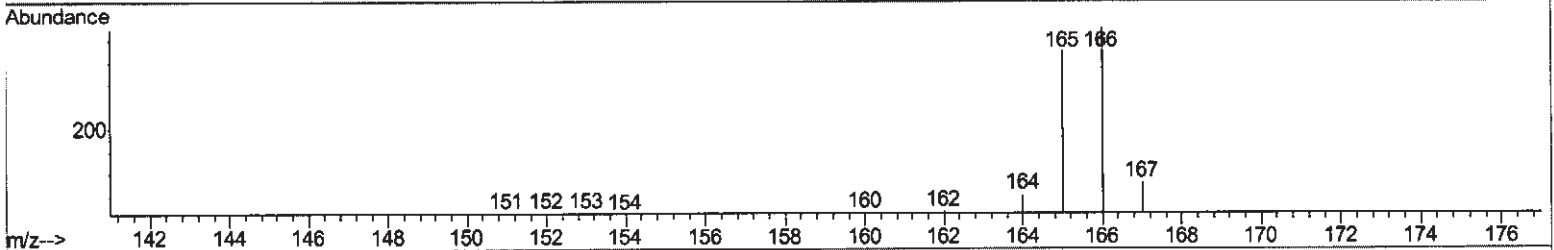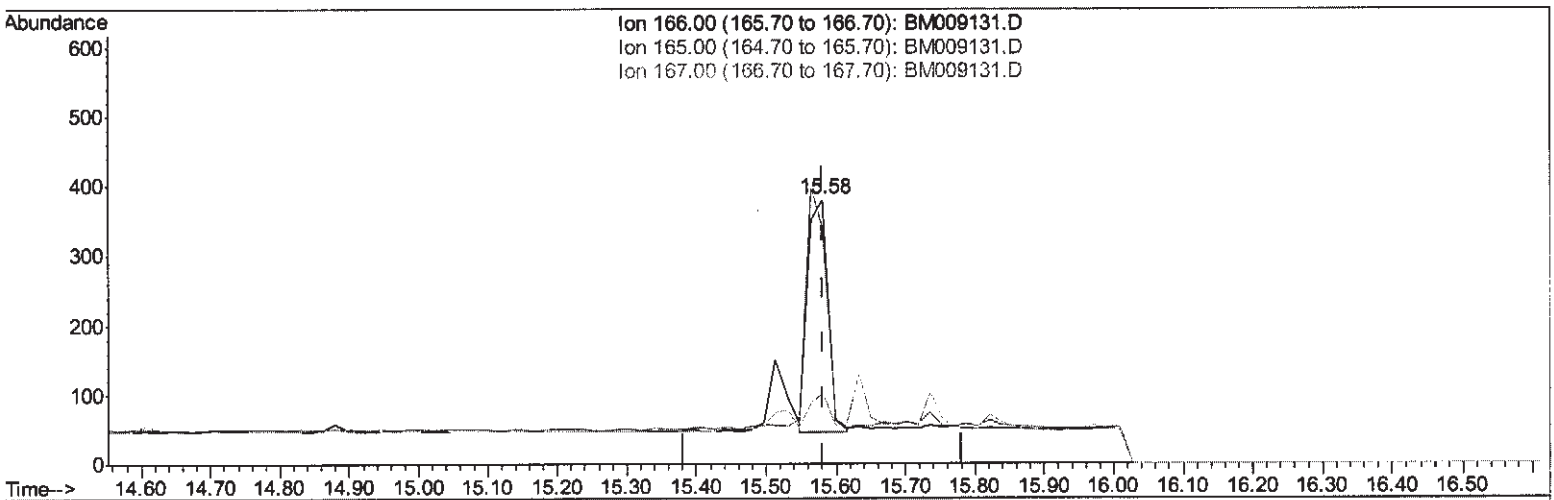

(9) Fluorene

15.581min (-0.000) 0.26ng/ul m

SJ 3/16/17

response 681

Ion	Exp%	Act%
166.00	100	100
165.00	91.80	89.24
167.00	18.30	26.77#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM030817\
Data File : BM009131.D
Acq On : 09 Mar 2017 06:22
Operator : SJ/MA
Sample : I2069-06
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AG7

Manual Integrations
APPROVED

mohammad
3/9/2017 2:02:46 PM

Quant Time: Mar 09 07:03:20 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 09 02:44:03 2017
Response via : Initial Calibration

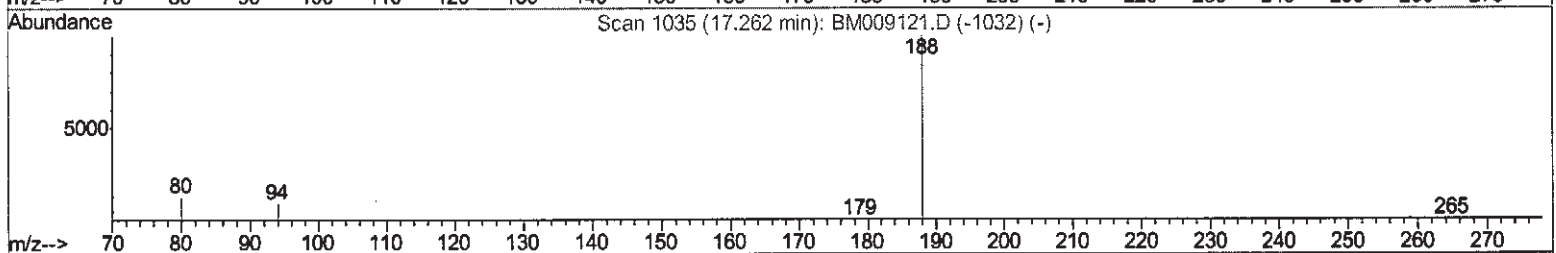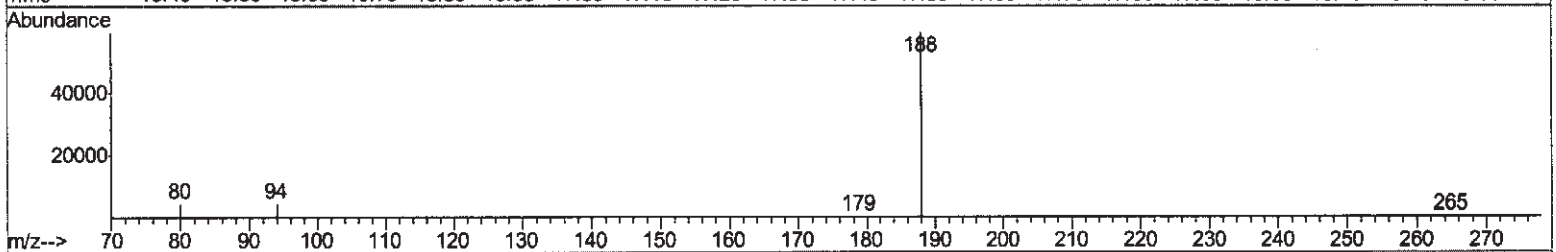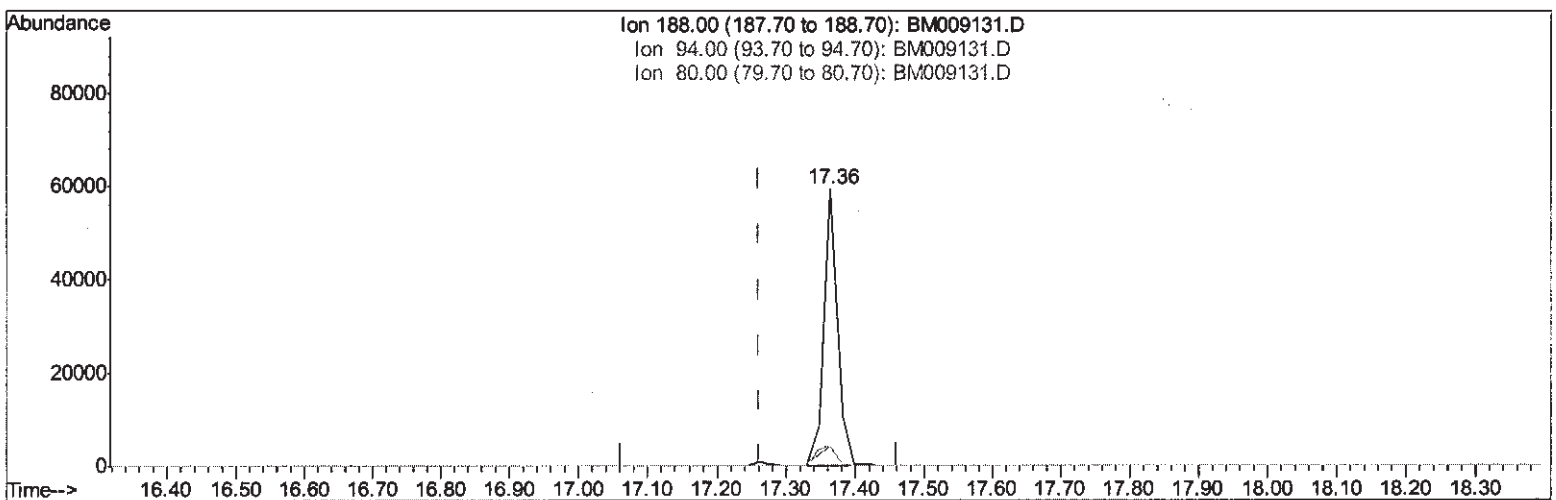

TIC: BM009131.D

(10) Phenanthrene-d10 (I)

17.365min (+0.103) 0.40ng/ul

response 80848

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	7.01#
80.00	11.80	7.07#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM030817\
Data File : BM009131.D
Acq On : 09 Mar 2017 06:22
Operator : SJ/MA
Sample : I2069-06
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AG7

Manual Integrations
APPROVED

mohammad
3/9/2017 2:02:46 PM

Quant Time: Mar 09 07:03:20 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 09 02:44:03 2017
Response via : Initial Calibration

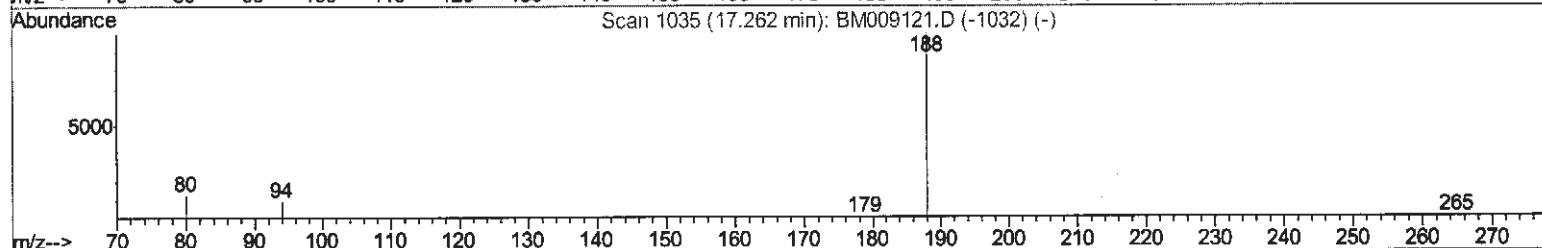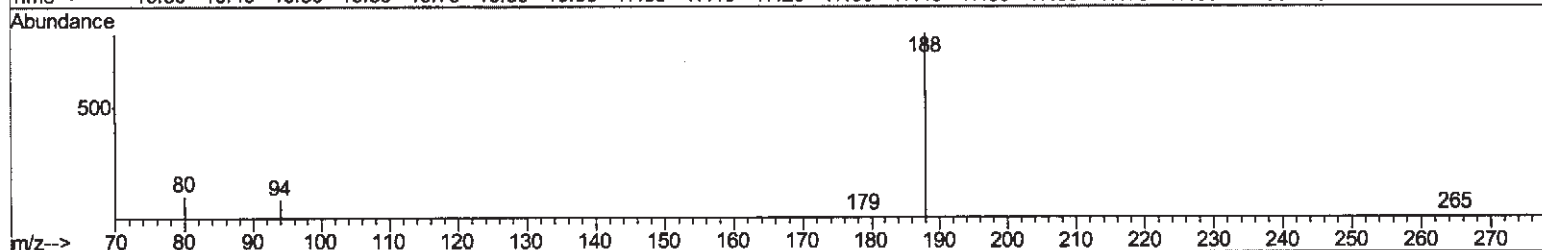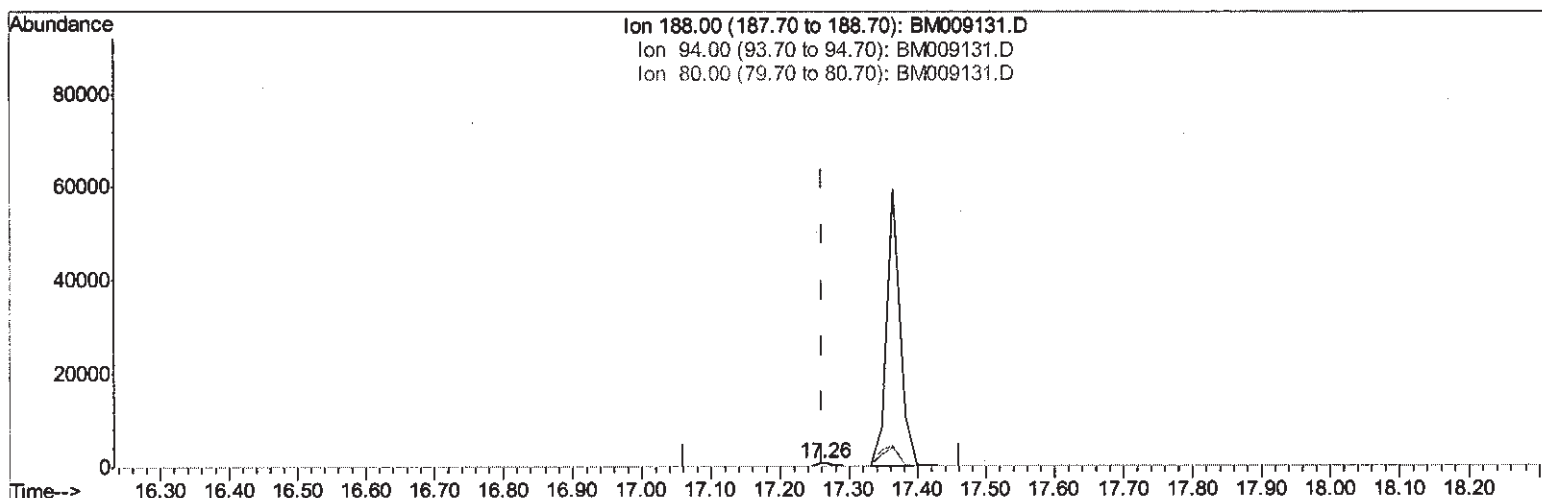

TIC: BM009131.D

(10) Phenanthrene-d10 (I)

17.262min (-0.000) 0.40ng/ul m SJ 3/16/17

response 1269

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	14.66#
80.00	11.80	16.77#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM030817\
Data File : BM009131.D
Acq On : 09 Mar 2017 06:22
Operator : SJ/MA
Sample : I2069-06
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AG7

Manual Integrations
APPROVED

mohammad
3/9/2017 2:02:46 PM

Quant Time: Mar 09 07:03:20 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 09 02:44:03 2017
Response via : Initial Calibration

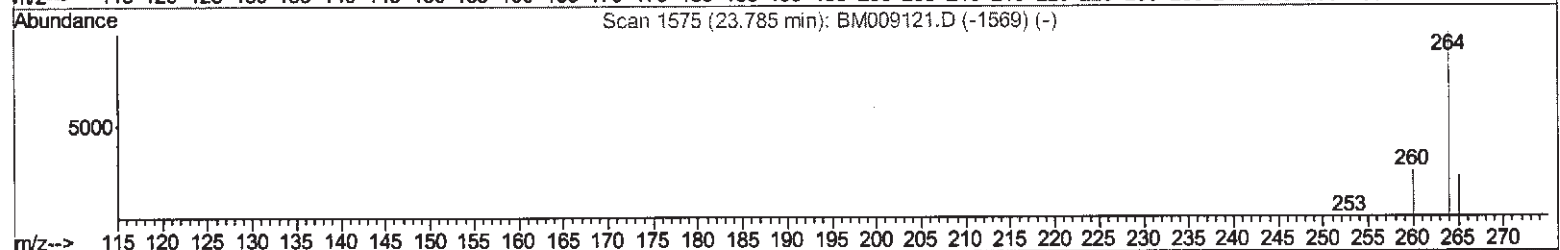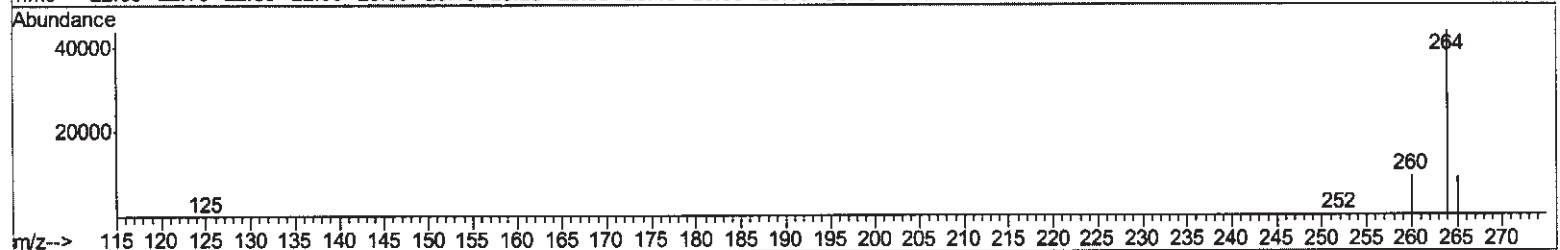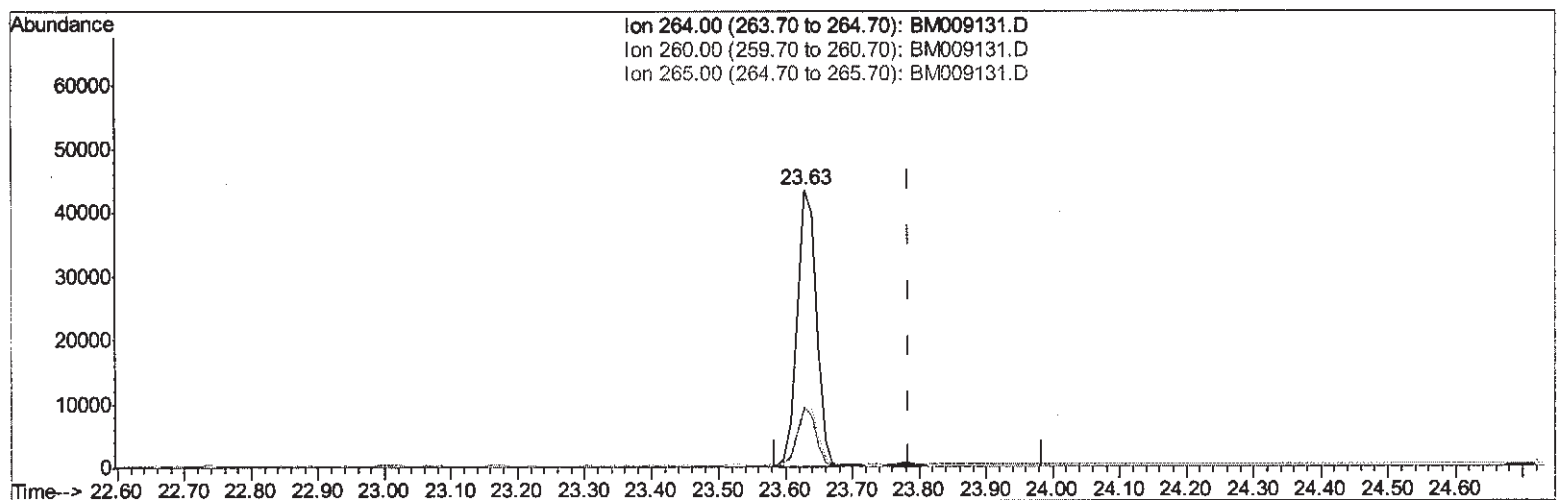

TIC: BM009131.D

(20) Perylene-d12 (I)

23.628min (-0.156) 0.40ng/ul

response 85240

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	21.62#
265.00	103.50	20.98#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM030817\
Data File : BM009131.D
Acq On : 09 Mar 2017 06:22
Operator : SJ/MA
Sample : I2069-06
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AG7

Manual Integrations
APPROVED

mohammad
3/9/2017 2:02:46 PM

Quant Time: Mar 09 07:03:20 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 09 02:44:03 2017
Response via : Initial Calibration

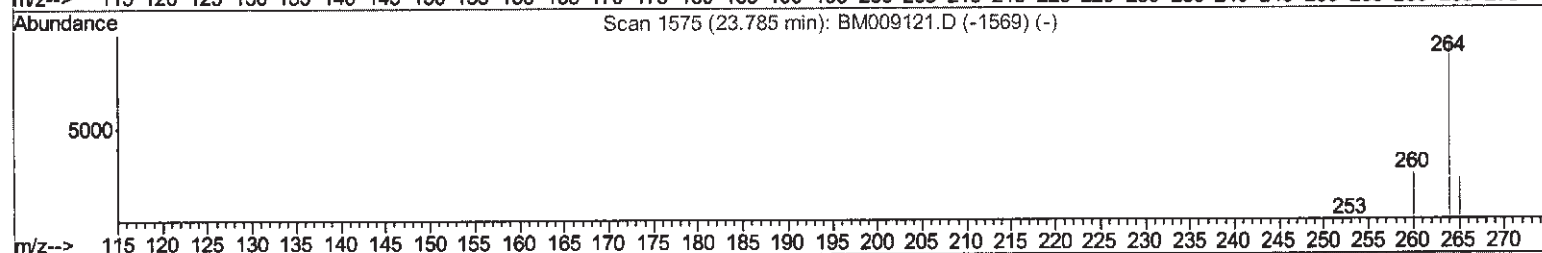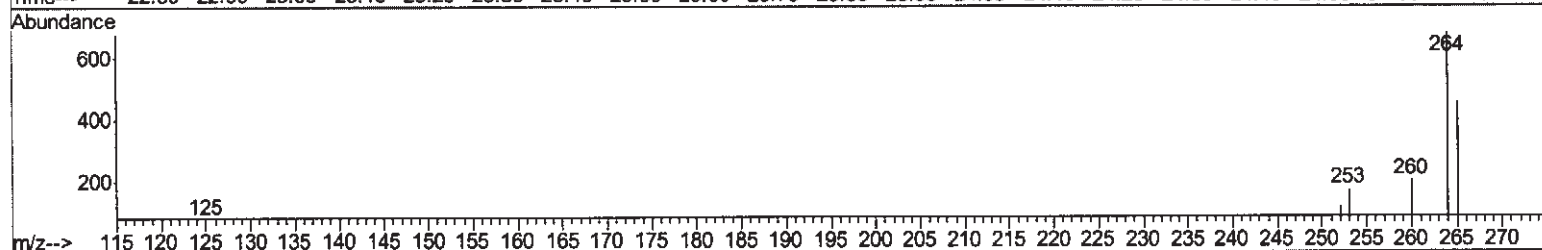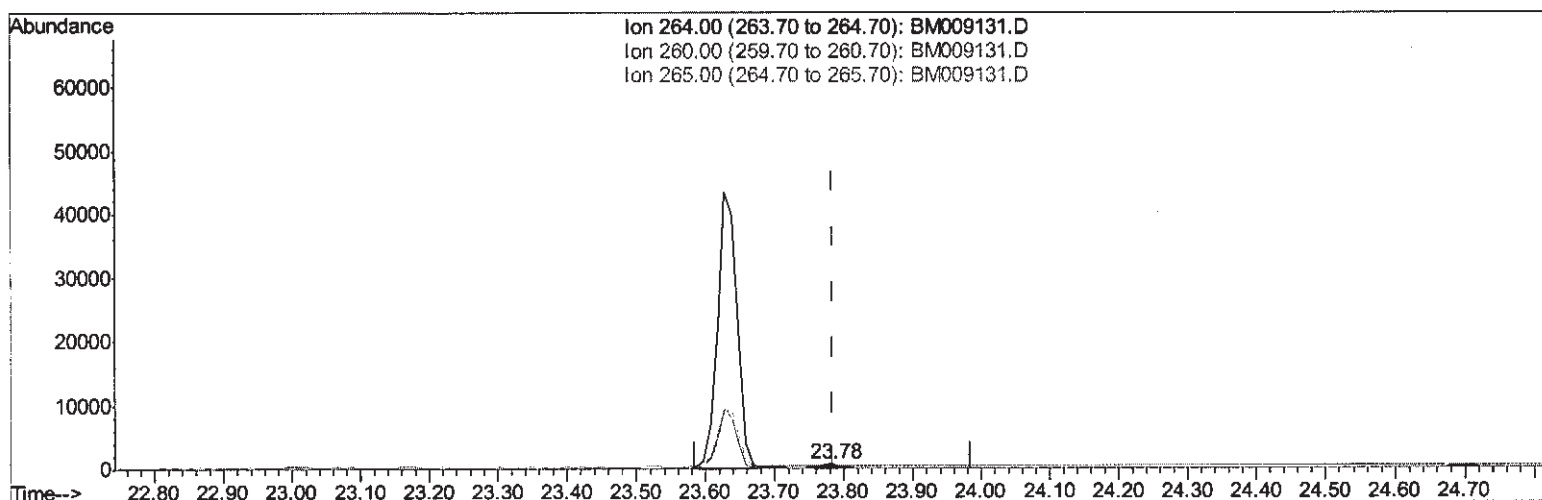

TIC: BM009131.D

(20) Perylene-d12 (I)

23.785min (-0.000) 0.40ng/ul m

SJ 3/16/17

response 1309

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	29.59
265.00	103.50	66.86#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM030817\
Data File : BM009131.D
Acq On : 09 Mar 2017 06:22
Operator : SJ/MA
Sample : I2069-06
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AG7

Manual Integrations
APPROVED

mohammad
3/9/2017 2:02:46 PM

Quant Time: Mar 09 07:05:03 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 09 02:44:03 2017
Response via : Initial Calibration

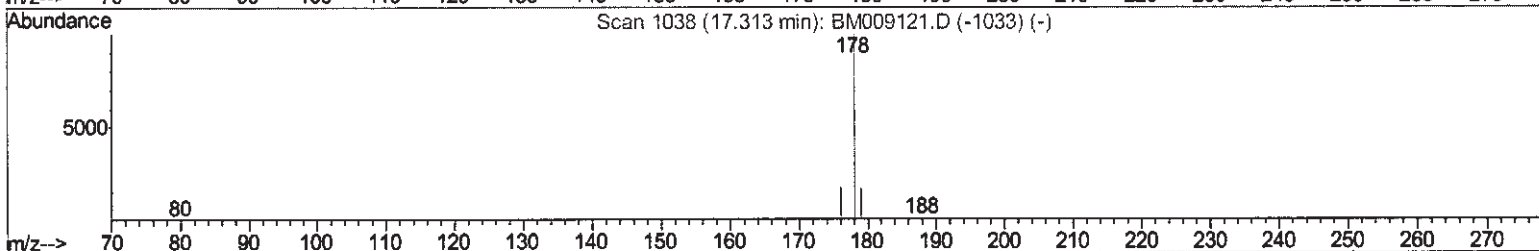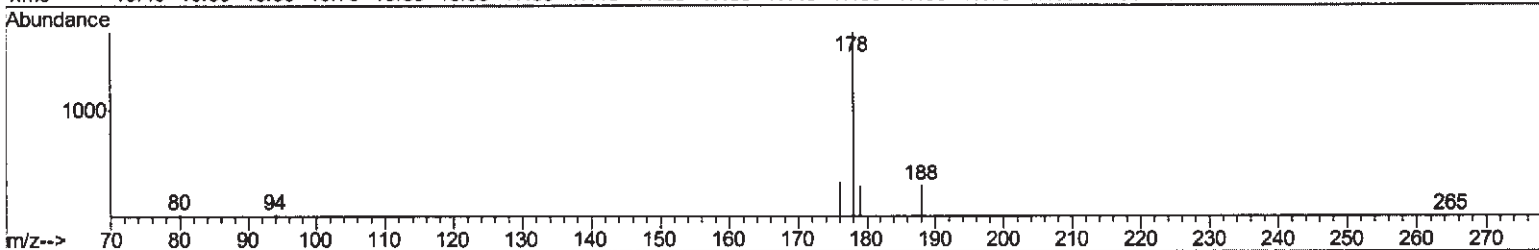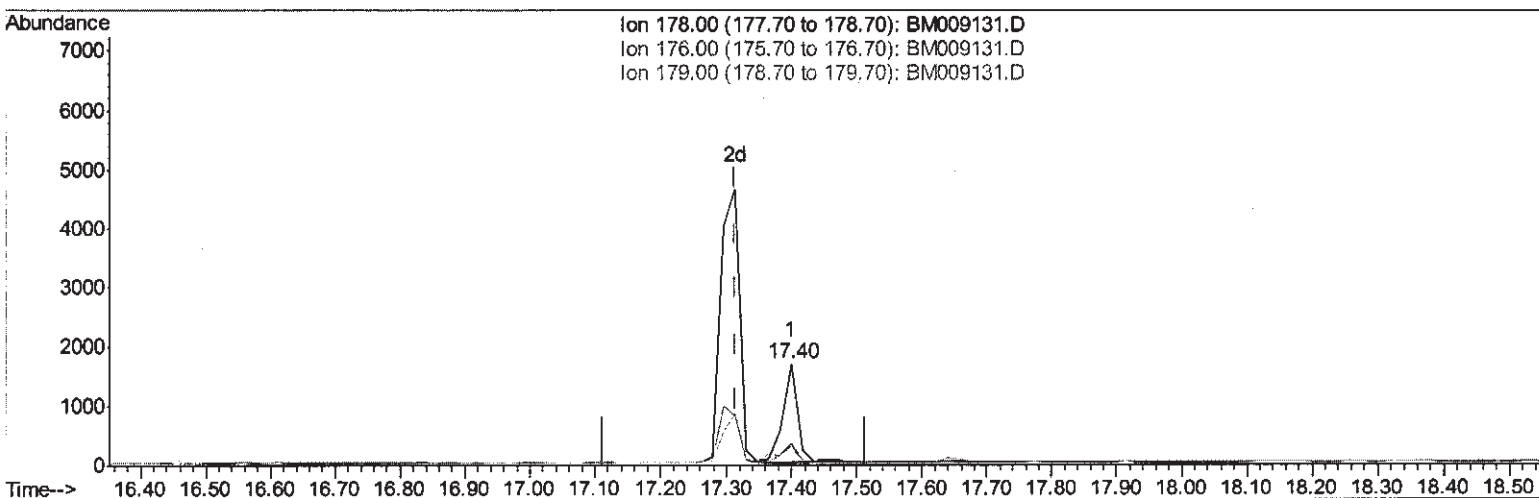

TIC: BM009131.D

(12) Phenanthrene

17.399min (+0.086) 0.66ng/ul

response 2617

Ion	Exp%	Act%
178.00	100	100
176.00	23.00	20.72
179.00	17.00	18.72
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM030817\
Data File : BM009131.D
Acq On : 09 Mar 2017 06:22
Operator : SJ/MA
Sample : I2069-06
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleID :
C0AG7

Manual Integrations
APPROVED

mohammad
3/9/2017 2:02:46 PM

Quant Time: Mar 09 07:05:03 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 09 02:44:03 2017
Response via : Initial Calibration

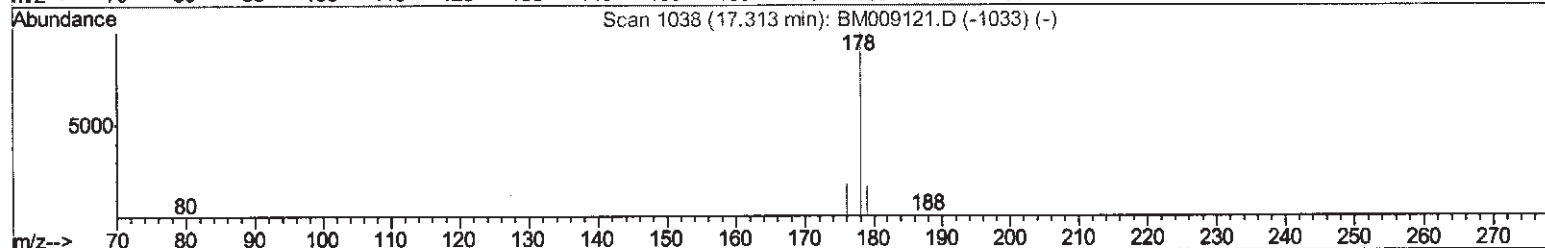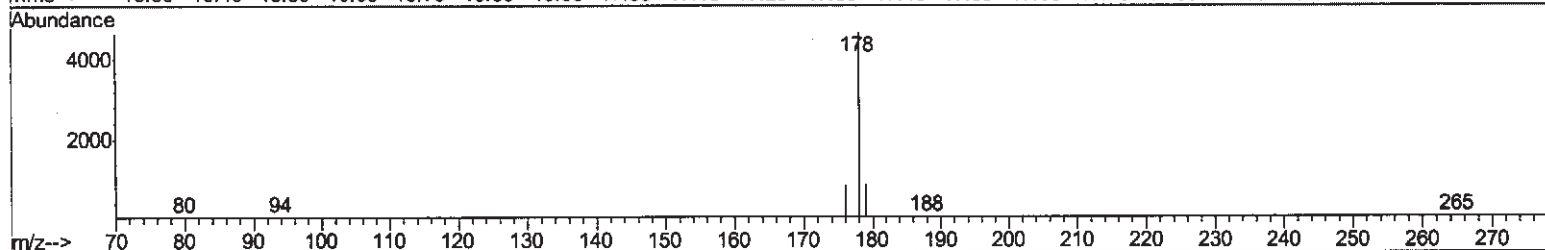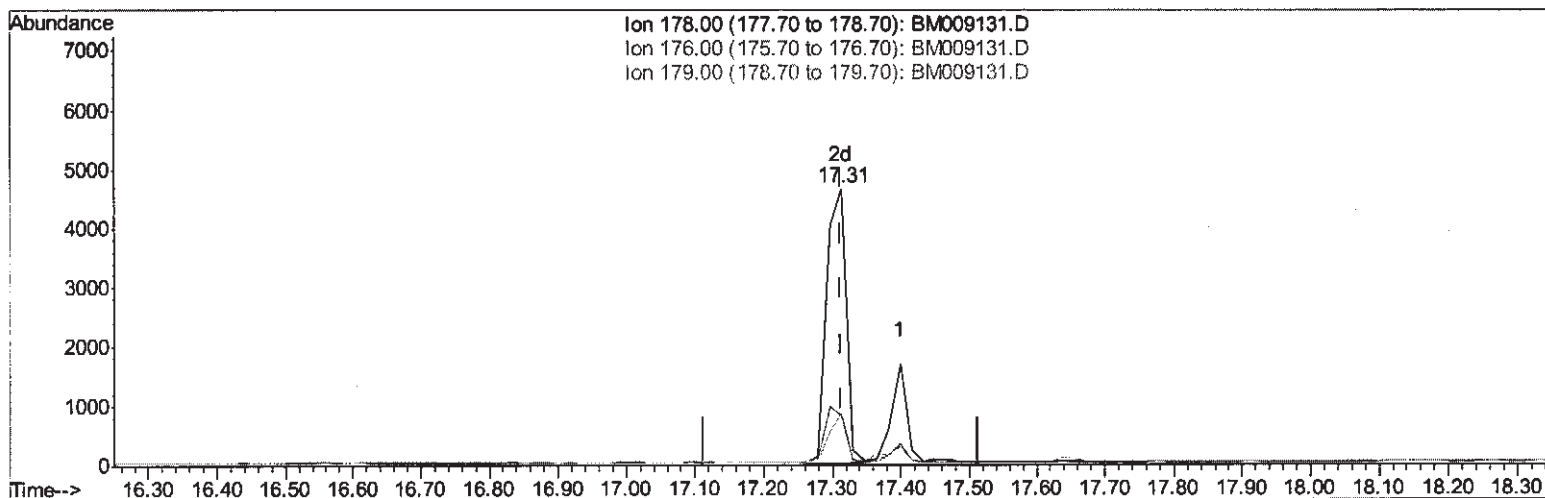

(12) Phenanthrene

17.313min (-0.000) 2.33ng/ul m

SJ 3/16/17

response 9289

Ion	Exp%	Act%
178.00	100	100
176.00	23.00	17.74#
179.00	17.00	18.60
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM030817\
Data File : BM009131.D
Acq On : 09 Mar 2017 06:22
Operator : SJ/MA
Sample : I2069-06
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AG7

Manual Integrations
APPROVED

mohammad
3/9/2017 2:02:46 PM

Quant Time: Mar 09 07:05:03 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 09 02:44:03 2017
Response via : Initial Calibration

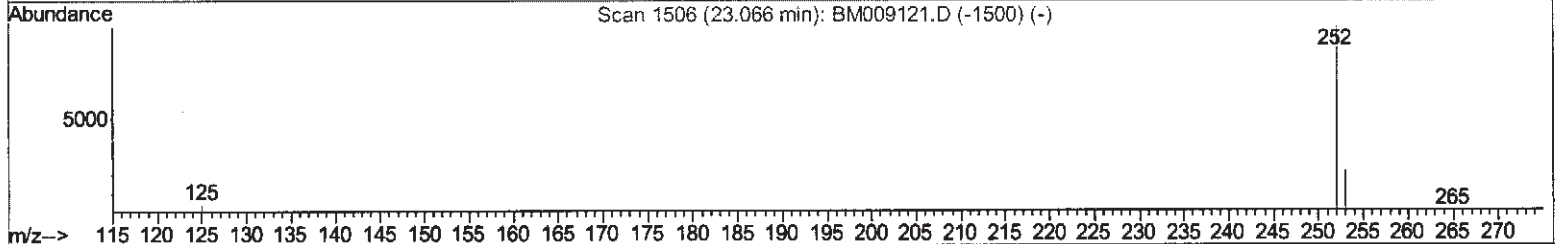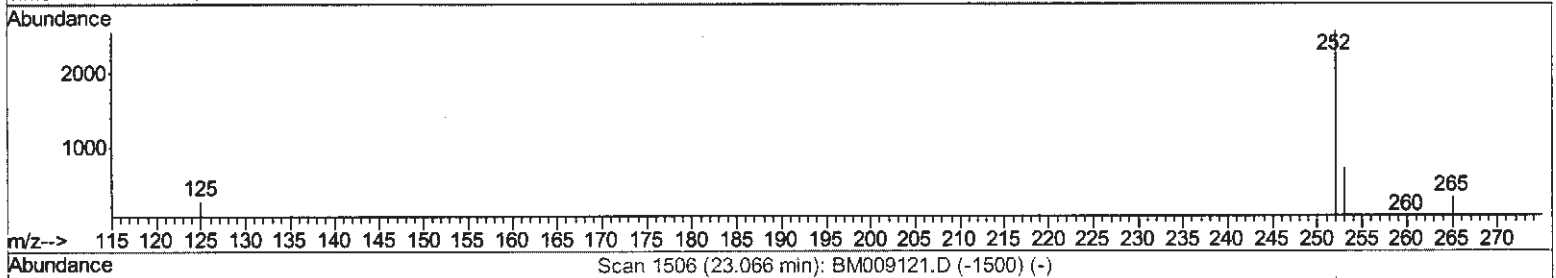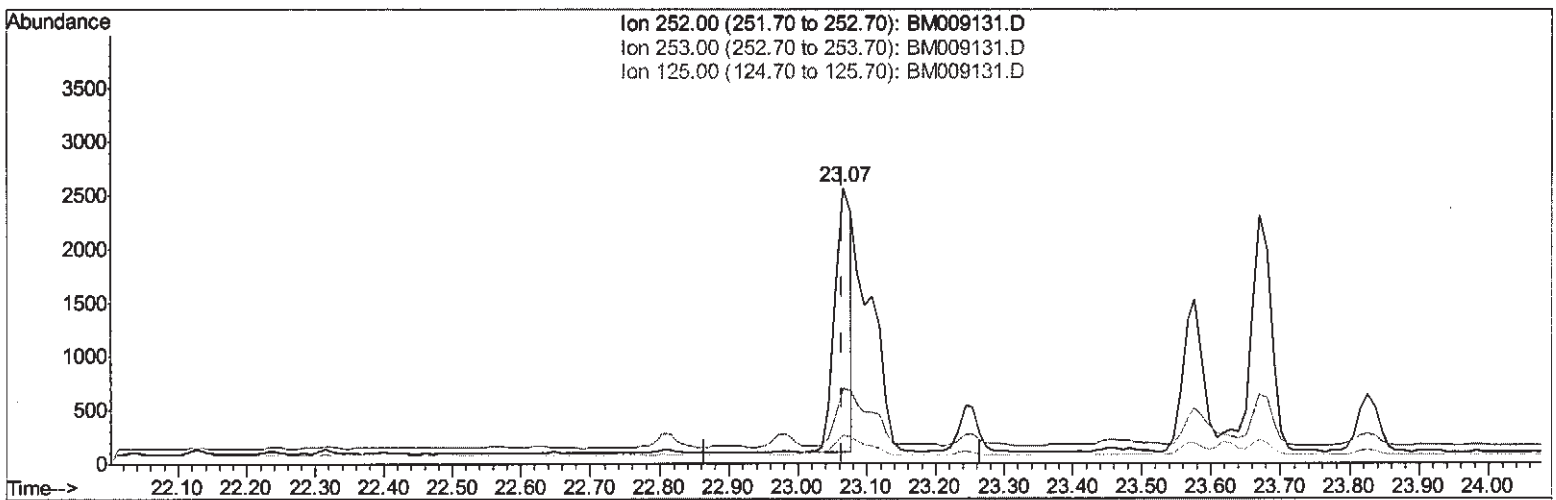

(21) Benzo(b)fluoranthene

23.066min (-0.000) 0.81ng/ul

response 4172

Ion	Exp%	Act%
252.00	100	100
253.00	32.10	27.34
125.00	17.50	10.35
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM030817\
Data File : BM009131.D
Acq On : 09 Mar 2017 06:22
Operator : SJ/MA
Sample : I2069-06
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AG7

Manual Integrations
APPROVED

mohammad
3/9/2017 2:02:46 PM

Quant Time: Mar 09 07:05:03 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 09 02:44:03 2017
Response via : Initial Calibration

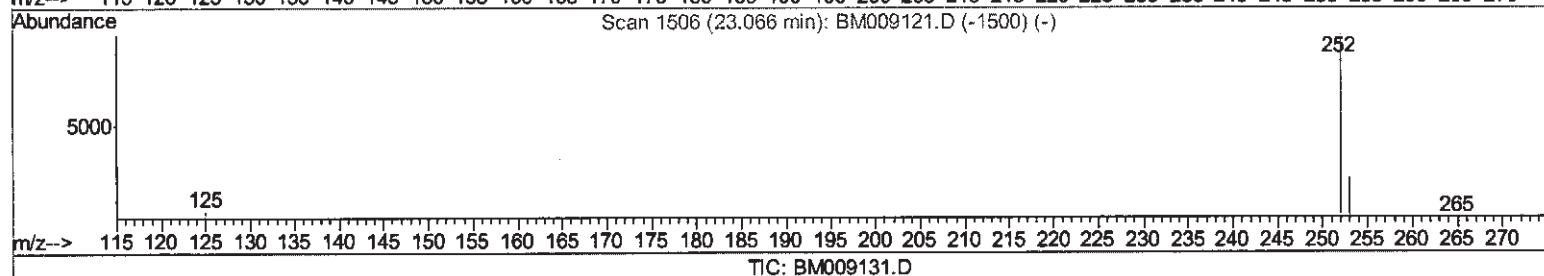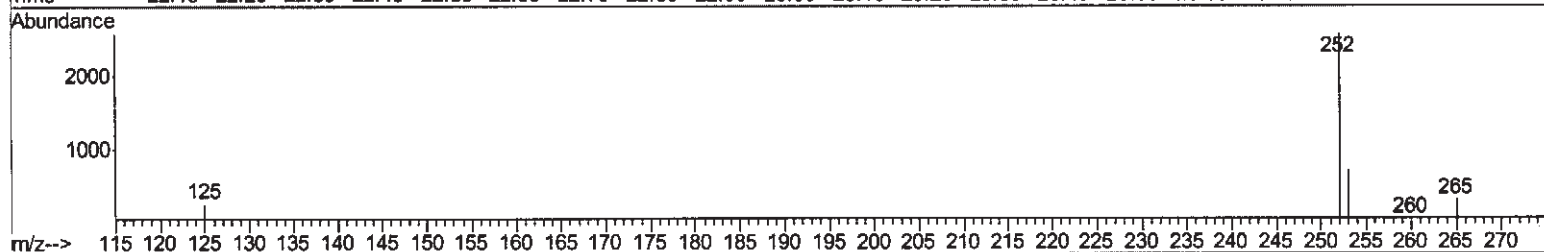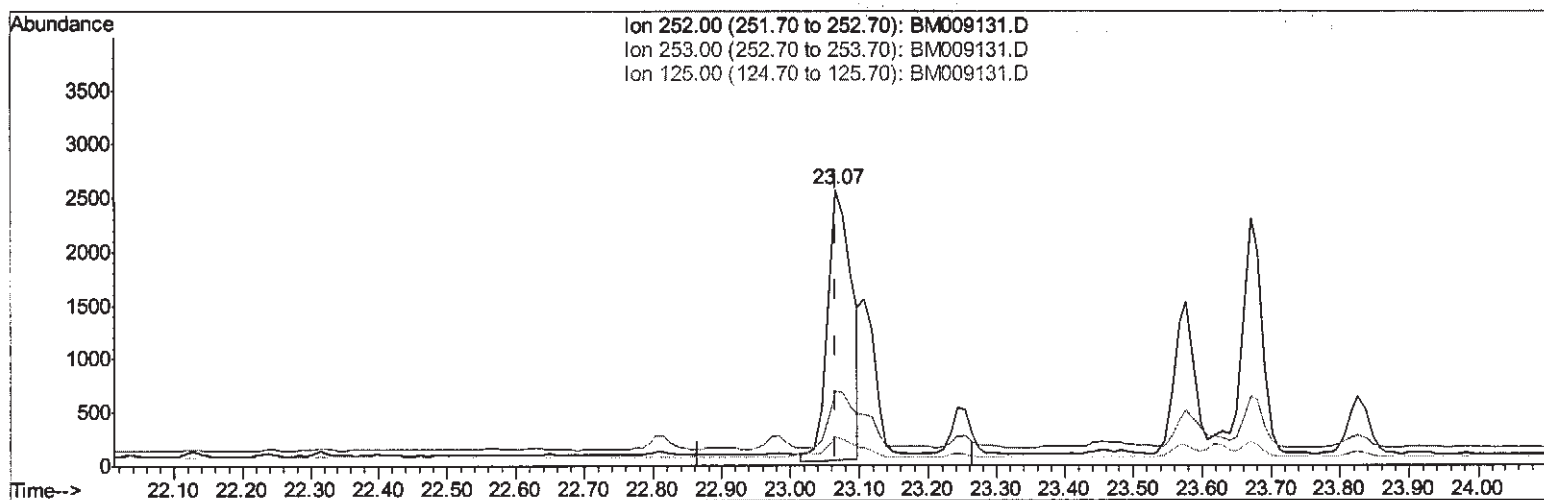

(21) Benzo(b)fluoranthene

23.066min (-0.000) 1.24ng/ul m

SJ 3/16/17

response 6373

Ion	Exp%	Act%
252.00	100	100
253.00	32.10	27.34
125.00	17.50	10.35
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM030817\
Data File : BM009131.D
Acq On : 09 Mar 2017 06:22
Operator : SJ/MA
Sample : I2069-06
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AG7

Manual Integrations
APPROVED

mohammad
3/9/2017 2:02:46 PM

Quant Time: Mar 09 07:05:03 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 09 02:44:03 2017
Response via : Initial Calibration

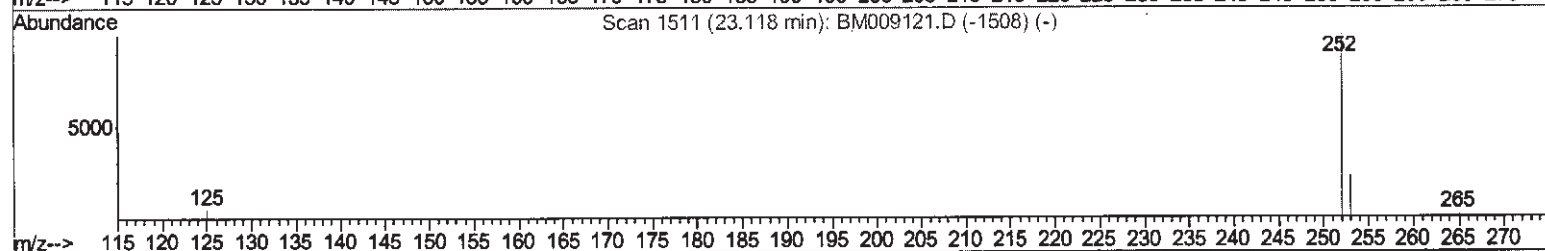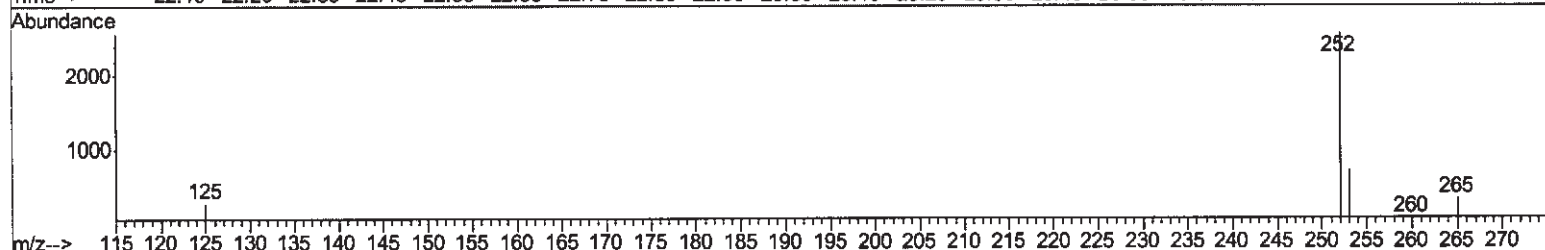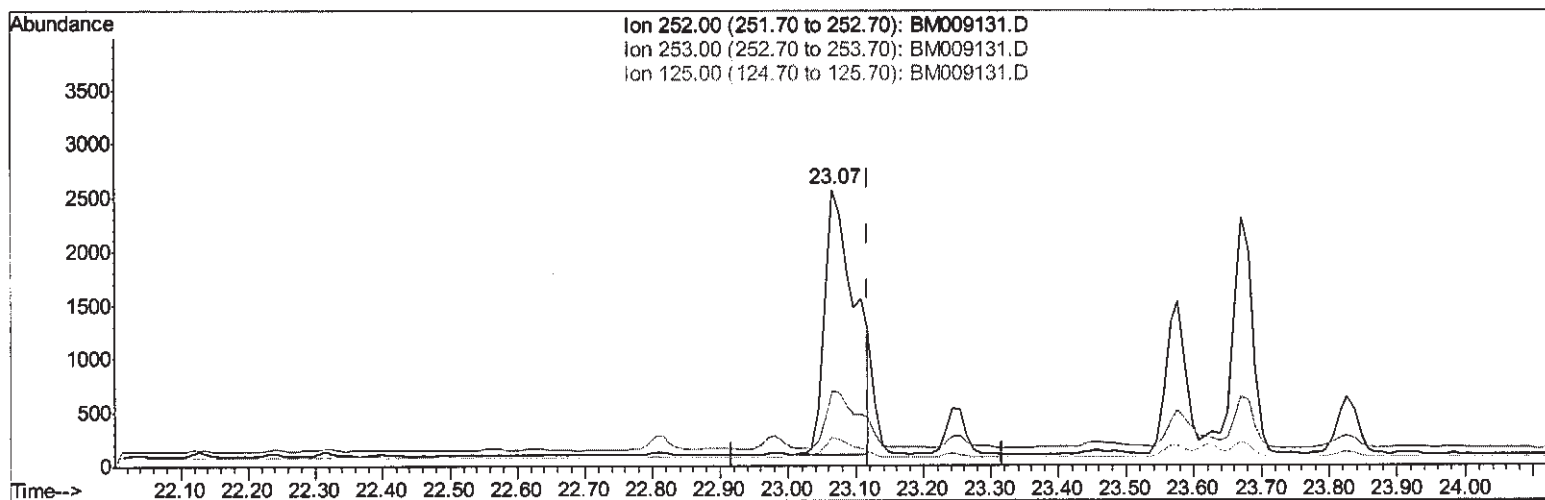

(22) Benzo(k)fluoranthene

23.066min (-0.052) 1.70ng/ul

response 7710

Ion	Exp%	Act%
252.00	100	100
253.00	30.60	27.34
125.00	17.10	10.35#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM030817\
Data File : BM009131.D
Acq On : 09 Mar 2017 06:22
Operator : SJ/MA
Sample : I2069-06
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AG7

Manual Integrations
APPROVED

mohammad
3/9/2017 2:02:46 PM

Quant Time: Mar 09 07:05:03 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 09 02:44:03 2017
Response via : Initial Calibration

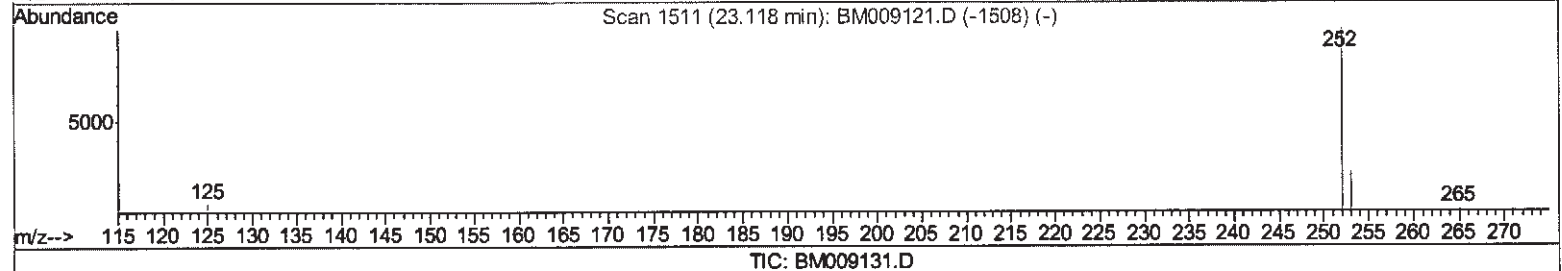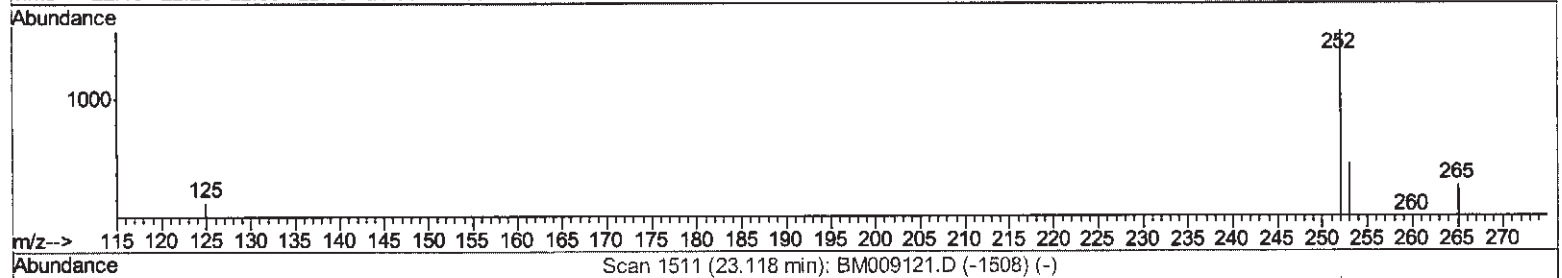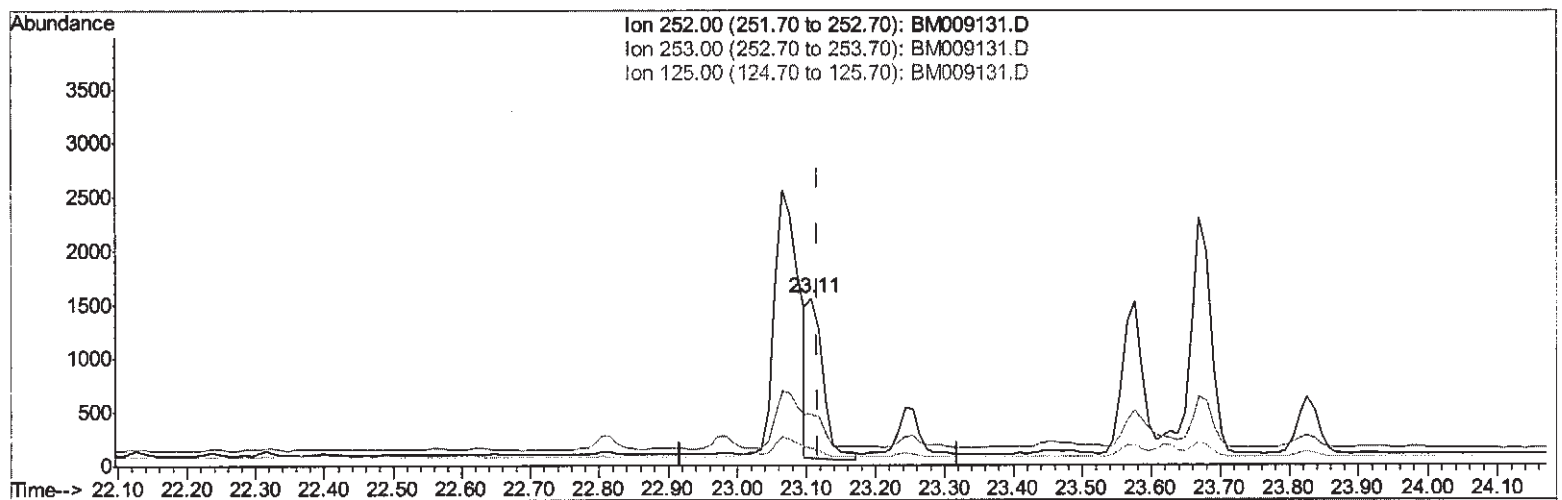

(22) Benzo(k)fluoranthene

23.107min (-0.011) 0.49ng/ul m

SJ 3/16/17

response 2206

Ion	Exp%	Act%
252.00	100	100
253.00	30.60	31.15
125.00	17.10	10.85#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM030817\
Data File : BM009131.D
Acq On : 09 Mar 2017 06:22
Operator : SJ/MA
Sample : I2069-06
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AG7

Manual Integrations
APPROVED

mohammad
3/9/2017 2:02:46 PM

Quant Time: Mar 09 07:05:03 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 09 02:44:03 2017
Response via : Initial Calibration

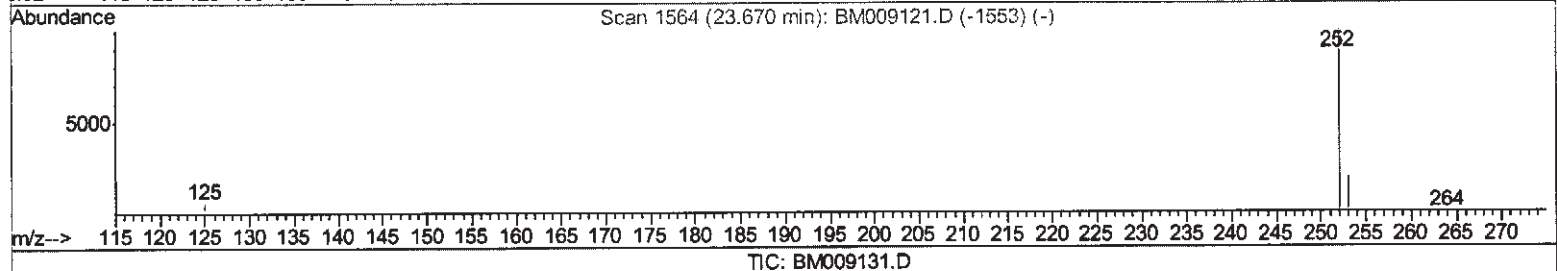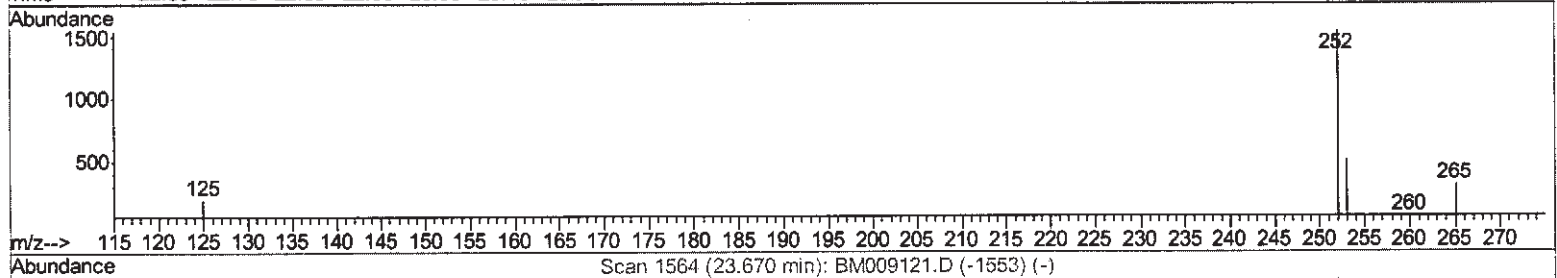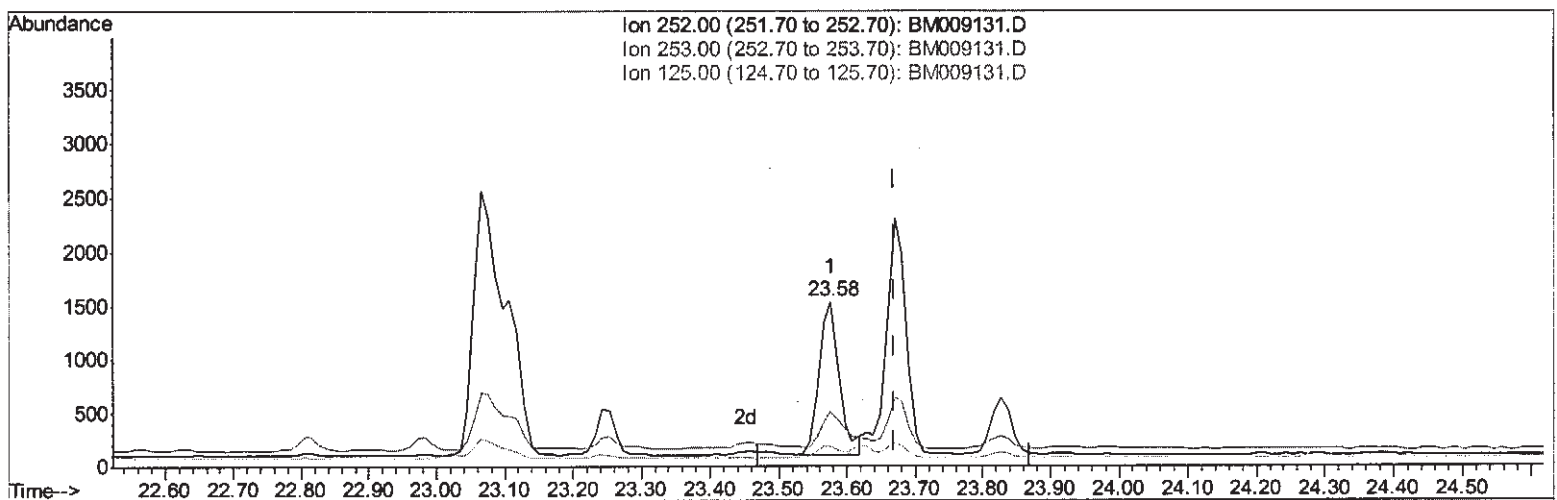

(23) Benzo(a)pyrene (C)

23.576min (-0.094) 0.64ng/ul

response 2975

Ion	Exp%	Act%
252.00	100	100
253.00	35.60	33.20
125.00	22.60	12.57#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM030817\
Data File : BM009131.D
Acq On : 09 Mar 2017 06:22
Operator : SJ/MA
Sample : I2069-06
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AG7

Manual Integrations
APPROVED

mohammad
3/9/2017 2:02:46 PM

Quant Time: Mar 09 07:05:03 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 09 02:44:03 2017
Response via : Initial Calibration

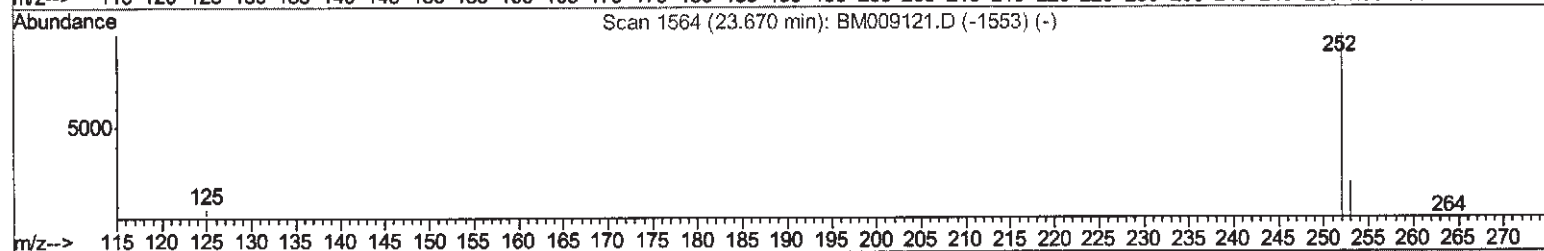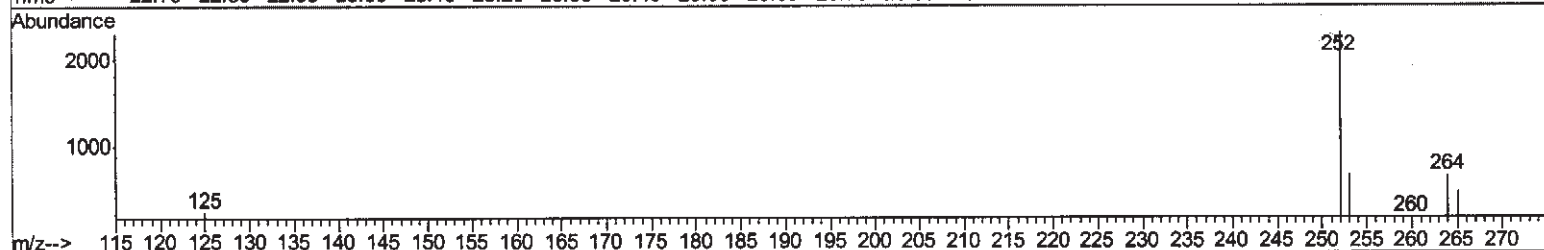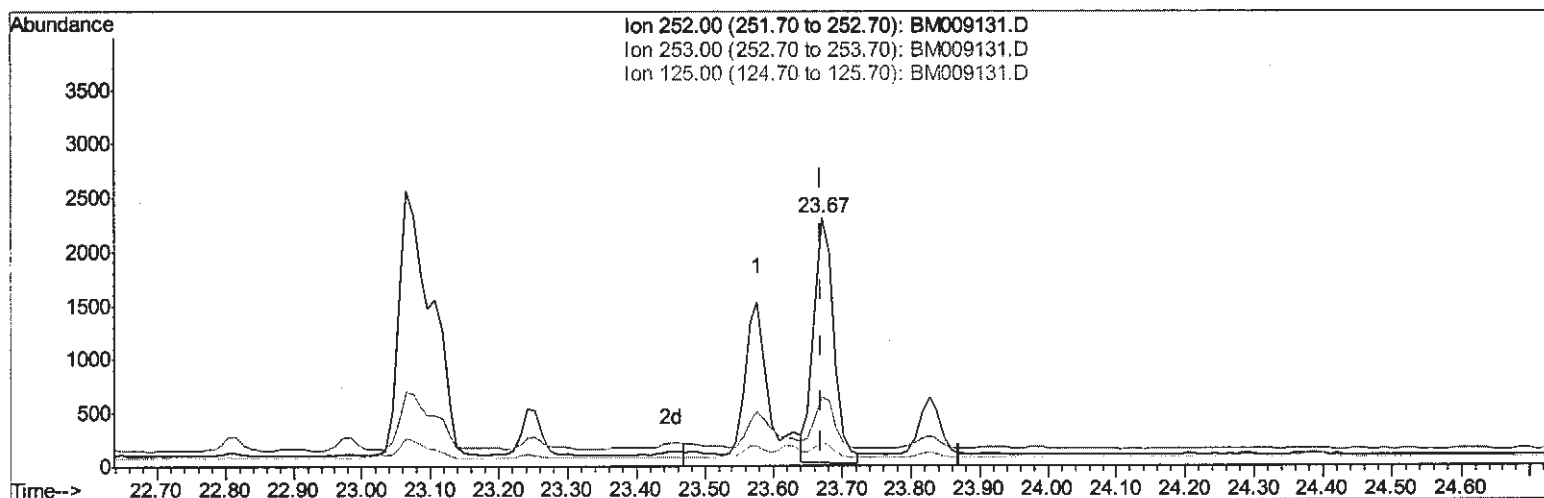

TIC: BM009131.D

(23) Benzo(a)pyrene (C)

23.670min (-0.000) 1.00ng/ul m

SJ 3/16/17

response 4632

Ion	Exp%	Act%
252.00	100	100
253.00	35.60	27.98#
125.00	22.60	9.66#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM030817\
Data File : BM009131.D
Acq On : 09 Mar 2017 06:22
Operator : SJ/MA
Sample : I2069-06
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AG7

Manual Integrations
APPROVED

mohammad
3/9/2017 2:02:46 PM

Quant Time: Mar 09 07:05:03 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 09 02:44:03 2017
Response via : Initial Calibration

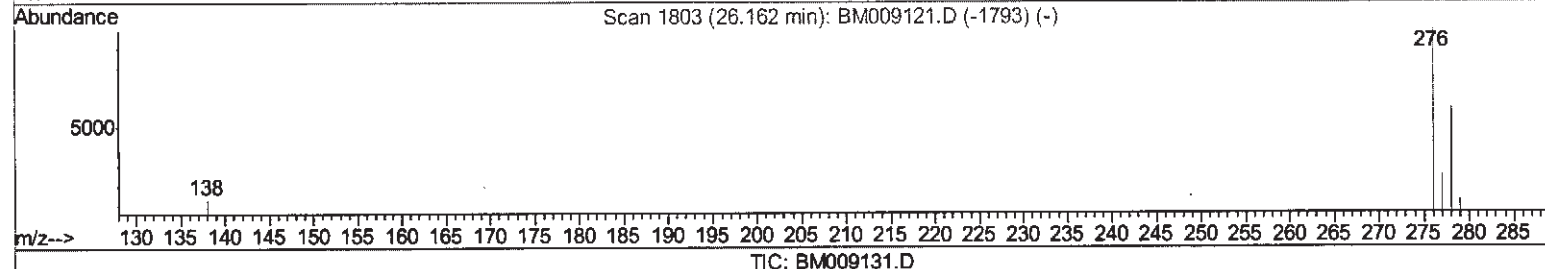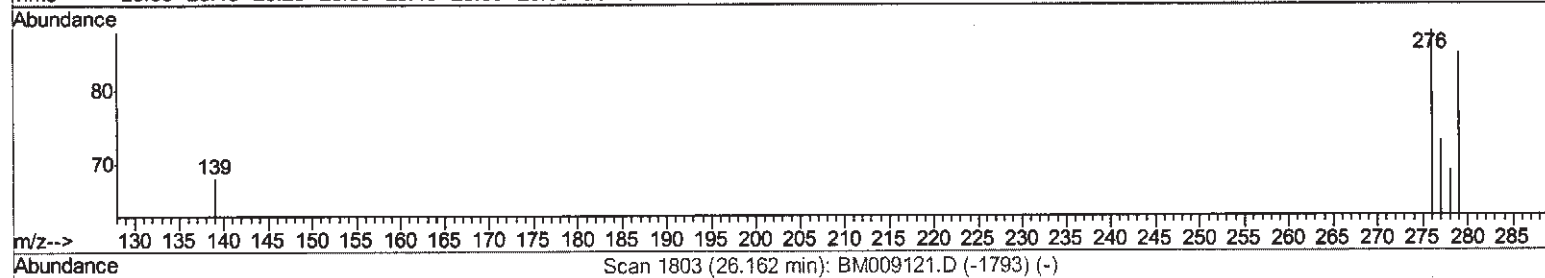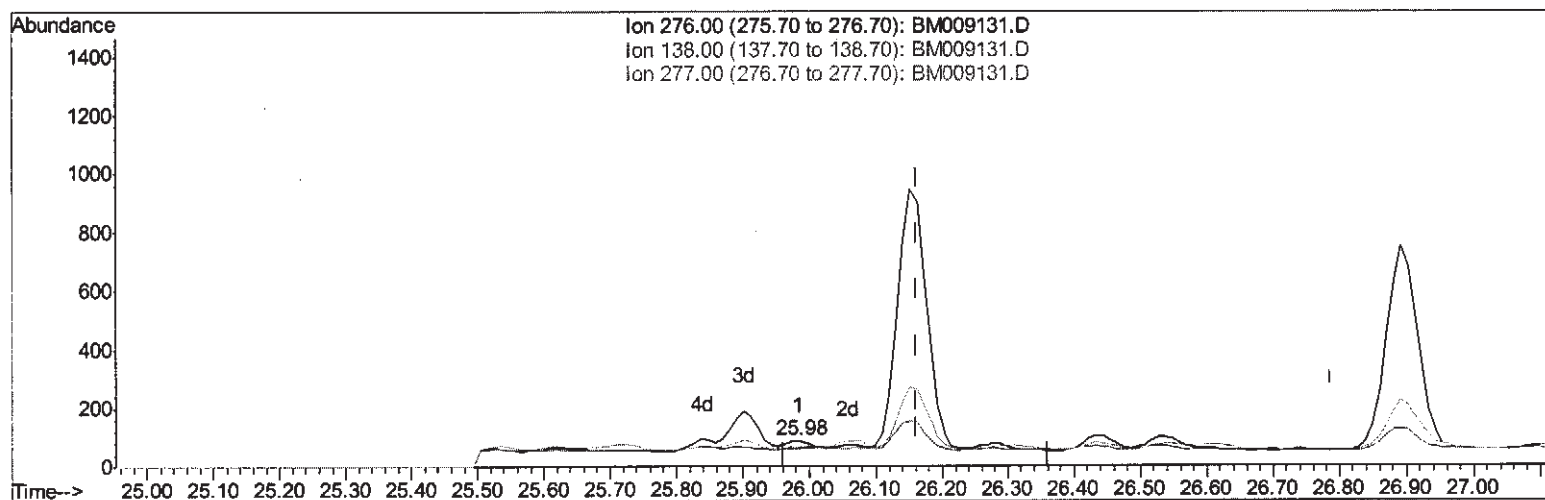

(24) Indeno(1,2,3-cd)pyrene

25.984min (-0.177) 0.01ng/ul

response 62

Ion	Exp%	Act%
276.00	100	100
138.00	23.90	0.00#
277.00	24.50	0.00#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM030817\
Data File : BM009131.D
Acq On : 09 Mar 2017 06:22
Operator : SJ/MA
Sample : I2069-06
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AG7

Manual Integrations
APPROVED

mohammad
3/9/2017 2:02:46 PM

Quant Time: Mar 09 07:05:03 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 09 02:44:03 2017
Response via : Initial Calibration

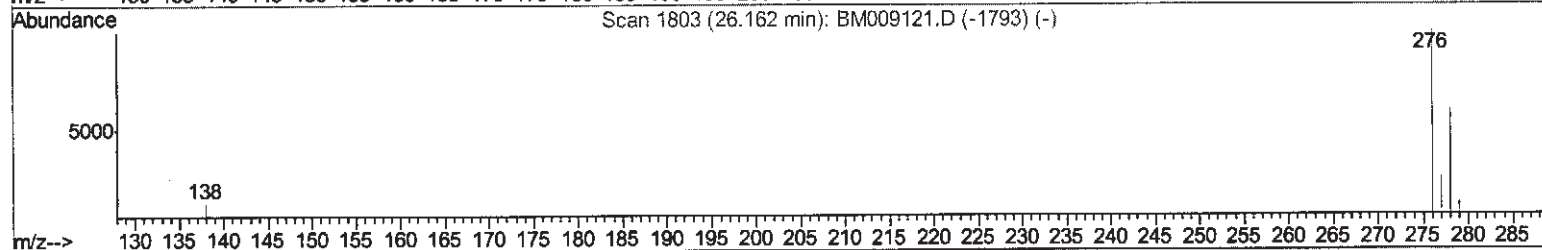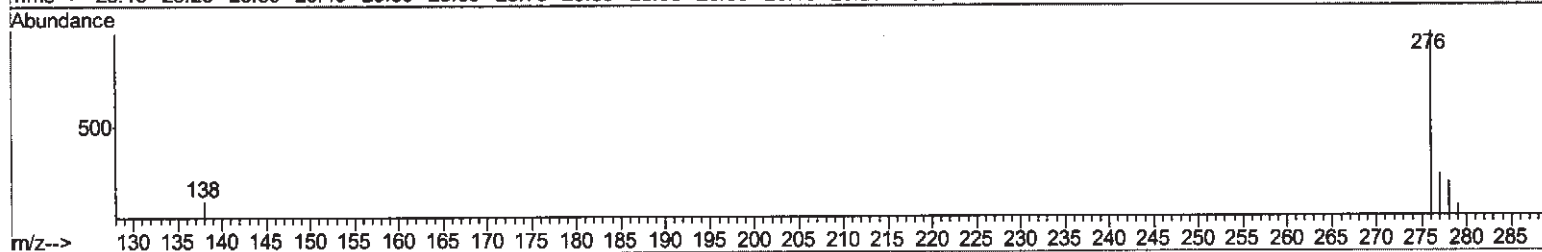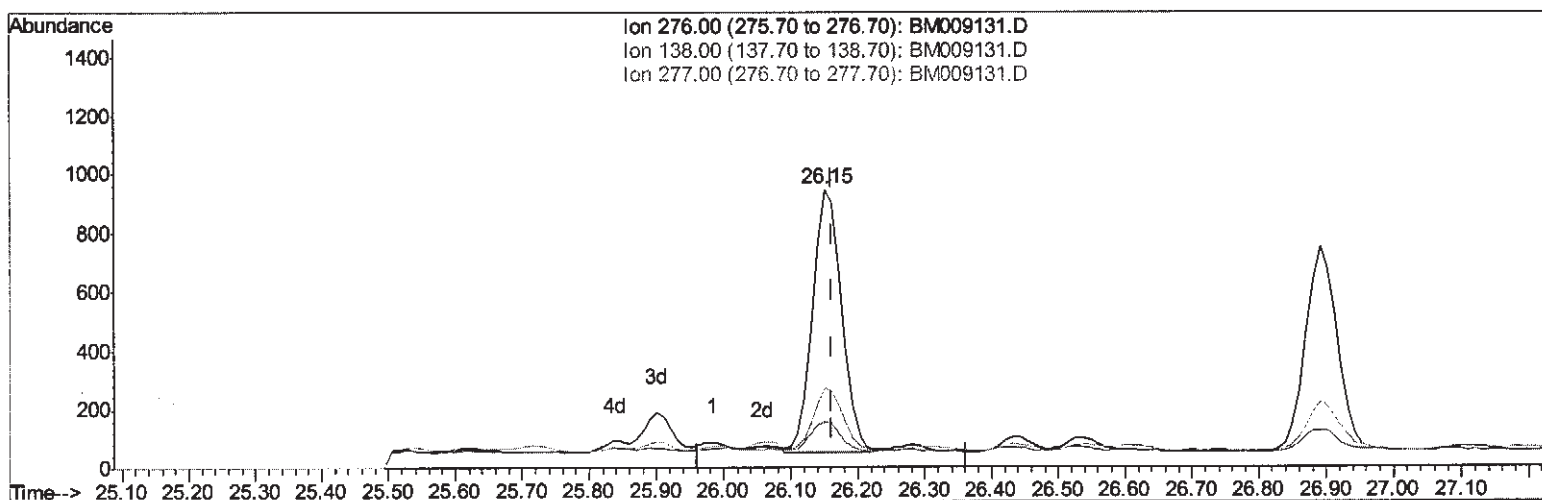

TIC: BM009131.D

(24) Indeno(1,2,3-cd)pyrene

26.151min (-0.011) 0.46ng/ui m

SJ 3/16/17

response 2723

Ion	Exp%	Act%
276.00	100	100
138.00	23.90	0.00#
277.00	24.50	0.00#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM030817\
Data File : BM009131.D
Acq On : 09 Mar 2017 06:22
Operator : SJ/MA
Sample : I2069-06
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AG7

Manual Integrations
APPROVED

mohammad
3/9/2017 2:02:46 PM

Quant Time: Mar 09 07:05:03 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 09 02:44:03 2017
Response via : Initial Calibration

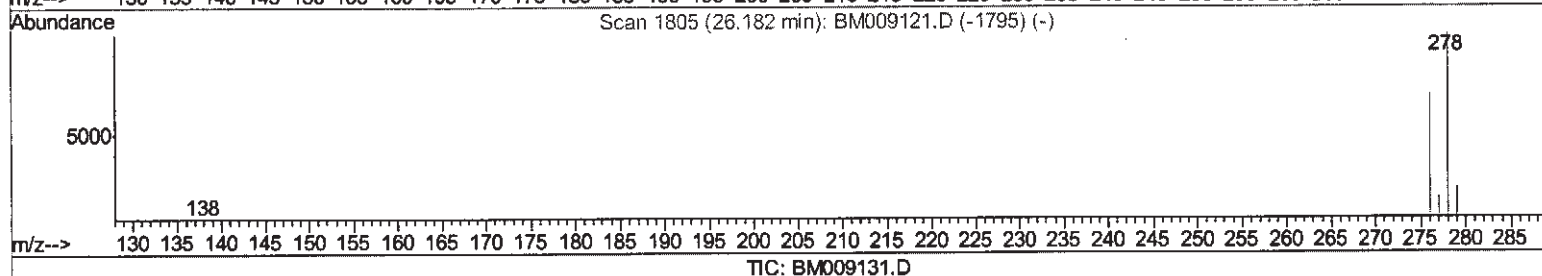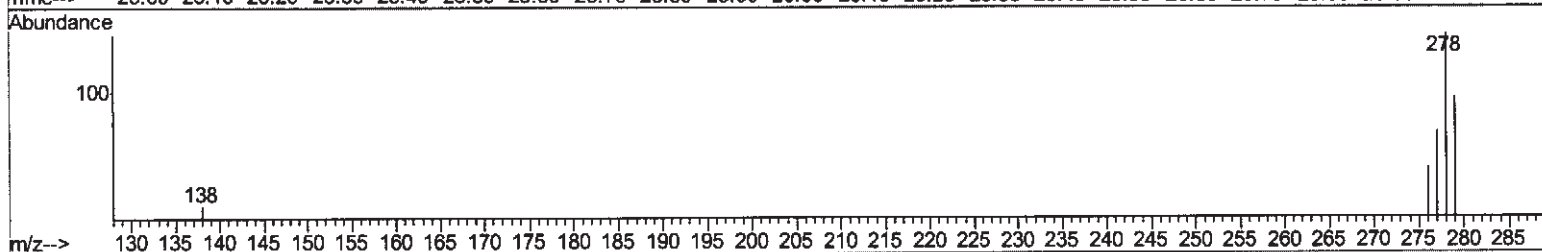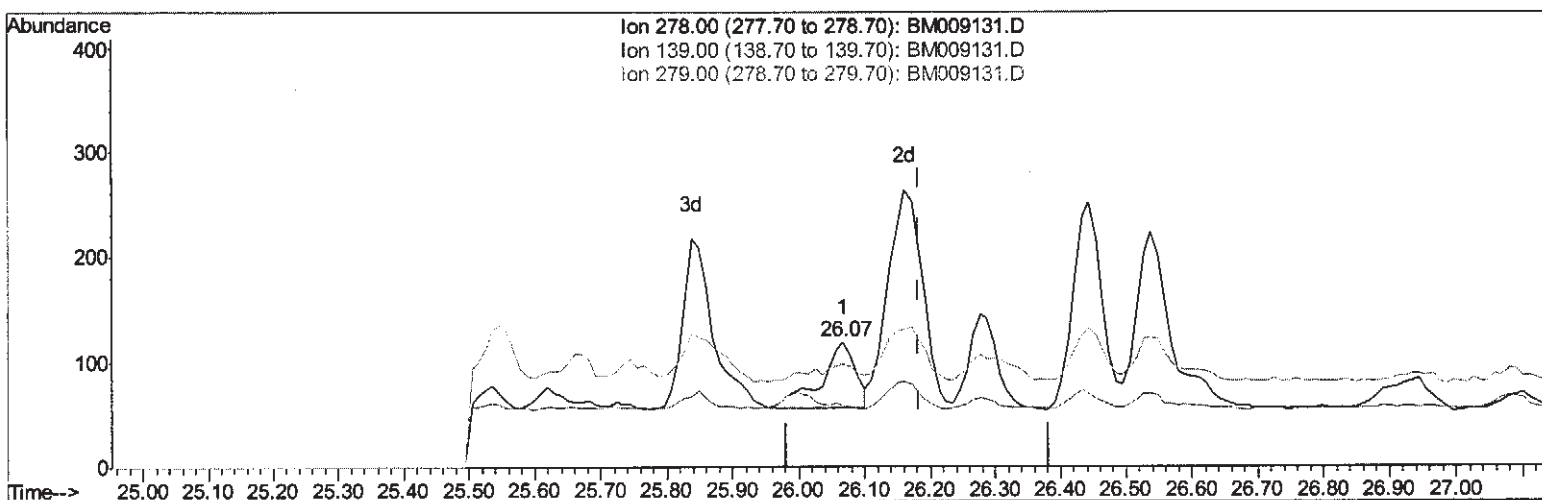

(25) Dibenzo(a,h)anthracene

26.068min (-0.115) 0.05ng/ul

response 224

Ion	Exp%	Act%
278.00	100	100
139.00	21.70	49.58#
279.00	32.40	82.35#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM030817\
Data File : BM009131.D
Acq On : 09 Mar 2017 06:22
Operator : SJ/MA
Sample : I2069-06
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AG7

Manual Integrations
APPROVED

mohammad
3/9/2017 2:02:46 PM

Quant Time: Mar 09 07:05:03 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 09 02:44:03 2017
Response via : Initial Calibration

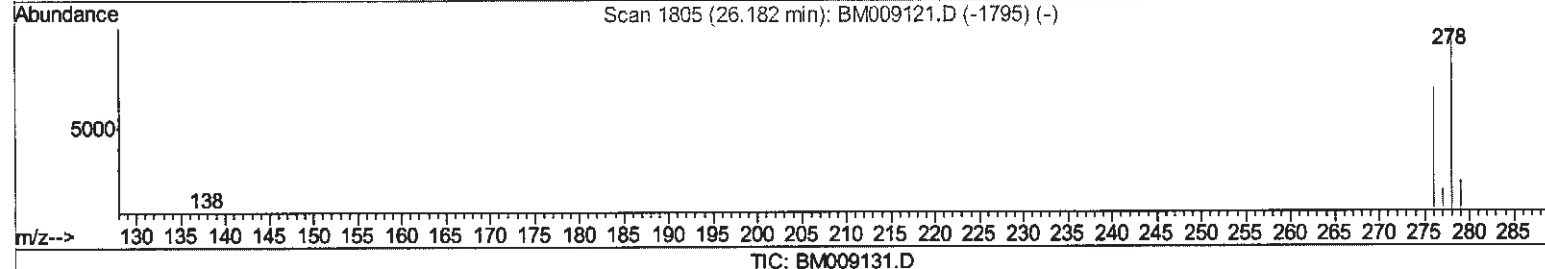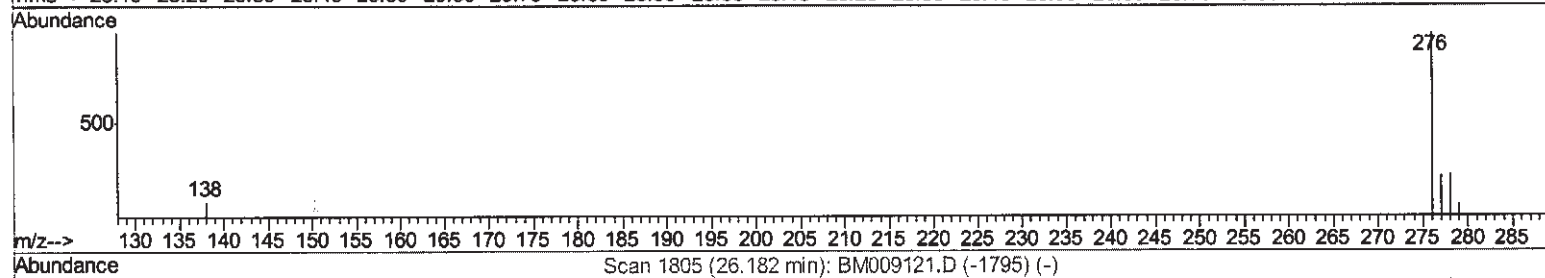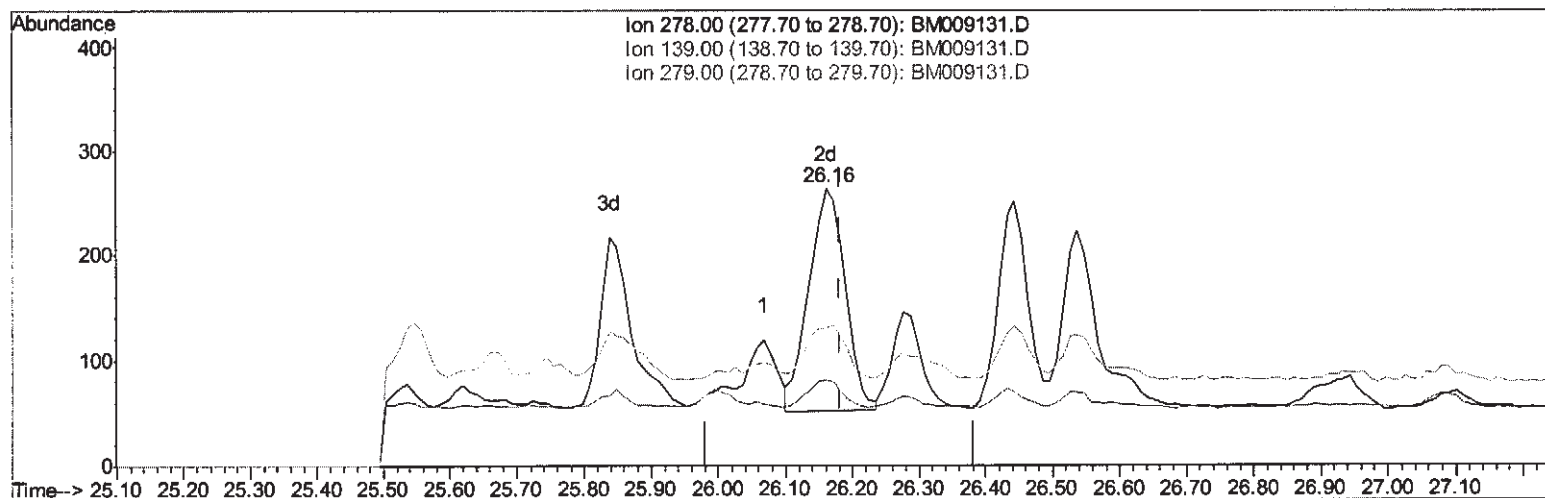

(25) Dibenzo(a,h)anthracene

26.162min (-0.021) 0.16ng/ul m

SJ 3/16/17

response 797

Ion	Exp%	Act%
278.00	100	100
139.00	21.70	30.68#
279.00	32.40	49.62#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM030817\
Data File : BM009131.D
Acq On : 09 Mar 2017 06:22
Operator : SJ/MA
Sample : I2069-06
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AG7

Manual Integrations
APPROVED

mohammad
3/9/2017 2:02:46 PM

Quant Time: Mar 09 07:05:03 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 09 02:44:03 2017
Response via : Initial Calibration

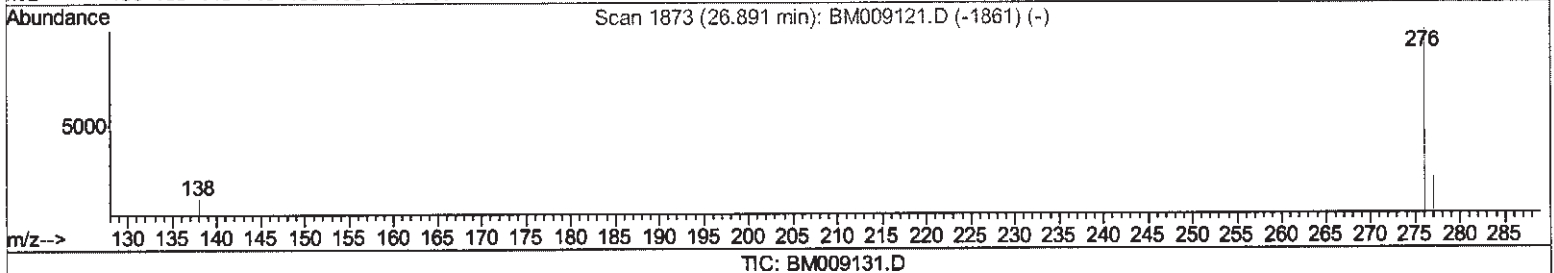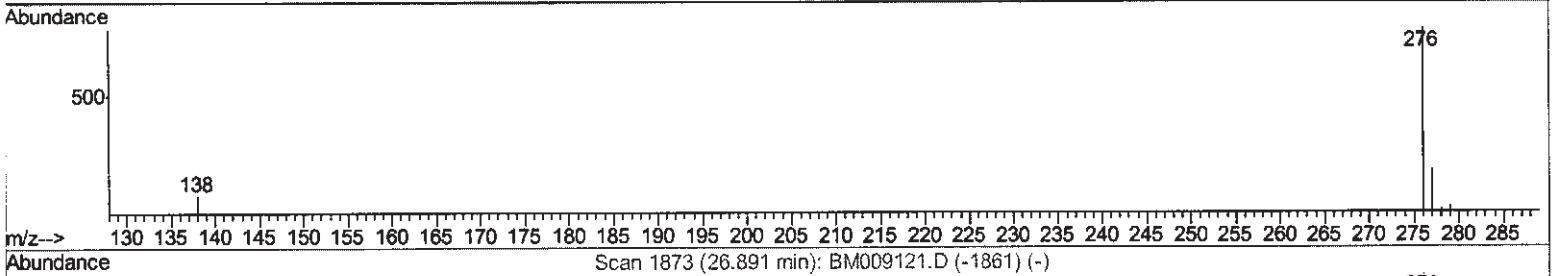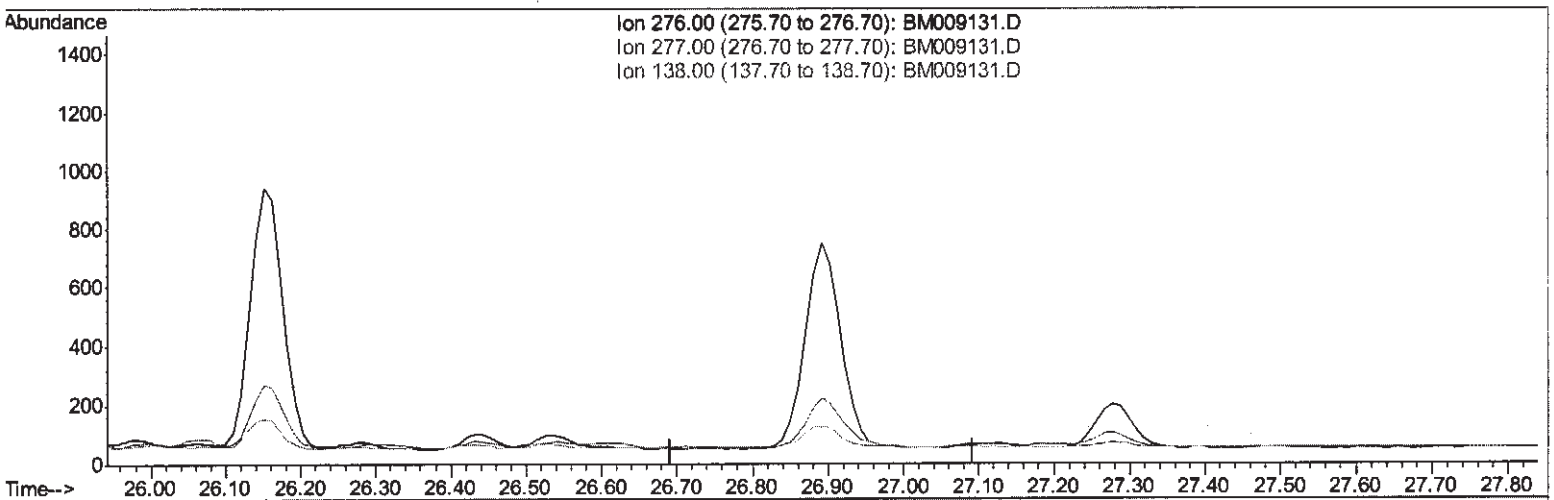

(26) Benzo(g,h,i)perylene

26.891min (-26.891) 0.00ng/ui

response 0

Ion	Exp%	Act%
276.00	100	0.00
277.00	27.30	0.00#
138.00	25.60	0.00#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM030817\
Data File : BM009131.D
Acq On : 09 Mar 2017 06:22
Operator : SJ/MA
Sample : I2069-06
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AG7

Manual Integrations
APPROVED

mohammad
3/9/2017 2:02:46 PM

Quant Time: Mar 09 07:05:03 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 09 02:44:03 2017
Response via : Initial Calibration

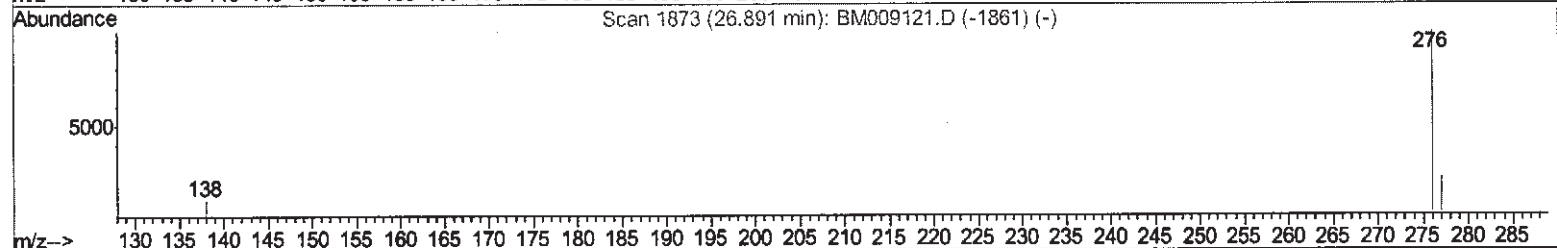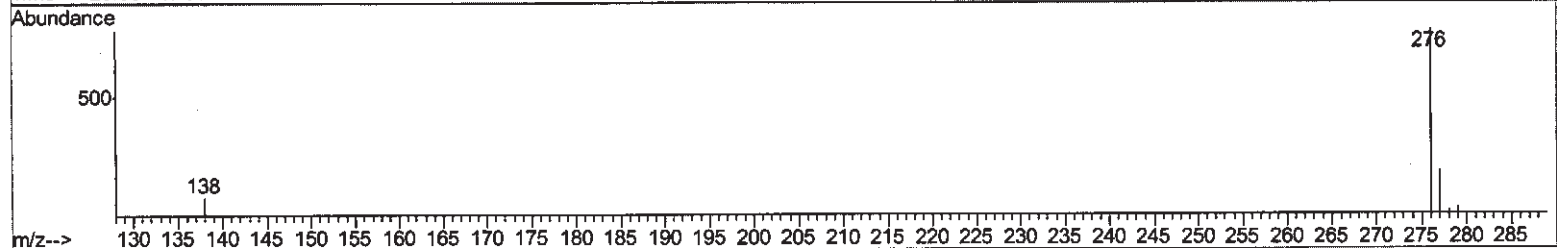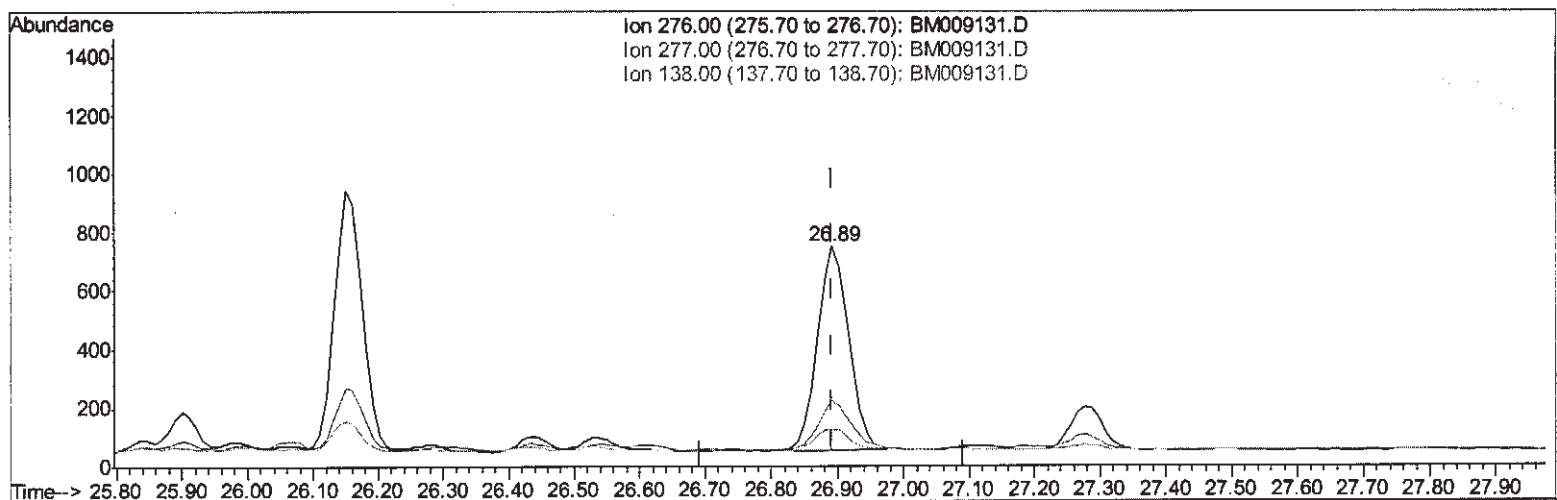

(26) Benzo(g,h,i)perylene

26.891min (-0.000) 0.46ng/ul m

SJ 3/16/17

response 2299

Ion	Exp%	Act%
276.00	100	100
277.00	27.30	29.52
138.00	25.60	16.49#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM030817\
 Data File : BM009131.D
 Acq On : 09 Mar 2017 06:22
 Operator : SJ/MA
 Sample : I2069-06
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AG7

Manual Integrations
 APPROVED

mohammad
 3/9/2017 2:02:46 PM

Quant Time: Mar 09 07:06:52 2017
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030317.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 09 02:44:03 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.88	152	294	0.40	ng/ul	0.00
2) Naphthalene-d8	10.68	136	929	0.40	ng/ul	-0.01
6) Acenaphthene-d10	14.52	164	566	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.26	188	1269m	0.40	ng/ul	0.00
16) Chrysene-d12	21.44	240	1390	0.40	ng/ul	-0.01
20) Perylene-d12	23.78	264	1309m	0.40	ng/ul	0.00

SJ 3/16/17

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	12.27	152	379	0.25	ng/ul	0.00
14) Fluoranthene-d10	19.30	212	1045	0.26	ng/ul	0.00

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
3) Naphthalene	10.73	128	323	0.12	ng/ul#	64
5) 2-Methylnaphthalene	12.34	142	174	0.09	ng/ul	100
8) Acenaphthene	14.59	153	427	0.19	ng/ul	93
9) Fluorene	15.58	166	681m	0.26	ng/ul	
12) Phenanthrene	17.31	178	9289m	2.33	ng/ul	
13) Anthracene	17.40	178	2615	0.66	ng/ul	98
15) Fluoranthene	19.33	202	12664	2.44	ng/ul	93
17) Pyrene	19.69	202	10768	2.25	ng/ul	97
18) Benzo(a)anthracene	21.42	228	5900	1.28	ng/ul	95
19) Chrysene	21.48	228	4519	1.03	ng/ul	96
21) Benzo(b)fluoranthene	23.07	252	6373m	1.24	ng/ul	
22) Benzo(k)fluoranthene	23.11	252	2206m	0.49	ng/ul	
23) Benzo(a)pyrene	23.67	252	4632m	1.00	ng/ul	
24) Indeno(1,2,3-cd)pyrene	26.15	276	2723m	0.46	ng/ul	
25) Dibenzo(a,h)anthracene	26.16	278	797m	0.16	ng/ul	
26) Benzo(g,h,i)perylene	26.89	276	2299m	0.46	ng/ul	

SJ 3/16/17

SJ 3/16/17

(#) = qualifier out of range (m) = manual integration (+) = signals summed