
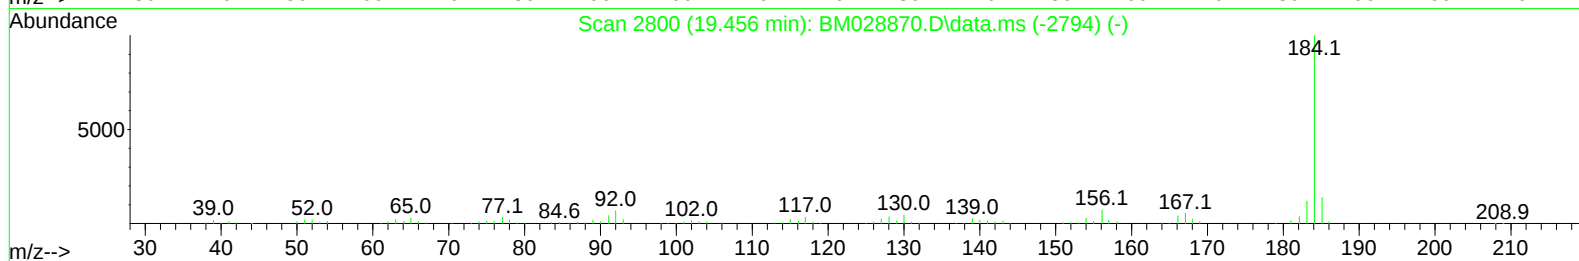
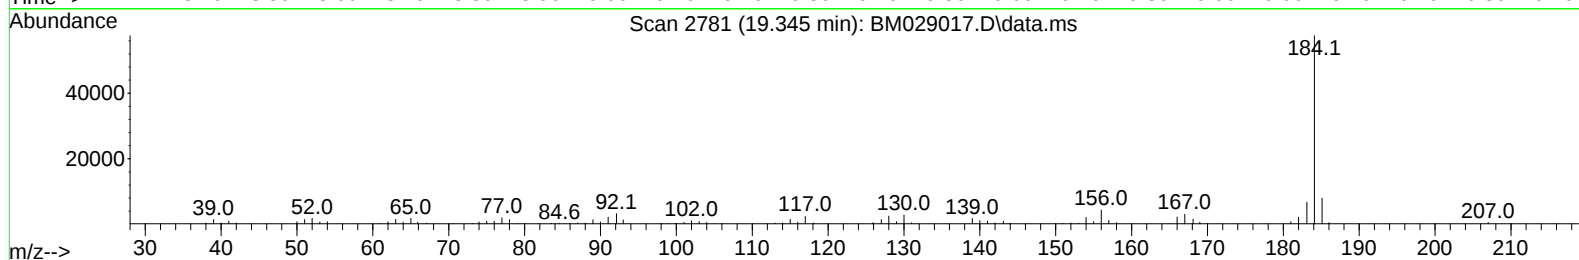


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030821\
Data File : BM029017.D
Acq On : 08 Mar 2021 14:00
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 08 14:37:18 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM022321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 05 13:17:12 2021
Response via : Initial Calibration

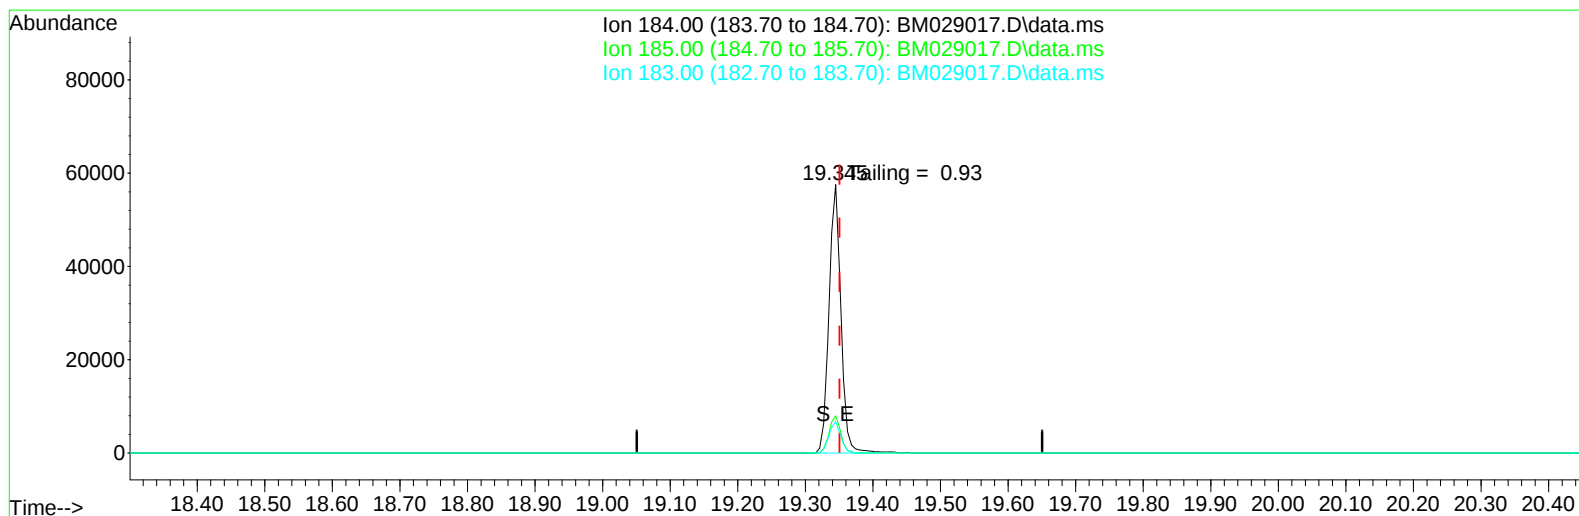

TIC: BM029017.D\data.ms

(77) Benzidine




19.345min (-0.006) 0.00 ng

response 70801

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.80	13.85
183.00	12.10	11.70
0.00	0.00	0.00

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030821\  
Data File : BM029017.D  
Acq On    : 08 Mar 2021  14:00  
Operator  : CG/JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Quant Time: Mar 08 14:37:18 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM022321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 05 13:17:12 2021
Response via : Initial Calibration

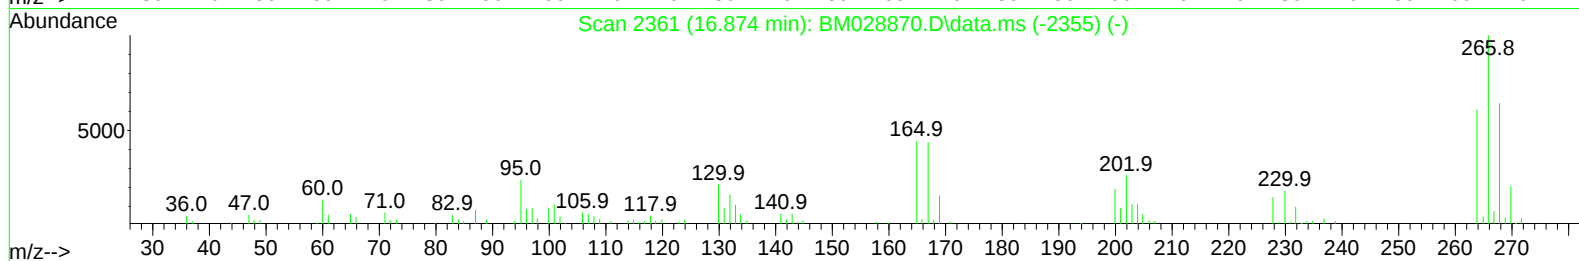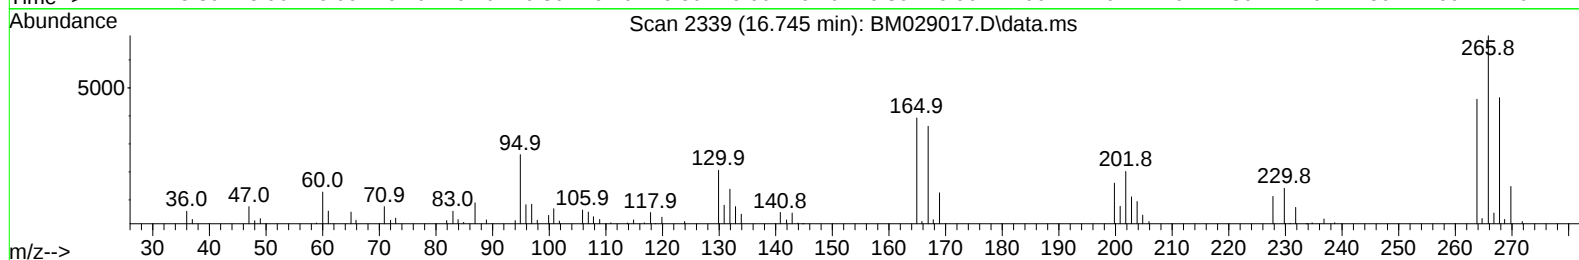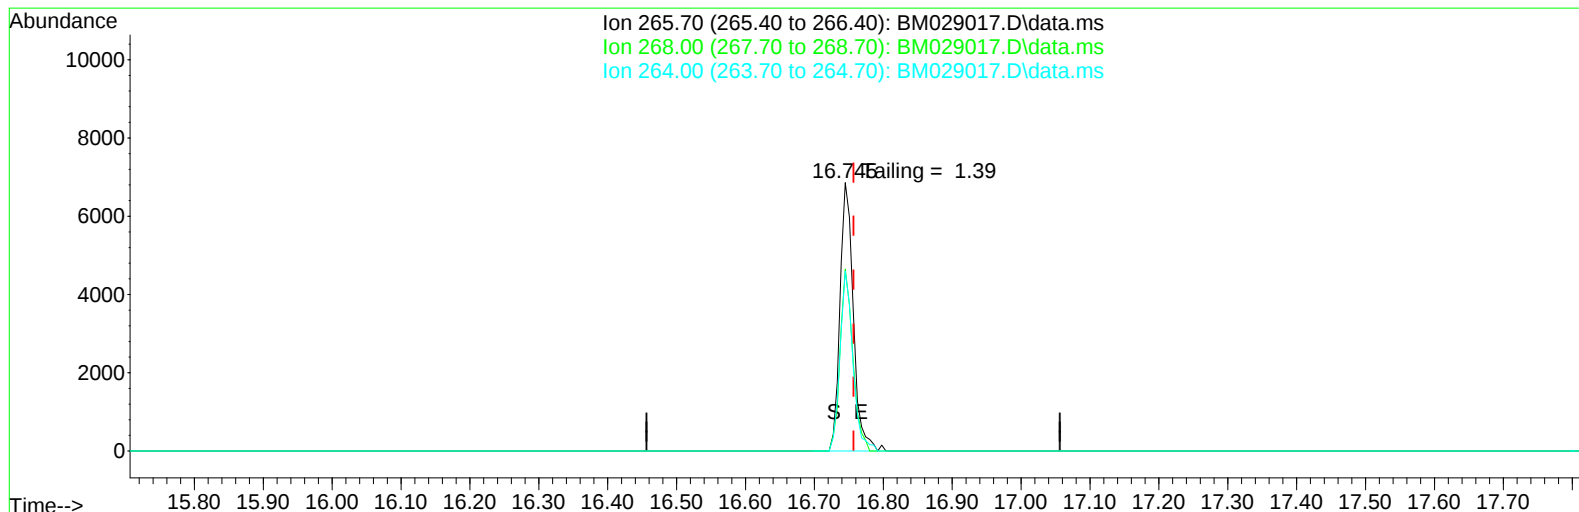

TIC: BM029017.D\data.ms

(70) **Pentachlorophenol (C)**

16.745min (-0.012) 0.00 ng

response	9255
----------	------

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.40	72.22
264.00	63.30	71.88
0.00	0.00	0.00