

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030821\
 Data File : BM029013.D
 Acq On : 08 Mar 2021 09:55
 Operator : CG/JU
 Sample : PB135023BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB135023BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM022321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM029013.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.246	379	384	396	rBV	255931	349356	63.46%	12.531%
2	6.875	655	661	672	rBV	231690	348596	63.32%	12.504%
3	7.669	791	796	803	rBB	44105	65971	11.98%	2.366%
4	8.845	990	996	1007	rBB	139405	220756	40.10%	7.918%
5	10.463	1265	1271	1280	rBB	56435	89354	16.23%	3.205%
6	12.957	1688	1695	1714	rBB	305143	426702	77.51%	15.306%
7	14.339	1925	1930	1938	rBB	74109	103775	18.85%	3.722%
8	15.839	2180	2185	2194	rBB	226994	304217	55.26%	10.912%
9	17.086	2392	2397	2404	rBB	84345	112488	20.43%	4.035%
10	19.715	2838	2844	2849	rBV	474648	550525	100.00%	19.747%
11	21.262	3102	3107	3111	rBV	94299	113631	20.64%	4.076%
12	23.421	3468	3474	3482	rVB2	58090	102508	18.62%	3.677%




Sum of corrected areas: 2787879

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030821\
Data File : BM029013.D
Acq On : 08 Mar 2021 09:55
Operator : CG/JU
Sample : PB135023BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB135023BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM022321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

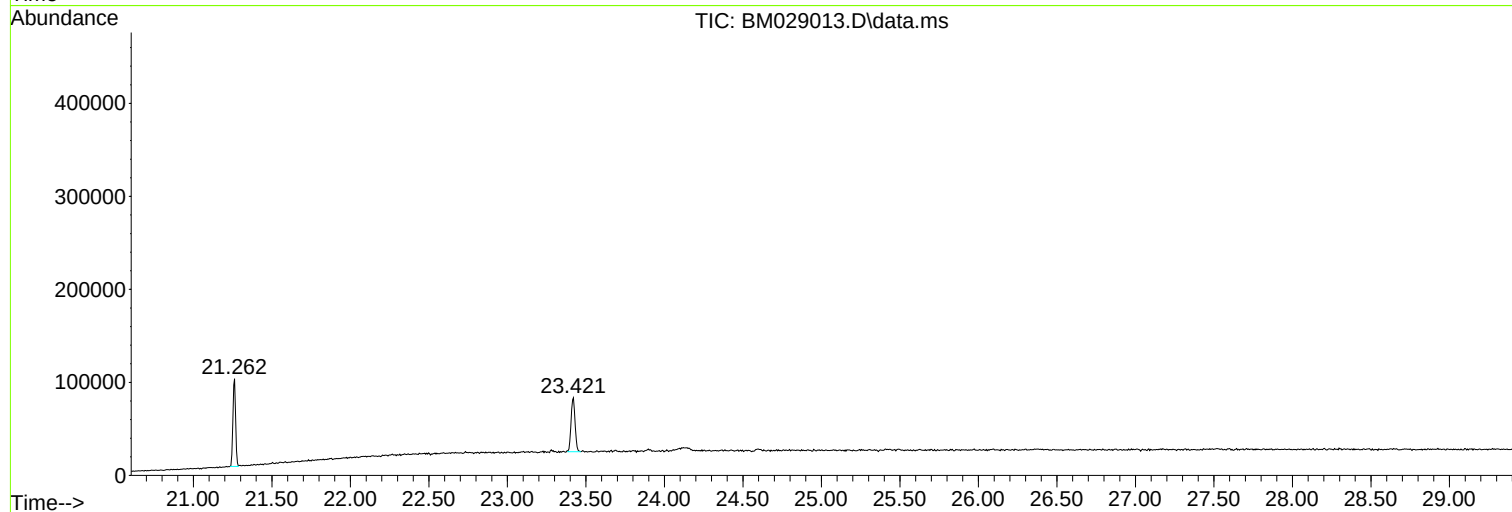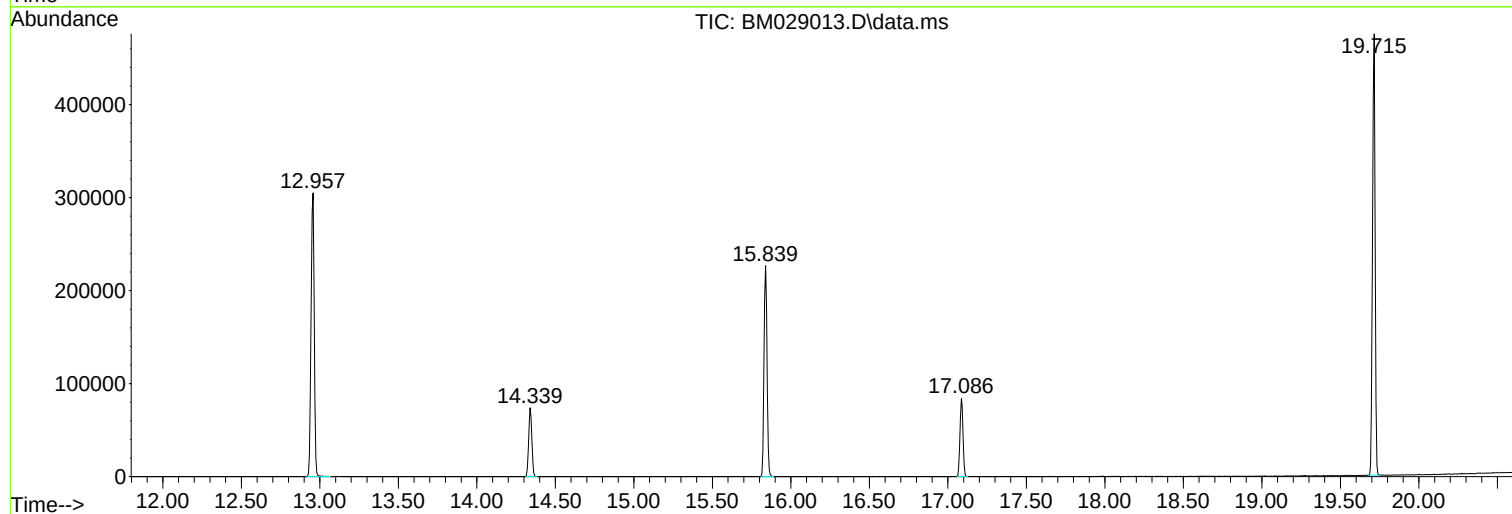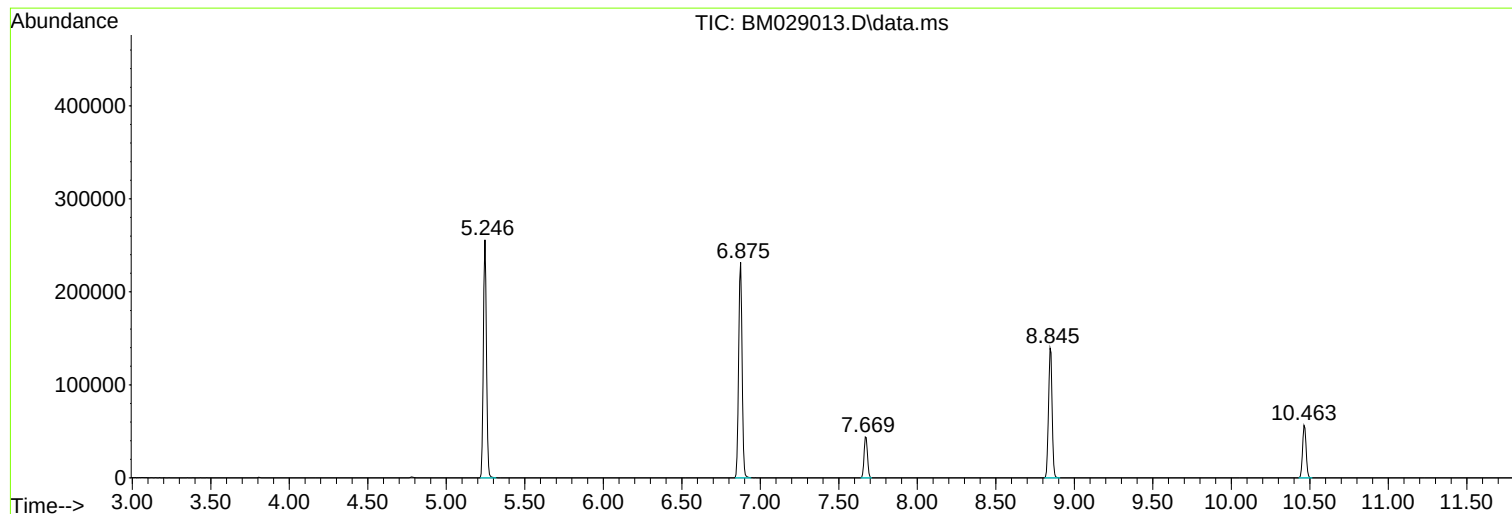

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030821\
Data File : BM029013.D
Acq On : 08 Mar 2021 09:55
Operator : CG/JU
Sample : PB135023BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB135023BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM022321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030821\
Data File : BM029013.D
Acq On : 08 Mar 2021 09:55
Operator : CG/JU
Sample : PB135023BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB135023BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM022321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------