

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030821\
 Data File : BM029019.D
 Acq On : 08 Mar 2021 15:13
 Operator : CG/JU
 Sample : PB135035BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB135035BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM022321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM029019.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.246	379	384	397	rBB	226793	308789	62.92%	13.029%
2	6.869	654	660	673	rBV	199427	302354	61.61%	12.757%
3	7.669	791	796	803	rBB	35068	51665	10.53%	2.180%
4	8.845	990	996	1006	rBV	125039	192388	39.20%	8.117%
5	10.463	1265	1271	1280	rBB	41826	64986	13.24%	2.742%
6	12.951	1688	1694	1703	rBV	263971	365367	74.45%	15.416%
7	14.339	1925	1930	1936	rBB	51908	71773	14.63%	3.028%
8	15.839	2180	2185	2195	rBB	192053	254483	51.86%	10.737%
9	17.086	2392	2397	2403	rBV	59314	77623	15.82%	3.275%
10	19.709	2838	2843	2849	rBV	410809	490737	100.00%	20.706%
11	21.256	3102	3106	3113	rVB2	74651	88625	18.06%	3.739%
12	23.415	3467	3473	3479	rBV	58987	101260	20.63%	4.272%




Sum of corrected areas: 2370050

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030821\
Data File : BM029019.D
Acq On : 08 Mar 2021 15:13
Operator : CG/JU
Sample : PB135035BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB135035BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM022321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

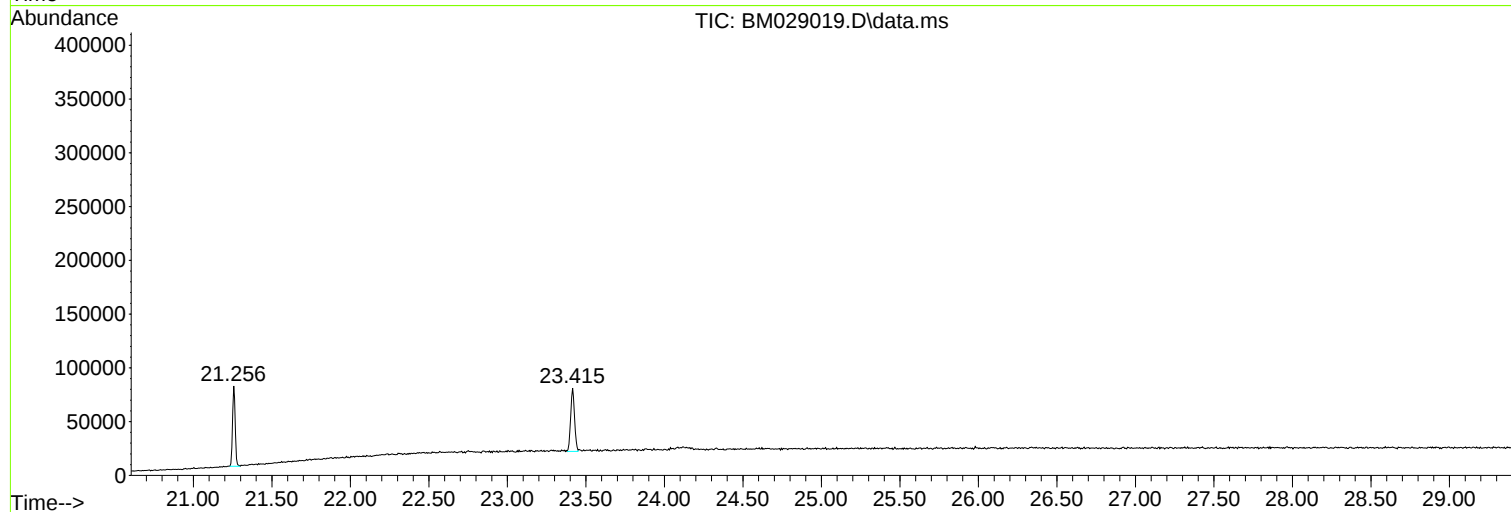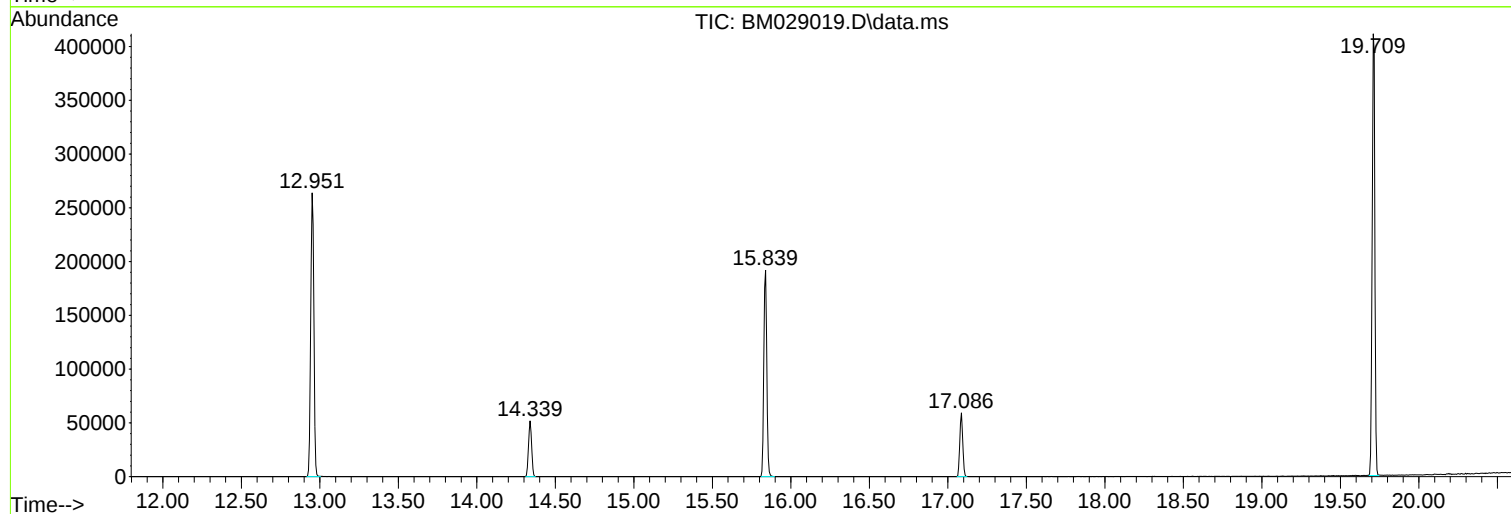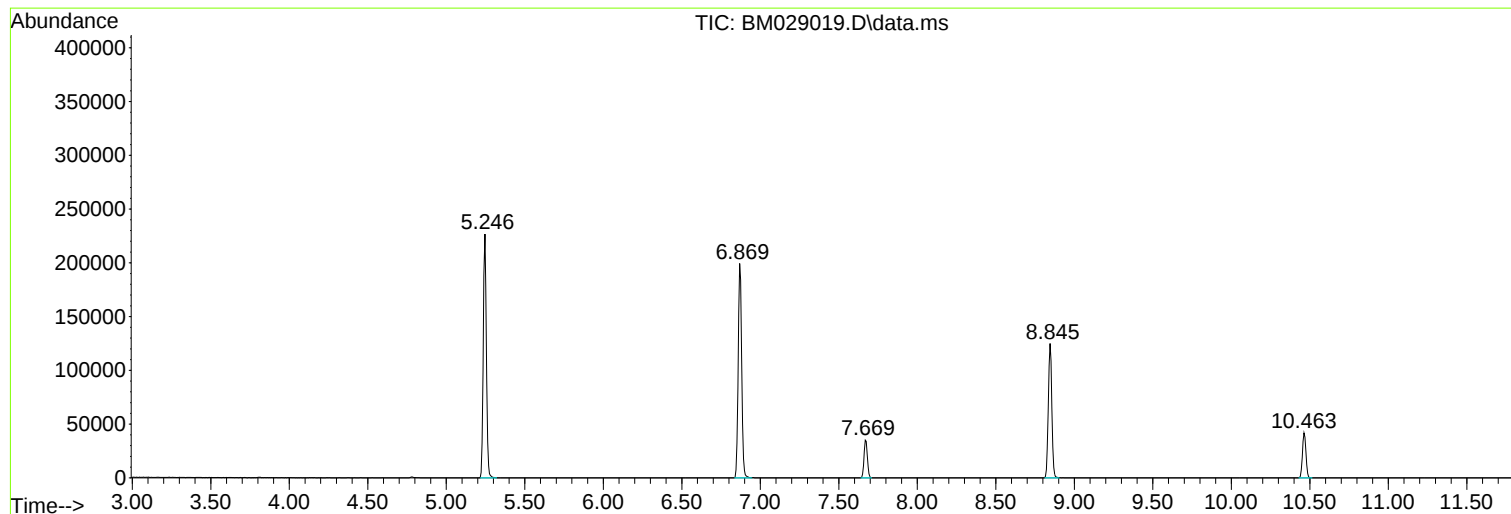

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030821\
Data File : BM029019.D
Acq On : 08 Mar 2021 15:13
Operator : CG/JU
Sample : PB135035BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB135035BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM022321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030821\
Data File : BM029019.D
Acq On : 08 Mar 2021 15:13
Operator : CG/JU
Sample : PB135035BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB135035BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM022321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------