

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030821\
 Data File : BM029023.D
 Acq On : 08 Mar 2021 17:42
 Operator : CG/JU
 Sample : M1576-12
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 IDW-GW807B-SO-030421

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM022321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM029023.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.099	15	19	27	rVB	34915	38989	6.58%	1.401%
2	4.269	213	218	225	rVV	33491	39671	6.70%	1.426%
3	4.728	289	296	301	rBV	17337	22772	3.84%	0.819%
4	4.775	301	304	312	rVB	5198	6483	1.09%	0.233%
5	5.246	379	384	393	rBV	182655	251967	42.54%	9.057%
6	6.869	654	660	670	rVB	147605	224878	37.97%	8.083%
7	7.669	791	796	803	rBV	39402	55911	9.44%	2.010%
8	8.845	989	996	1004	rBV	110538	172932	29.20%	6.216%
9	10.463	1265	1271	1277	rBV	47035	73024	12.33%	2.625%
10	12.951	1688	1694	1702	rBV	253336	345173	58.28%	12.407%
11	14.227	1901	1911	1917	rBV3	2694	6402	1.08%	0.230%
12	14.339	1925	1930	1935	rVB	61113	83358	14.07%	2.996%
13	15.839	2179	2185	2191	rVB	217733	296486	50.06%	10.657%
14	17.086	2391	2397	2402	rBV	71816	93232	15.74%	3.351%
15	17.986	2543	2550	2562	rBV	47269	65817	11.11%	2.366%
16	18.462	2624	2631	2637	rBV2	3803	6782	1.15%	0.244%
17	18.721	2670	2675	2680	rVB	24772	28921	4.88%	1.040%
18	18.809	2686	2690	2695	rBV	5402	7225	1.22%	0.260%
19	19.262	2760	2767	2775	rBV	28222	39704	6.70%	1.427%
20	19.362	2780	2784	2791	rVB	4612	6586	1.11%	0.237%
21	19.709	2838	2843	2848	rBV	479639	592307	100.00%	21.290%
22	20.974	3053	3058	3065	rBV	53010	68144	11.50%	2.449%
23	21.256	3102	3106	3112	rBV	93979	114707	19.37%	4.123%
24	23.415	3468	3473	3484	rVB2	67586	120617	20.36%	4.336%
25	23.985	3567	3570	3576	rVB8	10095	19969	3.37%	0.718%




Sum of corrected areas: 2782057

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030821\
Data File : BM029023.D
Acq On : 08 Mar 2021 17:42
Operator : CG/JU
Sample : M1576-12
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
IDW-GW807B-SO-030421

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM022321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

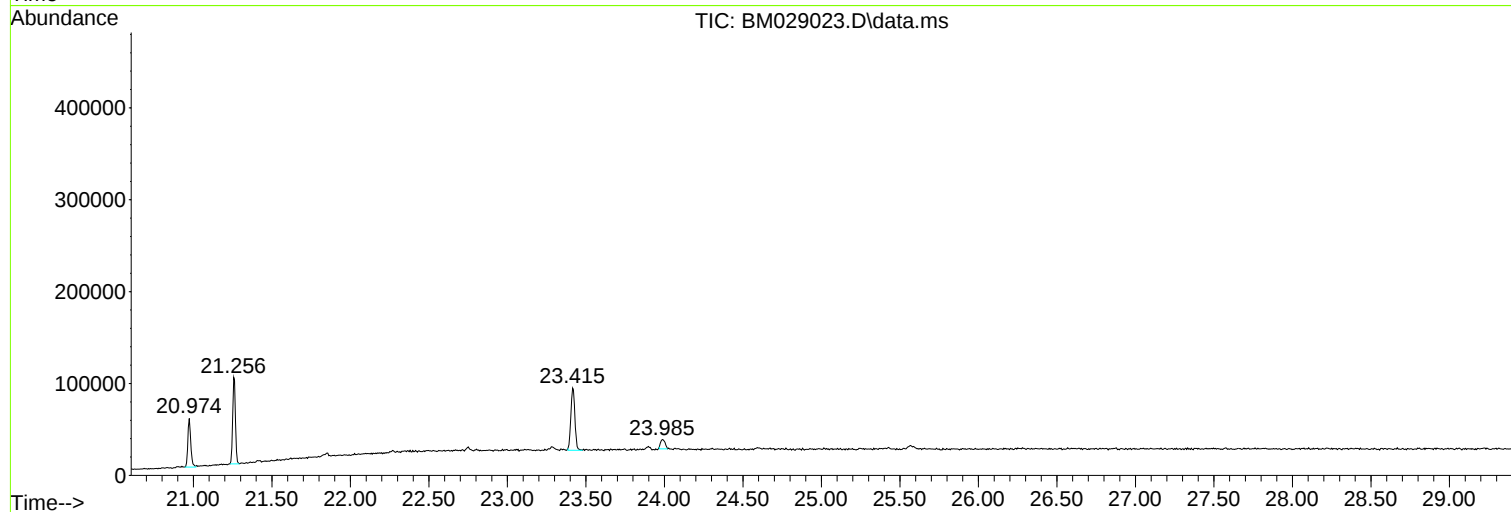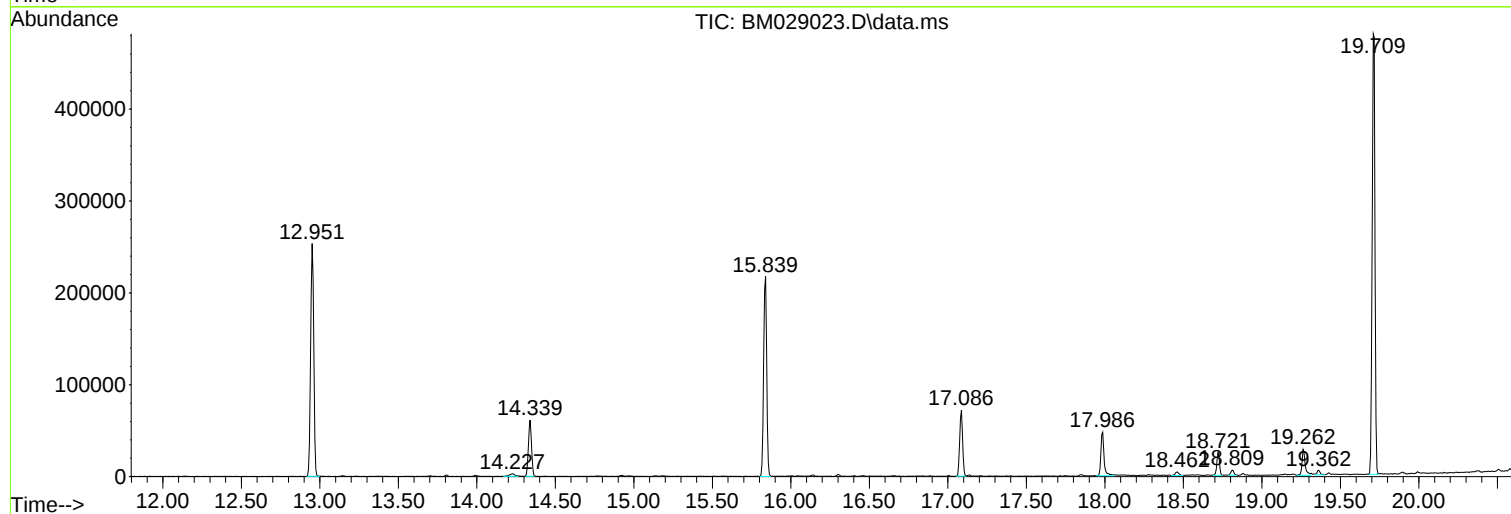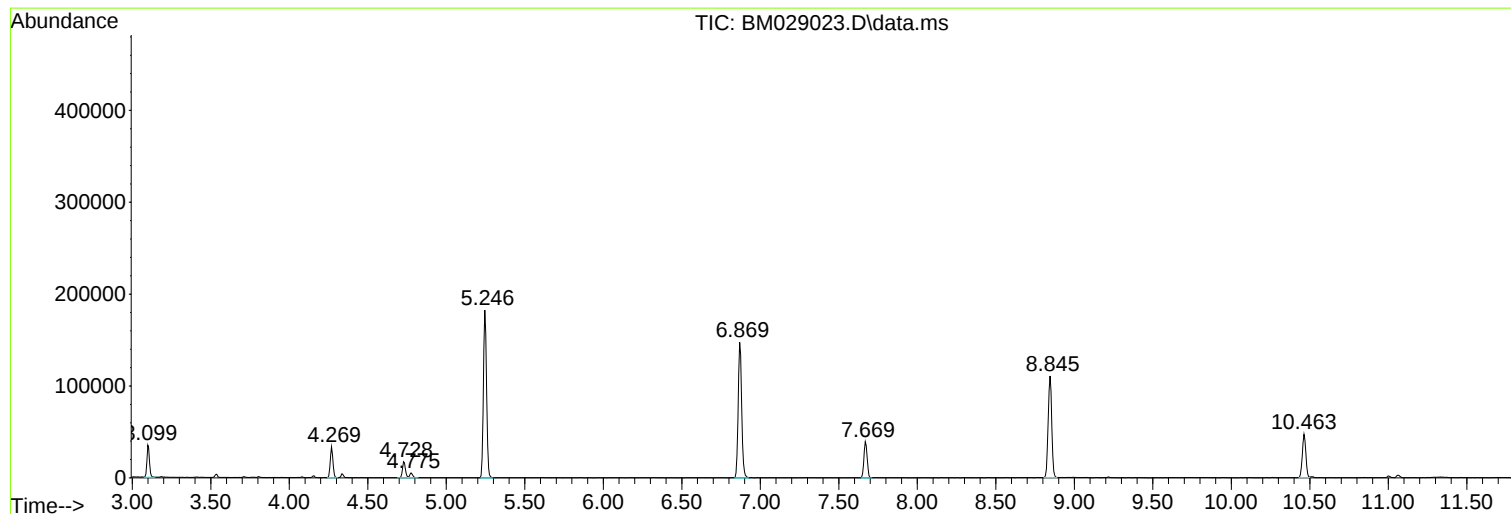

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030821\
Data File : BM029023.D
Acq On : 08 Mar 2021 17:42
Operator : CG/JU
Sample : M1576-12
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
IDW-GW807B-SO-030421

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM022321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030821\
Data File : BM029023.D
Acq On : 08 Mar 2021 17:42
Operator : CG/JU
Sample : M1576-12
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
IDW-GW807B-SO-030421

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM022321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
