
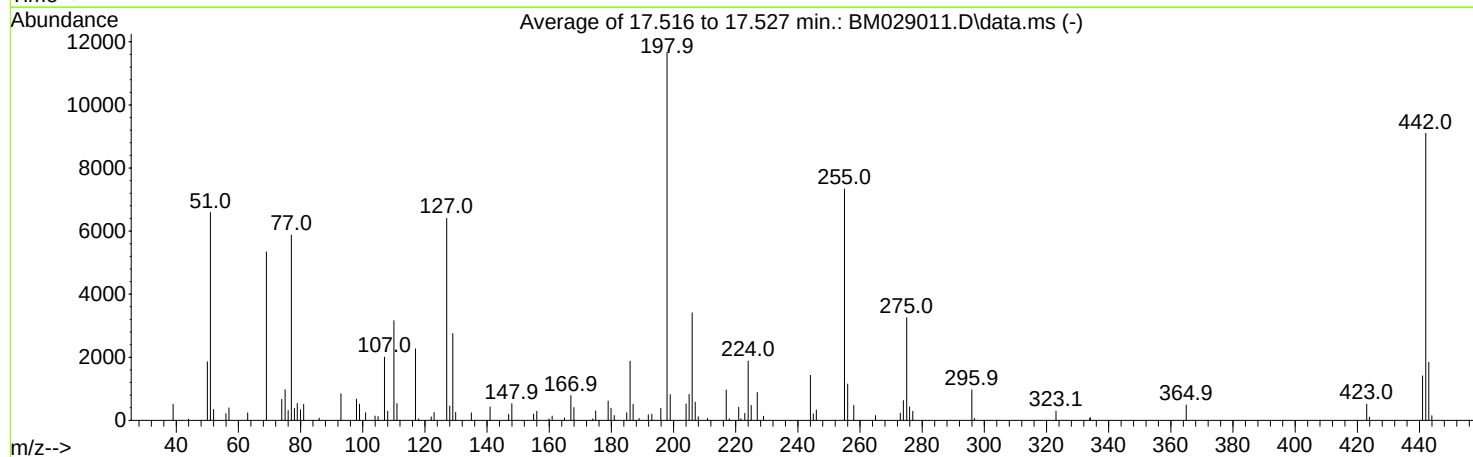


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030821\
 Data File : BM029011.D
 Acq On : 08 Mar 2021 08:41
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM022321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Mar 05 13:17:12 2021

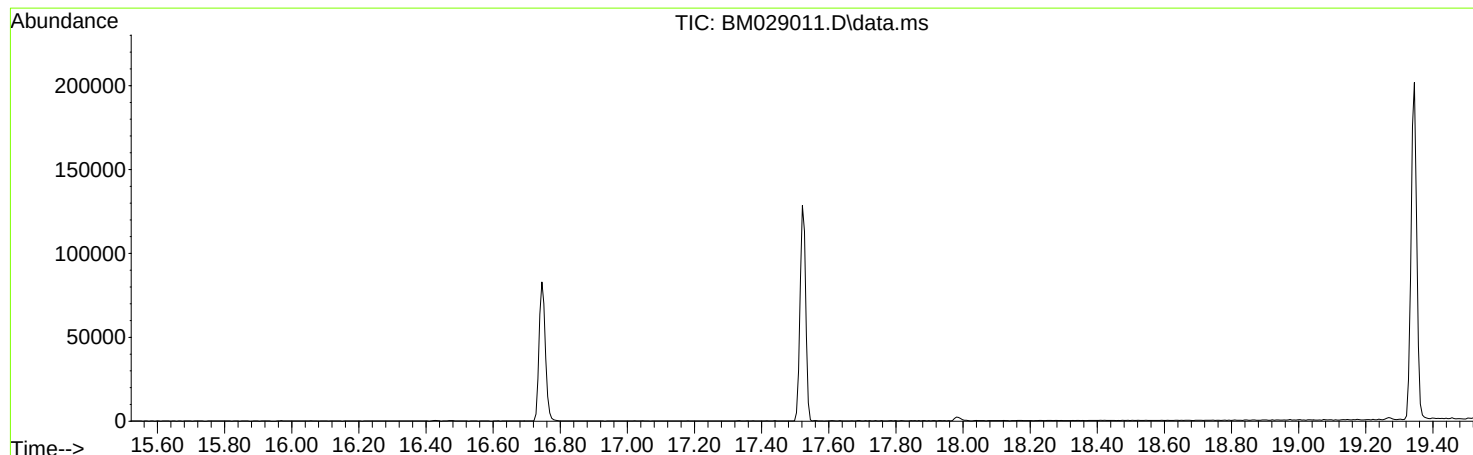

AutoFind: Scans 2470, 2471, 2472; Background Corrected with Scan 2465

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	56.5	6591	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	45.8	5341	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	54.9	6403	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	11662	PASS
199	198	5	9	7.0	818	PASS
275	198	10	60	27.9	3259	PASS
365	198	1	100	4.2	487	PASS
441	198	0.01	100	12.1	1411	PASS
442	442	50	100	100.0	9100	PASS
443	442	15	24	20.2	1842	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
3/8/2021	BNA_M	<u>BM029011.D</u>
Compound Name	Response	Retention Time
DDT	45812	20.56
DDD	119	20.12
DDE	0	19.95
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
119	45931	0.26

Instrument :
BNA_M
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030821\
Data File : BM029011.D
Acq On : 08 Mar 2021 08:41
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Mar 08 09:58:17 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM022321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 05 13:17:12 2021
Response via : Initial Calibration

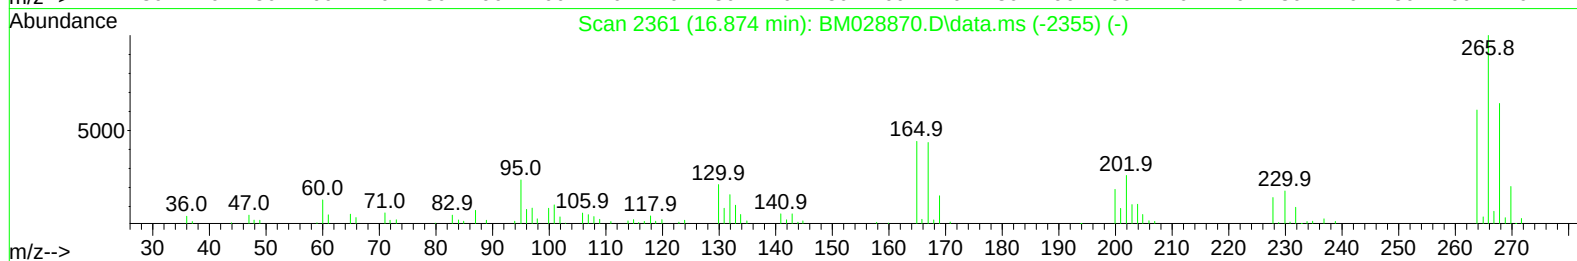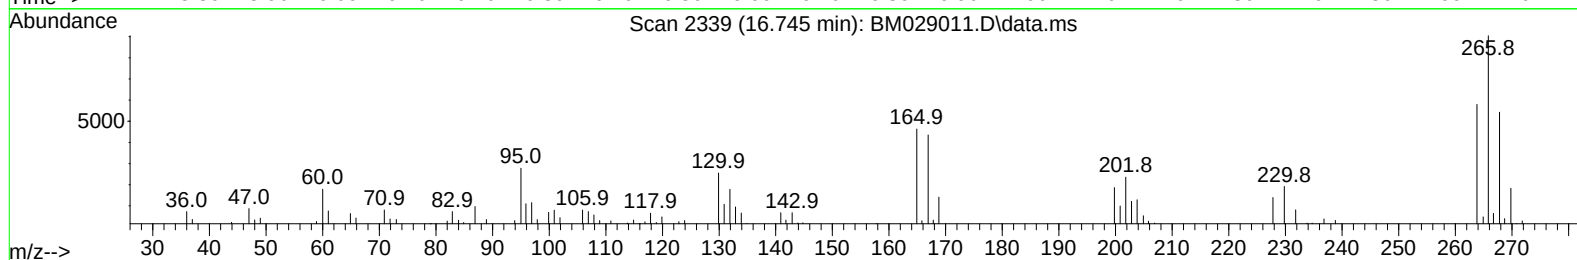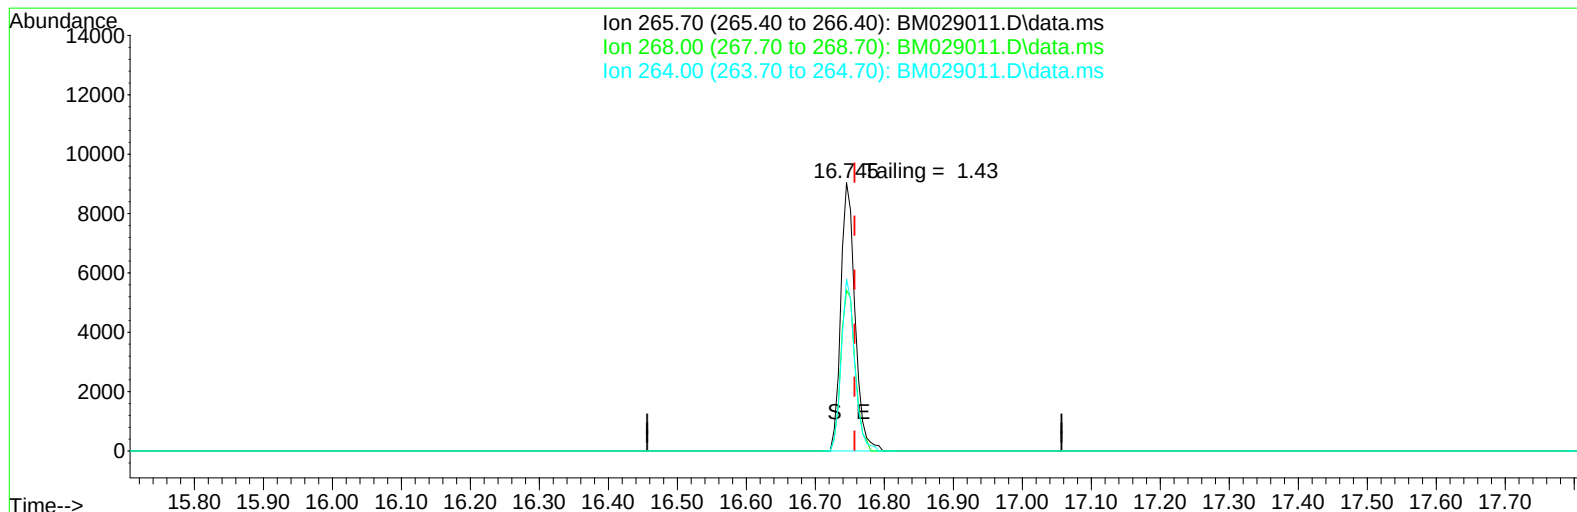

TIC: BM029011.D\data.ms

(70) Pentachlorophenol (C)

16.745min (-0.012) 0.00 ng




response 12916

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.40	64.40
264.00	63.30	64.13
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030821\
Data File : BM029011.D
Acq On : 08 Mar 2021 08:41
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Mar 08 09:58:17 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM022321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 05 13:17:12 2021
Response via : Initial Calibration

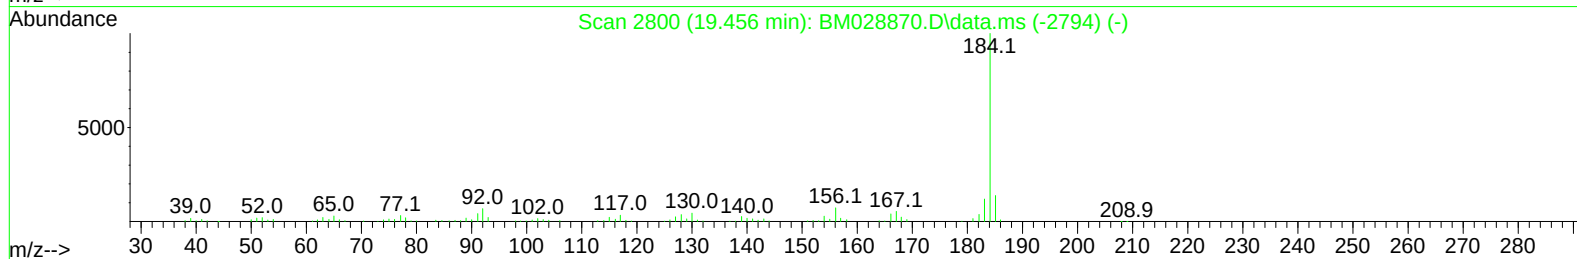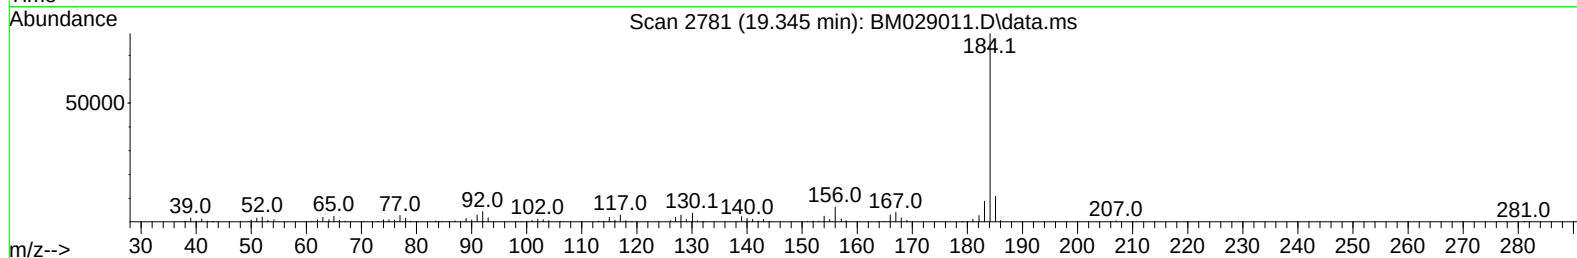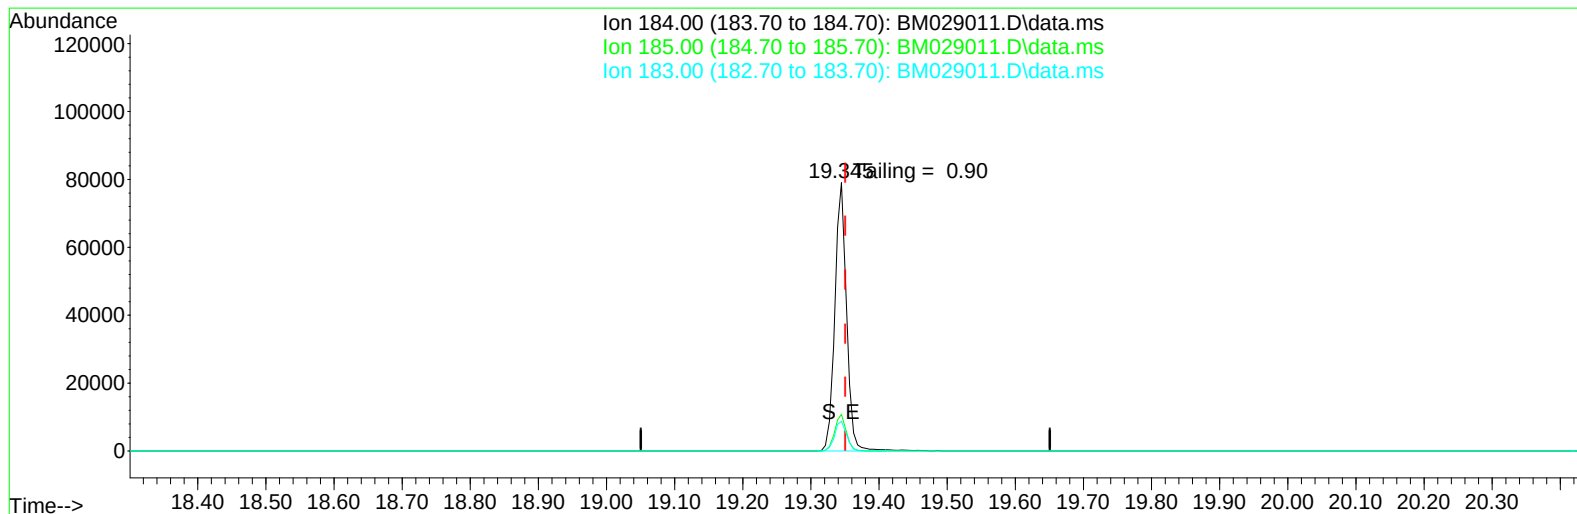

TIC: BM029011.D\data.ms

(77) Benzidine

19.345min (-0.006) 0.00 ng

response 94698

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.80	13.76
183.00	12.10	11.10
0.00	0.00	0.00