
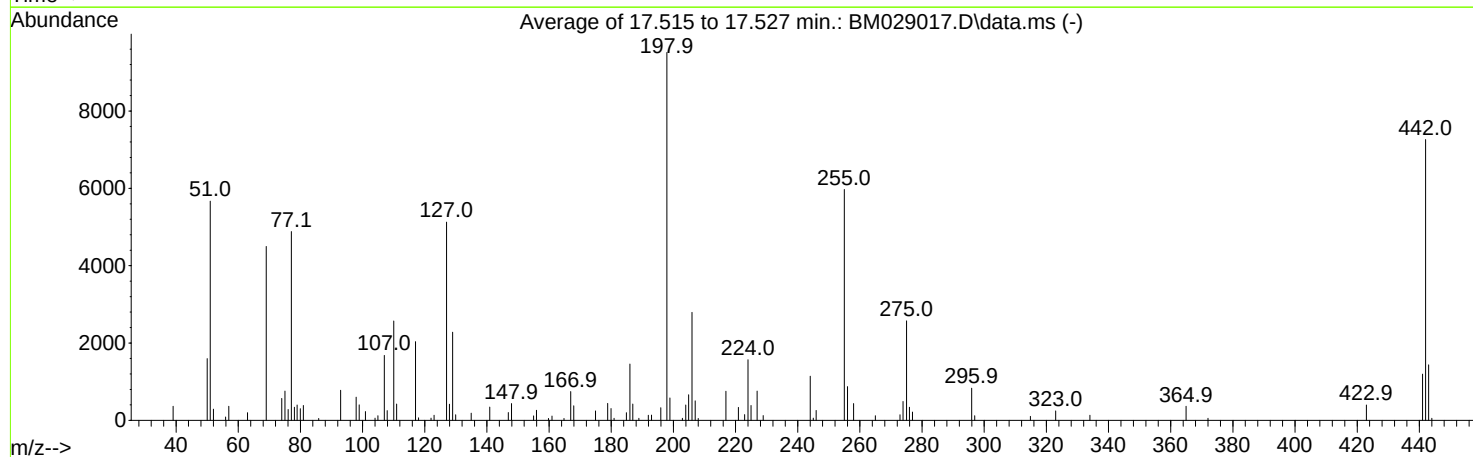


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030821\
 Data File : BM029017.D
 Acq On : 08 Mar 2021 14:00
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM022321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Mar 05 13:17:12 2021

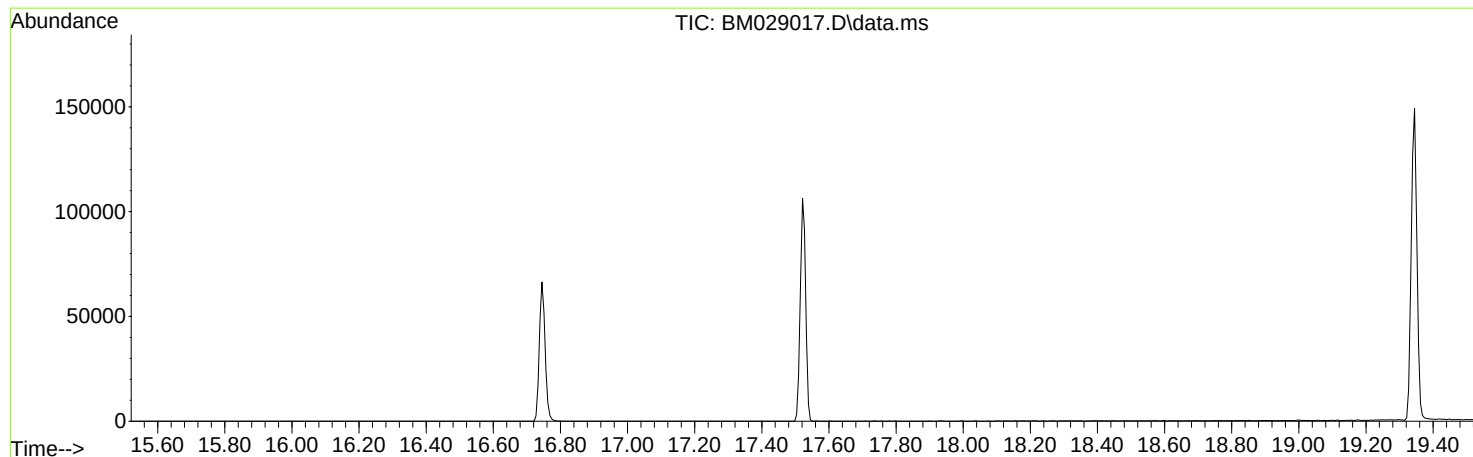

AutoFind: Scans 2470, 2471, 2472; Background Corrected with Scan 2465

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	59.6	5670	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	47.3	4497	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	53.9	5127	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	9512	PASS
199	198	5	9	6.1	580	PASS
275	198	10	60	27.1	2574	PASS
365	198	1	100	3.8	363	PASS
441	198	0.01	100	12.6	1197	PASS
442	442	50	100	100.0	7261	PASS
443	442	15	24	19.8	1437	PASS




DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/8/2021	BNA_M	<u>BM029017.D</u>
Compound Name	Response	Retention Time
DDT	36145	20.56
DDD	230	20.12
DDE	0	19.95
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
230	36375	0.63


```
Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030821\  
Data File : BM029017.D  
Acq On    : 08 Mar 2021  14:00  
Operator  : CG/JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Mar 08 14:37:18 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM022321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 05 13:17:12 2021
Response via : Initial Calibration

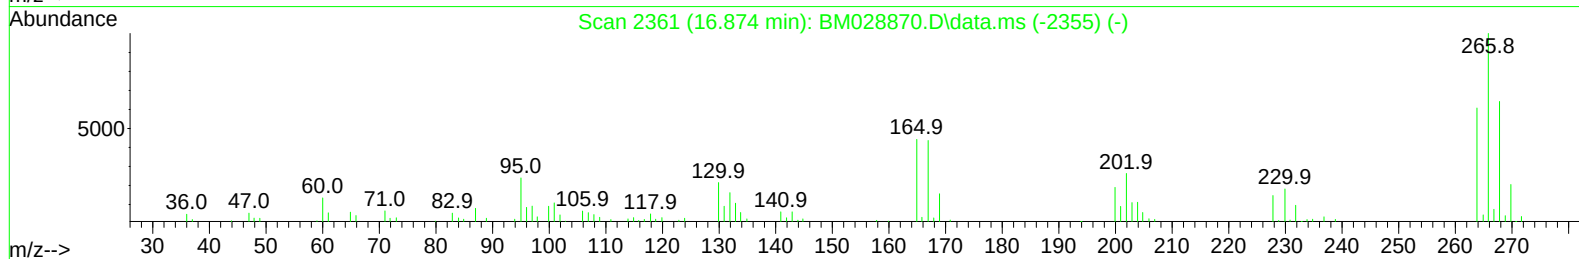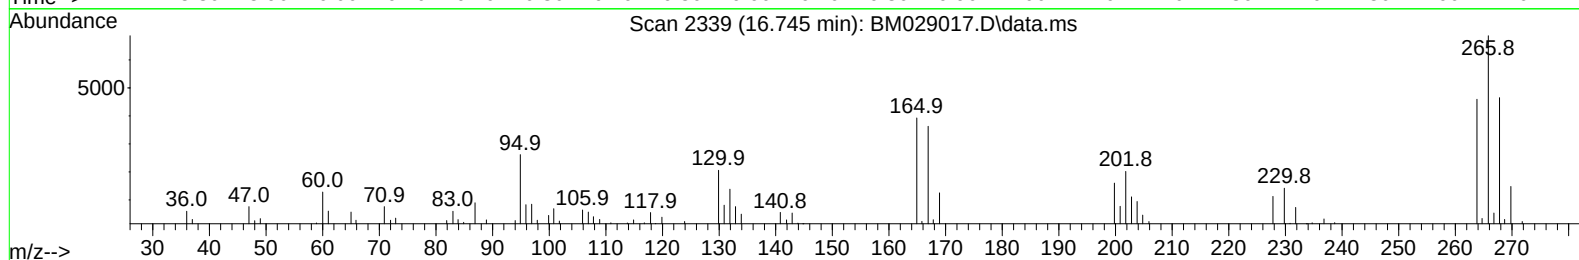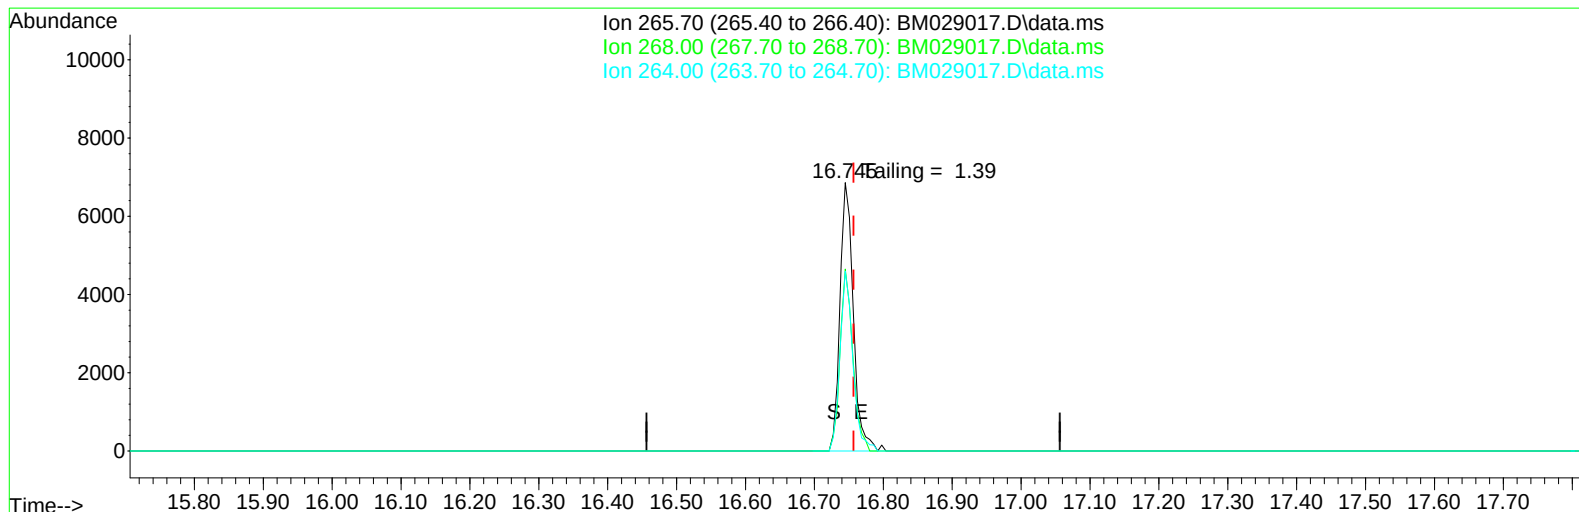

TIC: BM029017.D\data.ms

(70) Pentachlorophenol (C)

16.745min (-0.012) 0.00 ng

response 9255

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.40	72.22
264.00	63.30	71.88
0.00	0.00	0.00