

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030824\
 Data File : BM044565.D
 Acq On : 08 Mar 2024 15:12
 Operator : MA/JU
 Sample : PB159505BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK505

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM044565.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.275	28	32	38	rBV	72280	100177	1.51%	0.138%
2	3.669	95	99	118	rBV	953119	1646274	24.87%	2.264%
3	3.975	147	151	157	rVB2	16620	25743	0.39%	0.035%
4	6.887	639	646	659	rBV	1193773	1884164	28.46%	2.591%
5	7.063	670	676	690	rVB	993266	1620606	24.48%	2.228%
6	7.251	700	708	718	rBV	1140258	1852434	27.98%	2.547%
7	7.716	780	787	796	rBV	1046323	1647852	24.89%	2.266%
8	8.416	898	906	918	rBV	1454295	2356824	35.60%	3.241%
9	8.875	977	984	996	rBV	1099657	1897960	28.67%	2.610%
10	9.592	1098	1106	1120	rBV	947145	1584229	23.93%	2.178%
11	10.122	1186	1196	1212	rBV	1365797	2342400	35.38%	3.221%
12	10.498	1252	1260	1268	rVB	1529382	2529468	38.21%	3.478%
13	10.645	1277	1285	1310	rBV	1478940	2635394	39.81%	3.624%
14	12.098	1525	1532	1540	rBV2	21020	44583	0.67%	0.061%
15	13.251	1724	1728	1736	rVV6	5569	11327	0.17%	0.016%
16	13.333	1738	1742	1745	rBV4	4599	7115	0.11%	0.010%
17	13.780	1811	1818	1827	rBV	2575311	3566624	53.87%	4.904%
18	14.051	1855	1864	1875	rBV	2901126	4336876	65.51%	5.963%
19	14.363	1910	1917	1926	rBV	2318773	3453197	52.16%	4.748%
20	14.569	1945	1952	1967	rBV	1168195	1818260	27.46%	2.500%
21	15.357	2079	2086	2094	rBV	3674922	5365615	81.05%	7.378%
22	15.486	2101	2108	2121	rBV	1213324	1714956	25.90%	2.358%
23	15.598	2124	2127	2133	rVB4	16928	24465	0.37%	0.034%
24	16.145	2216	2220	2224	rBV4	11699	17164	0.26%	0.024%
25	16.792	2324	2330	2335	rBV7	5422	11154	0.17%	0.015%
26	16.904	2346	2349	2357	rVB5	6126	10326	0.16%	0.014%
27	17.116	2378	2385	2395	rBV	2850655	4015569	60.65%	5.521%
28	17.216	2395	2402	2416	rBV	4116470	5774226	87.22%	7.939%
29	18.033	2537	2541	2545	rBV6	5079	8573	0.13%	0.012%
30	19.074	2714	2718	2724	rBV2	47875	68353	1.03%	0.094%
31	19.151	2726	2731	2736	rVV	38257	56620	0.86%	0.078%
32	19.515	2786	2793	2802	rBV	5016704	6620415	100.00%	9.103%
33	21.309	3093	3098	3108	rBV	3151861	4055945	61.26%	5.577%
34	23.421	3450	3457	3465	rBV2	3122047	5781038	87.32%	7.949%
35	23.568	3475	3482	3493	rVB	2057193	3842283	58.04%	5.283%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030824\
Data File : BM044565.D
Acq On : 08 Mar 2024 15:12
Operator : MA/JU
Sample : PB159505BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK505

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 72728209

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030824\
Data File : BM044565.D
Acq On : 08 Mar 2024 15:12
Operator : MA/JU
Sample : PB159505BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK505

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

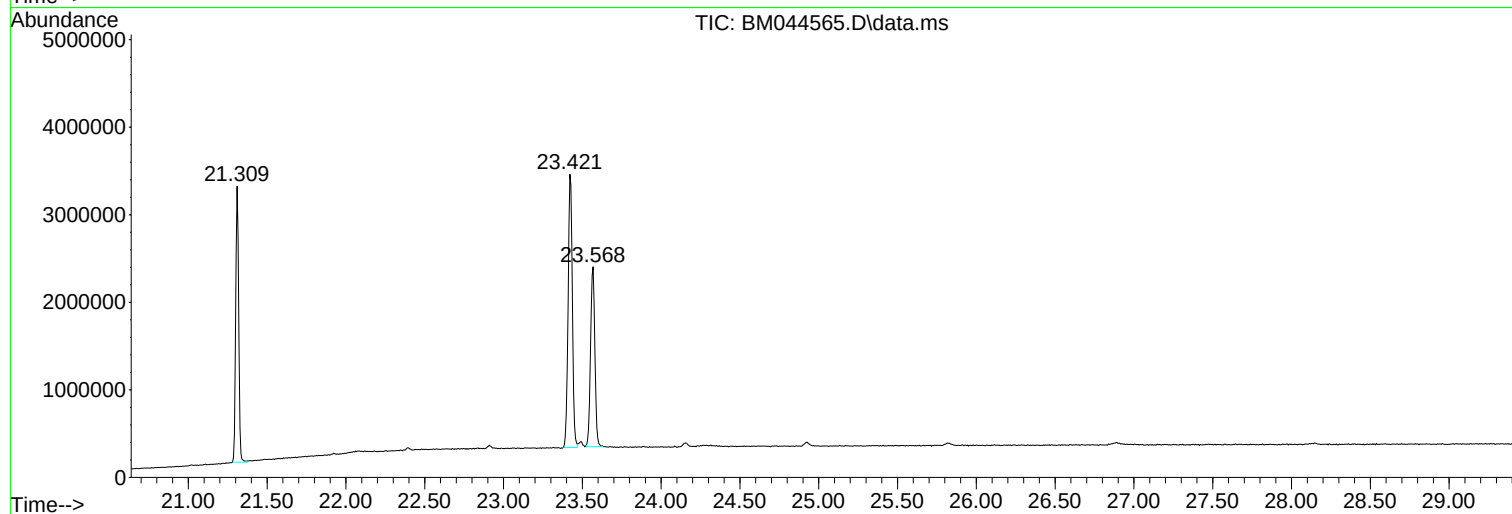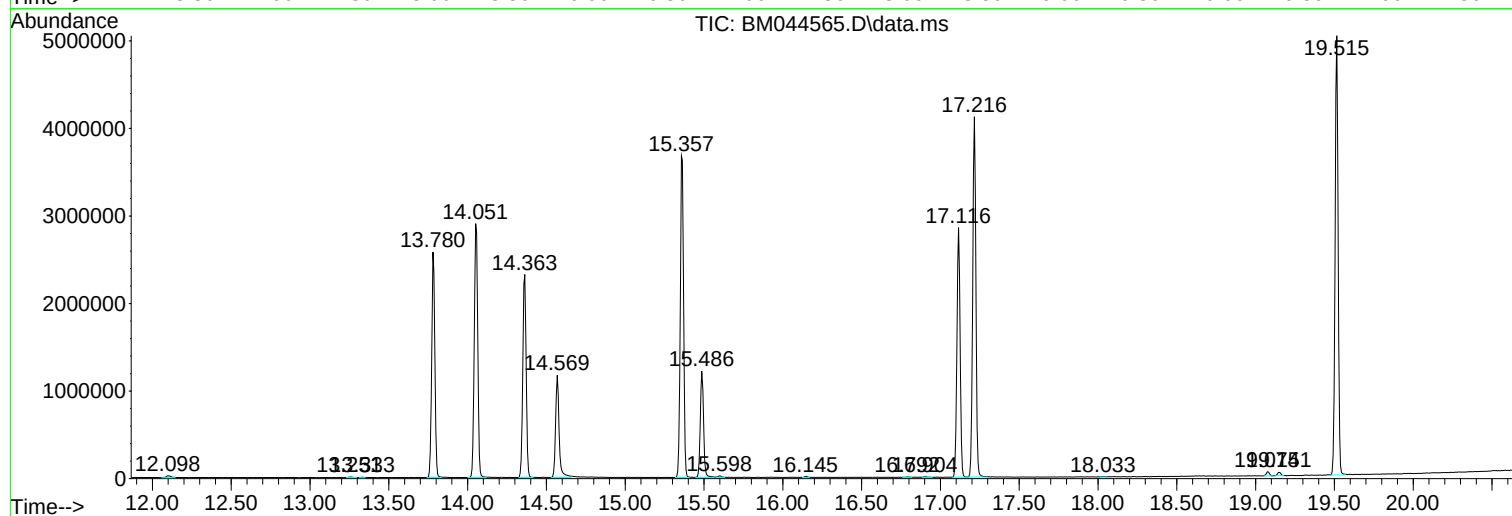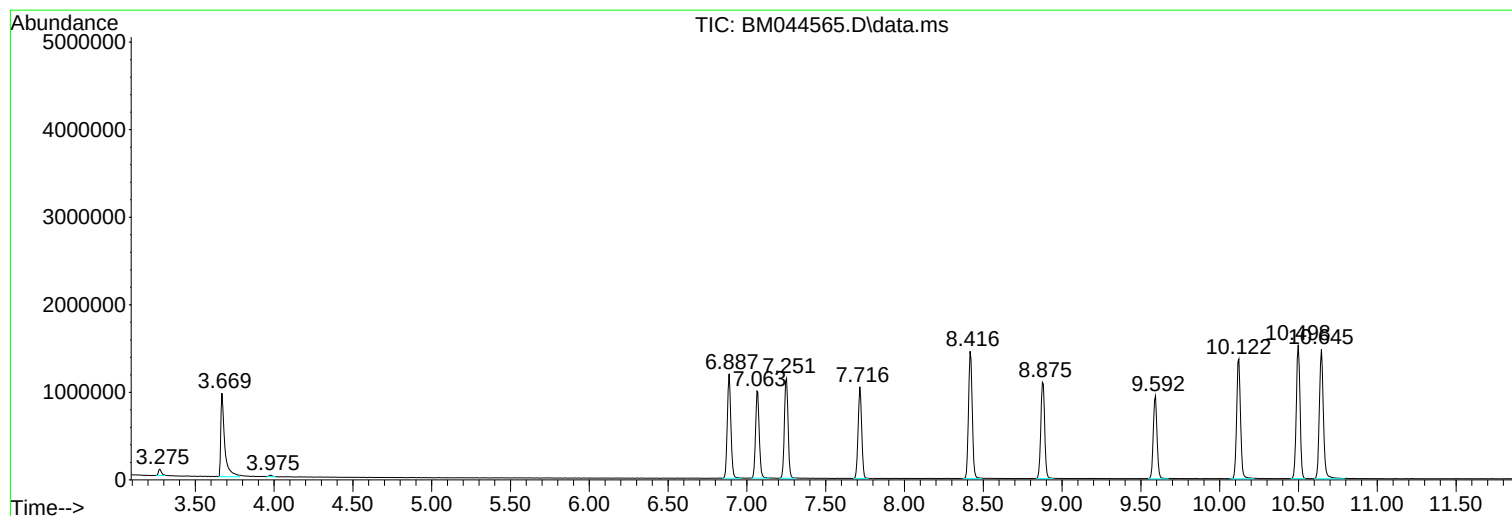

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030824\
Data File : BM044565.D
Acq On : 08 Mar 2024 15:12
Operator : MA/JU
Sample : PB159505BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK505

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030824\
Data File : BM044565.D
Acq On : 08 Mar 2024 15:12
Operator : MA/JU
Sample : PB159505BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK505

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc