

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030824\
 Data File : BM044566.D
 Acq On : 08 Mar 2024 15:48
 Operator : MA/JU
 Sample : P1703-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BH7G7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM044566.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.275	28	32	50	rVB2	71192	129505	1.48%	0.165%
2	3.675	97	100	119	rBV	353045	645170	7.36%	0.821%
3	3.975	148	151	158	rVB	16387	25942	0.30%	0.033%
4	6.887	640	646	655	rBV	319022	510073	5.82%	0.649%
5	7.063	670	676	691	rBV	1218997	1982119	22.63%	2.522%
6	7.251	700	708	718	rBV	1077764	1726256	19.71%	2.196%
7	7.334	718	722	725	rVB5	6992	11757	0.13%	0.015%
8	7.716	779	787	795	rBV	890492	1419213	16.20%	1.806%
9	8.416	899	906	919	rBV	934841	1513562	17.28%	1.926%
10	8.875	977	984	994	rBV	1421842	2384363	27.22%	3.034%
11	8.981	998	1002	1009	rVB8	8863	15840	0.18%	0.020%
12	9.592	1097	1106	1116	rBV	1131843	1895589	21.64%	2.412%
13	10.122	1188	1196	1211	rBV	1574470	2719077	31.04%	3.460%
14	10.498	1252	1260	1269	rVB	1340062	2209033	25.22%	2.811%
15	10.645	1276	1285	1300	rBV	1667819	2889802	32.99%	3.677%
16	11.933	1497	1504	1508	rBV5	6166	11705	0.13%	0.015%
17	12.098	1527	1532	1540	rBV	29381	51130	0.58%	0.065%
18	13.180	1711	1716	1721	rBV3	9611	15127	0.17%	0.019%
19	13.257	1723	1729	1735	rBV2	25603	44934	0.51%	0.057%
20	13.780	1811	1818	1827	rBV	3285208	4719391	53.87%	6.005%
21	14.057	1856	1865	1875	rBV	3828498	5773092	65.90%	7.346%
22	14.269	1896	1901	1906	rVB2	16790	21821	0.25%	0.028%
23	14.363	1909	1917	1927	rBV	2032846	3031967	34.61%	3.858%
24	14.574	1946	1953	1970	rBV	227981	455401	5.20%	0.579%
25	14.792	1983	1990	1995	rVB9	8464	19079	0.22%	0.024%
26	15.221	2057	2063	2069	rVB5	20373	34619	0.40%	0.044%
27	15.363	2080	2087	2096	rBV	4953656	7176756	81.92%	9.132%
28	15.486	2101	2108	2122	rVV	1778522	2424756	27.68%	3.085%
29	15.604	2122	2128	2138	rVB2	21795	46077	0.53%	0.059%
30	16.092	2206	2211	2218	rBV2	23150	47475	0.54%	0.060%
31	16.145	2218	2220	2225	rVB4	17219	19892	0.23%	0.025%
32	16.798	2326	2331	2337	rVB7	6979	9845	0.11%	0.013%
33	16.886	2342	2346	2352	rVV4	16946	30985	0.35%	0.039%
34	17.115	2378	2385	2395	rBV	2471356	3512700	40.10%	4.470%
35	17.215	2395	2402	2413	rBV	5499645	7751935	88.49%	9.864%
36	17.621	2467	2471	2476	rBV3	15623	22399	0.26%	0.029%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030824\
Data File : BM044566.D
Acq On : 08 Mar 2024 15:48
Operator : MA/JU
Sample : P1703-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH7G7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
Title : SVOA CALIBRATION

37	17.804	2498	2502	2507	rVB6	6665	11355	0.13%	0.014%
38	18.021	2534	2539	2548	rBV	114557	176398	2.01%	0.224%
39	18.321	2586	2590	2594	rVB3	13744	17220	0.20%	0.022%
40	18.957	2694	2698	2701	rBV5	18678	22515	0.26%	0.029%
41	19.080	2714	2719	2724	rBV2	62649	89570	1.02%	0.114%
42	19.151	2726	2731	2735	rVV	54185	74920	0.86%	0.095%
43	19.309	2753	2758	2767	rBV	107144	157686	1.80%	0.201%
44	19.515	2786	2793	2802	rBV	6707885	8760350	100.00%	11.147%
45	21.309	3093	3098	3107	rBV	2768146	3460204	39.50%	4.403%
46	23.421	3450	3457	3465	rBV2	4008453	7381890	84.26%	9.393%
47	23.562	3475	3481	3490	rVB	1672750	3141164	35.86%	3.997%




Sum of corrected areas: 78591659

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030824\
Data File : BM044566.D
Acq On : 08 Mar 2024 15:48
Operator : MA/JU
Sample : P1703-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH7G7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

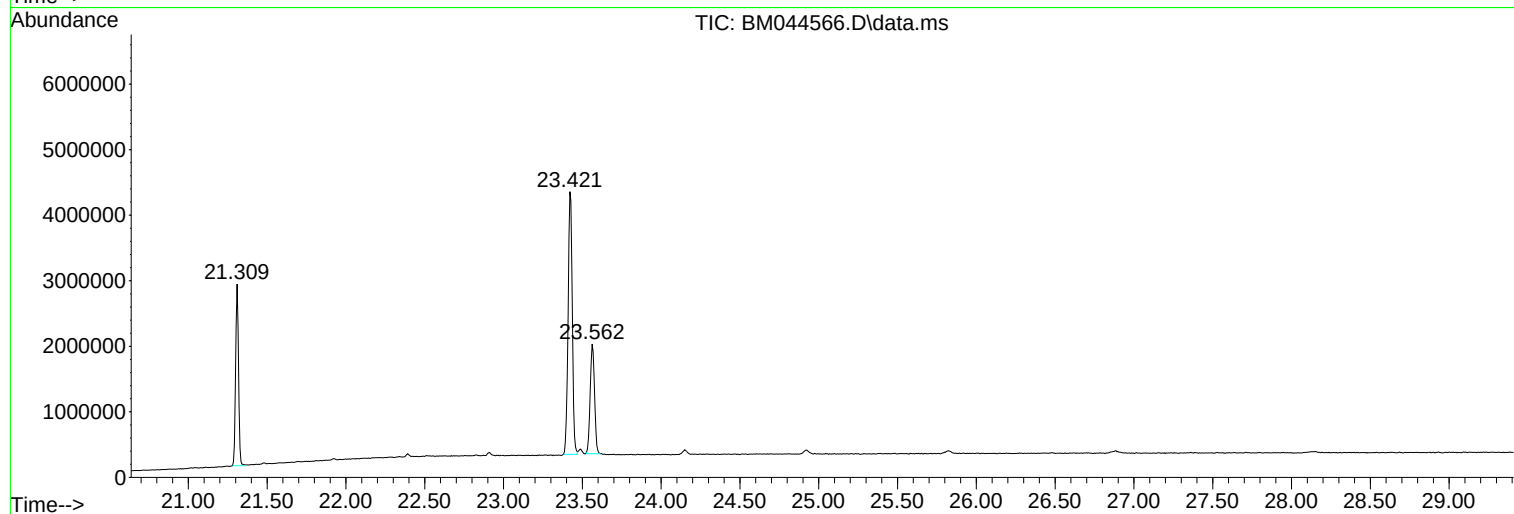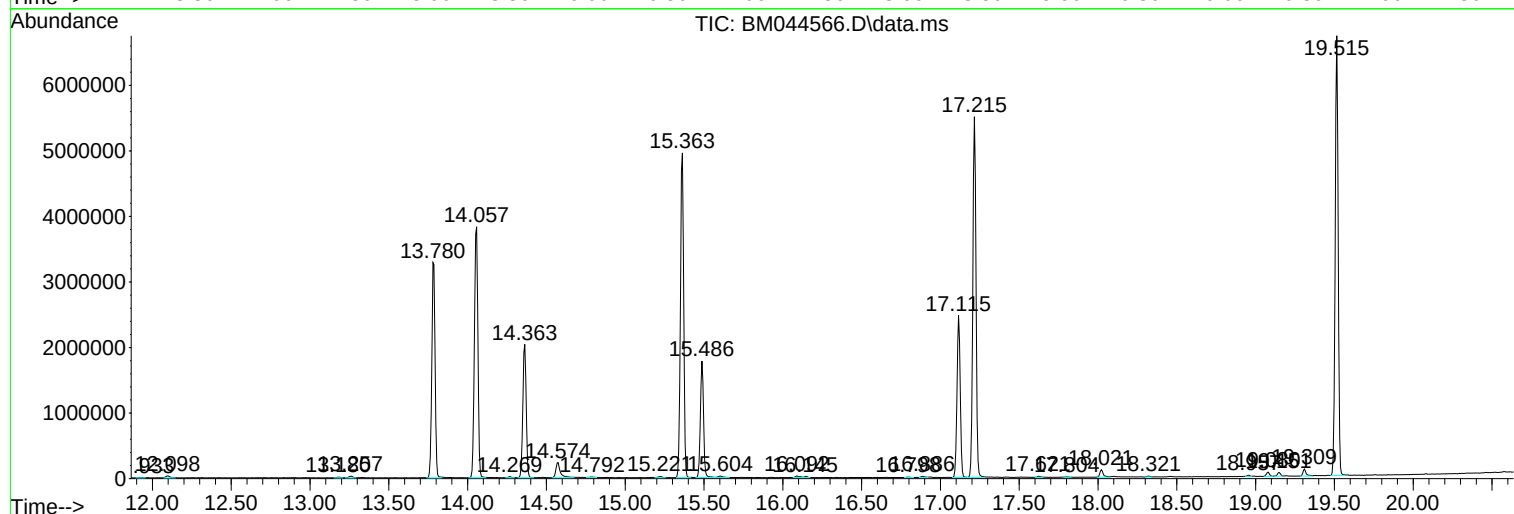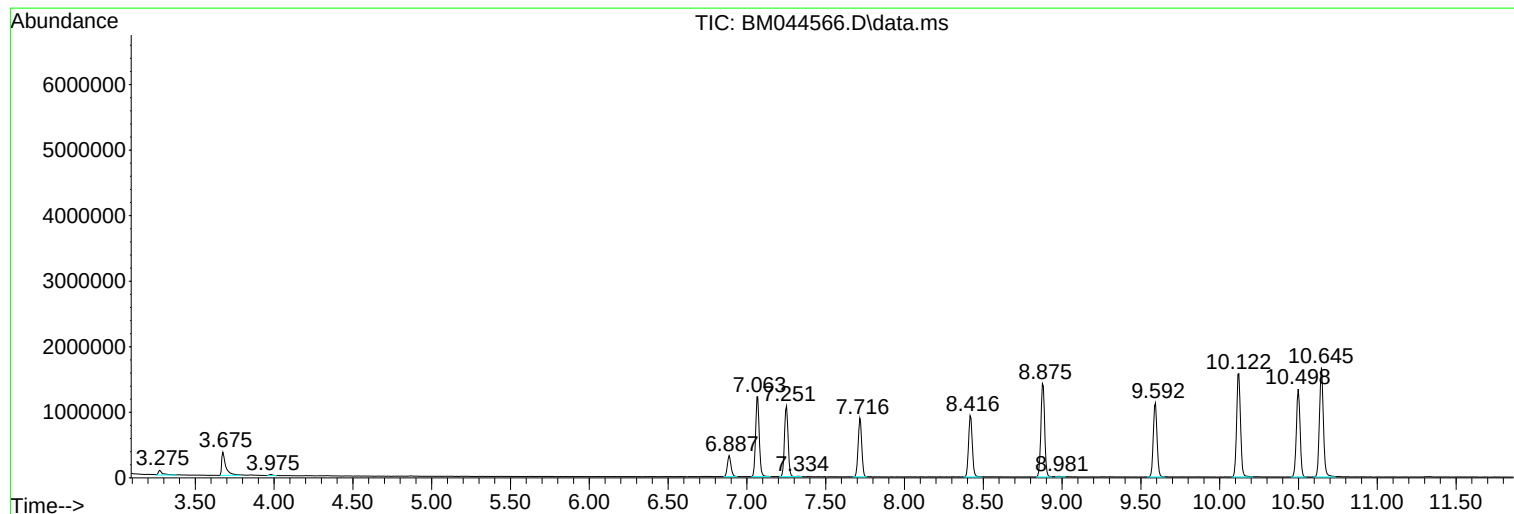

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030824\
Data File : BM044566.D
Acq On : 08 Mar 2024 15:48
Operator : MA/JU
Sample : P1703-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH7G7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030824\
Data File : BM044566.D
Acq On : 08 Mar 2024 15:48
Operator : MA/JU
Sample : P1703-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH7G7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc