

Quantitation Report (QT Reviewed)


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM030920\
 Data File : BM025420.D
 Acq On : 09 Mar 2020 18:49
 Operator : CG/JU
 Sample : L1612-10
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBDL2

Manual Integrations
 APPROVED

mohammad
 3/10/2020 7:59:05 AM

Quant Time: Mar 09 19:22:04 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030920.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Mar 09 13:32:56 2020
 Response via : Initial Calibration

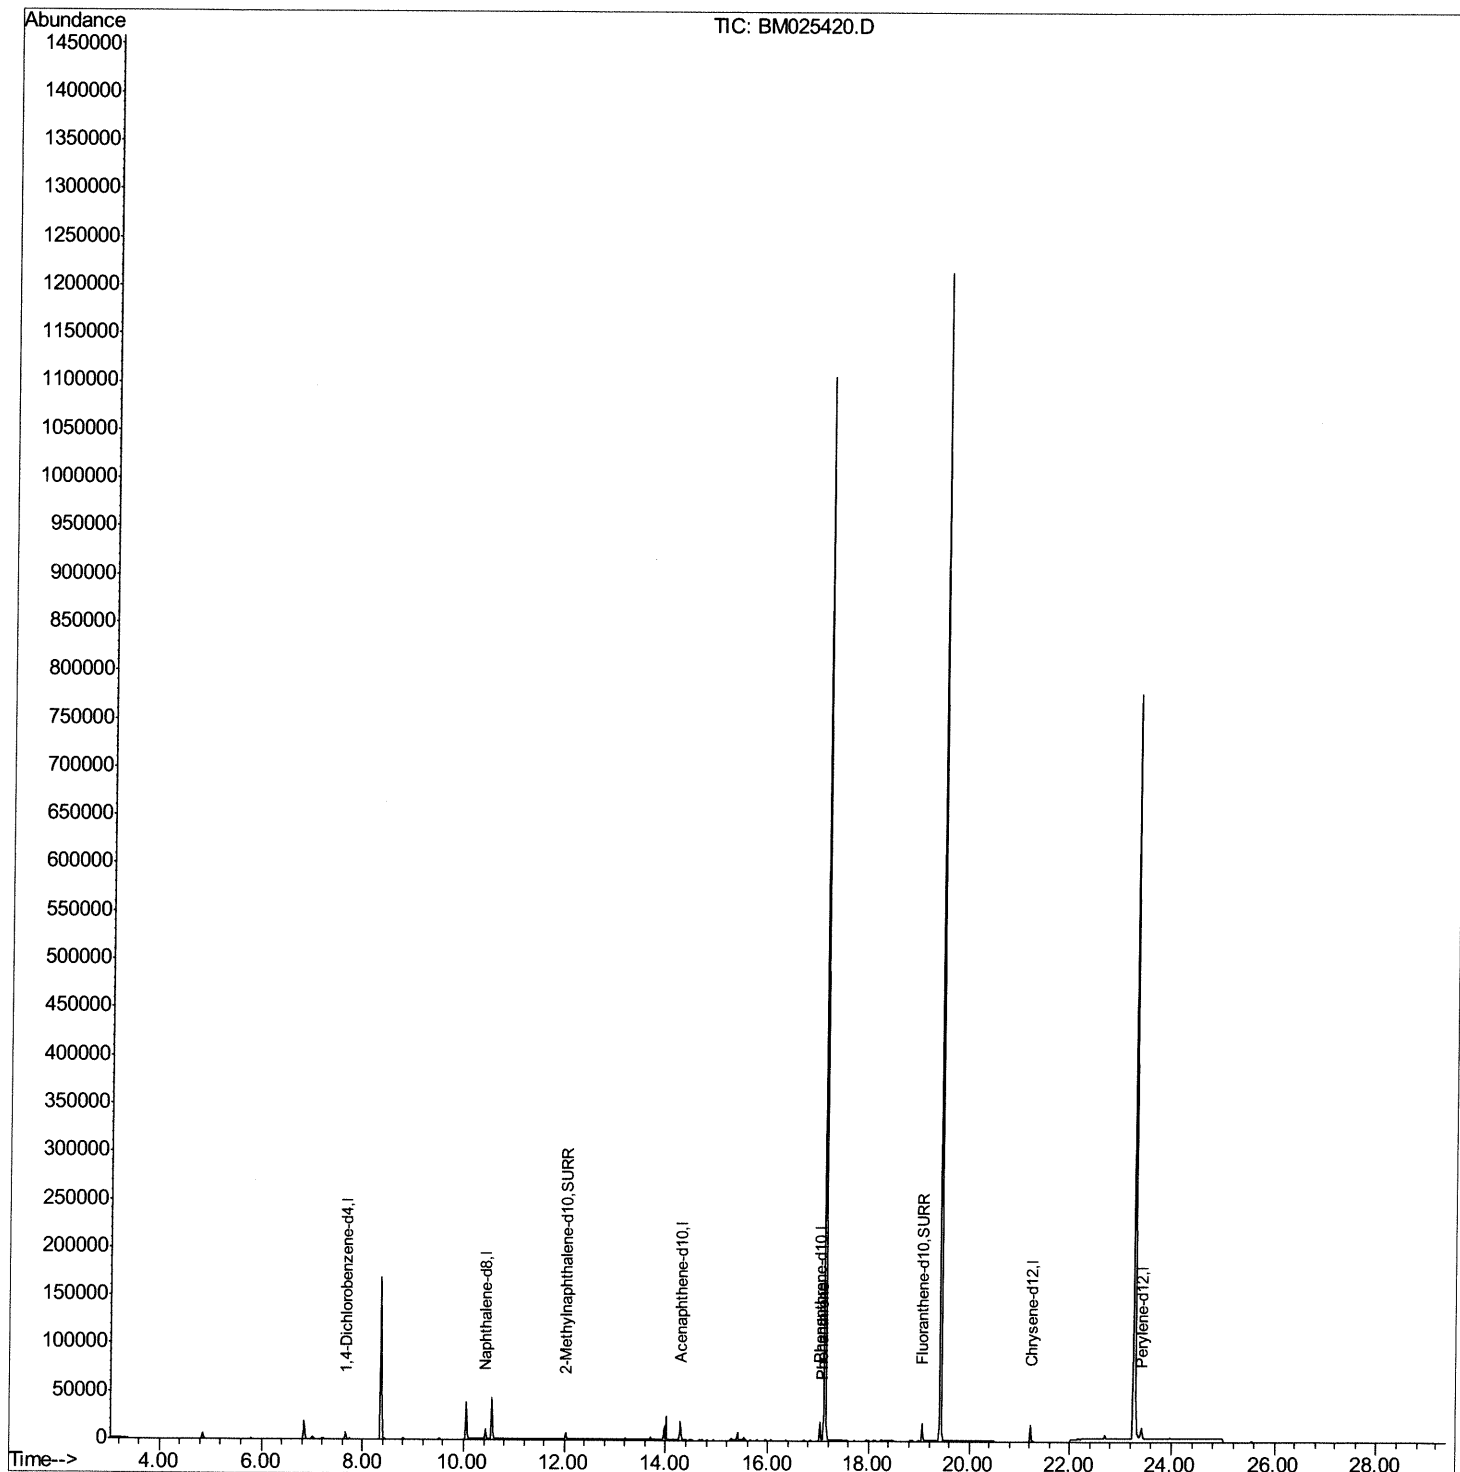

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM030920\
 Data File : BM025420.D
 Acq On : 09 Mar 2020 18:49
 Operator : CG/JU
 Sample : L1612-10
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBDL2

Manual Integrations
 APPROVED

mohammad
 3/10/2020 7:59:05 AM

Quant Time: Mar 09 19:21:09 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030920.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Mar 09 13:32:56 2020
 Response via : Initial Calibration

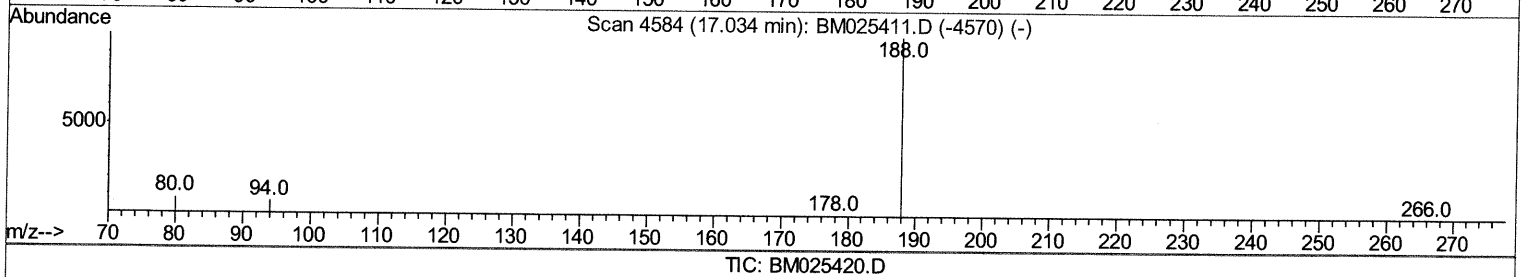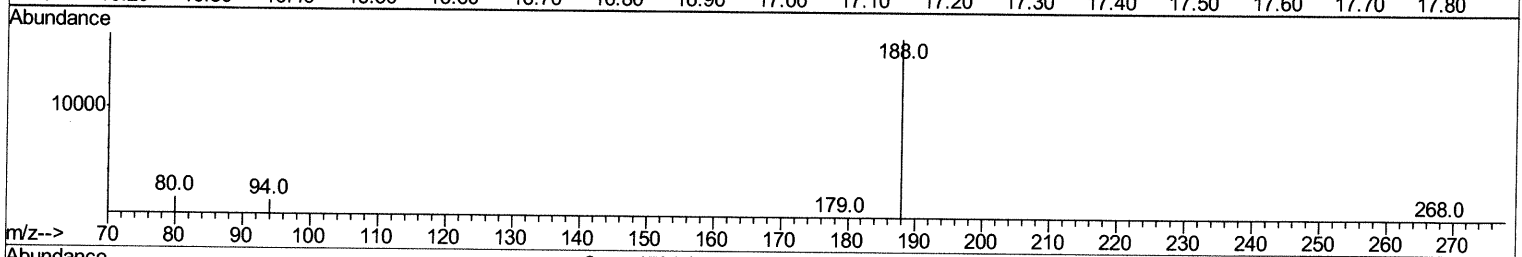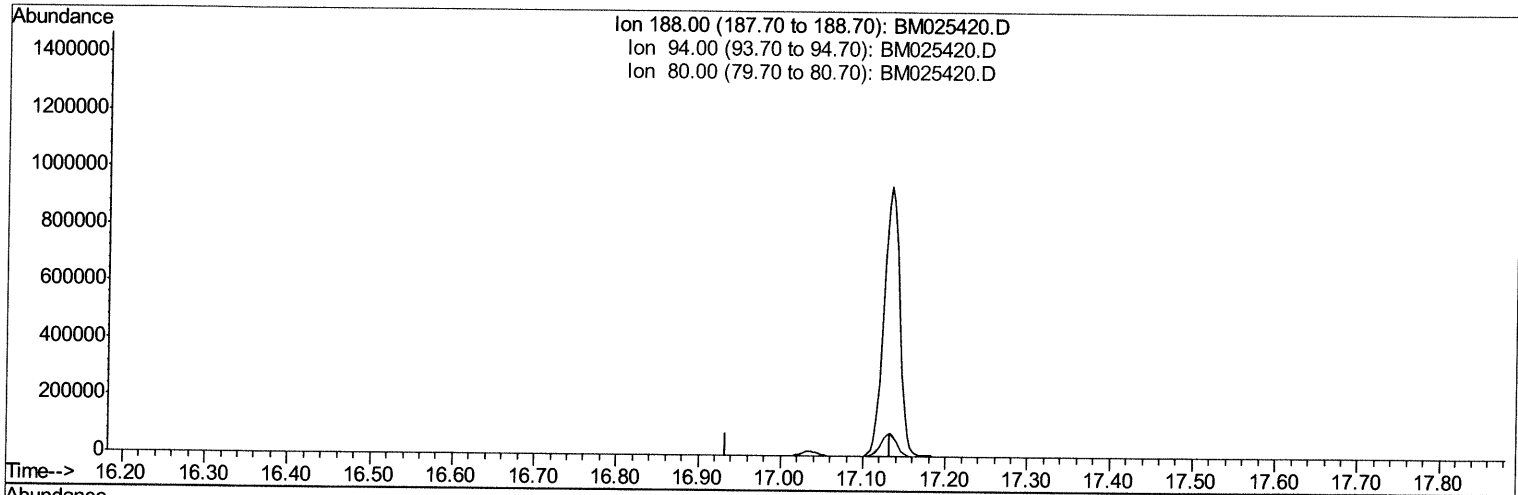

(10) Phenanthrene-d10 (I)

17.034min (-17.034) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	7.10	0.00#
80.00	8.70	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM030920\
 Data File : BM025420.D
 Acq On : 09 Mar 2020 18:49
 Operator : CG/JU
 Sample : L1612-10
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBDL2

Manual Integrations
 APPROVED

mohammad
 3/10/2020 7:59:05 AM

Quant Time: Mar 09 19:21:09 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030920.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Mar 09 13:32:56 2020
 Response via : Initial Calibration

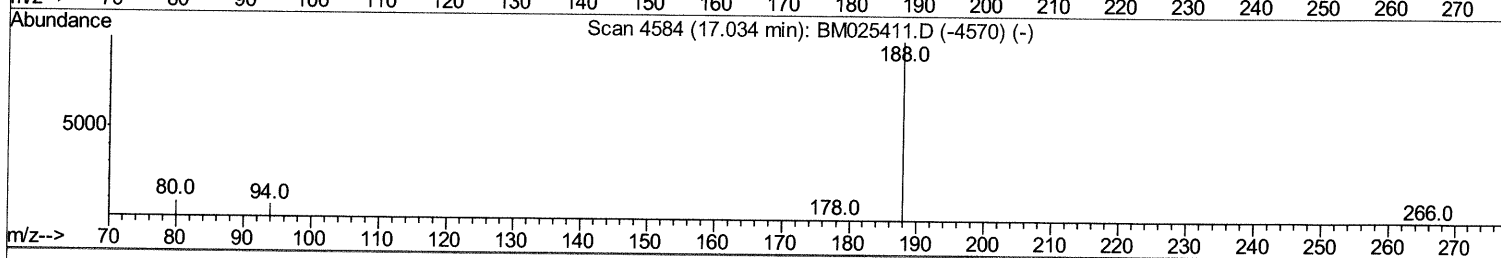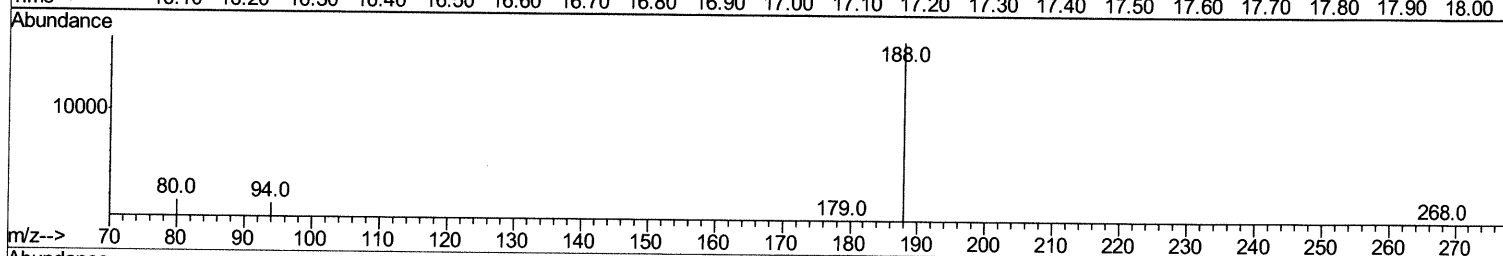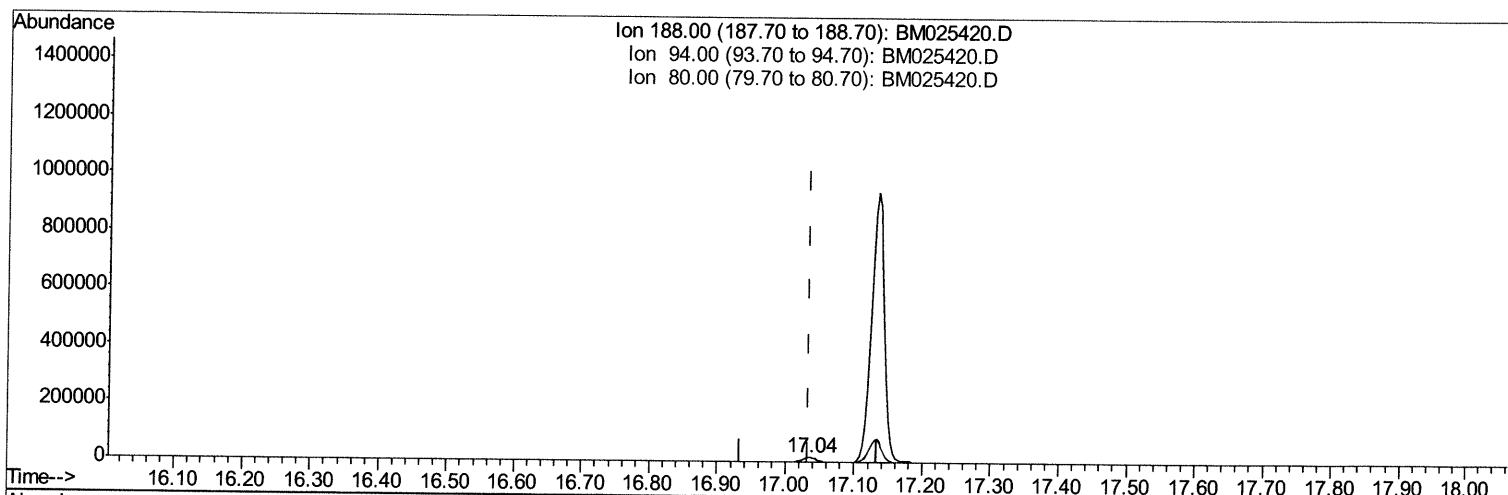

TIC: BM025420.D

(10) Phenanthrene-d10 (I)

17.036min (+0.002) 0.40ng/ul m 7403/16/20

response 23352

Ion	Exp%	Act%
188.00	100	100
94.00	7.10	8.04
80.00	8.70	9.18
0.00	0.00	0.00

Quantitation Report (QT Reviewed)

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM030920\
 Data File : BM025420.D
 Acq On : 09 Mar 2020 18:49
 Operator : CG/JU
 Sample : L1612-10
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBDL2

Manual Integrations
 APPROVED

mohammad
 3/10/2020 7:59:05 AM

Quant Time: Mar 09 19:22:04 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030920.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Mar 09 13:32:56 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Dichlorobenzene-d4	7.67	152	3328	0.40	ng/ul	0.00
2) Naphthalene-d8	10.43	136	14480	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.29	164	10647	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.04	188	23352m >	0.40	ng/ul >	0.00
16) Chrysene-d12	21.22	240	16230	0.40	ng/ul	0.00
20) Perylene-d12	23.41	264	15310	0.40	ng/ul	0.00

Ju 03/10/20

System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.03	152	8622	0.33	ng/ul	0.00
14) Fluoranthene-d10	19.06	212	19999	0.31	ng/ul	0.00

Target Compounds						
12) Phenanthrene	17.07	178	1484	0.020	ng/ul	Ovalue # 88

(#) = qualifier out of range (m) = manual integration (+) = signals summed