

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM030920\
Data File : BM025433.D
Acq On : 10 Mar 2020 03:17
Operator : CG/JU
Sample : PB127030BL
Misc :
ALS Vial : 27 Sample Multiplier: 1

Quant Time: Mar 10 11:39:44 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 09 13:32:56 2020
Response via : Initial Calibration

Instrument :

BNA_M

Client SampleId :


SBLK30

Manual Integrations

APPROVED

mohammad

3/11/2020 8:00:28 AM

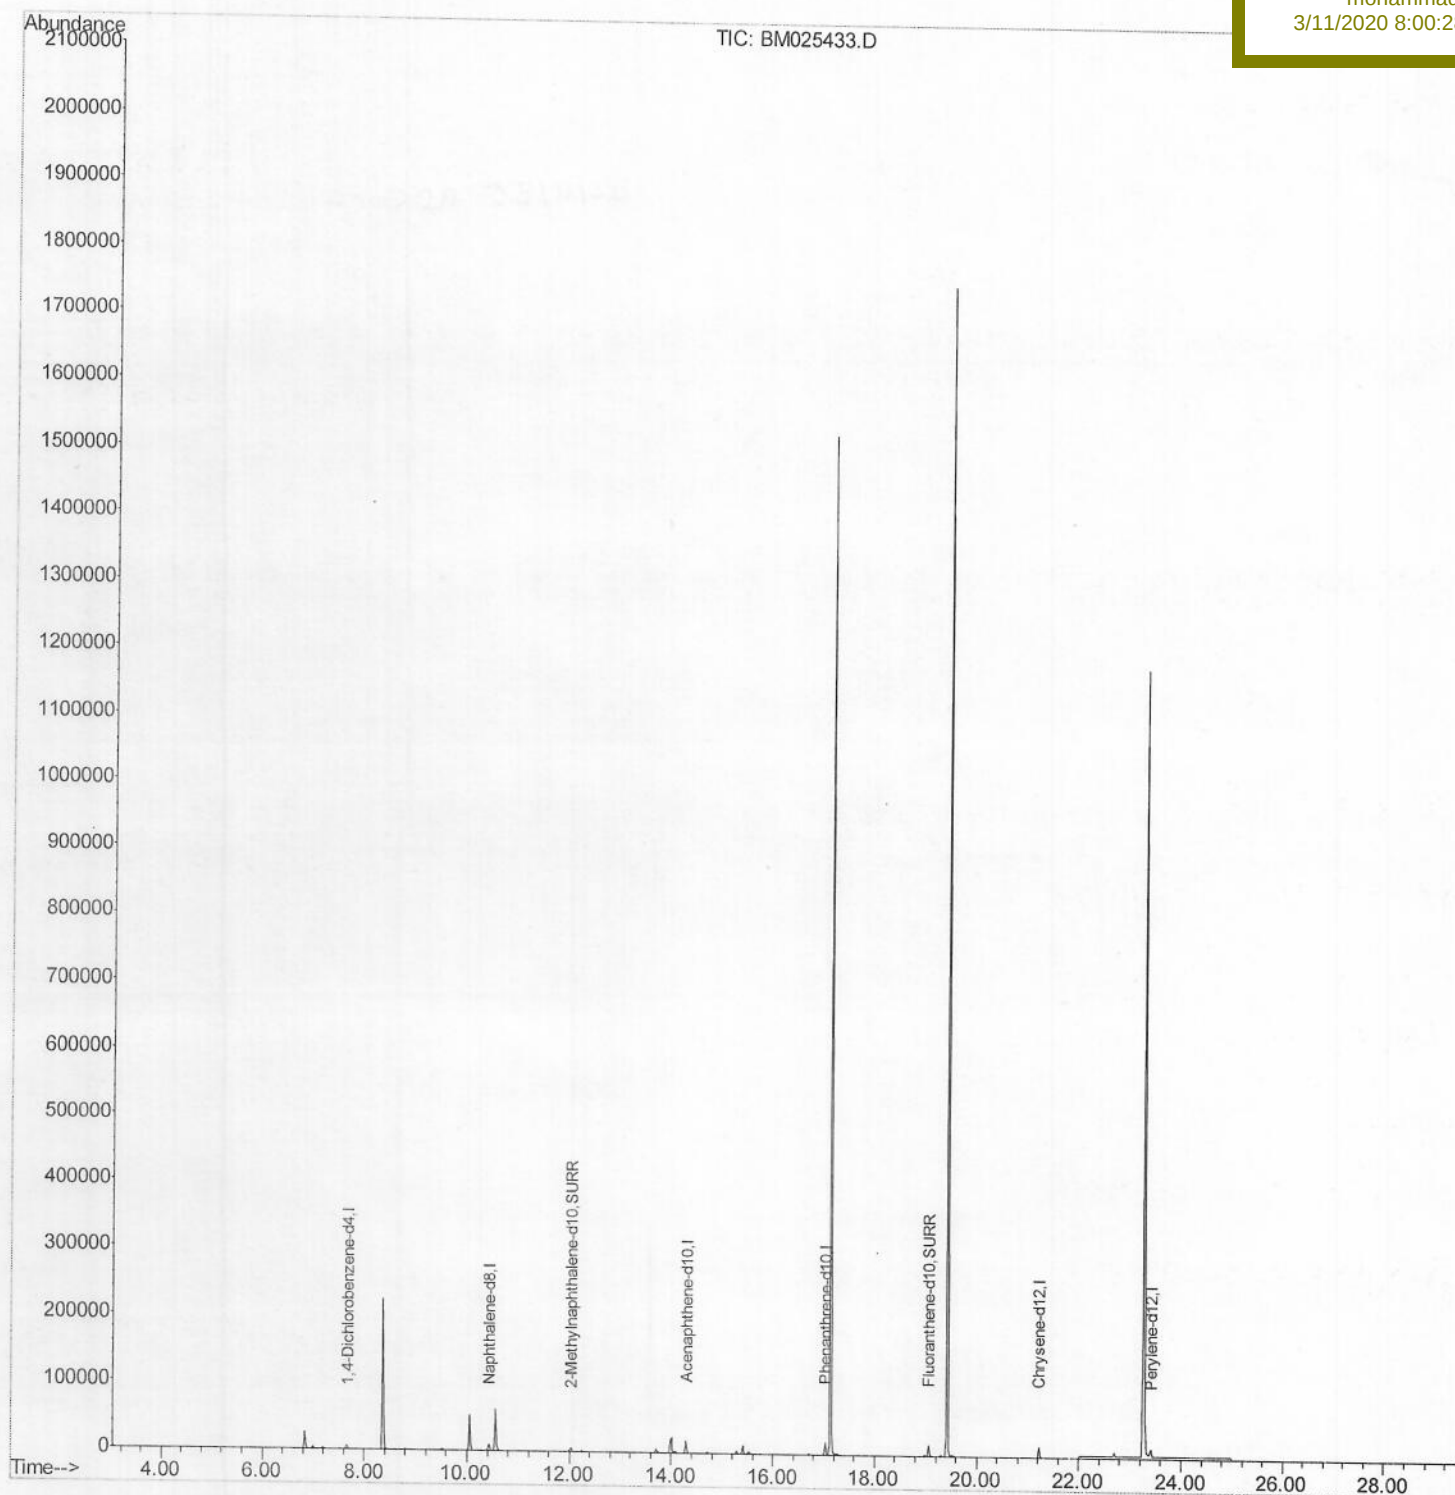

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM030920\
Data File : BM025433.D
Acq On : 10 Mar 2020 03:17
Operator : CG/JU
Sample : PB127030BL
Misc :
ALS Vial : 27 Sample Multiplier: 1

Quant Time: Mar 10 11:38:14 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 09 13:32:56 2020
Response via : Initial Calibration

Instrument :

BNA_M

ClientSampleId :




SBLK30

Manual Integrations

APPROVED

mohammad

3/11/2020 8:00:28 AM

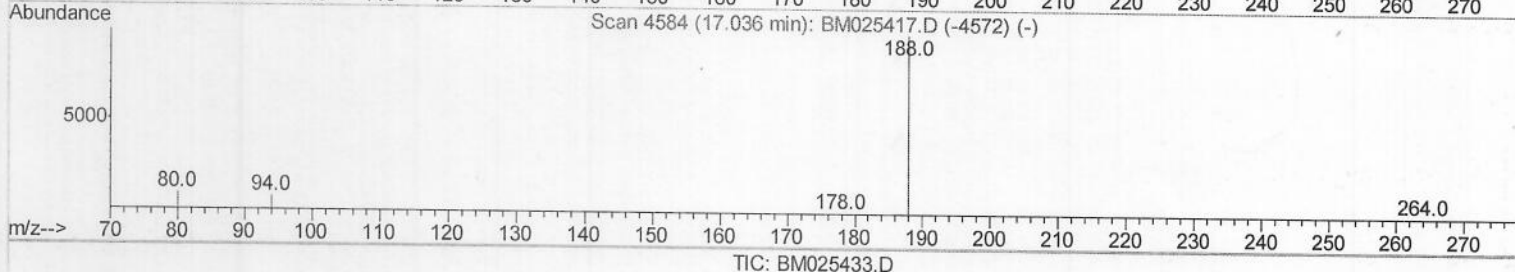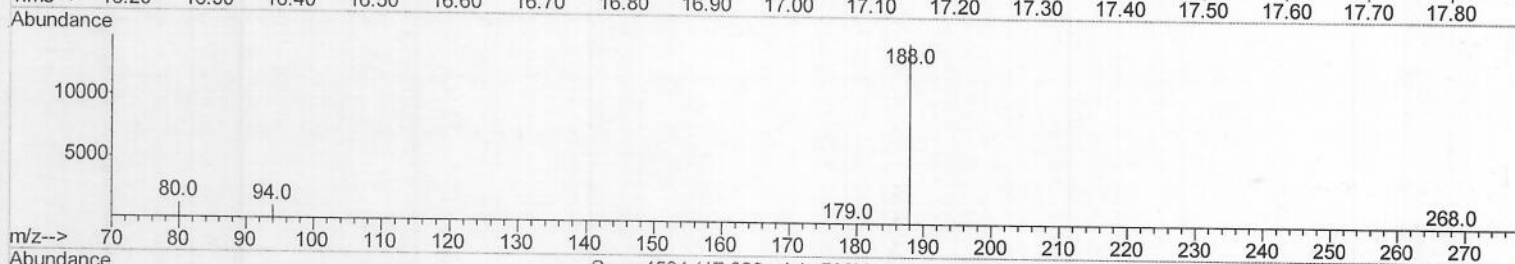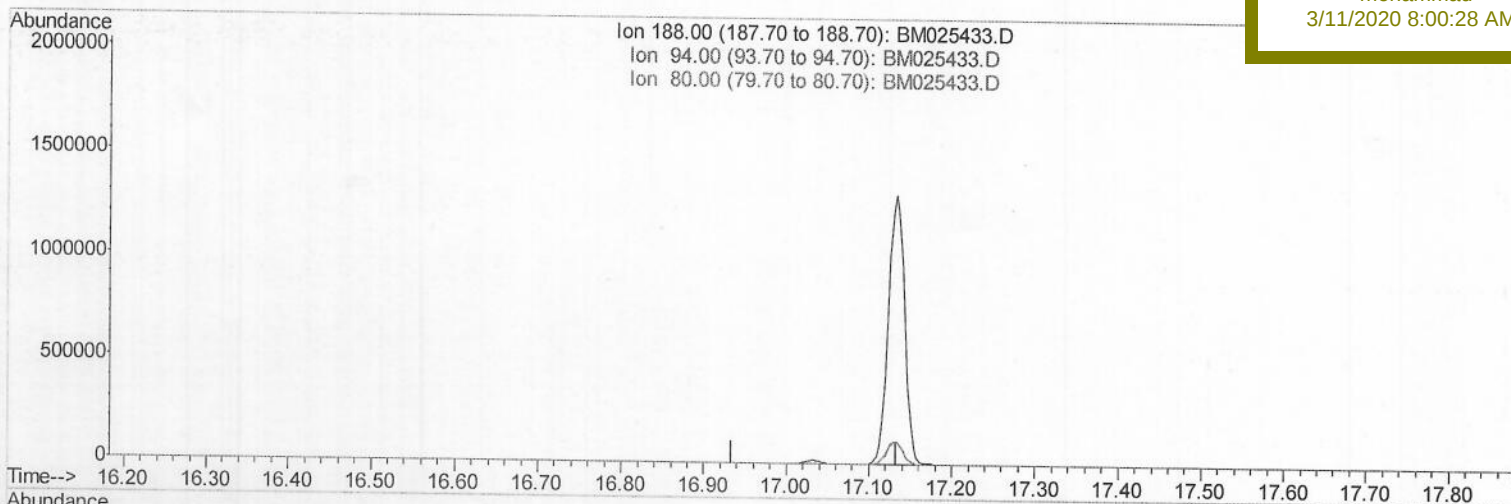

(10) Phenanthrene-d10 (I)

17.034min (-17.034) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	7.10	0.00#
80.00	8.70	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM030920\
 Data File : BM025433.D
 Acq On : 10 Mar 2020 03:17
 Operator : CG/JU
 Sample : PB127030BL
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Quant Time: Mar 10 11:38:14 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030920.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Mar 09 13:32:56 2020
 Response via : Initial Calibration

Instrument :
 BNA_M
 ClientSampleId :
 SBLK30

Manual Integrations
 APPROVED

mohammad
 3/11/2020 8:00:28 AM

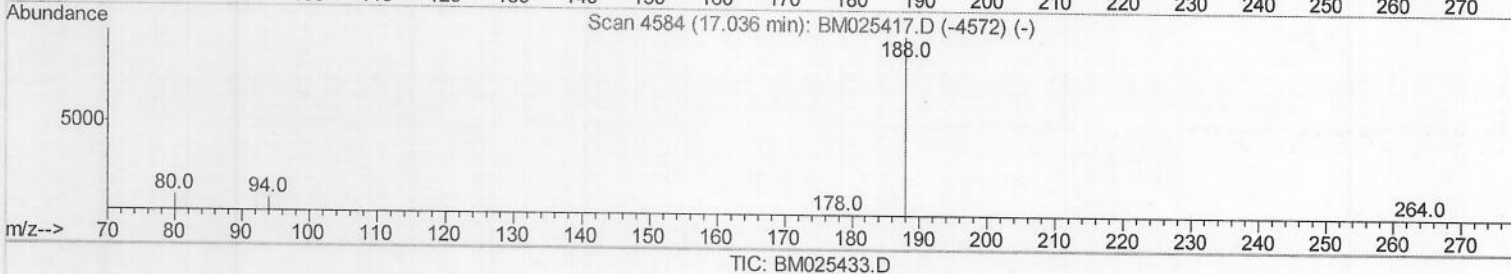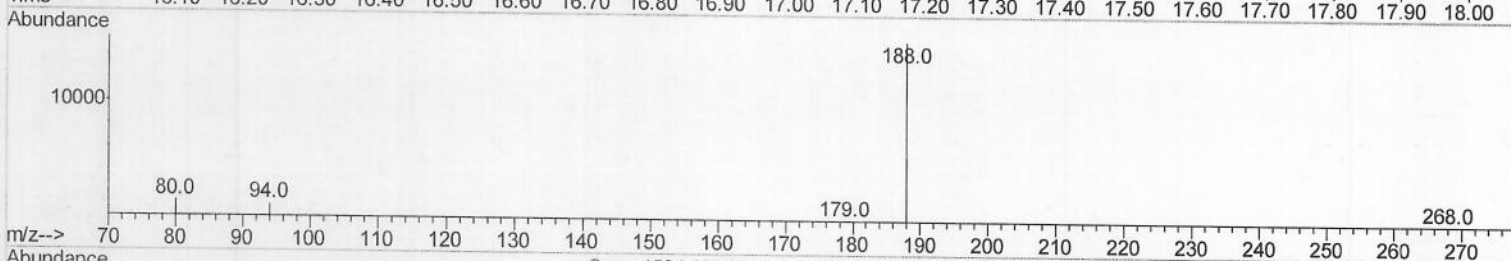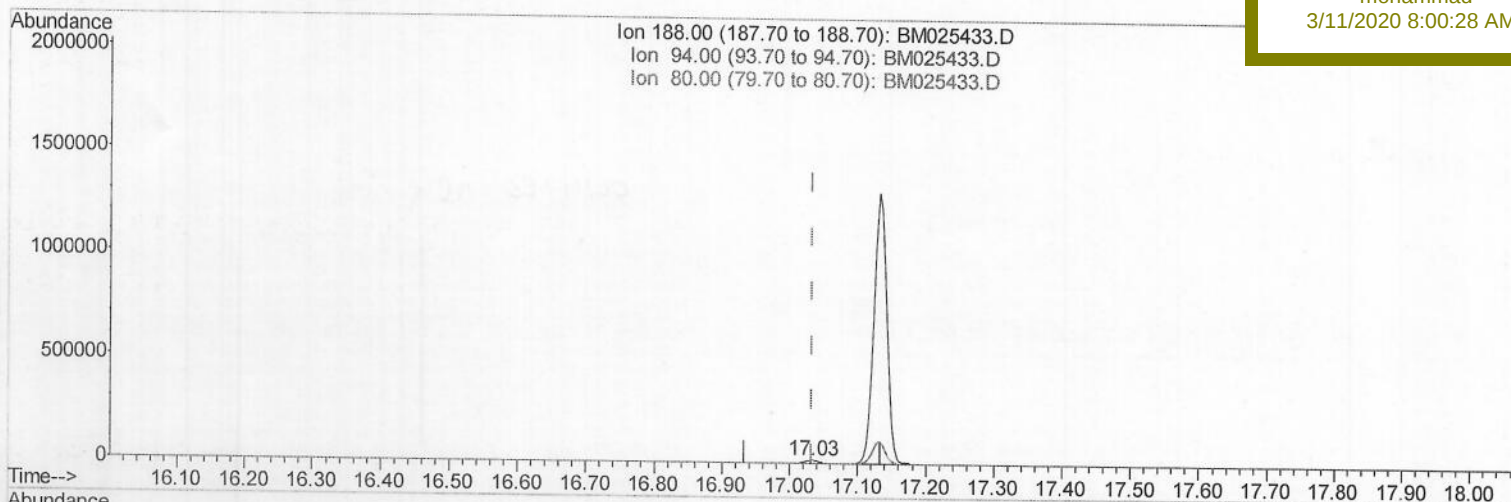

(10) Phenanthrene-d10 (l)

17.032min (-0.002) 0.40ng/ul m>20 03/11/20

response 21322

Ion	Exp%	Act%
188.00	100	100
94.00	7.10	7.39
80.00	8.70	8.88
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM030920\
Data File : BM025433.D
Acq On : 10 Mar 2020 03:17
Operator : CG/JU
Sample : PB127030BL
Misc :
ALS Vial : 27 Sample Multiplier: 1

Quant Time: Mar 10 11:39:44 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 09 13:32:56 2020
Response via : Initial Calibration

Instrument :
BNA_M
ClientSampleId :
SBLK30

Manual Integrations
APPROVED

mohammad
3/11/2020 8:00:28 AM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.66	152	2922	0.40	ng/ul	0.00
2) Naphthalene-d8	10.43	136	12375	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.29	164	9511	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.03	188	21322m	0.40	ng/ul	0.00
16) Chrysene-d12	21.22	240	15120	0.40	ng/ul	0.00
20) Perylene-d12	23.40	264	15168	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.02	152	7574	0.34	ng/ul	0.00
14) Fluoranthene-d10	19.06	212	19081	0.33	ng/ul	0.00

Target Compounds Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

JU 03/11/20