


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM030920\
Data File : BM025451.D
Acq On : 10 Mar 2020 14:09
Operator : CG/JU
Sample : L1617-07
Misc :
ALS Vial : 45 Sample Multiplier: 1

Quant Time: Mar 10 14:50:32 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 09 13:32:56 2020
Response via : Initial Calibration

Instrument :
BNA_M
ClientSampleId :
DBDS1

Manual Integrations
APPROVED

mohammad
3/11/2020 8:01:20 AM

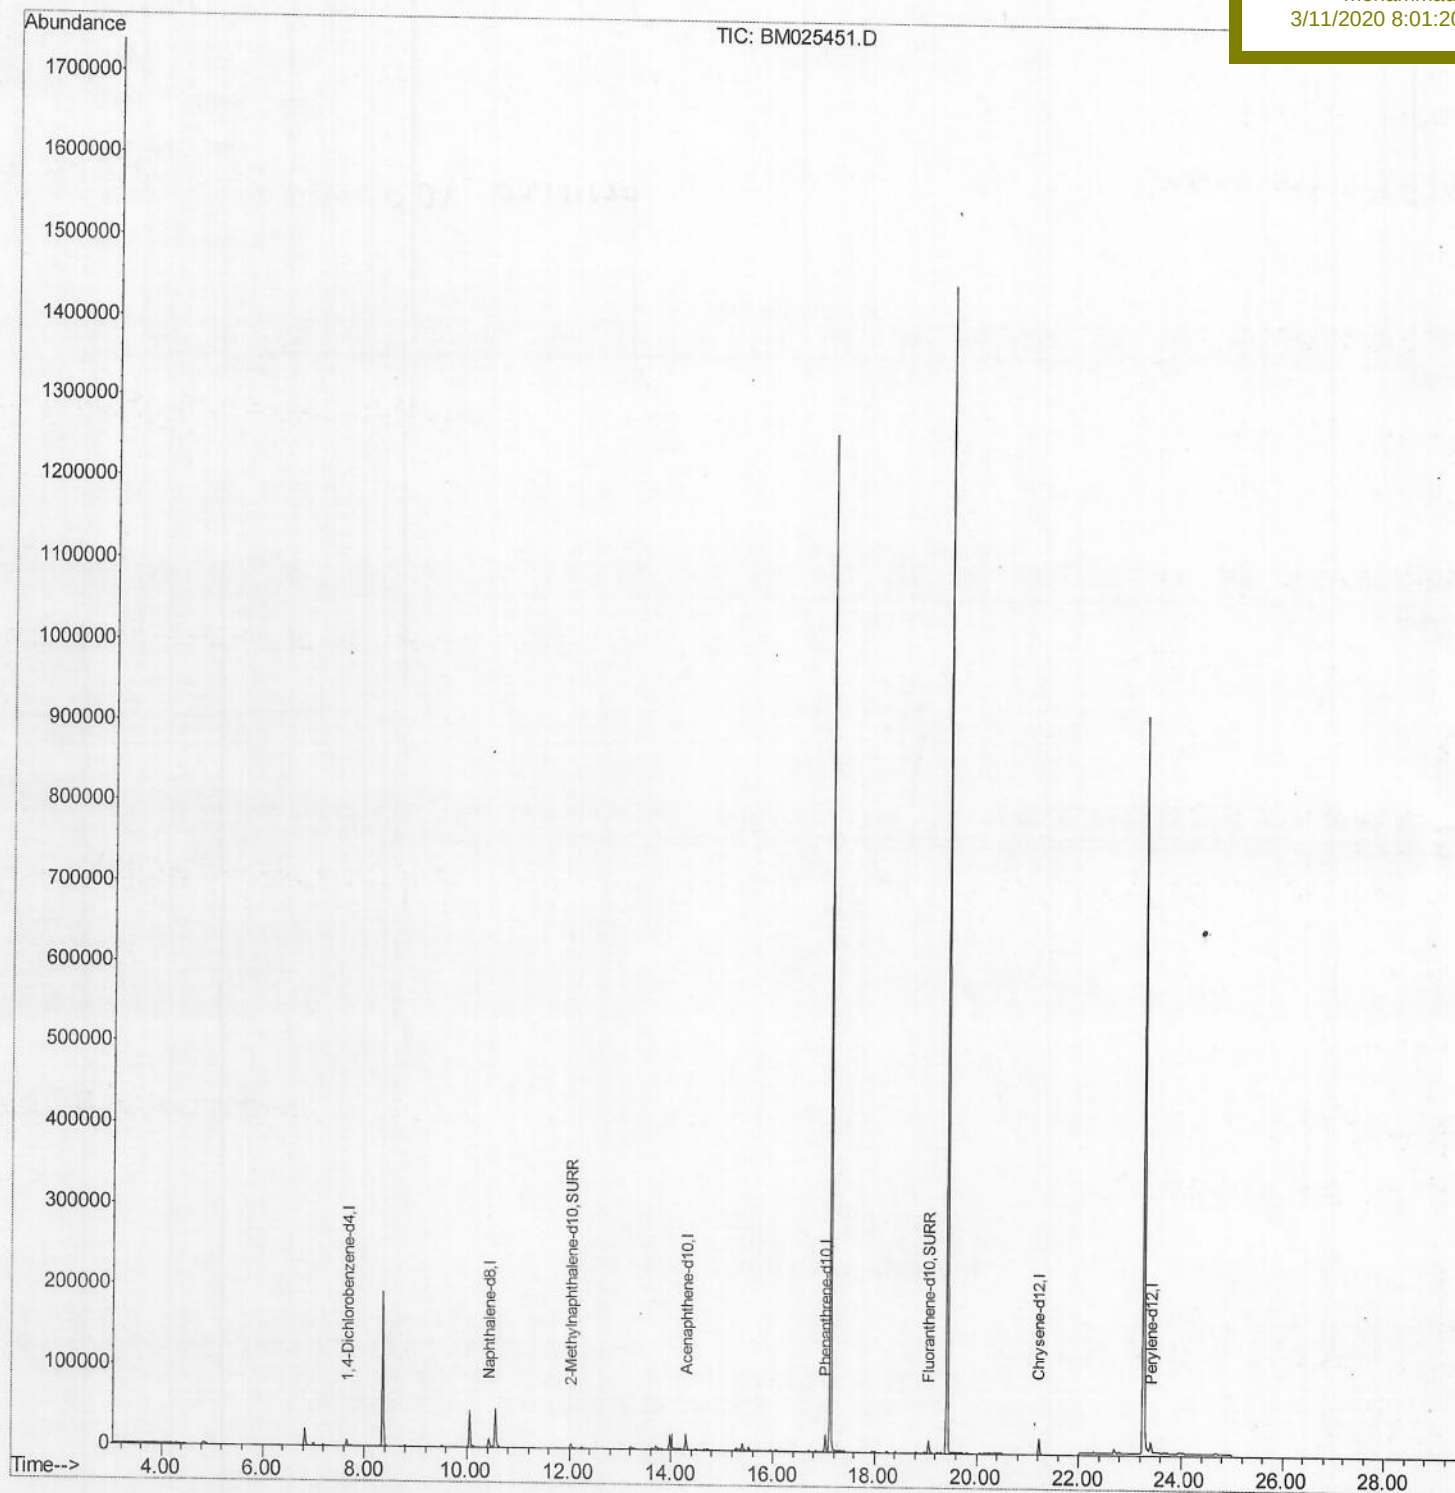

Quantitation Report (Qedit)

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM030920\

Data File : BM025451.D

Acq On : 10 Mar 2020 14:09

Operator : CG/JU

Sample : L1617-07

Misc :

ALS Vial : 45 Sample Multiplier: 1

Quant Time: Mar 10 14:49:25 2020

Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030920.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Mon Mar 09 13:32:56 2020

Response via : Initial Calibration

Instrument :

BNA_M

ClientSampleId :




DBDS1

Manual Integrations

APPROVED

mohammad

3/11/2020 8:01:20 AM

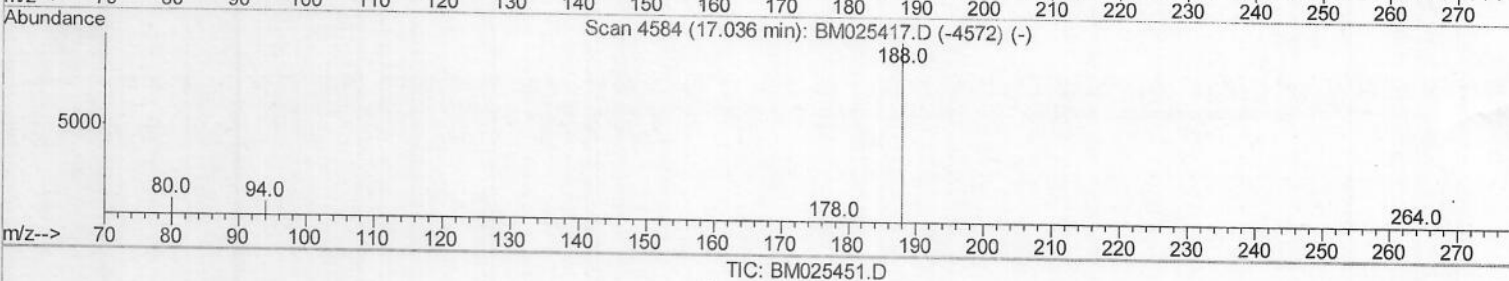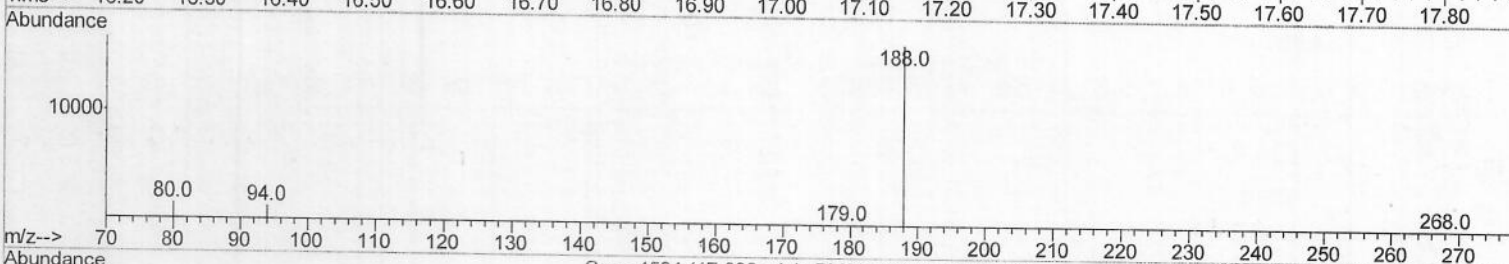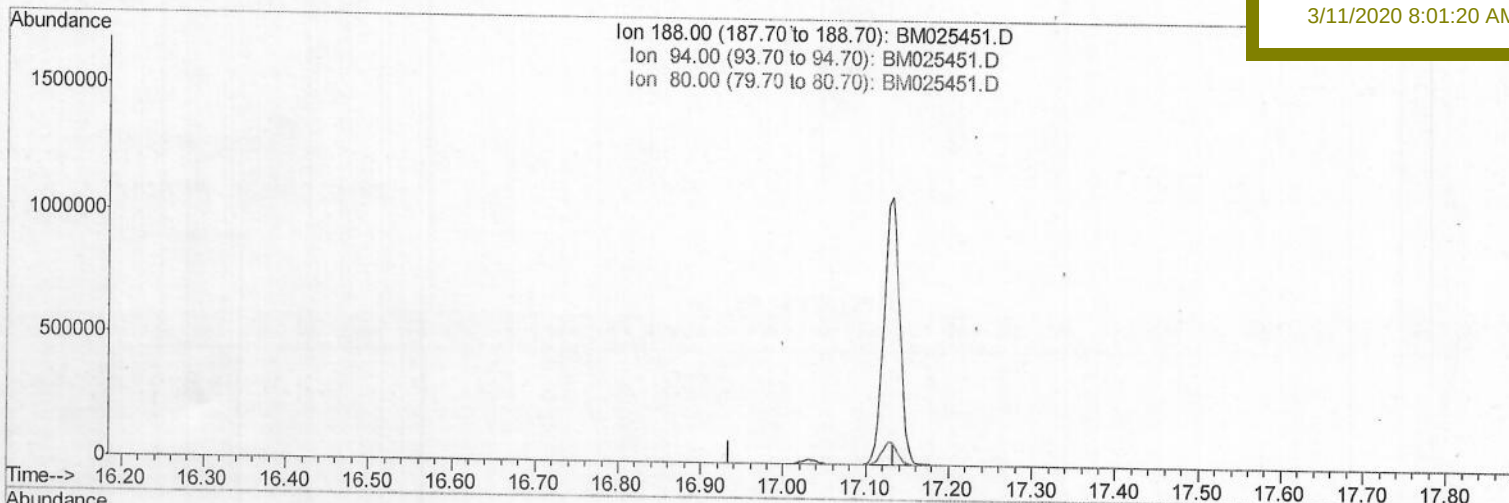

(10) Phenanthrene-d10 (I)

17.034min (-17.034) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	7.10	0.00#
80.00	8.70	0.00#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM030920\

Data File : BM025451.D

Acq On : 10 Mar 2020 14:09

Operator : CG/JU

Sample : L1617-07

Misc :

ALS Vial : 45 Sample Multiplier: 1

Quant Time: Mar 10 14:49:25 2020

Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030920.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Mon Mar 09 13:32:56 2020




Response via : Initial Calibration

Instrument :

BNA_M

ClientSampleId :

DBDS1

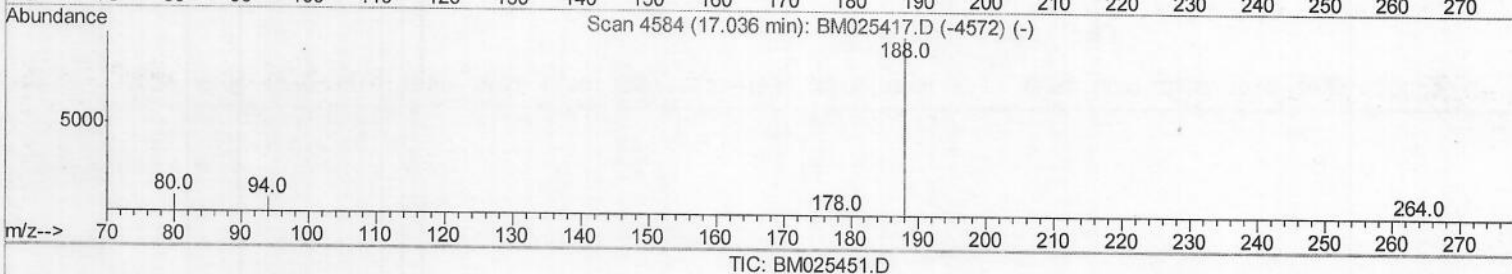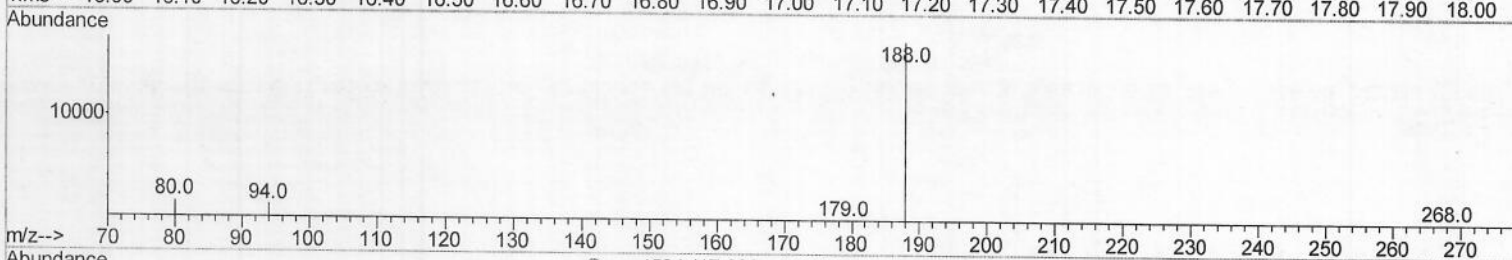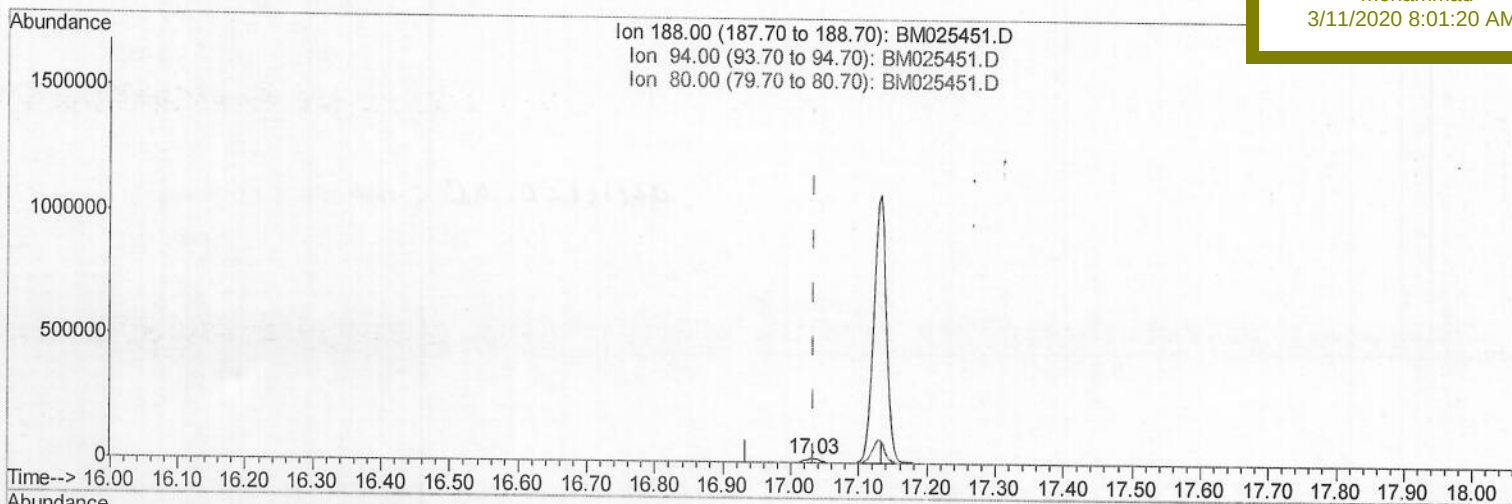Manual Integrations
APPROVEDmohammad
3/11/2020 8:01:20 AM

(10) Phenanthrene-d10 (I)

17.031min (-0.003) 0.40ng/ul m 350 03/11/20

response 24007

Ion	Exp%	Act%
188.00	100	100
94.00	7.10	7.70
80.00	8.70	9.37
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM030920\
Data File : BM025451.D
Acq On : 10 Mar 2020 14:09
Operator : CG/JU
Sample : L1617-07
Misc :
ALS Vial : 45 Sample Multiplier: 1

Quant Time: Mar 10 14:50:32 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 09 13:32:56 2020
Response via : Initial Calibration

Instrument :
BNA_M
ClientSampleId :
DBDS1

Manual Integrations
APPROVED

mohammad
3/11/2020 8:01:20 AM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.66	152	3234	0.40	ng/ul	0.00
2) Naphthalene-d8	10.43	136	14034	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.29	164	10628	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.03	188	24007m	0.40	ng/ul	0.00
16) Chrysene-d12	21.22	240	17259	0.40	ng/ul	0.00
20) Perylene-d12	23.40	264	16214	0.40	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	12.03	152	6691	0.26	ng/ul	0.00
14) Fluoranthene-d10	19.06	212	16285	0.25	ng/ul	0.00

Target Compounds	Ovalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

SV 03/11/20