

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM030920\

Data File : BM025455.D

Acq On : 10 Mar 2020 16:35

Operator : CG/JU

Sample : L1617-06

Misc :

ALS Vial : 49 Sample Multiplier: 1

Quant Time: Mar 10 17:08:13 2020

Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030920.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Mon Mar 09 13:32:56 2020

Response via : Initial Calibration

Instrument :

BNA_M

ClientSampleId :


DBDS0

Manual Integrations

APPROVED

mohammad

3/11/2020 8:01:49 AM

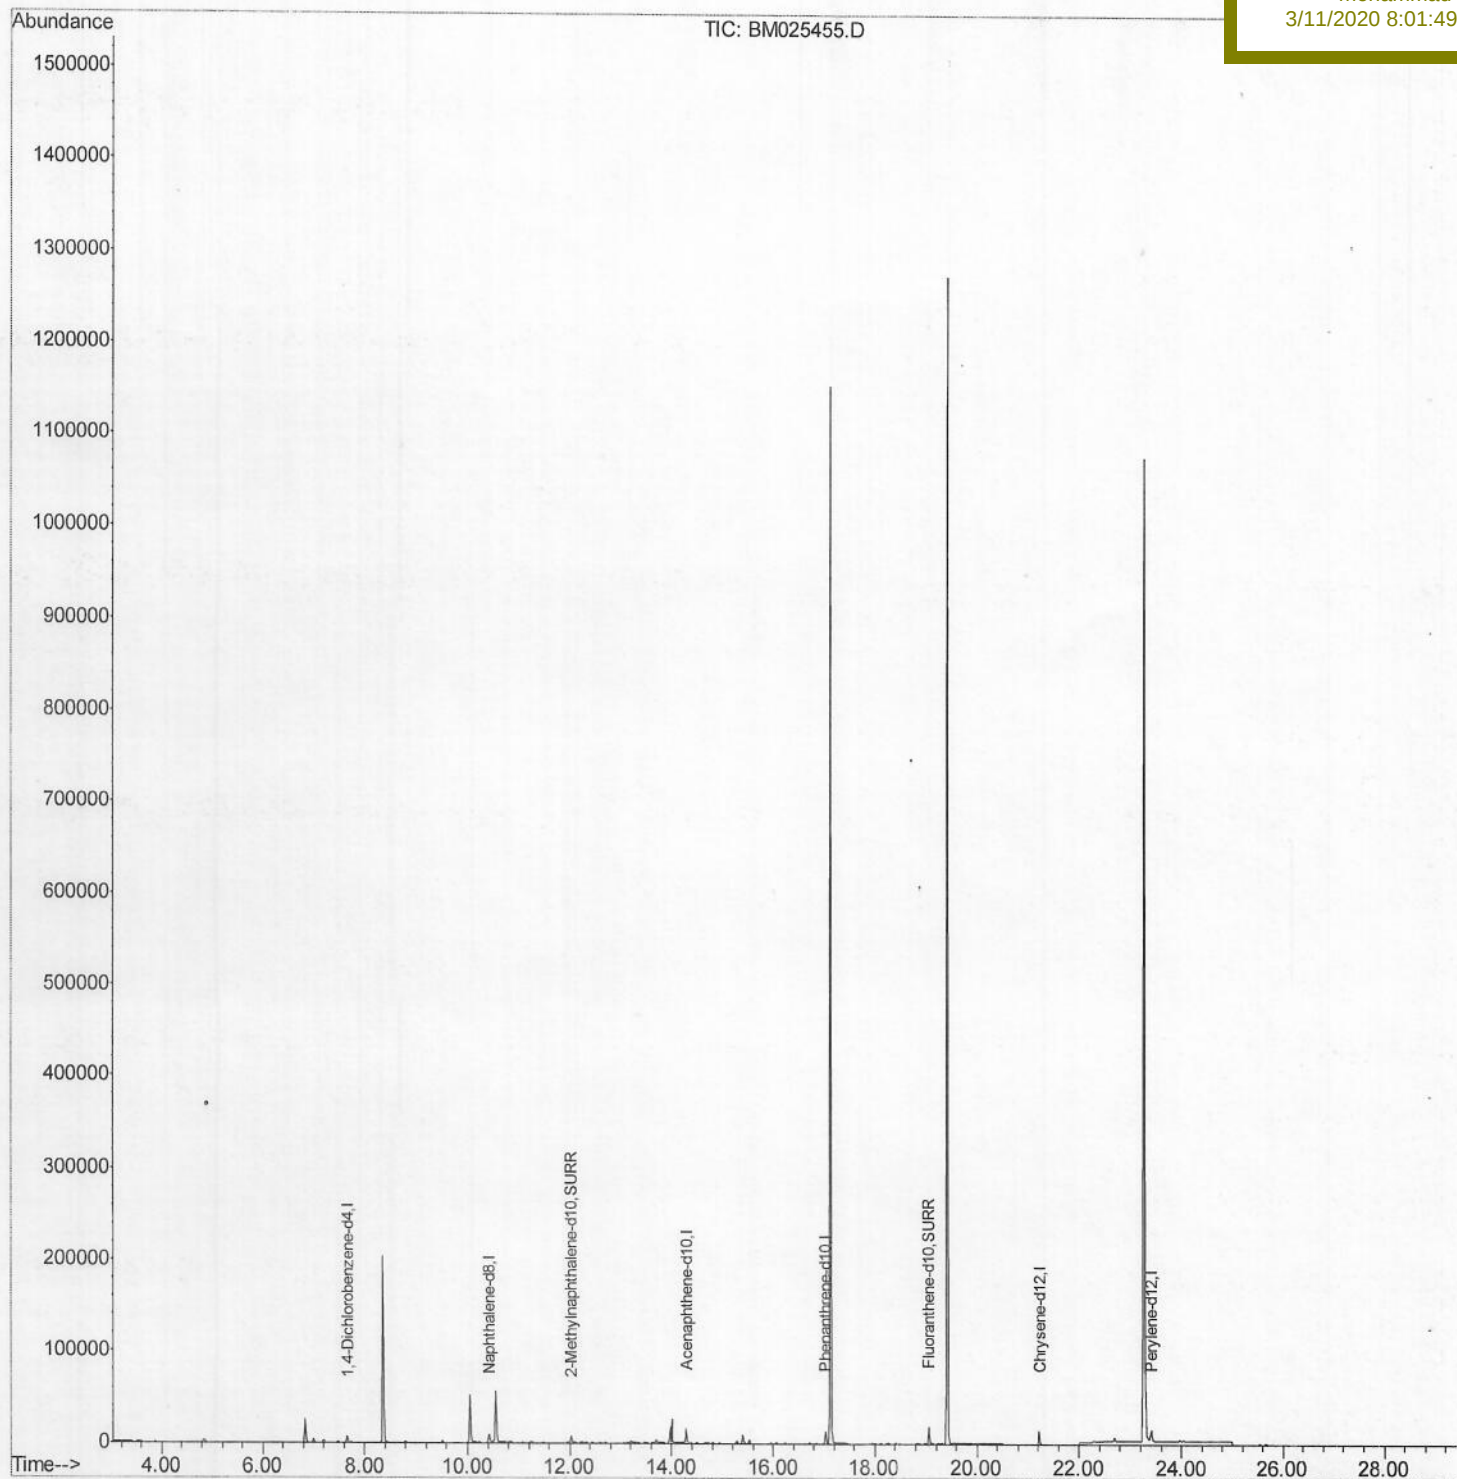

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM030920\

Data File : BM025455.D

Acq On : 10 Mar 2020 16:35

Operator : CG/JU

Sample : L1617-06

Misc :

ALS Vial : 49 Sample Multiplier: 1

Quant Time: Mar 10 17:07:04 2020

Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030920.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Mon Mar 09 13:32:56 2020

Response via : Initial Calibration

Instrument :

BNA_M

ClientSampleId :




DBDS0

Manual Integrations

APPROVED

mohammad

3/11/2020 8:01:49 AM

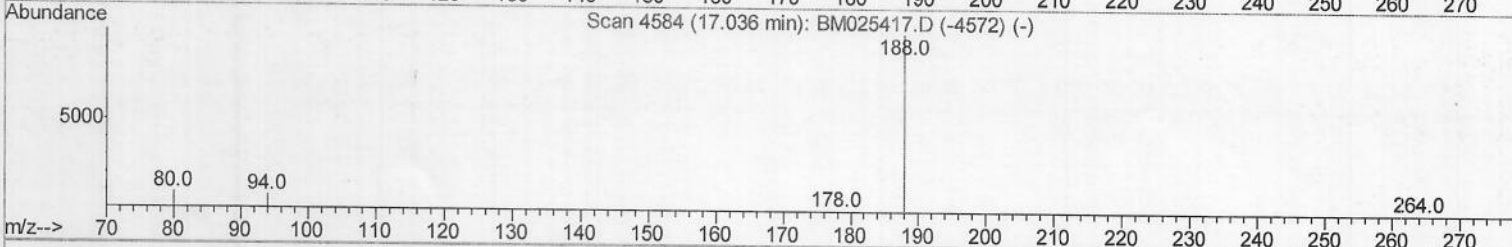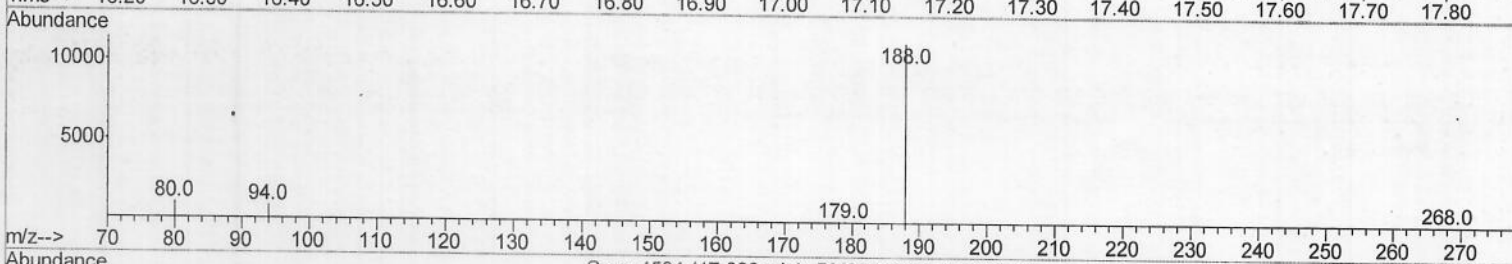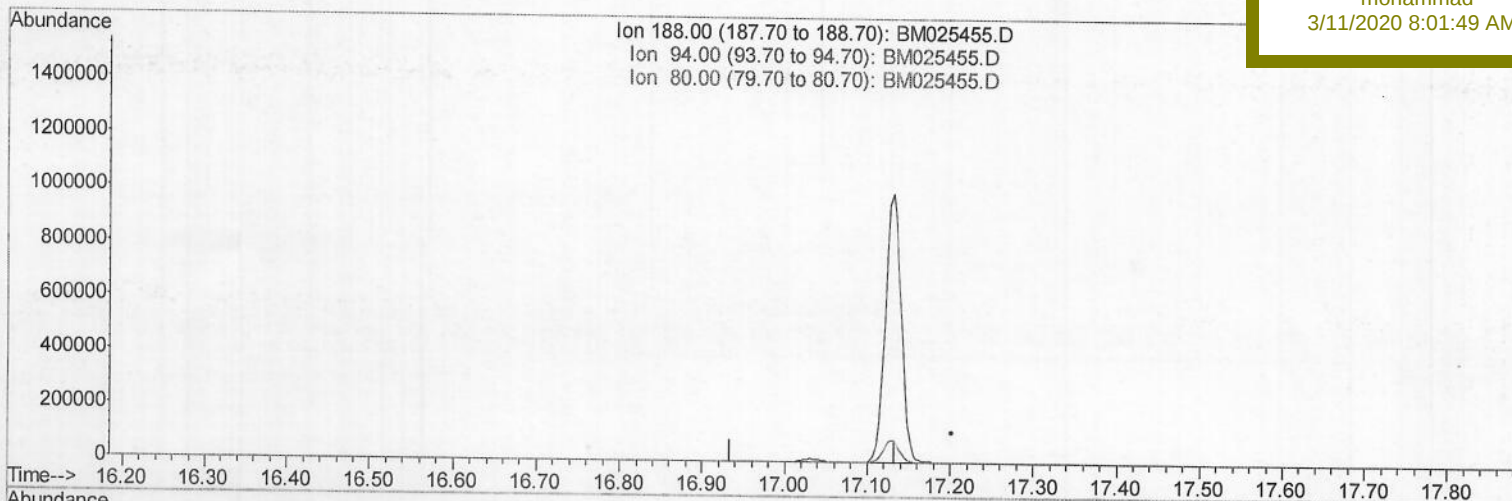

(10) Phenanthrene-d10 (I)

17.034min (-17.034) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	7.10	0.00#
80.00	8.70	0.00#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM030920\

Data File : BM025455.D

Acq On : 10 Mar 2020 16:35

Operator : CG/JU

Sample : L1617-06

Misc :

ALS Vial : 49 Sample Multiplier: 1

Quant Time: Mar 10 17:07:04 2020

Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030920.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Mon Mar 09 13:32:56 2020




Response via : Initial Calibration

Instrument :

BNA_M

ClientSampleId :

DBDS0

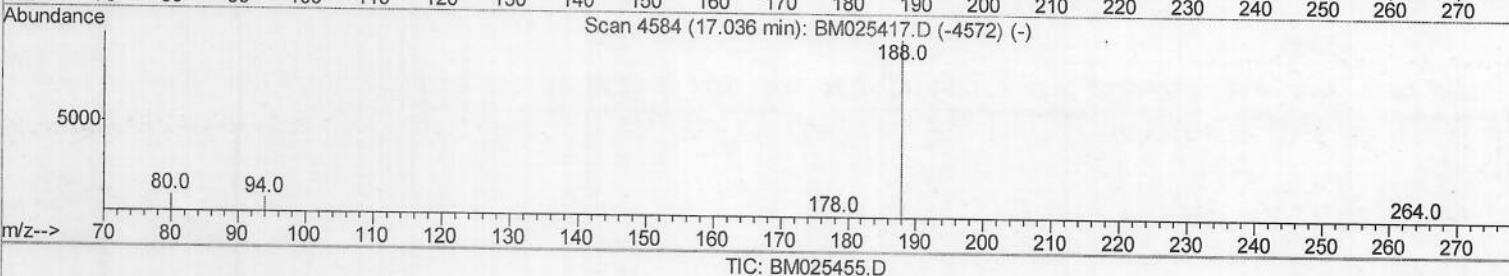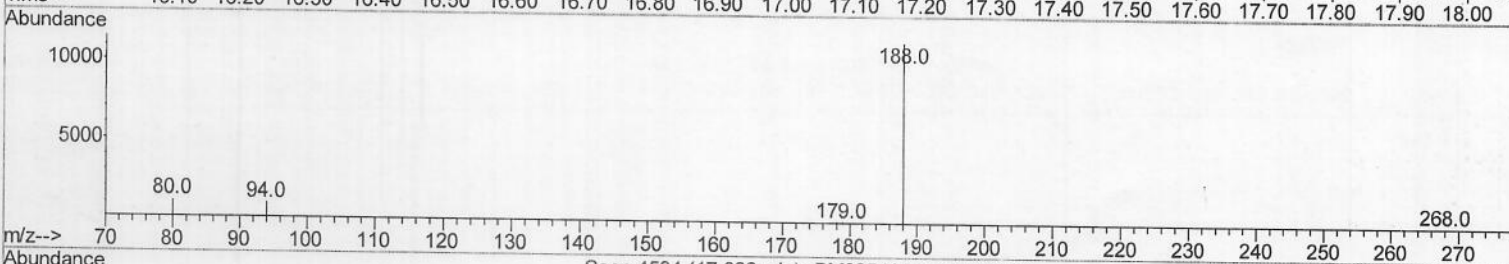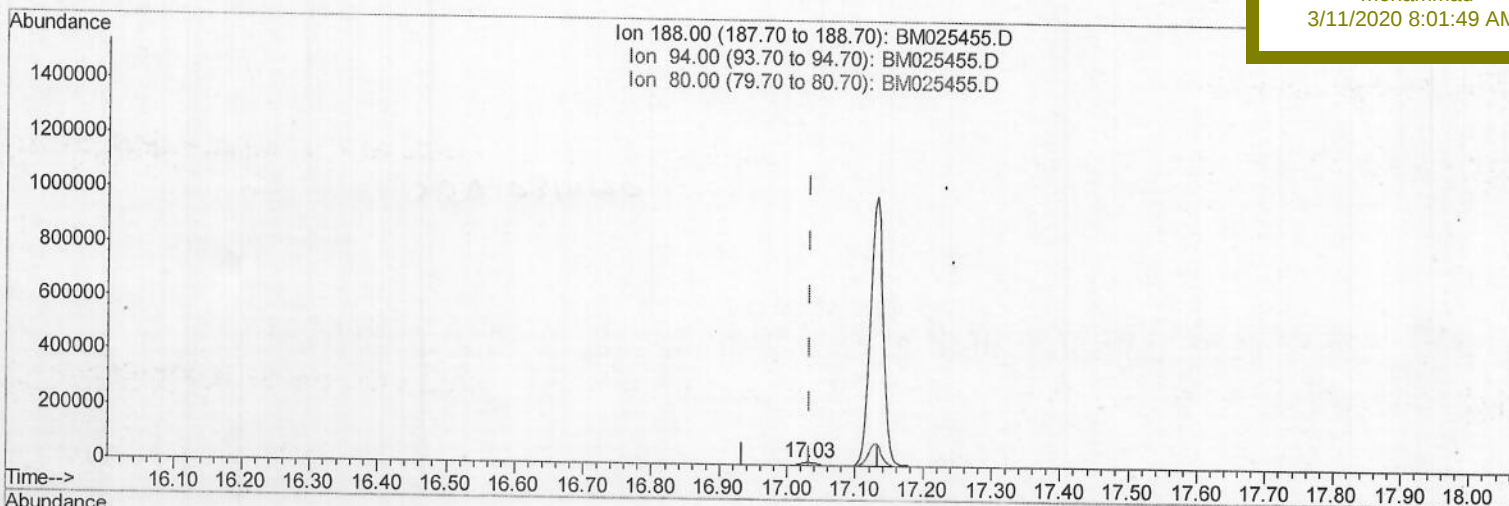Manual Integrations
APPROVEDmohammad
3/11/2020 8:01:49 AM

(10) Phenanthrene-d10 (I)

17.030min (-0.004) 0.40ng/ul m > Ju 03/11/20

response 16142

Ion	Exp%	Act%
188.00	100	100
94.00	7.10	8.52#
80.00	8.70	9.44
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM030920\
Data File : BM025455.D
Acq On : 10 Mar 2020 16:35
Operator : CG/JU
Sample : L1617-06
Misc :
ALS Vial : 49 Sample Multiplier: 1

Quant Time: Mar 10 17:08:13 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 09 13:32:56 2020
Response via : Initial Calibration

Instrument :
BNA_M
Client Sampled :
DBDS0

Manual Integrations
APPROVED

mohammad
3/11/2020 8:01:49 AM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.66	152	3043	0.40	ng/ul	0.00
2) Naphthalene-d8	10.43	136	12264	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.29	164	8296	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.03	188	16142m	0.40	ng/ul	0.00
16) Chrysene-d12	21.22	240	13148	0.40	ng/ul	0.00
20) Perylene-d12	23.41	264	15058	0.40	ng/ul	0.00

System Monitoring Compounds

4) 2-Methylnaphthalene-d10	12.02	152	10017	0.45	ng/ul	0.00
14) Fluoranthene-d10	19.06	212	19799	0.45	ng/ul	0.00

Target Compounds

Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed