


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM030920\
Data File : BM025472.D
Acq On : 11 Mar 2020 02:56
Operator : CG/JU
Sample : L1617-08
Misc :
ALS Vial : 66 Sample Multiplier: 1

Quant Time: Mar 11 03:48:34 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 10 23:48:01 2020
Response via : Initial Calibration

Instrument :
BNA_M
ClientSampleId :
DBDS2

Manual Integrations
APPROVED

mohammad
3/11/2020 8:02:21 AM

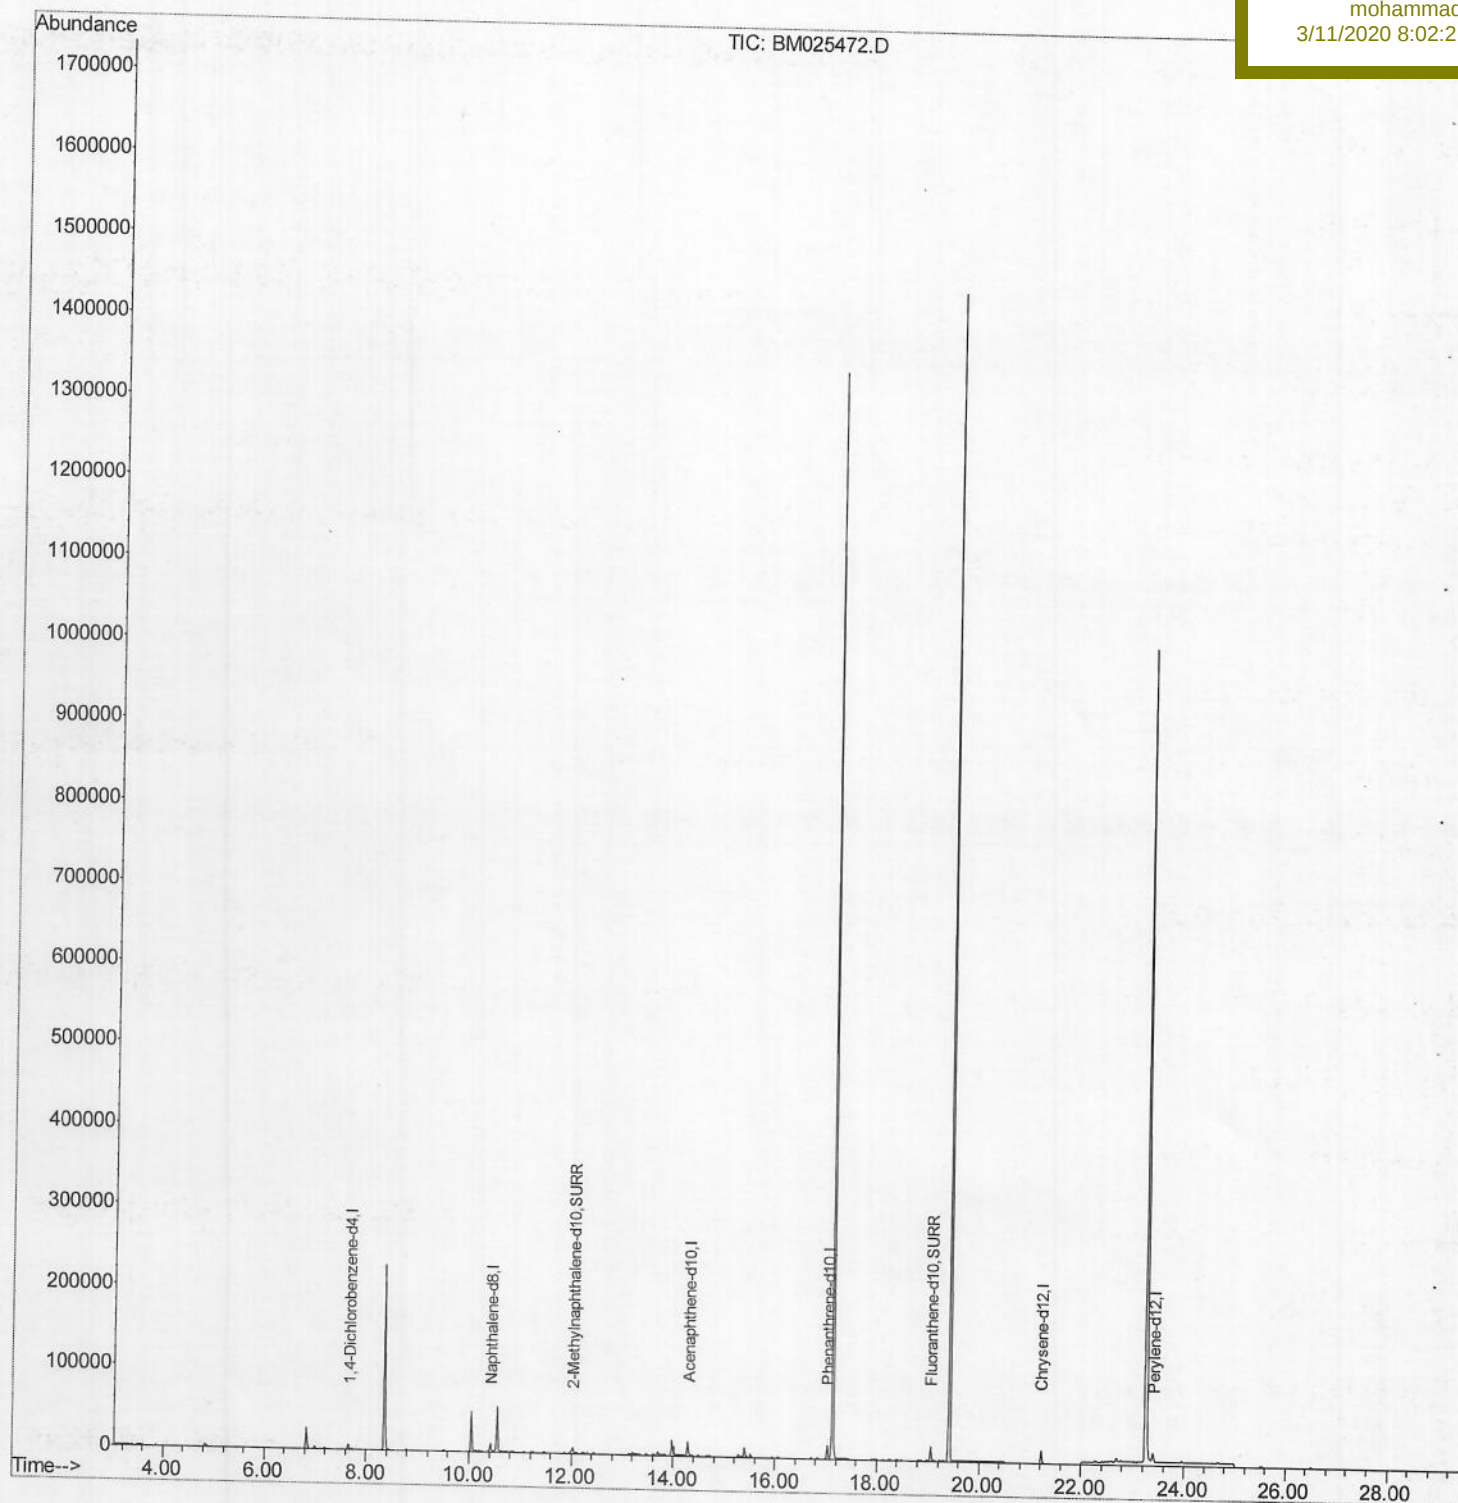

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM030920\
 Data File : BM025472.D
 Acq On : 11 Mar 2020 02:56
 Operator : CG/JU
 Sample : L1617-08
 Misc :
 ALS Vial : 66 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBDS2

Manual Integrations
 APPROVED

mohammad
 3/11/2020 8:02:21 AM

Quant Time: Mar 11 03:47:10 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030920.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Mar 10 23:48:01 2020
 Response via : Initial Calibration

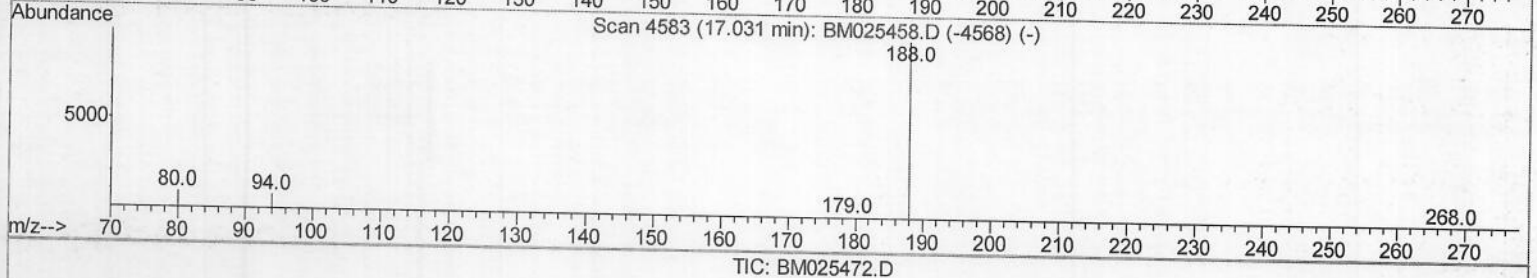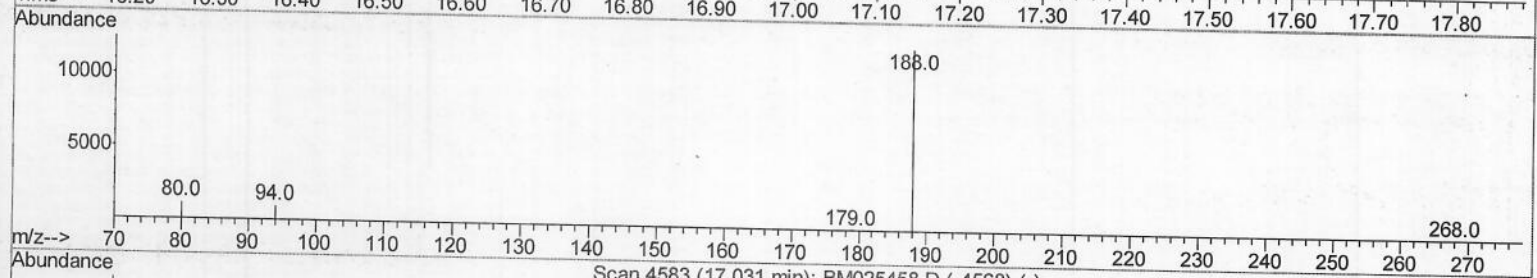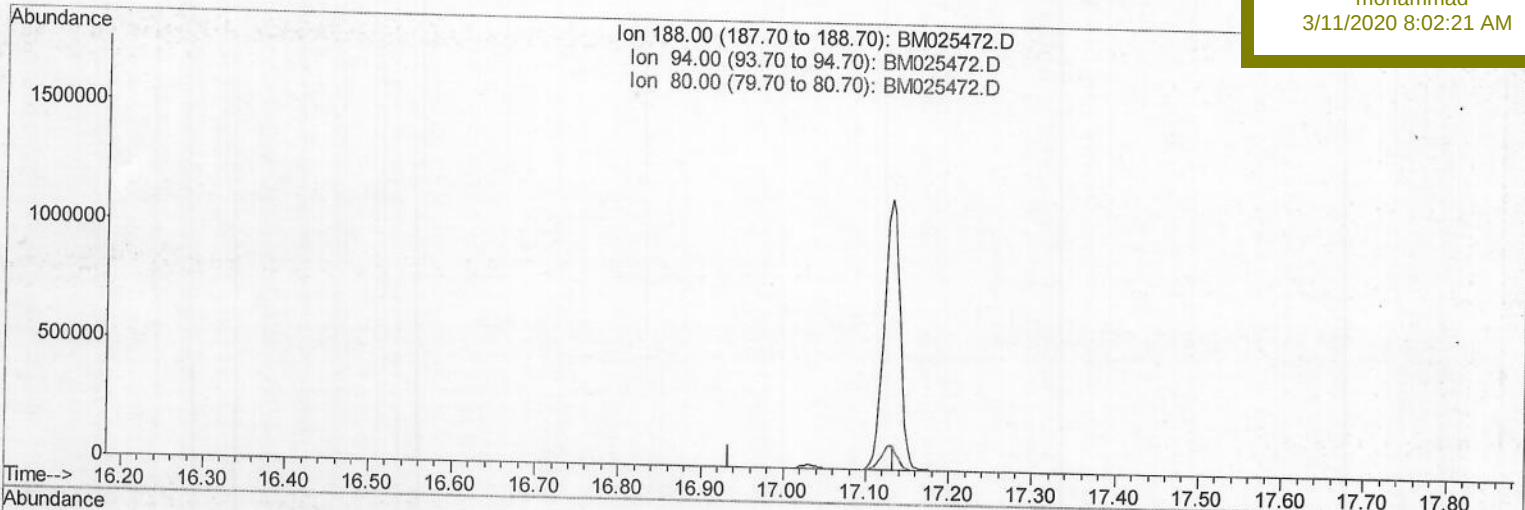

TIC: BM025472.D

(10) Phenanthrene-d10 (I)

17.034min (-17.034) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	7.10	0.00#
80.00	8.70	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM030920\
 Data File : BM025472.D
 Acq On : 11 Mar 2020 02:56
 Operator : CG/JU
 Sample : L1617-08
 Misc :
 ALS Vial : 66 Sample Multiplier: 1

Instrument :

BNA_M

ClientSampleId :

DBDS2




Manual Integrations

APPROVED

mohammad

3/11/2020 8:02:21 AM

Quant Time: Mar 11 03:47:10 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030920.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Mar 10 23:48:01 2020
 Response via : Initial Calibration

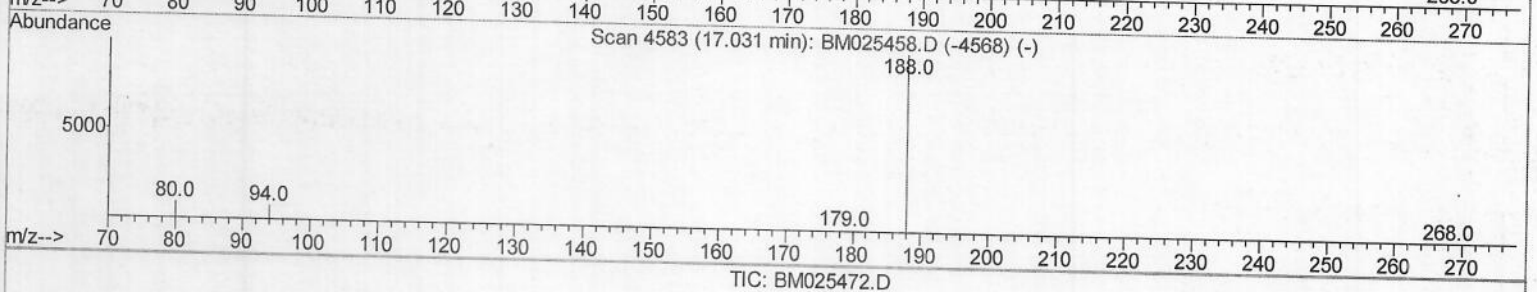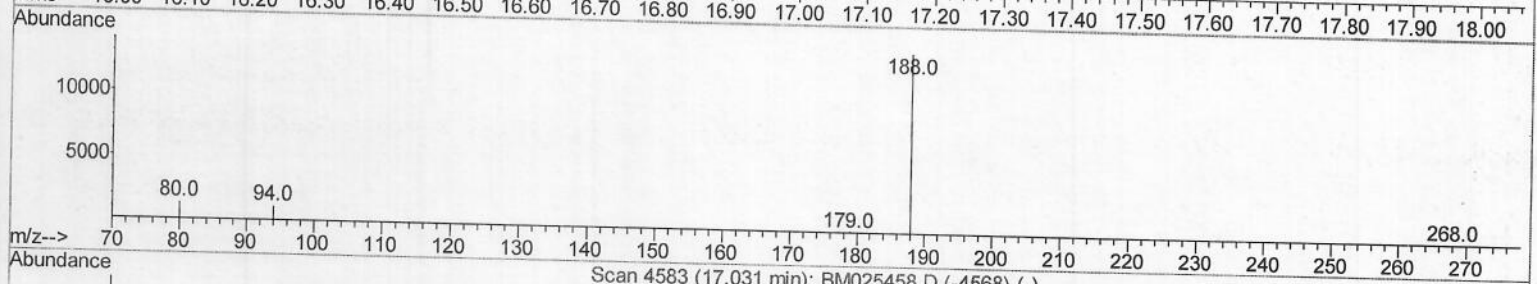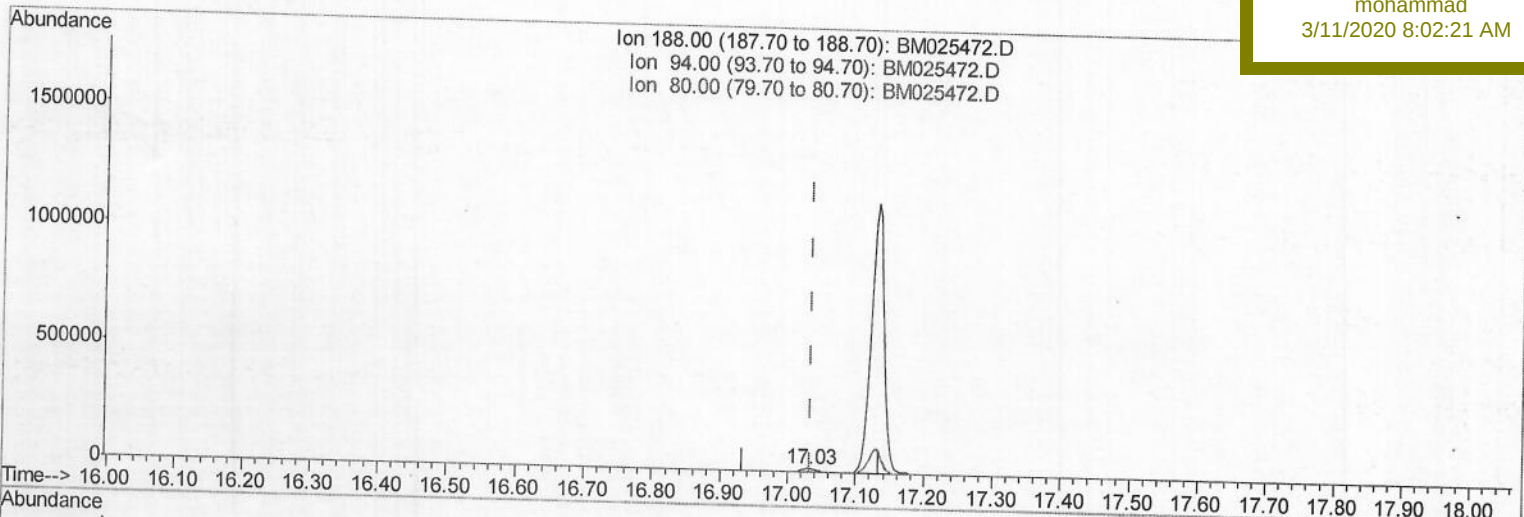

(10) Phenanthrene-d10 (I)

17.032min (-0.002) 0.40ng/ul m > JV 03/11/20

response 19200

Ion	Exp%	Act%
188.00	100	100
94.00	7.10	8.12
80.00	8.70	9.27
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM030920\
 Data File : BM025472.D
 Acq On : 11 Mar 2020 02:56
 Operator : CG/JU
 Sample : L1617-08
 Misc :
 ALS Vial : 66 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBDS2

Manual Integrations
 APPROVED

mohammad
 3/11/2020 8:02:21 AM

Quant Time: Mar 11 03:48:34 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030920.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Mar 10 23:48:01 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Dichlorobenzene-d4	7.66	152	2972	0.40	ng/ul	0.00
2) Naphthalene-d8	10.43	136	12885	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.29	164	9370	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.03	188	19200m	0.40	ng/ul	0.00
16) Chrysene-d12	21.22	240	13564	0.40	ng/ul	0.00
20) Perylene-d12	23.40	264	14572	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.02	152	9435	0.41	ng/ul	0.00
14) Fluoranthene-d10	19.06	212	20304	0.38	ng/ul	0.00

Target Compounds

Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed