

Quantitation Report (QT Reviewed)


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM030920\
Data File : BM025481.D
Acq On : 11 Mar 2020 09:00
Operator : CG/JU
Sample : PB127171BL
Misc :
ALS Vial : 74 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK71

Manual Integrations
APPROVED

mohammad
3/13/2020 8:48:23 AM

Quant Time: Mar 11 13:42:22 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 11 07:15:41 2020
Response via : Initial Calibration

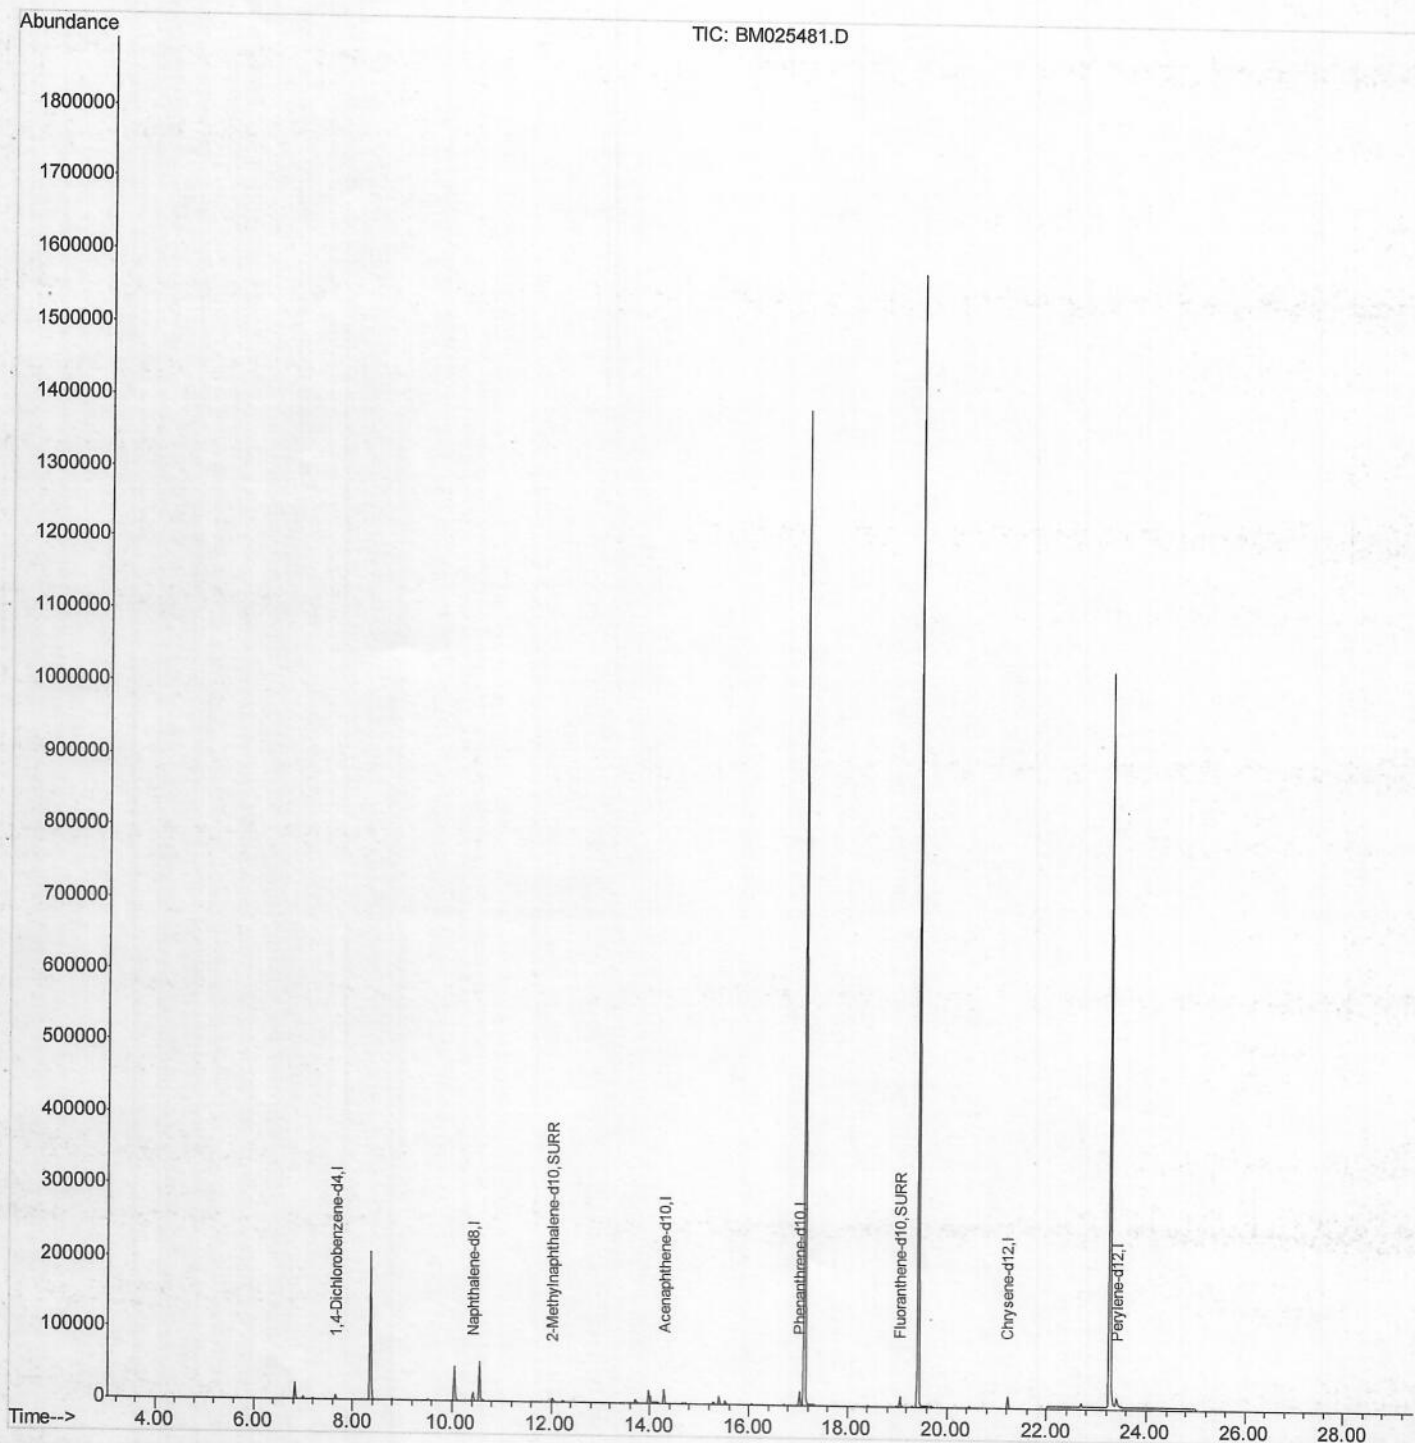

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM030920\
 Data File : BM025481.D
 Acq On : 11 Mar 2020 09:00
 Operator : CG/JU
 Sample : PB127171BL
 Misc :
 ALS Vial : 74 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK71

Manual Integrations
 APPROVED

mohammad
 3/13/2020 8:48:23 AM

Quant Time: Mar 11 13:41:12 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030920.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 11 07:15:41 2020
 Response via : Initial Calibration

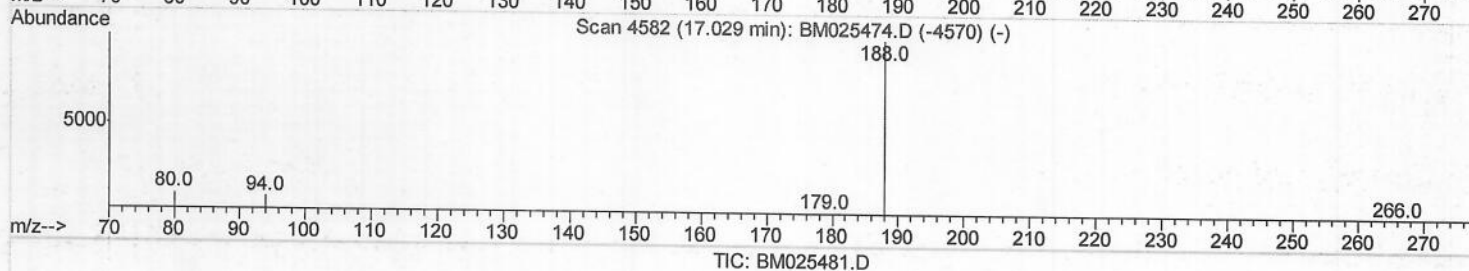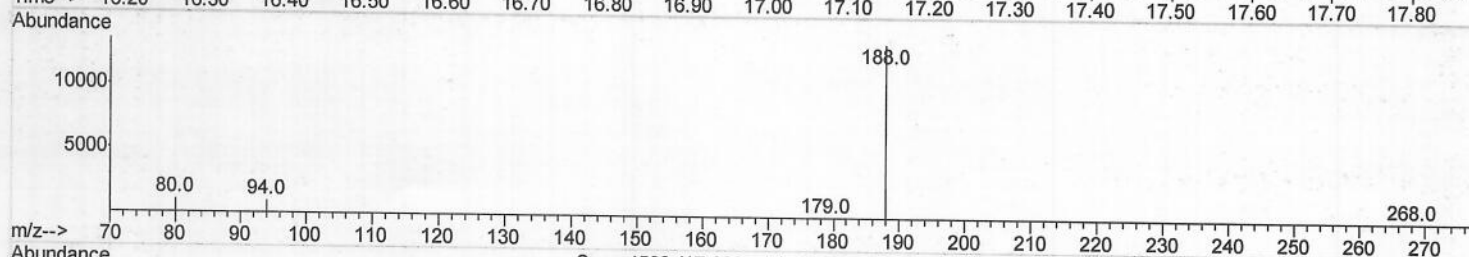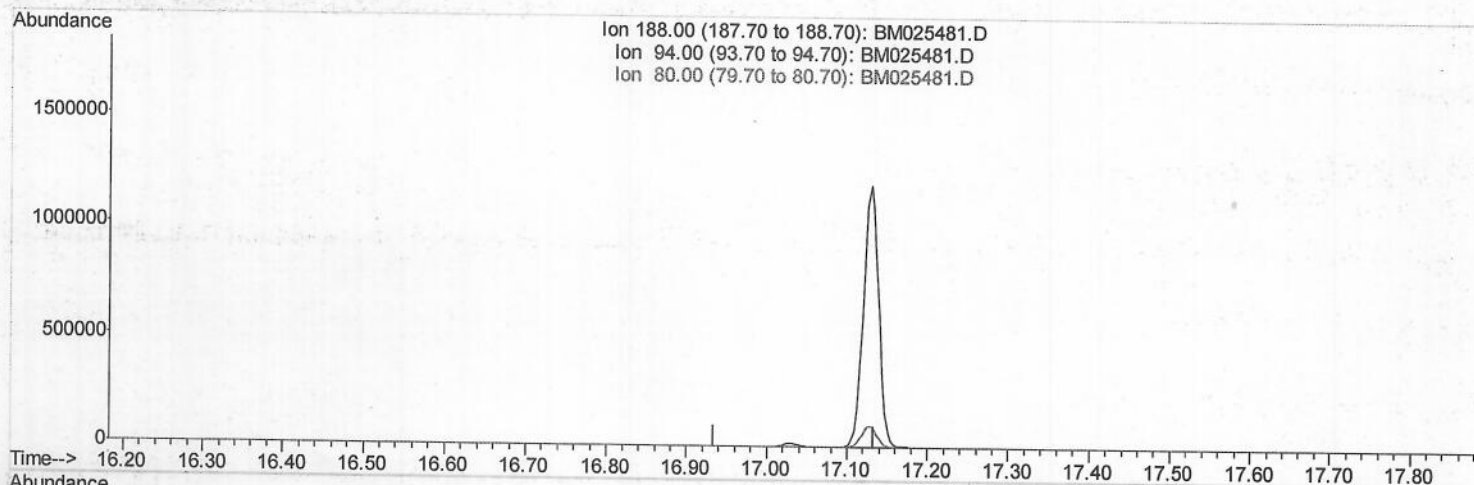

(10) Phenanthrene-d10 (I)

17.034min (-17.034) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	7.10	0.00#
80.00	8.70	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM030920\
 Data File : BM025481.D
 Acq On : 11 Mar 2020 09:00
 Operator : CG/JU
 Sample : PB127171BL
 Misc :
 ALS Vial : 74 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK71

Manual Integrations
 APPROVED

mohammad
 3/13/2020 8:48:23 AM

Quant Time: Mar 11 13:41:12 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030920.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 11 07:15:41 2020
 Response via : Initial Calibration

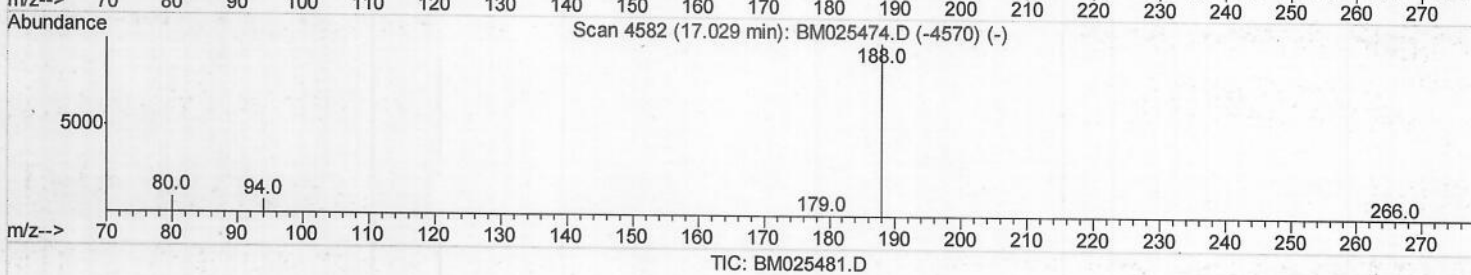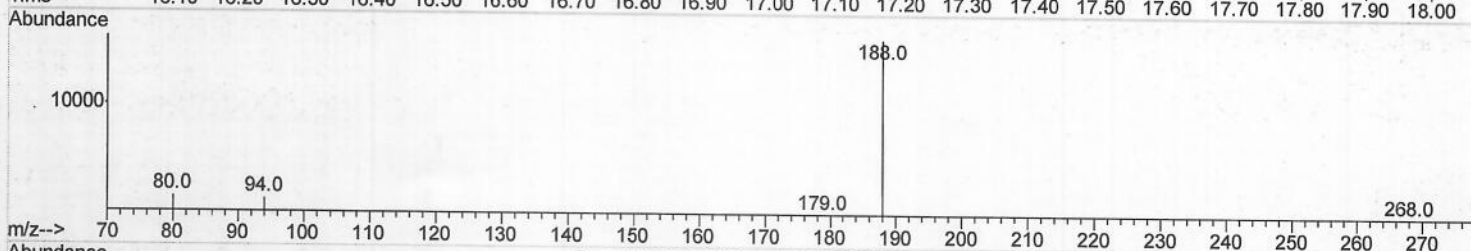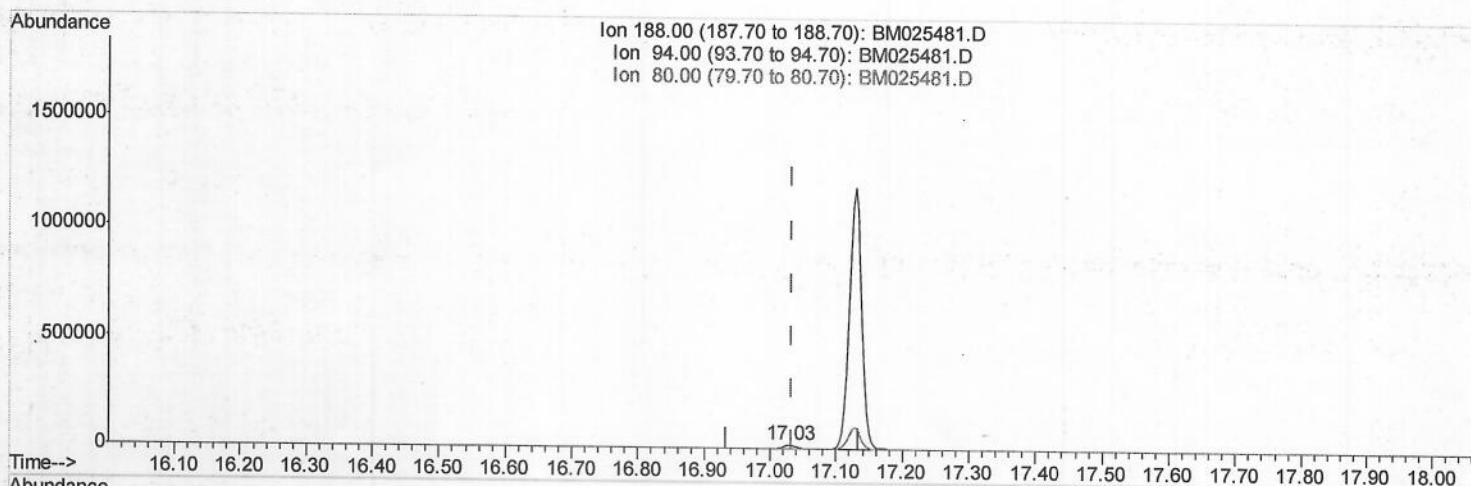

(10) Phenanthrene-d10 (I)

17.029min (-0.005) 0.40ng/ul m > 50 03/16/20

response 22092

Ion	Exp%	Act%
188.00	100	100
94.00	7.10	7.87
80.00	8.70	9.34
0.00	0.00	0.00

Quantitation Report (QT Reviewed)

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM030920\
 Data File : BM025481.D
 Acq On : 11 Mar 2020 09:00
 Operator : CG/JU
 Sample : PB127171BL
 Misc :
 ALS Vial : 74 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK71

Manual Integrations
 APPROVED

mohammad
 3/13/2020 8:48:23 AM

Quant Time: Mar 11 13:42:22 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030920.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 11 07:15:41 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.66	152	3365	0.40	ng/ul	0.00
2) Naphthalene-d8	10.43	136	14171	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.29	164	10079	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.03	188	22092m)	0.40	ng/ul	0.00
16) Chrysene-d12	21.22	240	14924	0.40	ng/ul	0.00
20) Perylene-d12	23.40	264	15142	0.40	ng/ul	0.00

JV 03/16/20

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	12.02	152	7093	0.28	ng/ul	0.00
14) Fluoranthene-d10	19.06	212	16891	0.28	ng/ul	0.00

Target Compounds

Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed