


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM030920\
Data File : BM025506.D
Acq On : 12 Mar 2020 00:10
Operator : CG/JU
Sample : PB127316BL
Misc :
ALS Vial : 99 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK16

Manual Integrations
APPROVED

mohammad
3/13/2020 8:50:03 AM

Quant Time: Mar 12 02:40:47 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 12 02:03:23 2020
Response via : Initial Calibration

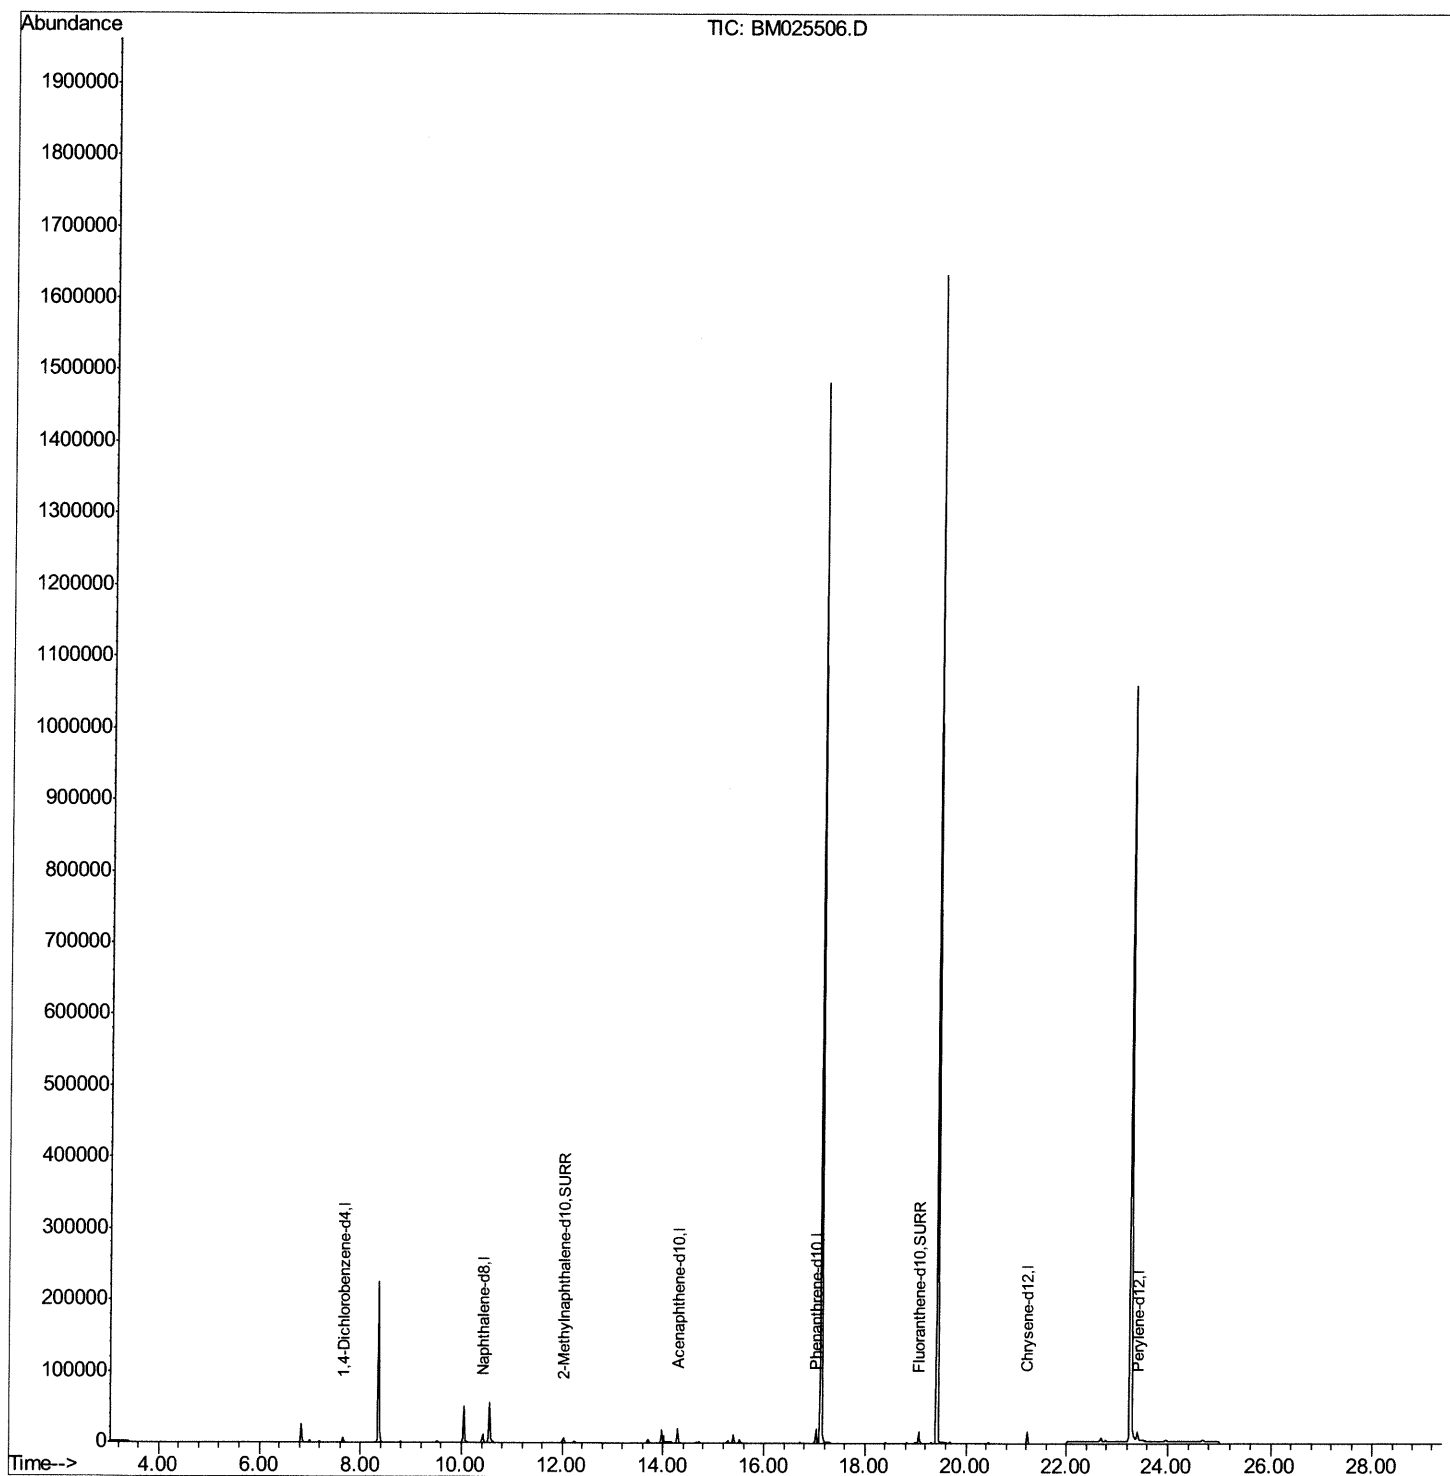

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM030920\
Data File : BM025506.D
Acq On : 12 Mar 2020 00:10
Operator : CG/JU
Sample : PB127316BL
Misc :
ALS Vial : 99 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK16

Manual Integrations
APPROVED

mohammad
3/13/2020 8:50:03 AM

Quant Time: Mar 12 02:39:51 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 12 02:03:23 2020
Response via : Initial Calibration

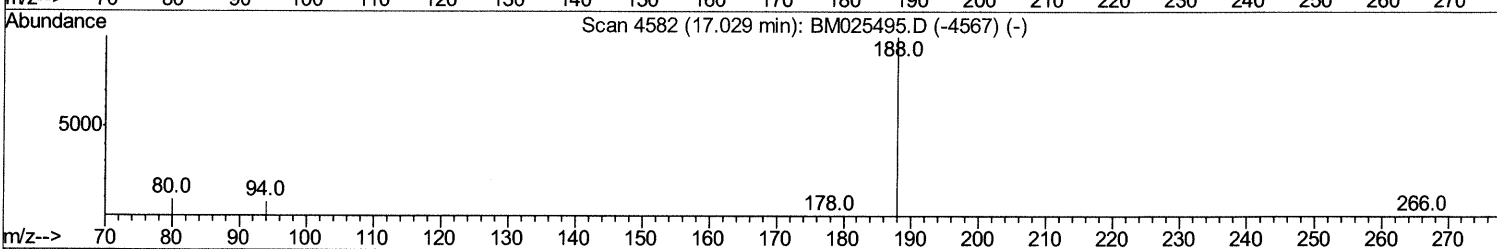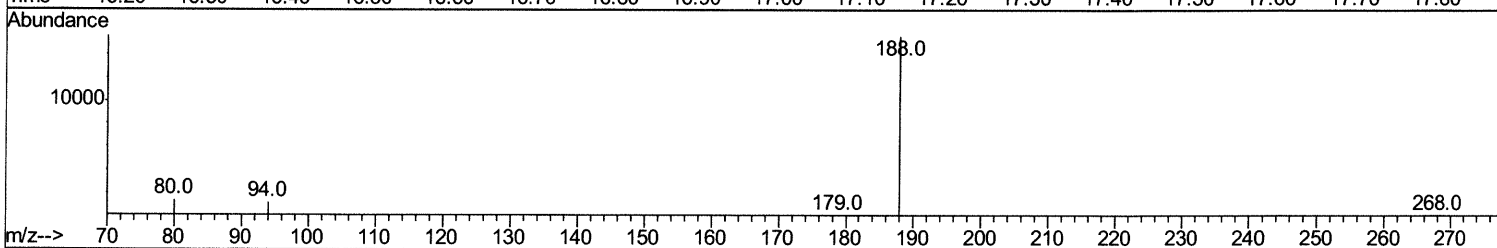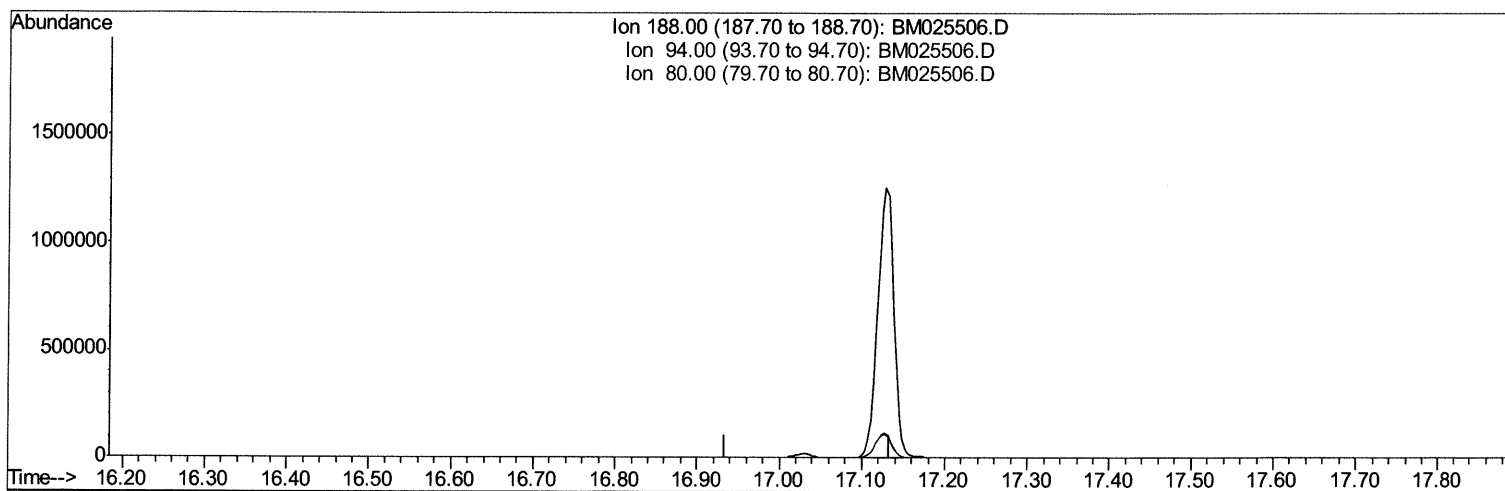

TIC: BM025506.D

(10) Phenanthrene-d10 (I)

17.034min (-17.034) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	7.10	0.00#
80.00	8.70	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM030920\
 Data File : BM025506.D
 Acq On : 12 Mar 2020 00:10
 Operator : CG/JU
 Sample : PB127316BL
 Misc :
 ALS Vial : 99 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK16

Manual Integrations
 APPROVED

mohammad
 3/13/2020 8:50:03 AM

Quant Time: Mar 12 02:39:51 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030920.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 12 02:03:23 2020
 Response via : Initial Calibration

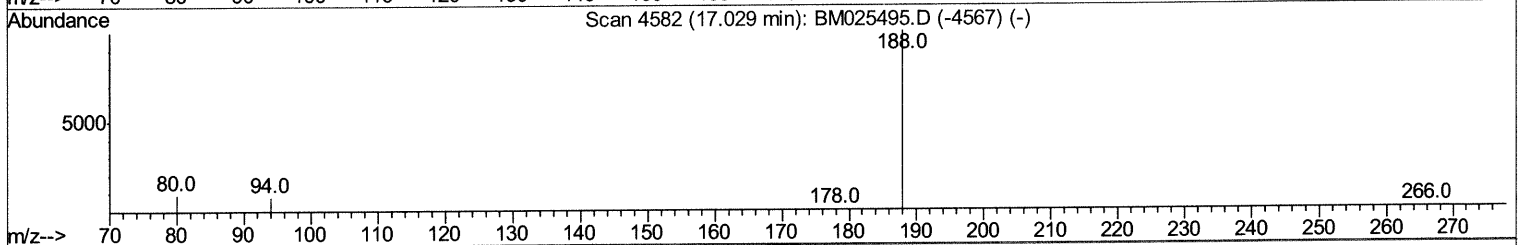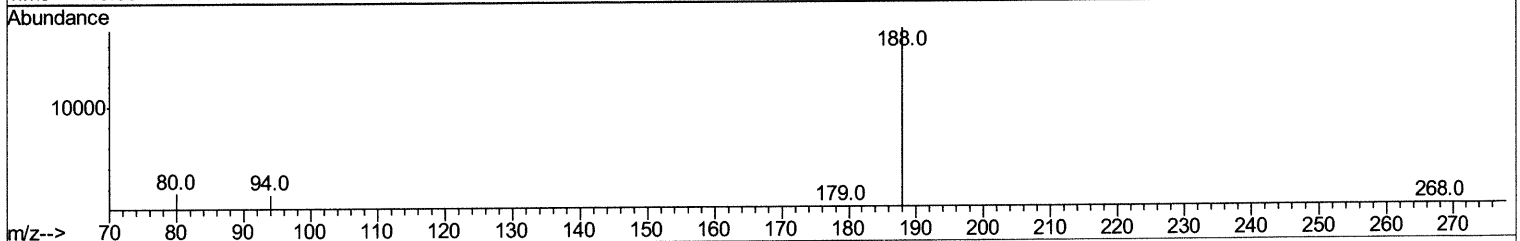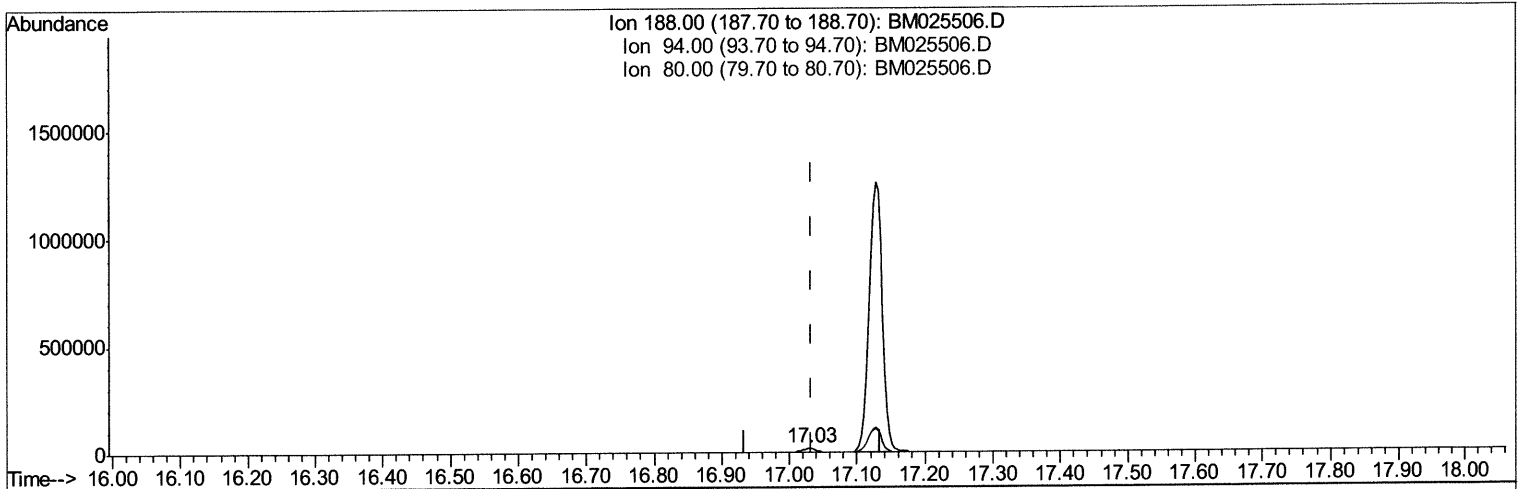

TIC: BM025506.D

(10) Phenanthrene-d10 (I)

17.030min (-0.004) 0.40ng/ul m *Ja 03/12/20*

response 24195

Ion	Exp%	Act%
188.00	100	100
94.00	7.10	7.84
80.00	8.70	8.86
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM030920\
 Data File : BM025506.D
 Acq On : 12 Mar 2020 00:10
 Operator : CG/JU
 Sample : PB127316BL
 Misc :
 ALS Vial : 99 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK16

Manual Integrations
 APPROVED

mohammad
 3/13/2020 8:50:03 AM

Quant Time: Mar 12 02:40:47 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030920.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 12 02:03:23 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.66	152	3598	0.40	ng/ul	0.00
2) Naphthalene-d8	10.42	136	15401	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.28	164	11218	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.03	188	24195m >	0.40	ng/ul >	0.00
16) Chrysene-d12	21.22	240	15833	0.40	ng/ul	0.00
20) Perylene-d12	23.40	264	16919	0.40	ng/ul	0.00

54 6/12/20

System Monitoring Compounds

4) 2-Methylnaphthalene-d10	12.02	152	7792	0.28	ng/ul	0.00
14) Fluoranthene-d10	19.06	212	18386	0.28	ng/ul	0.00

Target Compounds Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed