

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM030920\
 Data File : BM025420.D
 Acq On : 09 Mar 2020 18:49
 Operator : CG/JU
 Sample : L1612-10
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBDL2

Manual Integrations
 APPROVED

mohammad
 3/10/2020 7:59:05 AM

Quant Time: Mar 09 19:22:04 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030920.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Mar 09 13:32:56 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.67	152	3328	0.40	ng/ul	0.00
2) Naphthalene-d8	10.43	136	14480	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.29	164	10647	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.04	188	23352m	0.40	ng/ul	0.00
16) Chrysene-d12	21.22	240	16230	0.40	ng/ul	0.00
20) Perylene-d12	23.41	264	15310	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.03	152	8622	0.33	ng/ul	0.00
14) Fluoranthene-d10	19.06	212	19999	0.31	ng/ul	0.00
Target Compounds						
12) Phenanthrene	17.07	178	1484	0.020	ng/ul#	Ovalue 88

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM030920\
Data File : BM025420.D
Acq On : 09 Mar 2020 18:49
Operator : CG/JU
Sample : L1612-10
Misc :
ALS Vial : 14 Sample Multiplier: 1




Instrument :
BNA_M
ClientSampleId :
DBDL2

Manual Integrations
APPROVED

mohammad
3/10/2020 7:59:05 AM

Quant Time: Mar 09 19:22:04 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 09 13:32:56 2020
Response via : Initial Calibration

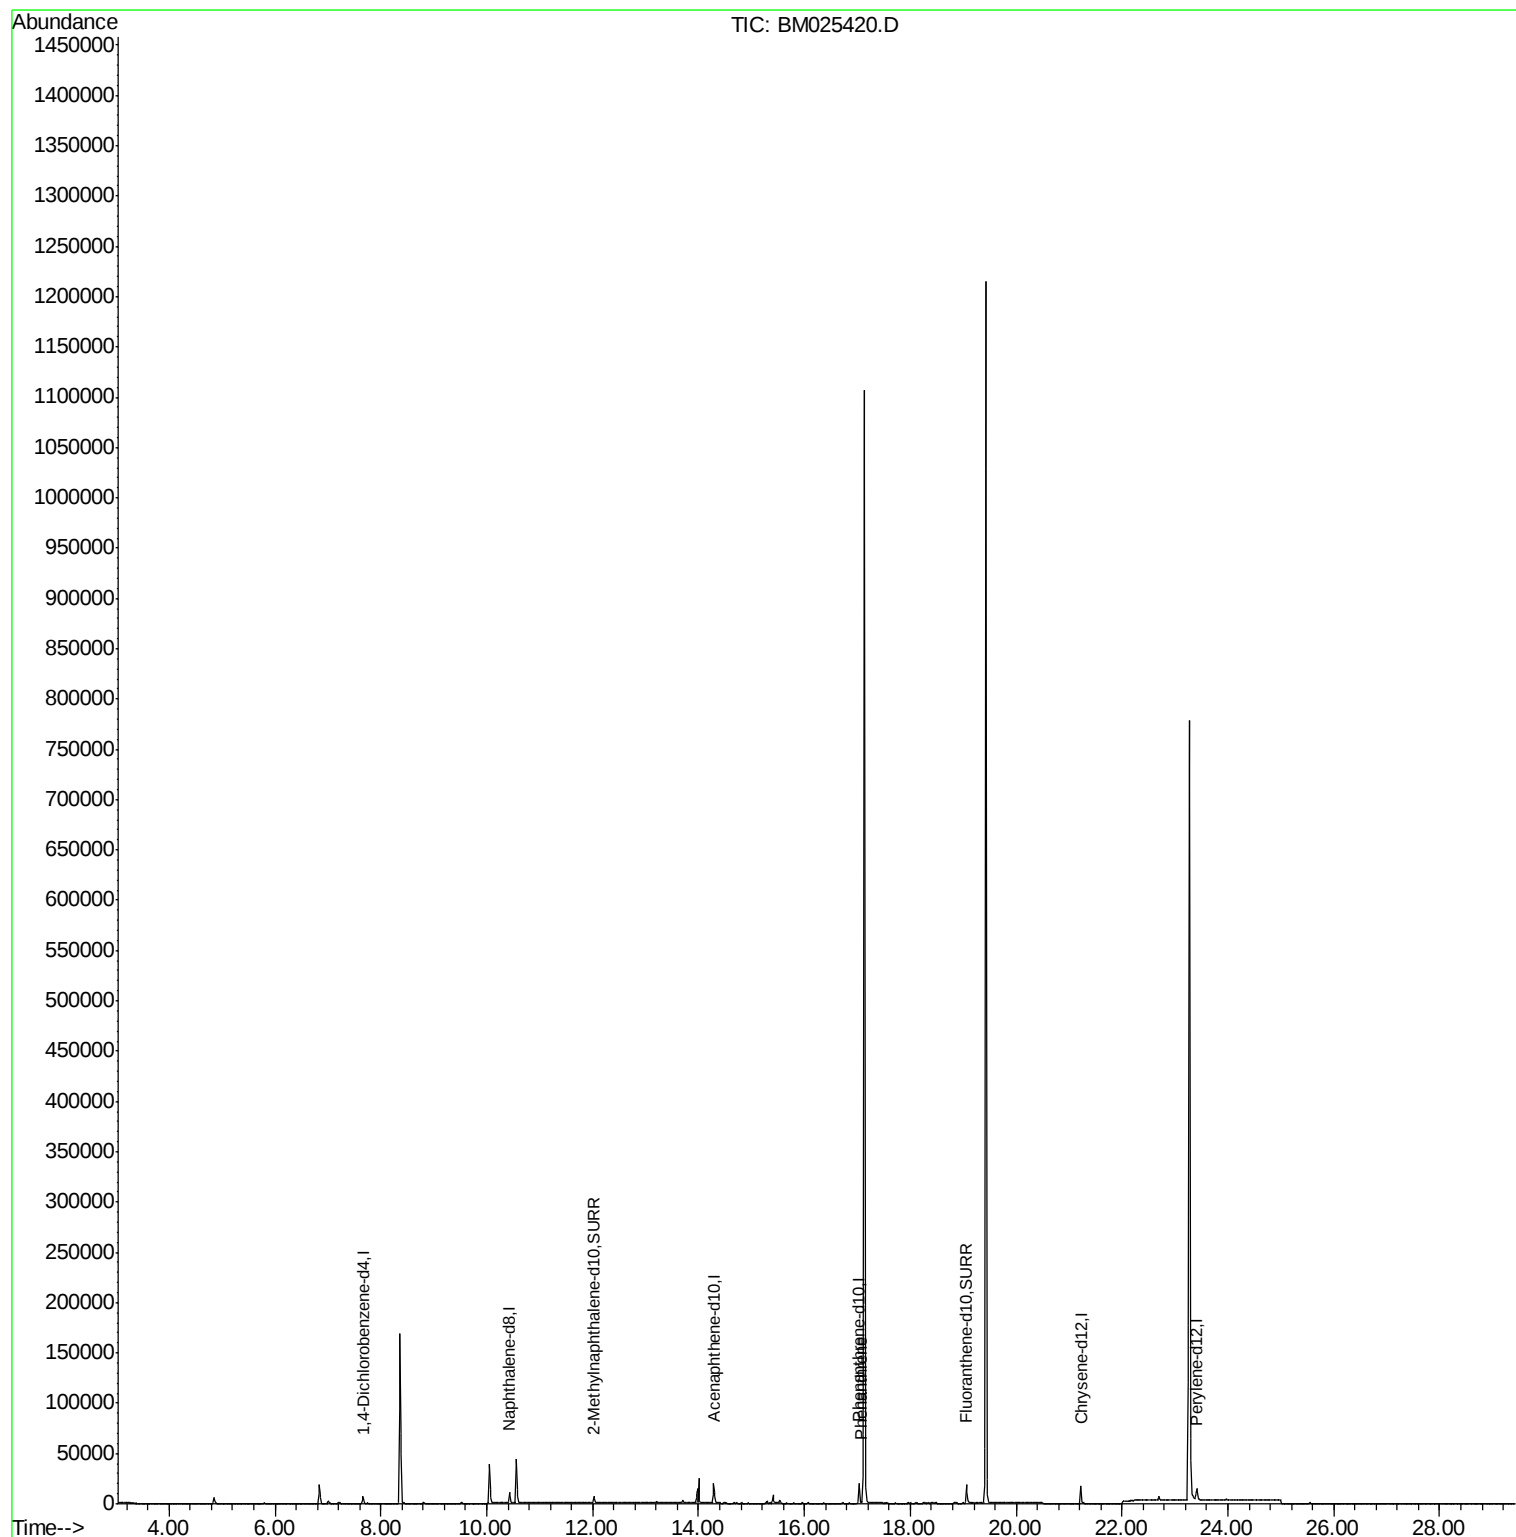

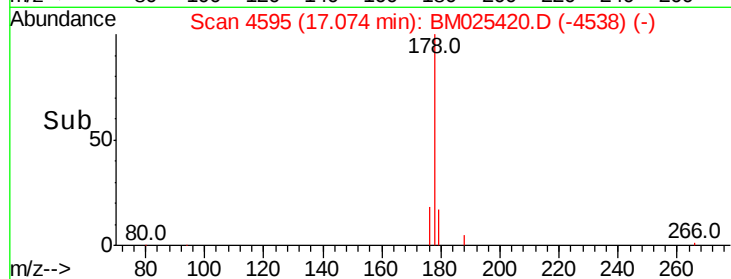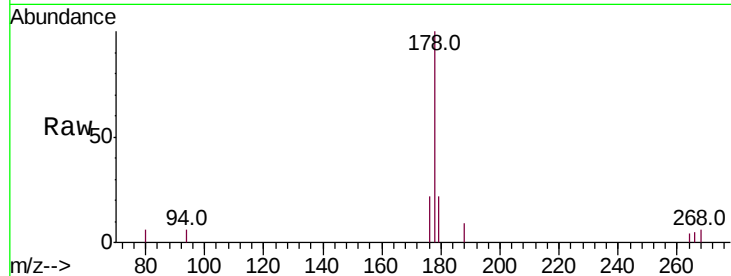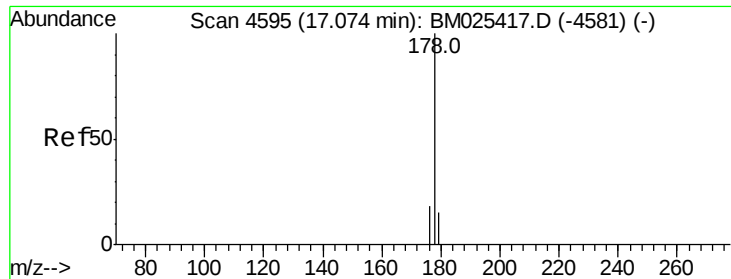

#12

Phenanthrene

Concen: 0.020 ng/ul

RT: 17.07 min Scan# 4595

Delta R.T. -0.00 min

Lab File: BM025420.D

Acq: 09 Mar 2020 18:49

Instrument :

BNA_M

ClientSampleId :

DBDL2

Tot Ion:	178	Resp:	1484
Ion Ratio	Lower	Upper	
178	100		
179	22.1	12.4	18.6#
176	22.4	14.8	22.2#

Manual Integrations
APPROVED

mohammad
3/10/2020 7:59:05 AM

