

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM030920\
 Data File : BM025460.D
 Acq On : 10 Mar 2020 19:38
 Operator : CG/JU
 Sample : L1617-20
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Mar 11 00:07:16 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030920.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Mar 10 23:48:01 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.66	152	3491	0.40	ng/ul	0.00
2) Naphthalene-d8	10.43	136	15307	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.29	164	10230	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.03	188	20927	0.40	ng/ul	0.00
16) Chrysene-d12	21.22	240	16295	0.40	ng/ul	0.00
20) Perylene-d12	23.41	264	19151	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.02	152	3486	0.13	ng/ul	0.00
14) Fluoranthene-d10	19.06	212	7908	0.14	ng/ul	0.00
Target Compounds					Ovalue	
3) Naphthalene	10.48	128	16973	0.375	ng/ul	99
5) 2-Methylnaphthalene	12.10	142	12502	0.386	ng/ul	100
7) Acenaphthylene	14.00	152	59235	1.417	ng/ul	99
8) Acenaphthene	14.35	153	79361	2.165	ng/ul	99
9) Fluorene	15.34	166	108304	2.424	ng/ul	100
12) Phenanthrene	17.07	178	656244	9.895	ng/ul	100
13) Anthracene	17.17	178	1561697	27.059	ng/ul	99
15) Fluoranthene	19.09	202	2819385	39.217	ng/ul	98
17) Pyrene	19.46	202	3275619	44.786	ng/ul	99
18) Benzo(a)anthracene	21.21	228	1490130	25.578	ng/ul	97
19) Chrysene	21.26	228	2027905	30.997	ng/ul	98
21) Benzo(b)fluoranthene	22.76	252	2654271m	35.001	ng/ul	
22) Benzo(k)fluoranthene	22.80	252	855454m	10.766	ng/ul	
23) Benzo(a)pyrene	23.32	252	1180566m	18.747	ng/ul	
24) Indeno(1,2,3-cd)pyrene	25.58	276	778599	9.113	ng/ul#	99
25) Dibenzo(a,h)anthracene	25.59	278	212374	2.955	ng/ul	97
26) Benzo(a,h,i)perylene	26.24	276	507270	6.845	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM030920\
Data File : BM025460.D
Acq On : 10 Mar 2020 19:38
Operator : CG/JU
Sample : L1617-20
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Mar 11 00:07:16 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 10 23:48:01 2020
Response via : Initial Calibration

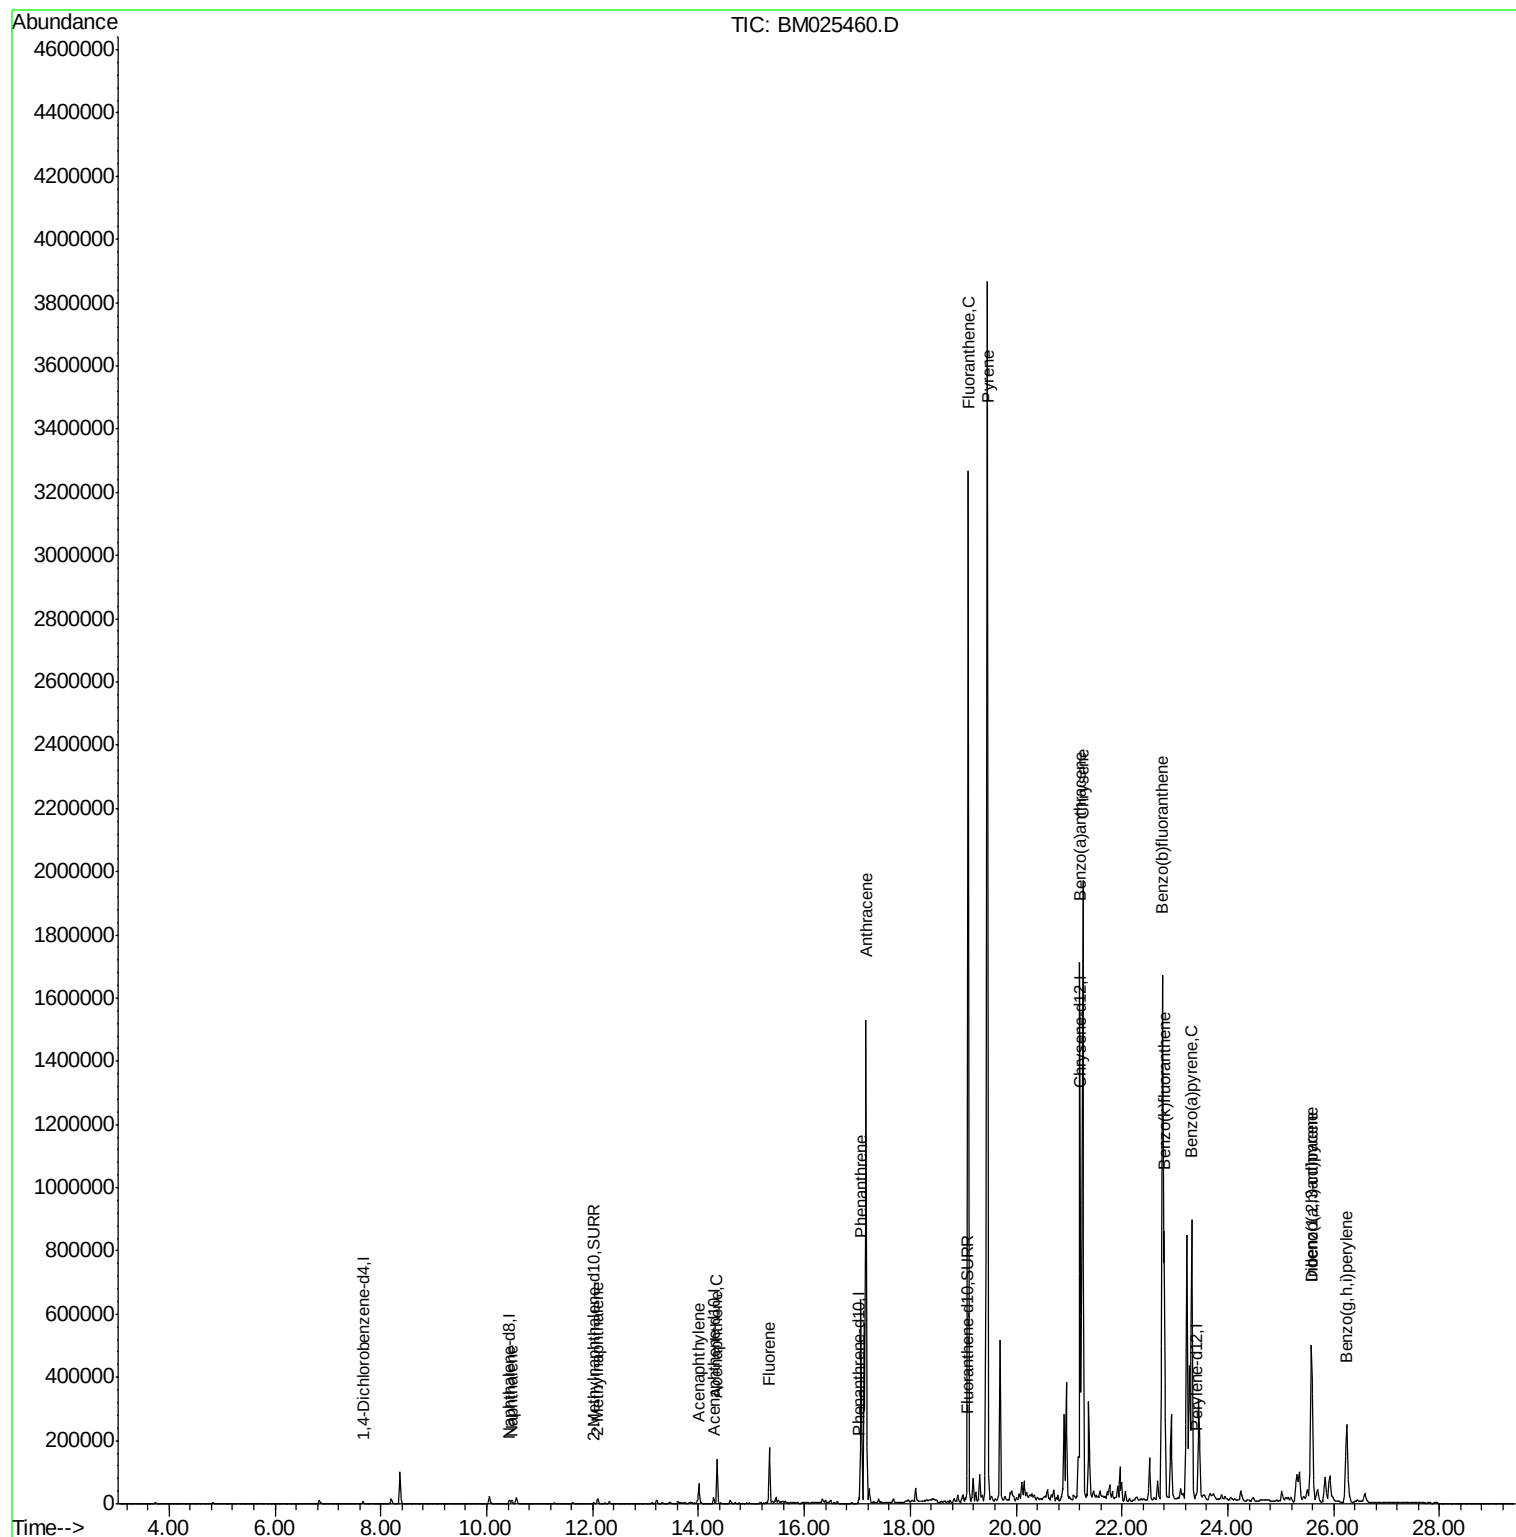

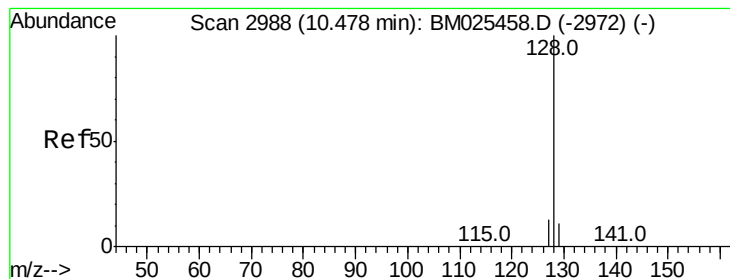

#3

Naphthalene

Concen: 0.375 ng/ul

RT: 10.48 min Scan# 2988

Delta R.T. 0.00 min

Lab File: BM025460.D

Acq: 10 Mar 2020 19:38

Instrument :

BNA_M

ClientSampleId :


Tot Ion:128 Resp: 16973

Ion Ratio Lower Upper

128 100

129 11.9 9.4 14.0




127 13.0 10.9 16.3

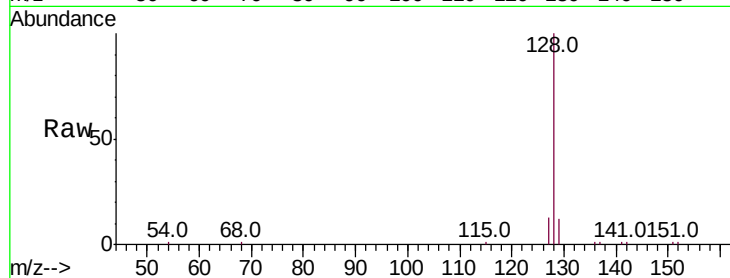

Abundance Ion 128.00 (127.70 to 128.70): E

Ion 129.00 (128.70 to 129.70): E

Ion 127.00 (126.70 to 127.70): E

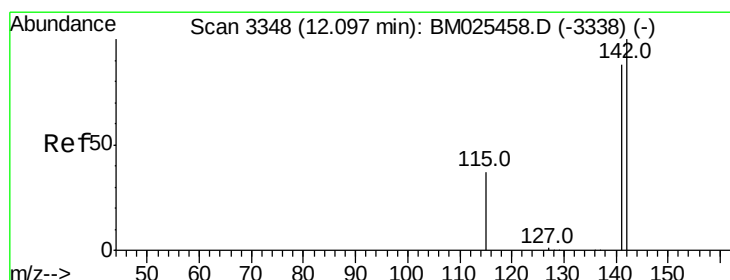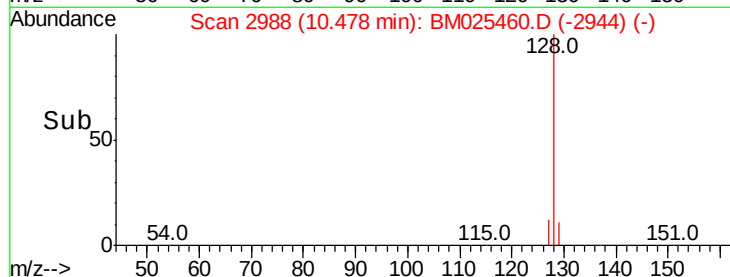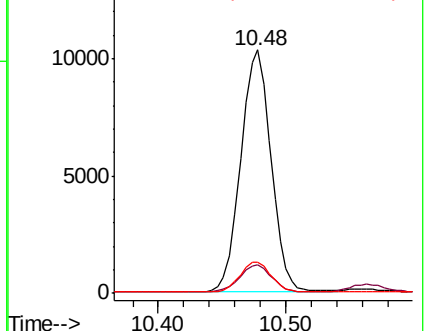

#5

2-Methylnaphthalene

Concen: 0.386 ng/ul

RT: 12.10 min Scan# 3348

Delta R.T. -0.00 min

Lab File: BM025460.D


Acq: 10 Mar 2020 19:38

Tgt Ion:142 Resp: 12502

Ion Ratio Lower Upper



142 100


141 87.0 69.8 104.6

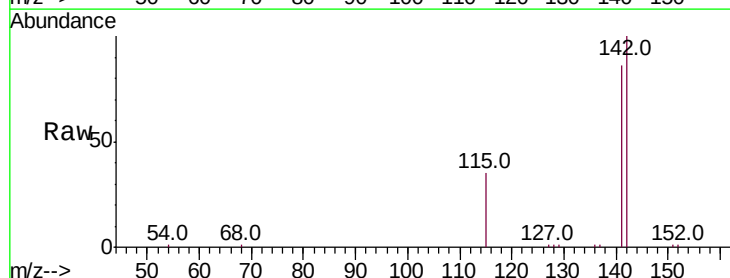

Abundance Ion 142.00 (141.70 to 142.70): E

Ion 141.00 (140.70 to 141.70): E

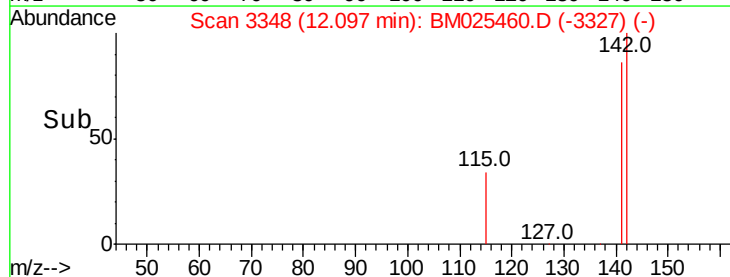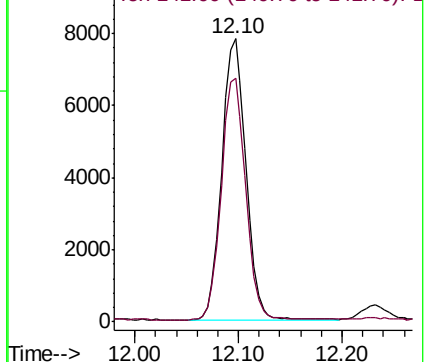

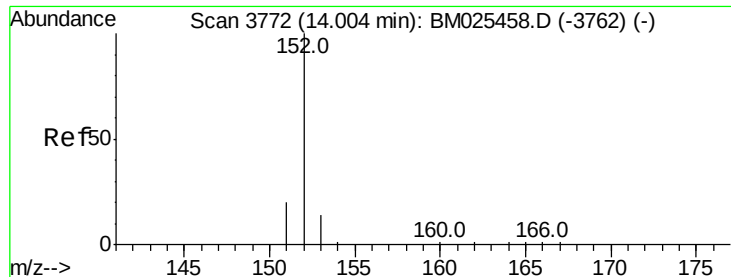

#7

Acenaphthylene

Concen: 1.417 ng/ul

RT: 14.00 min Scan# 3772

Delta R.T. -0.00 min

Lab File: BM025460.D

Acq: 10 Mar 2020 19:38

Instrument :

BNA_M

ClientSampled :


Tot Ion:152 Resp: 59235

Ion Ratio Lower Upper

152 100

151 19.6 16.2 24.2




153 13.4 10.6 16.0



Abundance Ion 152.00 (151.70 to 152.70): E

Ion 151.00 (150.70 to 151.70): E

Ion 153.00 (152.70 to 153.70): E

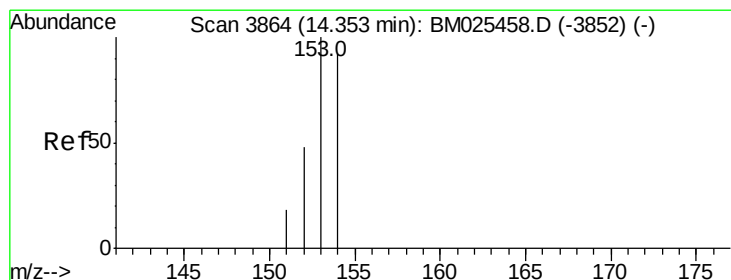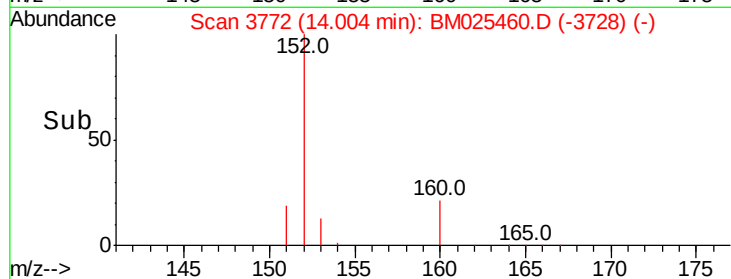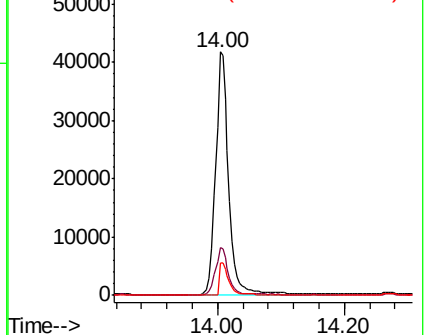

#8

Acenaphthene

Concen: 2.165 ng/ul

RT: 14.35 min Scan# 3863

Delta R.T. -0.00 min

Lab File: BM025460.D

Acq: 10 Mar 2020 19:38


Tgt Ion:153 Resp: 79361

Ion Ratio Lower Upper

153 100

152 47.2 39.5 59.3



154 89.6 71.7 107.5




Abundance Ion 153.00 (152.70 to 153.70): E

Ion 152.00 (151.70 to 152.70): E

Ion 154.00 (153.70 to 154.70): E



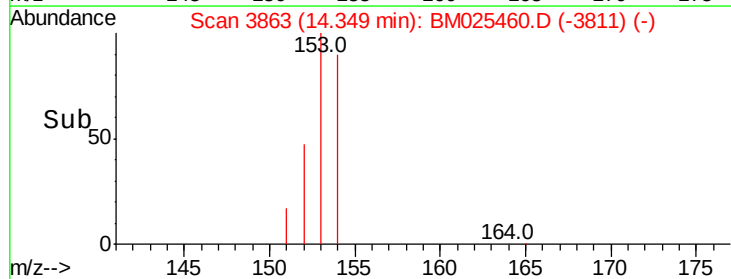
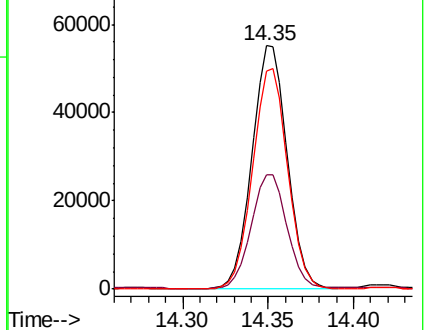


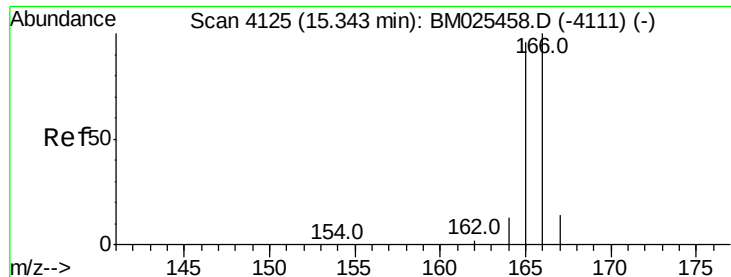

#9
Fluorene
 Concen: 2.424 ng/ul
 RT: 15.34 min Scan# 4124
 Delta R.T. -0.00 min
 Lab File: BM025460.D
 Acq: 10 Mar 2020 19:38




Instrument :
 BNA_M
 ClientSampleId :


Tot Ion:166 Resp: 108304
 Ion Ratio Lower Upper
 166 100
 165 96.2 76.8 115.2
 167 13.9 11.2 16.8

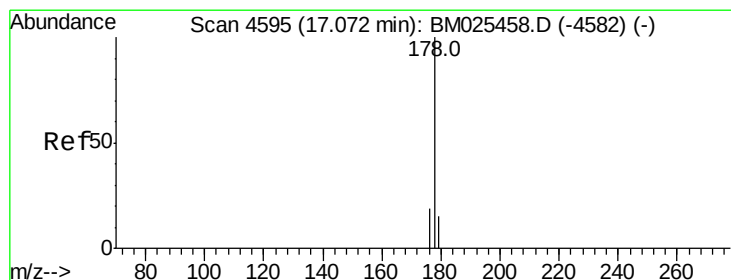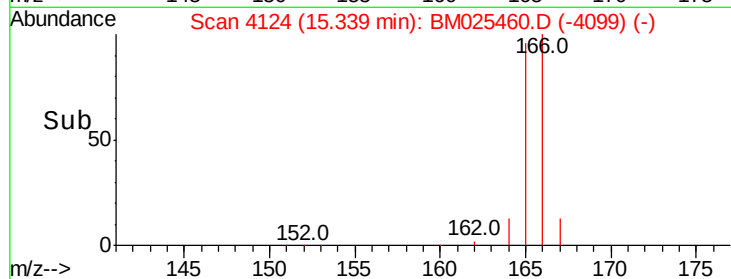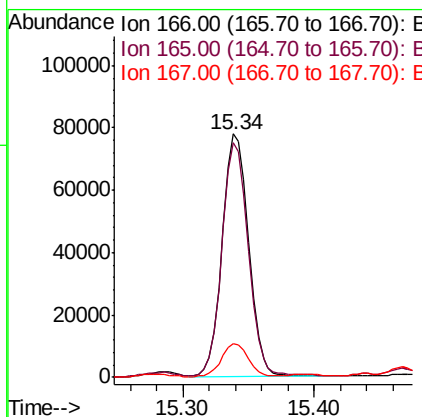

#12
Phenanthrene
 Concen: 9.895 ng/ul
 RT: 17.07 min Scan# 4595
 Delta R.T. -0.00 min
 Lab File: BM025460.D
 Acq: 10 Mar 2020 19:38

Tgt Ion:178 Resp: 656244
 Ion Ratio Lower Upper
 178 100
 179 15.5 12.4 18.6
 176 18.3 14.8 22.2


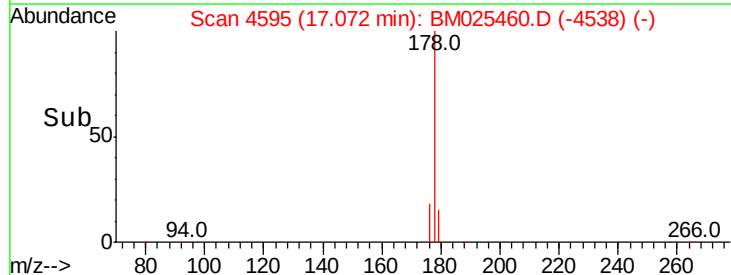
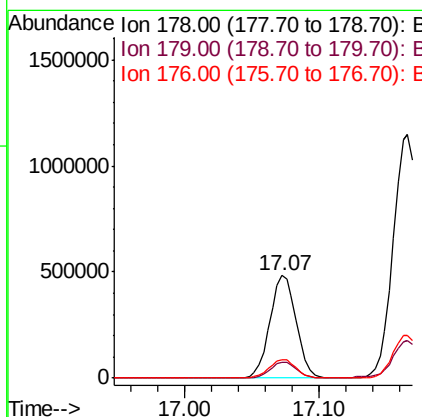



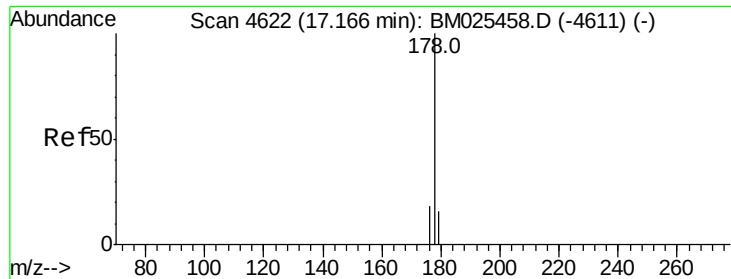

#13
 Anthracene
 Concen: 27.059 ng/ul
 RT: 17.17 min Scan# 4622
 Delta R.T. 0.00 min
 Lab File: BM025460.D
 Acq: 10 Mar 2020 19:38




Instrument :
 BNA_M
 ClientSampled :


Tot Ion:178 Resp: 1561697
 Ion Ratio Lower Upper
 178 100
 179 15.6 12.6 18.8
 176 17.5 14.5 21.7

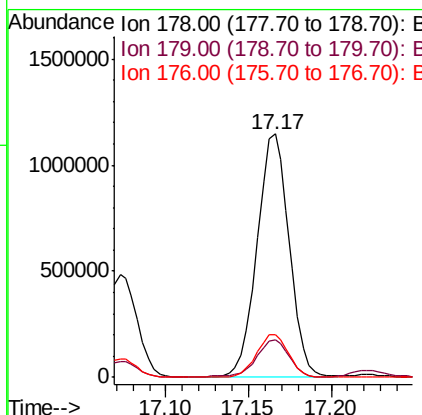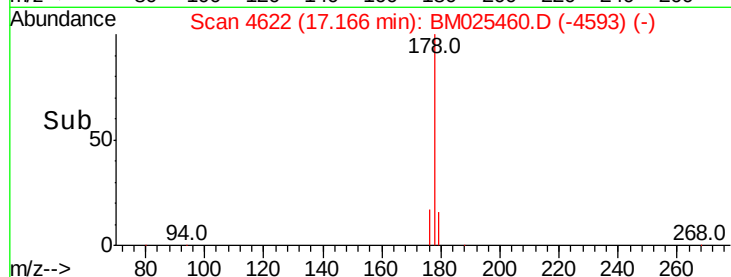

#15
 Fluoranthene
 Concen: 39.217 ng/ul
 RT: 19.09 min Scan# 5162
 Delta R.T. 0.00 min
 Lab File: BM025460.D
 Acq: 10 Mar 2020 19:38

Tgt Ion:202 Resp: 2819385
 Ion Ratio Lower Upper
 202 100
 101 8.5 0.0 27.5
 100 6.6 0.0 26.0

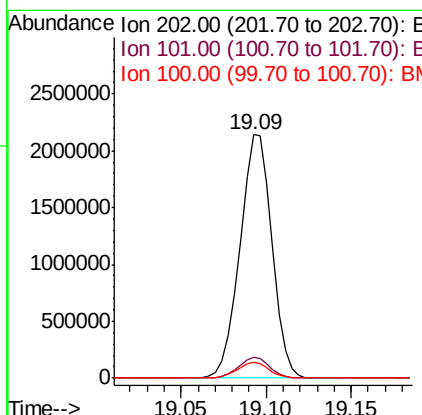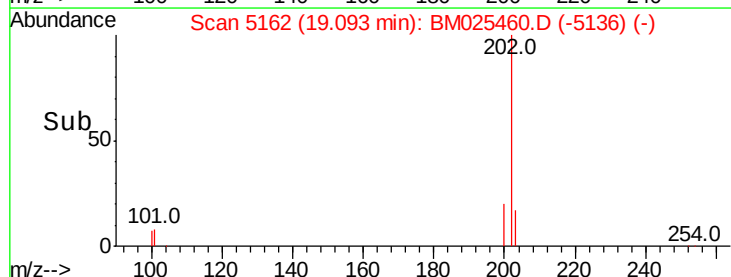

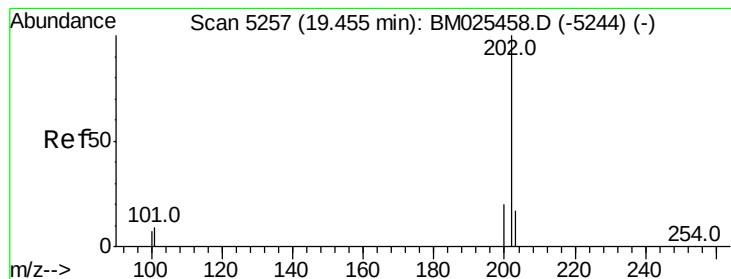

#17

Pvrene

Concen: 44.786 ng/ul

RT: 19.46 min Scan# 5258

Delta R.T. 0.00 min

Lab File: BM025460.D

Acq: 10 Mar 2020 19:38

Instrument :

BNA_M

ClientSampleId :


Tot Ion:202 Resp: 3275619

Ion Ratio Lower Upper

202 100

101 9.5 7.1 10.7




100 7.7 6.0 9.0



Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): E

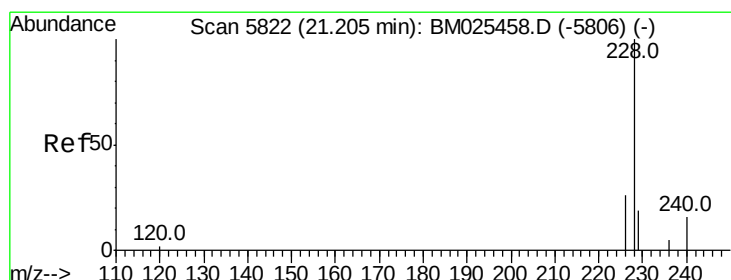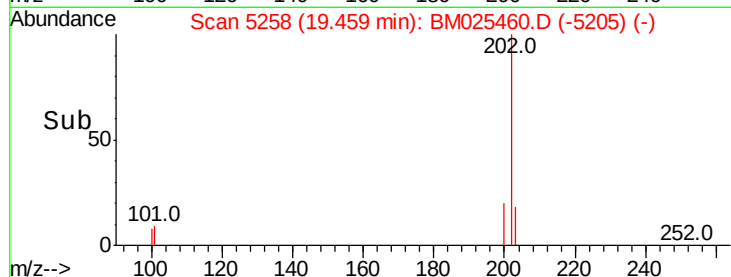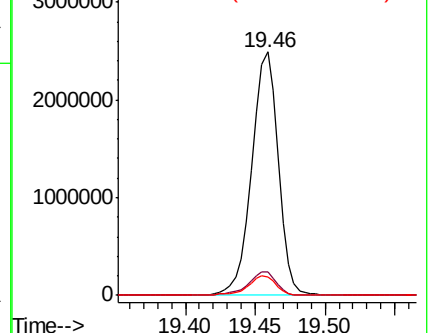

#18

Benzo(a)anthracene

Concen: 25.578 ng/ul

RT: 21.21 min Scan# 5823

Delta R.T. 0.00 min

Lab File: BM025460.D

Acq: 10 Mar 2020 19:38


Tgt Ion:228 Resp: 1490130

Ion Ratio Lower Upper

228 100

229 21.2 15.6 23.4



226 27.9 21.1 31.7

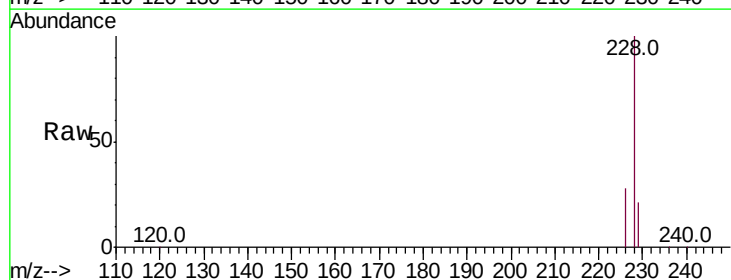


Abundance Ion 228.00 (227.70 to 228.70): E

Ion 229.00 (228.70 to 229.70): E

Ion 226.00 (225.70 to 226.70): E

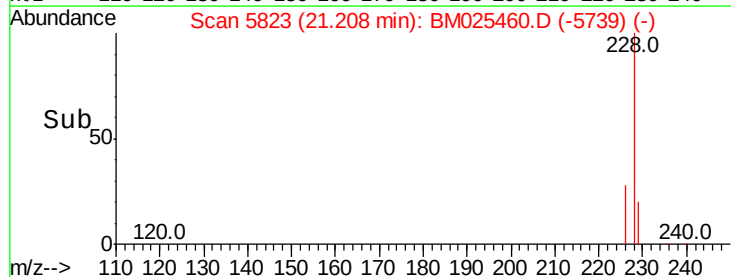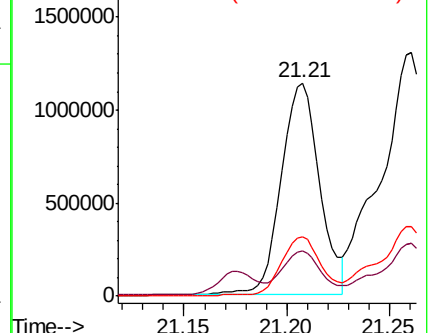

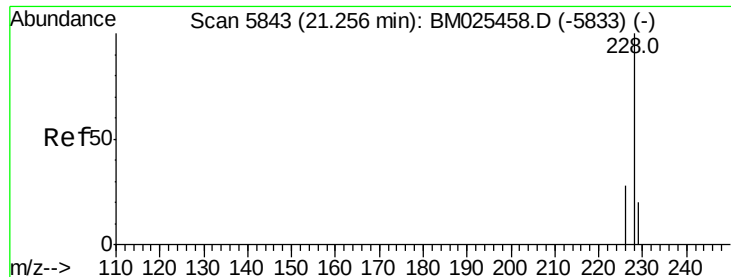

#19

Chrysene

Concen: 30.997 ng/ul

RT: 21.26 min Scan# 5845

Delta R.T. 0.00 min

Lab File: BM025460.D

Acq: 10 Mar 2020 19:38

Instrument :

BNA_M

ClientSampleId :


Tot Ion:228 Resp: 2027905

Ion Ratio Lower Upper




228 100

226 28.8 23.6 35.4

229 21.5 16.3 24.5

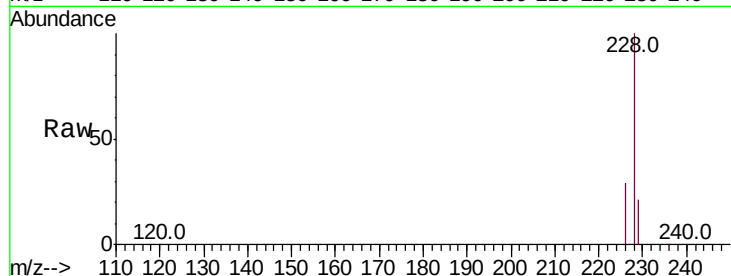

Abundance Ion 228.00 (227.70 to 228.70): E
Ion 226.00 (225.70 to 226.70): E
Ion 229.00 (228.70 to 229.70): E

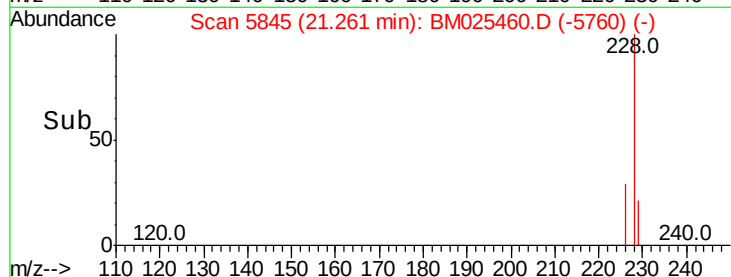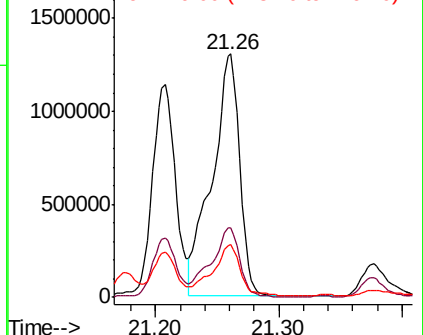

#21

Benzo(b)fluoranthene

Concen: 35.001 ng/ul m

RT: 22.76 min Scan# 6466

Delta R.T. 0.01 min

Lab File: BM025460.D

Acq: 10 Mar 2020 19:38


Tgt Ion:252 Resp: 2654271

Ion Ratio Lower Upper



252 100


253 22.9 0.0 50.2

125 7.2 0.0 17.6



Abundance Ion 252.00 (251.70 to 252.70): E
Ion 253.00 (252.70 to 253.70): E
Ion 125.00 (124.70 to 125.70): E

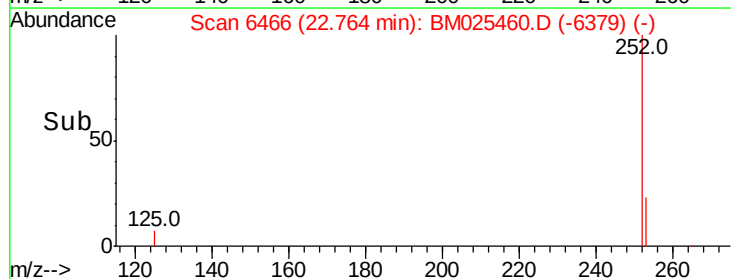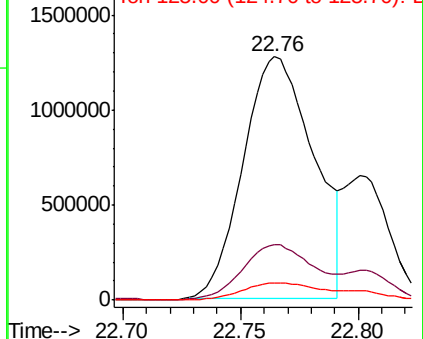

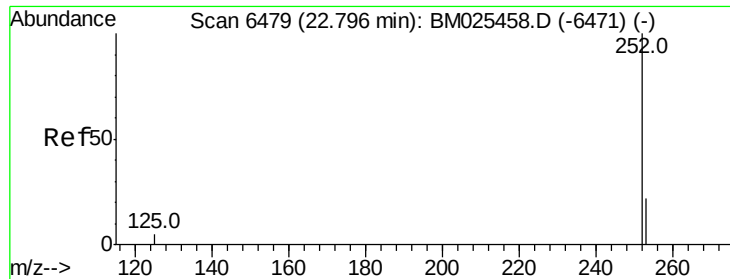

#22

Benzo(k)fluoranthene

Concen: 10.766 ng/ul m

RT: 22.80 min Scan# 6481

Delta R.T. 0.00 min

Lab File: BM025460.D

Acq: 10 Mar 2020 19:38

Instrument :

BNA_M

ClientSampleId :


Tot Ion:252 Resp: 855454

Ion Ratio Lower Upper




252 100

253 23.7 19.8 29.8

125 7.2 7.1 10.7

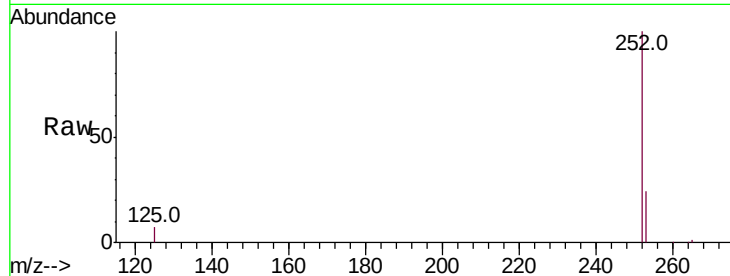

Abundance Ion 252.00 (251.70 to 252.70): E
Ion 253.00 (252.70 to 253.70): E
Ion 125.00 (124.70 to 125.70): E

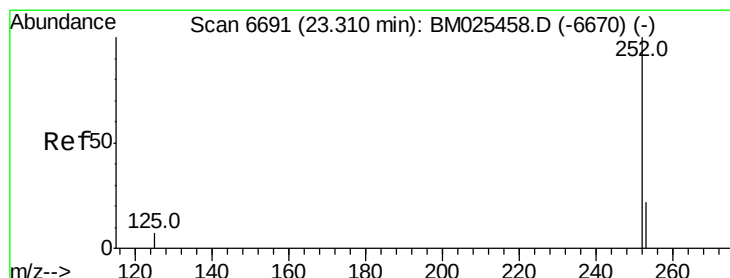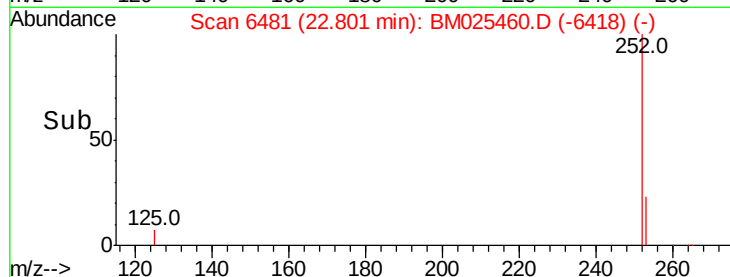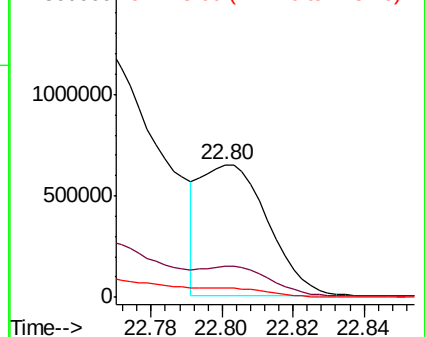

#23

Benzo(a)pyrene

Concen: 18.747 ng/ul m

RT: 23.32 min Scan# 6694

Delta R.T. 0.01 min

Lab File: BM025460.D

Acq: 10 Mar 2020 19:38


Tgt Ion:252 Resp: 1180566

Ion Ratio Lower Upper



252 100


253 23.1 21.3 31.9

125 7.6 8.5 12.7#

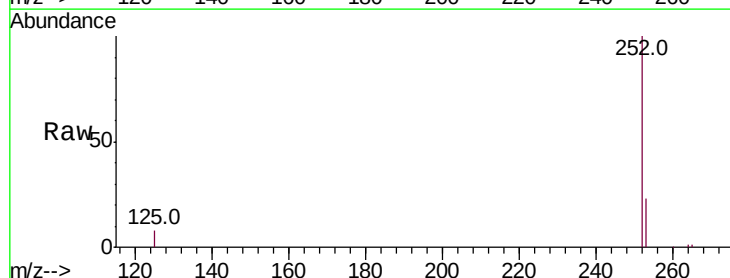

Abundance Ion 252.00 (251.70 to 252.70): E
Ion 253.00 (252.70 to 253.70): E
Ion 125.00 (124.70 to 125.70): E



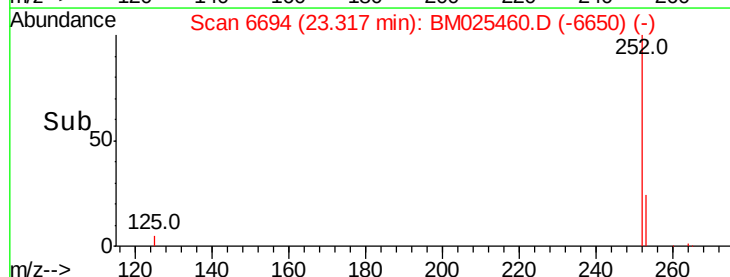
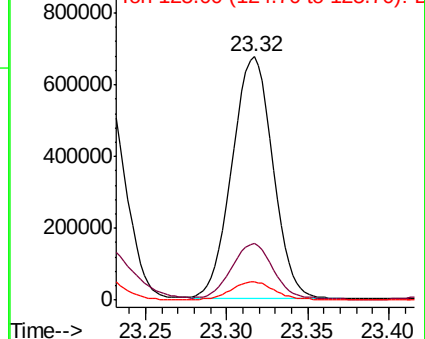


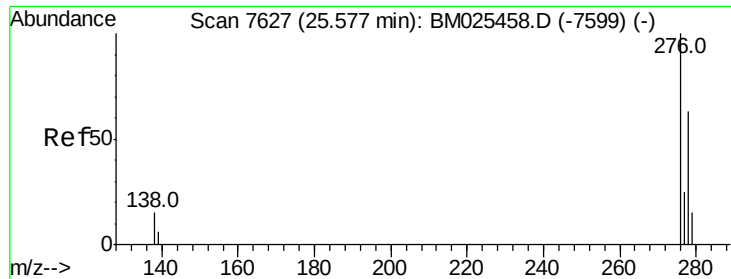

#24
 Indeno(1,2,3-cd)pyrene
 Concen: 9.113 ng/ul
 RT: 25.58 min Scan# 7629
 Delta R.T. 0.00 min
 Lab File: BM025460.D
 Acq: 10 Mar 2020 19:38




Instrument :
 BNA_M
 ClientSampleId :


Tot Ion:276 Resp: 778599
 Ion Ratio Lower Upper
 276 100
 138 15.0 12.3 18.5
 227 0.0 0.0 0.0

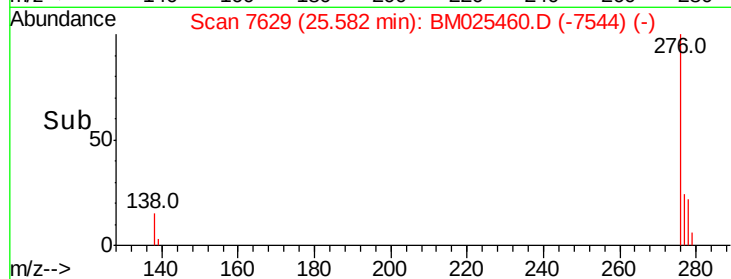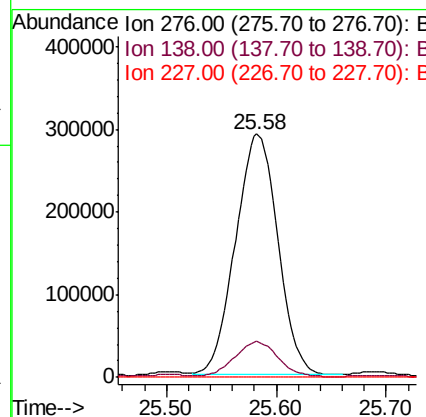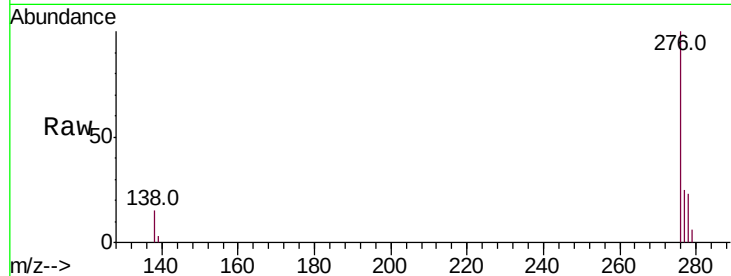

#25
 Dibenzo(a,h)anthracene
 Concen: 2.955 ng/ul
 RT: 25.59 min Scan# 7631
 Delta R.T. -0.01 min
 Lab File: BM025460.D
 Acq: 10 Mar 2020 19:38

Tgt Ion:278 Resp: 212374
 Ion Ratio Lower Upper
 278 100
 139 12.2 9.0 13.6
 279 27.8 21.1 31.7

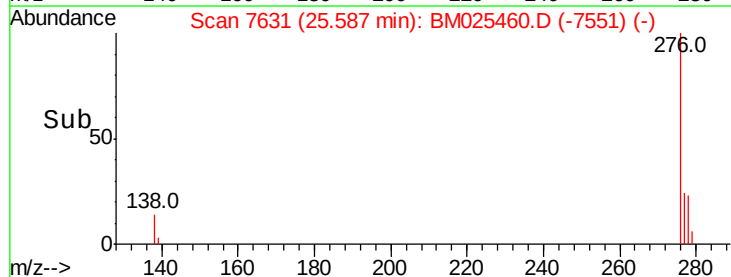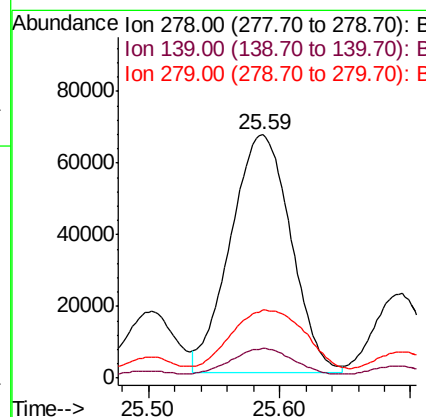

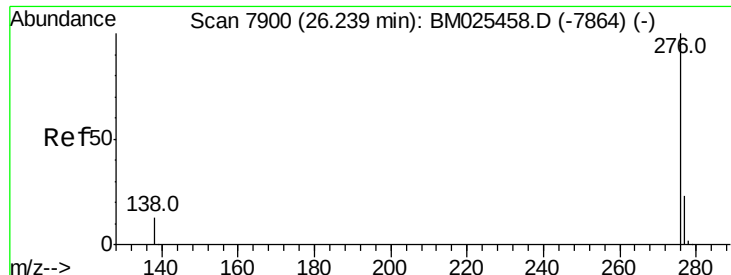

#26

Benzo(a,h,i)perylene

Concen: 6.845 ng/ul

RT: 26.24 min Scan# 7902

Delta R.T. 0.00 min

Lab File: BM025460.D

Acq: 10 Mar 2020 19:38

Instrument :

BNA_M

ClientSampleId :


Tot Ion:276 Resp: 507270

Ion Ratio Lower Upper

276 100

138 14.8 11.0 16.4

277 24.2 19.8 29.6

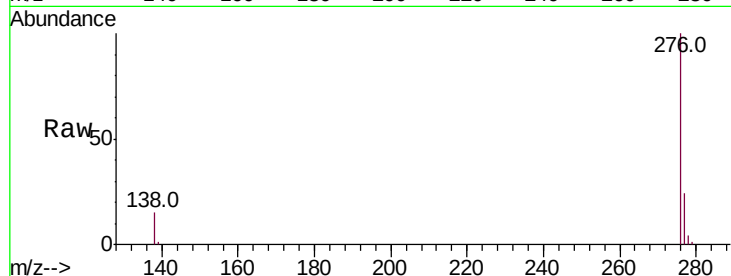

Abundance Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 277.00 (276.70 to 277.70): E

