

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM030920\
 Data File : BM025462.D
 Acq On : 10 Mar 2020 20:51
 Operator : CG/JU
 Sample : L1617-04
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBDR8

Quant Time: Mar 11 00:08:43 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030920.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Mar 10 23:48:01 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.66	152	3590	0.40	ng/ul	0.00
2) Naphthalene-d8	10.43	136	14753	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.29	164	9866	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.03	188	21367	0.40	ng/ul	0.00
16) Chrysene-d12	21.22	240	18567	0.40	ng/ul	0.00
20) Perylene-d12	23.40	264	20480	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.03	152	5957	0.22	ng/ul	0.00
14) Fluoranthene-d10	19.06	212	13843	0.24	ng/ul	0.00
Target Compounds						
12) Phenanthrene	17.08	178	1436	0.021	ng/ul#	Ovalue 89




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM030920\
Data File : BM025462.D
Acq On : 10 Mar 2020 20:51
Operator : CG/JU
Sample : L1617-04
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBDR8

Quant Time: Mar 11 00:08:43 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 10 23:48:01 2020
Response via : Initial Calibration

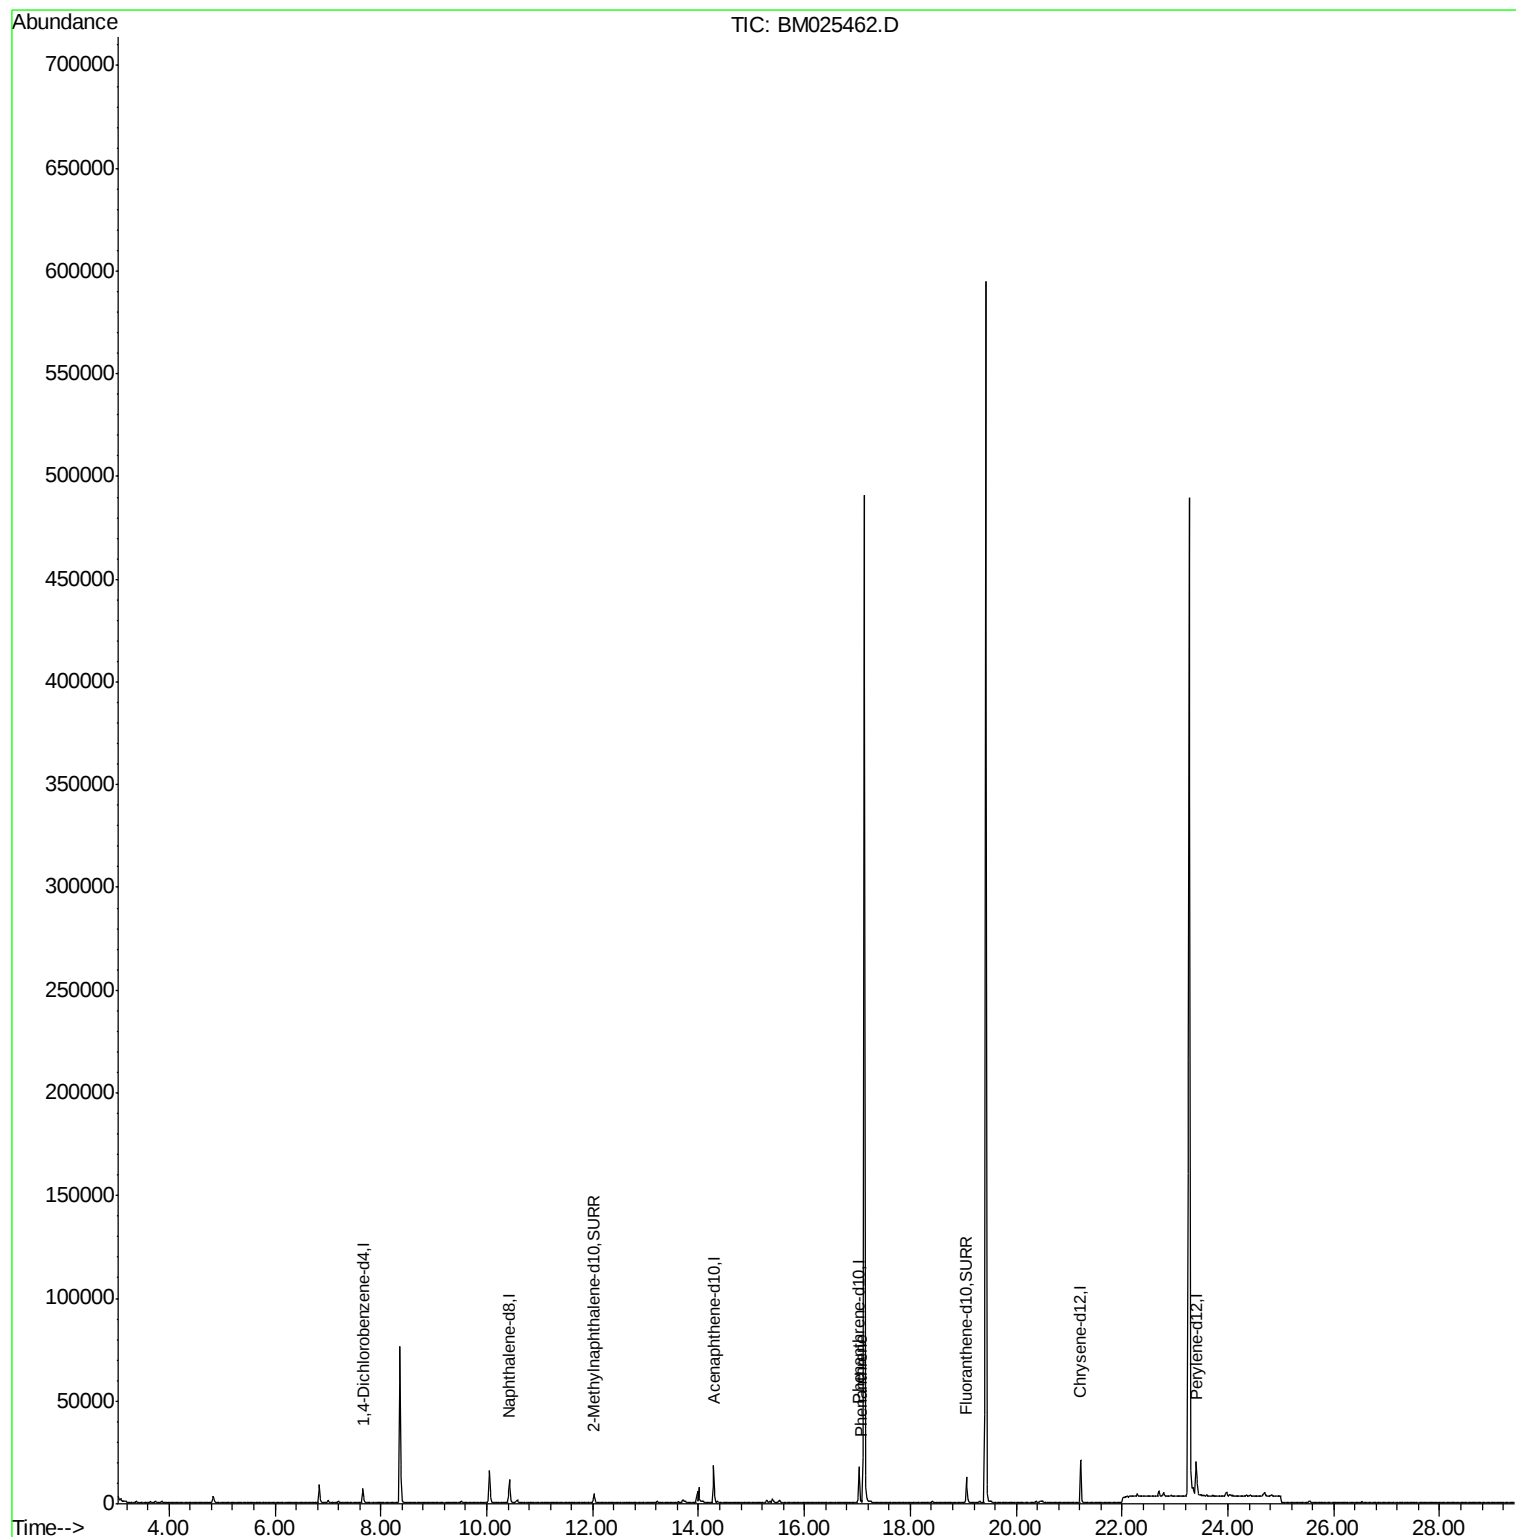

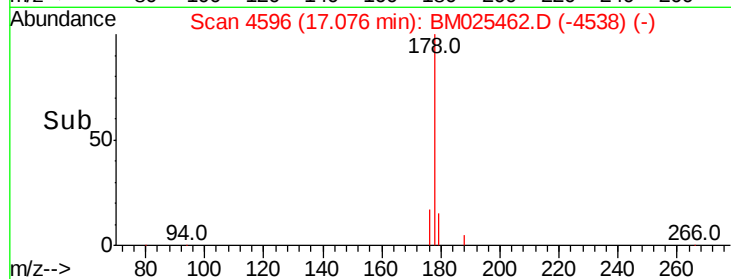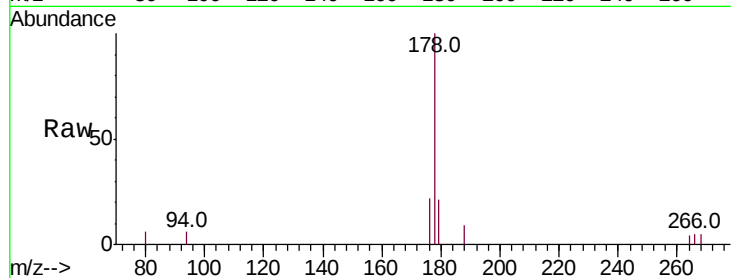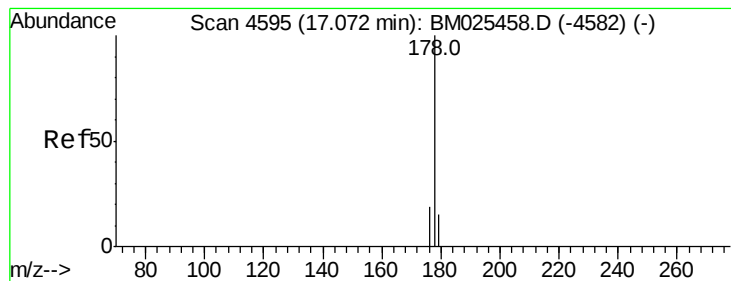

#12

Phenanthrene

Concen: 0.021 ng/ul

RT: 17.08 min Scan# 4596

Delta R.T. 0.00 min

Lab File: BM025462.D

Acq: 10 Mar 2020 20:51

Instrument :

BNA_M

ClientSampleId :

DBDR8

Tot Ion:178 Resp: 1436

Ion Ratio Lower Upper

178 100

179 21.2 12.4 18.6#

176 22.2 14.8 22.2#

