

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM030920\
 Data File : BM025475.D
 Acq On : 11 Mar 2020 05:22
 Operator : CG/JU
 Sample : L1617-20DL 5X
 Misc :
 ALS Vial : 69 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Mar 11 05:55:40 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030920.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Mar 10 23:48:01 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.66	152	3248	0.40	ng/ul	0.00
2) Naphthalene-d8	10.43	136	13686	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.29	164	9298	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.03	188	21771	0.40	ng/ul	0.00
16) Chrysene-d12	21.22	240	20180	0.40	ng/ul	0.00
20) Perylene-d12	23.40	264	20384	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.02	152	586	0.02	ng/ul	0.00
14) Fluoranthene-d10	19.06	212	1732	0.03	ng/ul	0.00
Target Compounds				Ovalue		
3) Naphthalene	10.48	128	2794	0.069	ng/ul#	93
5) 2-Methylnaphthalene	12.10	142	2015	0.070	ng/ul	100
7) Acenaphthylene	14.00	152	11442	0.301	ng/ul	99
8) Acenaphthene	14.35	153	13230	0.397	ng/ul	99
9) Fluorene	15.34	166	18981	0.467	ng/ul	100
12) Phenanthrene	17.07	178	125553	1.820	ng/ul	100
13) Anthracene	17.16	178	313826	5.227	ng/ul	99
15) Fluoranthene	19.09	202	636831	8.515	ng/ul	100
17) Pyrene	19.45	202	753576	8.320	ng/ul	100
18) Benzo(a)anthracene	21.20	228	350993	4.865	ng/ul	97
19) Chrysene	21.25	228	509858	6.293	ng/ul	98
21) Benzo(b)fluoranthene	22.75	252	677188m	8.390	ng/ul	
22) Benzo(k)fluoranthene	22.79	252	194712m	2.302	ng/ul	
23) Benzo(a)pyrene	23.30	252	274405m	4.094	ng/ul	
24) Indeno(1,2,3-cd)pyrene	25.57	276	172161	1.893	ng/ul#	100
25) Dibenzo(a,h)anthracene	25.58	278	47006	0.614	ng/ul	96
26) Benzo(a,h,i)perylene	26.23	276	109519	1.388	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM030920\
Data File : BM025475.D
Acq On : 11 Mar 2020 05:22
Operator : CG/JU
Sample : L1617-20DL 5X
Misc :
ALS Vial : 69 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Mar 11 05:55:40 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 10 23:48:01 2020
Response via : Initial Calibration

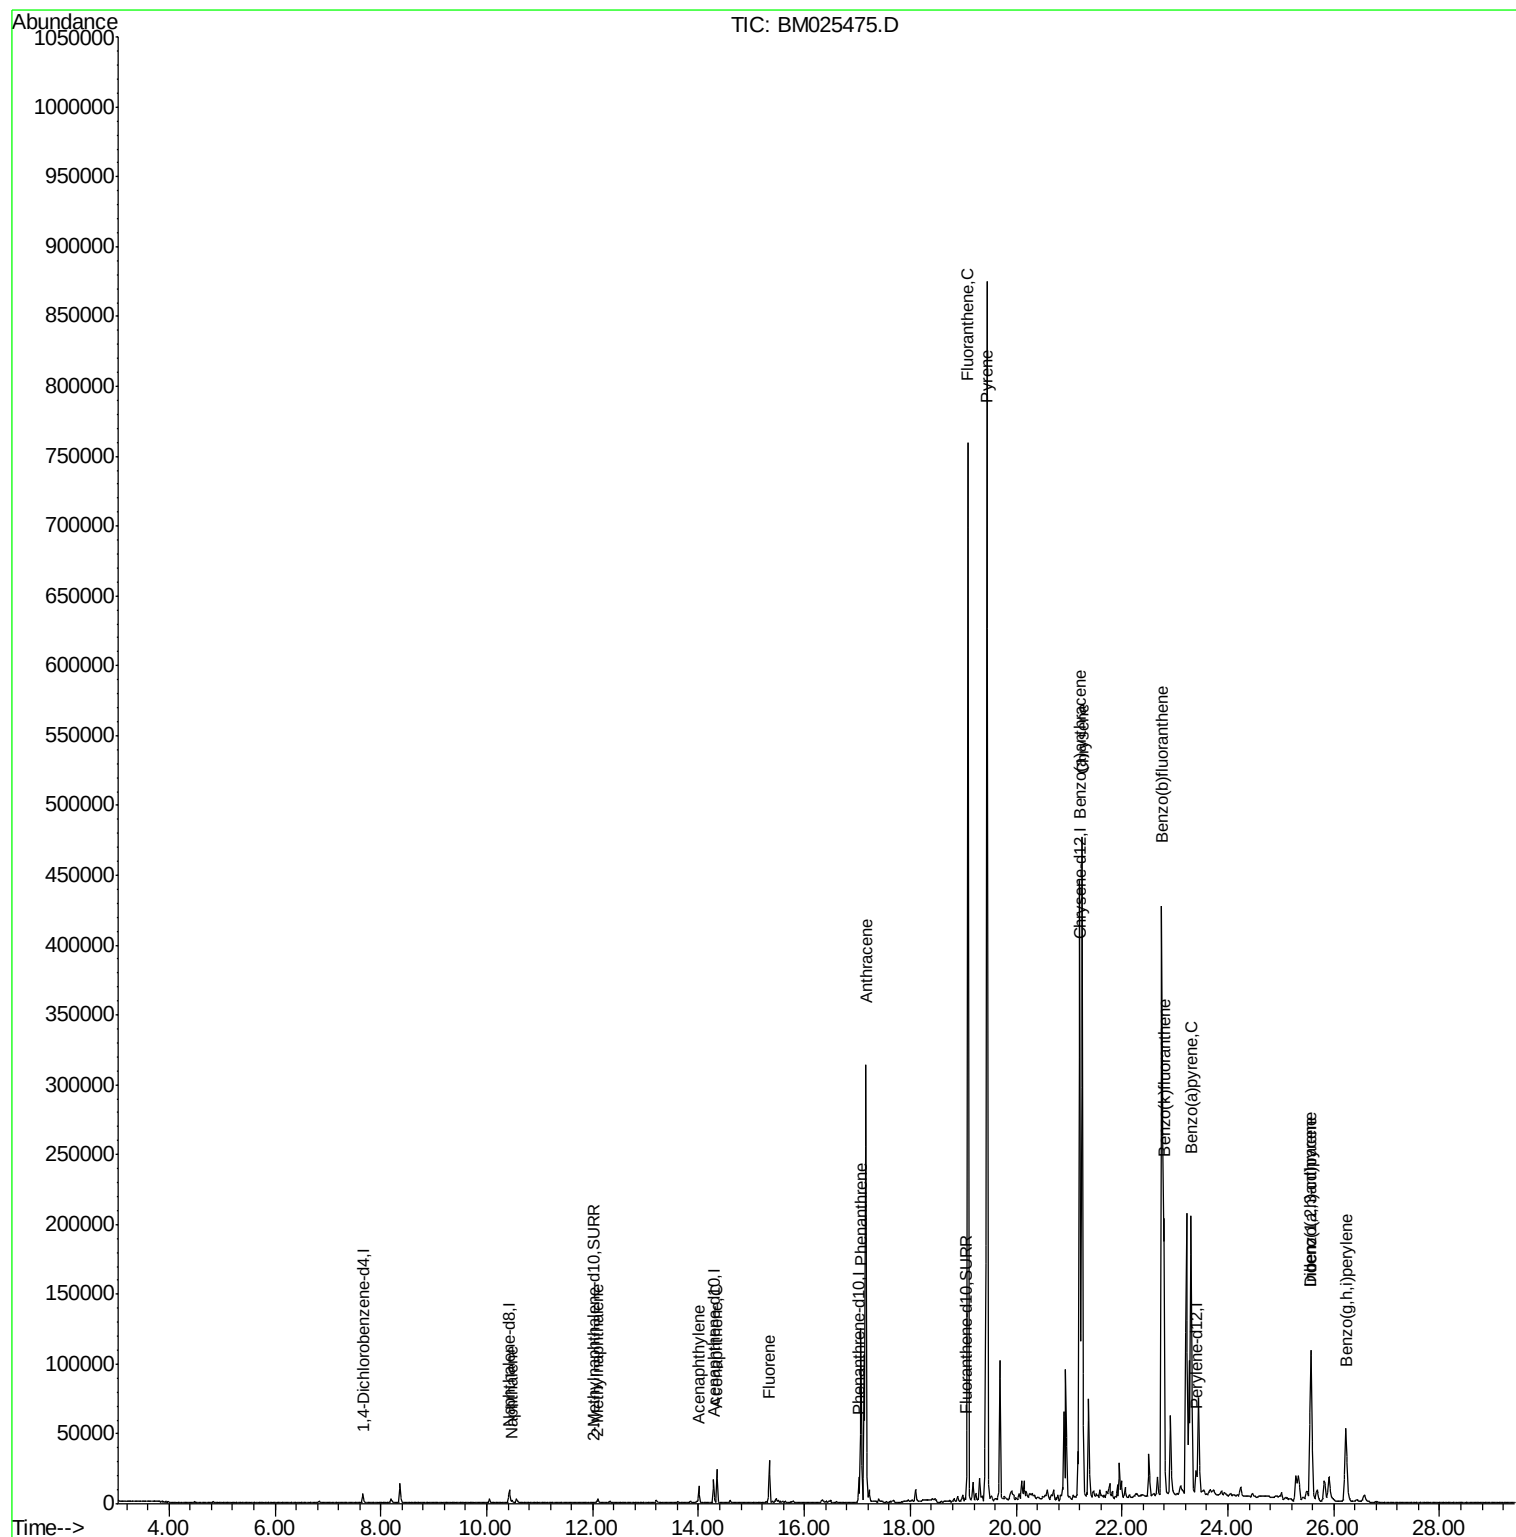

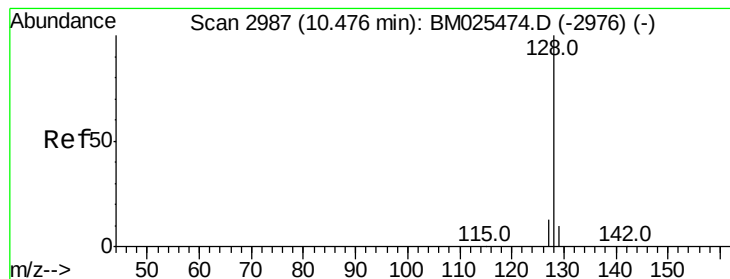

#3

Naphthalene

Concen: 0.069 ng/ul

RT: 10.48 min Scan# 2988

Delta R.T. -0.00 min

Lab File: BM025475.D

Acq: 11 Mar 2020 05:22

Instrument :

BNA_M

ClientSampleId :


Tot Ion:128 Resp: 2794

Ion Ratio Lower Upper

128 100

129 15.2 9.4 14.0#




127 15.9 10.9 16.3

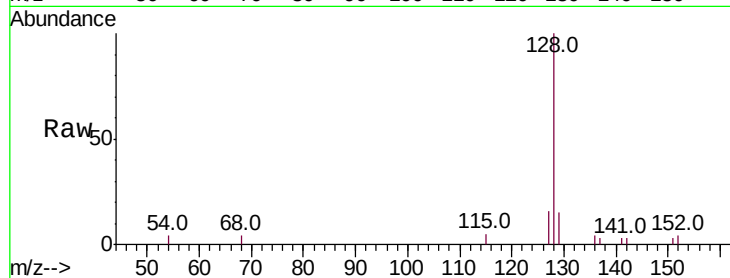

Abundance Ion 128.00 (127.70 to 128.70): E

Ion 129.00 (128.70 to 129.70): E

Ion 127.00 (126.70 to 127.70): E

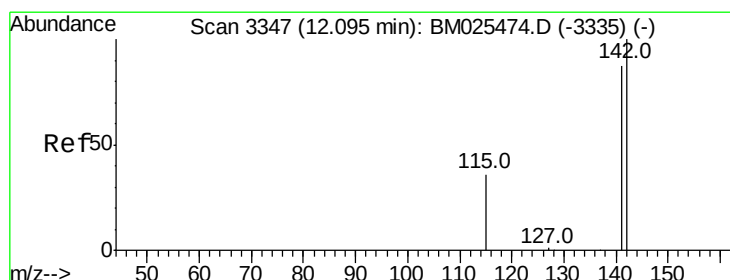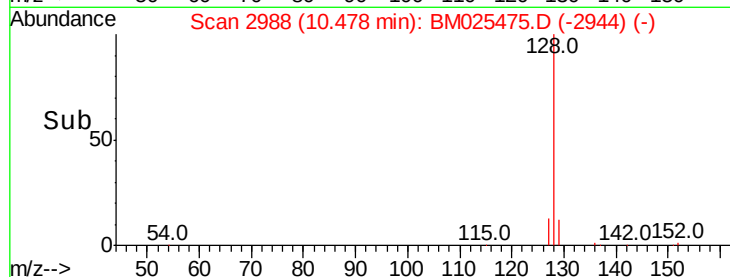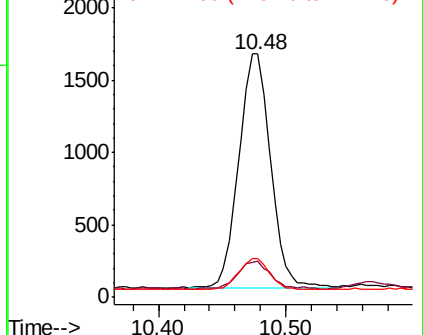

#5

2-Methylnaphthalene

Concen: 0.070 ng/ul

RT: 12.10 min Scan# 3348

Delta R.T. -0.00 min

Lab File: BM025475.D


Acq: 11 Mar 2020 05:22

Tgt Ion:142 Resp: 2015

Ion Ratio Lower Upper



142 100


141 86.9 69.8 104.6

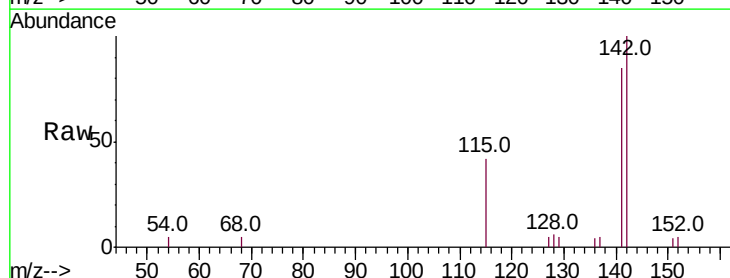

Abundance Ion 142.00 (141.70 to 142.70): E

Ion 141.00 (140.70 to 141.70): E

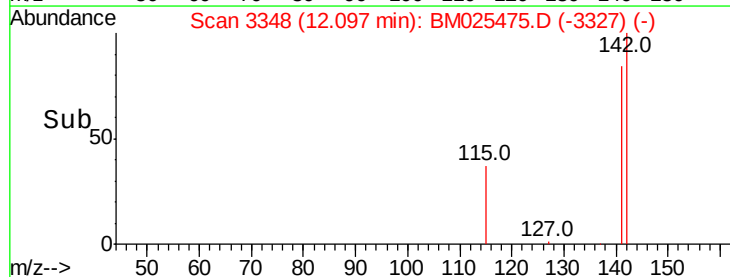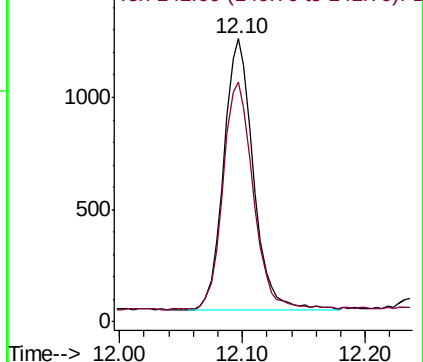

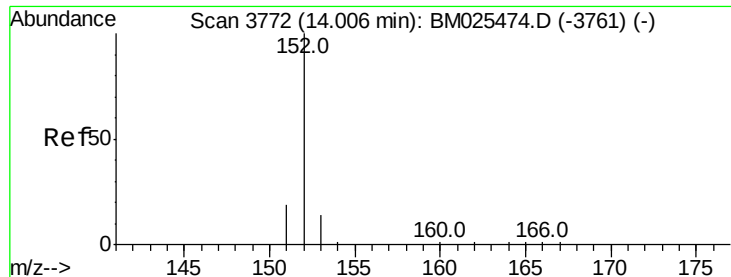

#7

Acenaphthylene

Concen: 0.301 ng/ul

RT: 14.00 min Scan# 3772

Delta R.T. -0.00 min

Lab File: BM025475.D

Acq: 11 Mar 2020 05:22

Instrument :

BNA_M

ClientSampleId :





Tot Ion:152 Resp: 11442

Ion Ratio Lower Upper

152 100

151 19.8 16.2 24.2

153 13.6 10.6 16.0

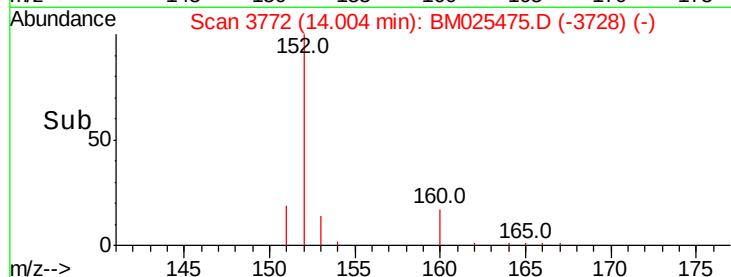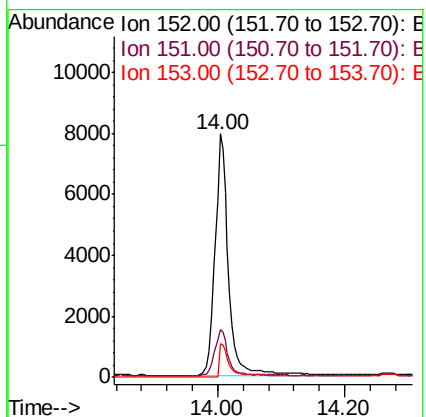

#8

Acenaphthene

Concen: 0.397 ng/ul

RT: 14.35 min Scan# 3863

Delta R.T. -0.00 min

Lab File: BM025475.D

Acq: 11 Mar 2020 05:22




Tgt Ion:153 Resp: 13230


Ion Ratio Lower Upper

153 100

152 49.2 39.5 59.3

154 90.8 71.7 107.5


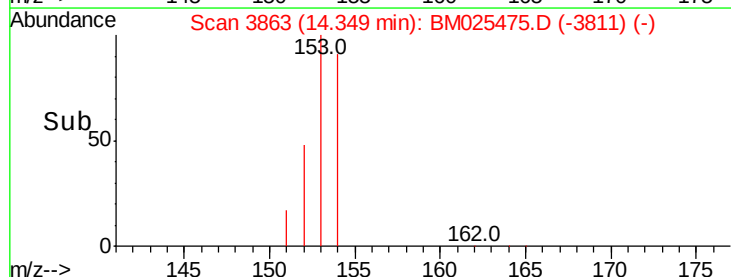
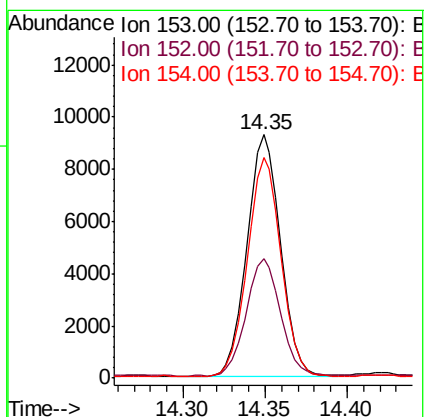



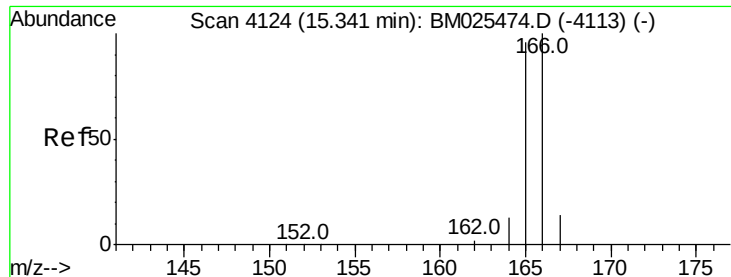

#9
Fluorene
 Concen: 0.467 ng/ul
 RT: 15.34 min Scan# 4124
 Delta R.T. -0.00 min
 Lab File: BM025475.D
 Acq: 11 Mar 2020 05:22




Instrument :
 BNA_M
 ClientSampleId :


Tot Ion:166 Resp: 18981
 Ion Ratio Lower Upper
 166 100
 165 95.6 76.8 115.2
 167 13.9 11.2 16.8

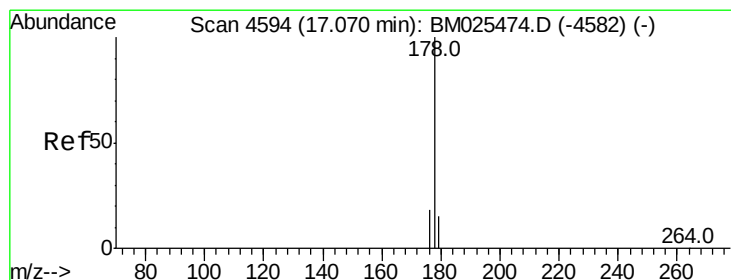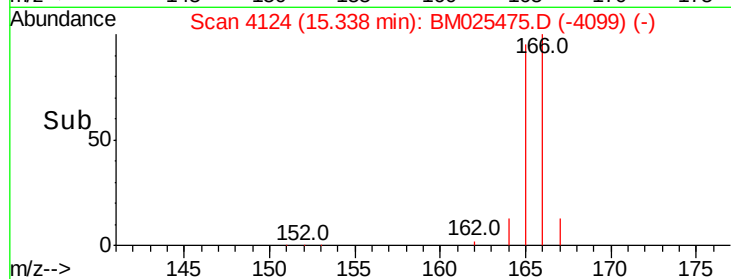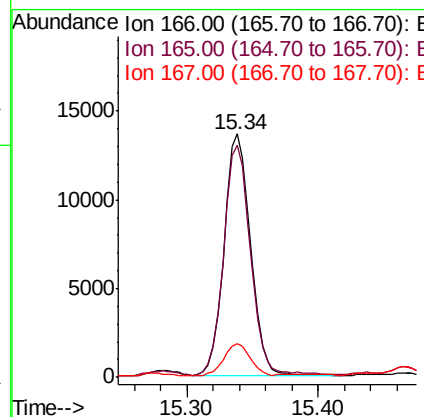

#12
Phenanthrene
 Concen: 1.820 ng/ul
 RT: 17.07 min Scan# 4595
 Delta R.T. -0.00 min
 Lab File: BM025475.D
 Acq: 11 Mar 2020 05:22

Tgt Ion:178 Resp: 125553
 Ion Ratio Lower Upper
 178 100
 179 15.3 12.4 18.6
 176 18.3 14.8 22.2


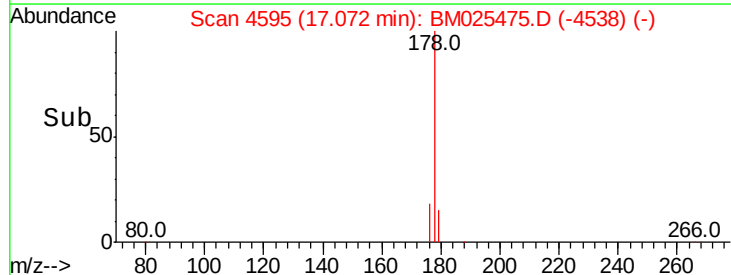
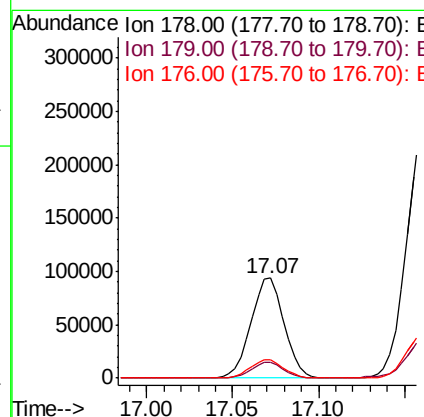



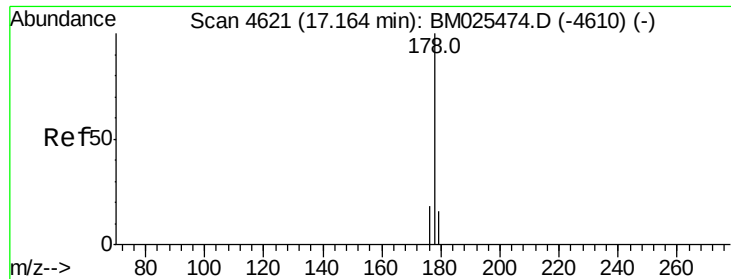

#13
 Anthracene
 Concen: 5.227 ng/ul
 RT: 17.16 min Scan# 4621
 Delta R.T. -0.00 min
 Lab File: BM025475.D
 Acq: 11 Mar 2020 05:22




Instrument :
 BNA_M
 ClientSampleId :


Tot Ion:178 Resp: 313826
 Ion Ratio Lower Upper
 178 100
 179 15.4 12.6 18.8
 176 17.6 14.5 21.7

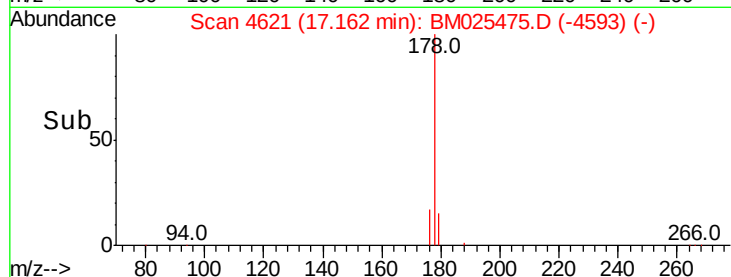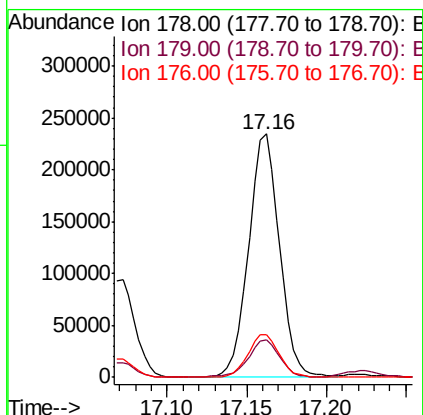

#15
 Fluoranthene
 Concen: 8.515 ng/ul
 RT: 19.09 min Scan# 5161
 Delta R.T. -0.00 min
 Lab File: BM025475.D
 Acq: 11 Mar 2020 05:22

Tgt Ion:202 Resp: 636831
 Ion Ratio Lower Upper
 202 100
 101 7.7 0.0 27.5
 100 6.0 0.0 26.0

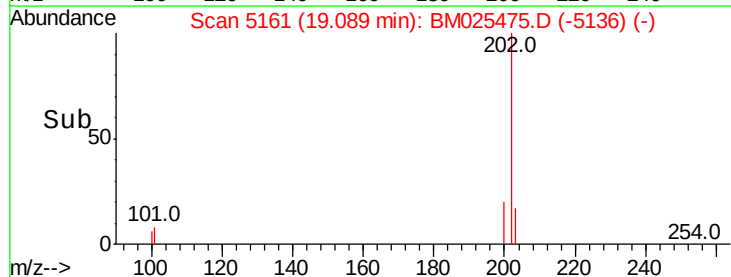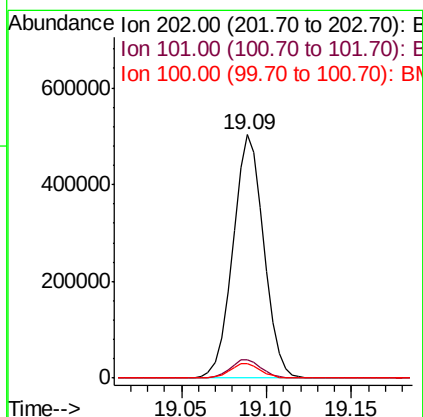

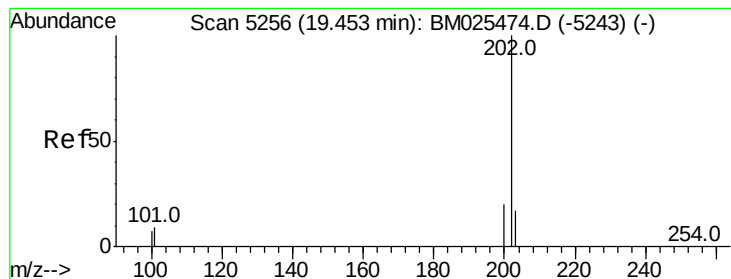

#17

Pvrene

Concen: 8.320 ng/ul

RT: 19.45 min Scan# 5256

Delta R.T. -0.00 min

Lab File: BM025475.D

Acq: 11 Mar 2020 05:22

Instrument :

BNA_M

ClientSampleId :


Tot Ion:202 Resp: 753576

Ion Ratio Lower Upper

202 100

101 9.0 7.1 10.7




100 7.4 6.0 9.0



Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B

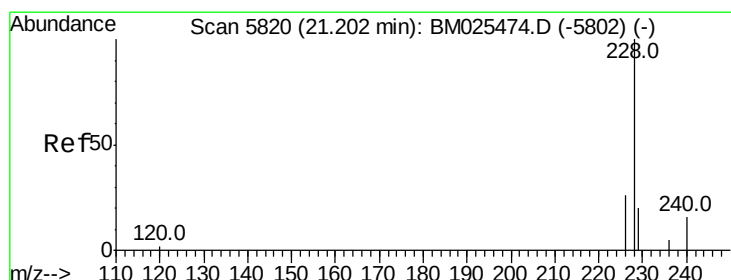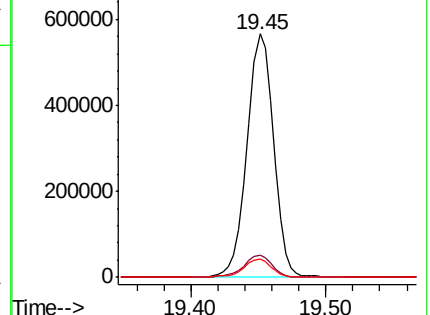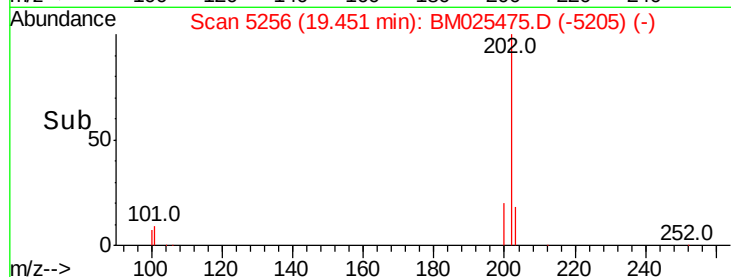

#18

Benzo(a)anthracene

Concen: 4.865 ng/ul

RT: 21.20 min Scan# 5821

Delta R.T. -0.00 min

Lab File: BM025475.D

Acq: 11 Mar 2020 05:22


Tgt Ion:228 Resp: 350993

Ion Ratio Lower Upper

228 100

229 21.2 15.6 23.4



226 27.4 21.1 31.7




Abundance Ion 228.00 (227.70 to 228.70): E

Ion 229.00 (228.70 to 229.70): E

Ion 226.00 (225.70 to 226.70): E

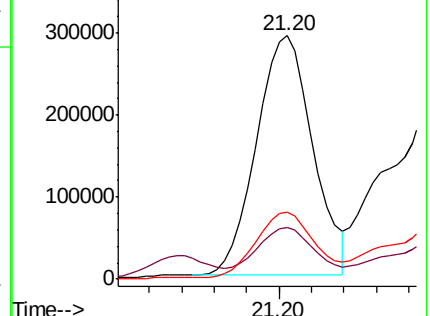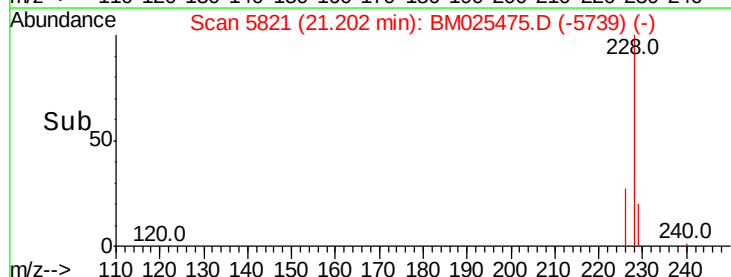

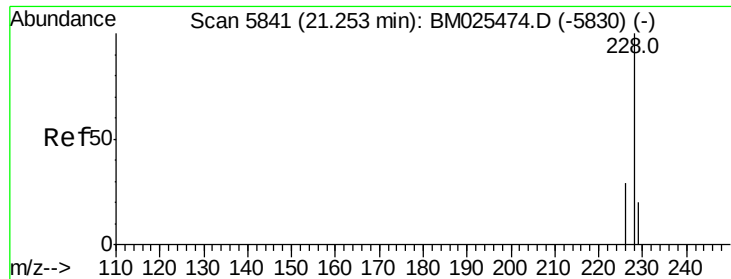

#19

Chrysene

Concen: 6.293 ng/ul

RT: 21.25 min Scan# 5842

Delta R.T. -0.00 min

Lab File: BM025475.D

Acq: 11 Mar 2020 05:22

Instrument :

BNA_M

ClientSampleId :


Tot Ion:228 Resp: 509858

Ion Ratio Lower Upper

228 100

226 28.9 23.6 35.4




229 21.4 16.3 24.5

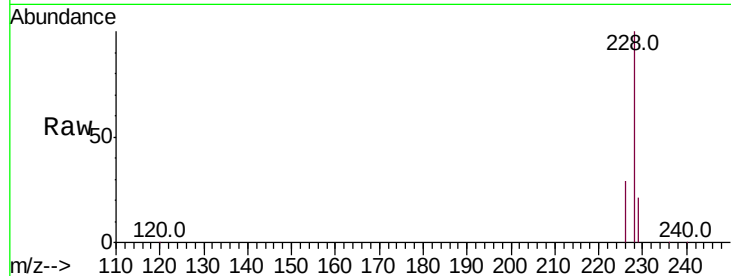

Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

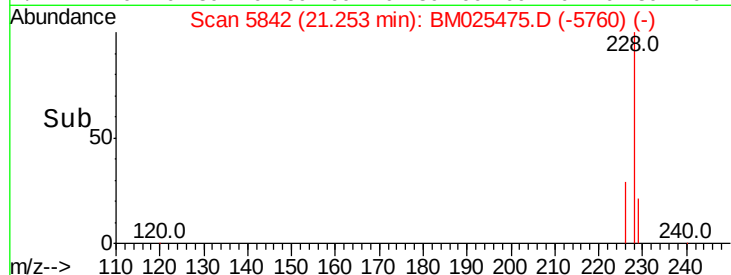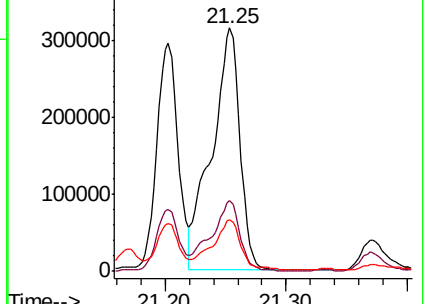

#21

Benzo(b)fluoranthene

Concen: 8.390 ng/ul m

RT: 22.75 min Scan# 6462

Delta R.T. -0.00 min

Lab File: BM025475.D

Acq: 11 Mar 2020 05:22


Tgt Ion:252 Resp: 677188

Ion Ratio Lower Upper

252 100

253 22.7 0.0 50.2



125 7.3 0.0 17.6




Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E



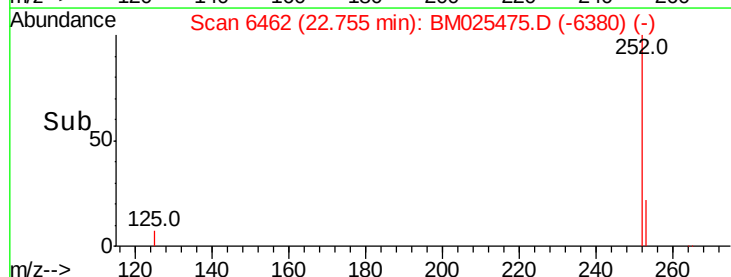
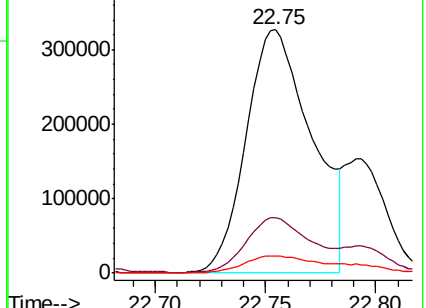


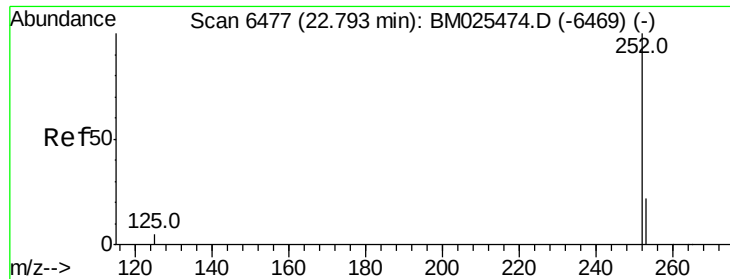

#22
Benzo(k)fluoranthene
Concen: 2.302 ng/ul m
RT: 22.79 min Scan# 6478
Delta R.T. -0.01 min
Lab File: BM025475.D
Acq: 11 Mar 2020 05:22




Instrument :
BNA_M
ClientSampleId :


Tot Ion:252 Resp: 194712
Ion Ratio Lower Upper
252 100
253 23.9 19.8 29.8
125 7.4 7.1 10.7

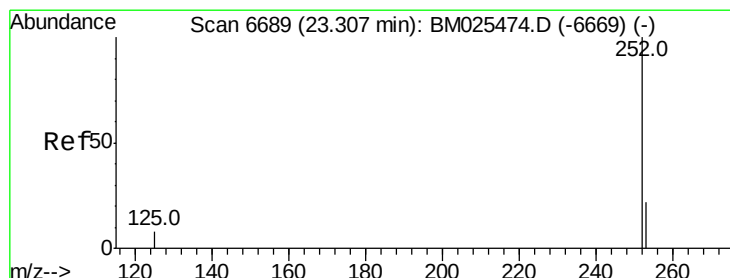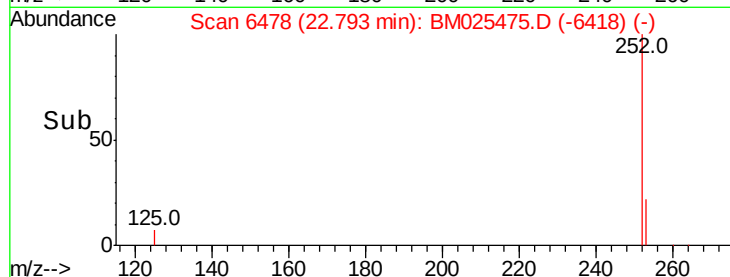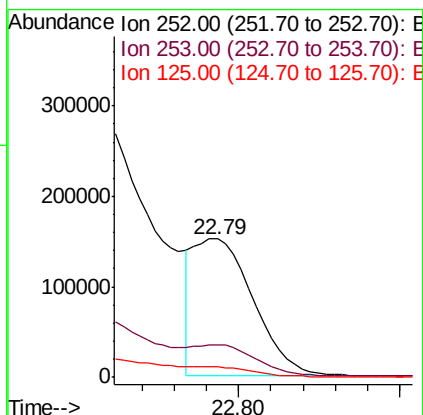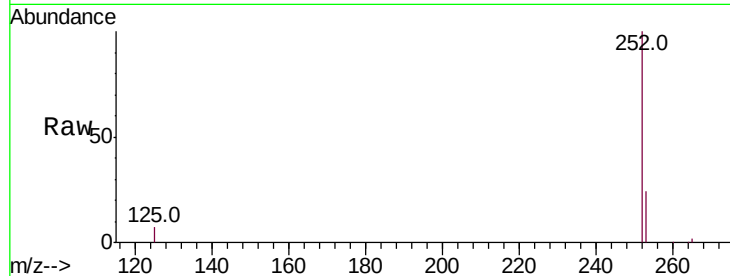

#23
Benzo(a)pyrene
Concen: 4.094 ng/ul m
RT: 23.30 min Scan# 6689
Delta R.T. -0.01 min
Lab File: BM025475.D
Acq: 11 Mar 2020 05:22

Tgt Ion:252 Resp: 274405
Ion Ratio Lower Upper
252 100
253 23.1 21.3 31.9
125 7.8 8.5 12.7#

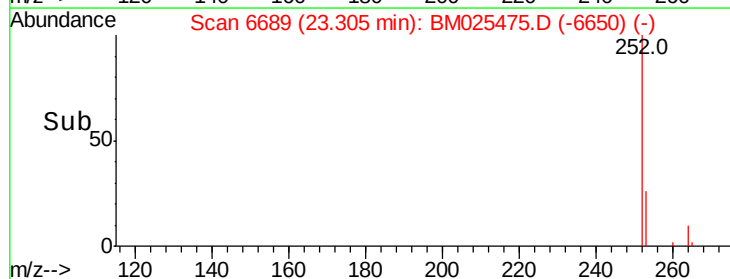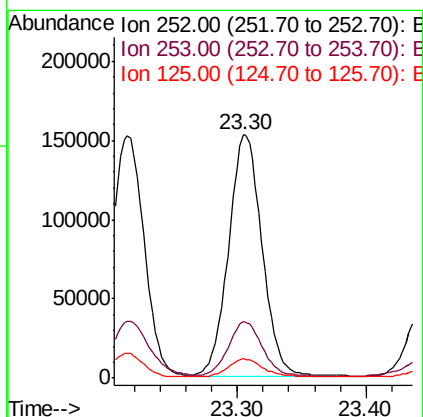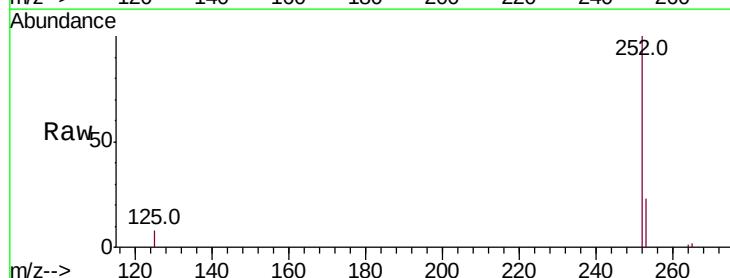




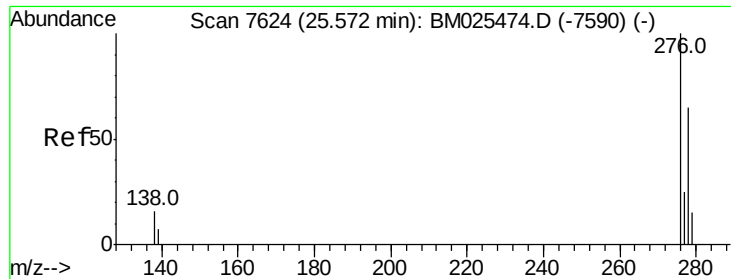


#24

Indeno(1,2,3-cd)pyrene
Concen: 1.893 ng/ul
RT: 25.57 min Scan# 7624
Delta R.T. -0.01 min
Lab File: BM025475.D
Acq: 11 Mar 2020 05:22

Instrument :
BNA_M
ClientSampleId :




Tot Ion:276 Resp: 172161
Ion Ratio Lower Upper
276 100
138 15.2 12.3 18.5
227 0.0 0.0 0.0

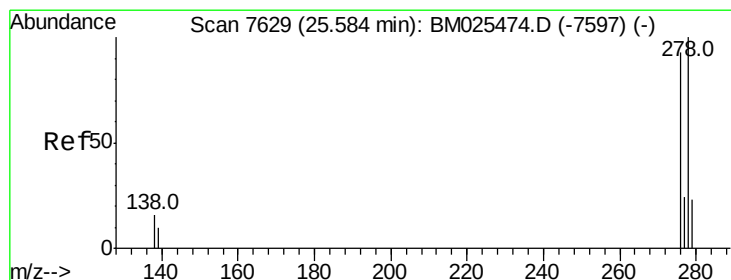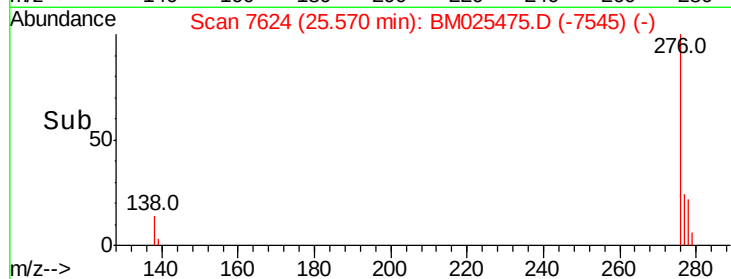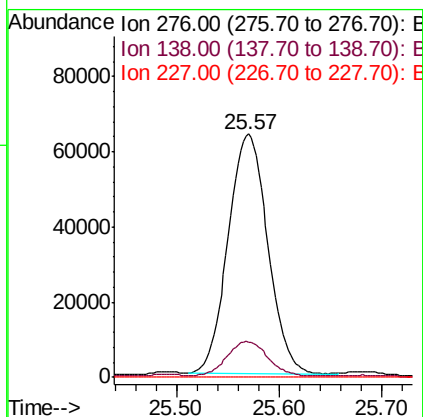


#25

Dibenzo(a,h)anthracene
Concen: 0.614 ng/ul
RT: 25.58 min Scan# 7627
Delta R.T. -0.02 min
Lab File: BM025475.D
Acq: 11 Mar 2020 05:22

Tgt Ion:278 Resp: 47006
Ion Ratio Lower Upper
278 100
139 12.7 9.0 13.6
279 28.7 21.1 31.7

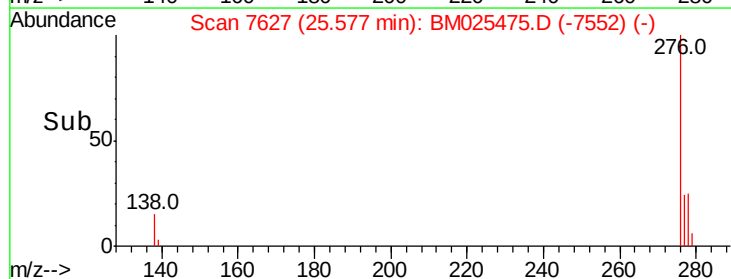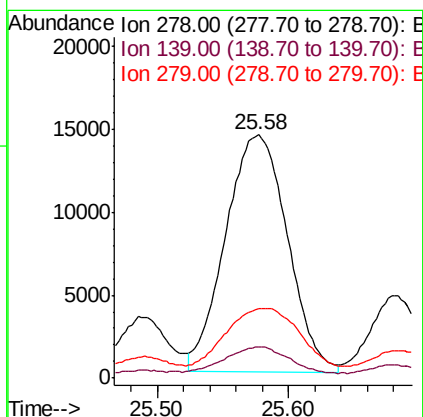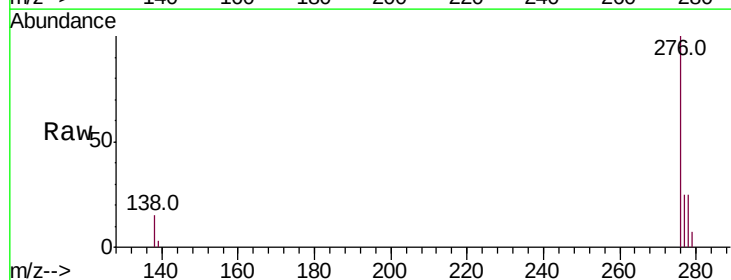

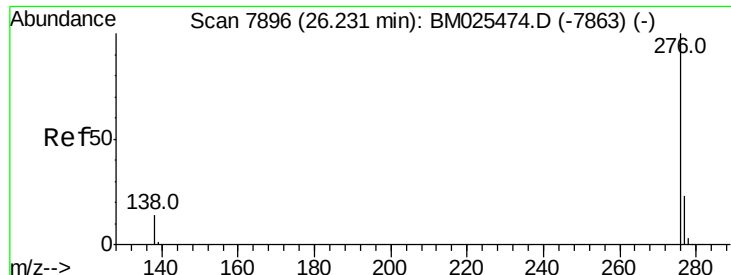

#26

Benzo(a,h,i)perylene

Concen: 1.388 ng/ul

RT: 26.23 min Scan# 7897

Delta R.T. -0.01 min

Lab File: BM025475.D

Acq: 11 Mar 2020 05:22

Instrument :

BNA_M

ClientSampleId :


Tot Ion:276 Resp: 109519

Ion Ratio Lower Upper

276 100

138 15.1 11.0 16.4

277 23.9 19.8 29.6

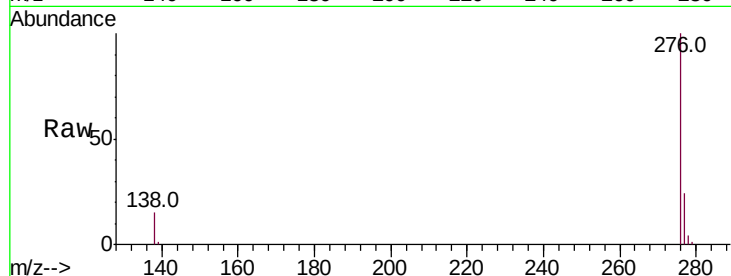

Abundance Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 277.00 (276.70 to 277.70): E

