
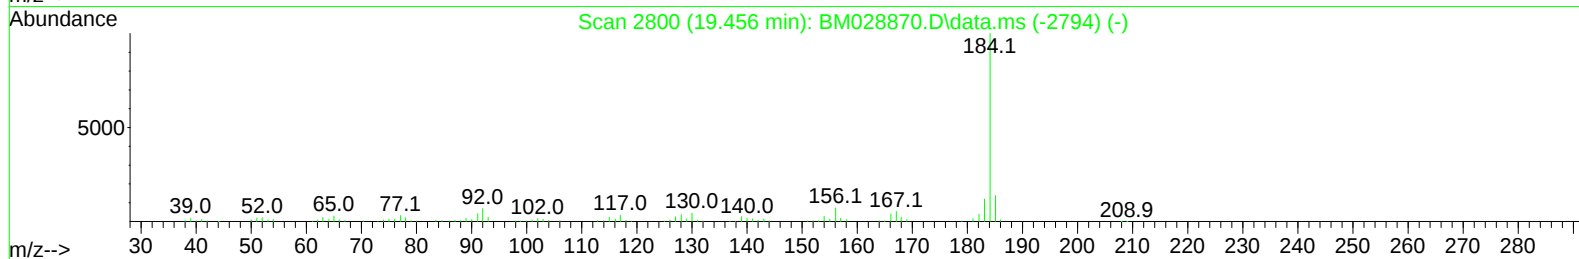
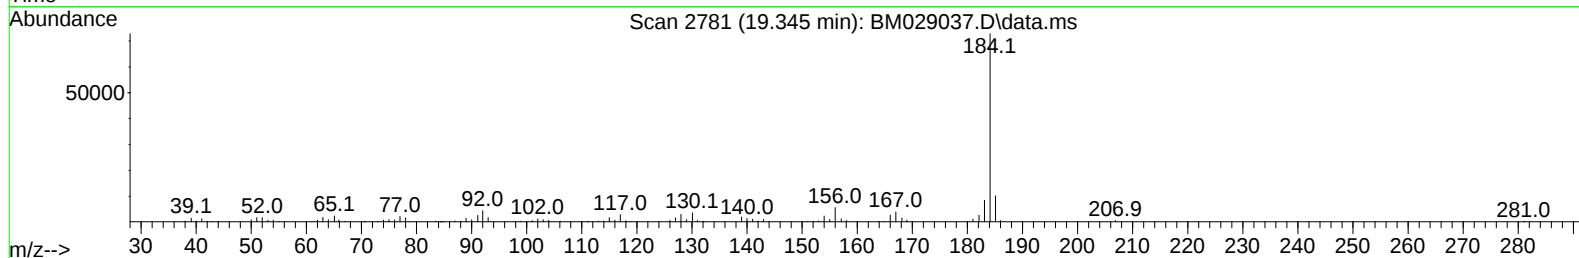


```
Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030921\  
Data File : BM029037.D  
Acq On    : 09 Mar 2021  08:52  
Operator  : CG/JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Quant Time: Mar 09 09:59:36 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM022321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 05 13:17:12 2021
Response via : Initial Calibration

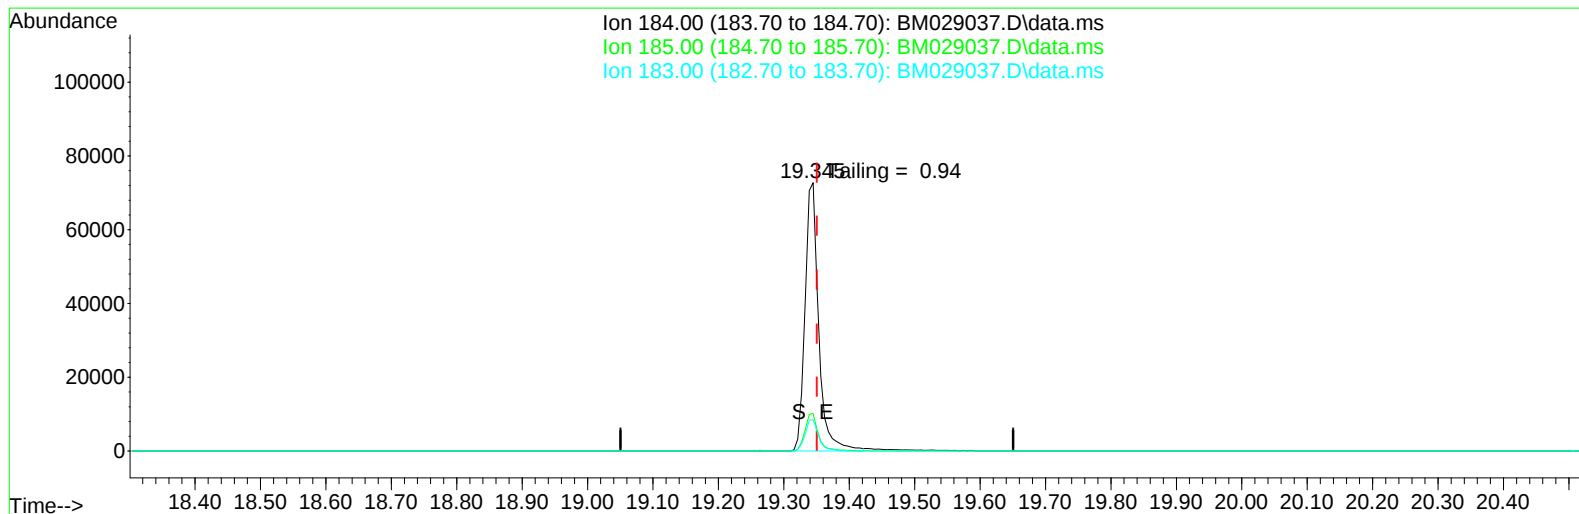

TIC: BM029037.D\data.ms

(77) Benzidine




19.345min (-0.006) 0.00 ng

response **107394**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.80	13.97
183.00	12.10	11.63
0.00	0.00	0.00

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030921\  
Data File : BM029037.D  
Acq On    : 09 Mar 2021  08:52  
Operator  : CG/JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Quant Time: Mar 09 09:59:36 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM022321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 05 13:17:12 2021
Response via : Initial Calibration

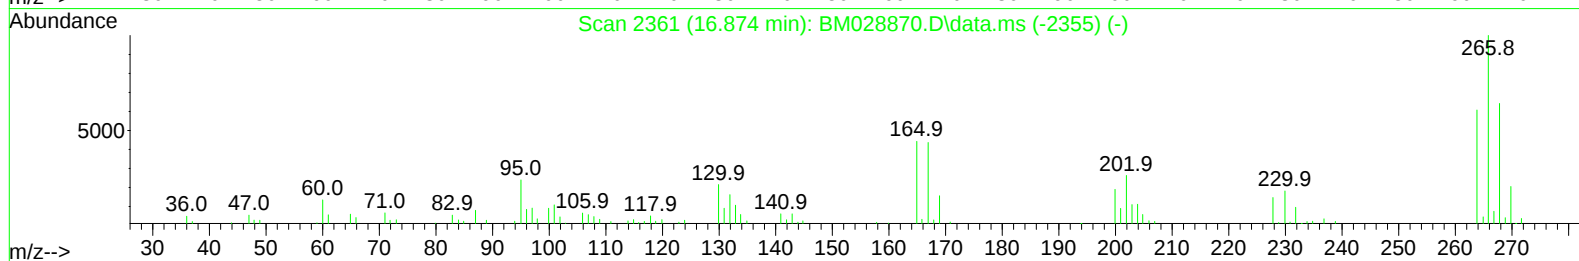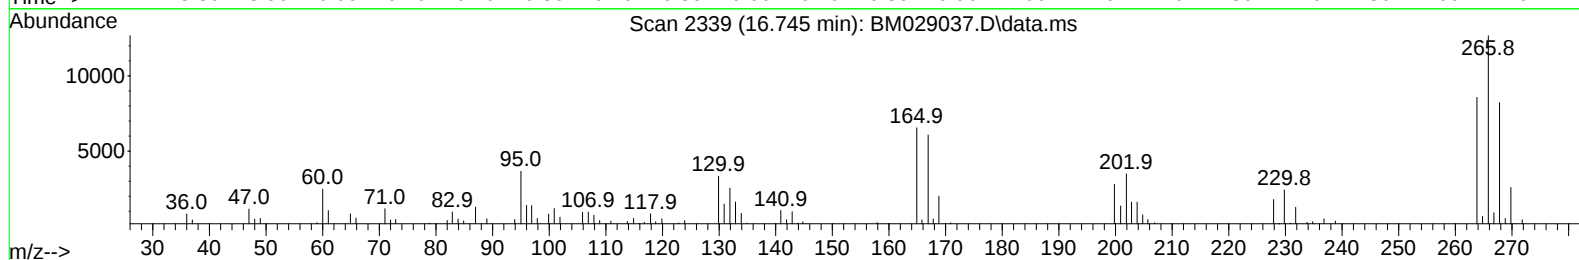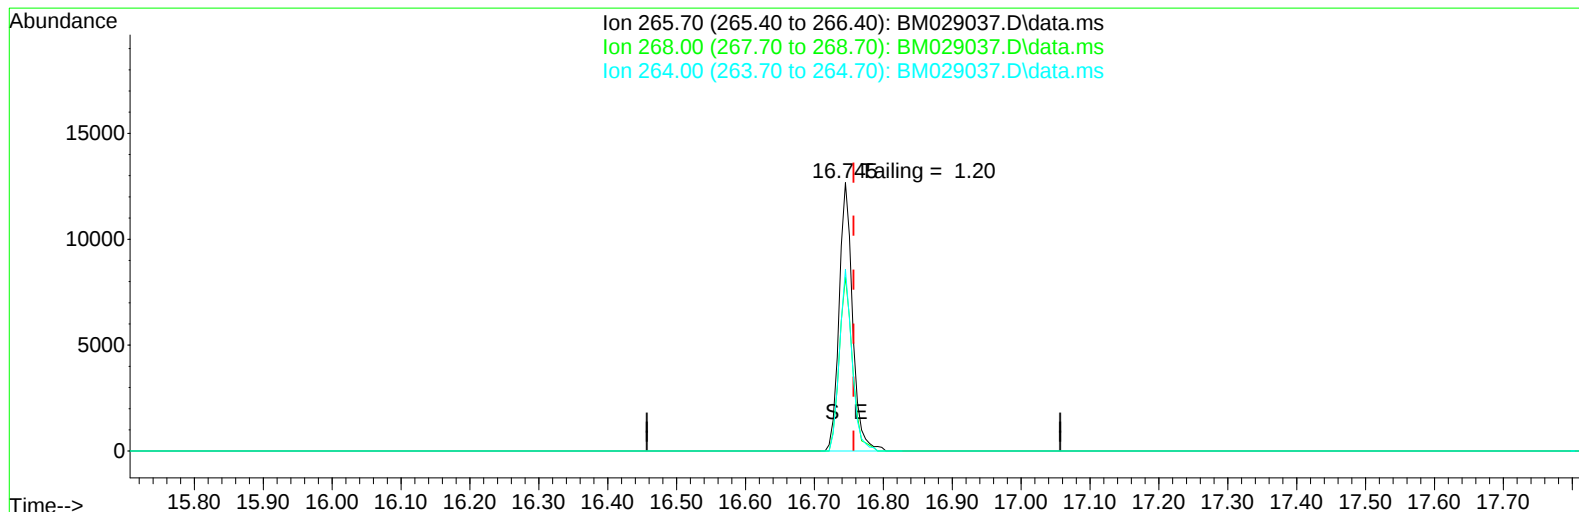

TIC: BM029037.D\data.ms

(70) Pentachlorophenol (C)

16.745min (-0.012) 0.00 ng

response **17207**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.40	64.87
264.00	63.30	67.70
0.00	0.00	0.00