
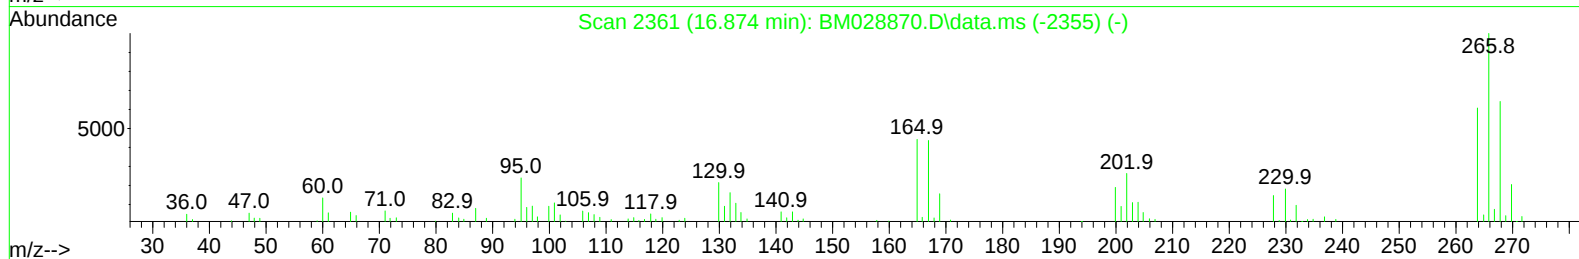
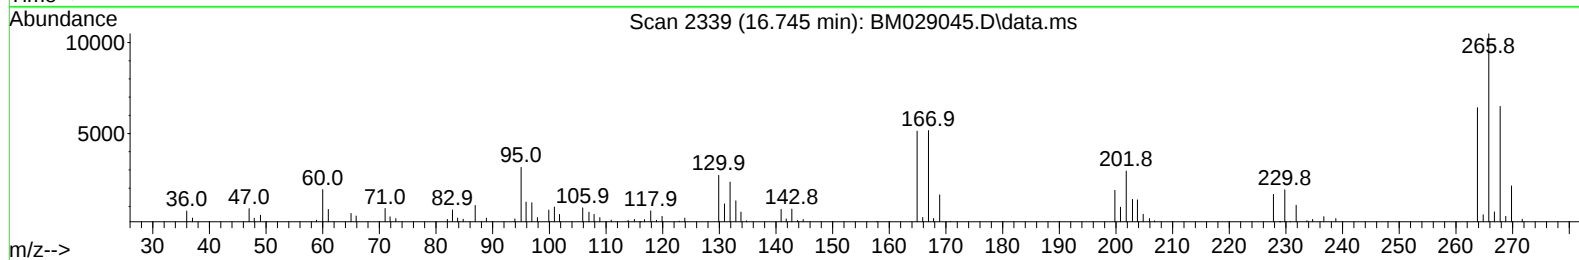


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030921\
Data File : BM029045.D
Acq On : 09 Mar 2021 14:31
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 09 15:35:15 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM022321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 09 10:08:02 2021
Response via : Initial Calibration

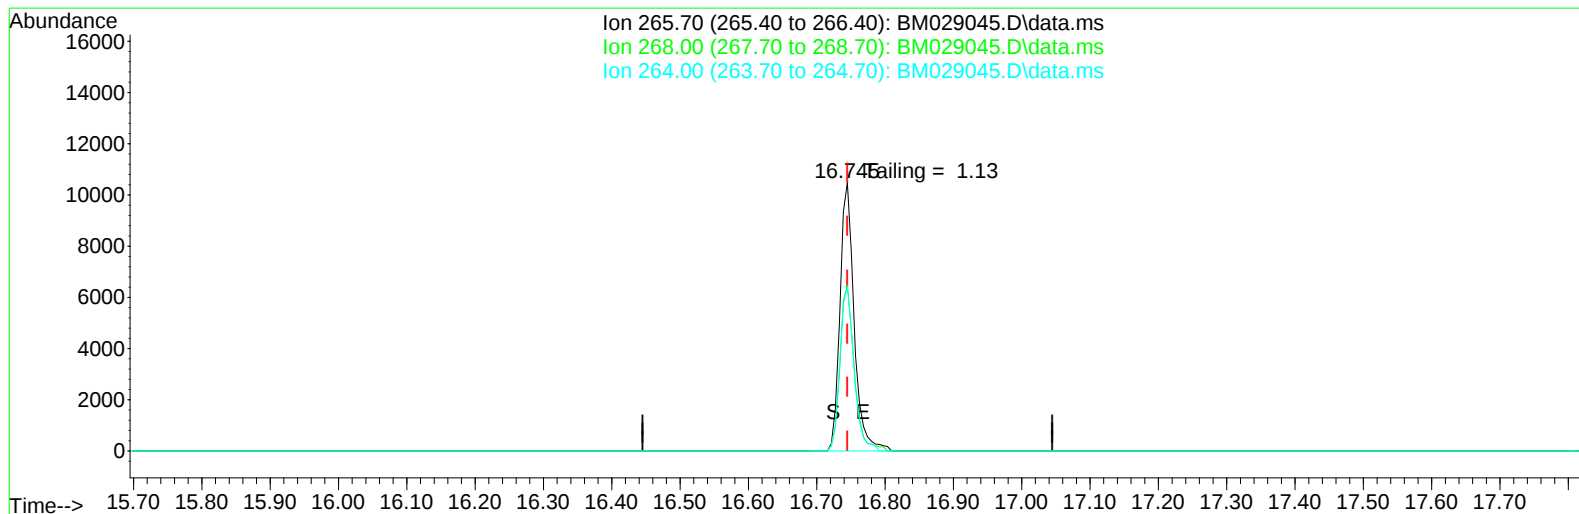

TIC: BM029045.D\data.ms

(70) Pentachlorophenol (C)




16.745min (-0.000) 0.00 ng

response 15109

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.40	61.90
264.00	63.30	61.24
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030921\
 Data File : BM029045.D
 Acq On : 09 Mar 2021 14:31
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 09 15:35:15 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM022321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Mar 09 10:08:02 2021
 Response via : Initial Calibration

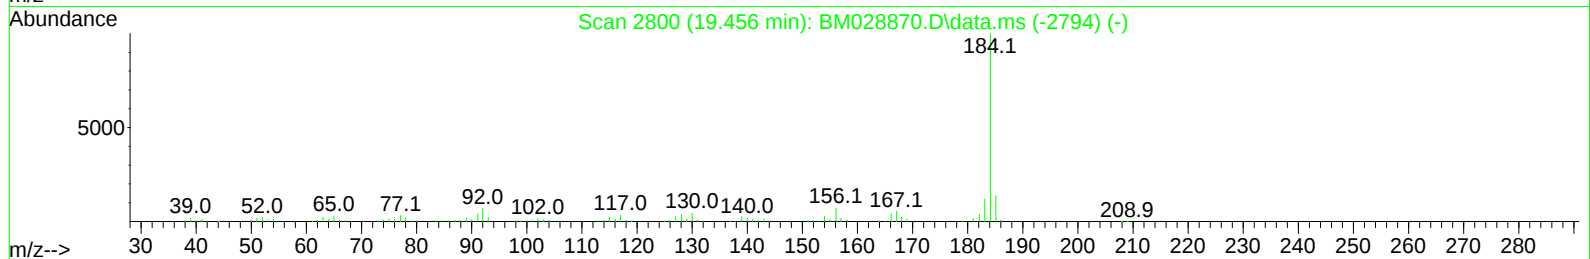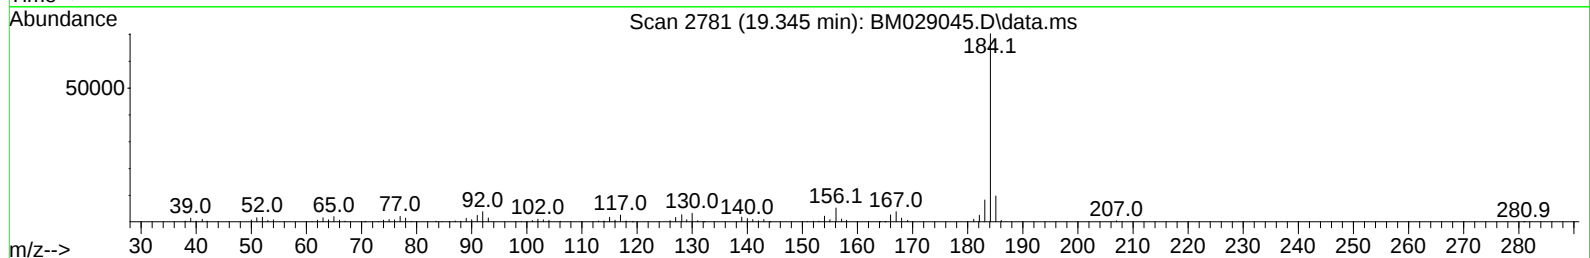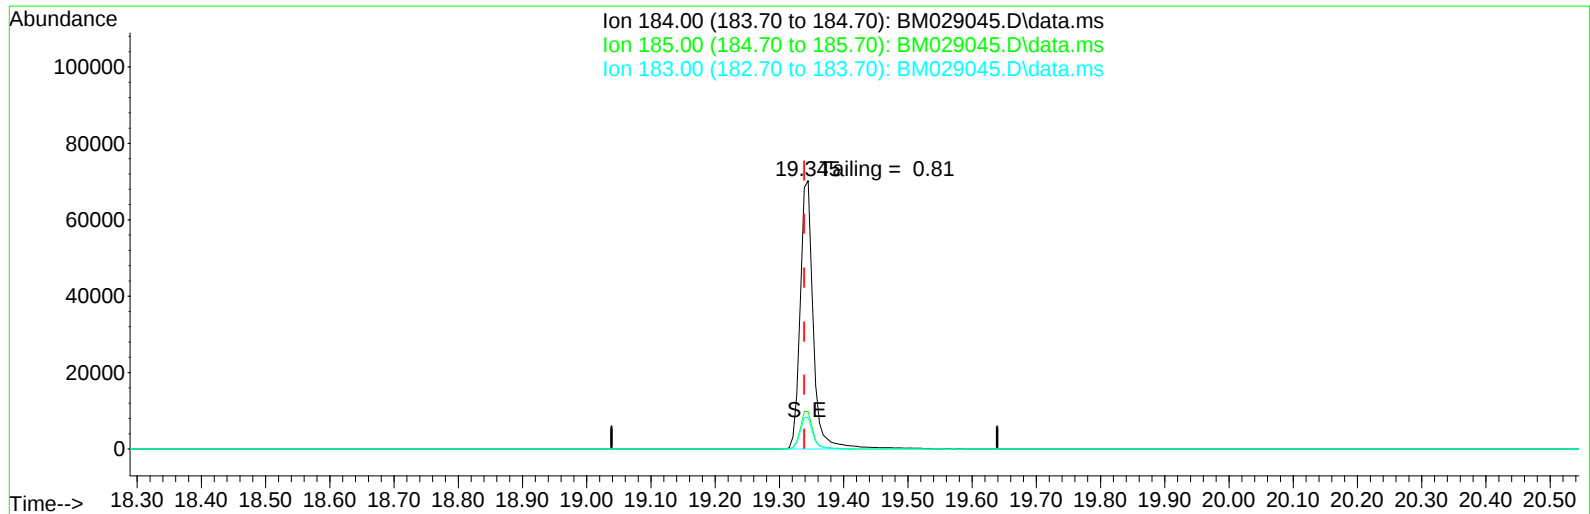

TIC: BM029045.D\data.ms

(77) Benzidine

19.345min (+ 0.006) 0.00 ng

response 100104

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.80	13.95
183.00	12.10	11.78
0.00	0.00	0.00