

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM030921\  
 Data File : BM029039.D  
 Acq On : 09 Mar 2021 10:04  
 Operator : CG/JU  
 Sample : PB135024BL  
 Misc :  
 ALS Vial : 3 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 ClientSampleId :  
 PB135024BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM022321.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM029039.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 5.246       | 378           | 384         | 394          | rBV      | 228755         | 317808        | 54.97%          | 12.296%       |
| 2         | 6.869       | 654           | 660         | 675          | rBV      | 204588         | 309001        | 53.45%          | 11.955%       |
| 3         | 7.669       | 791           | 796         | 802          | rBB      | 37981          | 55213         | 9.55%           | 2.136%        |
| 4         | 8.845       | 989           | 996         | 1007         | rBV      | 125292         | 197757        | 34.21%          | 7.651%        |
| 5         | 10.463      | 1265          | 1271        | 1279         | rBB      | 44416          | 68791         | 11.90%          | 2.662%        |
| 6         | 12.951      | 1688          | 1694        | 1705         | rBV      | 273470         | 385224        | 66.64%          | 14.905%       |
| 7         | 14.339      | 1924          | 1930        | 1935         | rBB      | 57370          | 80063         | 13.85%          | 3.098%        |
| 8         | 15.839      | 2179          | 2185        | 2194         | rBV      | 199484         | 280059        | 48.44%          | 10.836%       |
| 9         | 17.086      | 2391          | 2397        | 2406         | rBB      | 68270          | 88676         | 15.34%          | 3.431%        |
| 10        | 19.709      | 2838          | 2843        | 2848         | rBV      | 491057         | 578102        | 100.00%         | 22.367%       |
| 11        | 21.256      | 3102          | 3106        | 3111         | rBV      | 86279          | 109052        | 18.86%          | 4.219%        |
| 12        | 23.415      | 3468          | 3473        | 3481         | rBV2     | 65480          | 114857        | 19.87%          | 4.444%        |




Sum of corrected areas: 2584603

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM030921\  
Data File : BM029039.D  
Acq On : 09 Mar 2021 10:04  
Operator : CG/JU  
Sample : PB135024BL  
Misc :  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
PB135024BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM022321.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

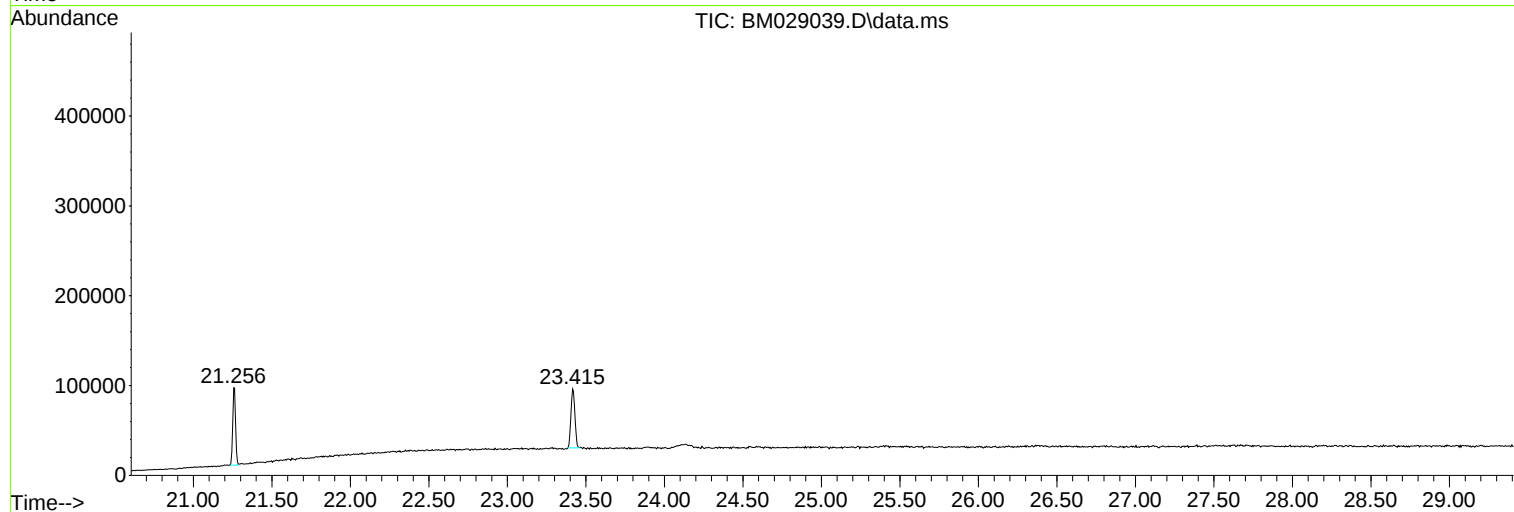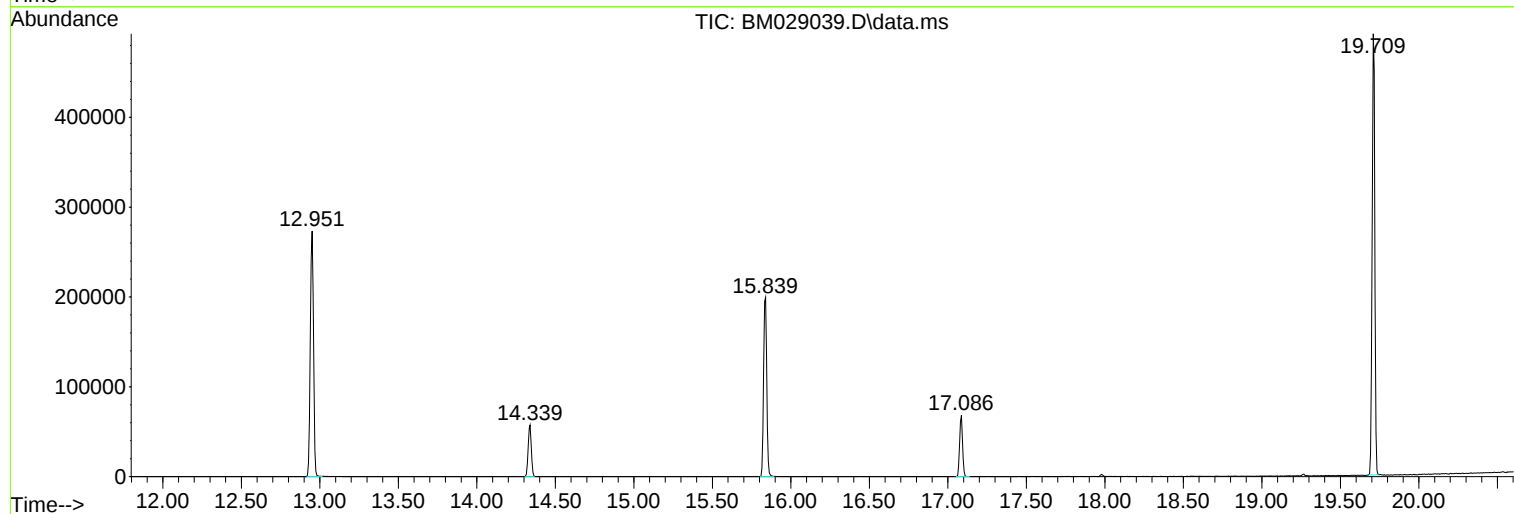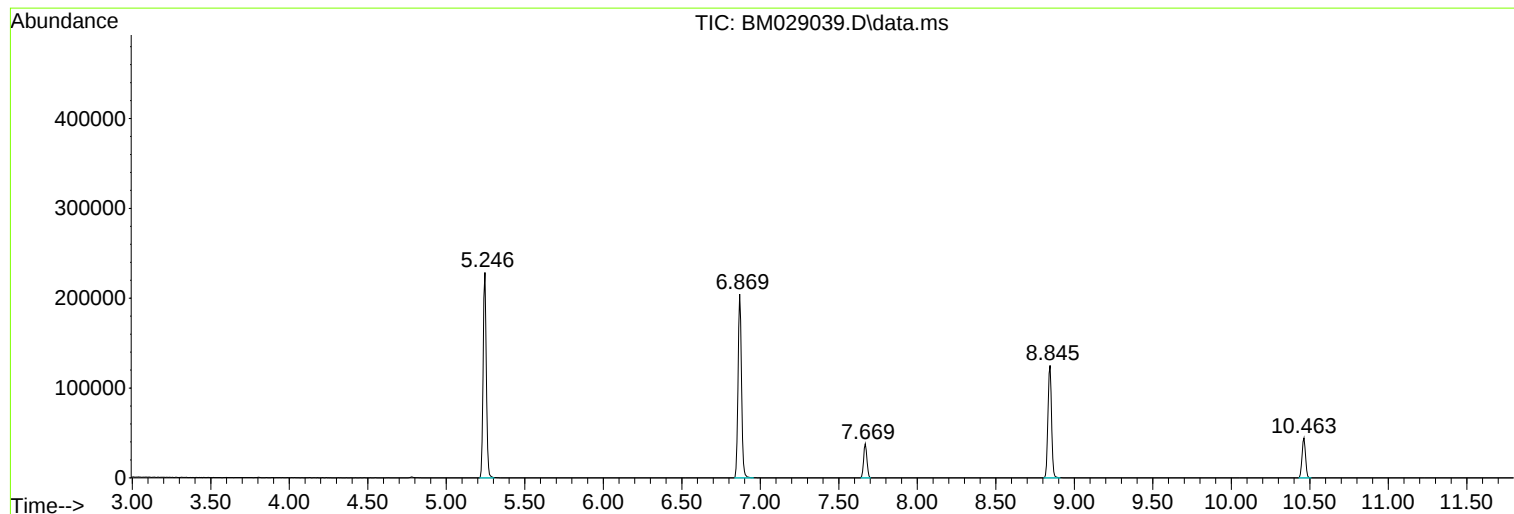

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM030921\  
Data File : BM029039.D  
Acq On : 09 Mar 2021 10:04  
Operator : CG/JU  
Sample : PB135024BL  
Misc :  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
PB135024BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM022321.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM030921\  
Data File : BM029039.D  
Acq On : 09 Mar 2021 10:04  
Operator : CG/JU  
Sample : PB135024BL  
Misc :  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
PB135024BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM022321.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | # | RT | Resp | Conc |
|------------------|----|---------|-------|----------|---|----|------|------|
|------------------|----|---------|-------|----------|---|----|------|------|