

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030921\
 Data File : BM029047.D
 Acq On : 09 Mar 2021 15:44
 Operator : CG/JU
 Sample : PB135064BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB135064BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM022321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM029047.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.246	378	384	398	rBV	196224	282744	49.61%	11.326%
2	6.869	654	660	678	rBV	177674	275397	48.32%	11.032%
3	7.669	791	796	803	rBB	37298	54665	9.59%	2.190%
4	8.845	989	996	1008	rBV	109915	176163	30.91%	7.057%
5	10.463	1264	1271	1280	rBB	46339	74149	13.01%	2.970%
6	12.951	1687	1694	1705	rBV	246605	355346	62.35%	14.234%
7	14.333	1924	1929	1936	rBB	63990	91238	16.01%	3.655%
8	15.833	2179	2184	2196	rBB	200859	268467	47.10%	10.754%
9	17.086	2391	2397	2407	rBB	74872	105431	18.50%	4.223%
10	19.709	2838	2843	2848	rBV	491868	569967	100.00%	22.831%
11	21.256	3102	3106	3111	rBV	106476	124308	21.81%	4.979%
12	23.415	3467	3473	3482	rVB2	67115	118576	20.80%	4.750%




Sum of corrected areas: 2496451

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030921\
Data File : BM029047.D
Acq On : 09 Mar 2021 15:44
Operator : CG/JU
Sample : PB135064BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB135064BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM022321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

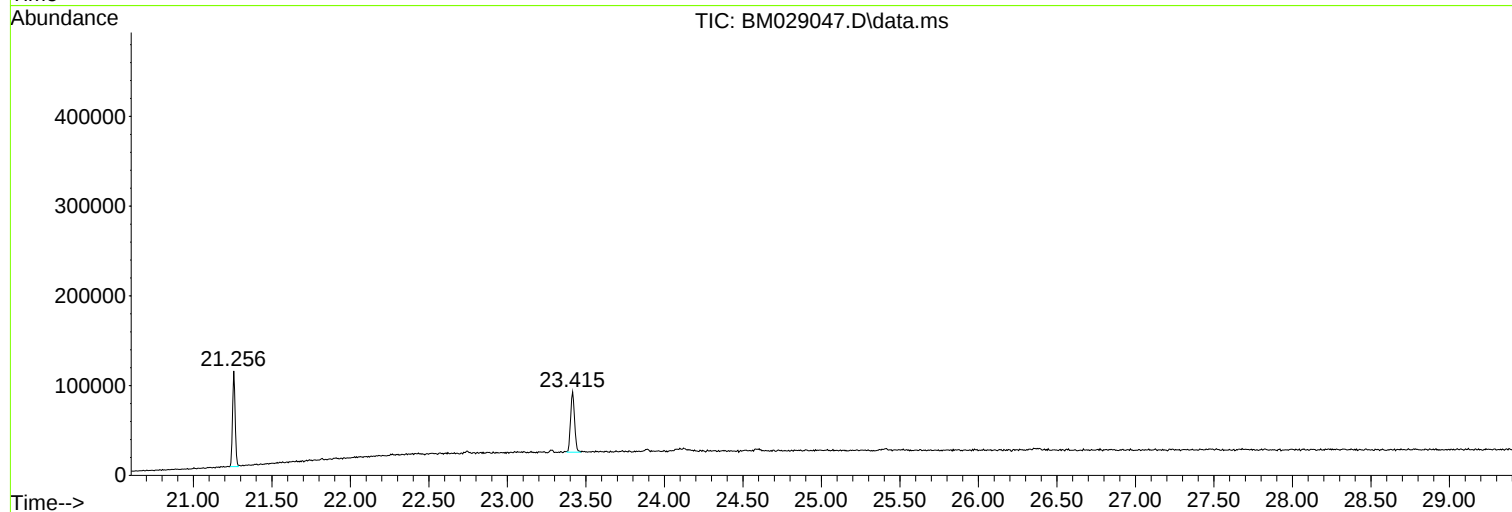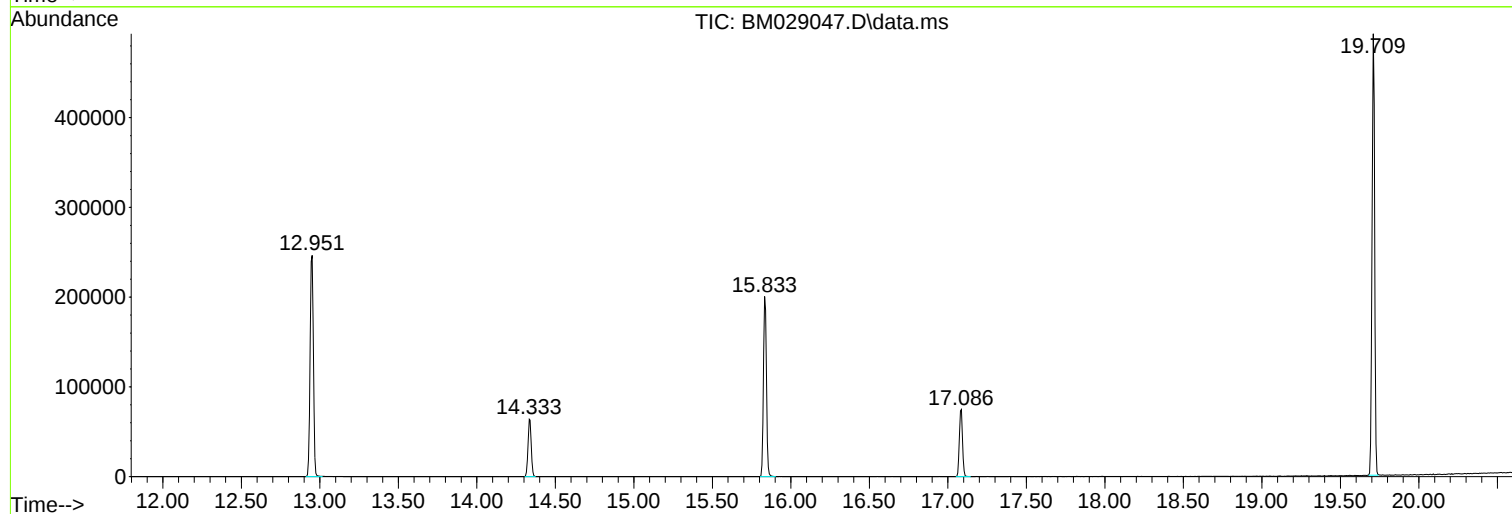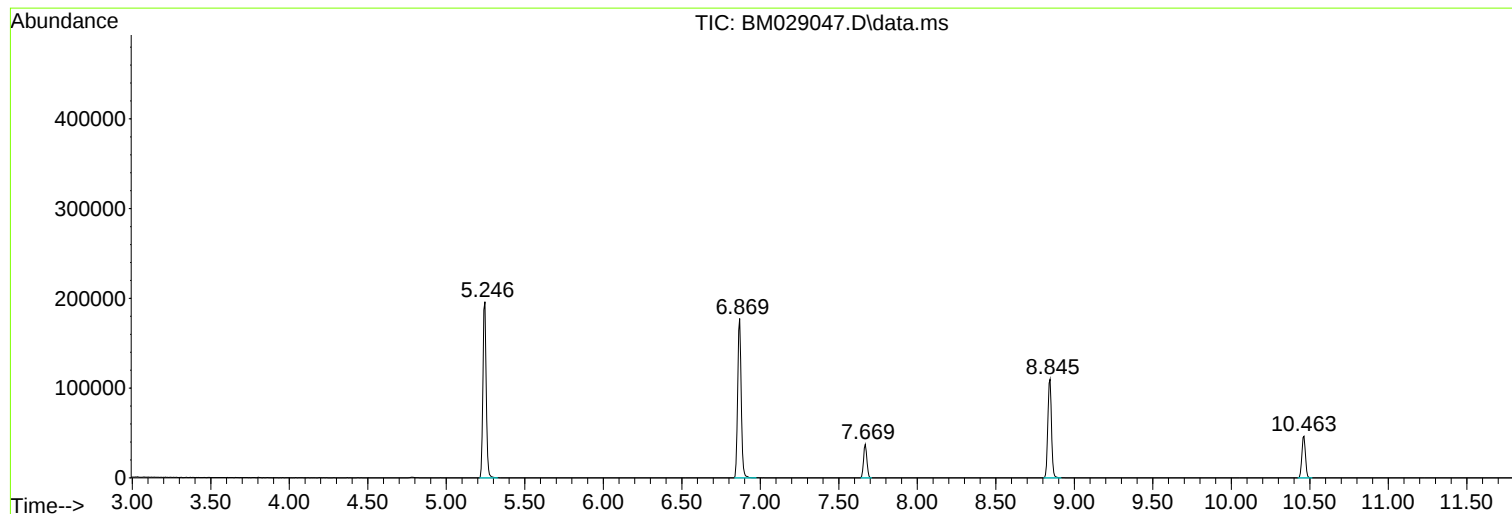

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030921\
Data File : BM029047.D
Acq On : 09 Mar 2021 15:44
Operator : CG/JU
Sample : PB135064BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB135064BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM022321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030921\
Data File : BM029047.D
Acq On : 09 Mar 2021 15:44
Operator : CG/JU
Sample : PB135064BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB135064BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM022321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------