

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030923\
 Data File : BM038941.D
 Acq On : 09 Mar 2023 12:14
 Operator : CG/JU
 Sample : PB151257BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Mar 09 13:33:03 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM030323.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Mar 03 22:01:14 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.995	152	11306	0.400	ng/ul	-0.01
4) Naphthalene-d8	10.806	136	39298	0.400	ng/ul	-0.02
9) Acenaphthene-d10	14.633	164	22810	0.400	ng/ul	-0.01
13) Phenanthrene-d10	17.375	188	44621	0.400	ng/ul	-0.01
17) Chrysene-d12	21.553	240	34750	0.400	ng/ul	0.00
23) Perylene-d12	23.997	264	27377	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.375	96	70711	5.527	ng/ul	-0.01
6) 2-Methylnaphthalene-d10	12.395	152	13699	0.288	ng/ul	-0.01
18) Fluoranthene-d10	19.398	212	26075	0.315	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.765	202	4908	0.041	ng/ul#	1
26) Benzo(a)pyrene	23.844	252	7451	0.087	ng/ul#	56

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030923\
Data File : BM038941.D
Acq On : 09 Mar 2023 12:14
Operator : CG/JU
Sample : PB151257BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Mar 09 13:33:03 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM030323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 03 22:01:14 2023
Response via : Initial Calibration

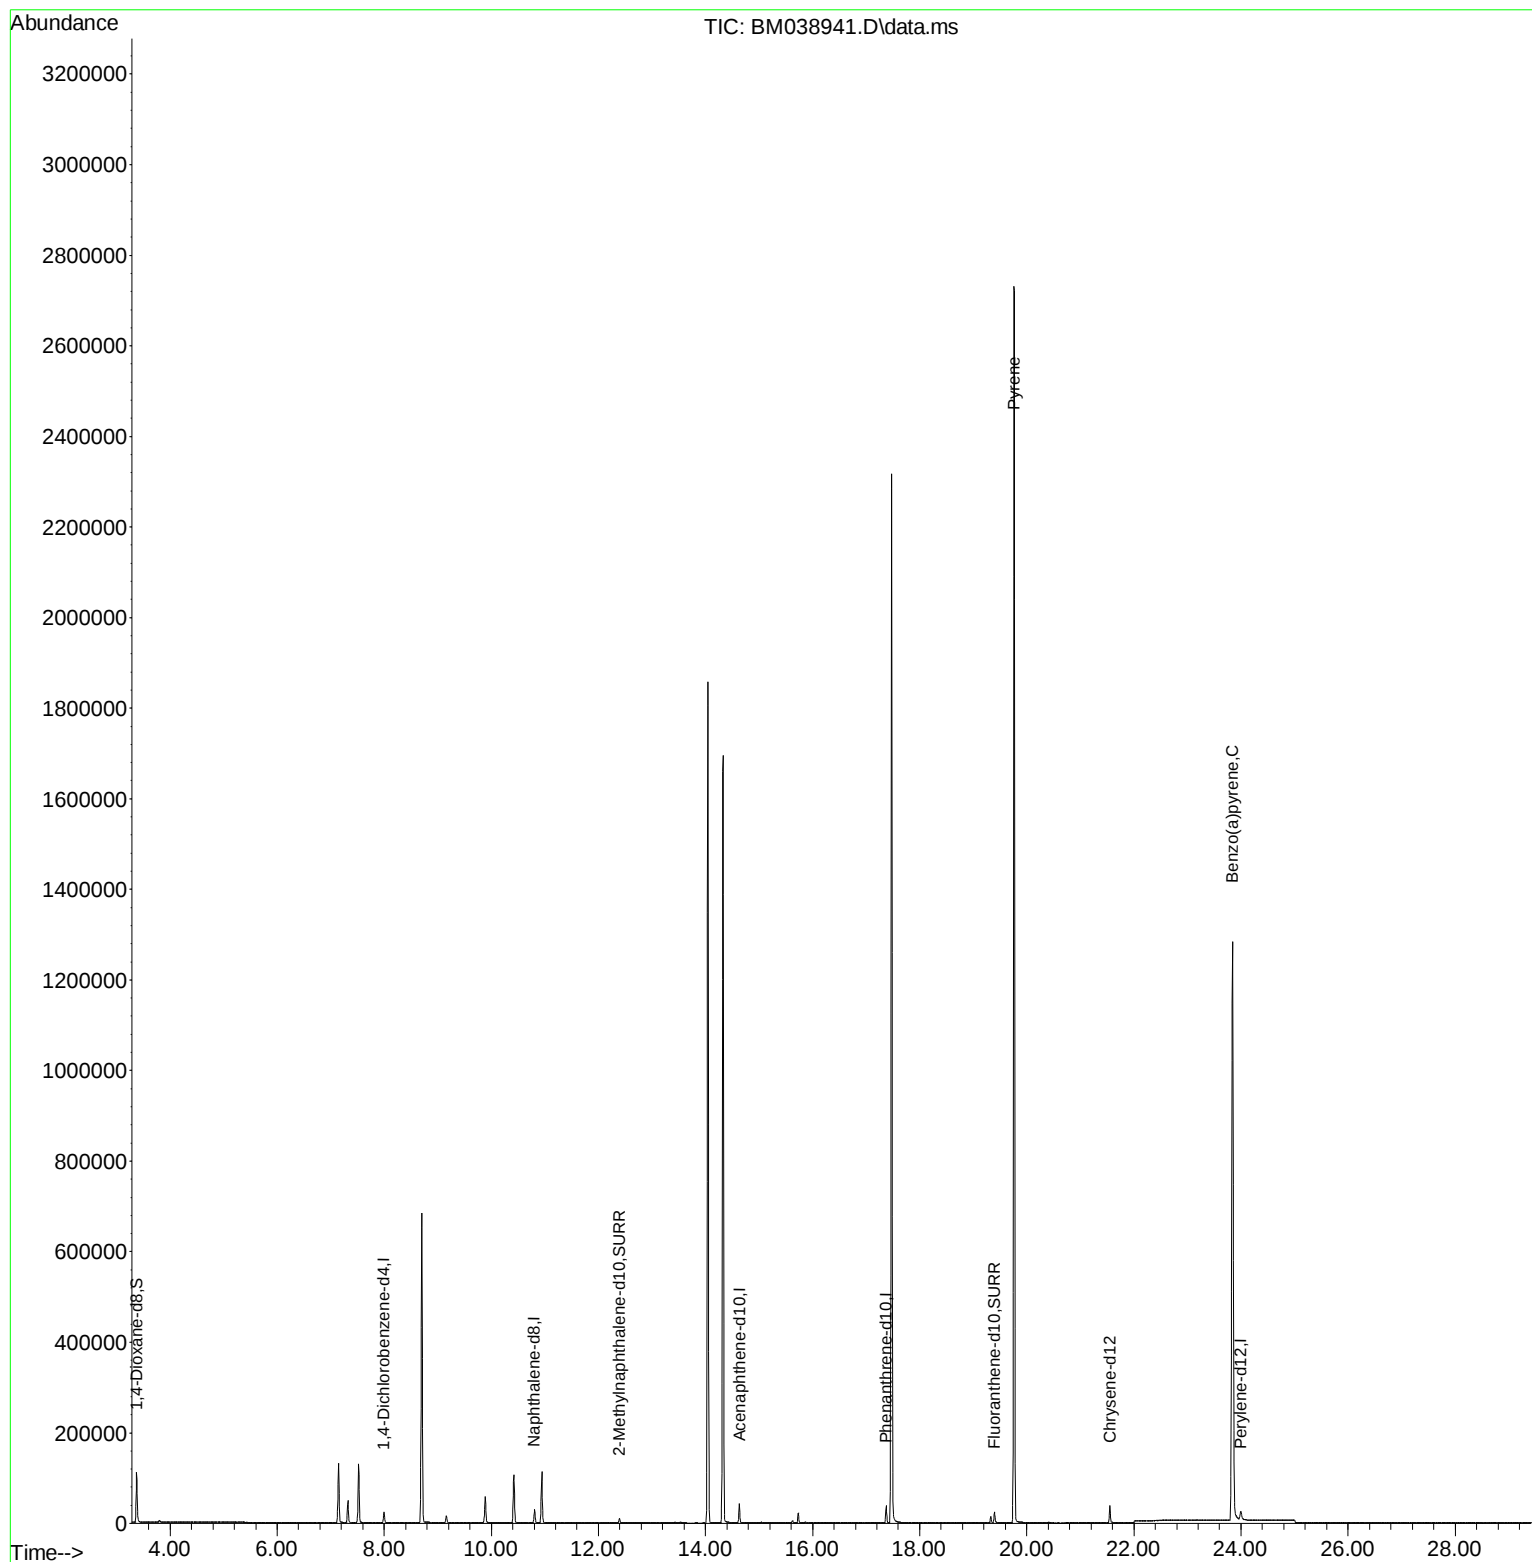

Abundance Scan 3645 (19.789 min): BM038940.D\data.ms (-3620) (-)

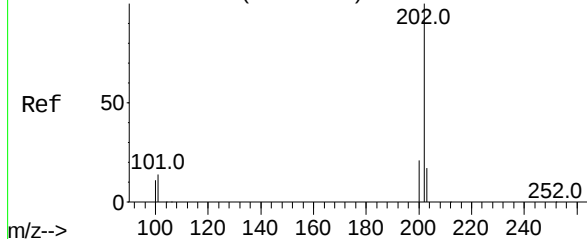

Pyrene

Concen: 0.041 ng/ul

RT: 19.765 min Scan#

Delta R.T. -0.030 min

Lab File: BM038941.D

Acq: 09 Mar 2023 12:14

Instrument :

BNA_M

ClientSampleId :



Tgt Ion:202 Resp: 4908

Ion Ratio Lower Upper


202 100

101 152.2 11.2 16.8#


100 1076.1 9.0 13.6#

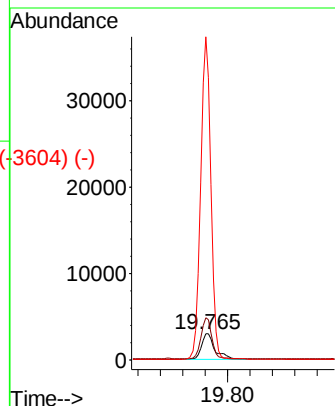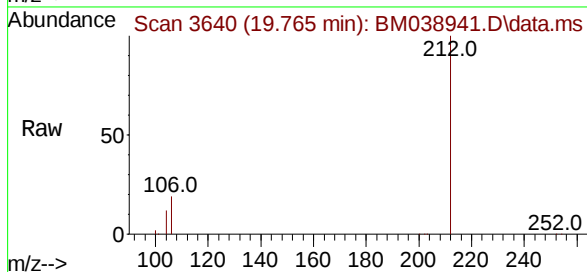

Abundance Scan 3640 (19.765 min): BM038941.D\data.ms (-3604) (-)

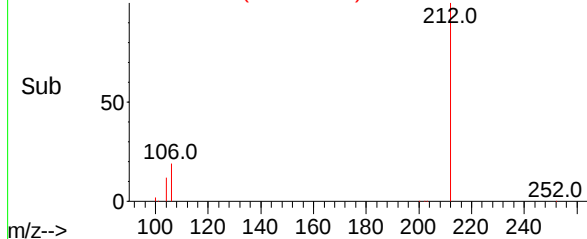

Abundance Scan 4957 (23.888 min): BM038940.D\data.ms (-4920) (-)

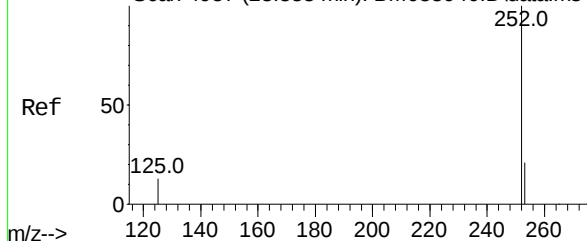

Benzo(a)pyrene

Concen: 0.087 ng/ul

RT: 23.844 min Scan# 4942

Delta R.T. -0.055 min

Lab File: BM038941.D

Acq: 09 Mar 2023 12:14



Tgt Ion:252 Resp: 7451

Ion Ratio Lower Upper

252 100

253 43.7 20.3 30.5#

125 41.4 14.0 21.0#

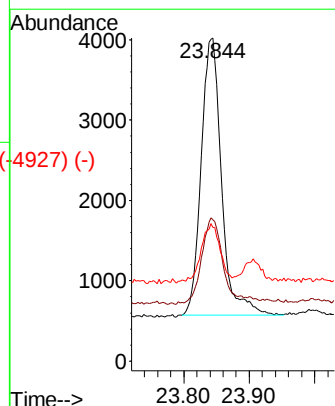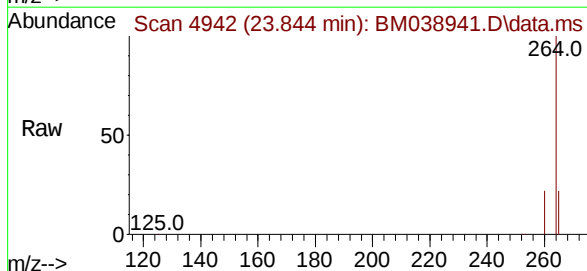

Abundance Scan 4942 (23.844 min): BM038941.D\data.ms (-4927) (-)

