

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030923\
 Data File : BM038955.D
 Acq On : 09 Mar 2023 21:47
 Operator : CG/JU
 Sample : PB151259BL
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK259

Quant Time: Mar 10 03:54:17 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM030323.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 09 13:36:03 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.995	152	9032	0.400	ng/ul	0.00
4) Naphthalene-d8	10.805	136	30862	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.633	164	17262	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.374	188	34691	0.400	ng/ul	0.00
17) Chrysene-d12	21.553	240	27742	0.400	ng/ul	0.00
23) Perylene-d12	23.996	264	23912	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.375	96	70574	6.906	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.395	152	13518	0.362	ng/ul	0.00
18) Fluoranthene-d10	19.398	212	26388	0.400	ng/ul	0.00
Target Compounds						Qvalue
12) Fluorene	15.623	166	4513	0.077	ng/ul#	14
20) Pyrene	19.765	202	4298	0.045	ng/ul#	1
26) Benzo(a)pyrene	23.841	252	7984	0.107	ng/ul#	64


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030923\
Data File : BM038955.D
Acq On : 09 Mar 2023 21:47
Operator : CG/JU
Sample : PB151259BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK259

Quant Time: Mar 10 03:54:17 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM030323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 09 13:36:03 2023
Response via : Initial Calibration




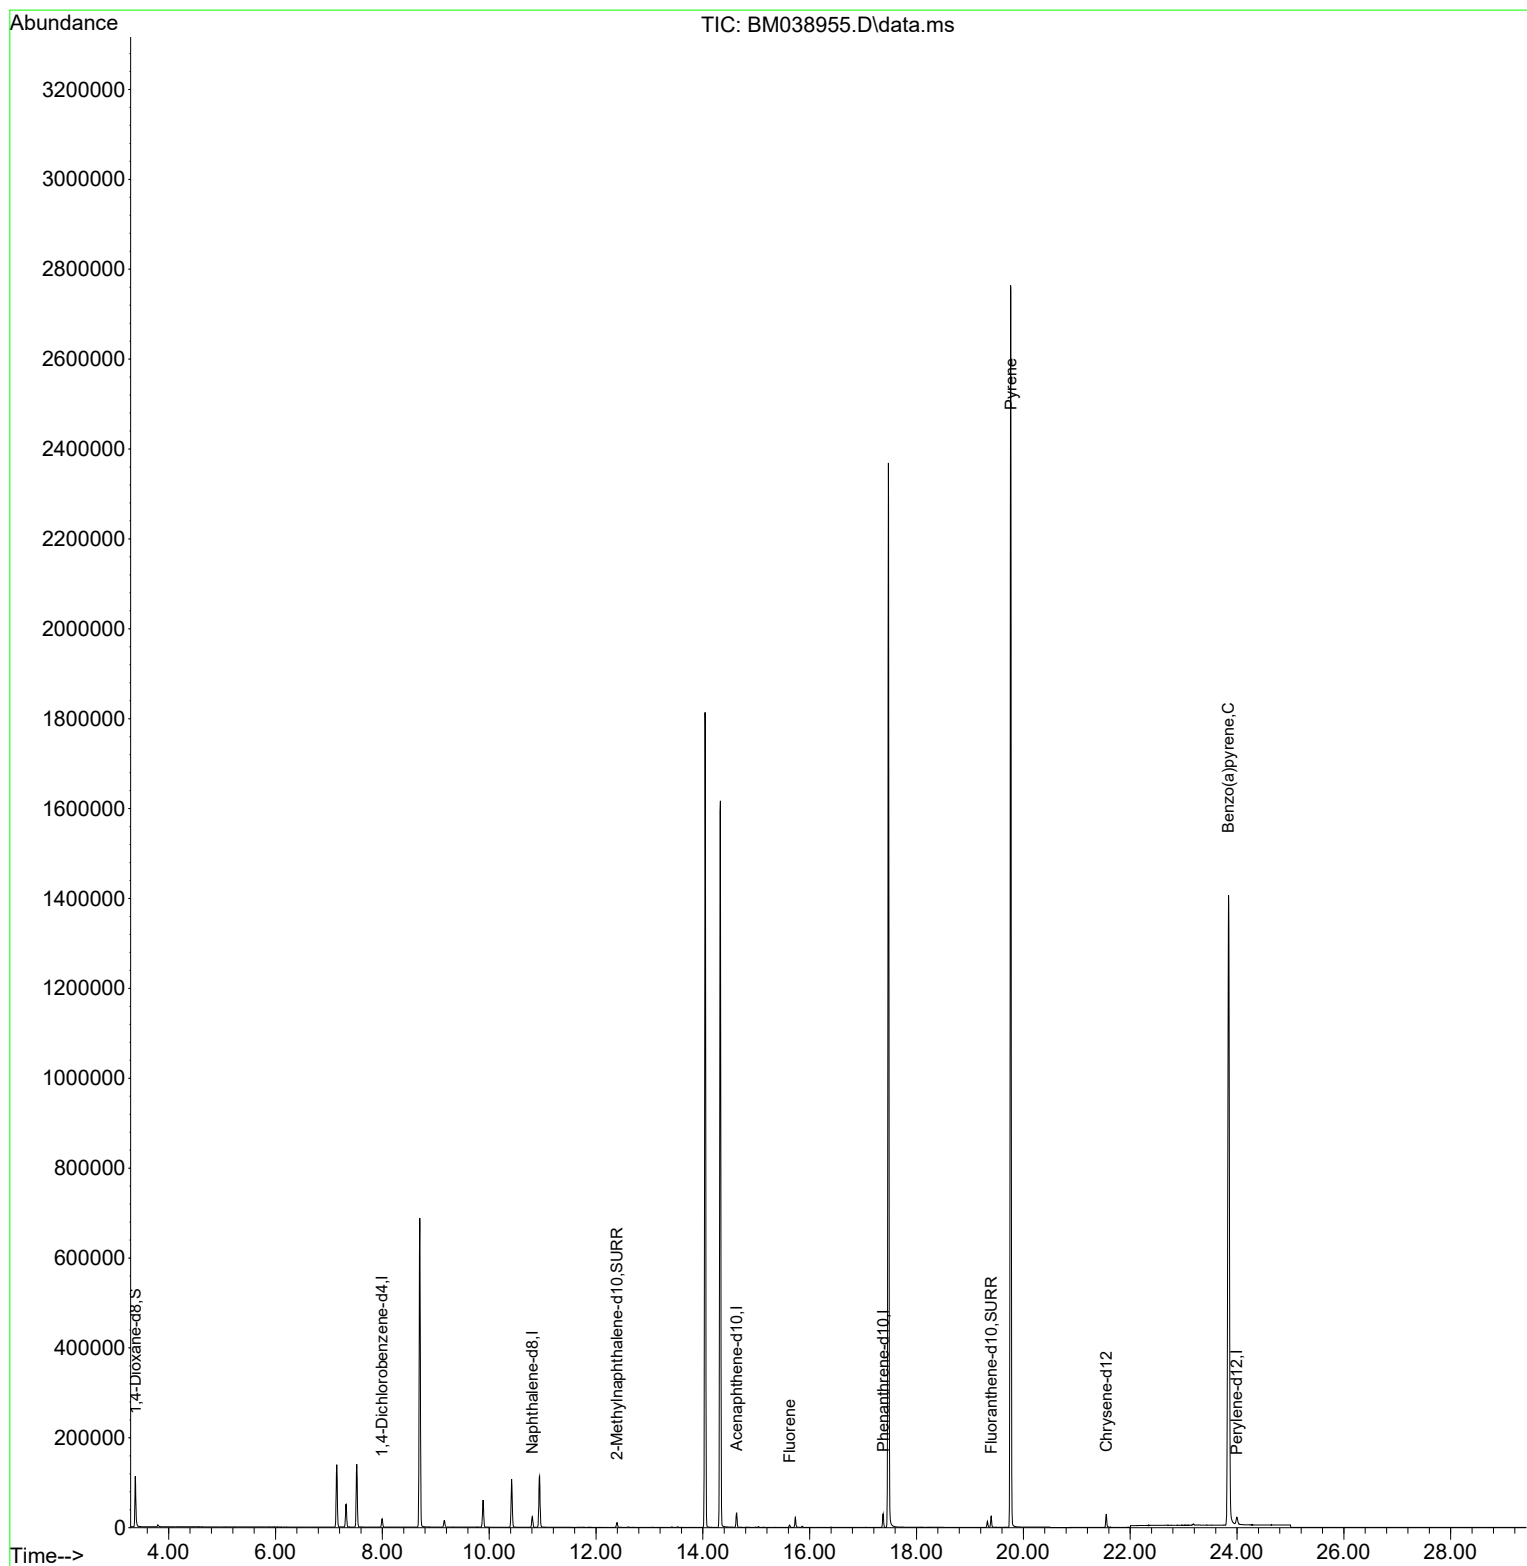


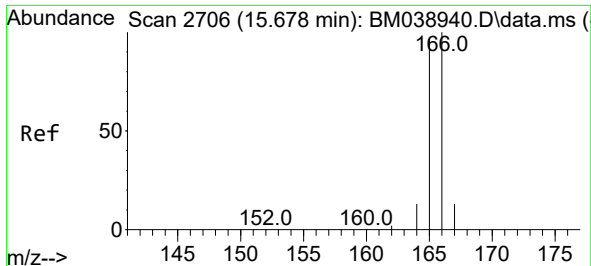

#12
Fluorene
Concen: 0.077 ng/ul
RT: 15.623 min Scan# 2
Delta R.T. -0.056 min
Lab File: BM038955.D
Acq: 09 Mar 2023 21:47




Instrument :
BNA_M
ClientSampleId :
SBLK259


Tgt Ion:166 Resp: 4513
Ion Ratio Lower Upper
166 100
165 6.5 77.8 116.6#
167 32.0 11.4 17.2#

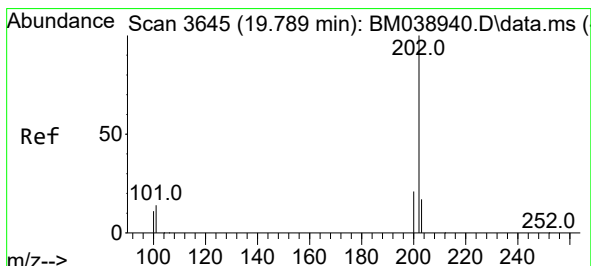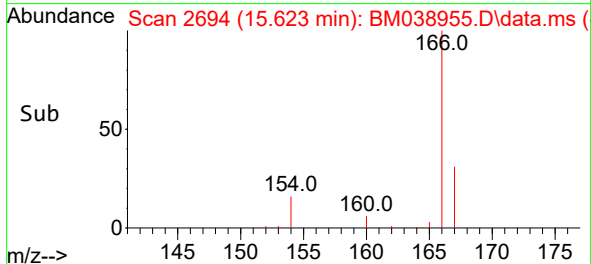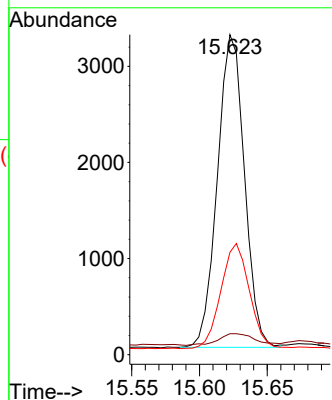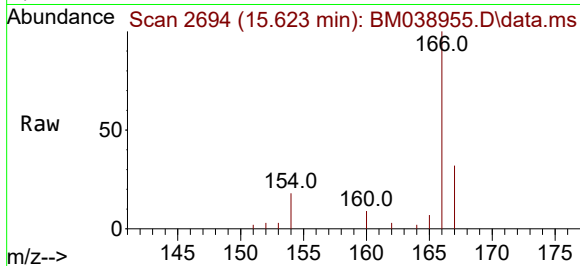

#20
Pyrene
Concen: 0.045 ng/ul
RT: 19.765 min Scan# 3640
Delta R.T. -0.023 min
Lab File: BM038955.D
Acq: 09 Mar 2023 21:47


Tgt Ion:202 Resp: 4298
Ion Ratio Lower Upper
202 100
101 151.6 11.2 16.8#
100 1064.6 9.0 13.6#

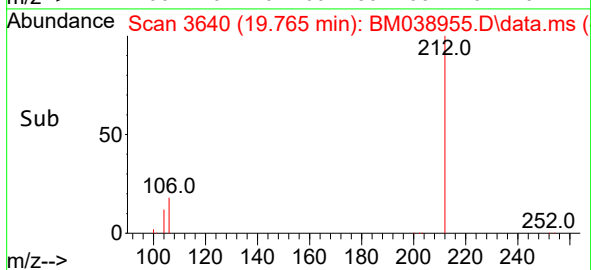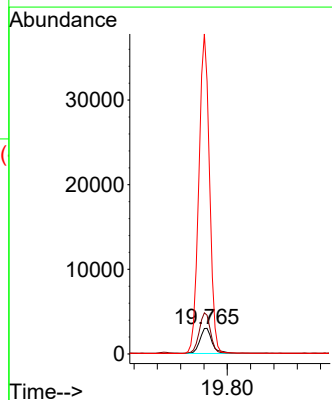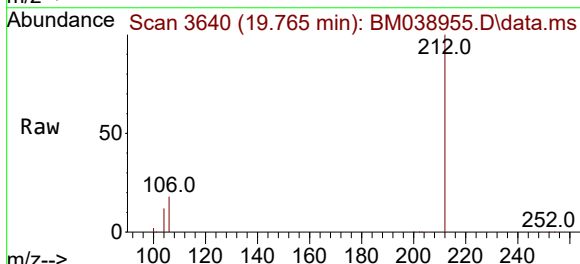

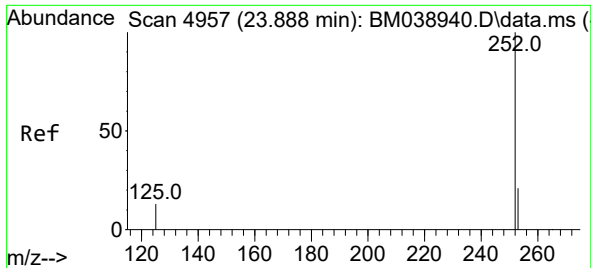

#26
Benzo(a)pyrene
Concen: 0.107 ng/ul
RT: 23.841 min Scan# 4957
Delta R.T. -0.047 min
Lab File: BM038955.D
Acq: 09 Mar 2023 21:47

Instrument :
BNA_M
ClientSampleId :
SBLK259

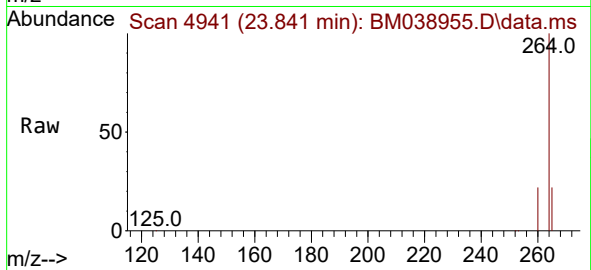

Tgt Ion:252 Resp: 7984
Ion Ratio Lower Upper
252 100
253 40.2 20.3 30.5#
125 37.4 14.0 21.0#

