

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030923\
 Data File : BM038958.D
 Acq On : 09 Mar 2023 23:41
 Operator : CG/JU
 Sample : 01729-02
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0BY6

Quant Time: Mar 10 03:54:38 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM030323.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 09 13:36:03 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.995	152	11146	0.400	ng/ul	0.00
4) Naphthalene-d8	10.804	136	38810	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.631	164	21908	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.373	188	45432	0.400	ng/ul	0.00
17) Chrysene-d12	21.551	240	33952	0.400	ng/ul	0.00
23) Perylene-d12	23.995	264	27081	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.375	96	54383	4.312	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.393	152	14574	0.310	ng/ul	0.00
18) Fluoranthene-d10	19.397	212	32715	0.405	ng/ul	0.00
Target Compounds						Qvalue
7) 2-Methylnaphthalene	12.465	142	1946	0.035	ng/ul	99
20) Pyrene	19.764	202	5639	0.048	ng/ul#	1
26) Benzo(a)pyrene	23.840	252	8539	0.101	ng/ul#	61


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030923\
Data File : BM038958.D
Acq On : 09 Mar 2023 23:41
Operator : CG/JU
Sample : 01729-02
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0BY6

Quant Time: Mar 10 03:54:38 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM030323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 09 13:36:03 2023
Response via : Initial Calibration




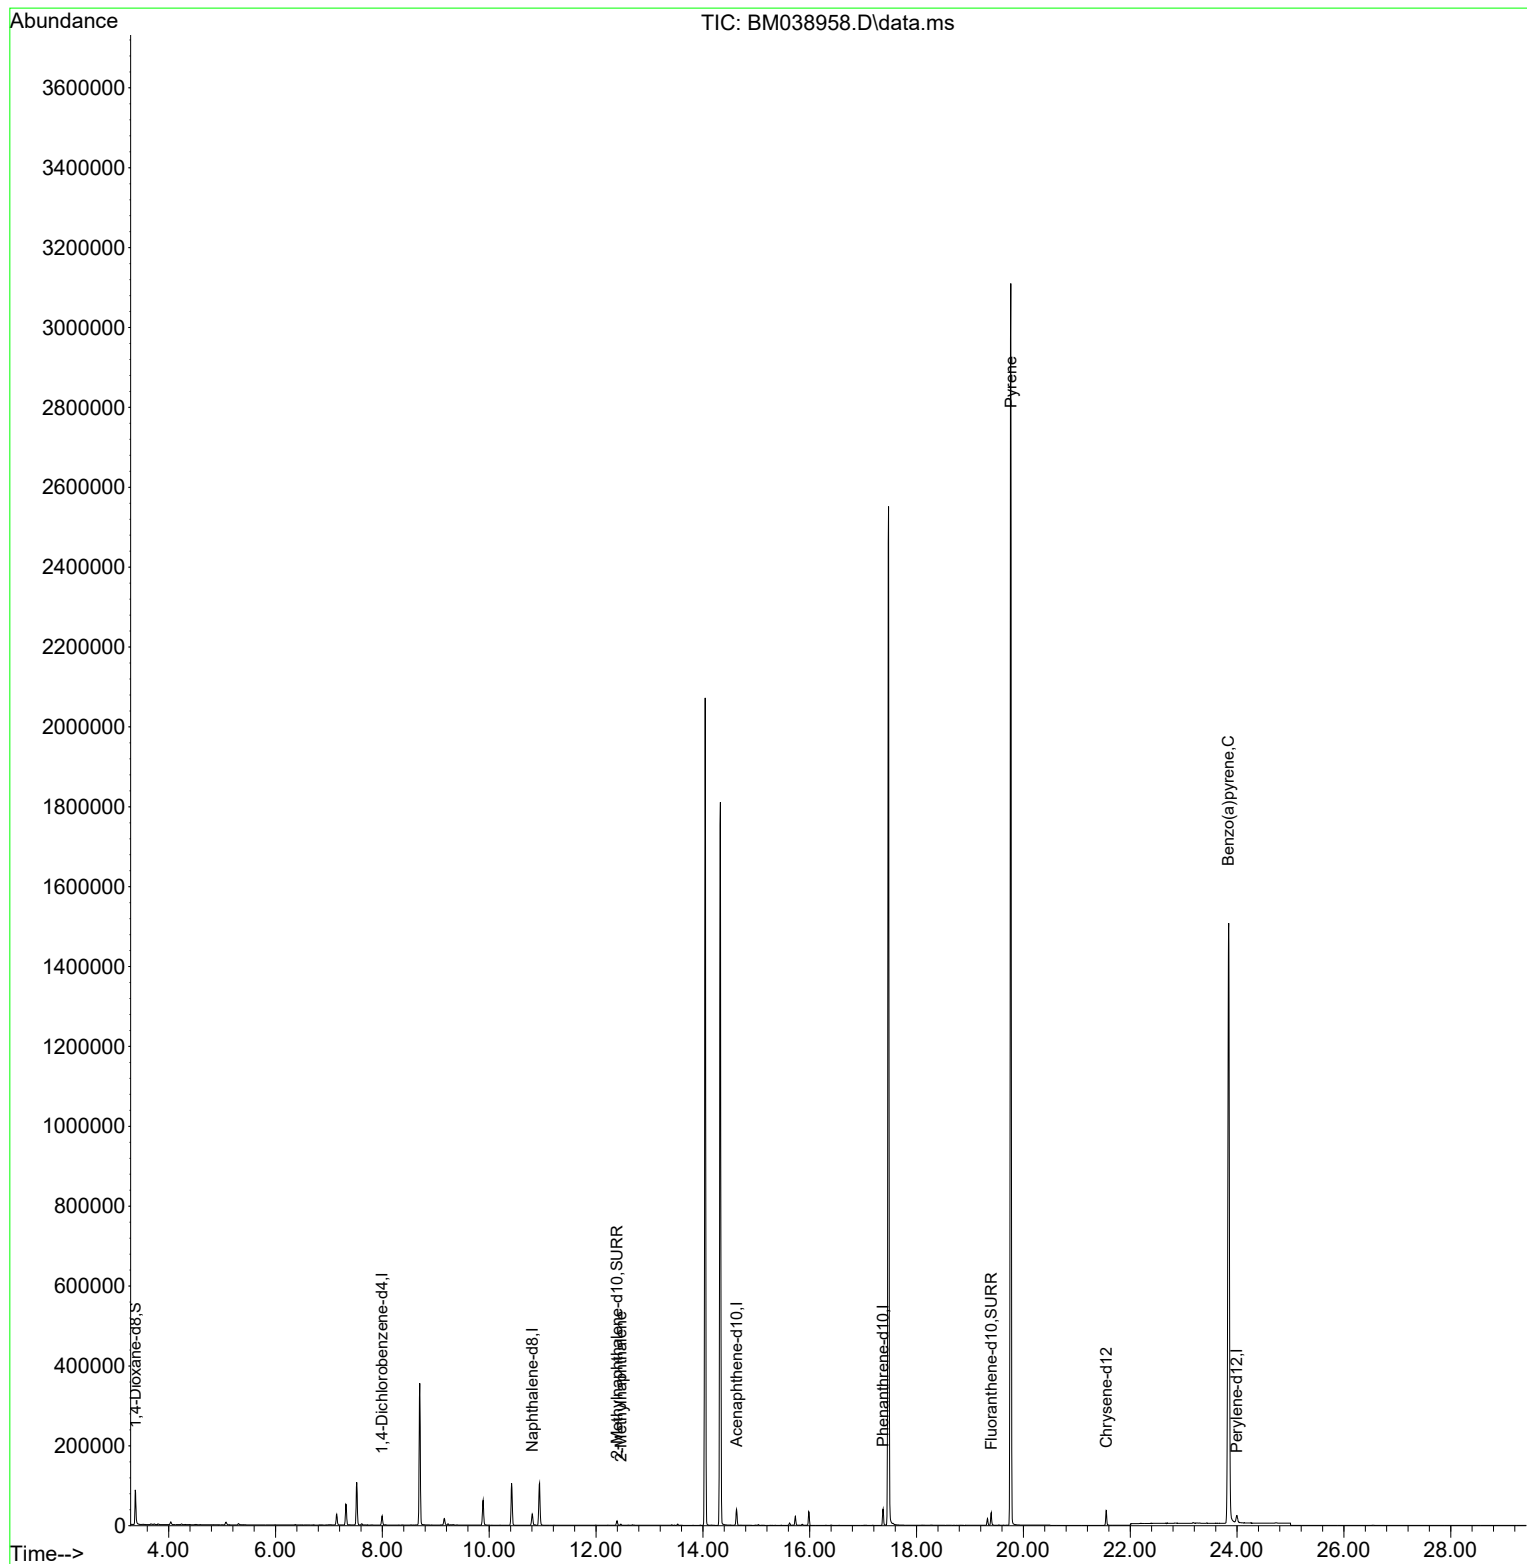


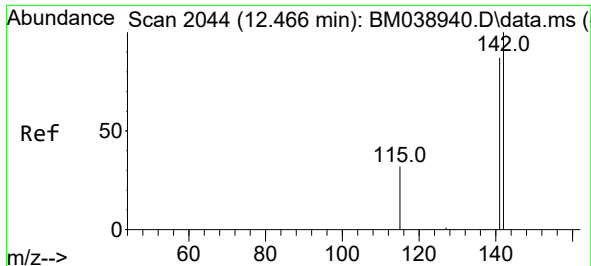

#7
2-Methylnaphthalene
Concen: 0.035 ng/ul
RT: 12.465 min Scan# 2044
Delta R.T. -0.001 min
Lab File: BM038958.D
Acq: 09 Mar 2023 23:41




Instrument :
BNA_M
ClientSampleId :
C0BY6


Tgt Ion:142 Resp: 1946
Ion Ratio Lower Upper
142 100
141 88.1 69.9 104.9

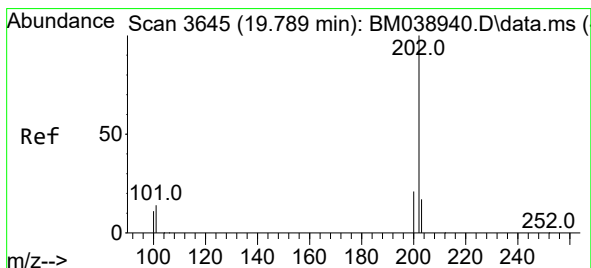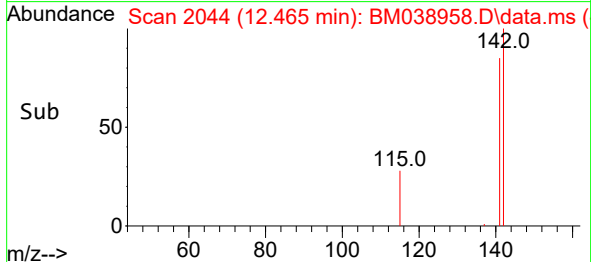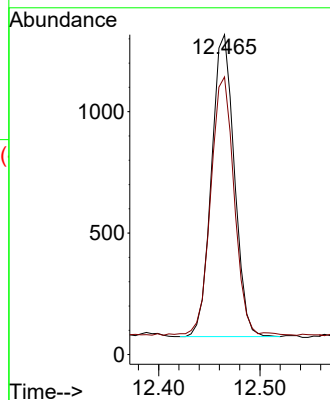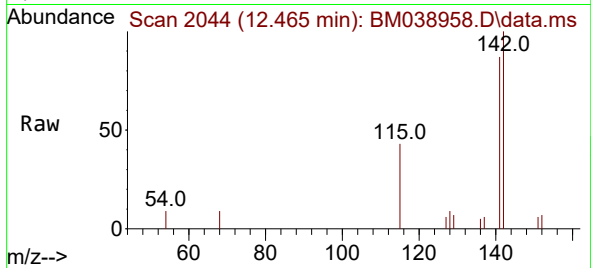

#20
Pyrene
Concen: 0.048 ng/ul
RT: 19.764 min Scan# 3640
Delta R.T. -0.025 min
Lab File: BM038958.D
Acq: 09 Mar 2023 23:41


Tgt Ion:202 Resp: 5639
Ion Ratio Lower Upper
202 100
101 152.4 11.2 16.8#
100 1099.6 9.0 13.6#

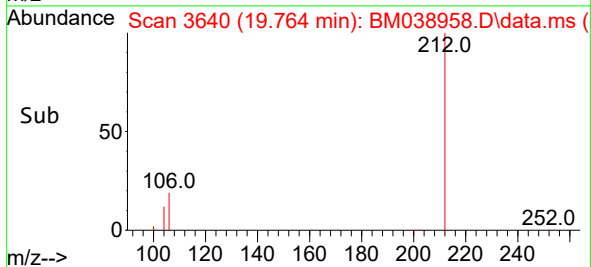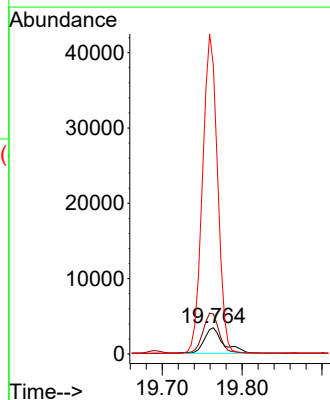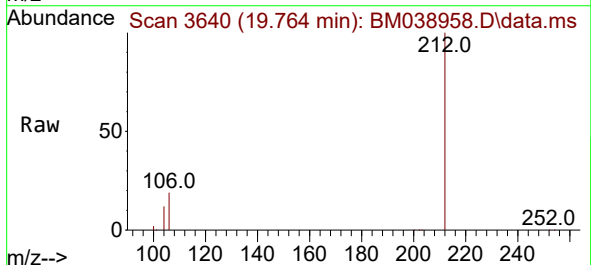

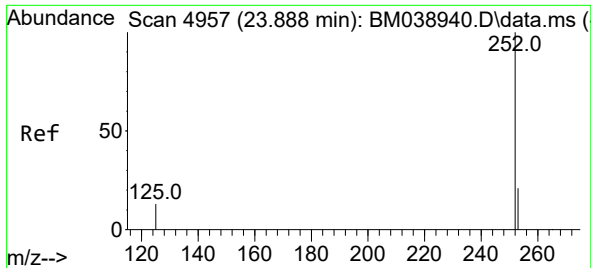

#26
 Benzo(a)pyrene
 Concen: 0.101 ng/ul
 RT: 23.840 min Scan# 4957
 Delta R.T. -0.048 min
 Lab File: BM038958.D
 Acq: 09 Mar 2023 23:41

Instrument :
 BNA_M
 ClientSampleId :
 C0BY6

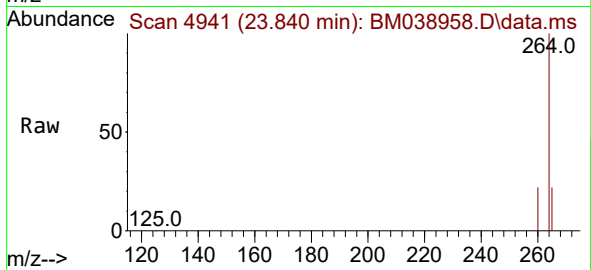

Tgt Ion:252 Resp: 8539
 Ion Ratio Lower Upper
 252 100
 253 41.4 20.3 30.5#
 125 39.0 14.0 21.0#

