

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030923\
 Data File : BM038960.D
 Acq On : 10 Mar 2023 00:57
 Operator : CG/JU
 Sample : 01729-04
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0BY8

Quant Time: Mar 10 03:54:52 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM030323.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 09 13:36:03 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.995	152	10935	0.400	ng/ul	0.00
4) Naphthalene-d8	10.806	136	37054	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.628	164	21572	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.375	188	43697	0.400	ng/ul	0.00
17) Chrysene-d12	21.550	240	31544	0.400	ng/ul	0.00
23) Perylene-d12	23.994	264	24262	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.375	96	51014	4.123	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.389	152	12286	0.274	ng/ul	0.00
18) Fluoranthene-d10	19.398	212	30529	0.407	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.413	88	2085	0.166	ng/ul#	63
20) Pyrene	19.761	202	5251	0.048	ng/ul#	1
26) Benzo(a)pyrene	23.839	252	7409	0.098	ng/ul#	55


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030923\
Data File : BM038960.D
Acq On : 10 Mar 2023 00:57
Operator : CG/JU
Sample : 01729-04
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0BY8

Quant Time: Mar 10 03:54:52 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM030323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 09 13:36:03 2023
Response via : Initial Calibration




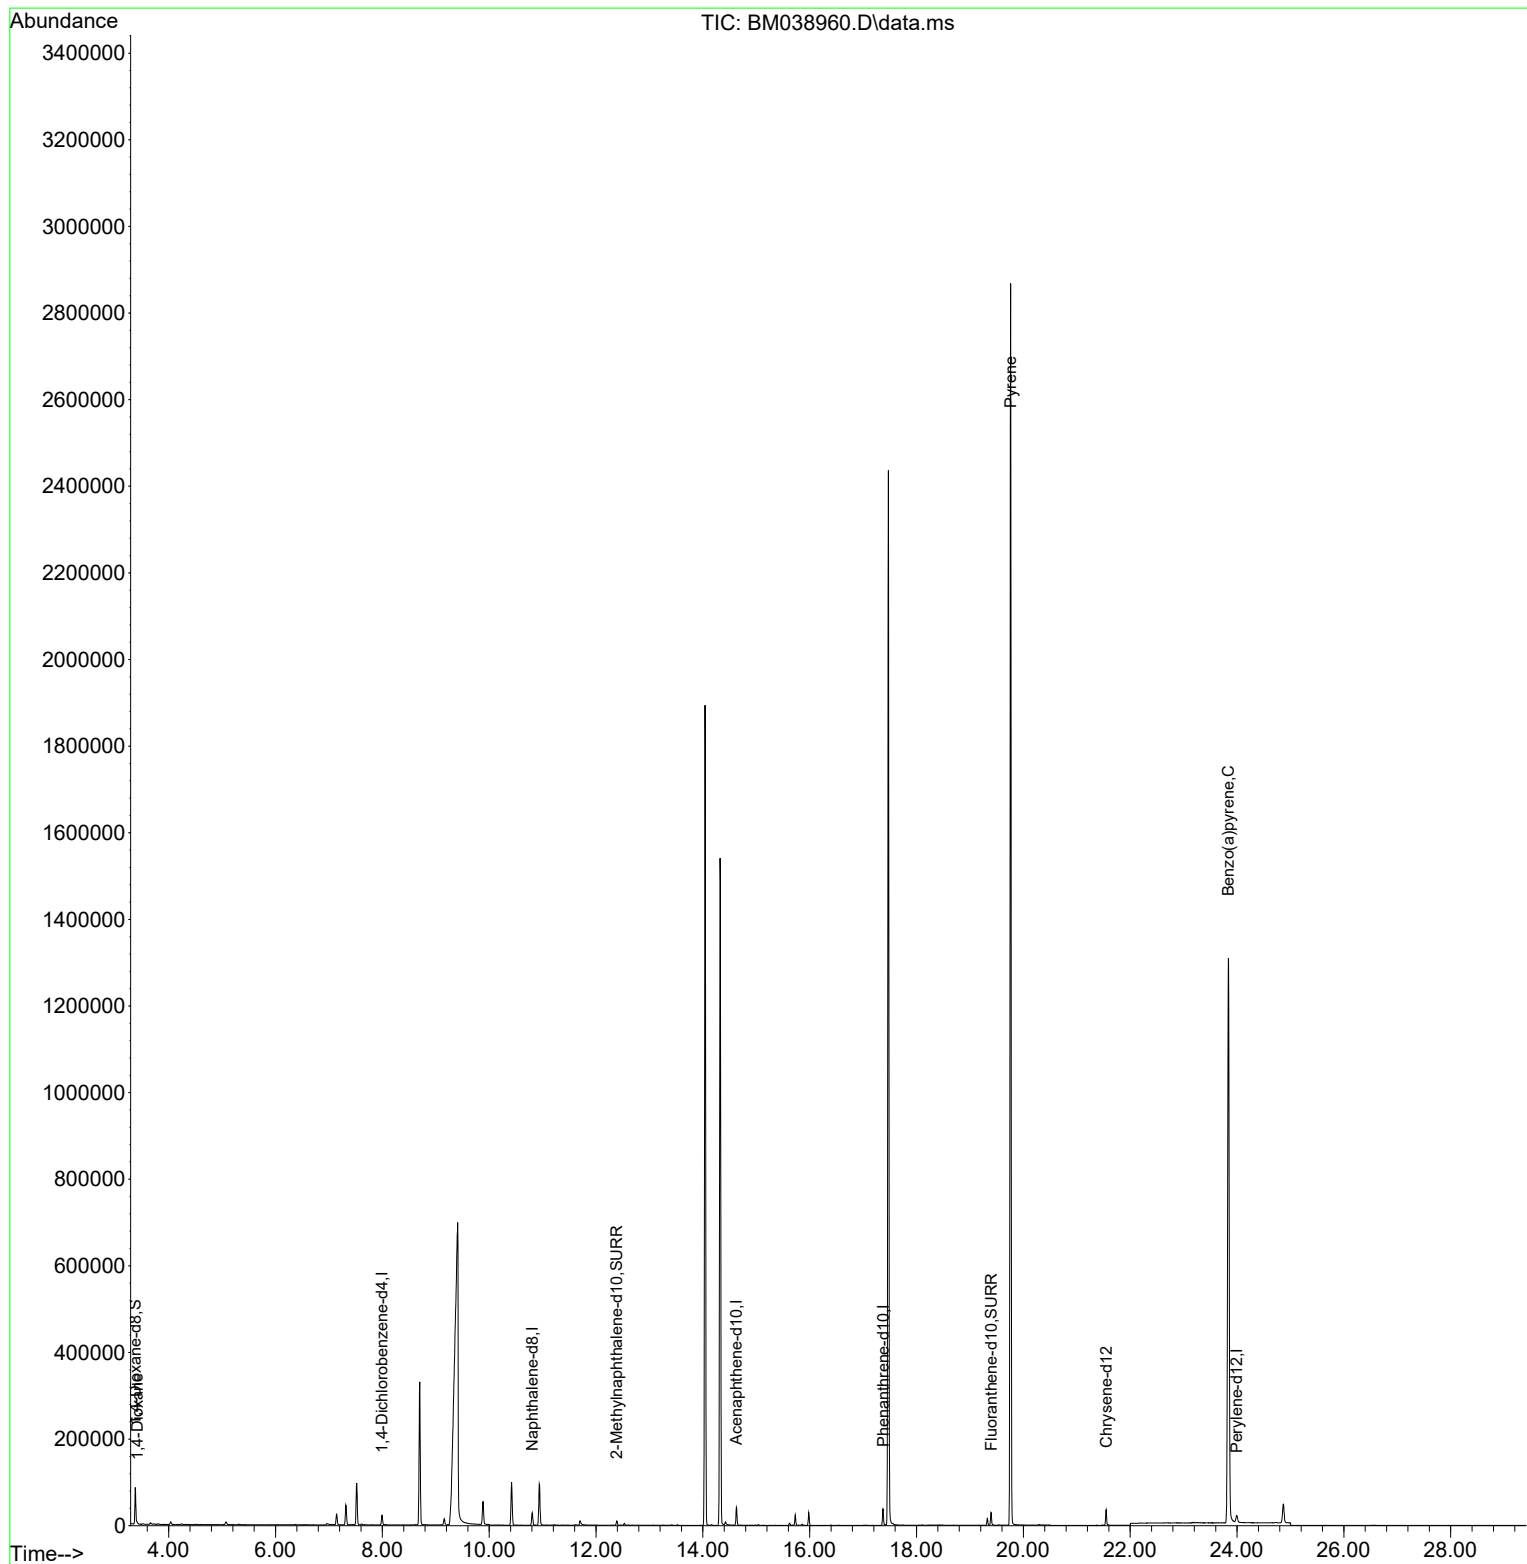


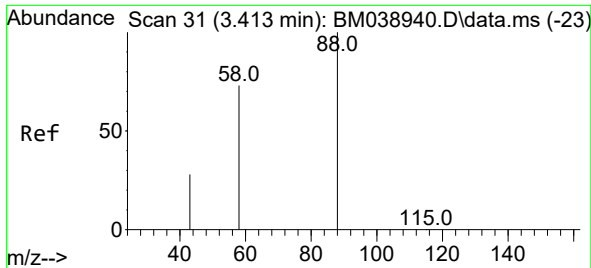

#2
1,4-Dioxane
Concen: 0.166 ng/ul
RT: 3.413 min Scan# 31
Delta R.T. -0.000 min
Lab File: BM038960.D
Acq: 10 Mar 2023 00:57




Instrument :
BNA_M
ClientSampleId :
C0BY8


Tgt Ion: 88 Resp: 2085
Ion Ratio Lower Upper
88 100
43 91.7 27.2 40.8#
58 65.6 50.8 76.2

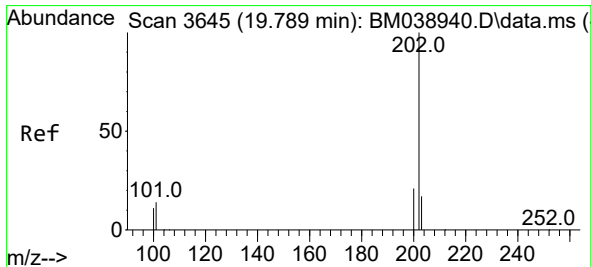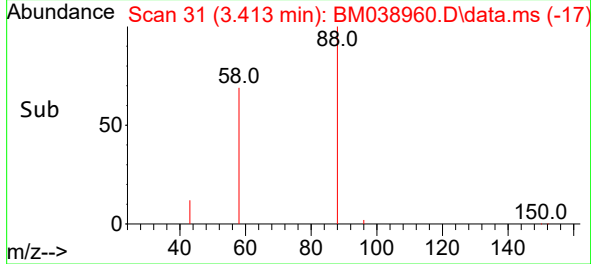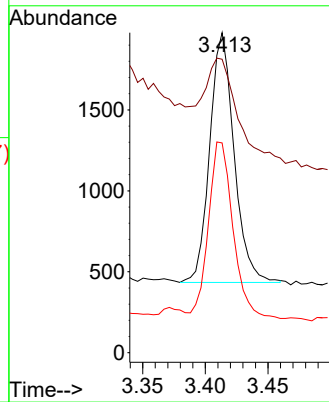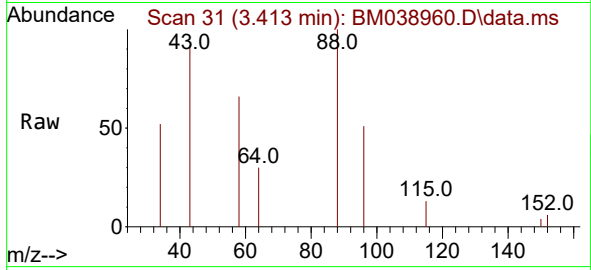

#20
Pyrene
Concen: 0.048 ng/ul
RT: 19.761 min Scan# 3639
Delta R.T. -0.028 min
Lab File: BM038960.D
Acq: 10 Mar 2023 00:57


Tgt Ion: 202 Resp: 5251
Ion Ratio Lower Upper
202 100
101 155.7 11.2 16.8#
100 1154.1 9.0 13.6#

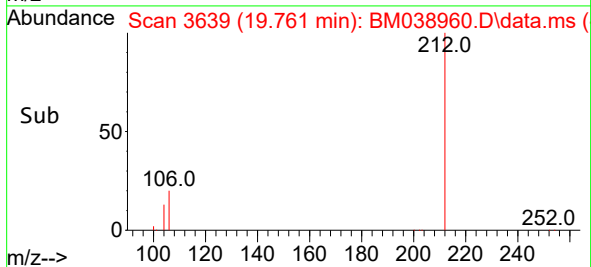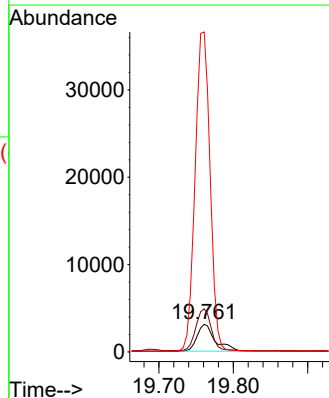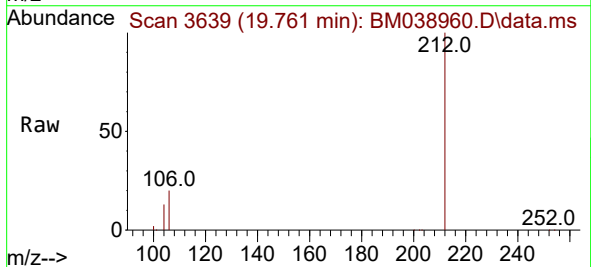

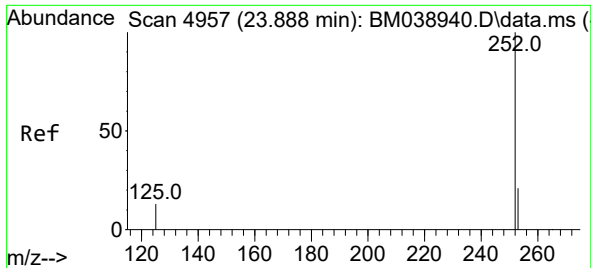

#26
Benzo(a)pyrene
Concen: 0.098 ng/ul
RT: 23.839 min Scan# 4957
Delta R.T. -0.050 min
Lab File: BM038960.D
Acq: 10 Mar 2023 00:57

Instrument :
BNA_M
ClientSampleId :
C0BY8

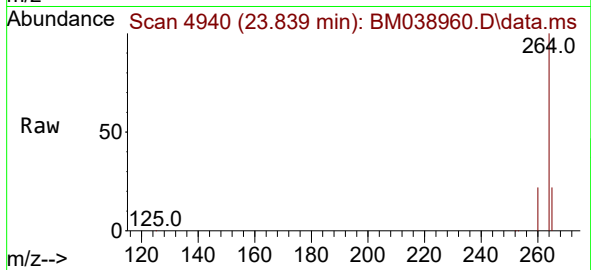

Tgt Ion:252 Resp: 7409
Ion Ratio Lower Upper
252 100
253 42.5 20.3 30.5#
125 44.0 14.0 21.0#

