

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030923\
 Data File : BM038972.D
 Acq On : 10 Mar 2023 09:27
 Operator : CG/JU
 Sample : PB151313BL
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK313

Quant Time: Mar 10 23:14:35 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM030323.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 09 13:36:03 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.991	152	8382	0.400	ng/ul	0.00
4) Naphthalene-d8	10.806	136	28706	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.628	164	15846	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.374	188	32039	0.400	ng/ul	0.00
17) Chrysene-d12	21.556	240	22374	0.400	ng/ul	0.00
23) Perylene-d12	24.002	264	17455	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.371	96	61514	6.486	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.389	152	11727	0.338	ng/ul	0.00
18) Fluoranthene-d10	19.398	212	21260	0.399	ng/ul	0.00
Target Compounds						Qvalue
12) Fluorene	15.623	166	3947	0.074	ng/ul#	13
20) Pyrene	19.765	202	3461	0.044	ng/ul#	1
26) Benzo(a)pyrene	23.847	252	5926	0.109	ng/ul#	58


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030923\
Data File : BM038972.D
Acq On : 10 Mar 2023 09:27
Operator : CG/JU
Sample : PB151313BL
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK313

Quant Time: Mar 10 23:14:35 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM030323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 09 13:36:03 2023
Response via : Initial Calibration




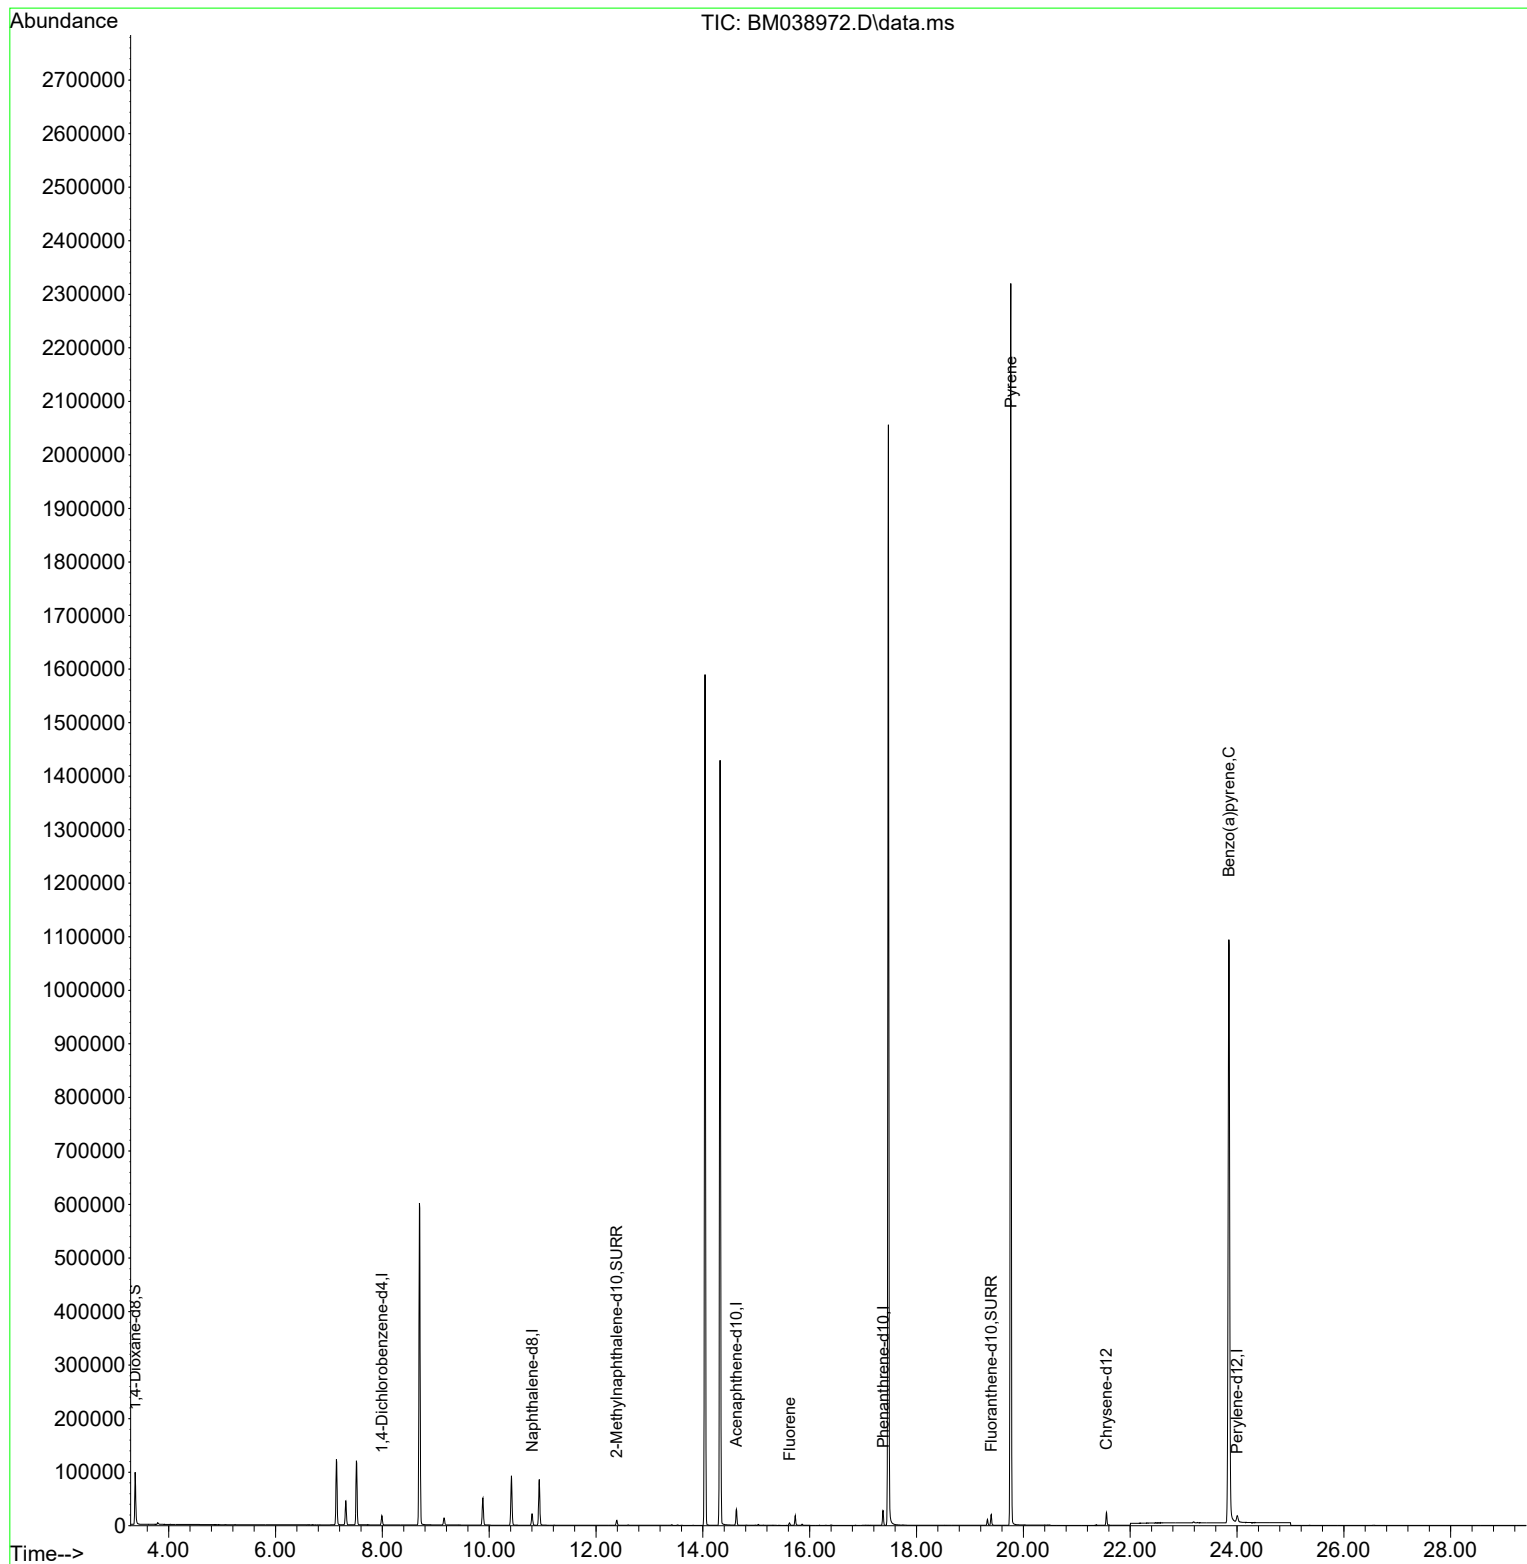


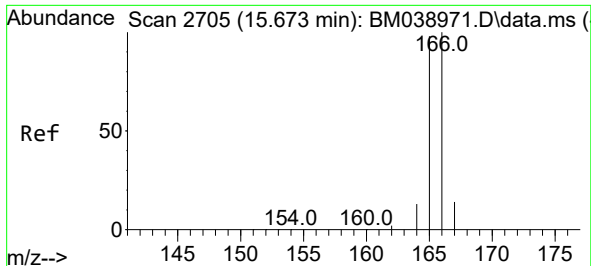

#12
Fluorene
Concen: 0.074 ng/ul
RT: 15.623 min Scan# 2
Delta R.T. -0.056 min
Lab File: BM038972.D
Acq: 10 Mar 2023 09:27




Instrument :
BNA_M
ClientSampleId :
SBLK313


Tgt Ion:166 Resp: 3947
Ion Ratio Lower Upper
166 100
165 6.9 77.8 116.6#
167 35.6 11.4 17.2#

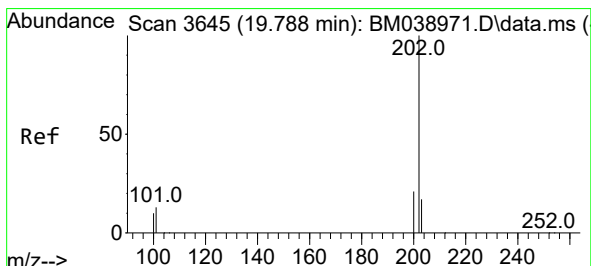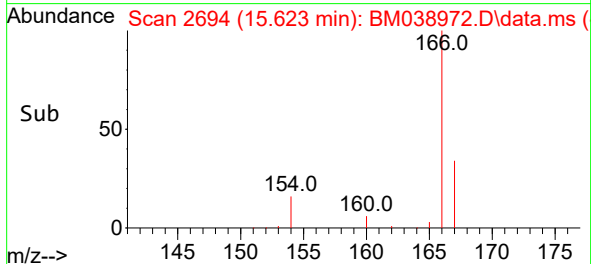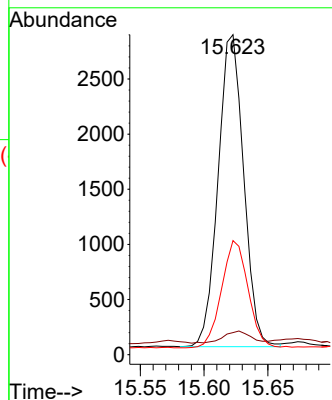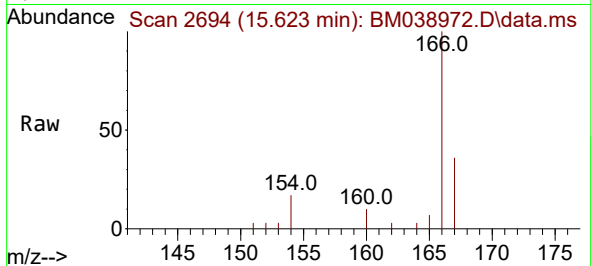

#20
Pyrene
Concen: 0.044 ng/ul
RT: 19.765 min Scan# 3640
Delta R.T. -0.023 min
Lab File: BM038972.D
Acq: 10 Mar 2023 09:27


Tgt Ion:202 Resp: 3461
Ion Ratio Lower Upper
202 100
101 155.5 11.2 16.8#
100 1115.9 9.0 13.6#

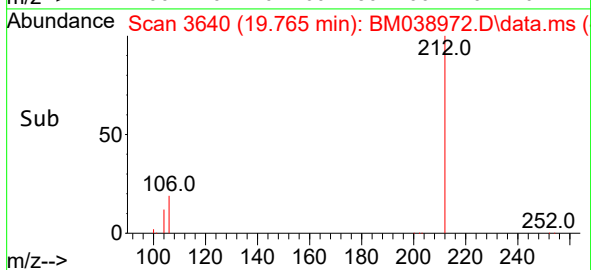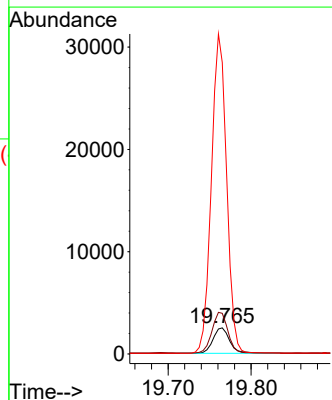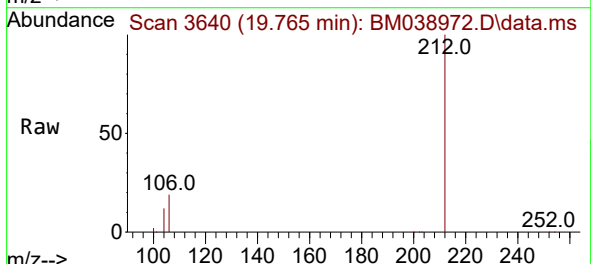

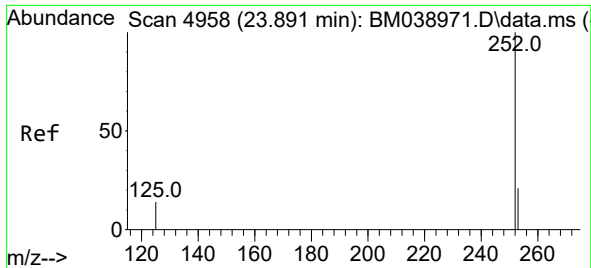

#26
Benzo(a)pyrene
Concen: 0.109 ng/ul
RT: 23.847 min Scan# 4943
Delta R.T. -0.041 min
Lab File: BM038972.D
Acq: 10 Mar 2023 09:27

Instrument :
BNA_M
ClientSampleId :
SBLK313

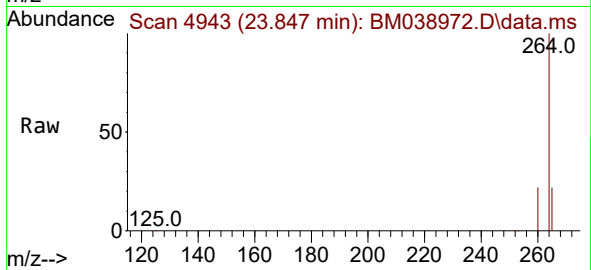

Tgt Ion:252 Resp: 5926
Ion Ratio Lower Upper
252 100
253 42.0 20.3 30.5#
125 42.0 14.0 21.0#

