




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030923\
 Data File : BM038951.D
 Acq On : 09 Mar 2023 18:35
 Operator : CG/JU
 Sample : 01784-07
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DCAD9

Manual IntegrationsAPPROVED

Quant Time: Mar 10 03:53:38 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM030323.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 09 13:36:03 2023
 Response via : Initial Calibration

Reviewed By :Christian Giraldo 03/10/2023
 Supervised By :Jagrut Upadhyay 03/10/2023

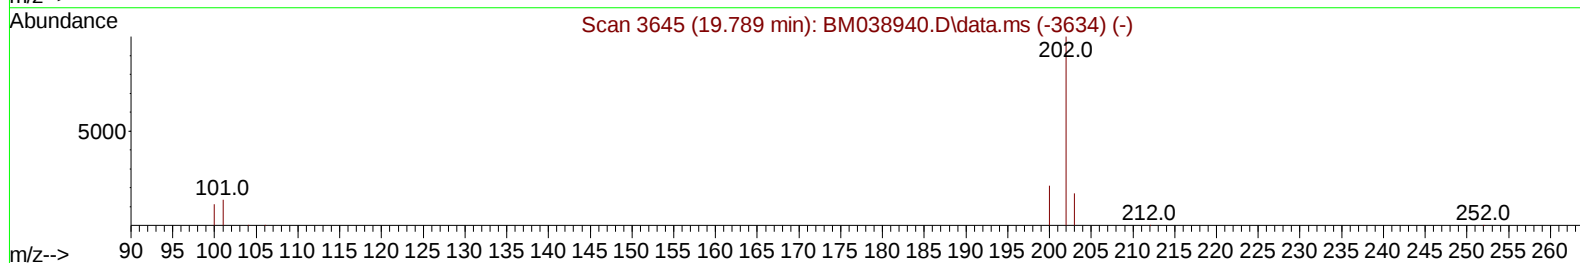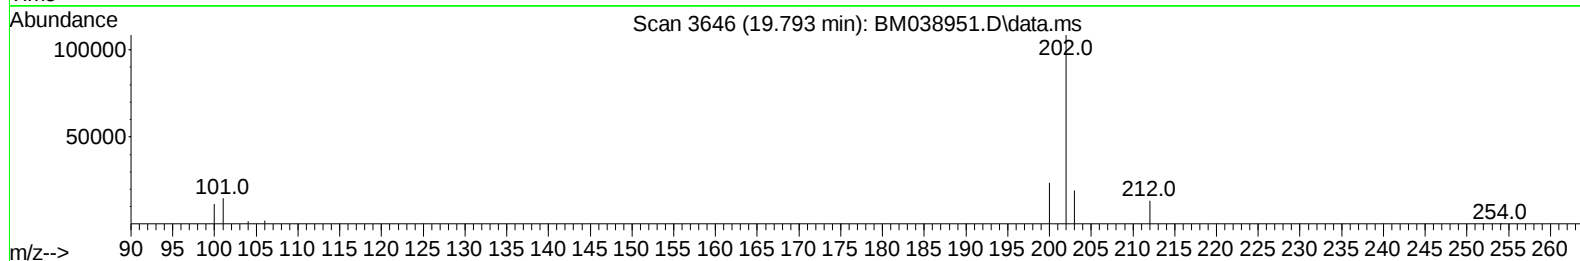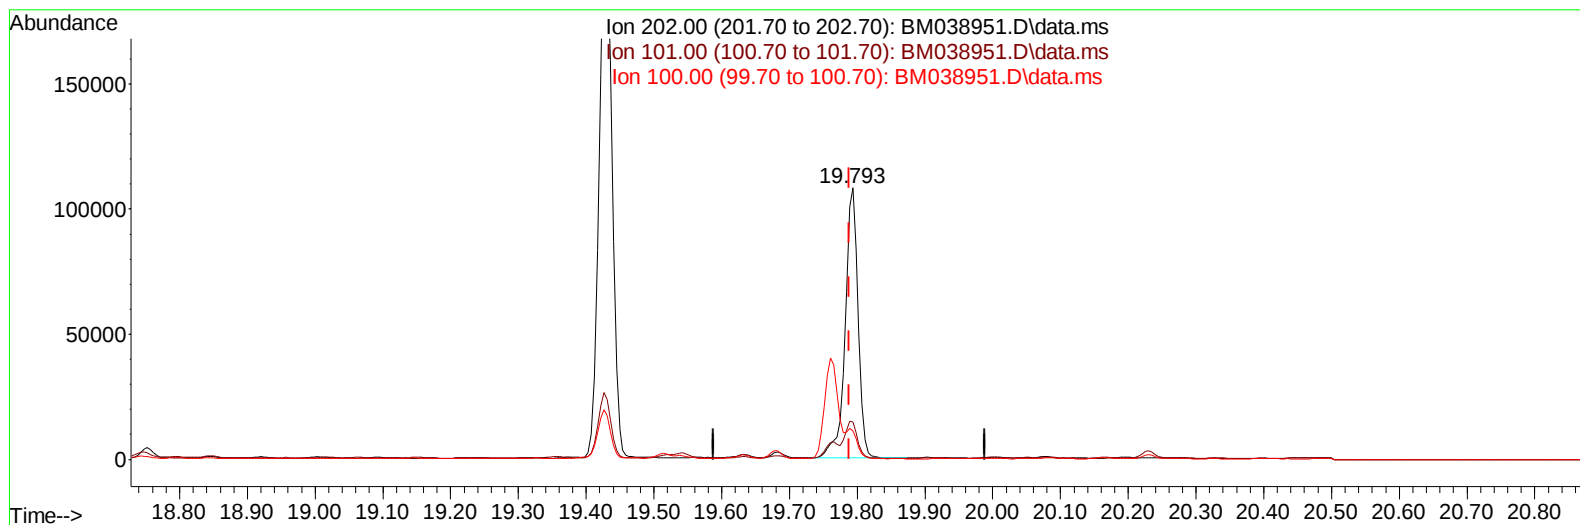

TIC: BM038951.D\data.ms

(20) Pyrene

19.793min (+ 0.005) 1.35 ng/u1

response 144354

Ion	Exp%	Act%
202.00	100.00	100.00
101.00	14.00	13.70
100.00	11.30	10.60
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030923\
Data File : BM038951.D
Acq On : 09 Mar 2023 18:35
Operator : CG/JU
Sample : 01784-07
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DCAD9

Manual IntegrationsAPPROVED

Quant Time: Mar 10 03:53:38 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM030323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 09 13:36:03 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 03/10/2023
Supervised By :Jagrut Upadhyay 03/10/2023

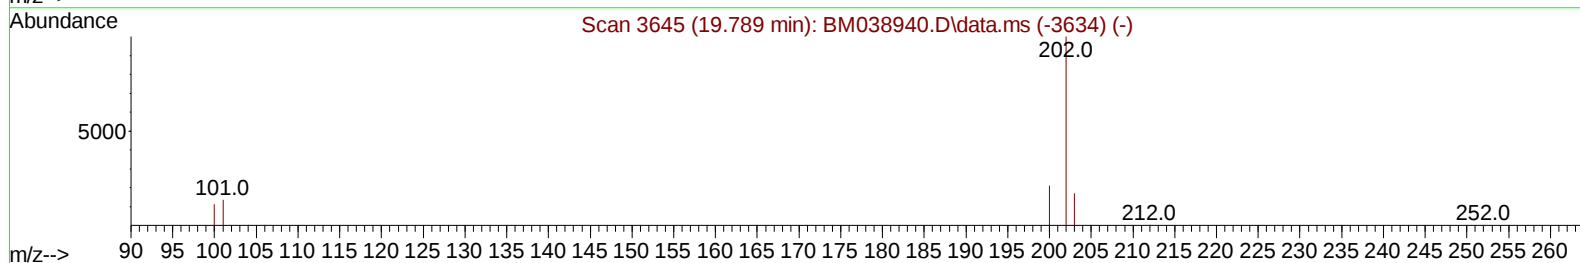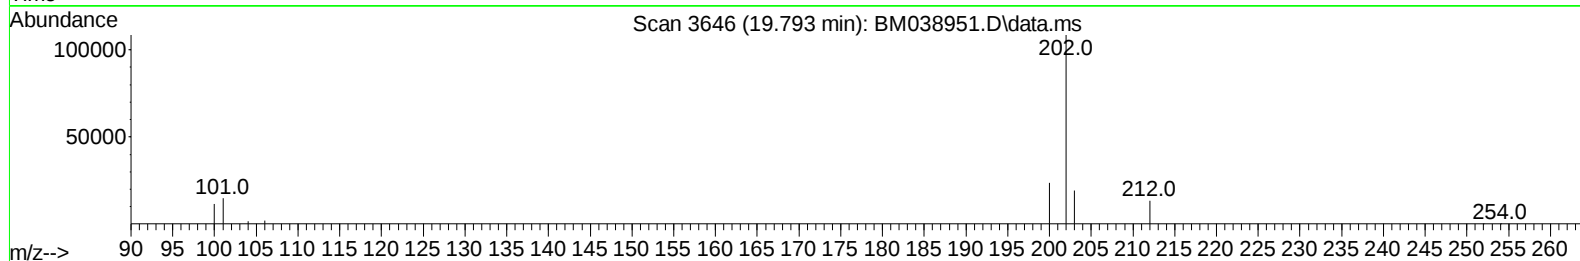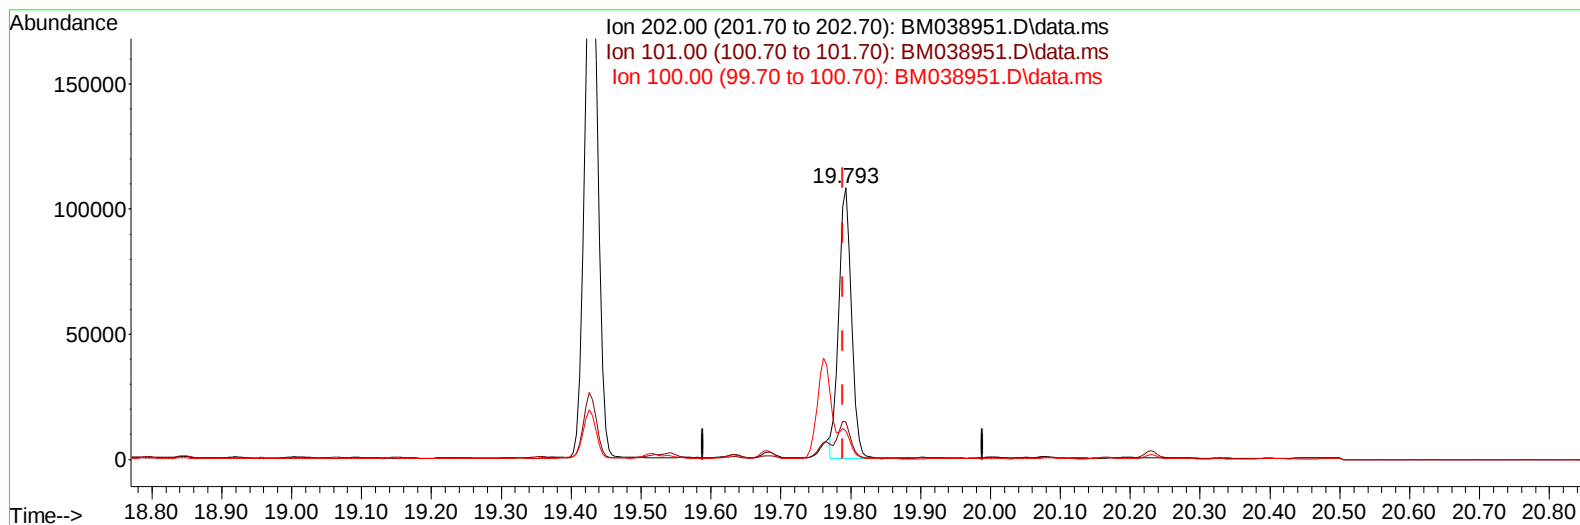

TIC: BM038951.D\data.ms

(20) Pyrene

19.793min (+ 0.005) 1.28 ng/ul m

response 136579

Ion	Exp%	Act%
202.00	100.00	100.00
101.00	14.00	13.70
100.00	11.30	10.60
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030923\
 Data File : BM038951.D
 Acq On : 09 Mar 2023 18:35
 Operator : CG/JU
 Sample : 01784-07
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DCAD9

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 03/10/2023
 Supervised By :Jagrut Upadhyay 03/10/2023

Quant Time: Mar 10 03:53:38 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM030323.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 09 13:36:03 2023
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.999	152		8995	0.400	ng/ul	0.00
4) Naphthalene-d8	10.811	136		31512	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.633	164		22193	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.375	188		42541	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.553	240		30635	0.400	ng/ul	0.00
23) Perylene-d12	24.002	264		22857	0.400	ng/ul	0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.376	96		50962	5.007	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.395	152		16747	0.439	ng/ul	0.00
18) Fluoranthene-d10	19.398	212		39167	0.537	ng/ul	0.00
Target Compounds							Qvalue
5) Naphthalene	10.861	128		3618557	48.030	ng/ul	100
7) 2-Methylnaphthalene	12.466	142		67610	1.479	ng/ul	100
8) 1-Methylnaphthalene	12.686	142		781715	16.300	ng/ul	98
10) Acenaphthylene	14.355	152		220462	2.732	ng/ul	98
11) Acenaphthene	14.702	153		4403368	66.348	ng/ul	92
12) Fluorene	15.678	166		951592	12.700	ng/ul	98
14) Pentachlorophenol	17.024	266		2635	0.257	ng/ul	99
15) Phenanthrene	17.421	178		3311754	29.449	ng/ul	99
16) Anthracene	17.510	178		325368	3.514	ng/ul	99
19) Fluoranthene	19.431	202		280316	2.702	ng/ul	99
20) Pyrene	19.793	202		136579m	1.282	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030923\
Data File : BM038951.D
Acq On : 09 Mar 2023 18:35
Operator : CG/JU
Sample : 01784-07
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DCAD9

Manual IntegrationsAPPROVED

Quant Time: Mar 10 03:53:38 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM030323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 09 13:36:03 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 03/10/2023
Supervised By :Jagrut Upadhyay 03/10/2023

