

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030923\
 Data File : BM038953.D
 Acq On : 09 Mar 2023 19:53
 Operator : CG/JU
 Sample : 01784-09
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DCAF3

Quant Time: Mar 10 03:53:57 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM030323.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 09 13:36:03 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.995	152	9982	0.400	ng/u1	0.00
4) Naphthalene-d8	10.811	136	35160	0.400	ng/u1	0.00
9) Acenaphthene-d10	14.633	164	19917	0.400	ng/u1	0.00
13) Phenanthrene-d10	17.374	188	41237	0.400	ng/u1	0.00
17) Chrysene-d12	21.553	240	30452	0.400	ng/u1	0.00
23) Perylene-d12	23.999	264	24596	0.400	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.375	96	52678	4.664	ng/u1	0.00
6) 2-Methylnaphthalene-d10	12.395	152	14640	0.344	ng/u1	0.00
18) Fluoranthene-d10	19.398	212	33105	0.457	ng/u1	0.00
Target Compounds						
11) Acenaphthene	14.693	153	1402	0.024	ng/u1	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030923\
Data File : BM038953.D
Acq On : 09 Mar 2023 19:53
Operator : CG/JU
Sample : 01784-09
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DCAF3


Quant Time: Mar 10 03:53:57 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM030323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 09 13:36:03 2023
Response via : Initial Calibration

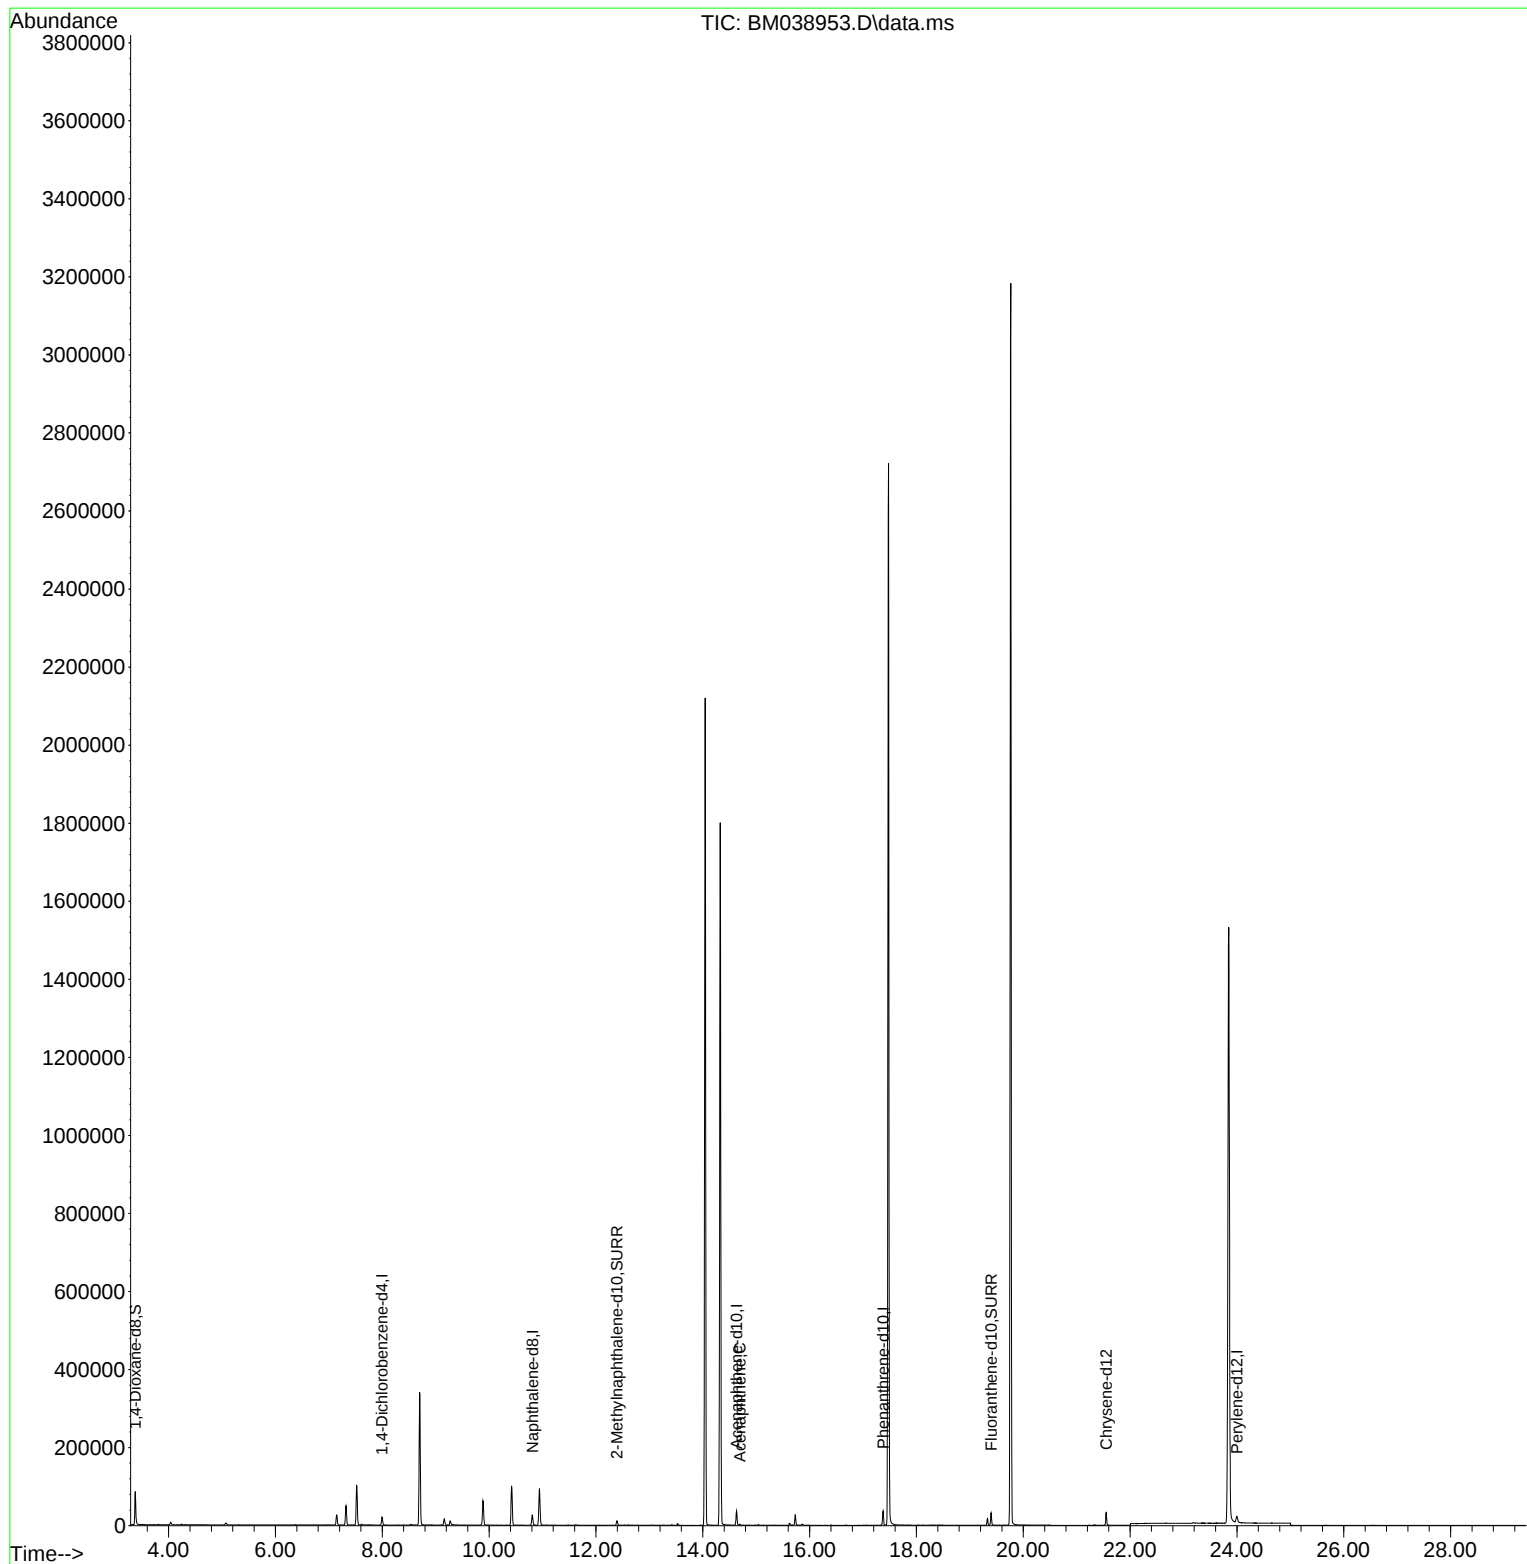

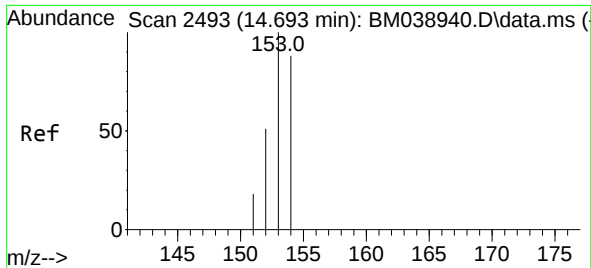

#11
Acenaphthene
Concen: 0.024 ng/ul
RT: 14.693 min Scan# 24
Delta R.T. -0.000 min
Lab File: BM038953.D
Acq: 09 Mar 2023 19:53

Instrument :
BNA_M
ClientSampleId :
DCAF3

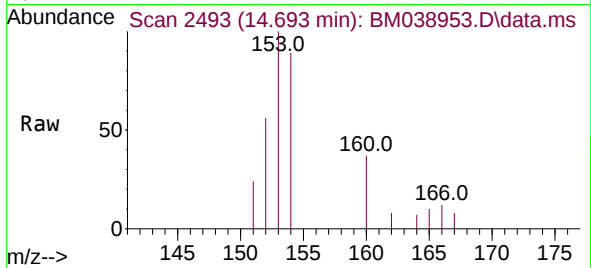

Tgt Ion:	153	Resp:	1402
Ion Ratio	Lower	Upper	
153	100		
152	55.7	44.2	66.2
154	89.2	70.6	105.8

