

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030923\
 Data File : BM038957.D
 Acq On : 09 Mar 2023 23:03
 Operator : CG/JU
 Sample : 01729-01
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0BY5

Quant Time: Mar 10 03:54:31 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM030323.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 09 13:36:03 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.995	152	8971	0.400	ng/u1	0.00
4) Naphthalene-d8	10.806	136	29800	0.400	ng/u1	0.00
9) Acenaphthene-d10	14.633	164	17242	0.400	ng/u1	0.00
13) Phenanthrene-d10	17.374	188	36332	0.400	ng/u1	0.00
17) Chrysene-d12	21.550	240	30021	0.400	ng/u1	0.00
23) Perylene-d12	23.996	264	24533	0.400	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.375	96	36620	3.608	ng/u1	0.00
6) 2-Methylnaphthalene-d10	12.389	152	8150	0.226	ng/u1	0.00
18) Fluoranthene-d10	19.398	212	20723	0.290	ng/u1	0.00
Target Compounds						
15) Phenanthrene	17.412	178	2108	0.022	ng/u1#	Qvalue 86


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030923\
Data File : BM038957.D
Acq On : 09 Mar 2023 23:03
Operator : CG/JU
Sample : 01729-01
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0BY5


Quant Time: Mar 10 03:54:31 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM030323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 09 13:36:03 2023
Response via : Initial Calibration

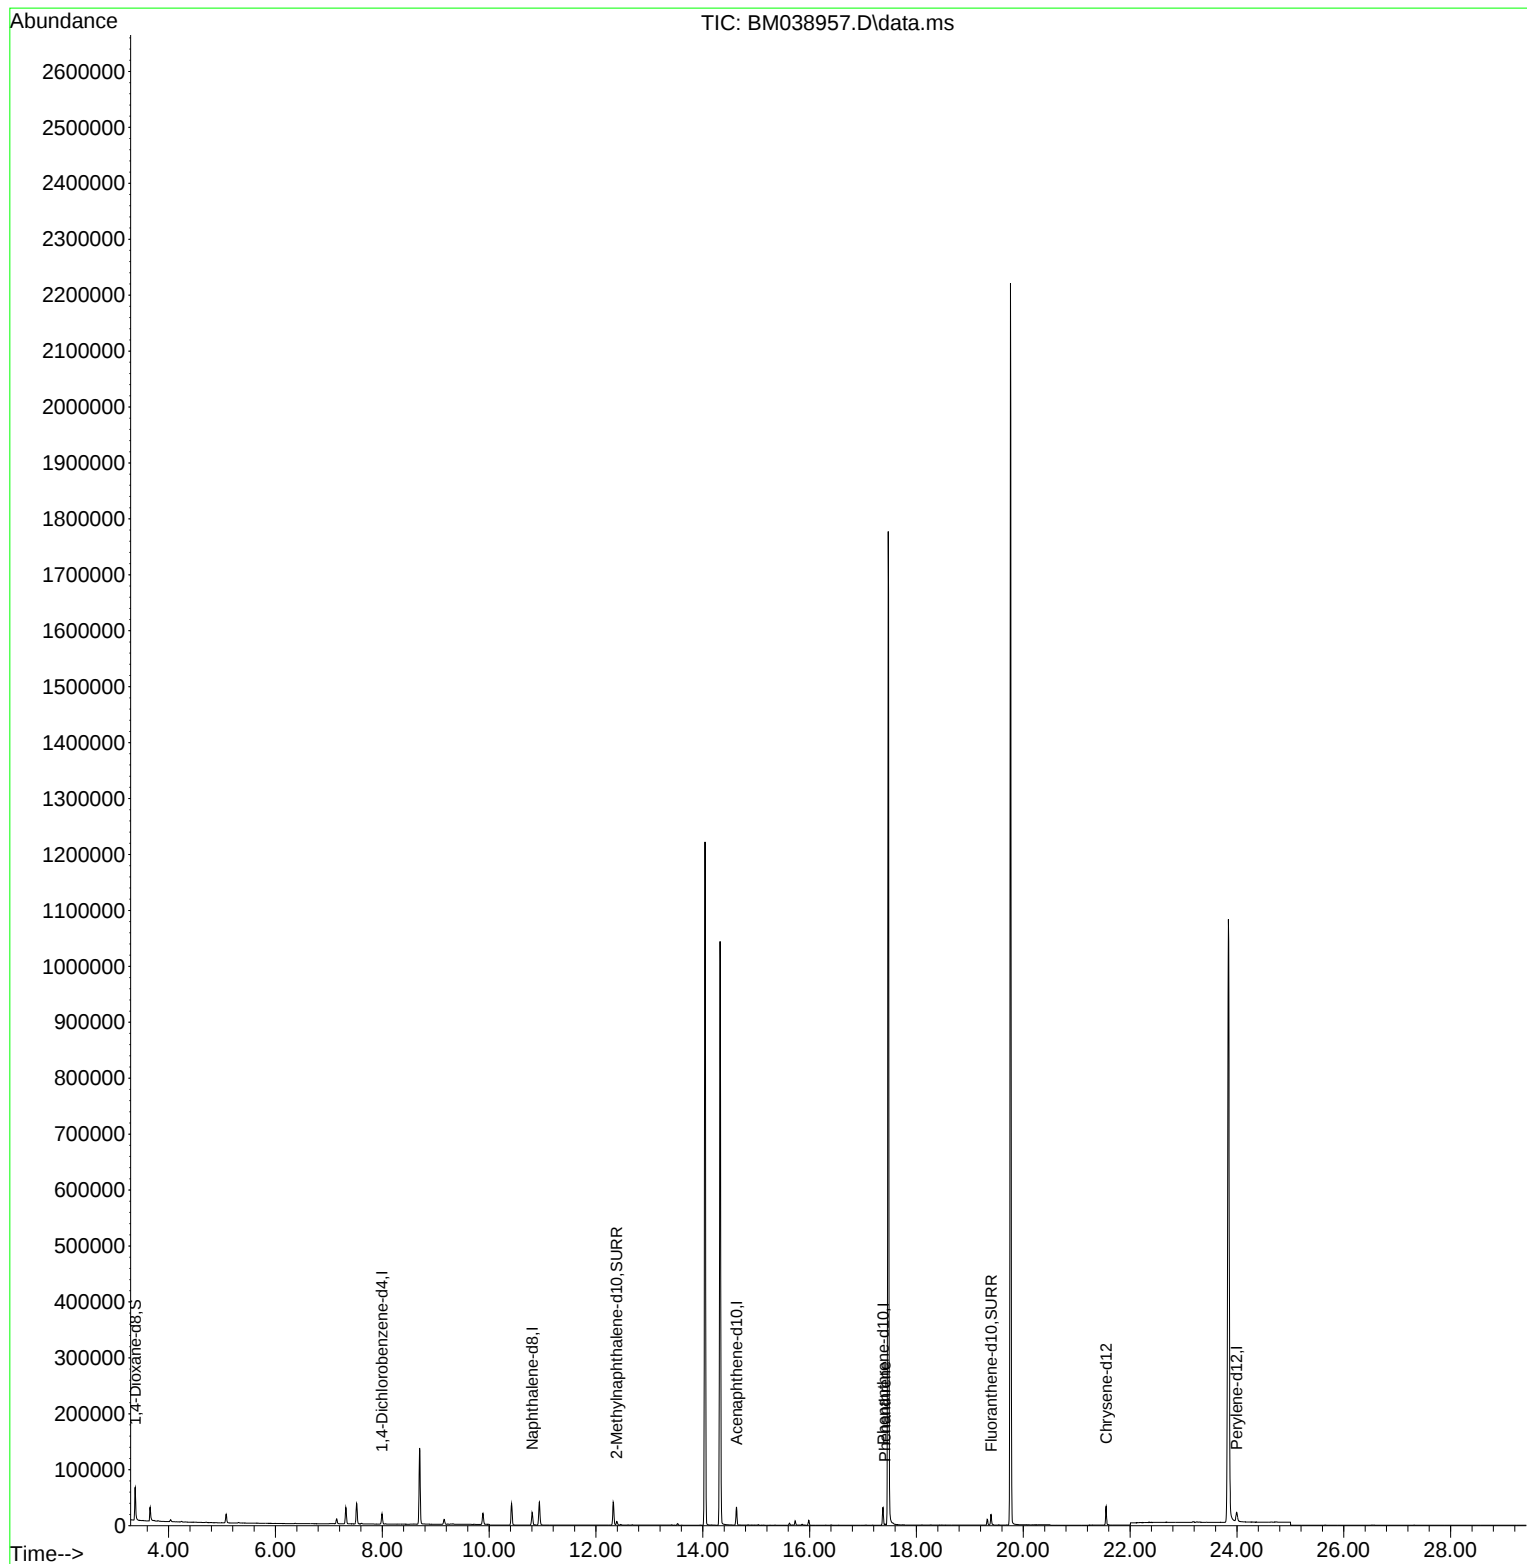

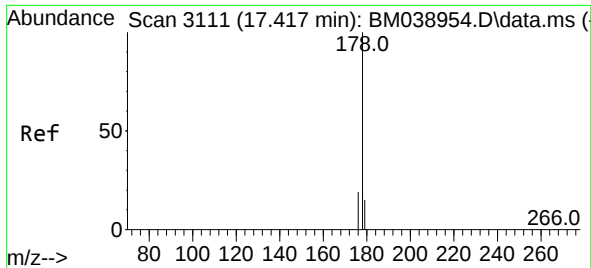

#15
 Phenanthrene
 Concen: 0.022 ng/ul
 RT: 17.412 min Scan# 3110
 Delta R.T. -0.004 min
 Lab File: BM038957.D
 Acq: 09 Mar 2023 23:03

Instrument :
 BNA_M
 ClientSampleId :
 C0BY5

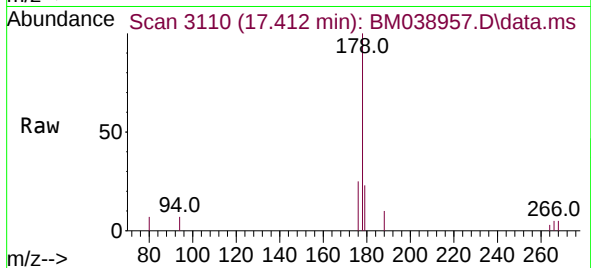

Tgt Ion:	178	Resp:	2108
Ion Ratio	Lower	Upper	
178	100		
179	23.4	12.7	19.1#
176	24.6	15.9	23.9#

