

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030923\
 Data File : BM038958.D
 Acq On : 09 Mar 2023 23:41
 Operator : CG/JU
 Sample : 01729-02
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0BY6

Quant Time: Mar 10 03:54:38 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM030323.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 09 13:36:03 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.995	152	11146	0.400	ng/u1	0.00
4) Naphthalene-d8	10.804	136	38810	0.400	ng/u1	0.00
9) Acenaphthene-d10	14.631	164	21908	0.400	ng/u1	0.00
13) Phenanthrene-d10	17.373	188	45432	0.400	ng/u1	0.00
17) Chrysene-d12	21.551	240	33952	0.400	ng/u1	0.00
23) Perylene-d12	23.995	264	27081	0.400	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.375	96	54383	4.312	ng/u1	0.00
6) 2-Methylnaphthalene-d10	12.393	152	14574	0.310	ng/u1	0.00
18) Fluoranthene-d10	19.397	212	32715	0.405	ng/u1	0.00
Target Compounds						
7) 2-Methylnaphthalene	12.465	142	1946	0.035	ng/u1	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030923\
Data File : BM038958.D
Acq On : 09 Mar 2023 23:41
Operator : CG/JU
Sample : 01729-02
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0BY6

Quant Time: Mar 10 03:54:38 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM030323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 09 13:36:03 2023
Response via : Initial Calibration

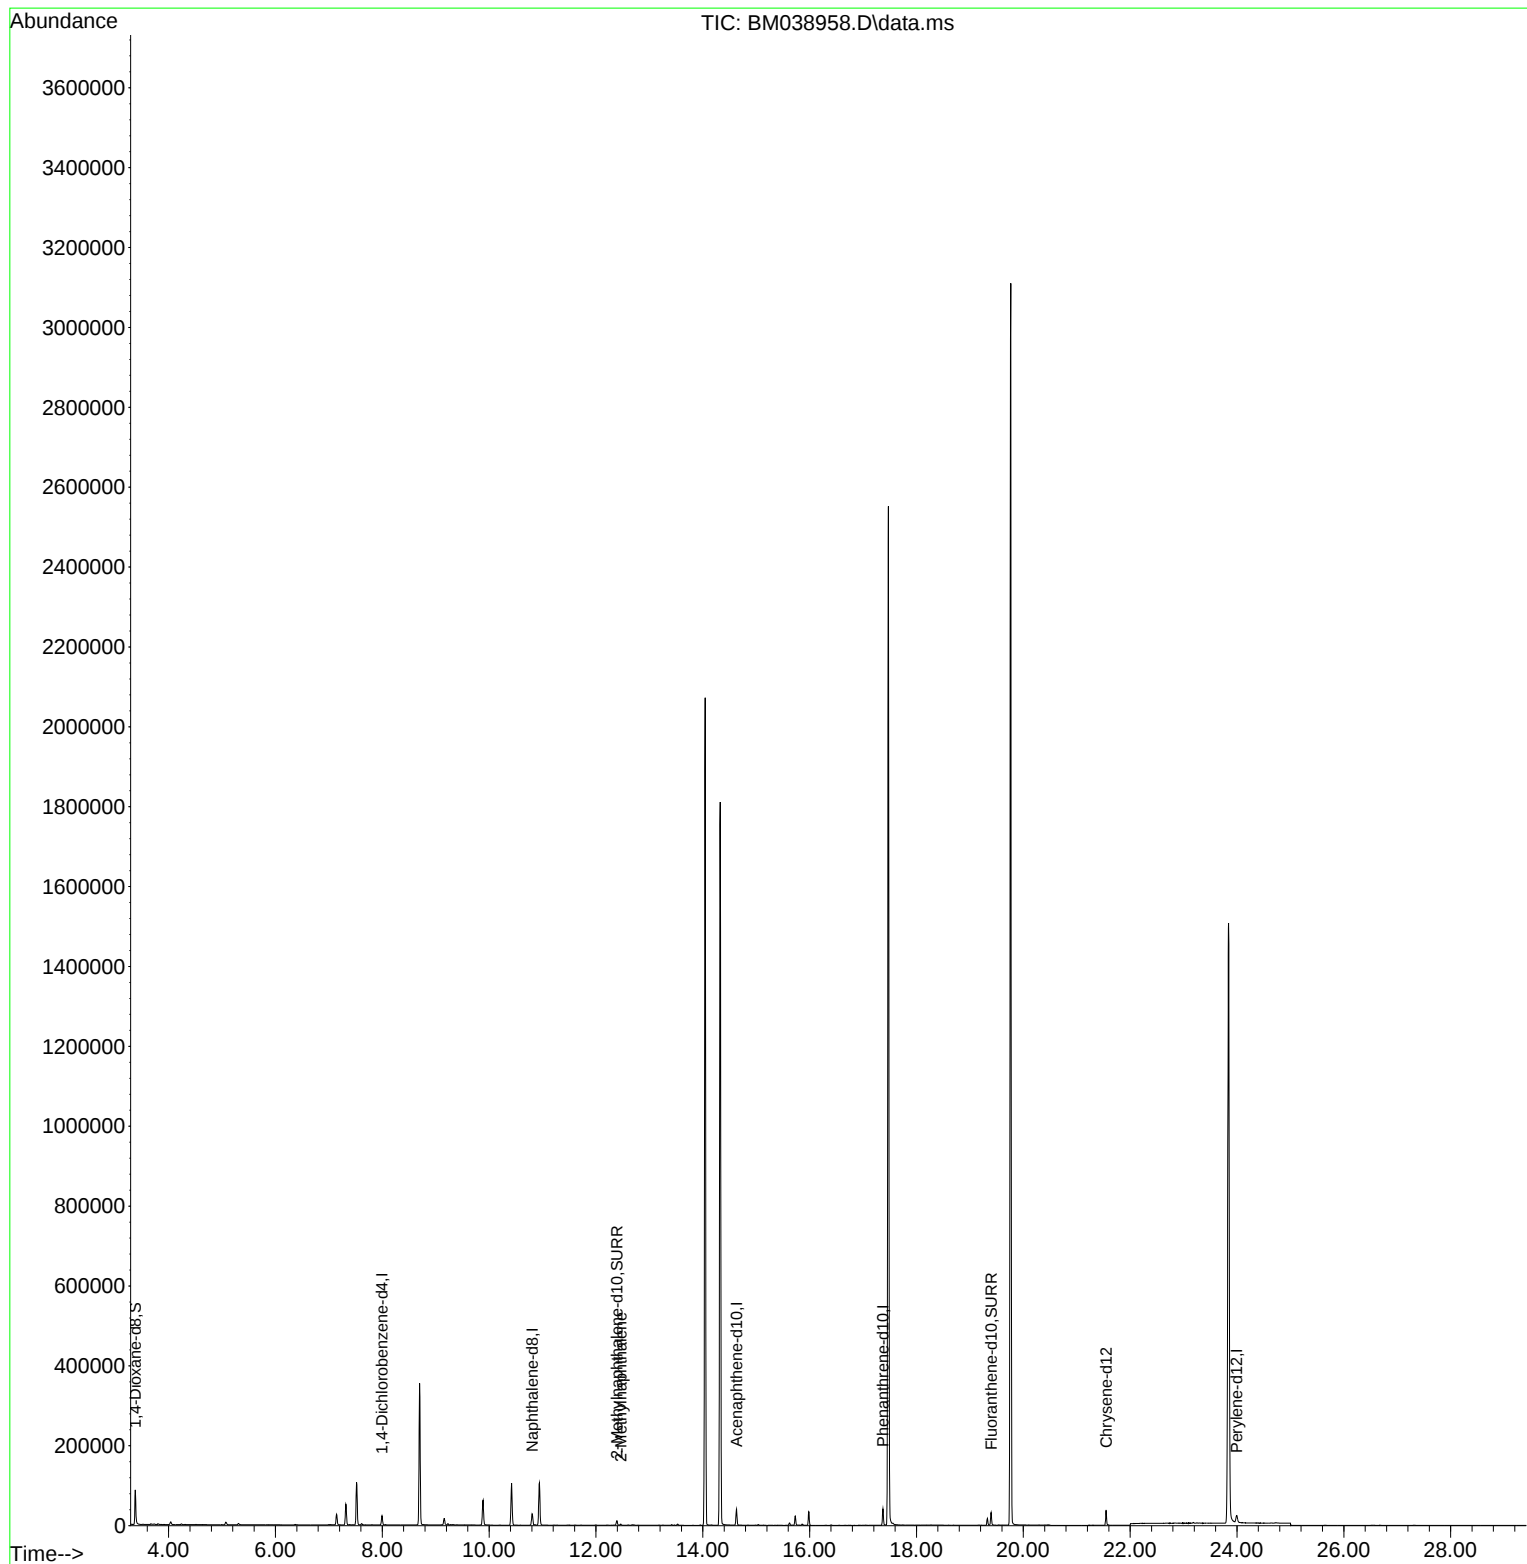

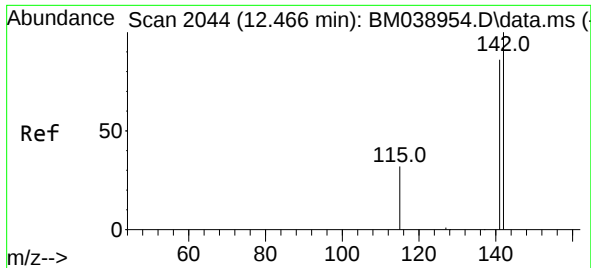

#7
 2-Methylnaphthalene
 Concen: 0.035 ng/ul
 RT: 12.465 min Scan# 2044
 Delta R.T. -0.001 min
 Lab File: BM038958.D
 Acq: 09 Mar 2023 23:41

Instrument :
 BNA_M
 ClientSampleId :
 C0BY6

Tgt Ion:142 Resp: 1946
 Ion Ratio Lower Upper
 142 100
 141 88.1 69.9 104.9

