

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030923\
 Data File : BM038981.D
 Acq On : 10 Mar 2023 15:03
 Operator : CG/JU
 Sample : 01784-20DL 5X
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DCAE9DL

Manual Integrations
 APPROVED

Reviewed By : Christian Giraldo 03/13/2023
 Supervised By : Jagrut Upadhyay 03/13/2023

Quant Time: Mar 10 23:15:59 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM030323.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 09 13:36:03 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.991	152	8207	0.400	ng/ul	0.00
4) Naphthalene-d8	10.805	136	28954	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.628	164	17913	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.370	188	35479	0.400	ng/ul	0.00
17) Chrysene-d12	21.553	240	28030	0.400	ng/ul	0.00
23) Perylene-d12	23.996	264	23854	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.375	96	3769	0.406	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.389	152	2526	0.072	ng/ul	0.00
18) Fluoranthene-d10	19.393	212	5806	0.087	ng/ul	0.00
Target Compounds						Qvalue
5) Naphthalene	10.860	128	10313359	148.986	ng/ul	98
7) 2-Methylnaphthalene	12.461	142	539963	12.855	ng/ul	100
8) 1-Methylnaphthalene	12.681	142	808852	18.355	ng/ul	98
10) Acenaphthylene	14.350	152	65238	1.002	ng/ul#	97
11) Acenaphthene	14.693	153	1357724	25.345	ng/ul	93
12) Fluorene	15.673	166	731944	12.103	ng/ul	99
14) Pentachlorophenol	17.020	266	16901	1.980	ng/ul	99
15) Phenanthrene	17.412	178	672049	7.166	ng/ul	99
16) Anthracene	17.505	178	50429	0.653	ng/ul	99
19) Fluoranthene	19.426	202	52862	0.557	ng/ul	99
20) Pyrene	19.788	202	24162m	0.248	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030923\
Data File : BM038981.D
Acq On : 10 Mar 2023 15:03
Operator : CG/JU
Sample : 01784-20DL 5X
Misc :
ALS Vial : 44 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
DCAE9DL

Manual Integrations
APPROVED

Reviewed By :Christian Giraldo 03/13/2023
Supervised By :Jagrut Upadhyay 03/13/2023


Quant Time: Mar 10 23:15:59 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM030323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 09 13:36:03 2023
Response via : Initial Calibration

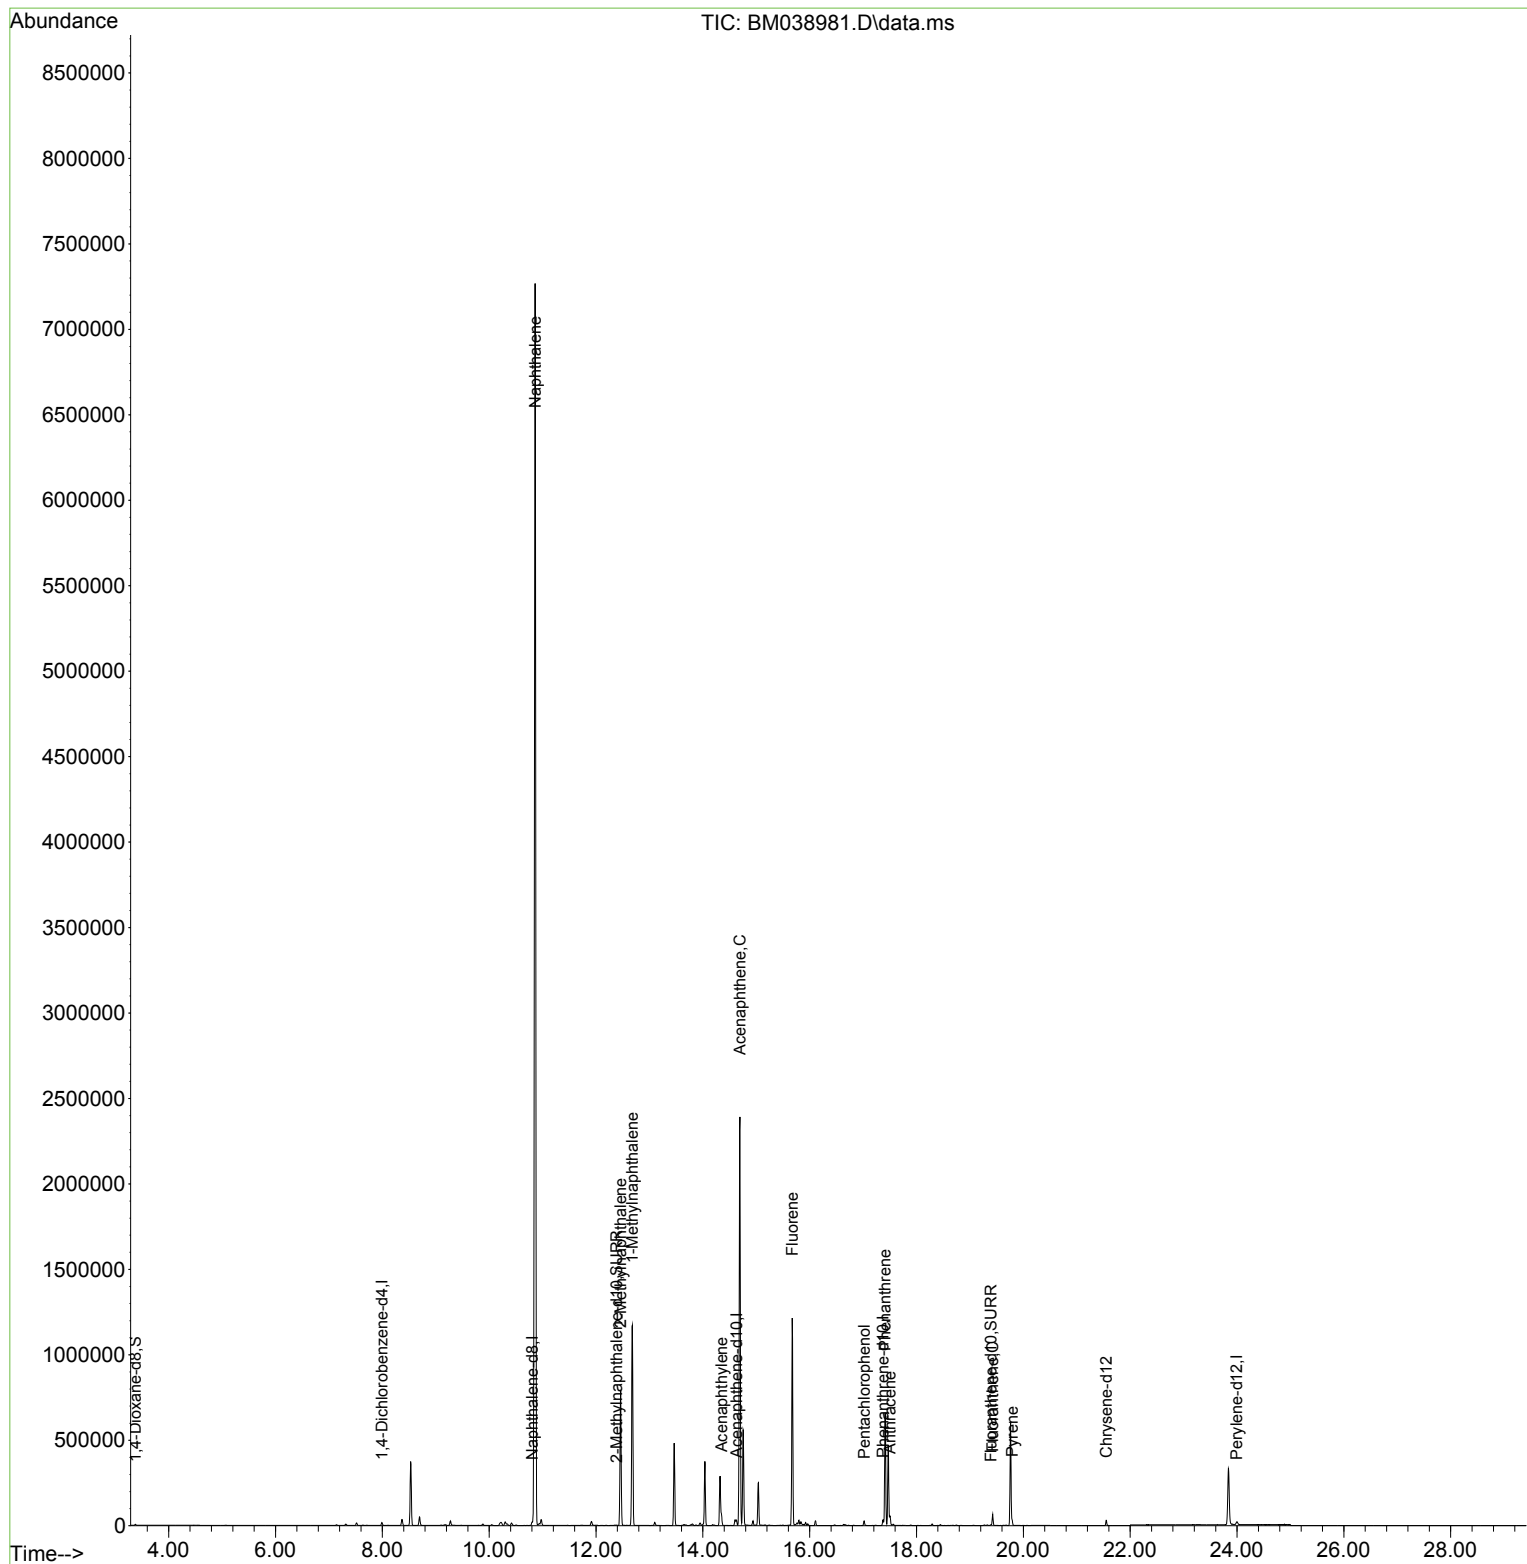

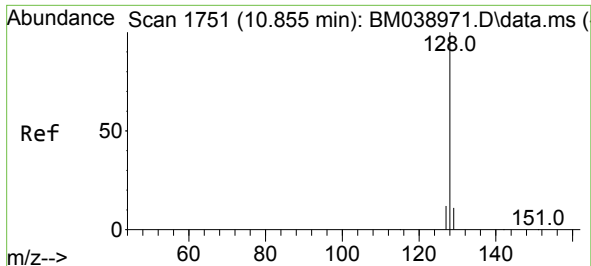

#5
Naphthalene
Concen: 148.986 ng/ul
RT: 10.860 min Scan# 1751
Delta R.T. 0.005 min
Lab File: BM038981.D
Acq: 10 Mar 2023 15:03




Instrument :
BNA_M
ClientSampleId :
DCAE9DL

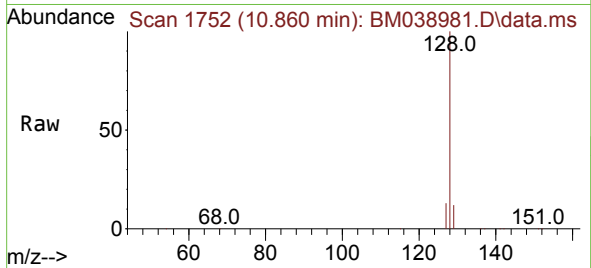

Tgt Ion:128 Resp:1031335
Ion Ratio Lower Upper
128 100
129 12.2 9.1 13.7
127 13.4 10.3 15.5




Manual Integrations
APPROVED


Reviewed By :Christian Giraldo 03/13/2023
Supervised By :Jagrut Upadhyay 03/13/2023

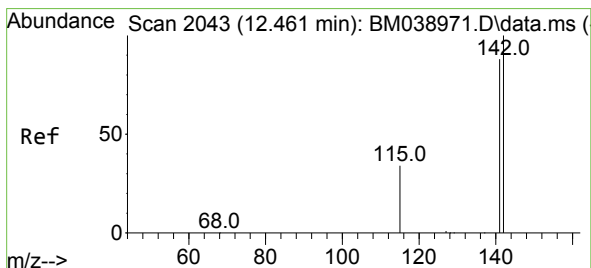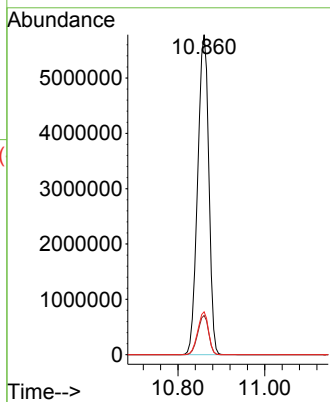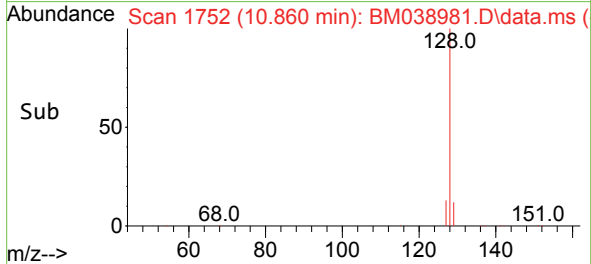

#7
2-Methylnaphthalene
Concen: 12.855 ng/ul
RT: 12.461 min Scan# 2043
Delta R.T. -0.006 min
Lab File: BM038981.D
Acq: 10 Mar 2023 15:03


Tgt Ion:142 Resp: 539963
Ion Ratio Lower Upper
142 100
141 87.2 69.9 104.9

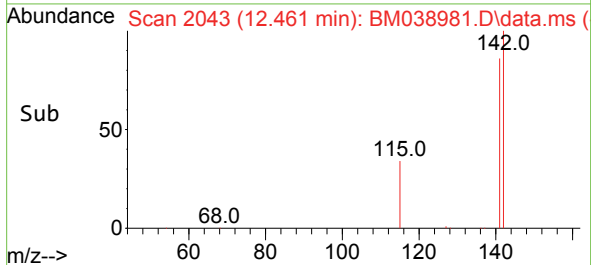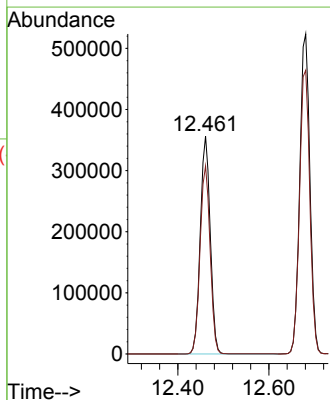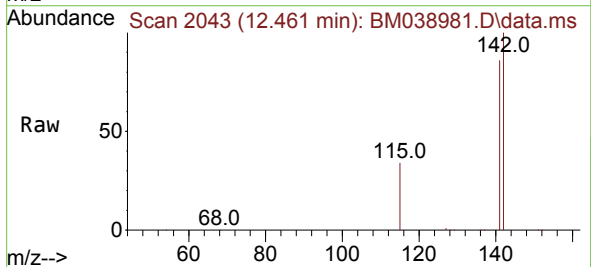

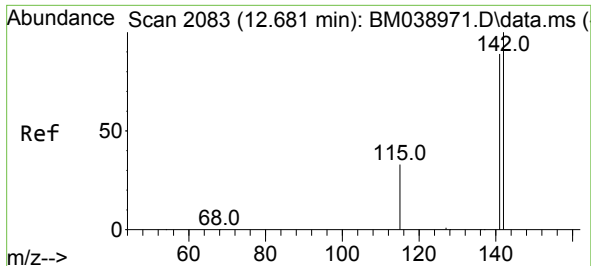

#8
1-Methylnaphthalene
Concen: 18.355 ng/ul
RT: 12.681 min Scan# 2083
Delta R.T. -0.000 min
Lab File: BM038981.D
Acq: 10 Mar 2023 15:03




Instrument :
BNA_M
ClientSampleId :
DCAE9DL

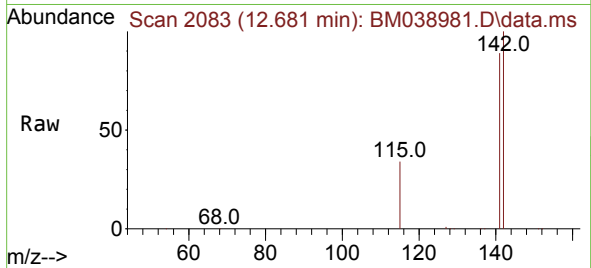

Tgt Ion:142 Resp: 80885
Ion Ratio Lower Upper
142 100
141 89.9 73.5 110.3




Manual Integrations
APPROVED


Reviewed By :Christian Giraldo 03/13/2023
Supervised By :Jagrut Upadhyay 03/13/2023

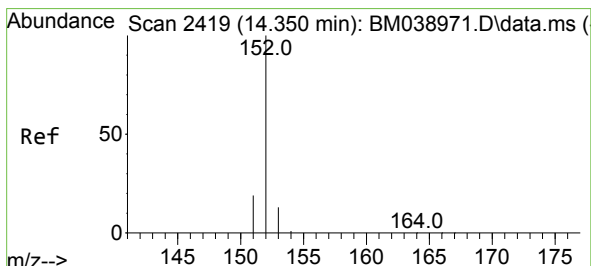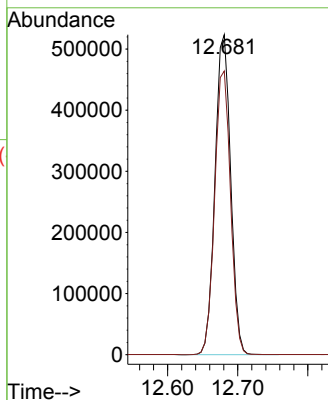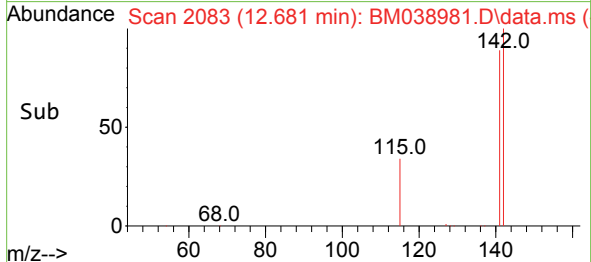

#10
Acenaphthylene
Concen: 1.002 ng/ul
RT: 14.350 min Scan# 2419
Delta R.T. -0.000 min
Lab File: BM038981.D
Acq: 10 Mar 2023 15:03


Tgt Ion:152 Resp: 65238
Ion Ratio Lower Upper
152 100
151 19.5 15.6 23.4
153 16.2 10.6 15.8#

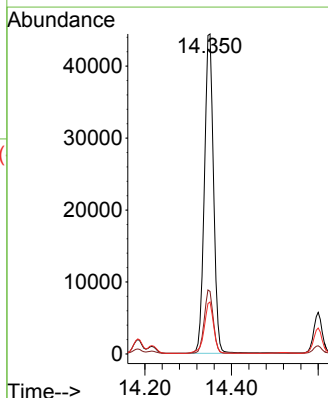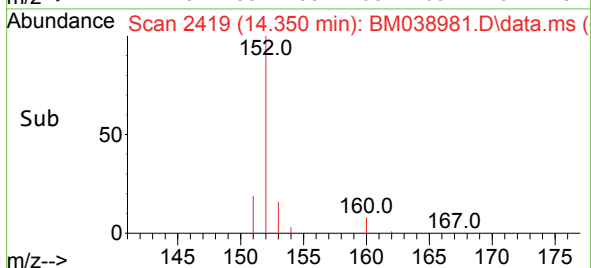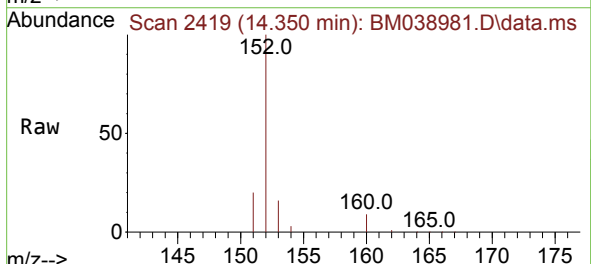

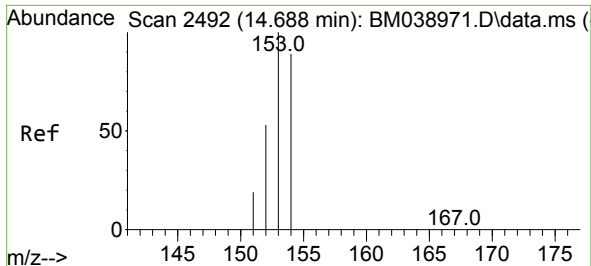

#11
Acenaphthene
Concen: 25.345 ng/ul
RT: 14.693 min Scan# 2493
Delta R.T. -0.000 min
Lab File: BM038981.D
Acq: 10 Mar 2023 15:03




Instrument :
BNA_M
ClientSampleId :
DCAE9DL

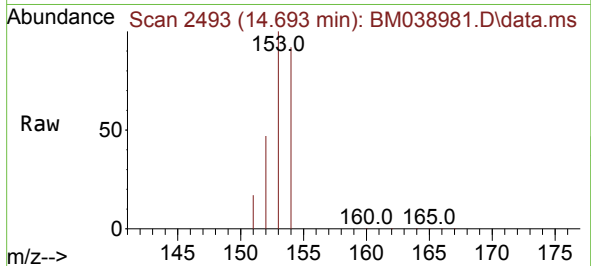

Tgt Ion:153 Resp: 1357724
Ion Ratio Lower Upper
153 100
152 47.4 44.2 66.2
154 92.2 70.6 105.8




Manual Integrations
APPROVED


Reviewed By :Christian Giraldo 03/13/2023
Supervised By :Jagrut Upadhyay 03/13/2023

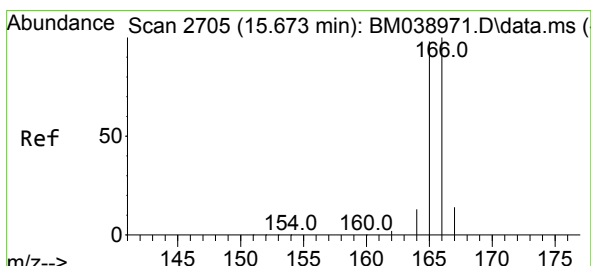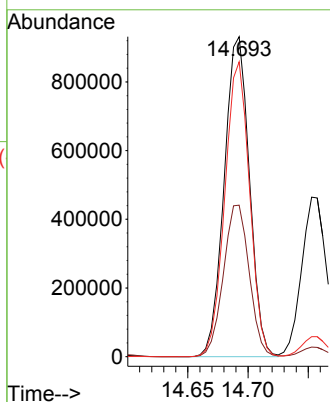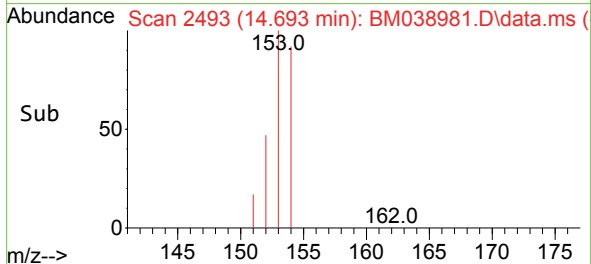

#12
Fluorene
Concen: 12.103 ng/ul
RT: 15.673 min Scan# 2705
Delta R.T. -0.005 min
Lab File: BM038981.D
Acq: 10 Mar 2023 15:03


Tgt Ion:166 Resp: 731944
Ion Ratio Lower Upper
166 100
165 95.8 77.8 116.6
167 13.7 11.4 17.2

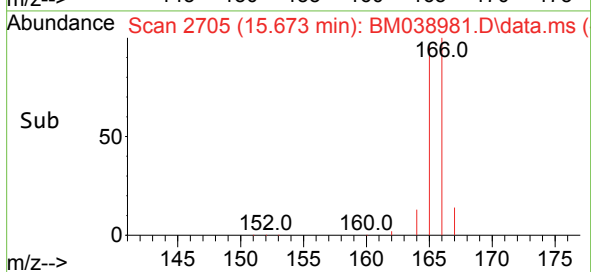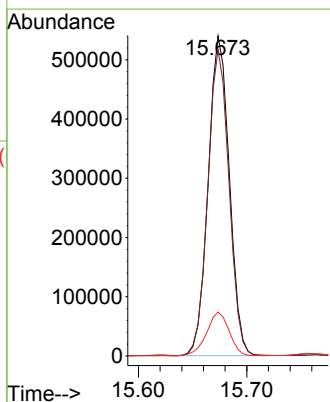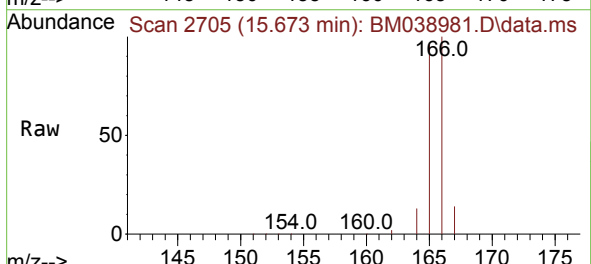

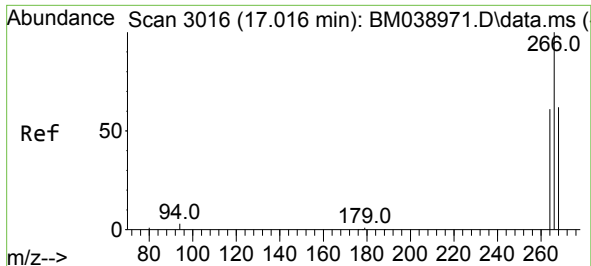

#14
Pentachlorophenol
Concen: 1.980 ng/ul
RT: 17.020 min Scan# 3016
Delta R.T. -0.000 min
Lab File: BM038981.D
Acq: 10 Mar 2023 15:03




Instrument :
BNA_M
ClientSampleId :
DCAE9DL

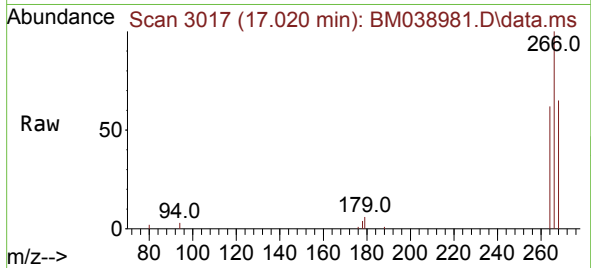

Tgt Ion:266 Resp: 1690
Ion Ratio Lower Upper
266 100
264 62.6 50.2 75.2
268 64.0 50.2 75.4




Manual Integrations
APPROVED


Reviewed By :Christian Giraldo 03/13/2023
Supervised By :Jagrut Upadhyay 03/13/2023

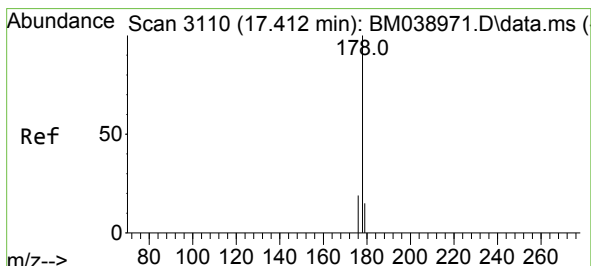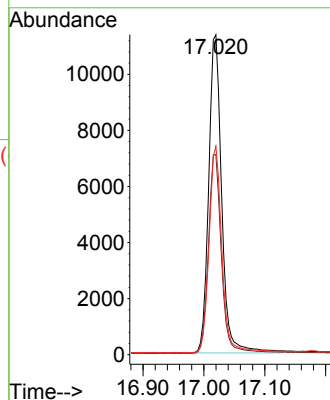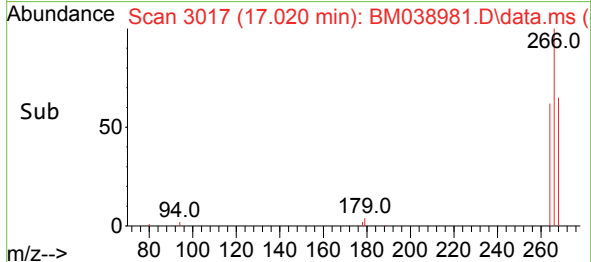

#15
Phenanthrene
Concen: 7.166 ng/ul
RT: 17.412 min Scan# 3110
Delta R.T. -0.004 min
Lab File: BM038981.D
Acq: 10 Mar 2023 15:03


Tgt Ion:178 Resp: 672049
Ion Ratio Lower Upper
178 100
179 15.4 12.7 19.1
176 19.3 15.9 23.9

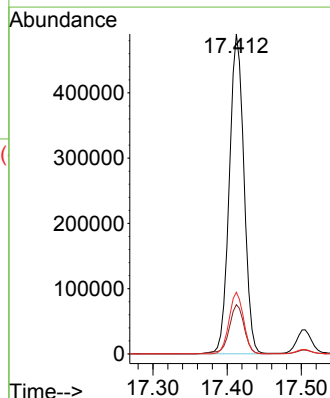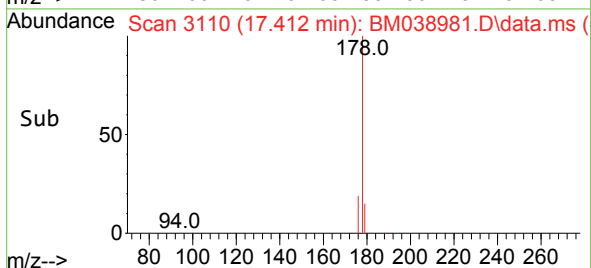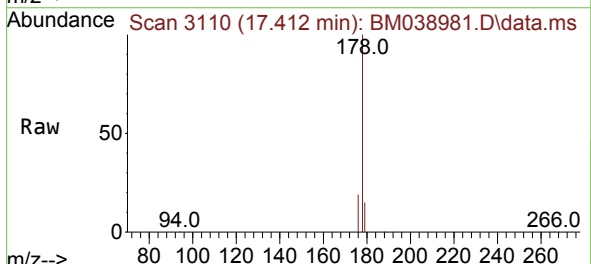

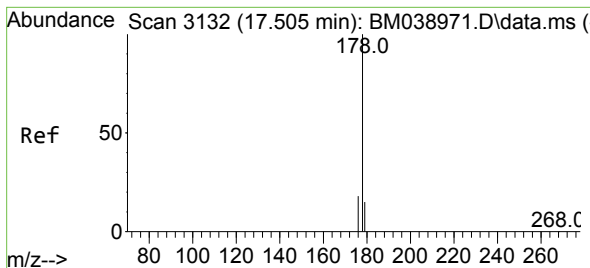

#16
 Anthracene
 Concen: 0.653 ng/ul
 RT: 17.505 min Scan# 3132
 Delta R.T. -0.000 min
 Lab File: BM038981.D
 Acq: 10 Mar 2023 15:03




Instrument :
 BNA_M
 ClientSampleId :
 DCAE9DL

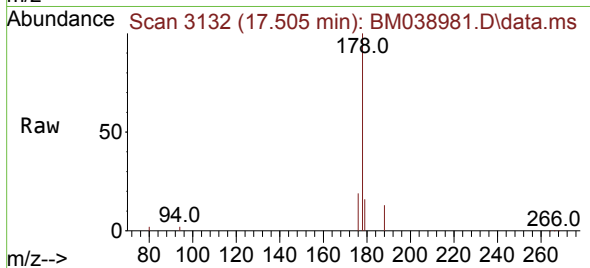


Tgt Ion:178 Resp: 50429
 Ion Ratio Lower Upper
 178 100
 179 15.7 13.0 19.6
 176 18.7 15.4 23.2

Manual Integrations
 APPROVED



Reviewed By :Christian Giraldo 03/13/2023
 Supervised By :Jagrut Upadhyay 03/13/2023

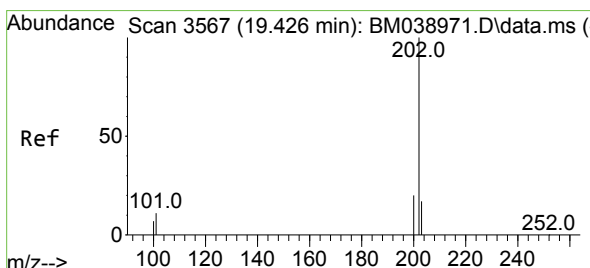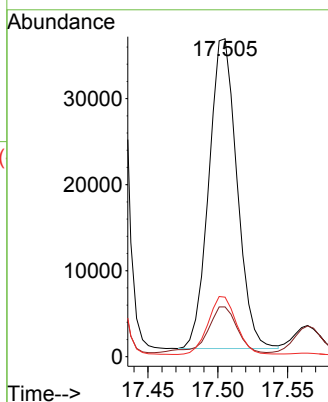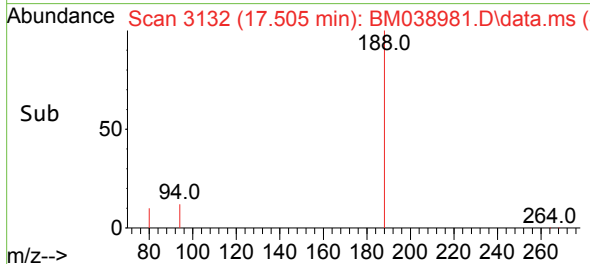


#19
 Fluoranthene
 Concen: 0.557 ng/ul
 RT: 19.426 min Scan# 3567
 Delta R.T. -0.000 min
 Lab File: BM038981.D
 Acq: 10 Mar 2023 15:03

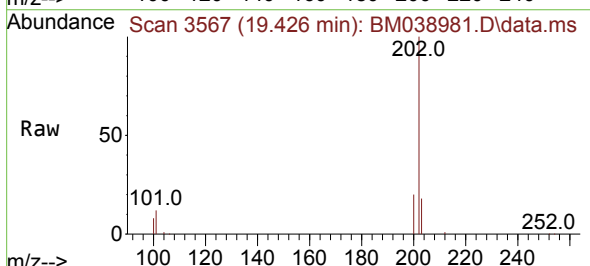


Tgt Ion:202 Resp: 52862
 Ion Ratio Lower Upper
 202 100
 101 11.6 8.9 13.3
 100 8.4 6.8 10.2

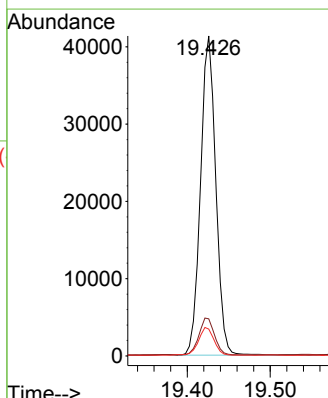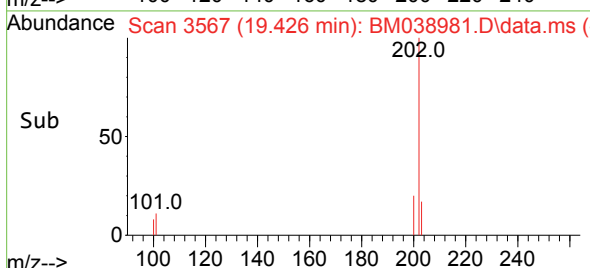

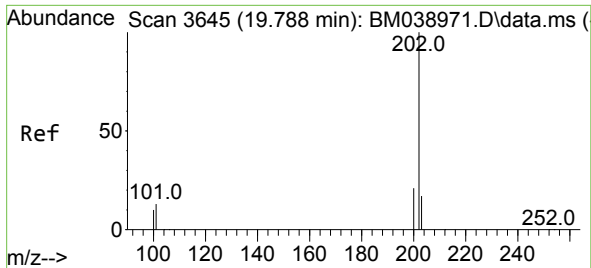

#20
Pyrene
Concen: 0.248 ng/ul m
RT: 19.788 min Scan# 30
Delta R.T. -0.000 min
Lab File: BM038981.D
Acq: 10 Mar 2023 15:03

Instrument :
BNA_M
ClientSampleId :
DCAE9DL

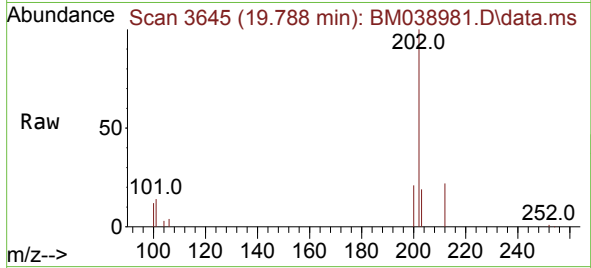

Tgt Ion:	202	Resp:	2416
Ion Ratio	Lower	Upper	
202	100		
101	14.0	11.2	16.8
100	11.5	9.0	13.6

Manual Integrations
APPROVED

Reviewed By :Christian Giraldo 03/13/2023
Supervised By :Jagrut Upadhyay 03/13/2023

