

Data Path : Z:\HPCHEM1\BNA M\DATA\BM031017\
 Data File : BM009180.D
 Acq On : 10 Mar 2017 18:10
 Operator : SJ/MA
 Sample : PB97487BL
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK87

Quant Time: Mar 11 00:54:38 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030317.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Mar 11 00:54:34 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.88	152	159	0.40	ng/ul	0.00
2) Naphthalene-d8	10.68	136	507	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.52	164	292	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.36	188	73281	0.40	ng/ul	0.10
16) Chrysene-d12	21.44	240	635	0.40	ng/ul	0.00
20) Perylene-d12	23.63	264	72202	0.40	ng/ul	-0.15
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.27	152	326	0.39	ng/ul	0.00
14) Fluoranthene-d10	19.30	212	853	0.00	ng/ul	0.00
Target Compounds						
9) Fluorene	15.51	166	152	0.11	ng/ul#	39
17) Pyrene	19.66	202	167	0.08	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM031017\
Data File : BM009180.D
Acq On : 10 Mar 2017 18:10
Operator : SJ/MA
Sample : PB97487BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK87

Quant Time: Mar 11 00:54:38 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Mar 11 00:54:34 2017
Response via : Initial Calibration

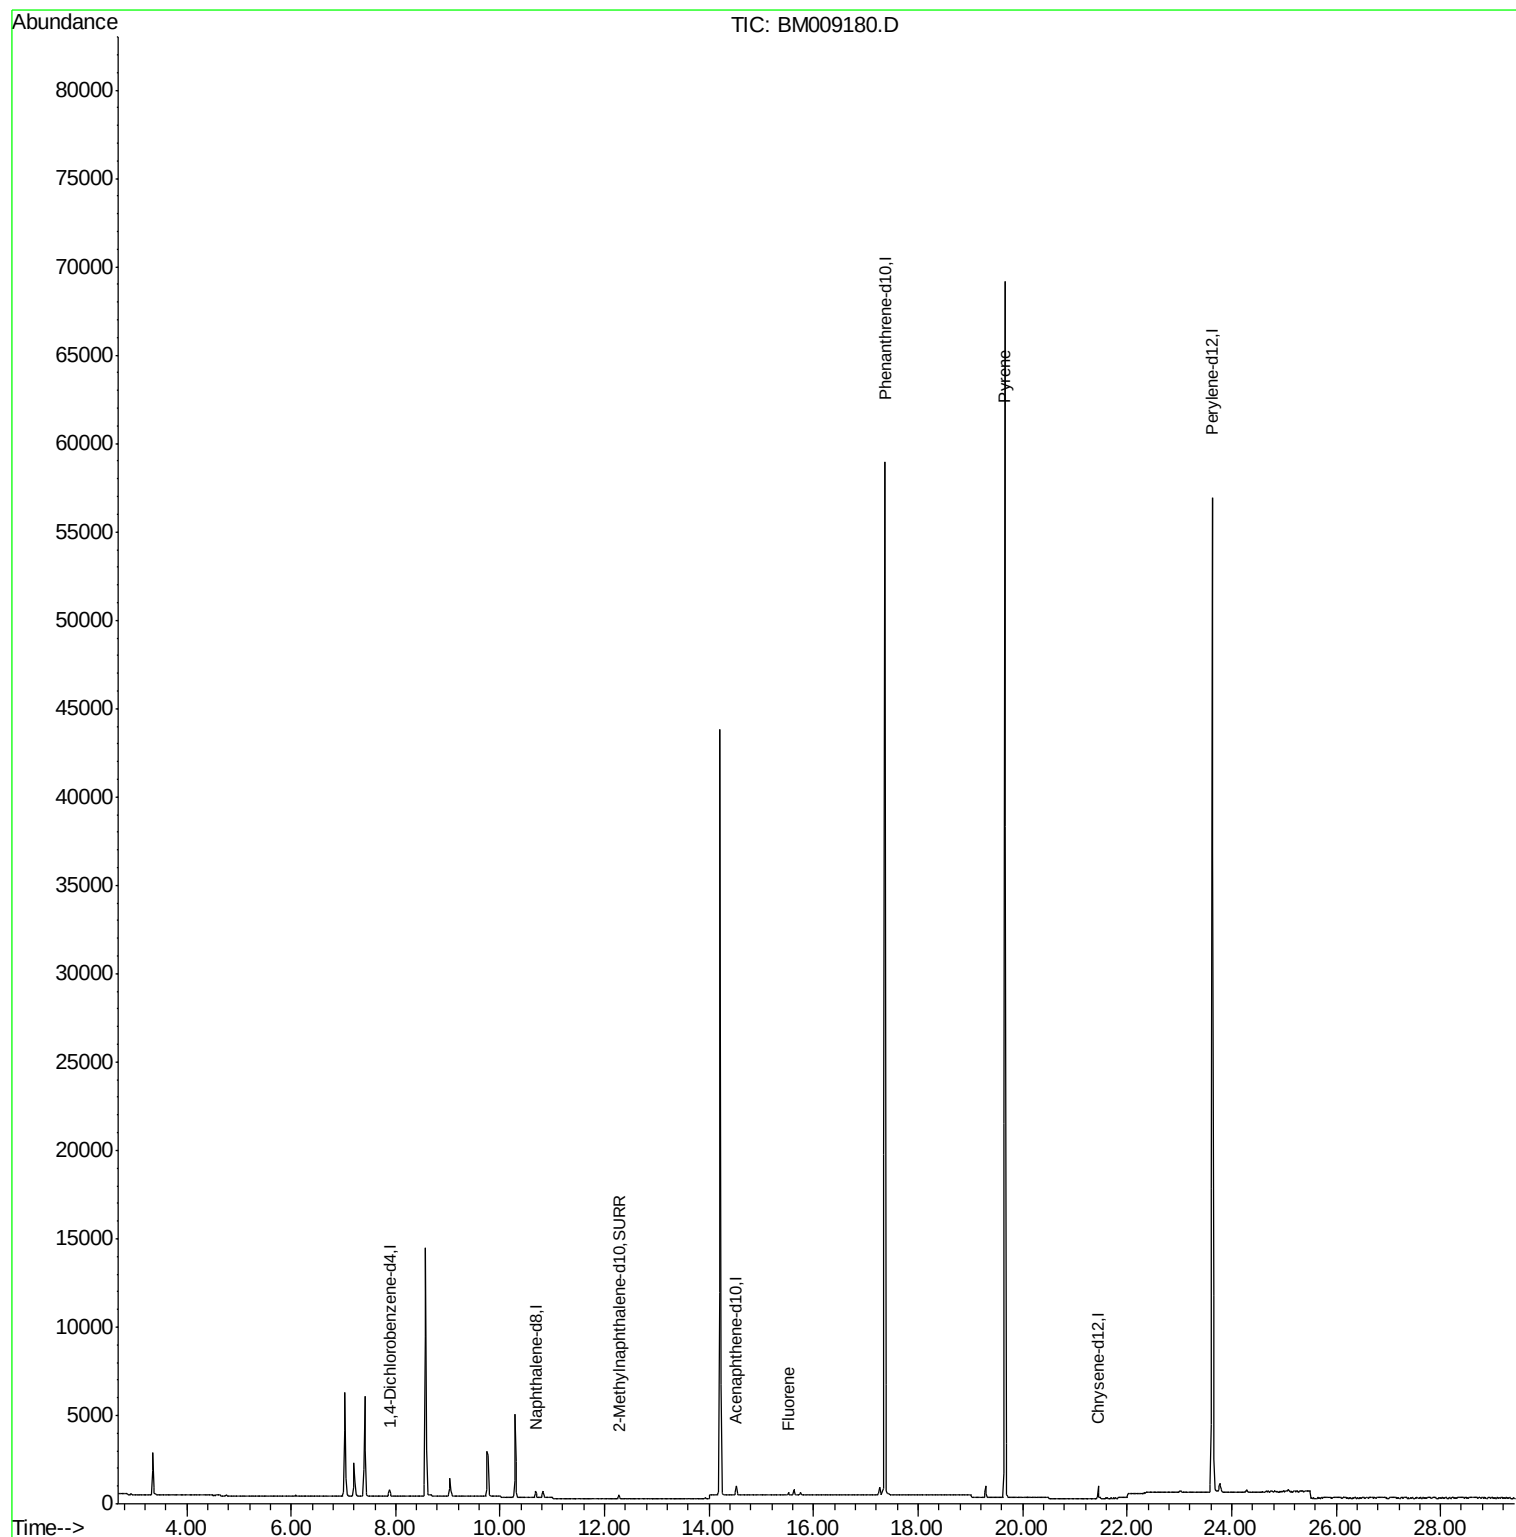

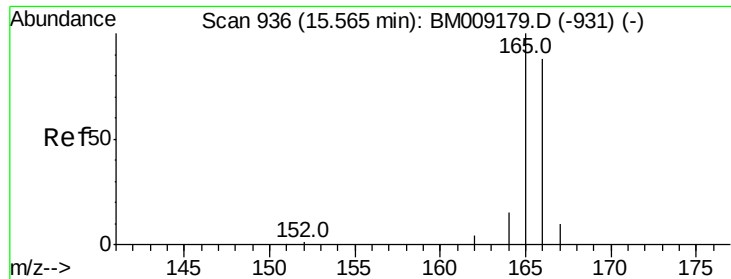

#9

Fluorene

Concen: 0.11 ng/ul

RT: 15.51 min Scan# 933

Delta R.T. -0.05 min

Lab File: BM009180.D

Acq: 10 Mar 2017 18:10

Instrument :

BNA_M

ClientSampleId :

SBLK87


Tot Ion:166 Resp: 152

Ion Ratio Lower Upper

166 100

165 36.2 73.4 110.2#




167 51.0 14.6 22.0#

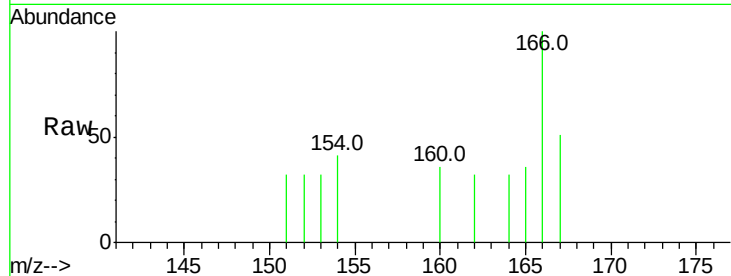

Abundance Ion 166.00 (165.70 to 166.70): E

Ion 165.00 (164.70 to 165.70): E

Ion 167.00 (166.70 to 167.70): E

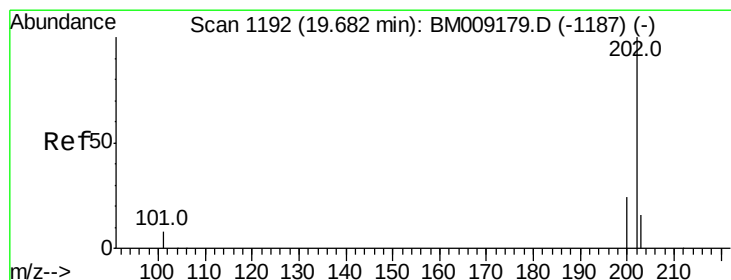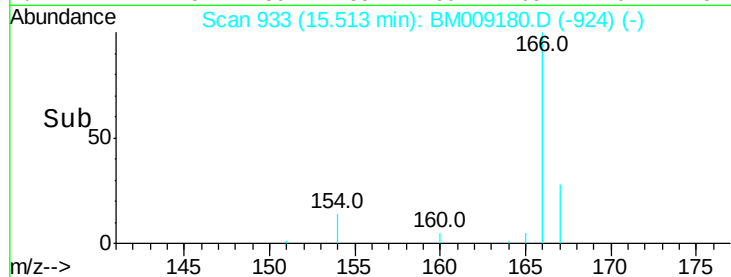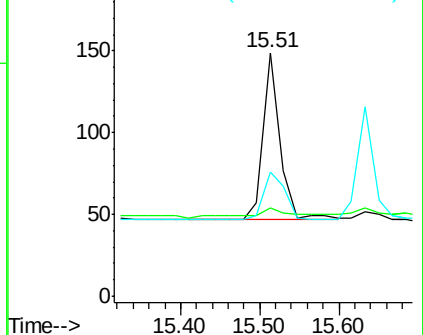

#17

Pyrene

Concen: 0.08 ng/ul

RT: 19.66 min Scan# 1190

Delta R.T. -0.02 min

Lab File: BM009180.D

Acq: 10 Mar 2017 18:10


Tgt Ion:202 Resp: 167

Ion Ratio Lower Upper

202 100

200 31.3 18.2 27.4#

203 141.7 15.6 23.4#

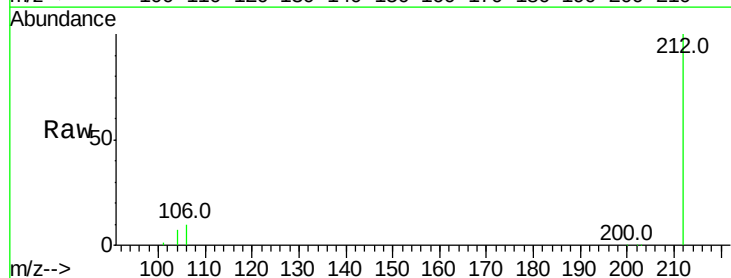

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 200.00 (199.70 to 200.70): E

Ion 203.00 (202.70 to 203.70): E

