


Data Path : Z:\HPCHEM1\BNA_M\Data\BM031017\
Data File : BM009173.D
Acq On : 10 Mar 2017 13:23
Operator : SJ/MA
Sample : I2062-06
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AC7

Manual Integrations
APPROVED

mohammad
3/13/2017 2:13:25 PM

Quant Time: Mar 10 16:23:17 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 10 15:19:24 2017
Response via : Initial Calibration

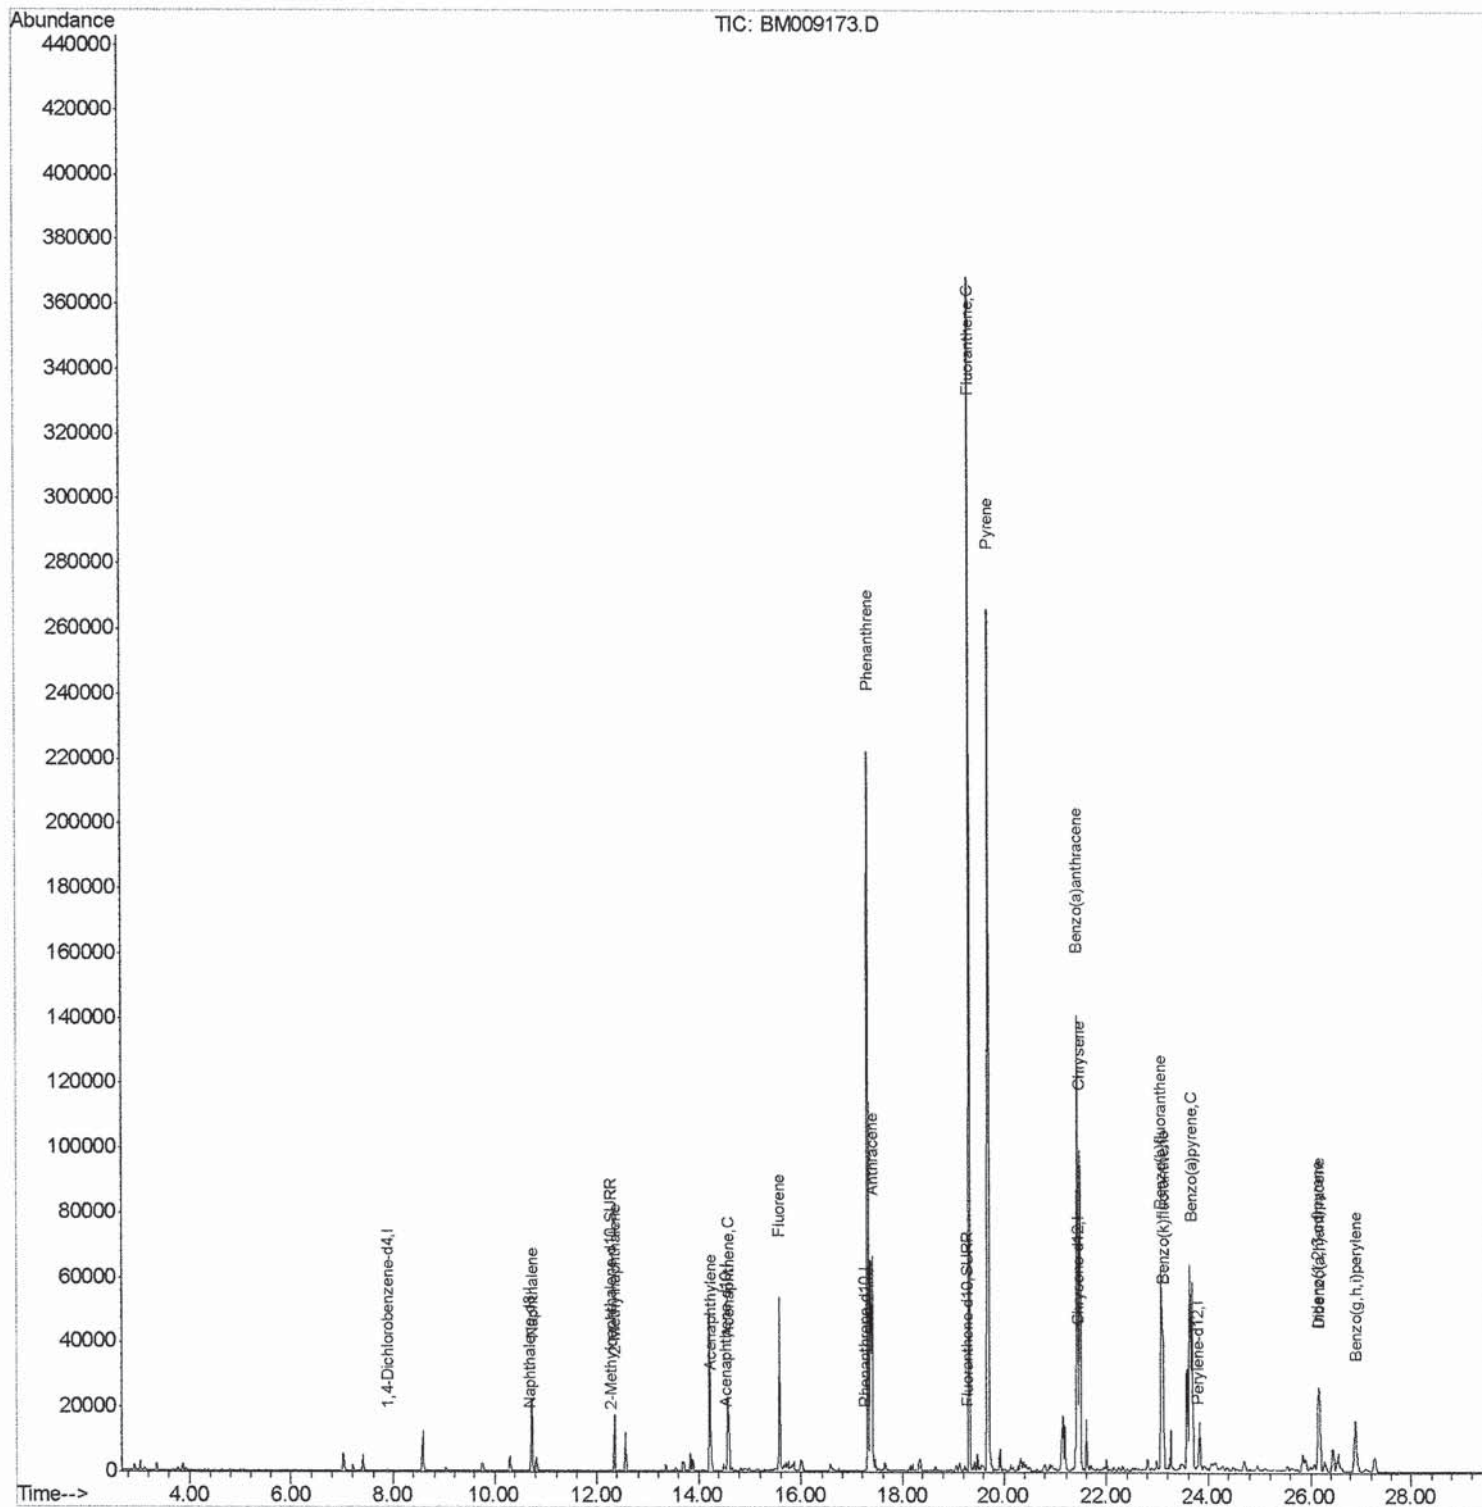




Data Path : Z:\HPCHEM1\BNA_M\Data\BM031017\
Data File : BM009173.D
Acq On : 10 Mar 2017 13:23
Operator : SJ/MA
Sample : I2062-06
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AC7

Manual Integrations
APPROVED

mohammad
3/13/2017 2:13:25 PM

Quant Time: Mar 10 15:43:09 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 10 15:19:24 2017
Response via : Initial Calibration

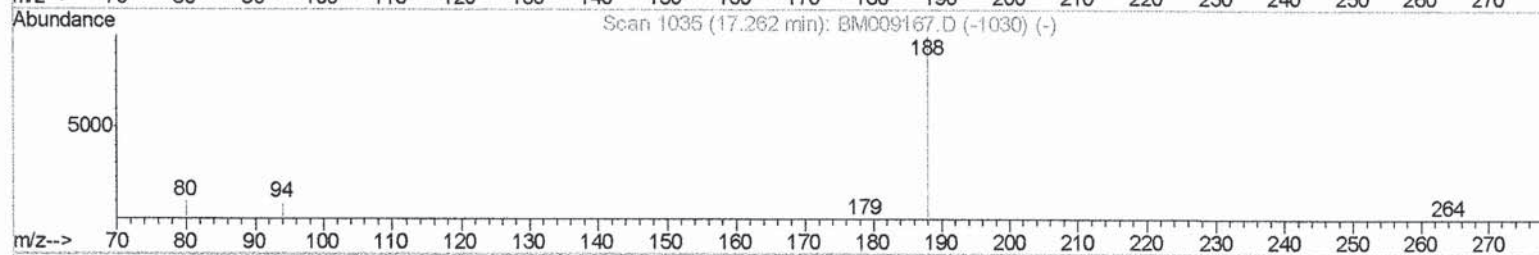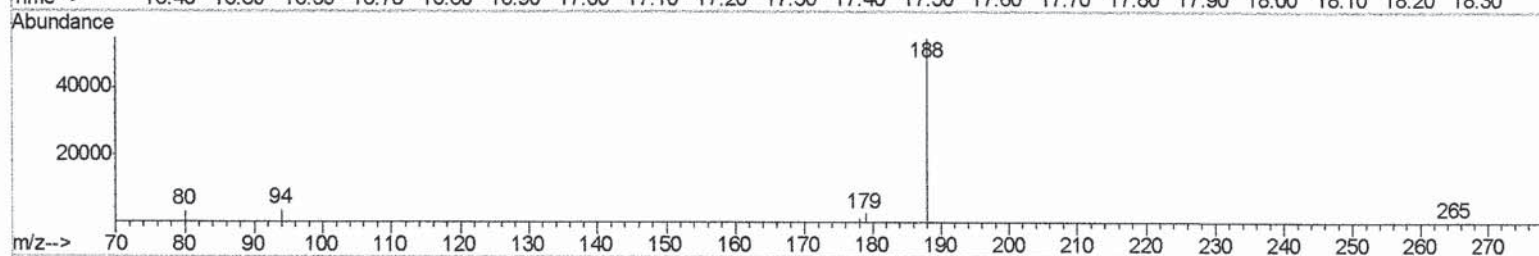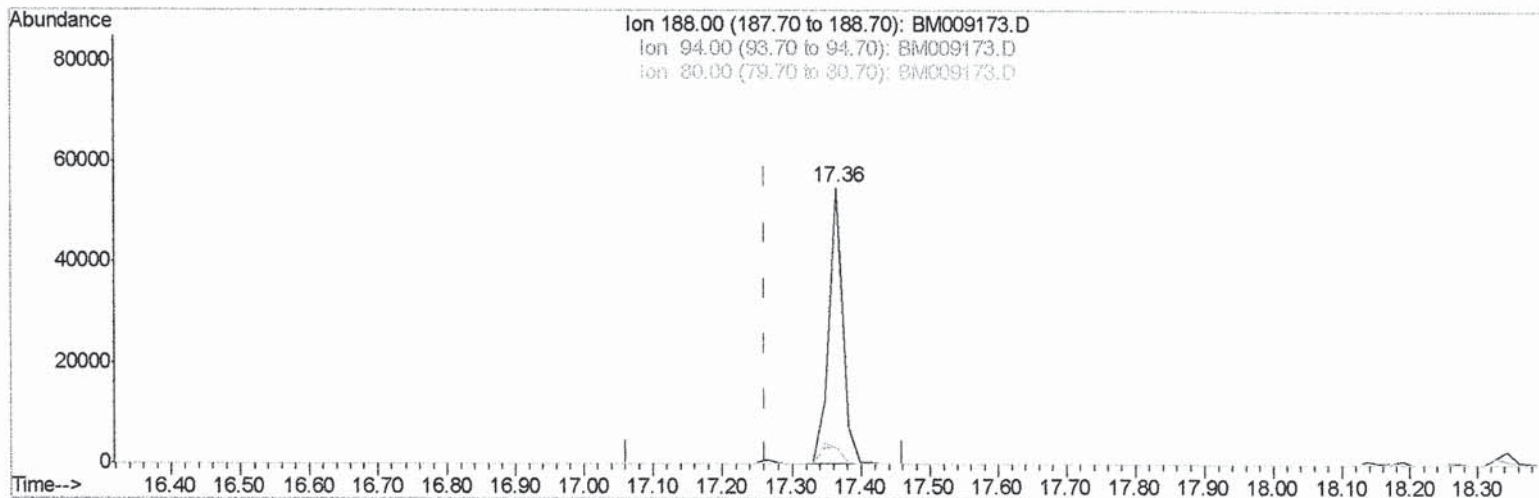

TIC: BM009173.D

(10) Phenanthrene-d10 (I)

17.365min (+0.103) 0.40ng/ul

response 76927

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	6.25#
80.00	11.80	5.92#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_M\Data\BM031017\
Data File : BM009173.D
Acq On : 10 Mar 2017 13:23
Operator : SJ/MA
Sample : I2062-06
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AC7

Manual Integrations
APPROVED

mohammad
3/13/2017 2:13:25 PM

Quant Time: Mar 10 15:43:09 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 10 15:19:24 2017
Response via : Initial Calibration

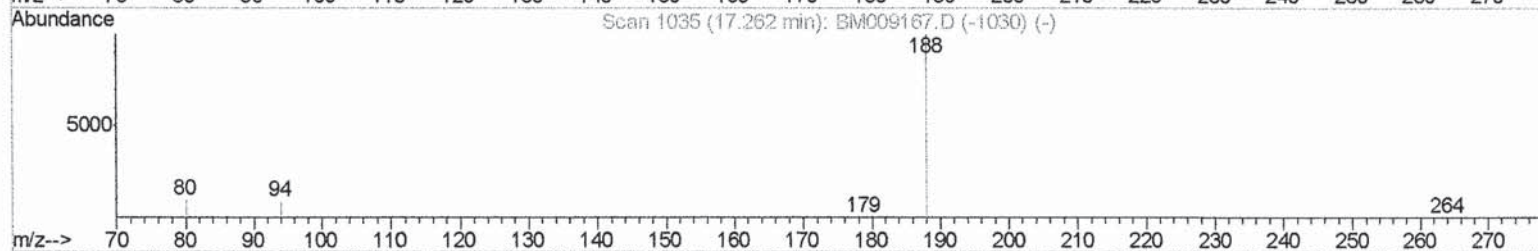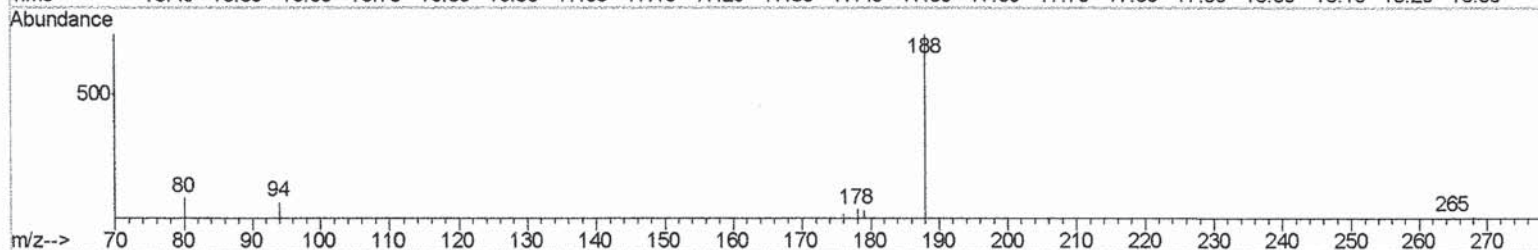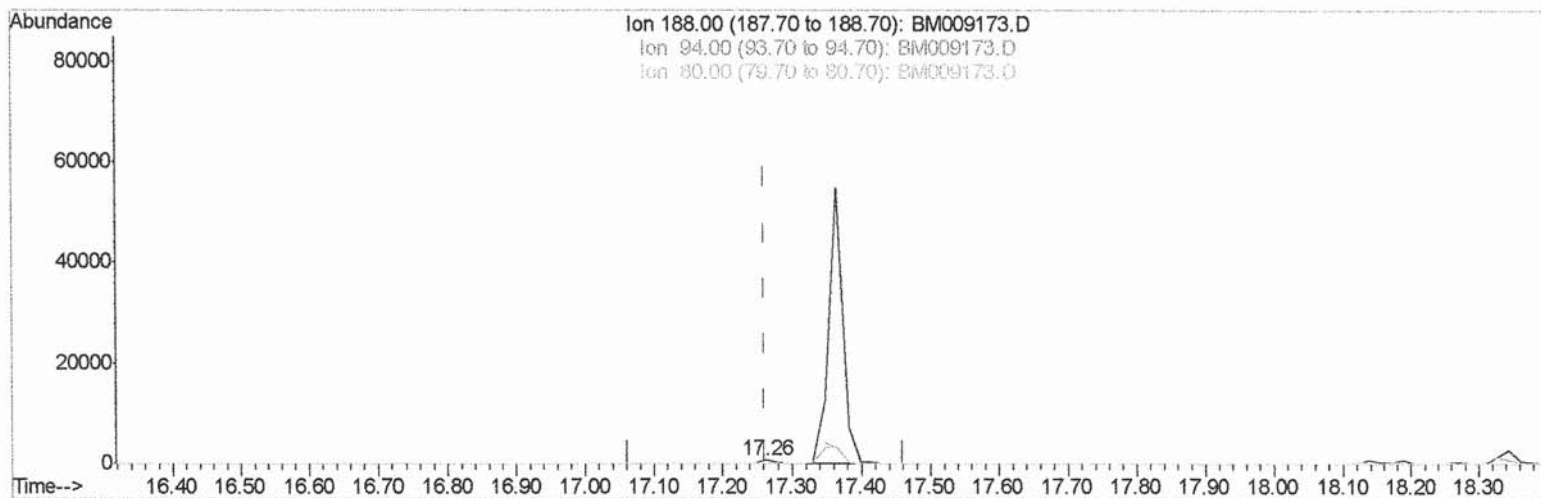

TIC: BM009173.D

(10) Phenanthrene-d10 (I)

17.262min (+0.000) 0.40ng/ul m

response 1062

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	14.48#
80.00	11.80	16.55#
0.00	0.00	0.00

SJ
03/13/17




Data Path : Z:\HPCHEM1\BNA_M\Data\BM031017\
Data File : BM009173.D
Acq On : 10 Mar 2017 13:23
Operator : SJ/MA
Sample : I2062-06
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AC7

Manual Integrations
APPROVED

mohammad
3/13/2017 2:13:25 PM

Quant Time: Mar 10 15:44:22 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 10 15:19:24 2017
Response via : Initial Calibration

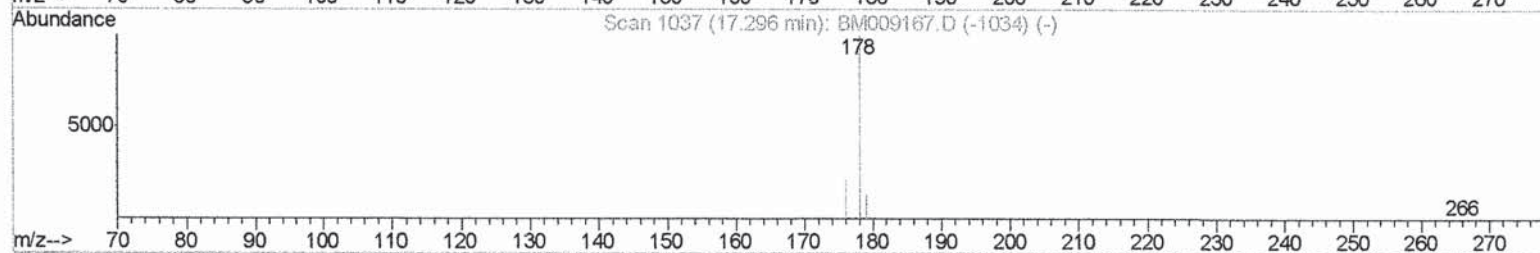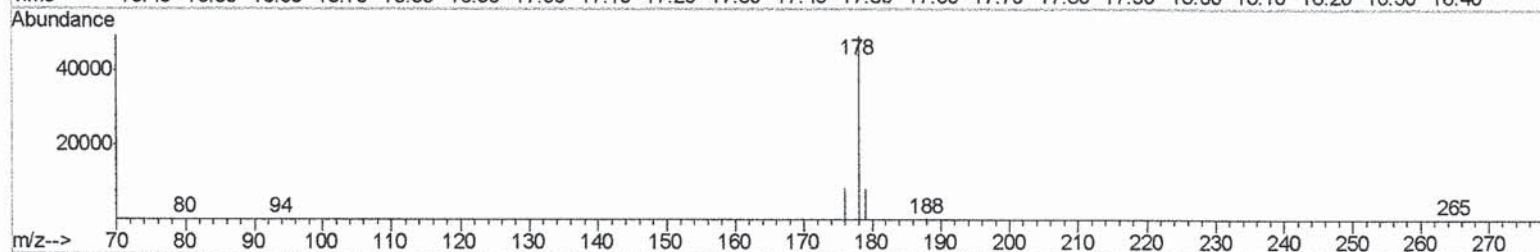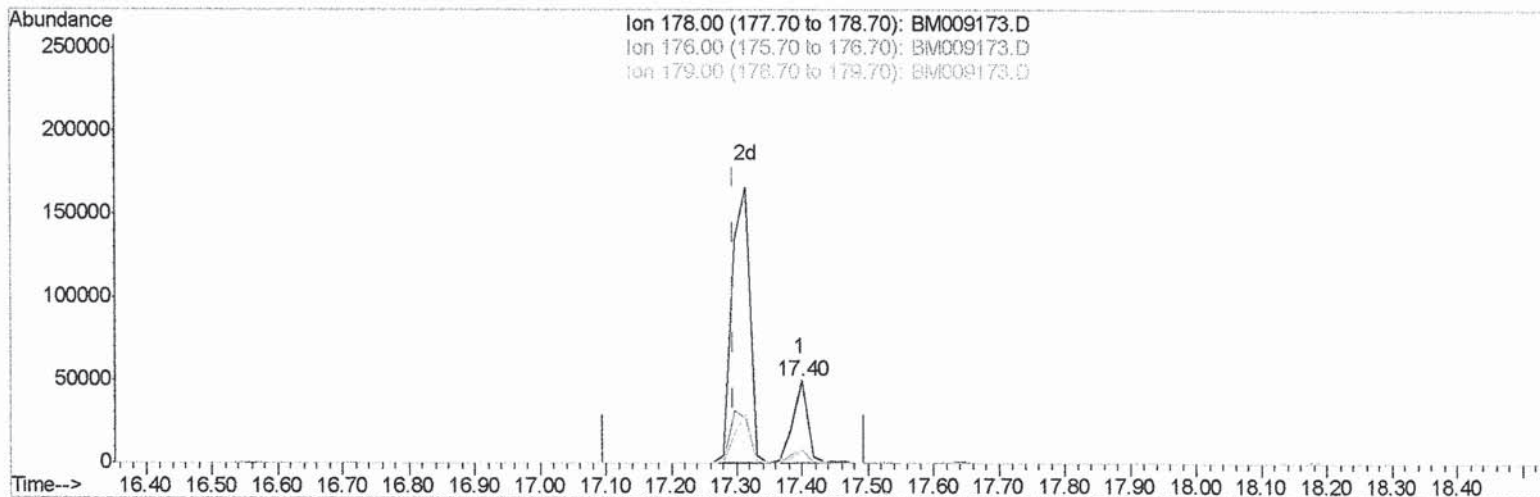

TIC: BM009173.D

(12) Phenanthrene

17.399min (+0.103) 23.51ng/ul

response 78386

Ion	Exp%	Act%
178.00	100	100
176.00	23.00	17.40#
179.00	17.00	16.45
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_M\Data\BM031017\
Data File : BM009173.D
Acq On : 10 Mar 2017 13:23
Operator : SJ/MA
Sample : I2062-06
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AC7

Manual Integrations
APPROVED

mohammad
3/13/2017 2:13:25 PM

Quant Time: Mar 10 15:44:22 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 10 15:19:24 2017
Response via : Initial Calibration

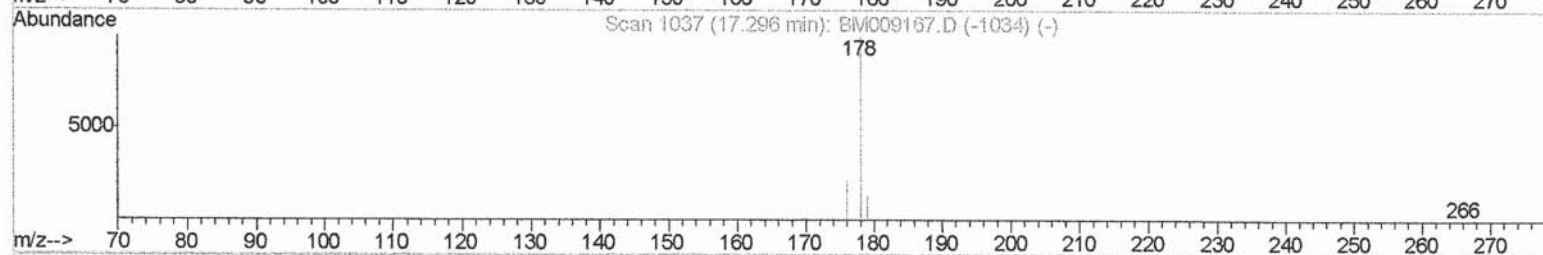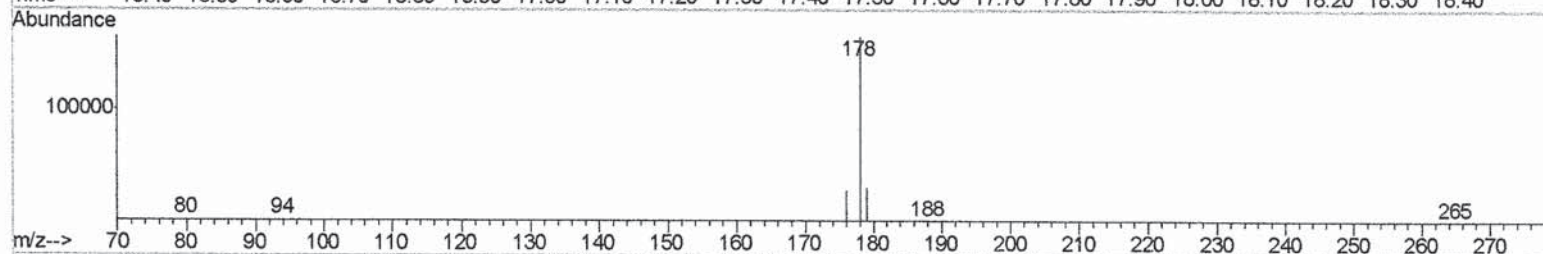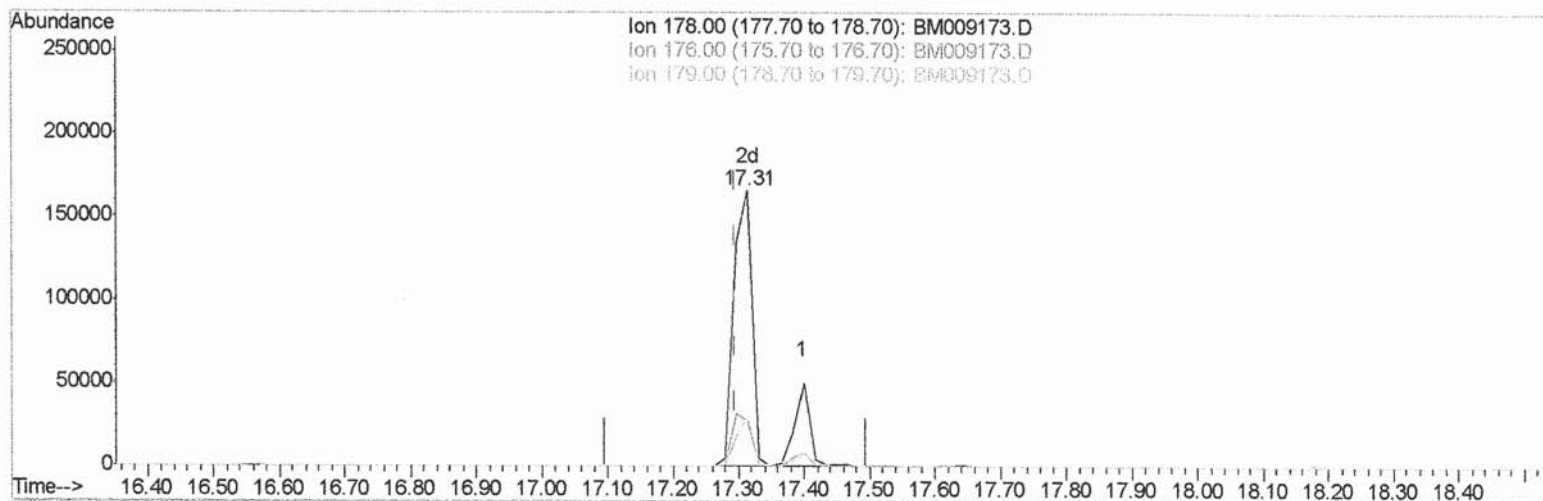

TIC: BM009173.D

(12) Phenanthrene

17.313min (+0.017) 95.95ng/ul m

response 319973

Ion	Exp%	Act%
178.00	100	100
176.00	23.00	16.15#
179.00	17.00	17.63
0.00	0.00	0.00

SJ
03/13/17




Data Path : Z:\HPCHEM1\BNA_M\Data\BM031017\
Data File : BM009173.D
Acq On : 10 Mar 2017 13:23
Operator : SJ/MA
Sample : I2062-06
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AC7

Manual Integrations
APPROVED

mohammad
3/13/2017 2:13:25 PM

Quant Time: Mar 10 15:44:22 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 10 15:19:24 2017
Response via : Initial Calibration

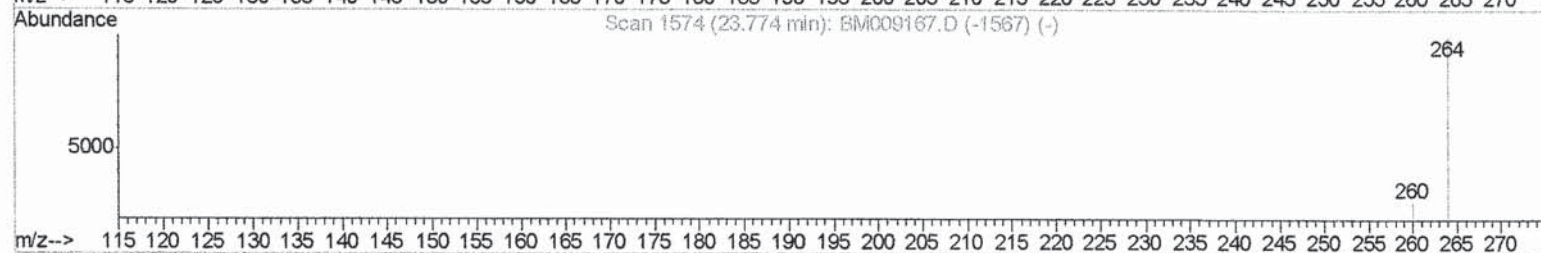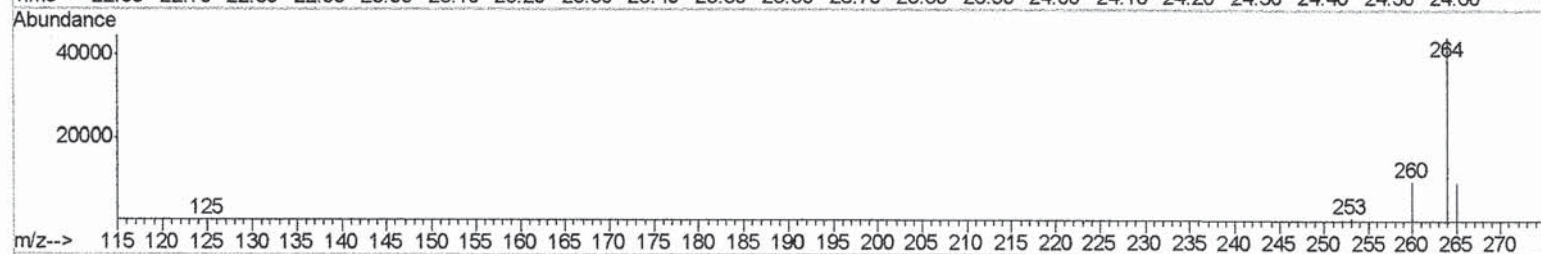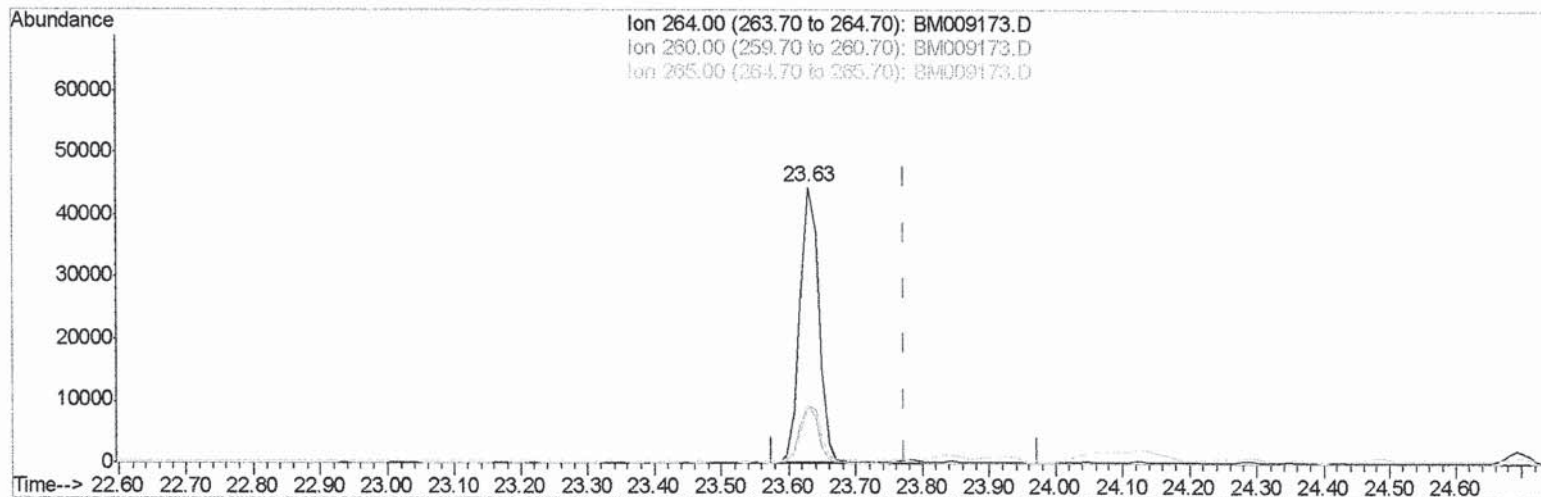

TIC: BM009173.D

(20) Perylene-d12 (I)
23.629min (-0.146) 0.40ng/ul
response 84674

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	21.33#
265.00	103.50	20.97#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_M\Data\BM031017\
Data File : BM009173.D
Acq On : 10 Mar 2017 13:23
Operator : SJ/MA
Sample : I2062-06
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AC7

Manual Integrations
APPROVED

mohammad
3/13/2017 2:13:25 PM

Quant Time: Mar 10 15:44:22 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 10 15:19:24 2017
Response via : Initial Calibration

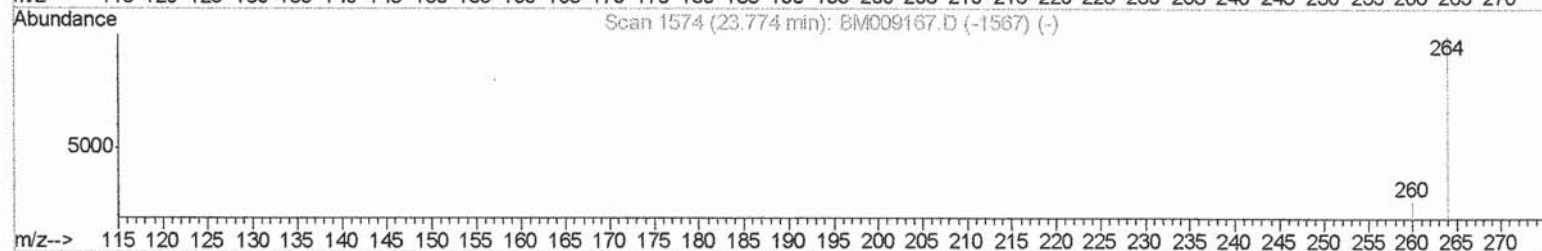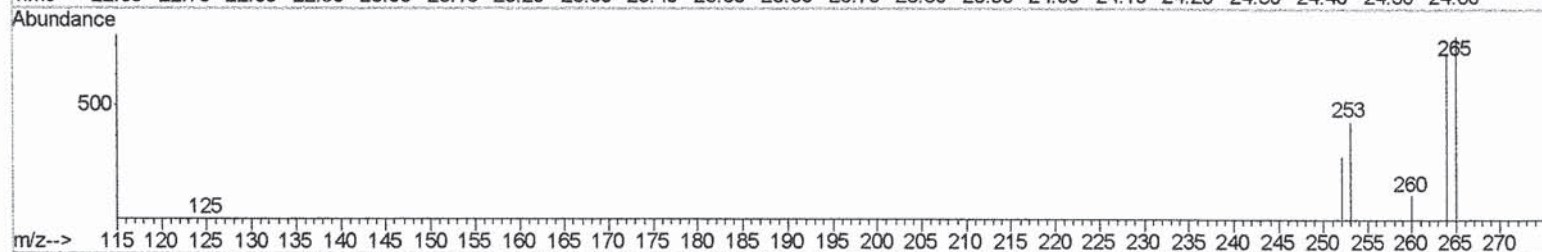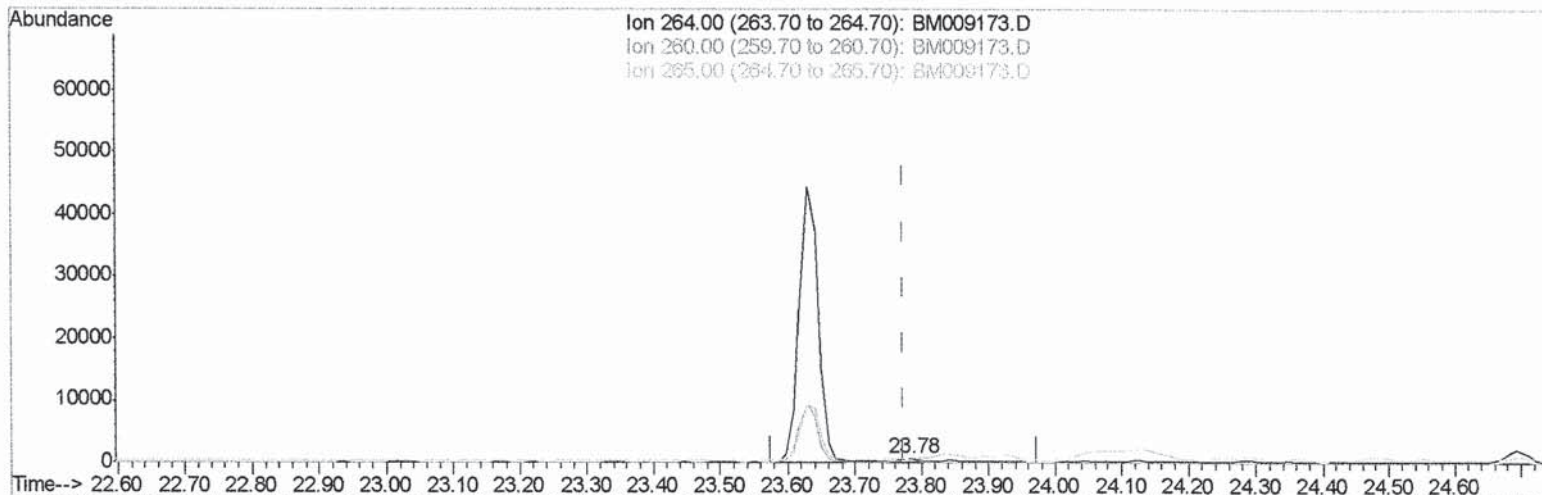

TIC: BM009173.D

(20) Perylene-d12 (I)

23.785min (+0.011) 0.40ng/ul m

response 1085

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	30.70
265.00	103.50	109.09
0.00	0.00	0.00

SJ
03/13/17




Data Path : Z:\HPCHEM1\BNA_M\Data\BM031017\
Data File : BM009173.D
Acq On : 10 Mar 2017 13:23
Operator : SJ/MA
Sample : I2062-06
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AC7

Manual Integrations
APPROVED

mohammad
3/13/2017 2:13:25 PM

Quant Time: Mar 10 15:45:35 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 10 15:19:24 2017
Response via : Initial Calibration

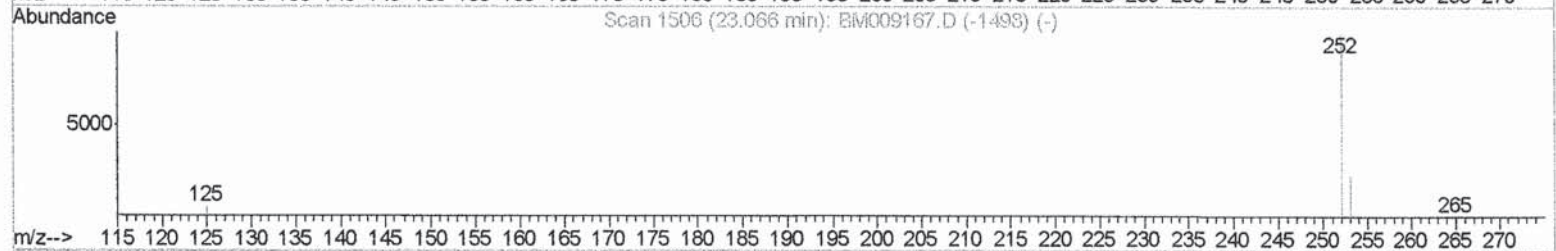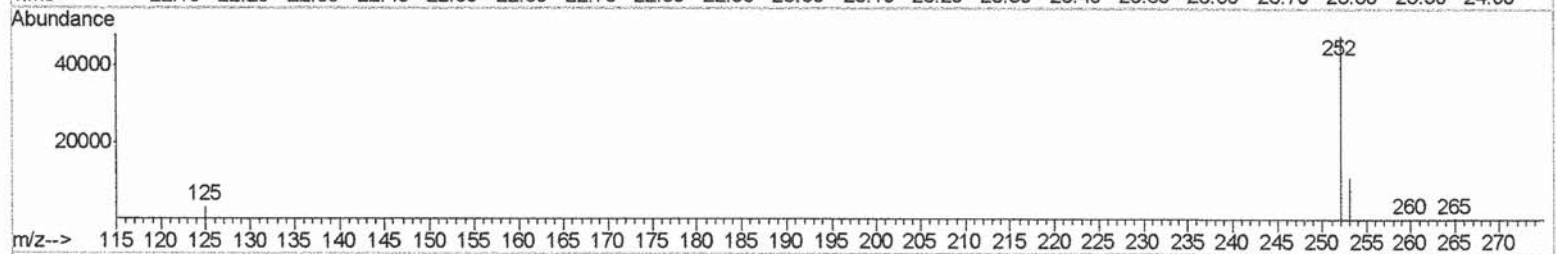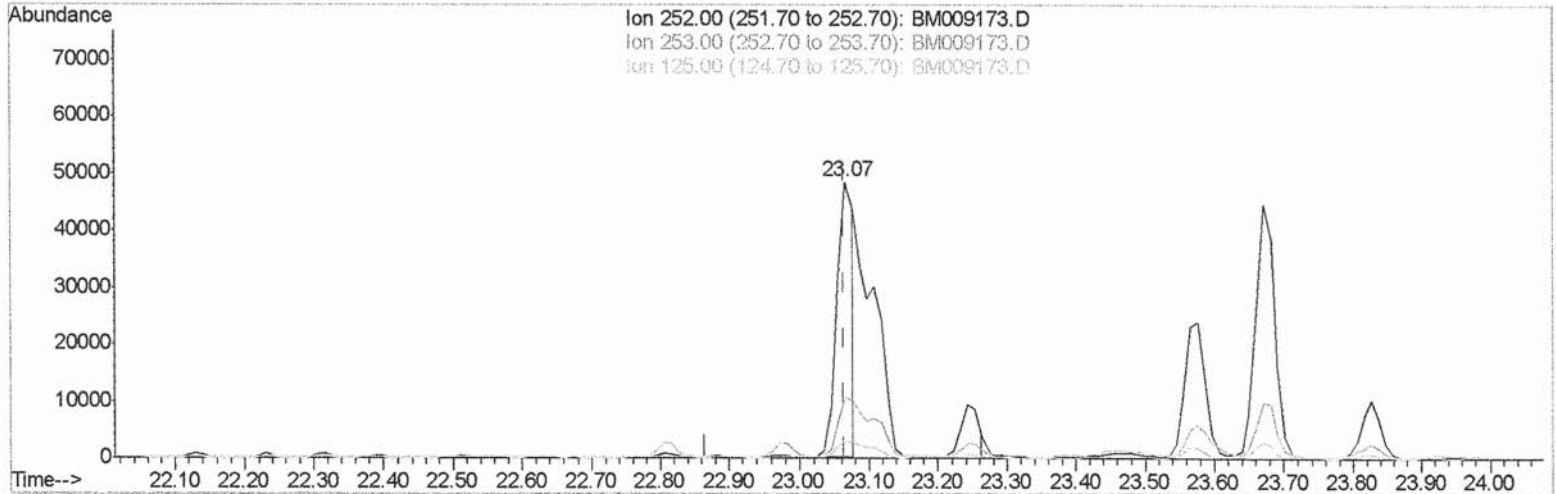

TIC: BM009173.D

(21) Benzo(b)fluoranthene

23.066min (+0.000) 19.49ng/ul

response 83088

Ion	Exp%	Act%
252.00	100	100
253.00	32.10	22.46
125.00	17.50	6.44
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM031017\
 Data File : BM009173.D
 Acq On : 10 Mar 2017 13:23
 Operator : SJ/MA
 Sample : I2062-06
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AC7

Manual Integrations
 APPROVED

mohammad
 3/13/2017 2:13:25 PM

Quant Time: Mar 10 15:45:35 2017
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030317.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Mar 10 15:19:24 2017
 Response via : Initial Calibration

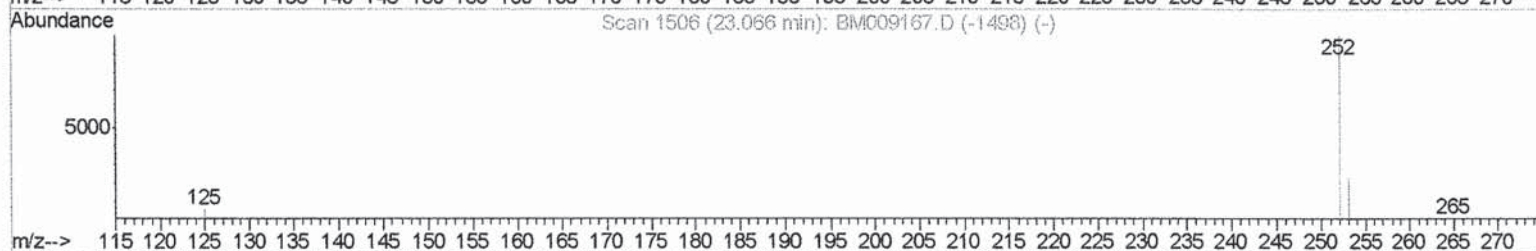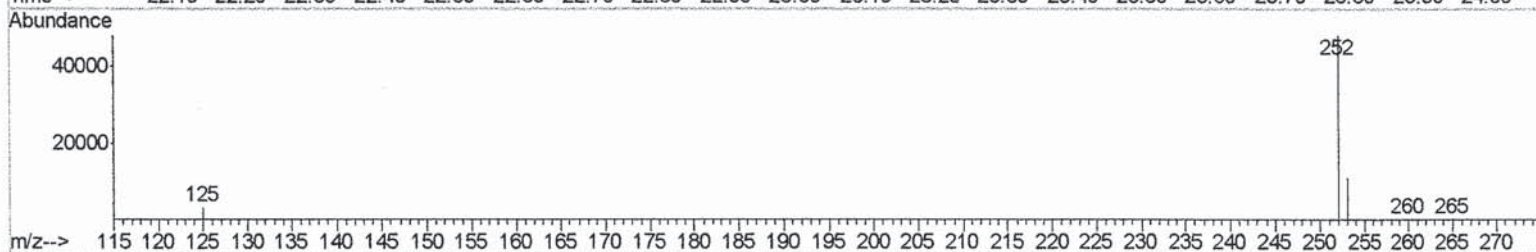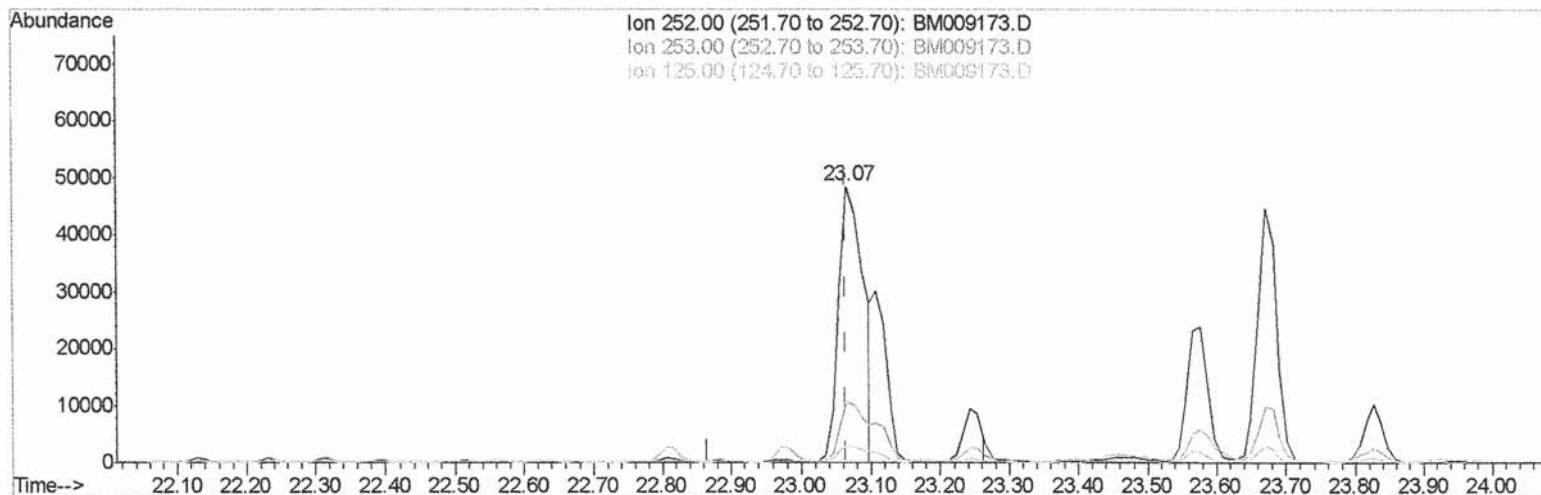

TIC: BM009173.D

(21) Benzo(b)fluoranthene

23.066min (+0.000) 28.68ng/ul m

response 122239

Ion	Exp%	Act%
252.00	100	100
253.00	32.10	22.46
125.00	17.50	6.44
0.00	0.00	0.00

> SJ
 03/13/17




Data Path : Z:\HPCHEM1\BNA_M\Data\BM031017\
Data File : BM009173.D
Acq On : 10 Mar 2017 13:23
Operator : SJ/MA
Sample : I2062-06
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AC7

Manual Integrations
APPROVED

mohammad
3/13/2017 2:13:25 PM

Quant Time: Mar 10 15:45:35 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 10 15:19:24 2017
Response via : Initial Calibration

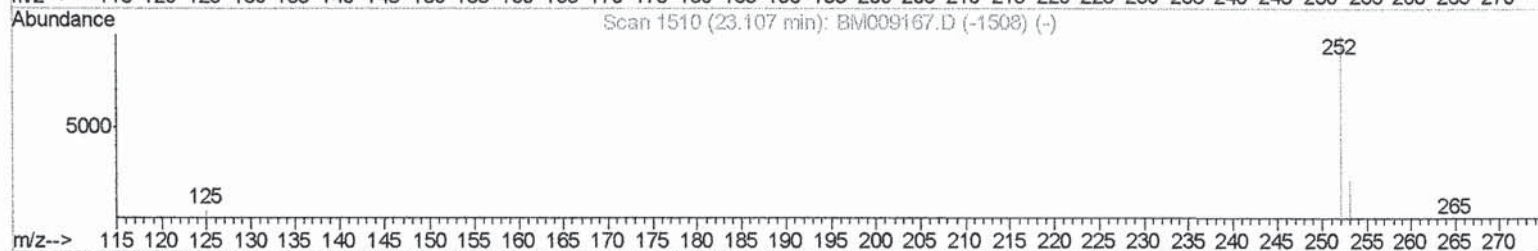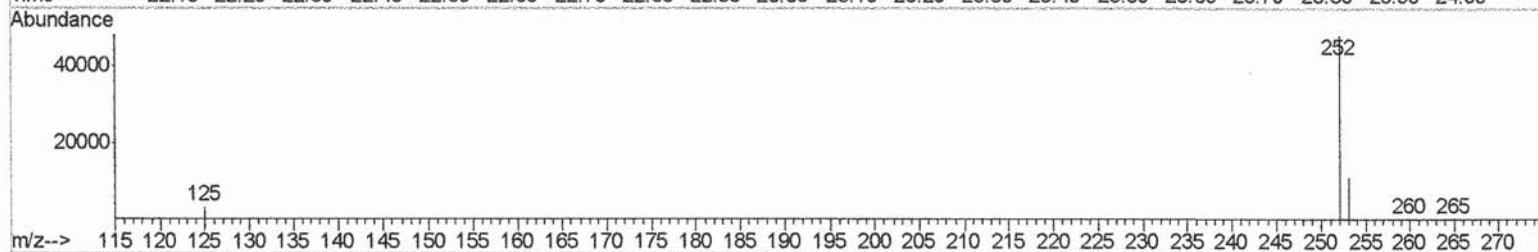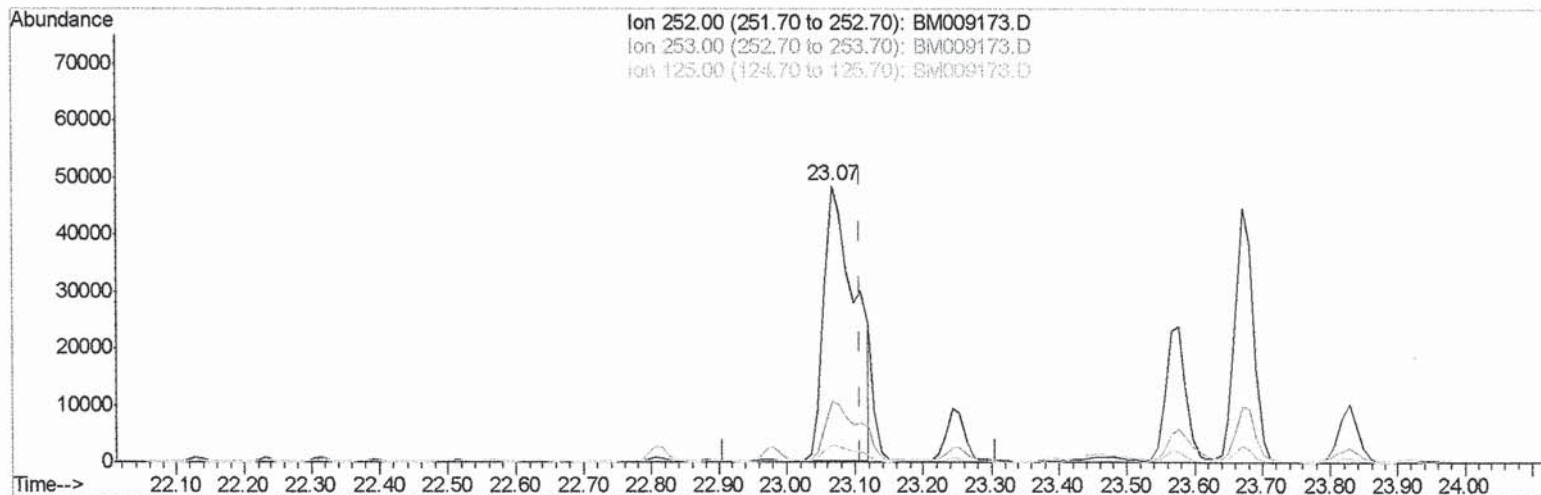

TIC: BM009173.D

(22) Benzo(k)fluoranthene

23.066min (-0.042) 41.13ng/ul

response 155005

Ion	Exp%	Act%
252.00	100	100
253.00	30.60	22.46#
125.00	17.10	6.44#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_M\Data\BM031017\
Data File : BM009173.D
Acq On : 10 Mar 2017 13:23
Operator : SJ/MA
Sample : I2062-06
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AC7

Manual Integrations
APPROVED

mohammad
3/13/2017 2:13:25 PM

Quant Time: Mar 10 15:45:35 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 10 15:19:24 2017
Response via : Initial Calibration

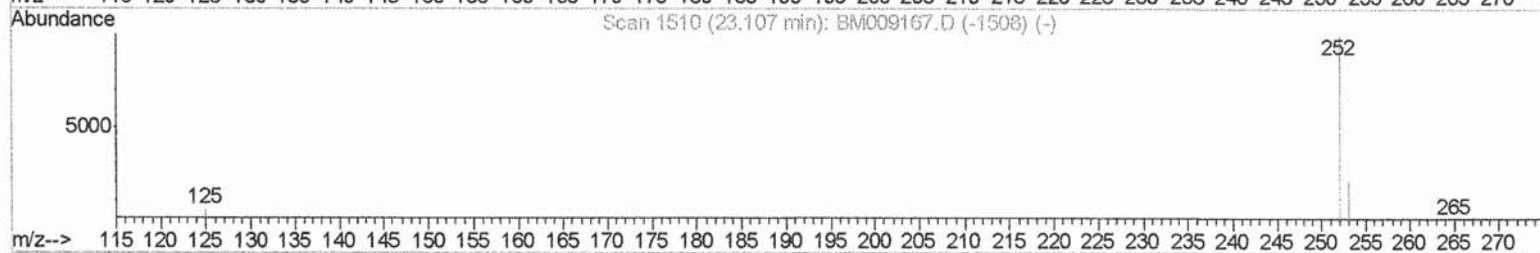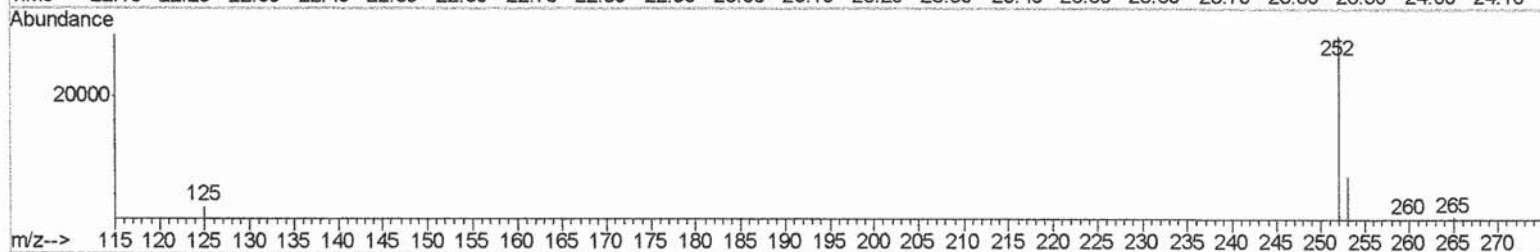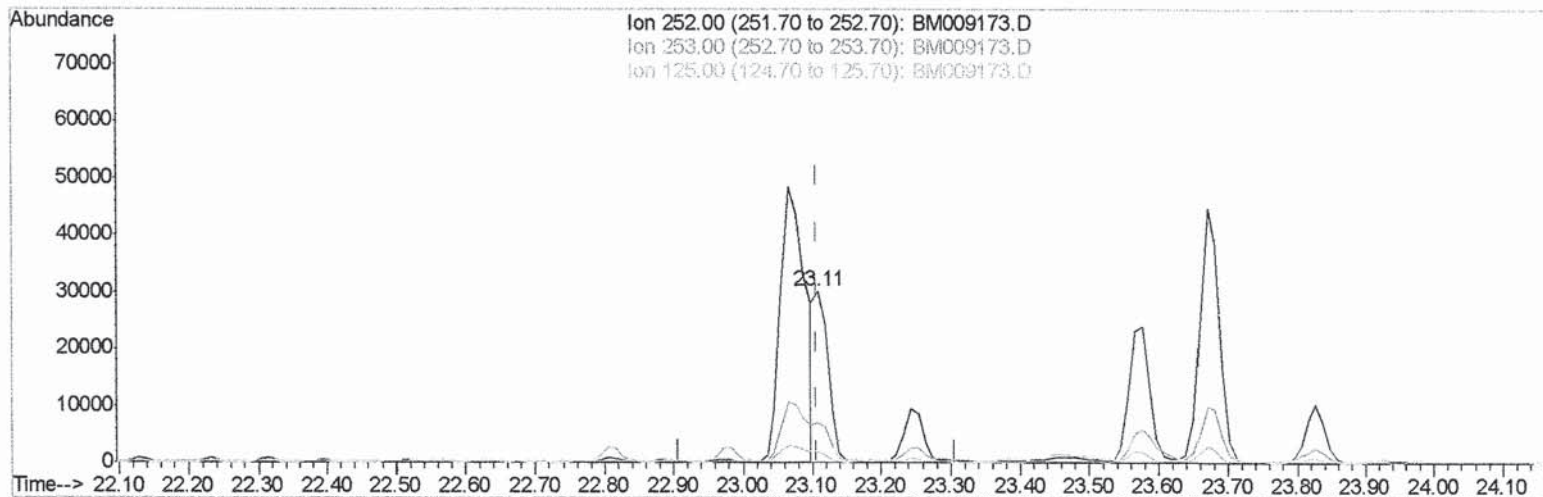

TIC: BM009173.D

(22) Benzo(k)fluoranthene

23.107min (+0.000) 10.97ng/ul m

response 41330

Ion	Exp%	Act%
252.00	100	100
253.00	30.60	23.59#
125.00	17.10	6.49#
0.00	0.00	0.00

> $\frac{5.5}{0.313117}$




Data Path : Z:\HPCHEM1\BNA_M\Data\BM031017\
Data File : BM009173.D
Acq On : 10 Mar 2017 13:23
Operator : SJ/MA
Sample : I2062-06
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AC7

Manual Integrations
APPROVED

mohammad
3/13/2017 2:13:25 PM

Quant Time: Mar 10 15:45:35 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 10 15:19:24 2017
Response via : Initial Calibration

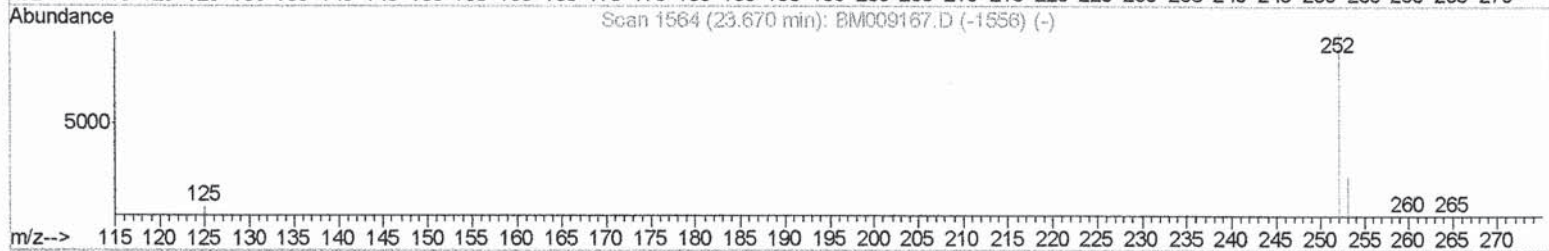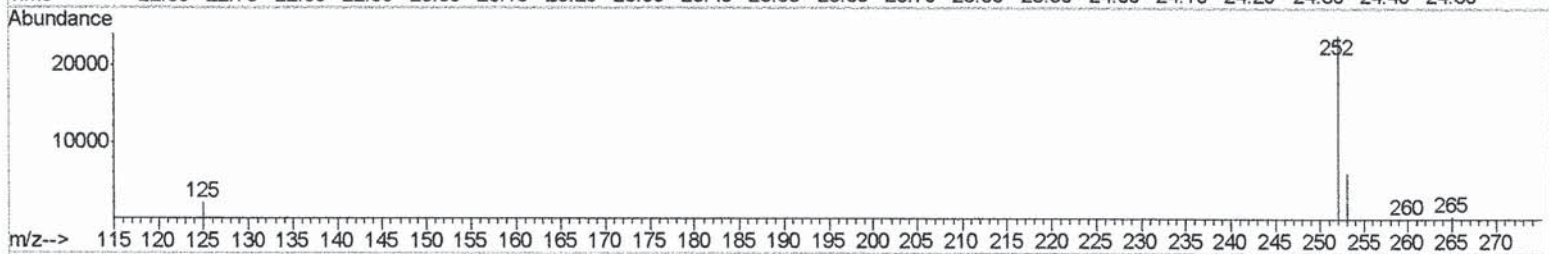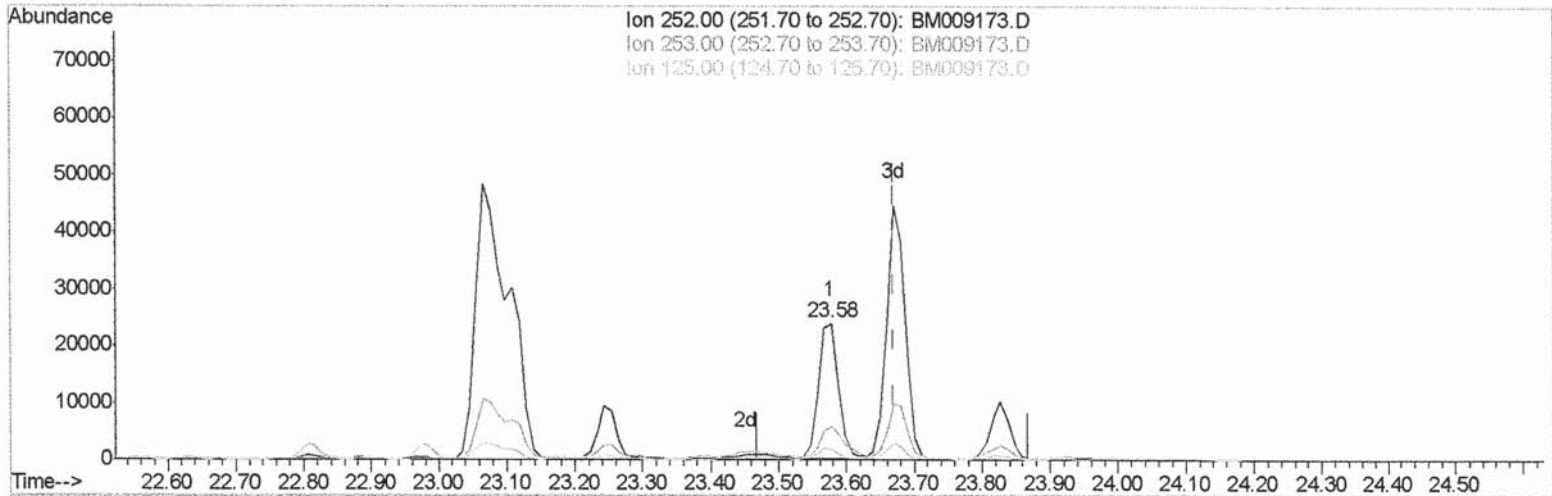

TIC: BM009173.D

(23) Benzo(a)pyrene (C)

23.576min (-0.094) 12.73ng/ul

response 48804

Ion	Exp%	Act%
252.00	100	100
253.00	35.60	24.95#
125.00	22.60	8.44#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_M\Data\BM031017\
Data File : BM009173.D
Acq On : 10 Mar 2017 13:23
Operator : SJ/MA
Sample : I2062-06
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AC7

Manual Integrations
APPROVED

mohammad
3/13/2017 2:13:25 PM

Quant Time: Mar 10 15:45:35 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 10 15:19:24 2017
Response via : Initial Calibration

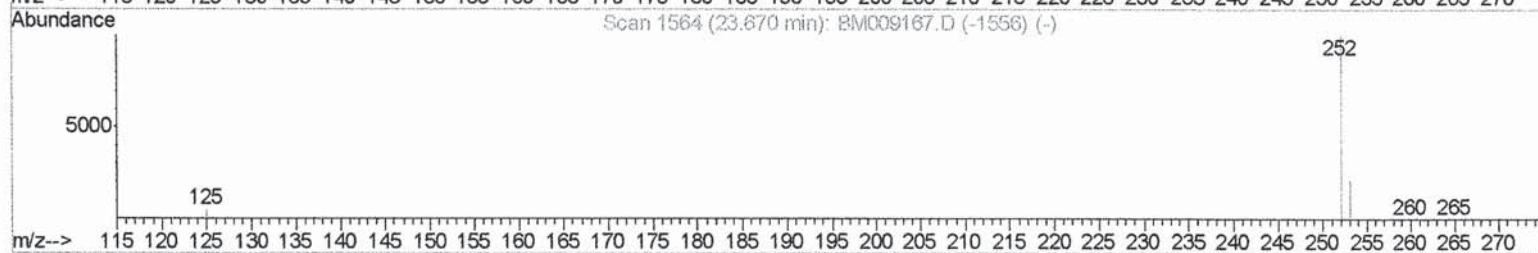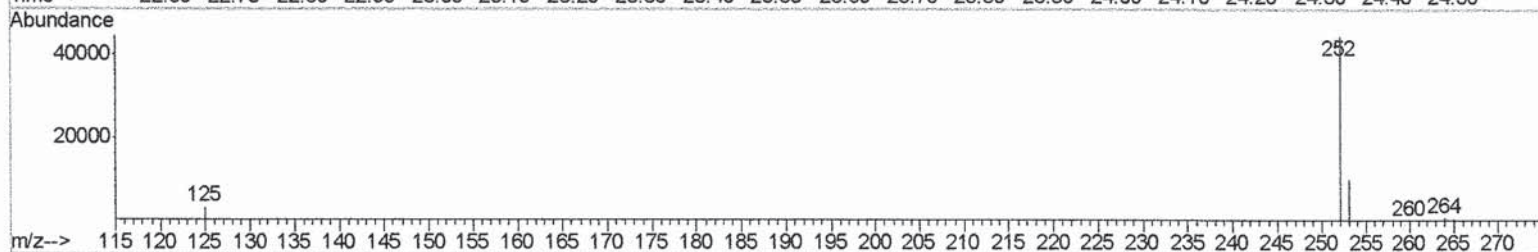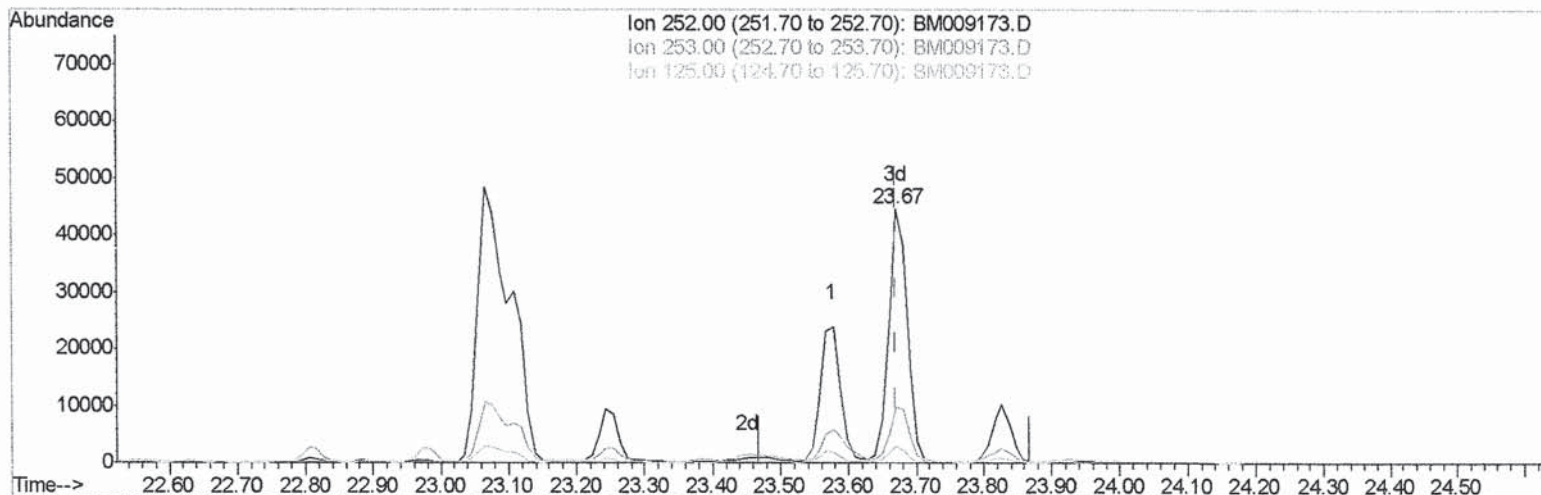

TIC: BM009173.D

(23) Benzo(a)pyrene (C)

23.670min (+0.000) 22.49ng/ul m

response 86259

Ion	Exp%	Act%
252.00	100	100
253.00	35.60	22.21#
125.00	22.60	6.82#
0.00	0.00	0.00

SJ
03/13/17

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM031017\
 Data File : BM009173.D
 Acq On : 10 Mar 2017 13:23
 Operator : SJ/MA
 Sample : I2062-06
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AC7

Manual Integrations
 APPROVED

mohammad
 3/13/2017 2:13:25 PM

Quant Time: Mar 10 15:45:35 2017
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030317.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Mar 10 15:19:24 2017
 Response via : Initial Calibration

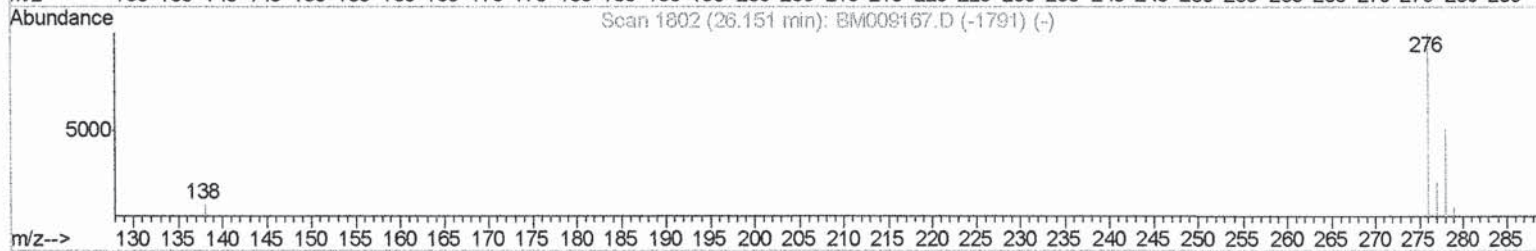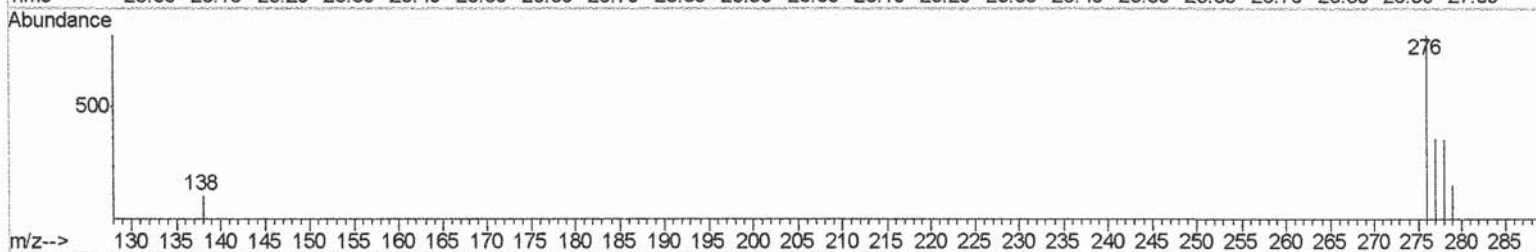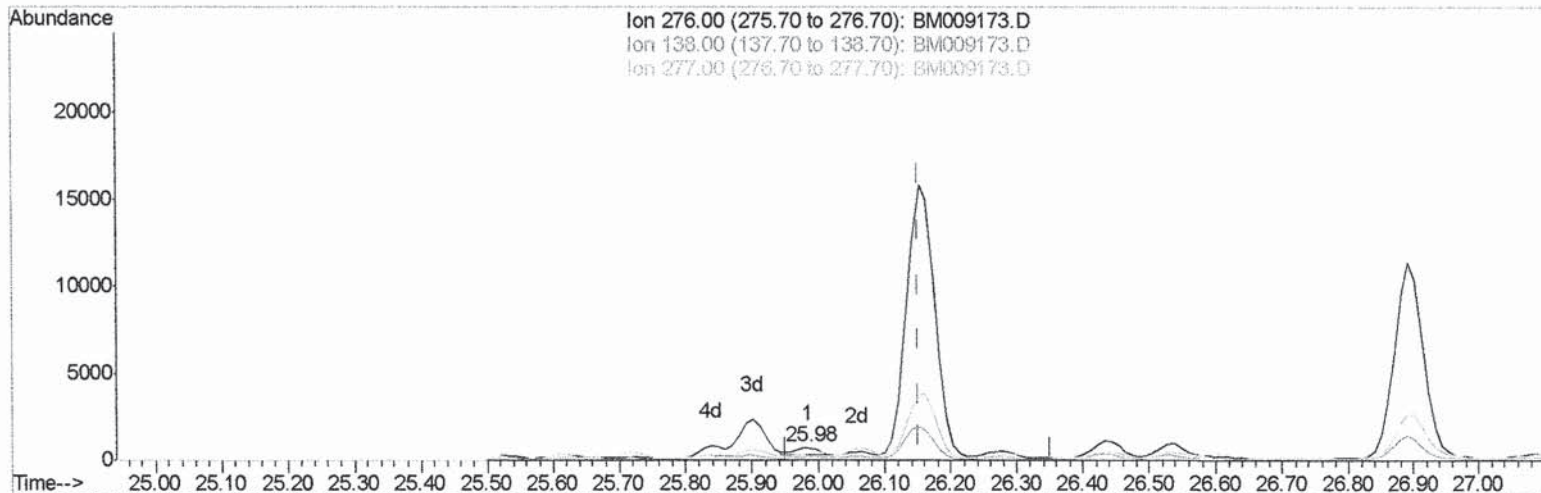

TIC: BM009173.D

(24) Indeno(1,2,3-cd)pyrene

25.984min (-0.167) 0.27ng/ul

response 1307

Ion	Exp%	Act%
276.00	100	100
138.00	23.90	19.36
277.00	24.50	52.18#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_M\Data\BM031017\
Data File : BM009173.D
Acq On : 10 Mar 2017 13:23
Operator : SJ/MA
Sample : I2062-06
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AC7

Manual Integrations
APPROVED

mohammad
3/13/2017 2:13:25 PM

Quant Time: Mar 10 15:45:35 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 10 15:19:24 2017
Response via : Initial Calibration

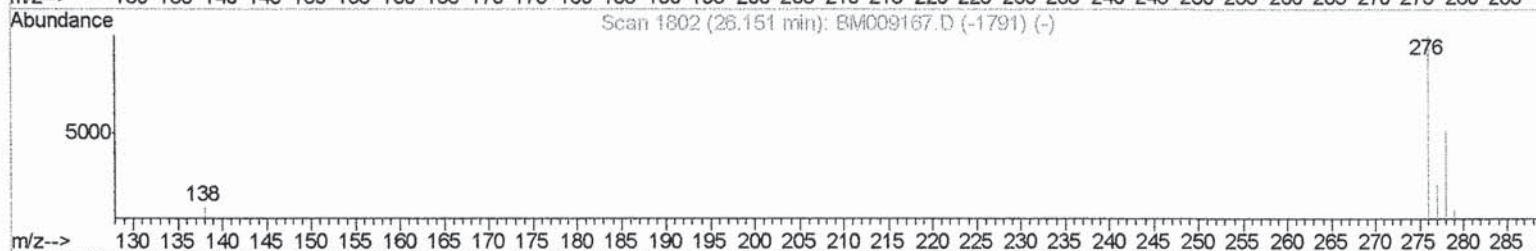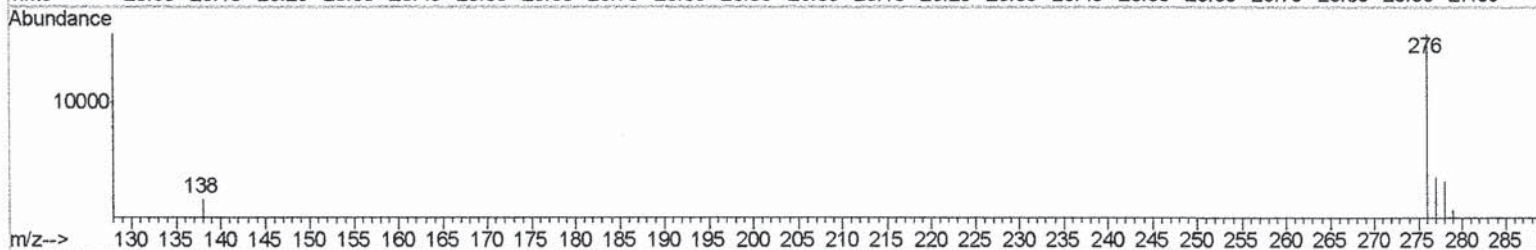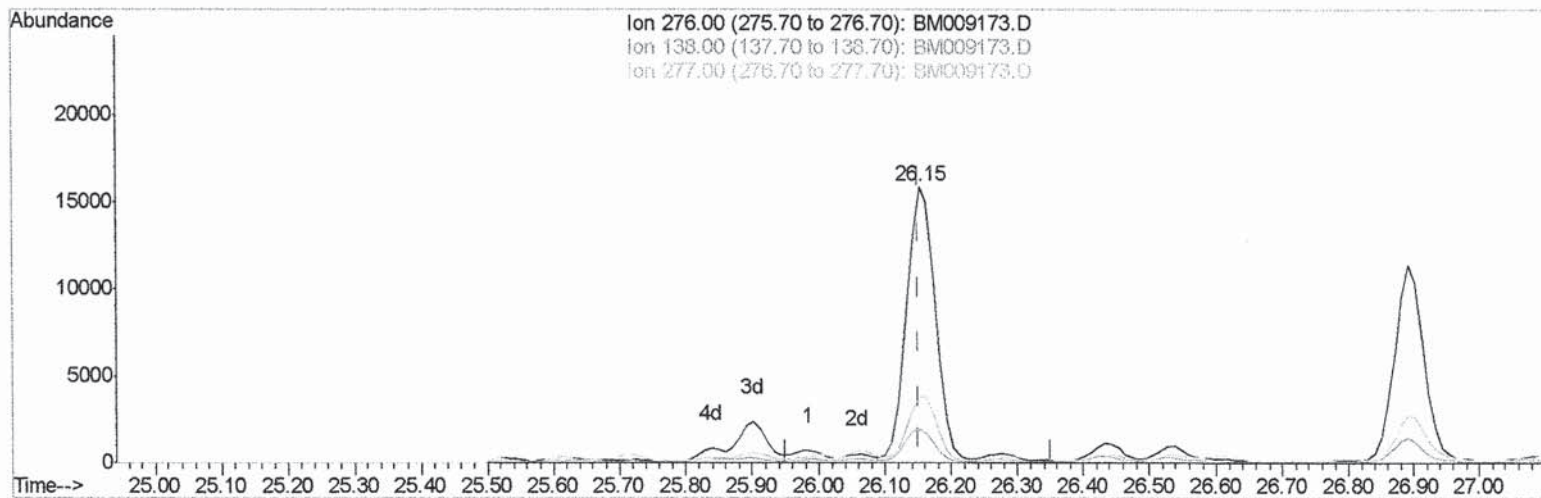

TIC: BM009173.D

(24) Indeno(1,2,3-cd)pyrene

26.151min (+0.000) 9.79ng/ul m

response 47739

Ion	Exp%	Act%
276.00	100	100
138.00	23.90	0.53#
277.00	24.50	1.43#
0.00	0.00	0.00

SJ
03/13/17




Data Path : Z:\HPCHEM1\BNA_M\Data\BM031017\
Data File : BM009173.D
Acq On : 10 Mar 2017 13:23
Operator : SJ/MA
Sample : I2062-06
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AC7

Manual Integrations
APPROVED

mohammad
3/13/2017 2:13:25 PM

Quant Time: Mar 10 15:45:35 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 10 15:19:24 2017
Response via : Initial Calibration

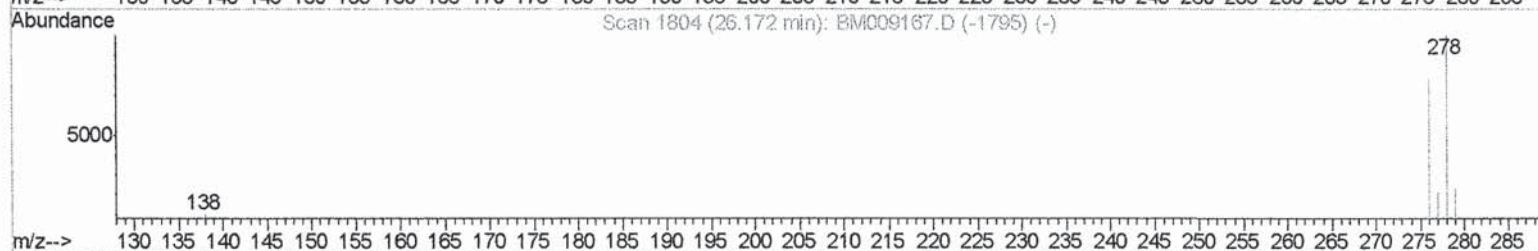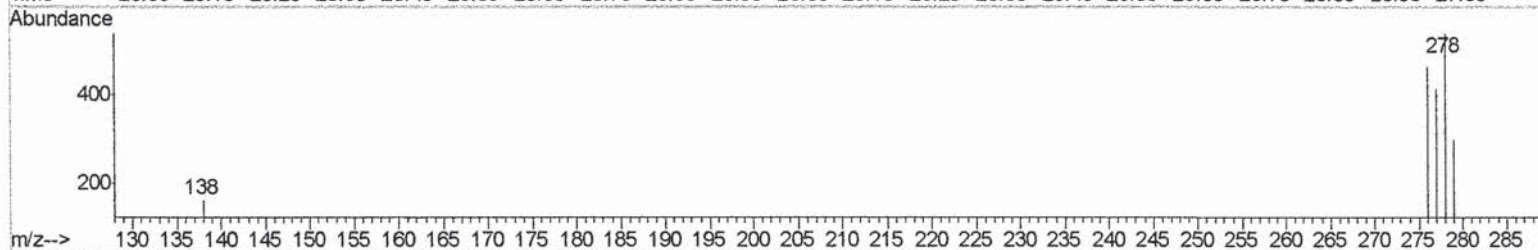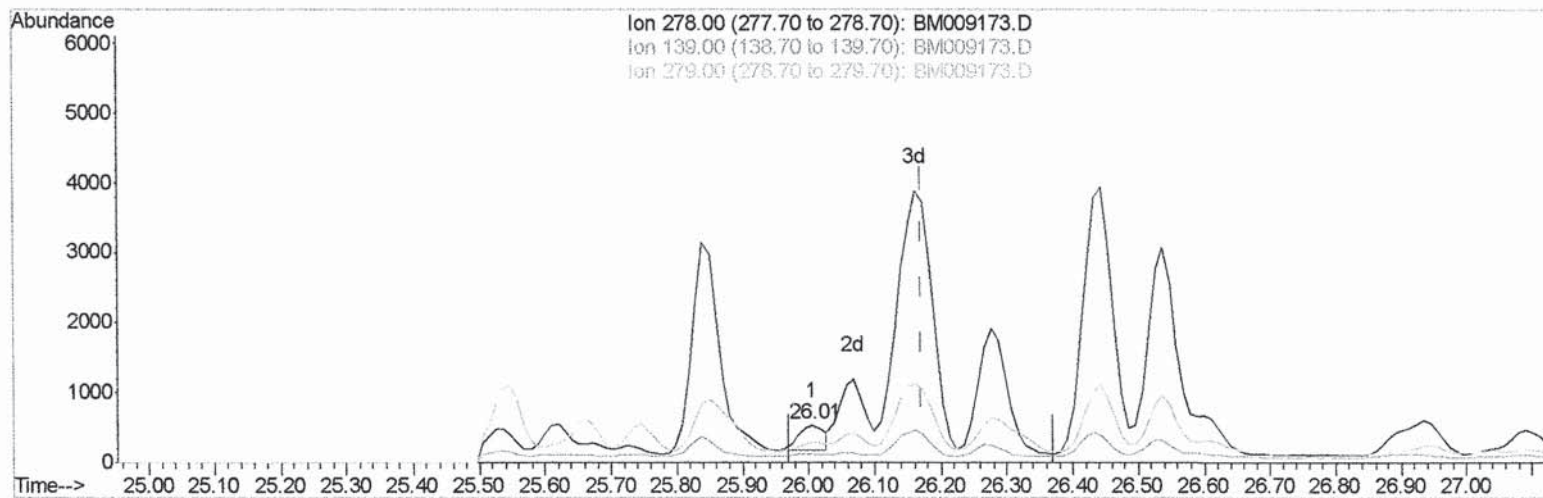

TIC: BM009173.D

(25) Dibenzo(a,h)anthracene

26.005min (-0.167) 0.23ng/ui

response 954

Ion	Exp%	Act%
278.00	100	100
139.00	21.70	22.74
279.00	32.40	55.82#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM031017\
 Data File : BM009173.D
 Acq On : 10 Mar 2017 13:23
 Operator : SJ/MA
 Sample : I2062-06
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AC7

Manual Integrations
 APPROVED

mohammad
 3/13/2017 2:13:25 PM

Quant Time: Mar 10 15:45:35 2017
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030317.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Mar 10 15:19:24 2017
 Response via : Initial Calibration

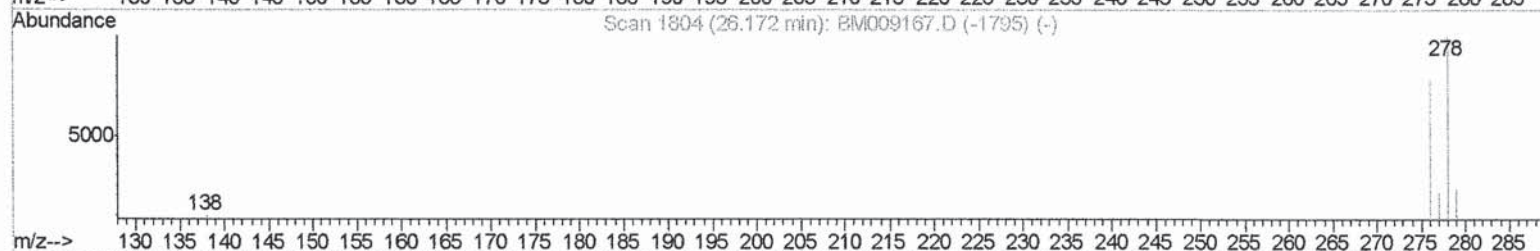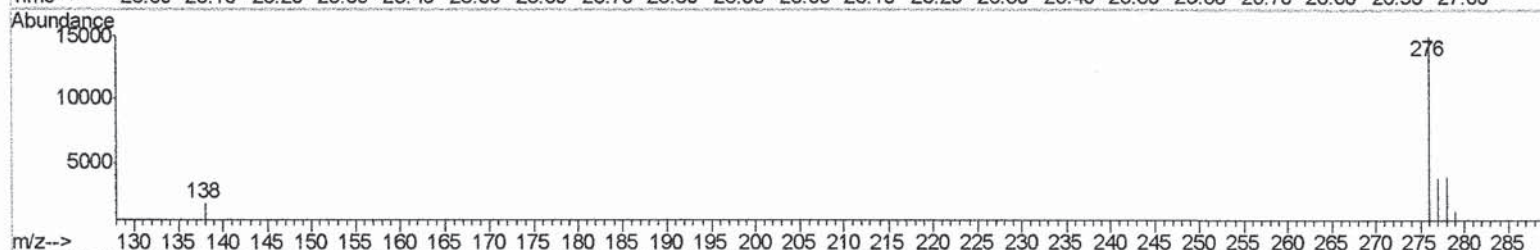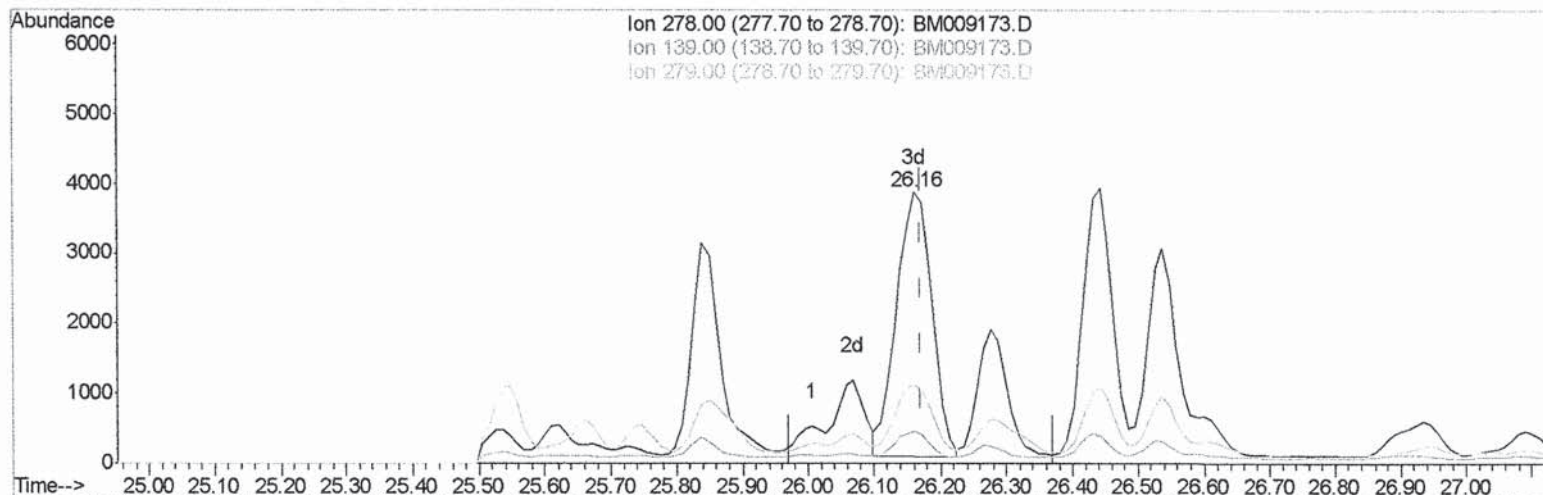

(25) Dibenzo(a,h)anthracene

26.162min (-0.010) 3.41ng/ul m

response 13979

Ion	Exp%	Act%
278.00	100	100
139.00	21.70	12.04#
279.00	32.40	29.08
0.00	0.00	0.00

> SJ
 03/13/17




Data Path : Z:\HPCHEM1\BNA_M\Data\BM031017\
Data File : BM009173.D
Acq On : 10 Mar 2017 13:23
Operator : SJ/MA
Sample : I2062-06
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AC7

Manual Integrations
APPROVED

mohammad
3/13/2017 2:13:25 PM

Quant Time: Mar 10 15:45:35 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 10 15:19:24 2017
Response via : Initial Calibration

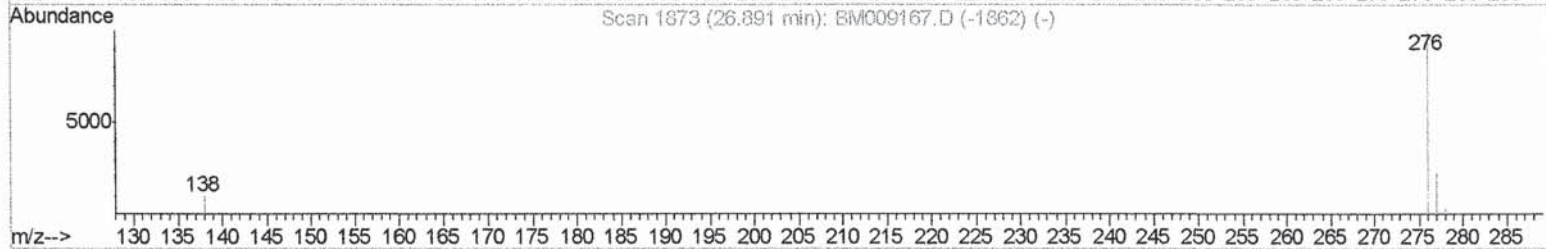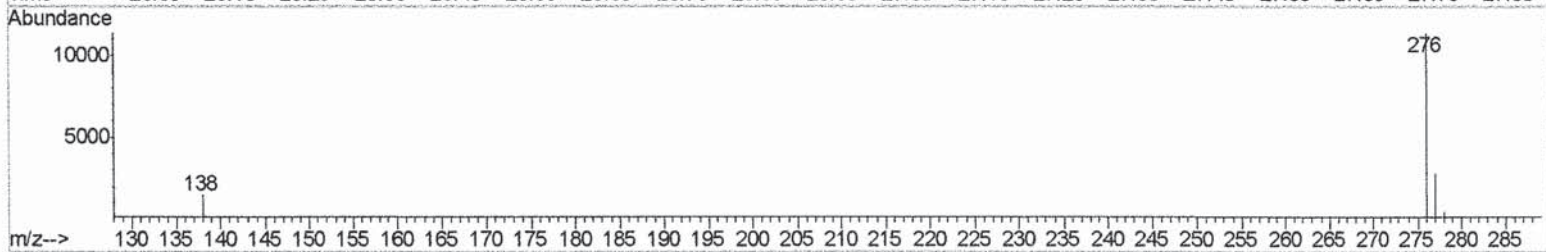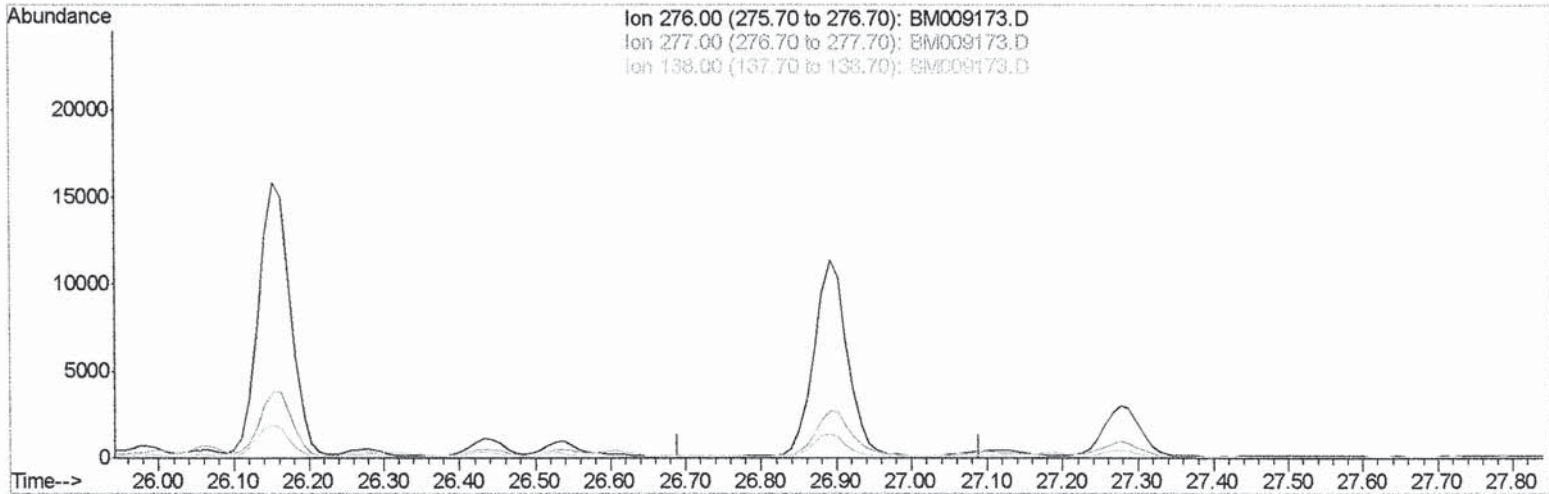

TIC: BM009173.D

(26) Benzo(g,h,i)perylene

26.891min (-26.891) 0.00ng/ul

response 0

Ion	Exp%	Act%
276.00	100	0.00
277.00	27.30	0.00#
138.00	25.60	0.00#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_M\Data\BM031017\
Data File : BM009173.D
Acq On : 10 Mar 2017 13:23
Operator : SJ/MA
Sample : I2062-06
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AC7

Manual Integrations
APPROVED

mohammad
3/13/2017 2:13:25 PM

Quant Time: Mar 10 15:45:35 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 10 15:19:24 2017
Response via : Initial Calibration

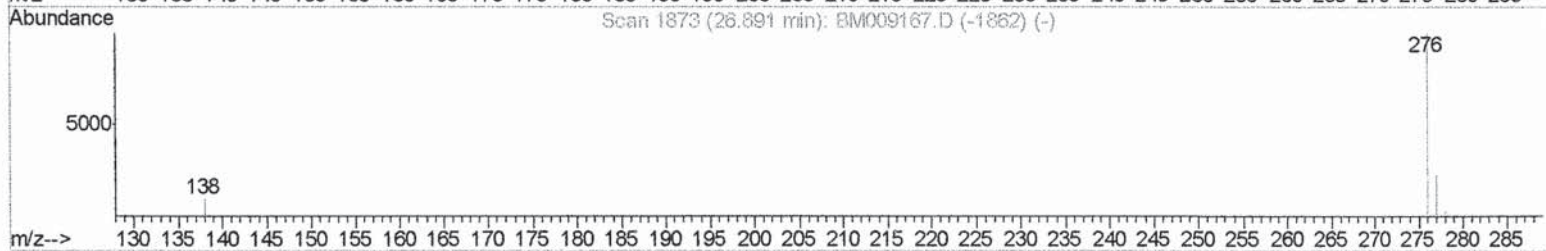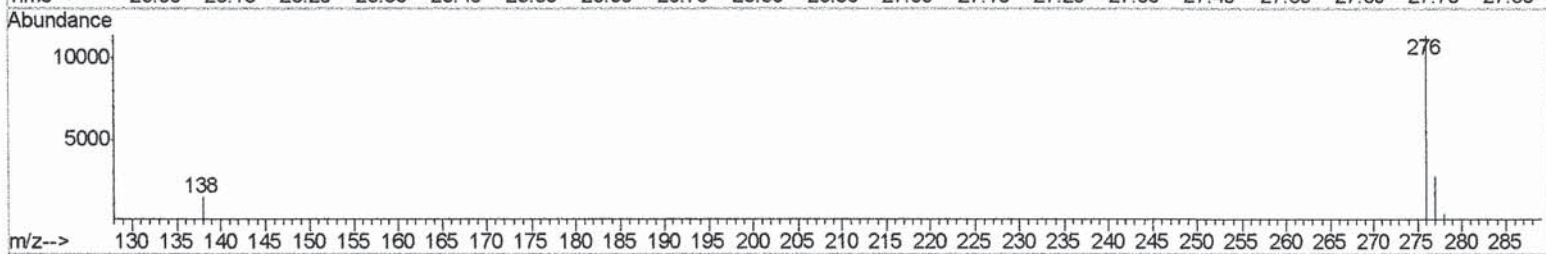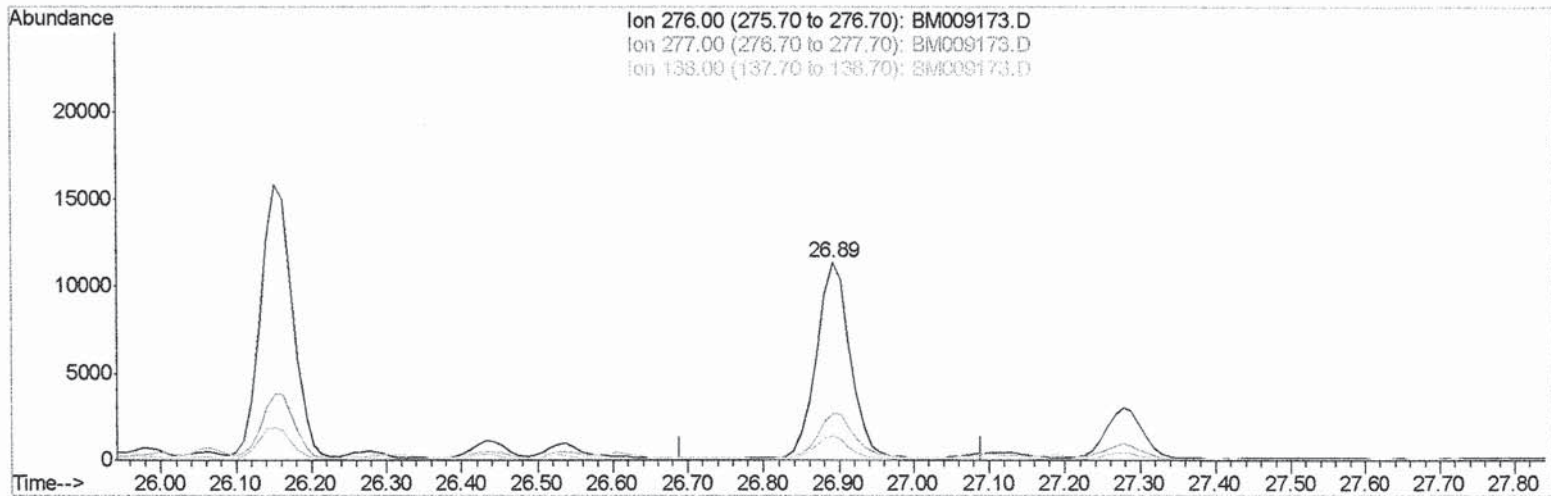

TIC: BM009173.D

(26) Benzo(g,h,i)perylene

26.891min (+0.000) 8.76ng/ul m

response 36446

Ion	Exp%	Act%
276.00	100	100
277.00	27.30	24.24
138.00	25.60	12.64#
0.00	0.00	0.00

> SJ
03/13/17




Data Path : Z:\HPCHEM1\BNA_M\Data\BM031017\
Data File : BM009173.D
Acq On : 10 Mar 2017 13:23
Operator : SJ/MA
Sample : I2062-06
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AC7

Manual Integrations
APPROVED

mohammad
3/13/2017 2:13:25 PM

Quant Time: Mar 10 15:48:01 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 10 15:19:24 2017
Response via : Initial Calibration

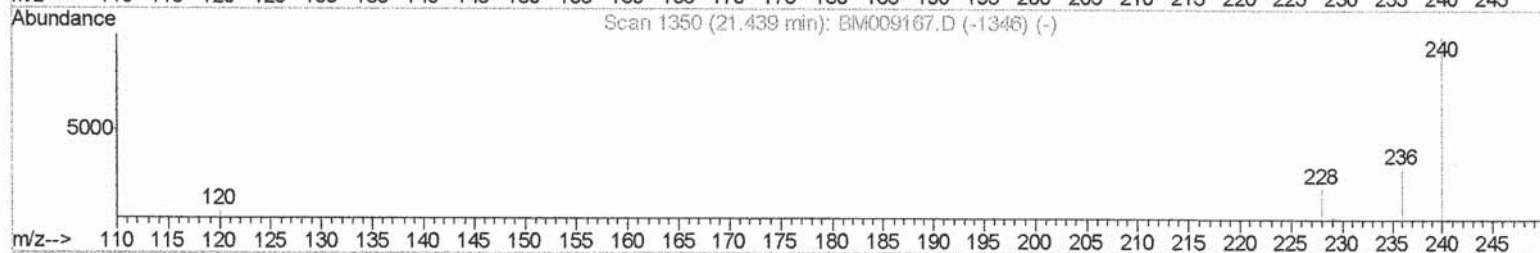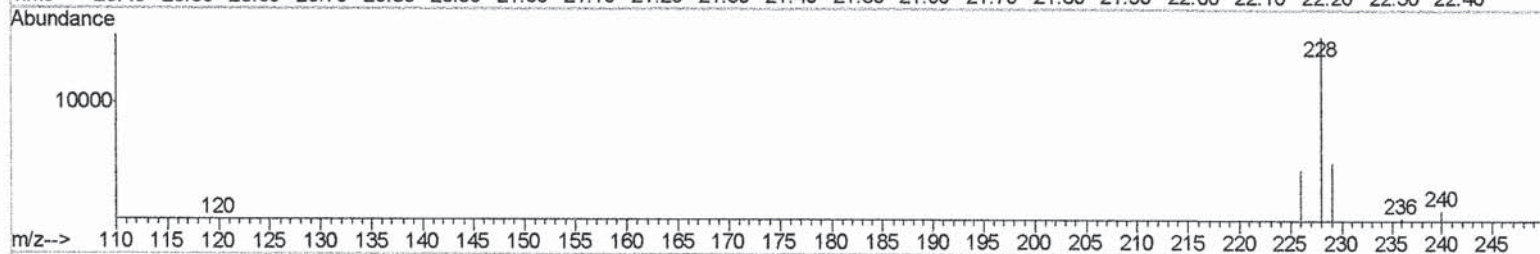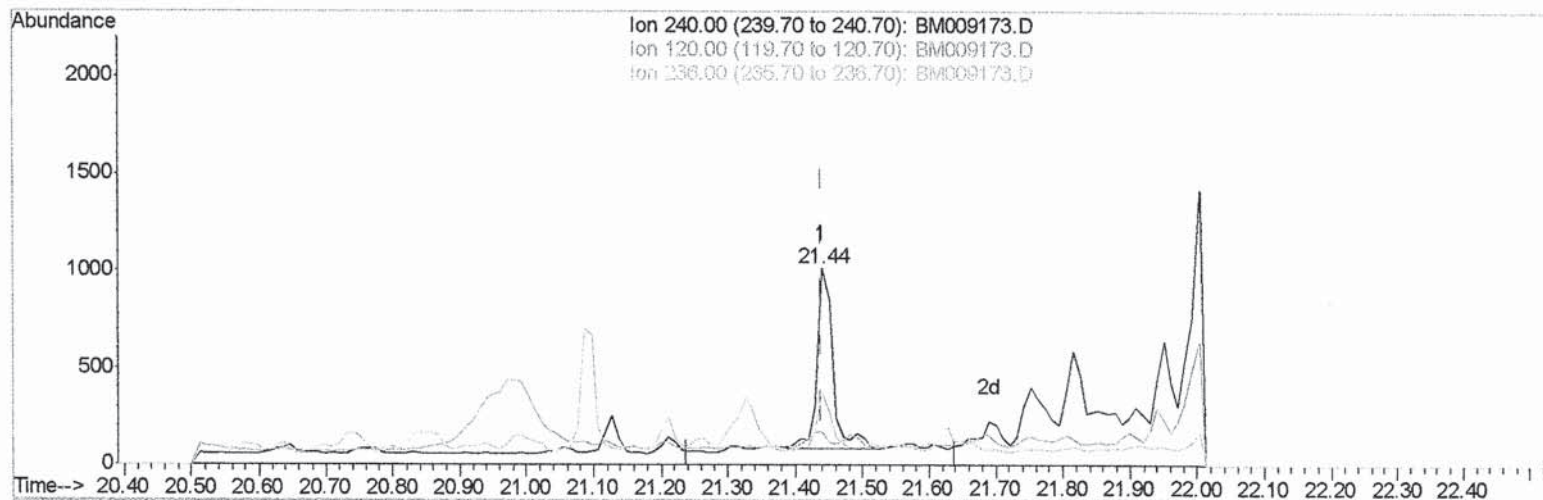

TIC: BM009173.D

(16) Chrysene-d12 (I)

21.440min (+0.000) 0.40ng/ul

response 1498

Ion	Exp%	Act%
240.00	100	100
120.00	20.60	16.78
236.00	34.90	37.02
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_M\Data\BM031017\
Data File : BM009173.D
Acq On : 10 Mar 2017 13:23
Operator : SJ/MA
Sample : I2062-06
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AC7

Manual Integrations
APPROVED

mohammad
3/13/2017 2:13:25 PM

Quant Time: Mar 10 15:48:01 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 10 15:19:24 2017
Response via : Initial Calibration

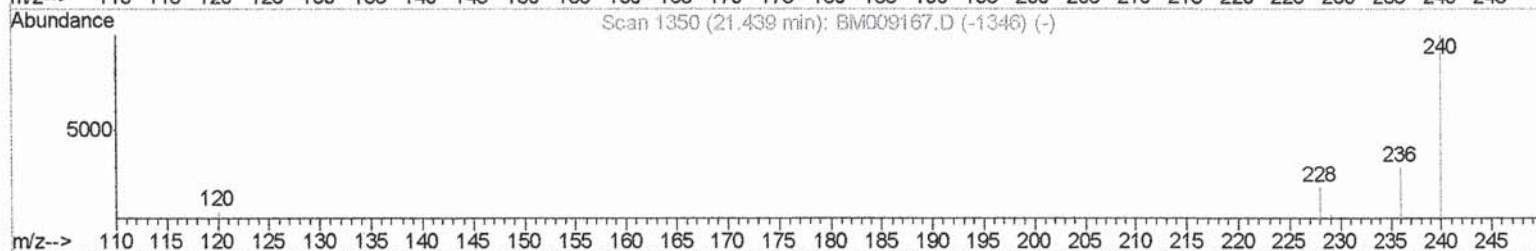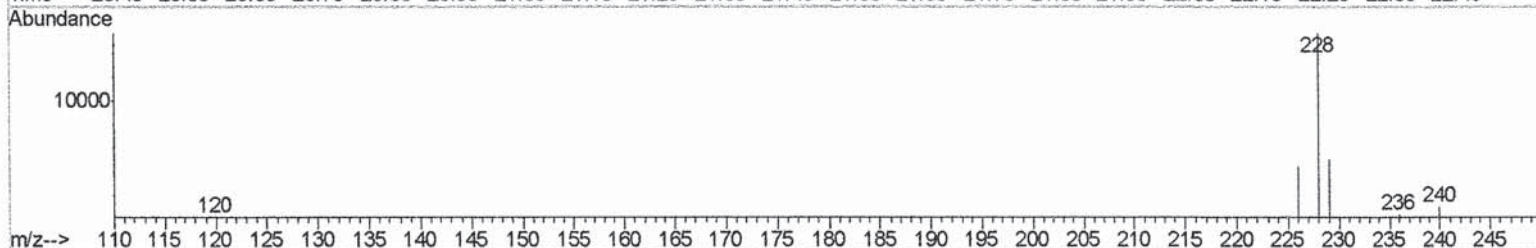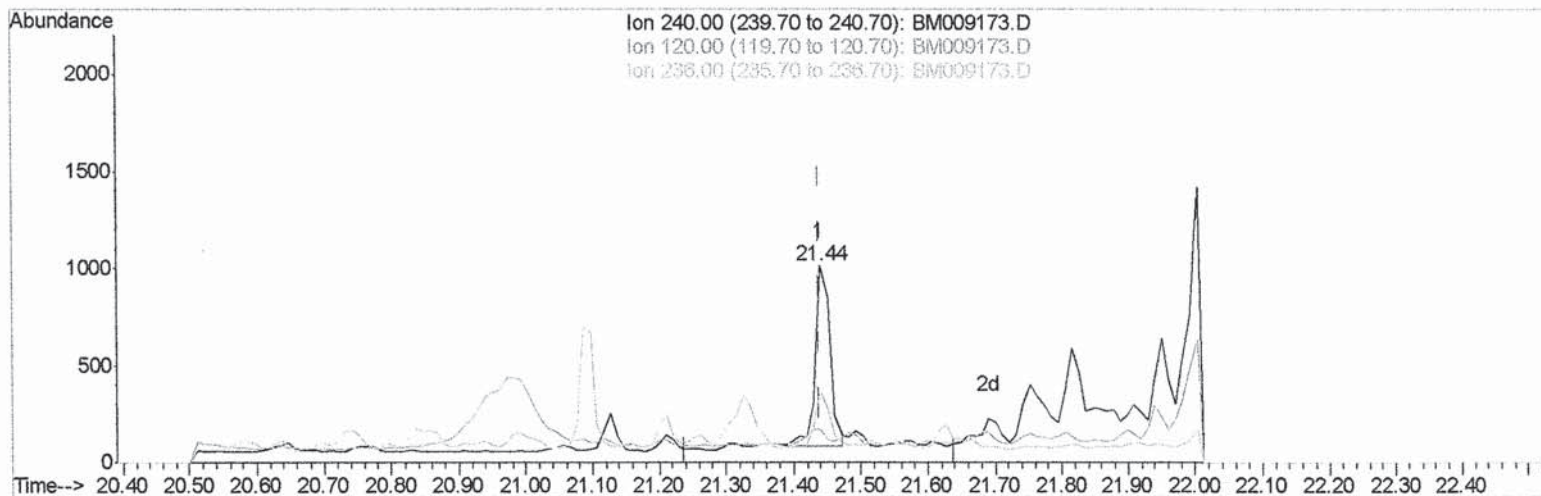

TIC: BM009173.D

(16) Chrysene-d12 (I)

21.440min (+0.000) 0.40ng/ul m

response 1413

Ion	Exp%	Act%
240.00	100	100
120.00	20.60	16.78
236.00	34.90	37.02
0.00	0.00	0.00

> SJ
03/13/17

Data Path : Z:\HPCHEM1\BNA_M\Data\BM031017\
 Data File : BM009173.D
 Acq On : 10 Mar 2017 13:23
 Operator : SJ/MA
 Sample : I2062-06
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AC7

Manual Integrations
 APPROVED

mohammad
 3/13/2017 2:13:25 PM

Quant Time: Mar 10 16:23:17 2017
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030317.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Mar 10 15:19:24 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Dichlorobenzene-d4	7.88	152	237	0.40	ng/ul	0.00
2) Naphthalene-d8	10.68	136	756	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.52	164	536	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.26	188	1062m	0.40	ng/ul	0.00
16) Chrysene-d12	21.44	240	1413m	0.40	ng/ul	0.00
20) Perylene-d12	23.78	264	1085m	0.40	ng/ul	0.01

SJ
 03/13/17

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev (Min)
4) 2-Methylnaphthalene-d10	12.27	152	356	0.28	ng/ul	0.00
14) Fluoranthene-d10	19.29	212	1157	0.35	ng/ul	0.00

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
3) Naphthalene	10.73	128	30348	13.92	ng/ul#	93
5) 2-Methylnaphthalene	12.34	142	12031	7.68	ng/ul	100
7) Acenaphthylene	14.23	152	6545	2.35	ng/ul	98
8) Acenaphthene	14.57	153	14897	6.96	ng/ul	90
9) Fluorene	15.56	166	38345	15.31	ng/ul#	81
12) Phenanthrene	17.31	178	319973m	95.95	ng/ul	
13) Anthracene	17.40	178	79480	24.13	ng/ul#	92
15) Fluoranthene	19.33	202	336236	77.30	ng/ul	92
17) Pyrene	19.69	202	251785	51.81	ng/ul	95
18) Benzo(a)anthracene	21.42	228	145319	30.95	ng/ul	94
19) Chrysene	21.47	228	100016	22.46	ng/ul	93
21) Benzo(b)fluoranthene	23.07	252	122239m	28.68	ng/ul	
22) Benzo(k)fluoranthene	23.11	252	41330m	10.97	ng/ul	
23) Benzo(a)pyrene	23.67	252	86259m	22.49	ng/ul	
24) Indeno(1,2,3-cd)pyrene	26.15	276	47739m	9.79	ng/ul	
25) Dibenzo(a,h)anthracene	26.16	278	13979m	3.41	ng/ul	
26) Benzo(g,h,i)perylene	26.89	276	36446m	8.76	ng/ul	

SJ
 03/13/17

SJ
 03/13/17

(#) = qualifier out of range (m) = manual integration (+) = signals summed