


Data Path : Z:\HPCHEM1\BNA_M\Data\BM031017\
Data File : BM009174.D
Acq On : 10 Mar 2017 13:58
Operator : SJ/MA
Sample : I2062-22
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AK8

Manual Integrations
APPROVED

mohammad
3/13/2017 2:13:28 PM

Quant Time: Mar 10 15:54:13 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 10 15:19:24 2017
Response via : Initial Calibration

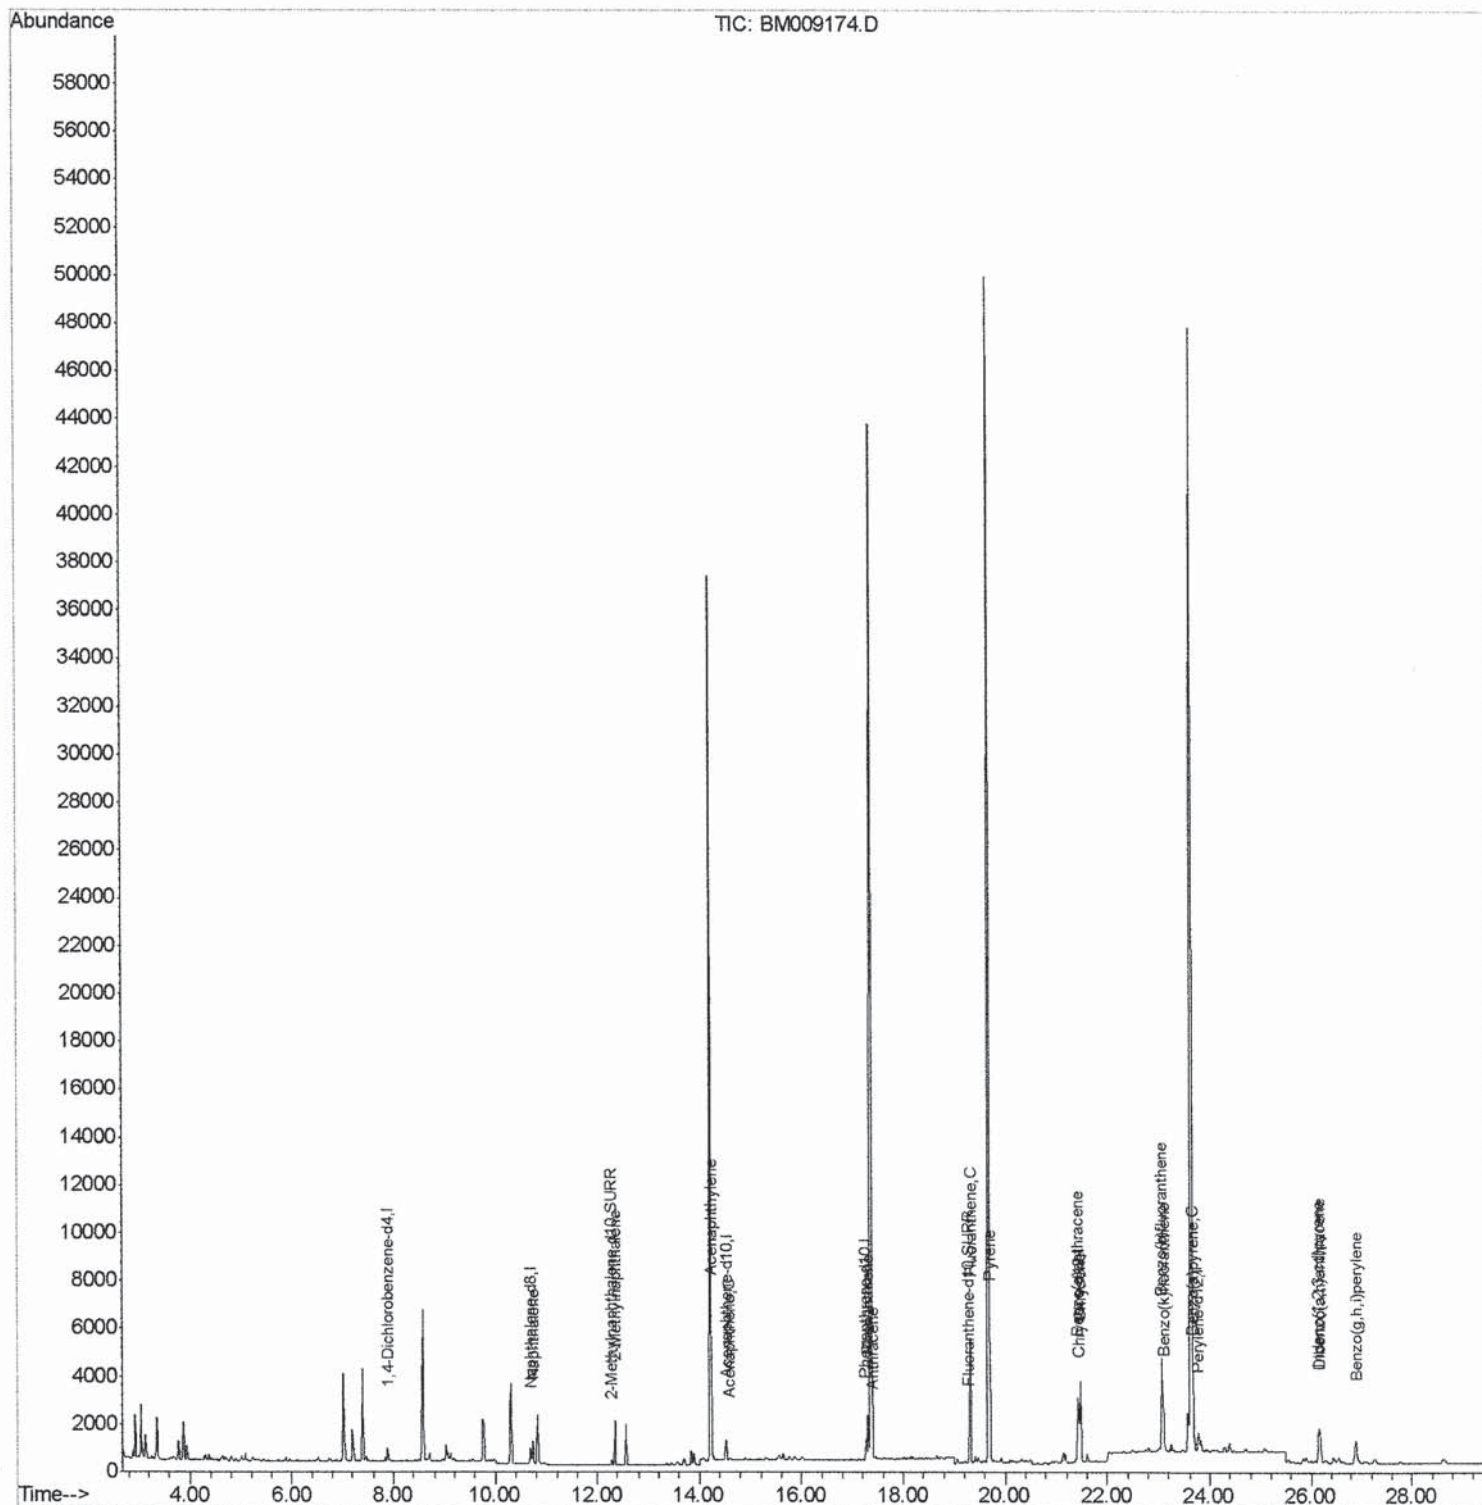



Data Path : Z:\HPCHEM1\BNA_M\Data\BM031017\
Data File : BM009174.D
Acq On : 10 Mar 2017 13:58
Operator : SJ/MA
Sample : I2062-22
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AK8

Manual Integrations
APPROVED

mohammad
3/13/2017 2:13:28 PM

Quant Time: Mar 10 15:48:48 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 10 15:19:24 2017
Response via : Initial Calibration

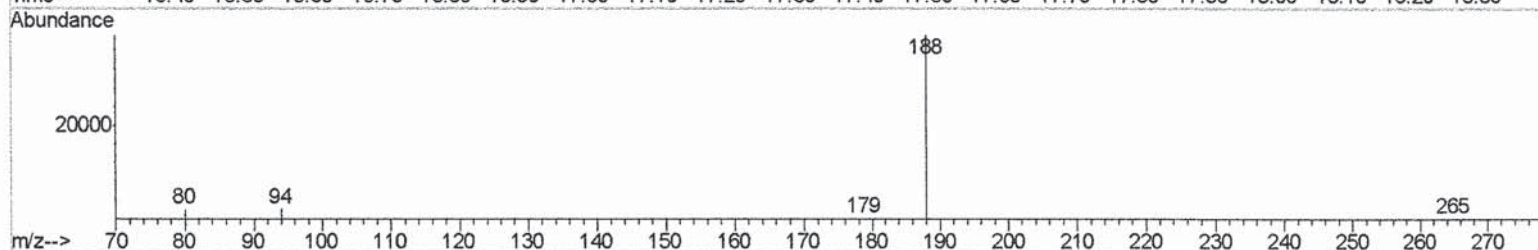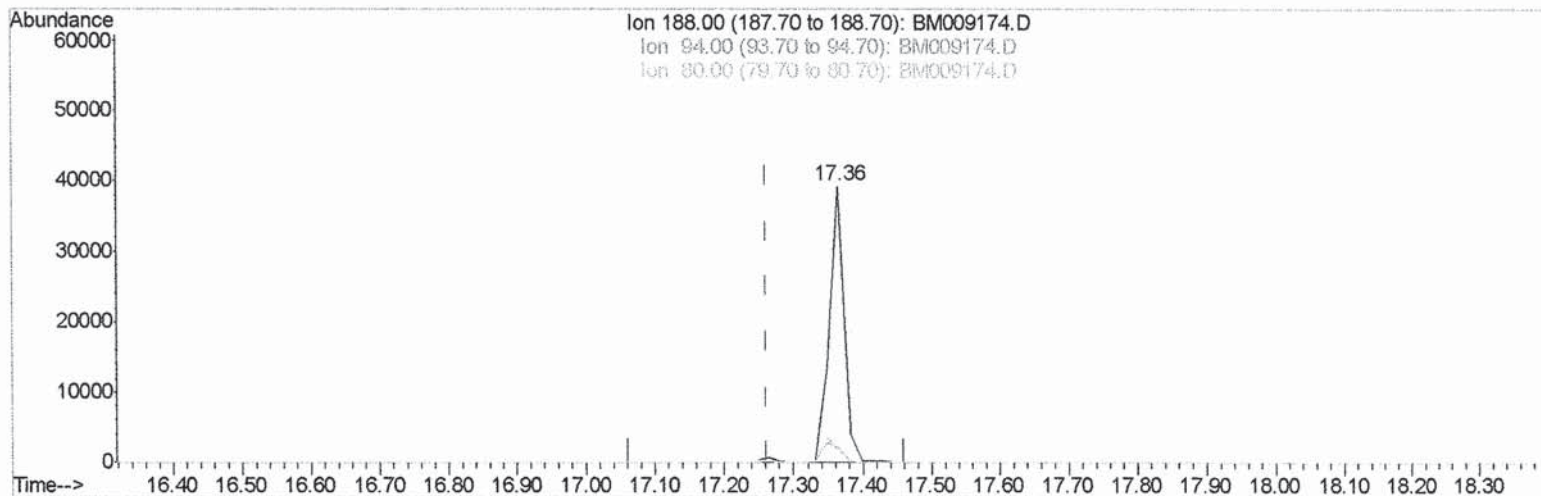

TIC: BM009174.D

(10) Phenanthrene-d10 (I)

17.365min (+0.103) 0.40ng/ul

response 58013

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	5.49#
80.00	11.80	5.10#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_M\Data\BM031017\
 Data File : BM009174.D
 Acq On : 10 Mar 2017 13:58
 Operator : SJ/MA
 Sample : I2062-22
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AK8

Manual Integrations
 APPROVED

mohammad
 3/13/2017 2:13:28 PM

Quant Time: Mar 10 15:48:48 2017
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030317.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Mar 10 15:19:24 2017
 Response via : Initial Calibration

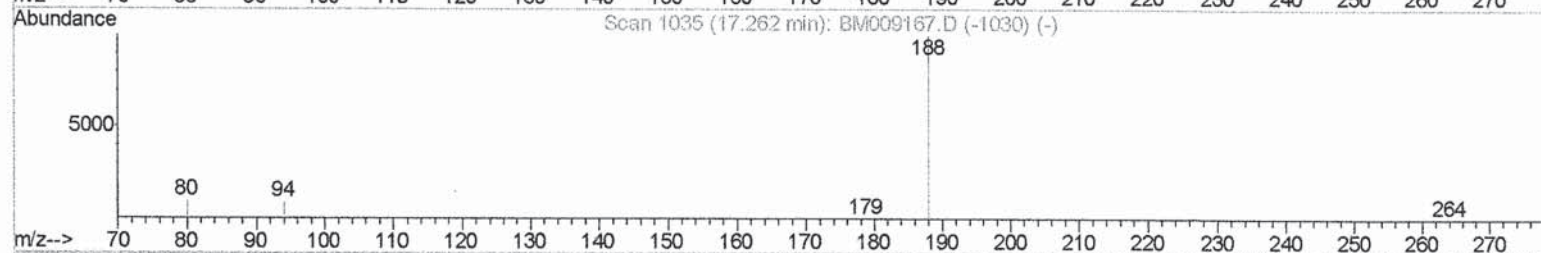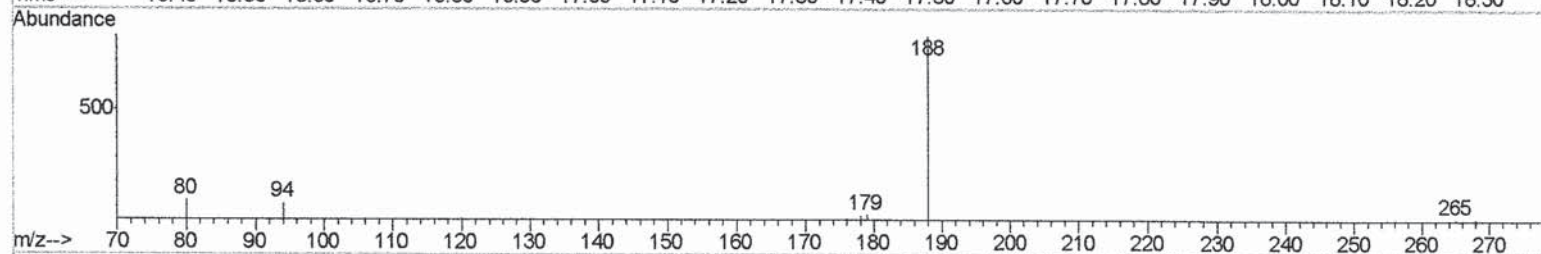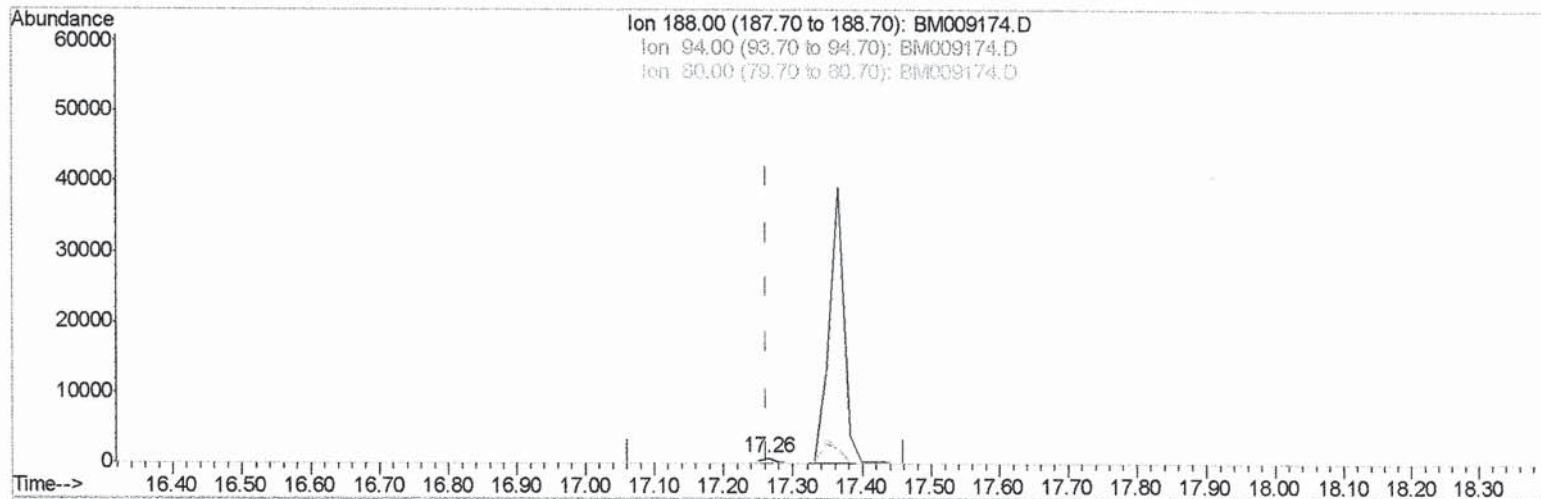

TIC: BM009174.D

(10) Phenanthrene-d10 (I)

17.262min (+0.000) 0.40ng/ul m

response 1098

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	13.82#
80.00	11.80	15.44#
0.00	0.00	0.00

SJ
 03/13/17

Quantitation Report (Qedit)



Data Path : Z:\HPCHEM1\BNA_M\Data\BM031017\
 Data File : BM009174.D
 Acq On : 10 Mar 2017 13:58
 Operator : SJ/MA
 Sample : I2062-22
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AK8

Manual Integrations
 APPROVED

mohammad
 3/13/2017 2:13:28 PM

Quant Time: Mar 10 15:50:08 2017
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030317.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Mar 10 15:19:24 2017
 Response via : Initial Calibration

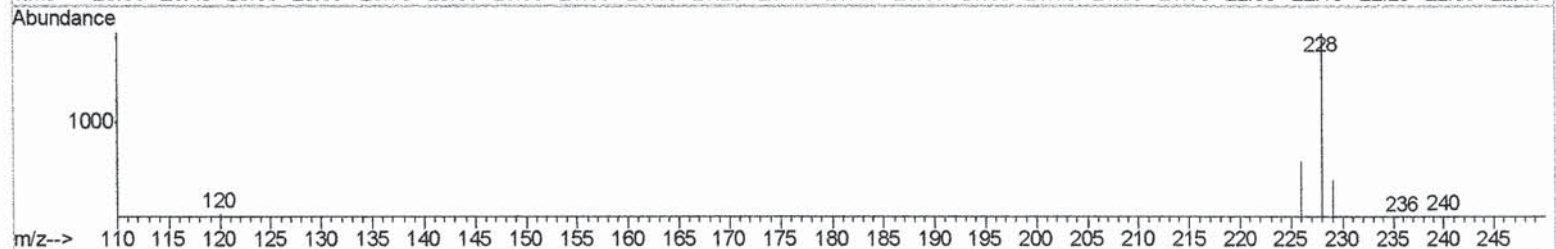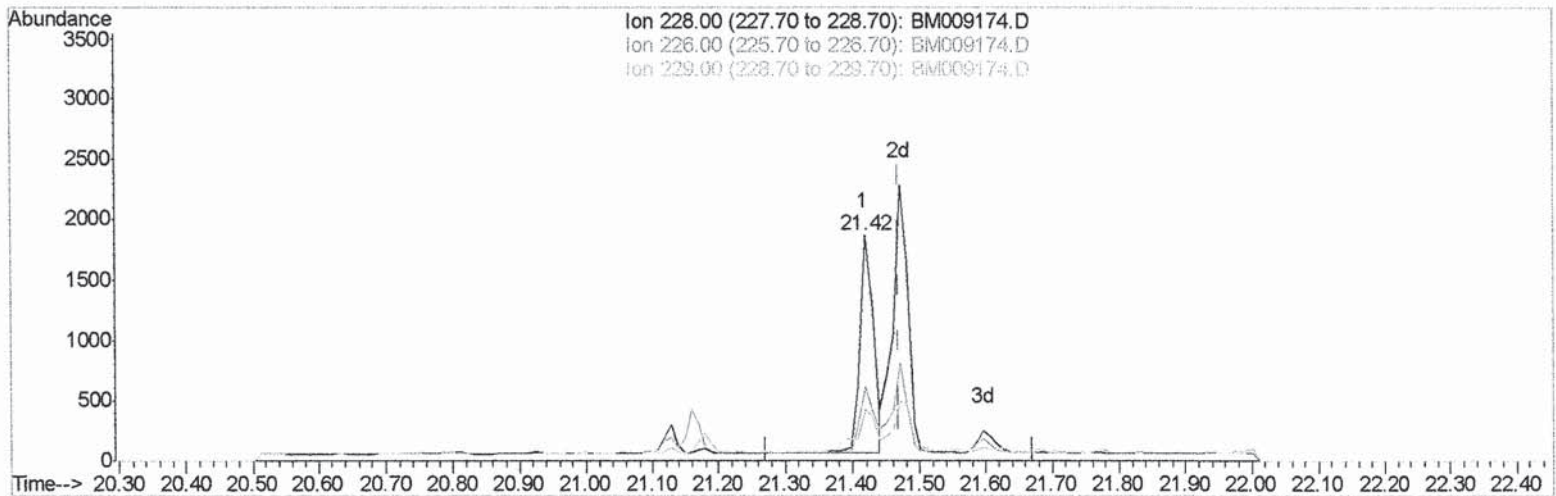

TIC: BM009174.D

(19) Chrysene

21.419min (-0.052) 0.68ng/ul

response 2557

Ion	Exp%	Act%
228.00	100	100
226.00	29.20	32.82
229.00	22.10	22.90
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_M\Data\BM031017\
Data File : BM009174.D
Acq On : 10 Mar 2017 13:58
Operator : SJ/MA
Sample : I2062-22
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AK8

Manual Integrations
APPROVED

mohammad
3/13/2017 2:13:28 PM

Quant Time: Mar 10 15:50:08 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 10 15:19:24 2017
Response via : Initial Calibration

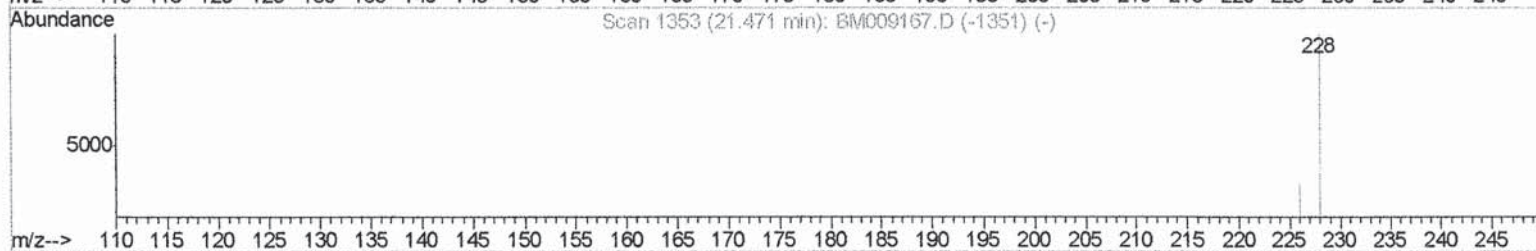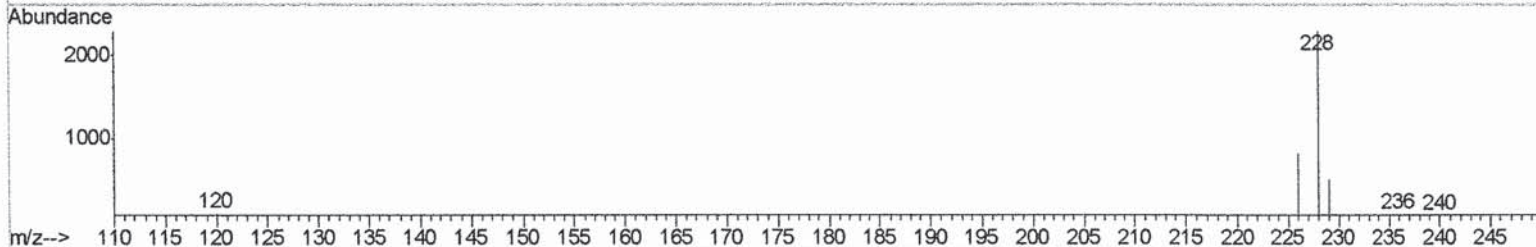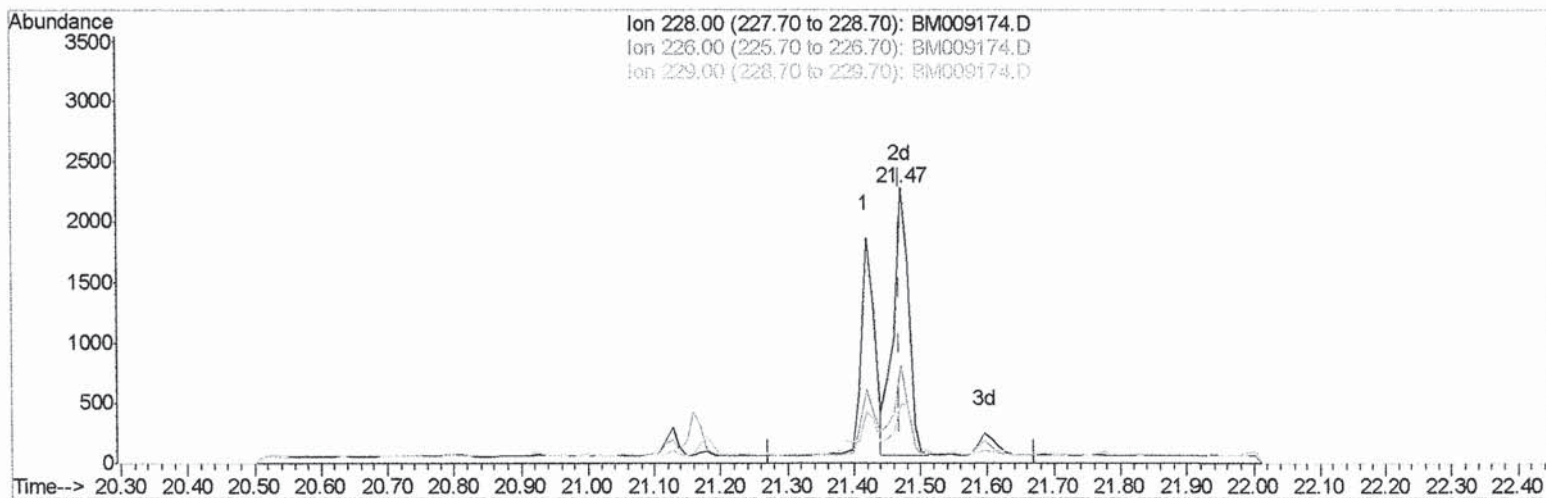

TIC: BM009174.D

(19) Chrysene

21.471min (+0.000) 0.96ng/ul m

response 3600

Ion	Exp%	Act%
228.00	100	100
226.00	29.20	35.54#
229.00	22.10	21.84
0.00	0.00	0.00

> SJ
03/13/17




Data Path : Z:\HPCHEM1\BNA_M\Data\BM031017\
Data File : BM009174.D
Acq On : 10 Mar 2017 13:58
Operator : SJ/MA
Sample : I2062-22
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AK8

Manual Integrations
APPROVED

mohammad
3/13/2017 2:13:28 PM

Quant Time: Mar 10 15:50:08 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 10 15:19:24 2017
Response via : Initial Calibration

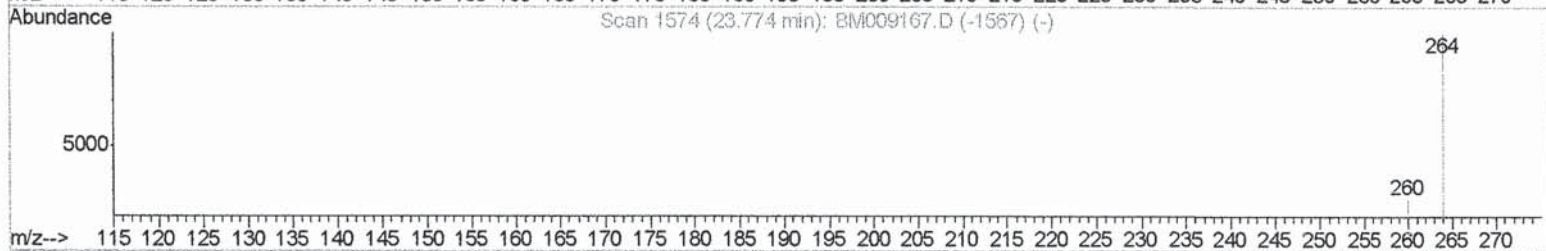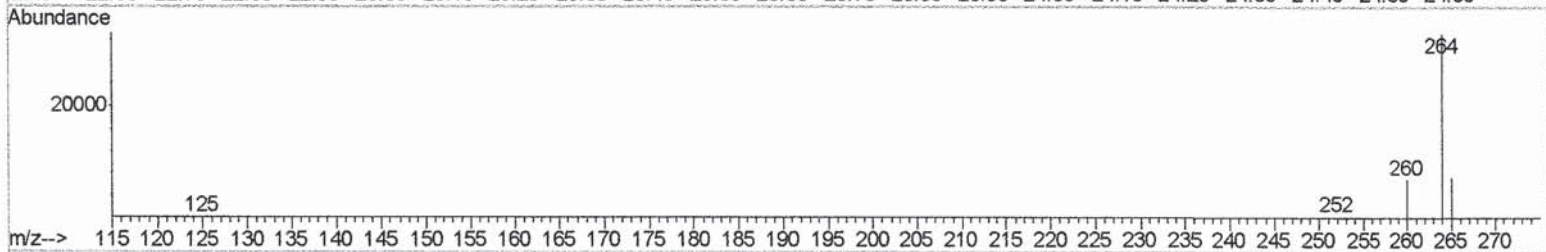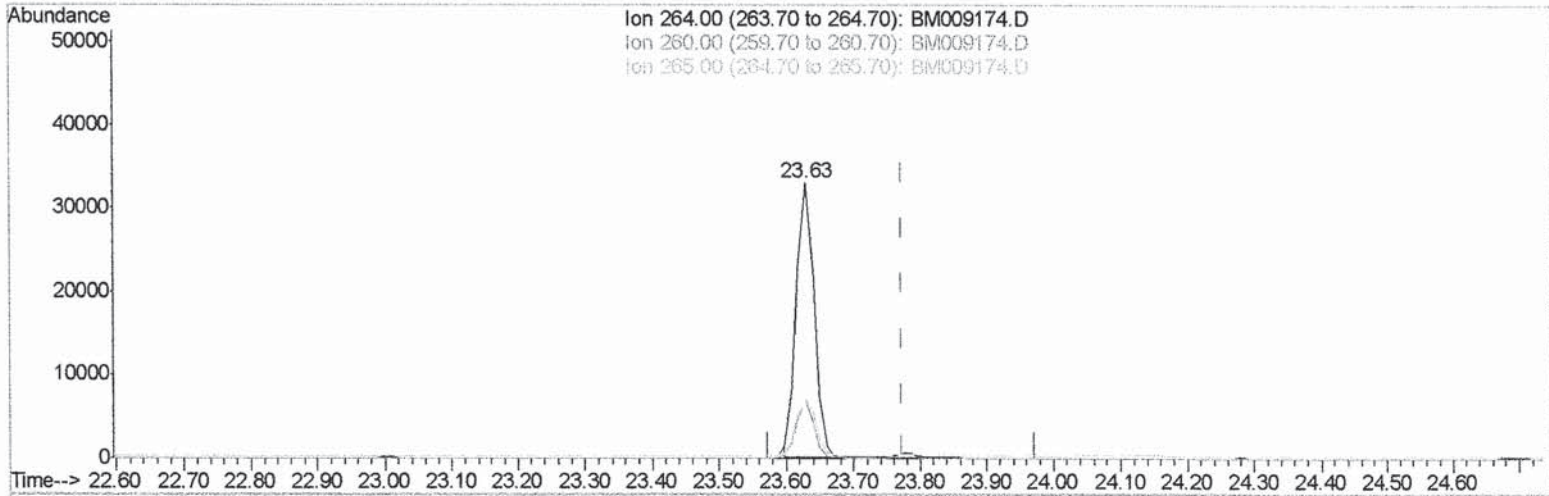

TIC: BM009174.D

(20) Perylene-d12 (I)
23.629min (-0.146) 0.40ng/ul
response 59411

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	20.84#
265.00	103.50	22.06#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_M\Data\BM031017\
 Data File : BM009174.D
 Acq On : 10 Mar 2017 13:58
 Operator : SJ/MA
 Sample : I2062-22
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AK8

Manual Integrations
 APPROVED

mohammad
 3/13/2017 2:13:28 PM

Quant Time: Mar 10 15:50:08 2017
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030317.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Mar 10 15:19:24 2017
 Response via : Initial Calibration

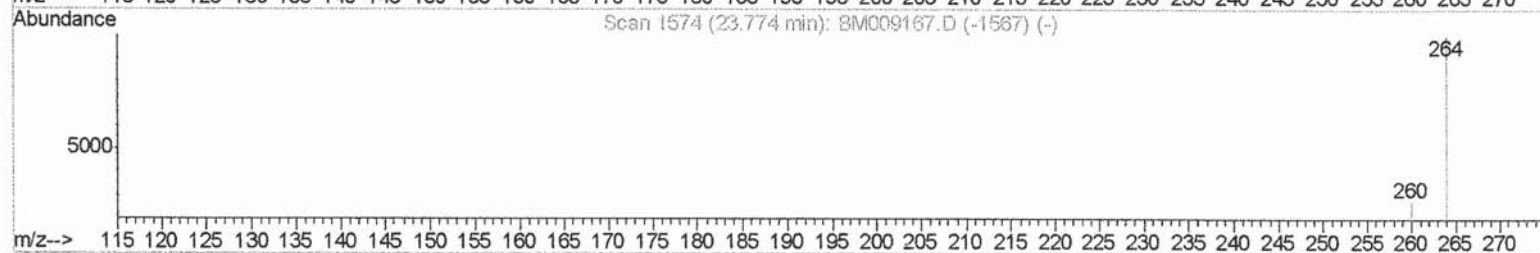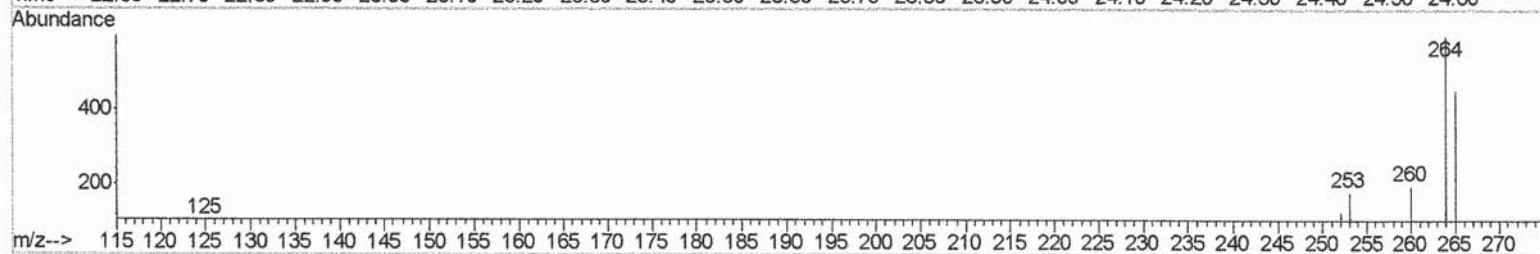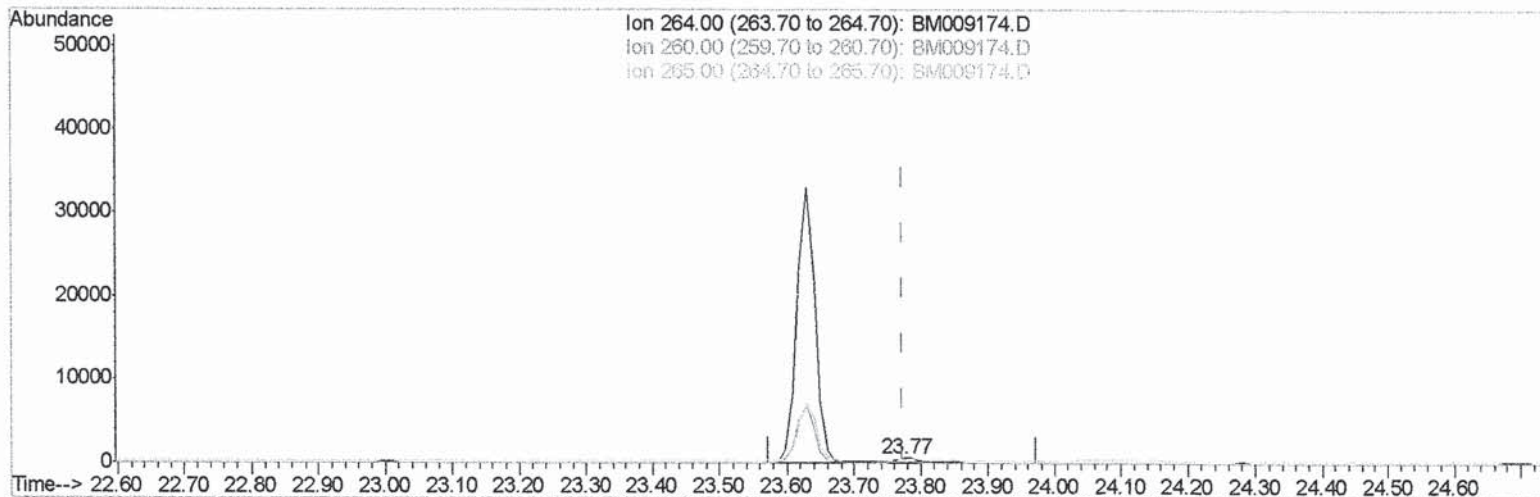

TIC: BM009174.D

(20) Perylene-d12 (I)

23.775min (+0.000) 0.40ng/ul m

response 1028

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	33.33
265.00	103.50	75.71#
0.00	0.00	0.00

SJ
 03/13/17




Data Path : Z:\HPCHEM1\BNA_M\Data\BM031017\
Data File : BM009174.D
Acq On : 10 Mar 2017 13:58
Operator : SJ/MA
Sample : I2062-22
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AK8

Manual Integrations
APPROVED

mohammad
3/13/2017 2:13:28 PM

Quant Time: Mar 10 15:51:15 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 10 15:19:24 2017
Response via : Initial Calibration

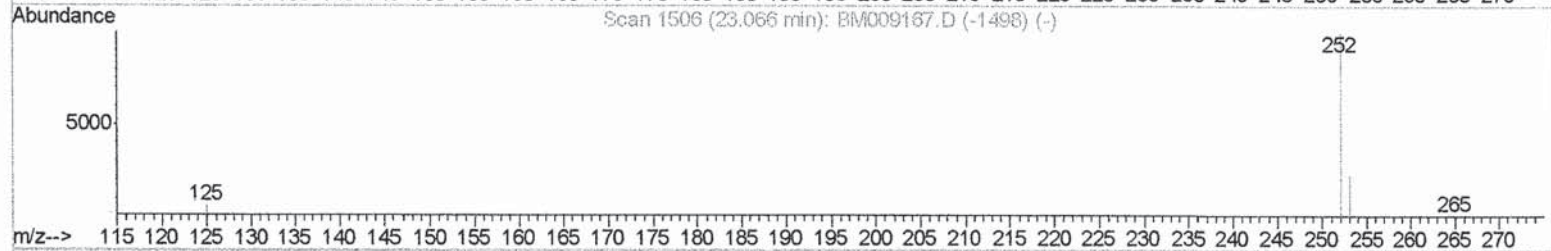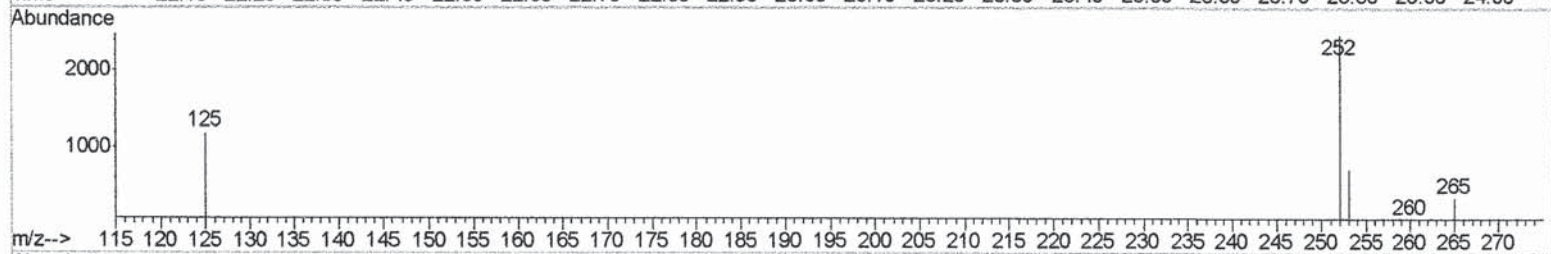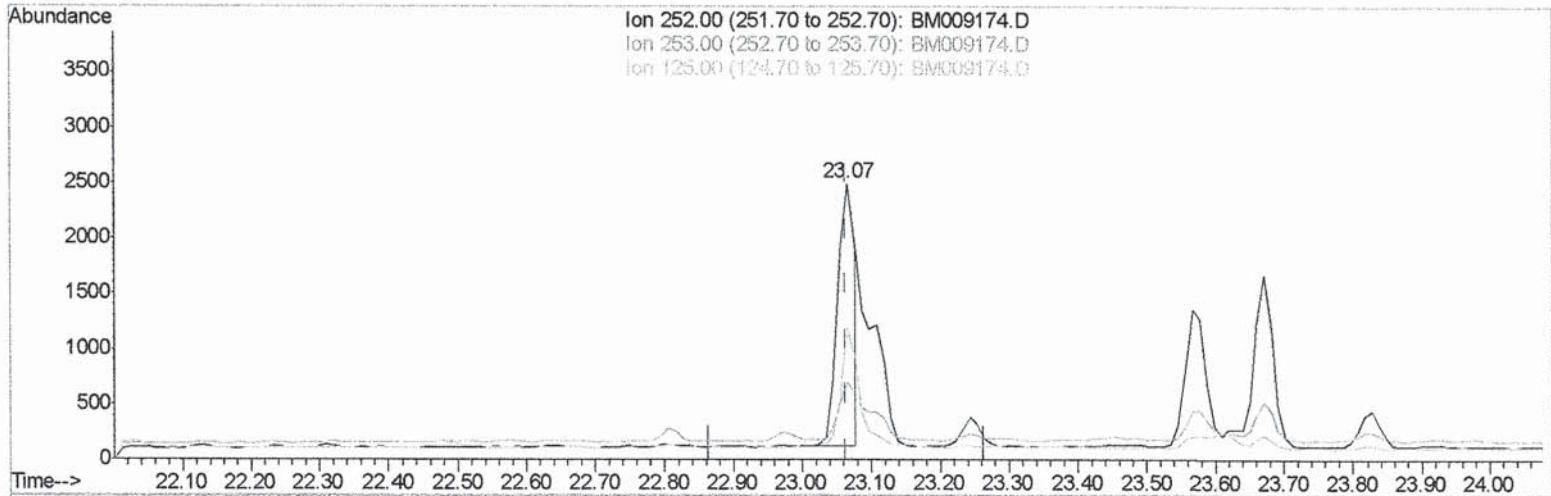

TIC: BM009174.D

(21) Benzo(b)fluoranthene
23.066min (+0.000) 1.03ng/ul
response 4142

Ion	Exp%	Act%
252.00	100	100
253.00	32.10	28.26
125.00	17.50	47.55#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM031017\
 Data File : BM009174.D
 Acq On : 10 Mar 2017 13:58
 Operator : SJ/MA
 Sample : I2062-22
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AK8

Manual Integrations
 APPROVED

mohammad
 3/13/2017 2:13:28 PM

Quant Time: Mar 10 15:51:15 2017
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030317.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Mar 10 15:19:24 2017
 Response via : Initial Calibration

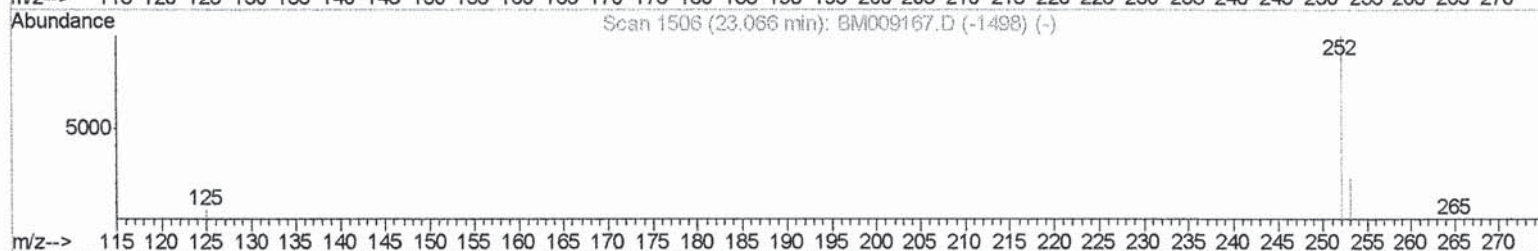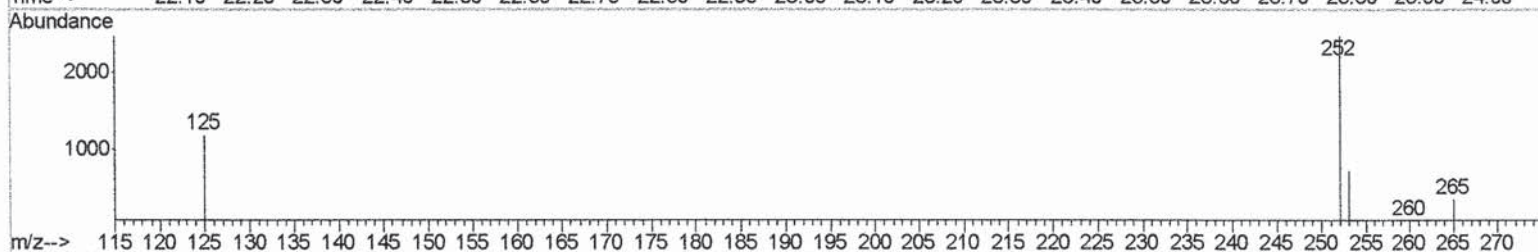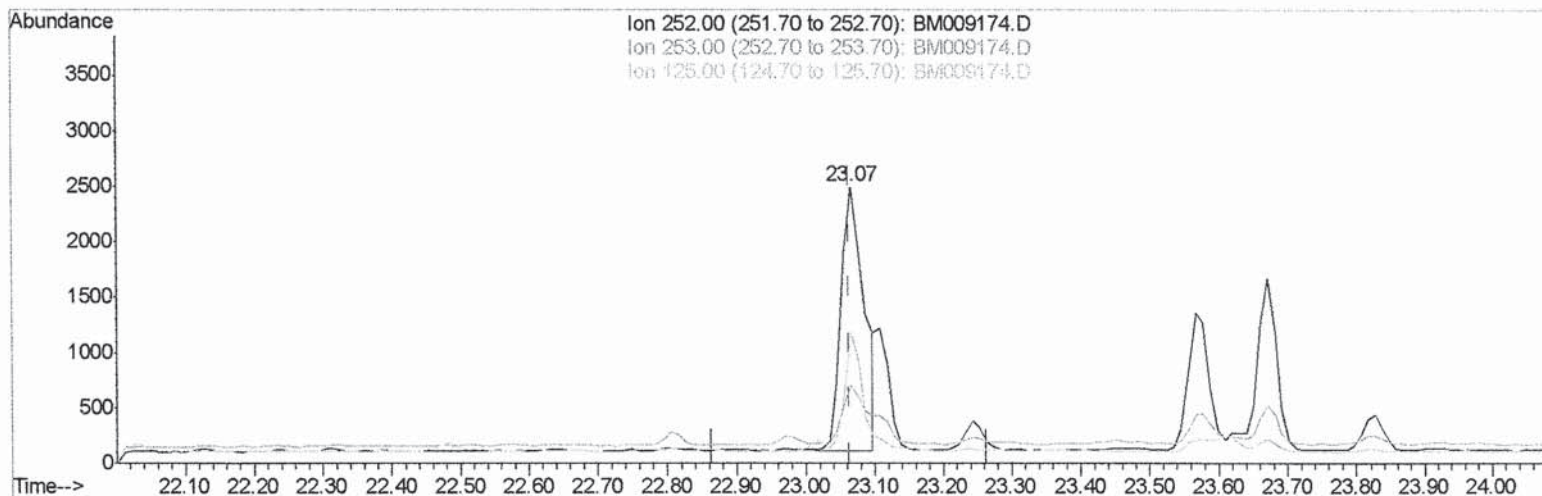

TIC: BM009174.D

(21) Benzo(b)fluoranthene

23.066min (+0.000) 1.39ng/ul m

response 5627

Ion	Exp%	Act%
252.00	100	100
253.00	32.10	28.26
125.00	17.50	47.55#
0.00	0.00	0.00

SJ
03/13/17



Data Path : Z:\HPCHEM1\BNA_M\Data\BM031017\
Data File : BM009174.D
Acq On : 10 Mar 2017 13:58
Operator : SJ/MA
Sample : I2062-22
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AK8

Manual Integrations
APPROVED

mohammad
3/13/2017 2:13:28 PM

Quant Time: Mar 10 15:51:15 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 10 15:19:24 2017
Response via : Initial Calibration

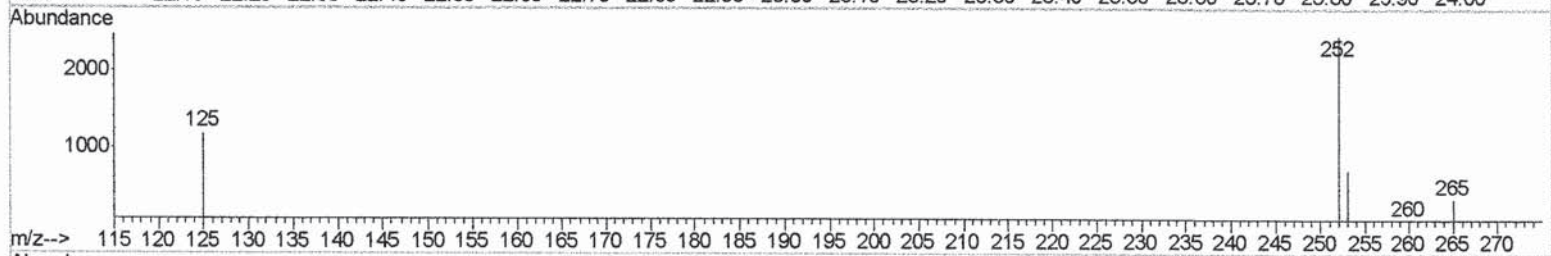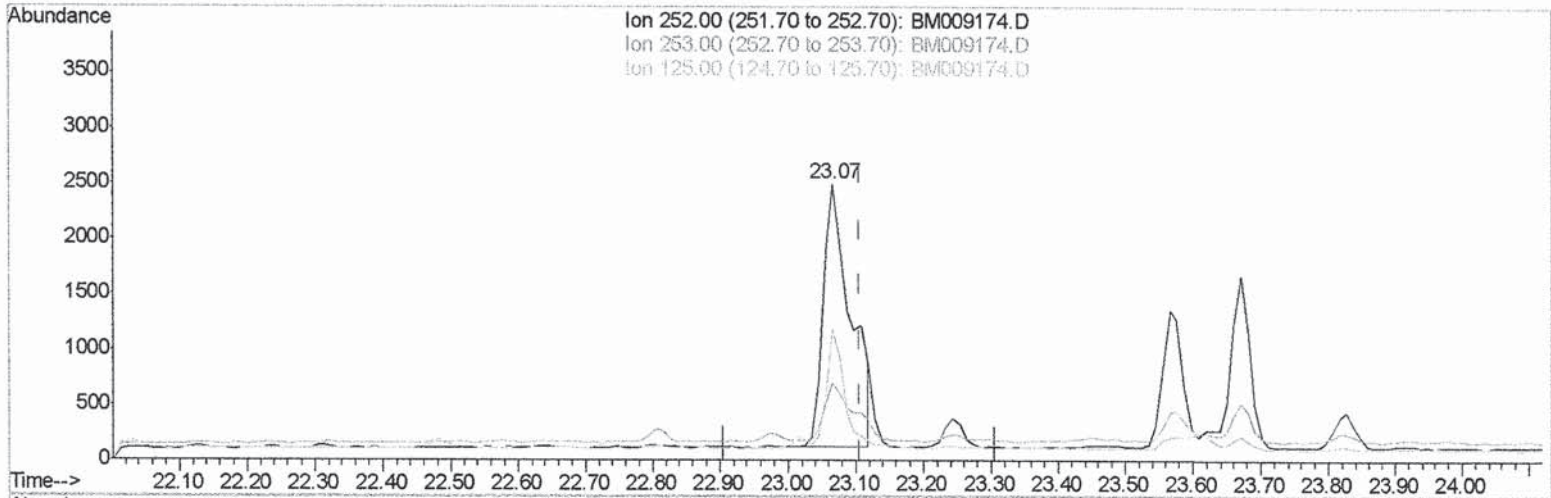

TIC: BM009174.D

(22) Benzo(k)fluoranthene
23.066min (-0.042) 1.88ng/ul
response 6728

Ion	Exp%	Act%
252.00	100	100
253.00	30.60	28.26
125.00	17.10	47.55#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_M\Data\BM031017\
Data File : BM009174.D
Acq On : 10 Mar 2017 13:58
Operator : SJ/MA
Sample : I2062-22
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AK8

Manual Integrations
APPROVED

mohammad
3/13/2017 2:13:28 PM

Quant Time: Mar 10 15:51:15 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 10 15:19:24 2017
Response via : Initial Calibration

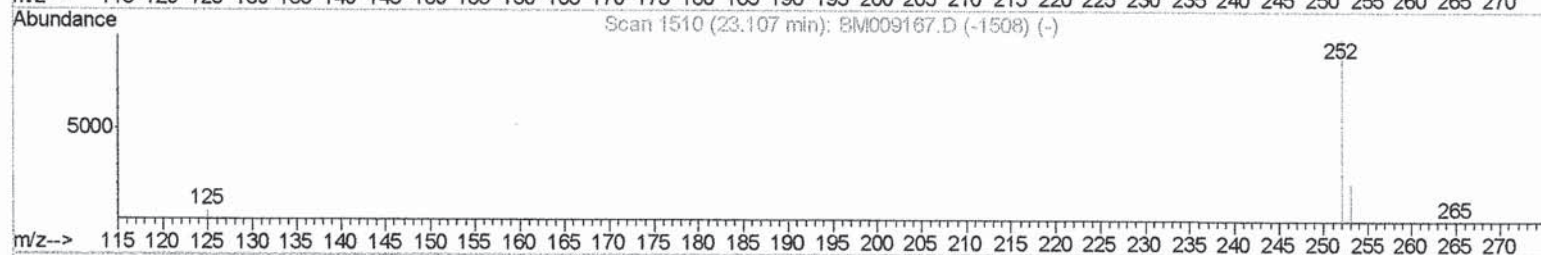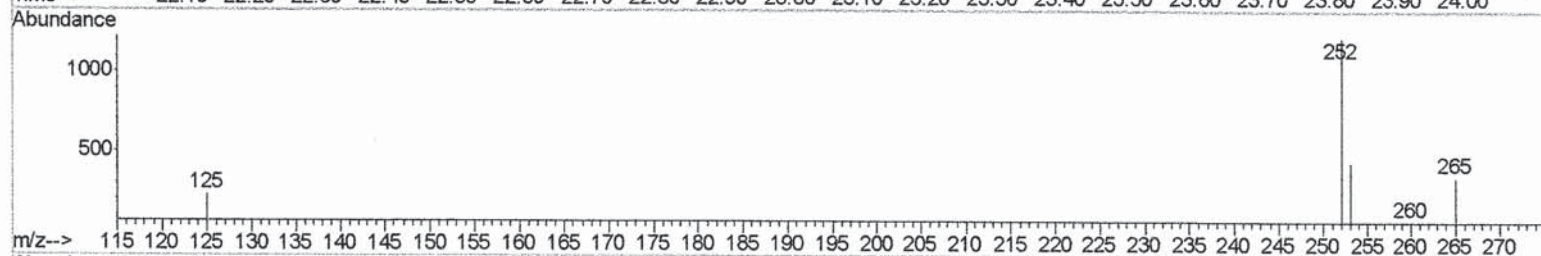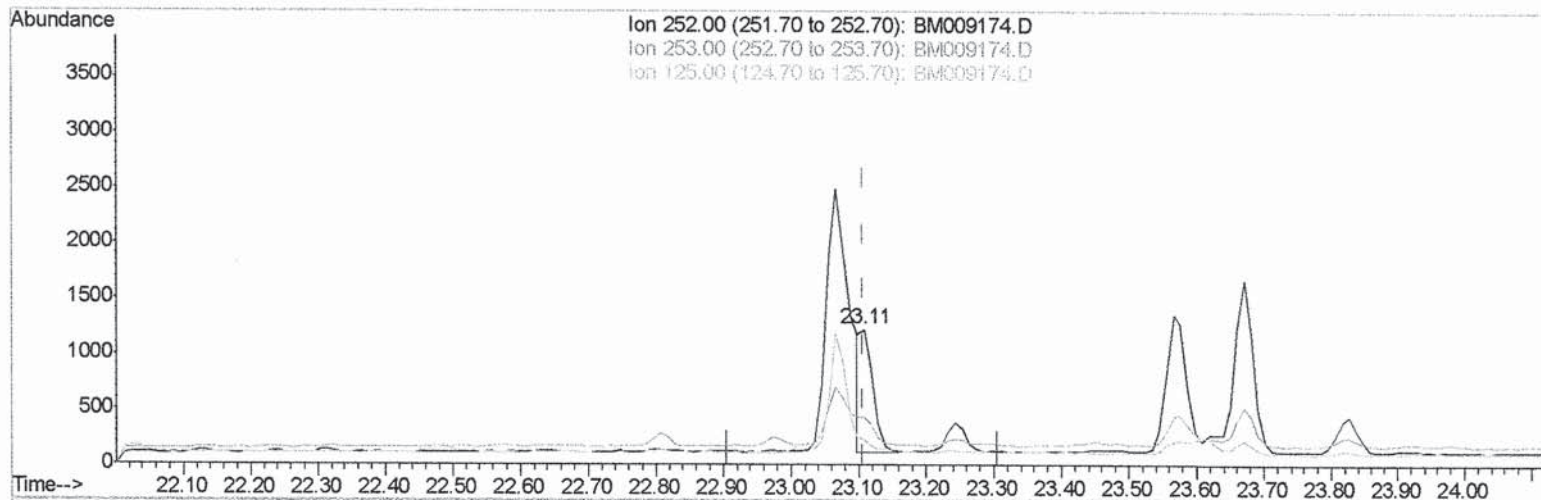

TIC: BM009174.D

(22) Benzo(k)fluoranthene

23.107min (+0.000) 0.39ng/ul m

response 1394

Ion	Exp%	Act%
252.00	100	100
253.00	30.60	35.48
125.00	17.10	18.68
0.00	0.00	0.00

55
03/13/17

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM031017\
 Data File : BM009174.D
 Acq On : 10 Mar 2017 13:58
 Operator : SJ/MA
 Sample : I2062-22
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AK8

Manual Integrations
 APPROVED

mohammad
 3/13/2017 2:13:28 PM

Quant Time: Mar 10 15:51:15 2017
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030317.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Mar 10 15:19:24 2017
 Response via : Initial Calibration

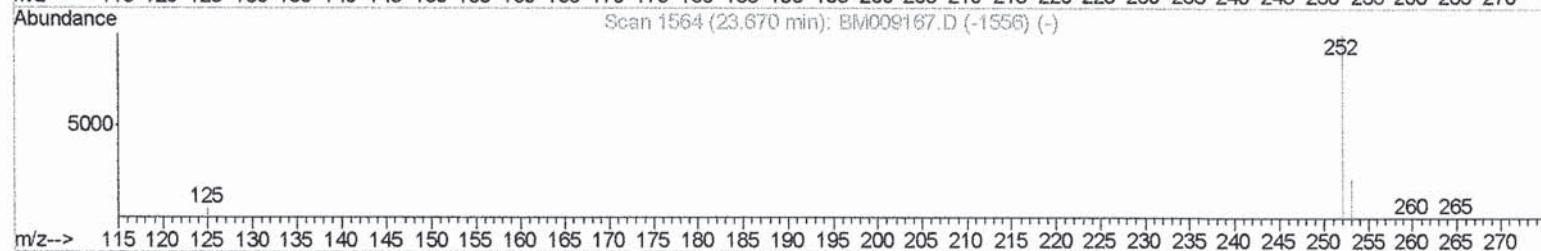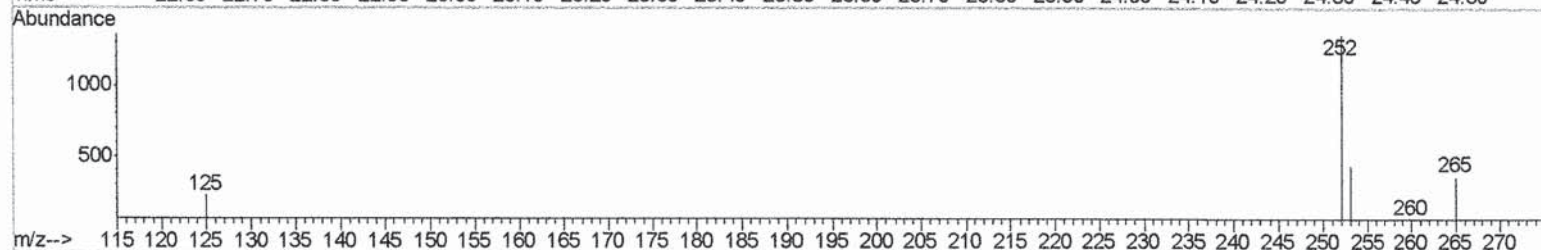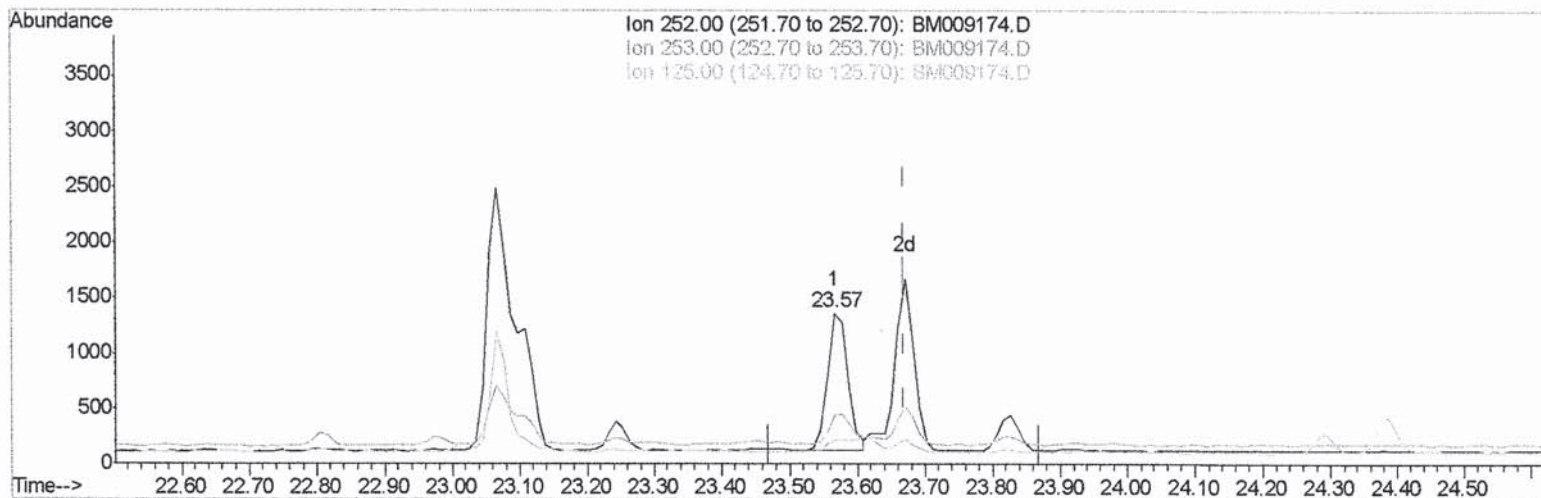

TIC: BM009174.D

(23) Benzo(a)pyrene (C)
 23.566min (-0.104) 0.71ng/ui
 response 2577

Ion	Exp%	Act%
252.00	100	100
253.00	35.60	32.33
125.00	22.60	16.16#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM031017\
 Data File : BM009174.D
 Acq On : 10 Mar 2017 13:58
 Operator : SJ/MA
 Sample : I2062-22
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AK8

Manual Integrations
 APPROVED

mohammad
 3/13/2017 2:13:28 PM

Quant Time: Mar 10 15:51:15 2017
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030317.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Mar 10 15:19:24 2017
 Response via : Initial Calibration

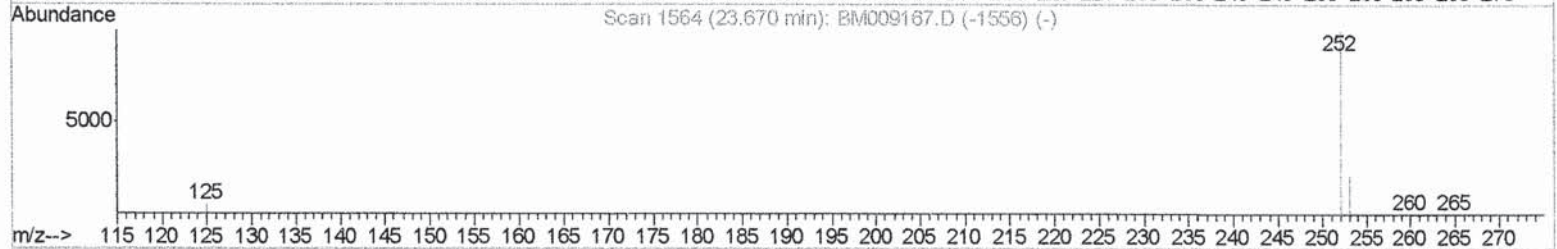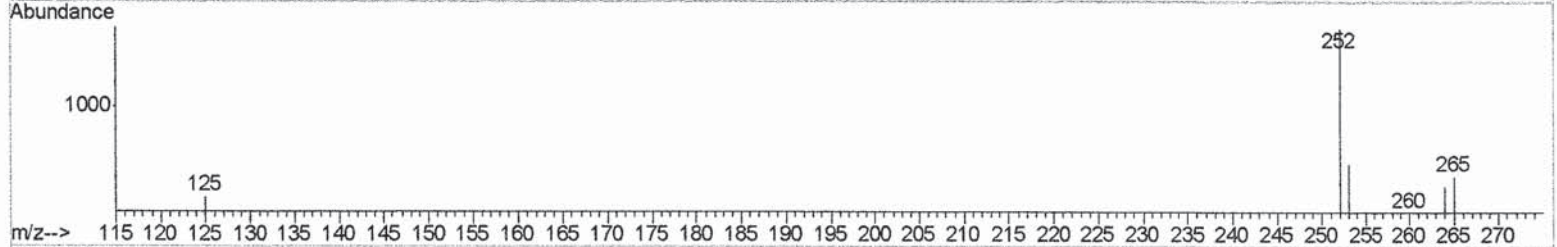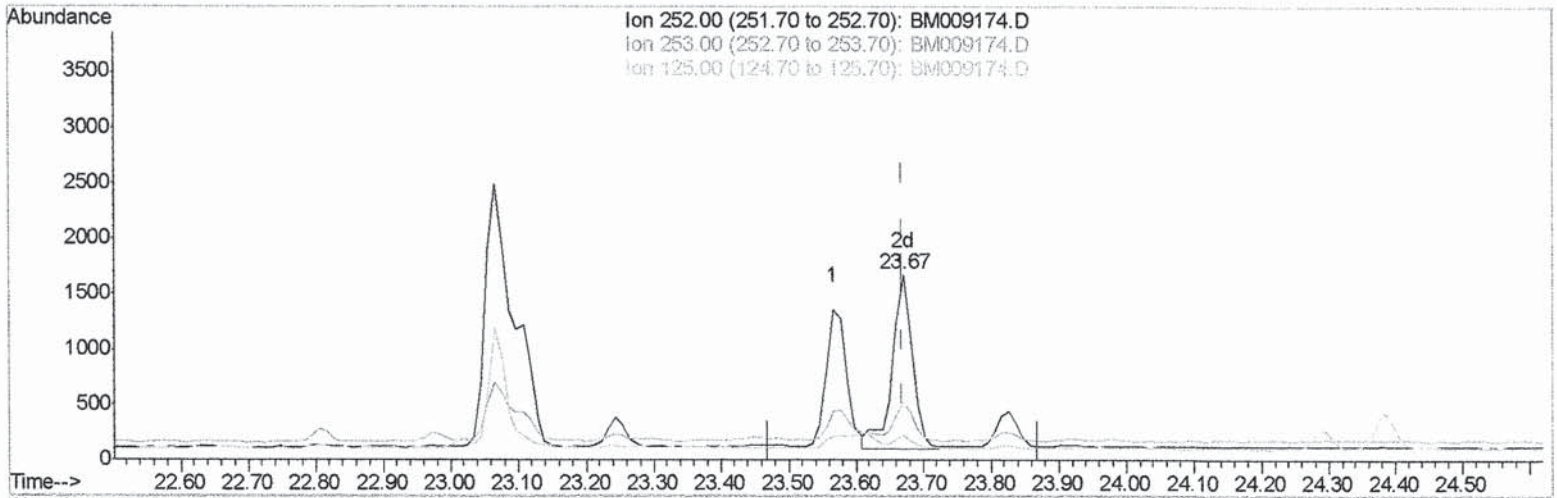

TIC: BM009174.D

(23) Benzo(a)pyrene (C)

23.670min (+0.000) 0.90ng/ul m

response 3276

Ion	Exp%	Act%
252.00	100	100
253.00	35.60	30.85
125.00	22.60	13.60#
0.00	0.00	0.00

SJ
 03/13/17




Data Path : Z:\HPCHEM1\BNA_M\Data\BM031017\
Data File : BM009174.D
Acq On : 10 Mar 2017 13:58
Operator : SJ/MA
Sample : I2062-22
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AK8

Manual Integrations
APPROVED

mohammad
3/13/2017 2:13:28 PM

Quant Time: Mar 10 15:51:15 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 10 15:19:24 2017
Response via : Initial Calibration

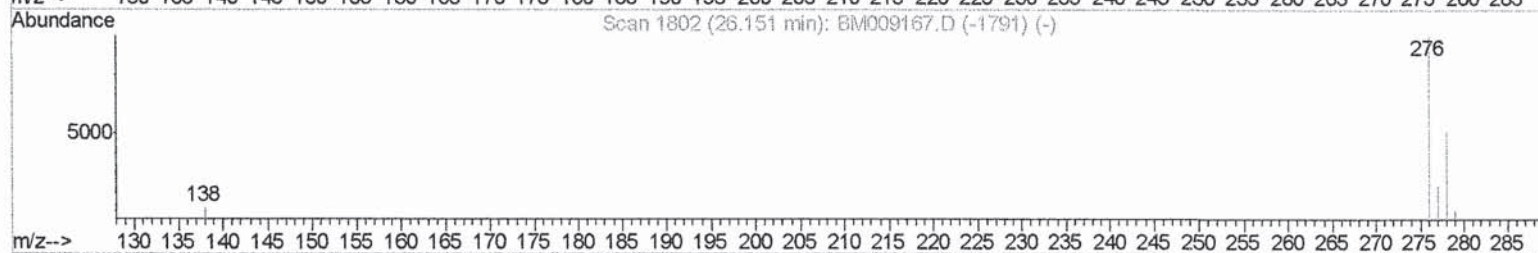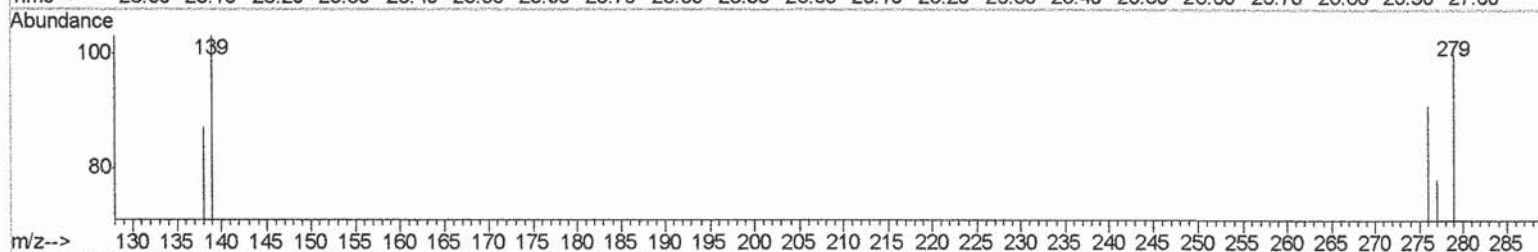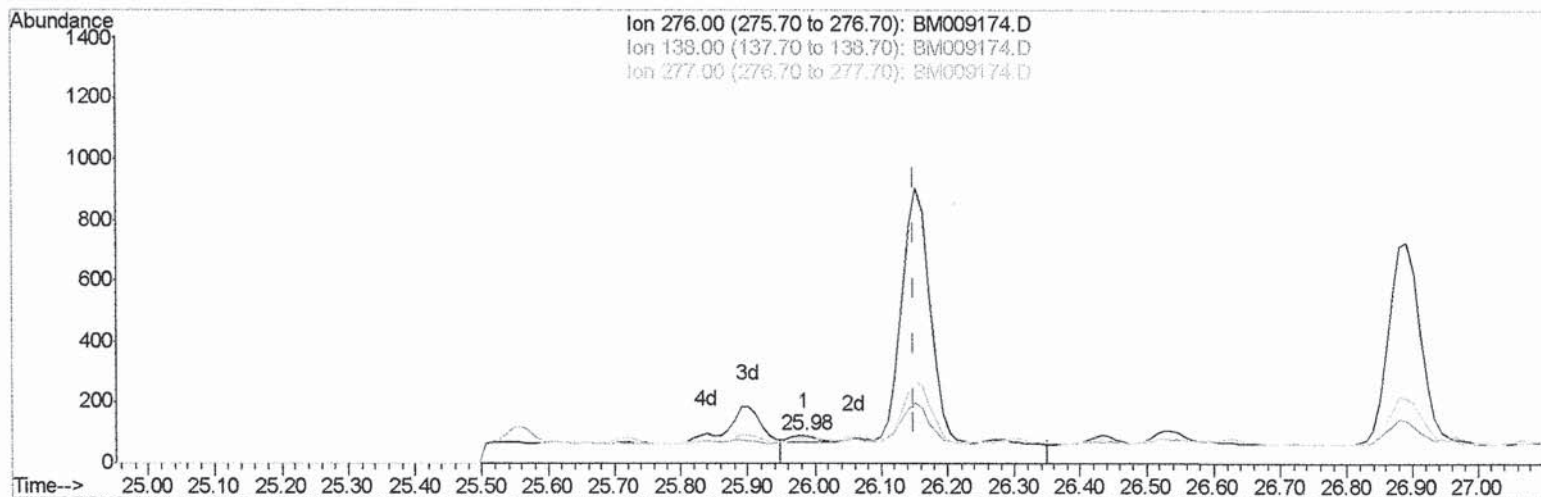

TIC: BM009174.D

(24) Indeno(1,2,3-cd)pyrene

25.985min (-0.167) 0.01ng/ul

response 44

Ion	Exp%	Act%
276.00	100	100
138.00	23.90	115.91#
277.00	24.50	72.73#
0.00	0.00	0.00

Quantitation Report (Qedit)



Data Path : Z:\HPCHEM1\BNA_M\Data\BM031017\
 Data File : BM009174.D
 Acq On : 10 Mar 2017 13:58
 Operator : SJ/MA
 Sample : I2062-22
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AK8

Manual Integrations
 APPROVED

mohammad
 3/13/2017 2:13:28 PM

Quant Time: Mar 10 15:51:15 2017
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030317.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Mar 10 15:19:24 2017
 Response via : Initial Calibration

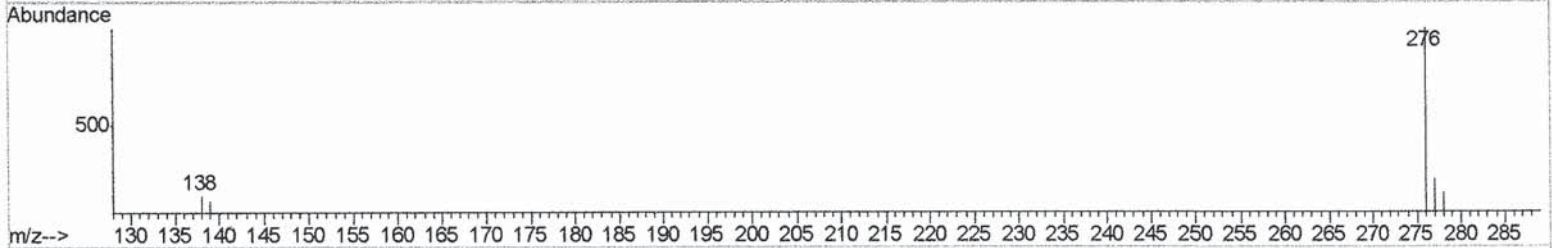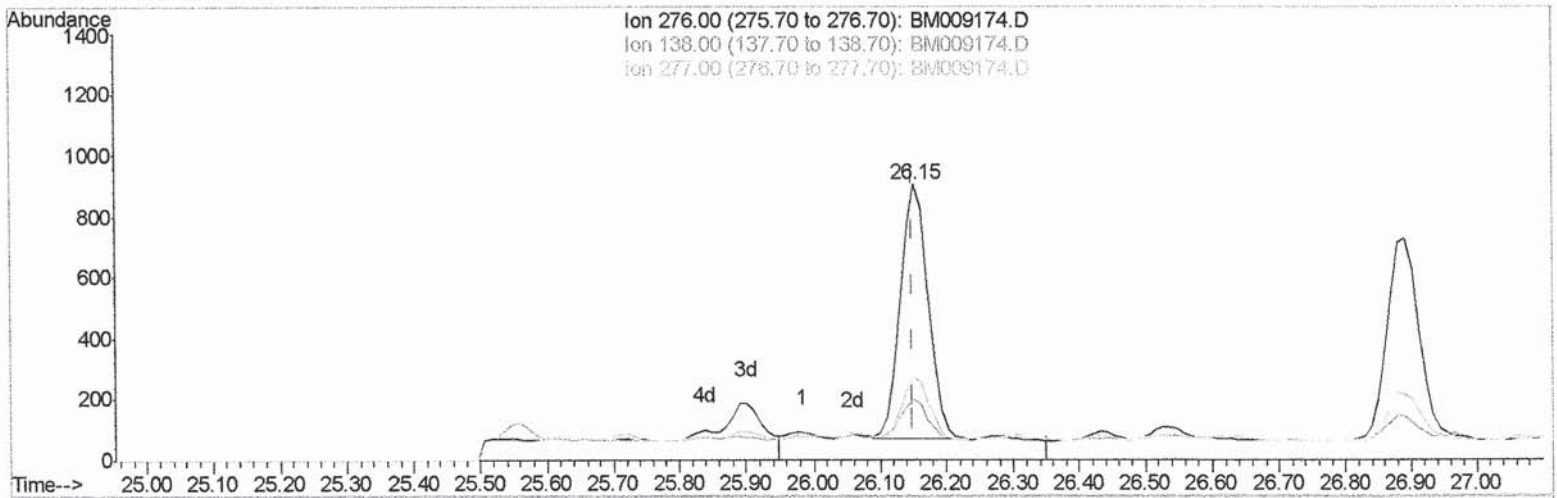

TIC: BM009174.D

(24) Indeno(1,2,3-cd)pyrene

26.151min (+0.000) 0.53ng/ul m

response 2449

Ion	Exp%	Act%
276.00	100	100
138.00	23.90	2.08#
277.00	24.50	1.31#
0.00	0.00	0.00

SJ
 03/13/17




Data Path : Z:\HPCHEM1\BNA_M\Data\BM031017\
Data File : BM009174.D
Acq On : 10 Mar 2017 13:58
Operator : SJ/MA
Sample : I2062-22
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AK8

Manual Integrations
APPROVED

mohammad
3/13/2017 2:13:28 PM

Quant Time: Mar 10 15:51:15 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 10 15:19:24 2017
Response via : Initial Calibration

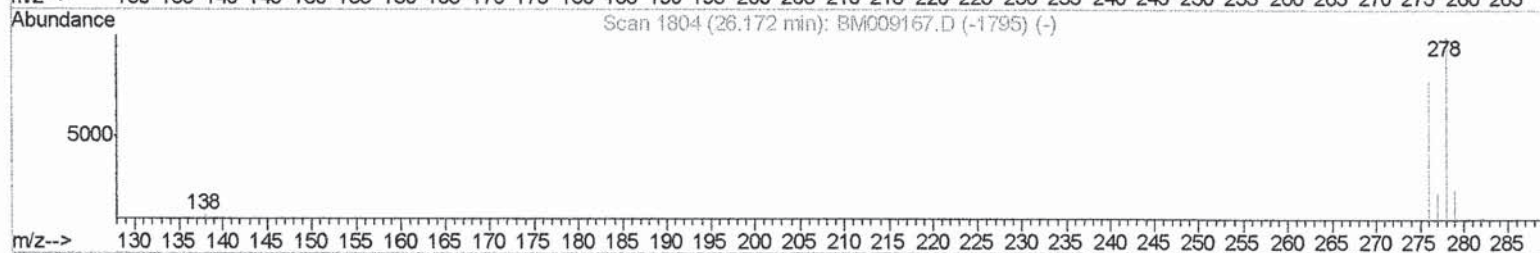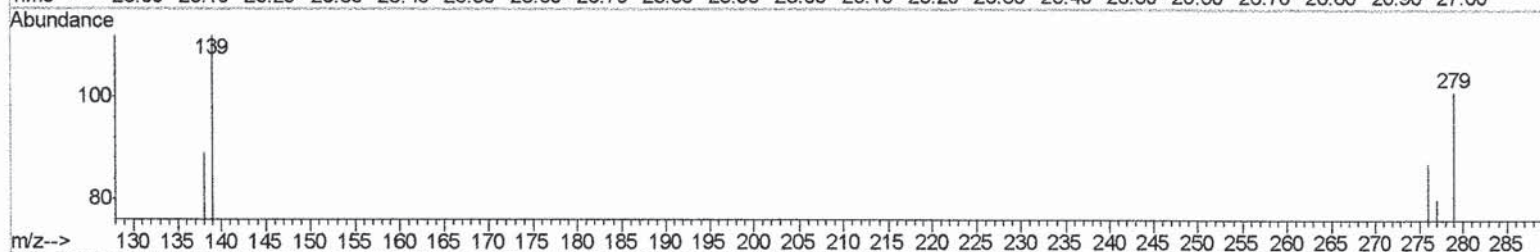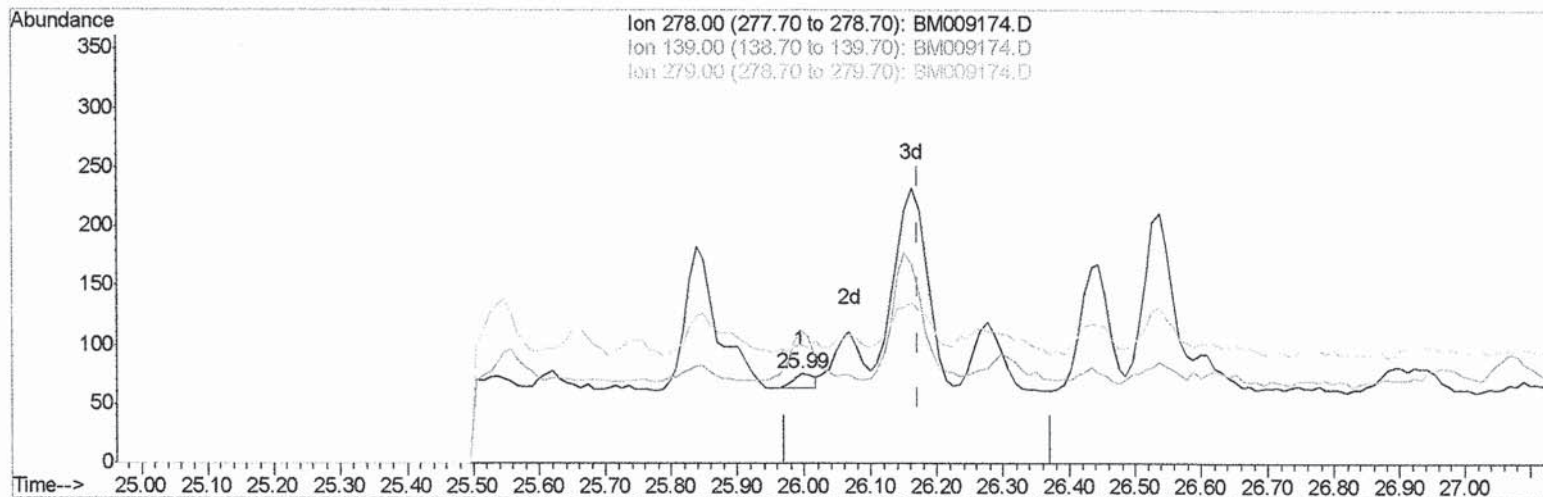

TIC: BM009174.D

(25) Dibenzo(a,h)anthracene

25.995min (-0.177) 0.01ng/ul

response 26

Ion	Exp%	Act%
278.00	100	100
139.00	21.70	147.37#
279.00	32.40	132.89#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM031017\
 Data File : BM009174.D
 Acq On : 10 Mar 2017 13:58
 Operator : SJ/MA
 Sample : I2062-22
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampled :
 C0AK8

Manual Integrations
 APPROVED

mohammad
 3/13/2017 2:13:28 PM

Quant Time: Mar 10 15:51:15 2017
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030317.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Mar 10 15:19:24 2017
 Response via : Initial Calibration

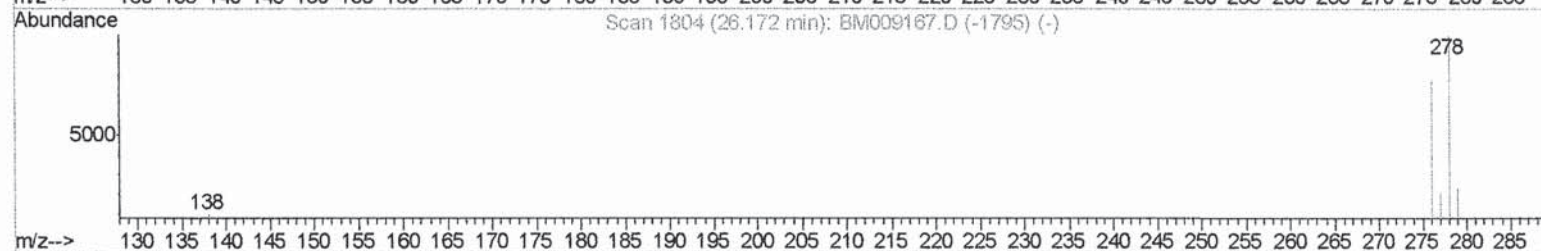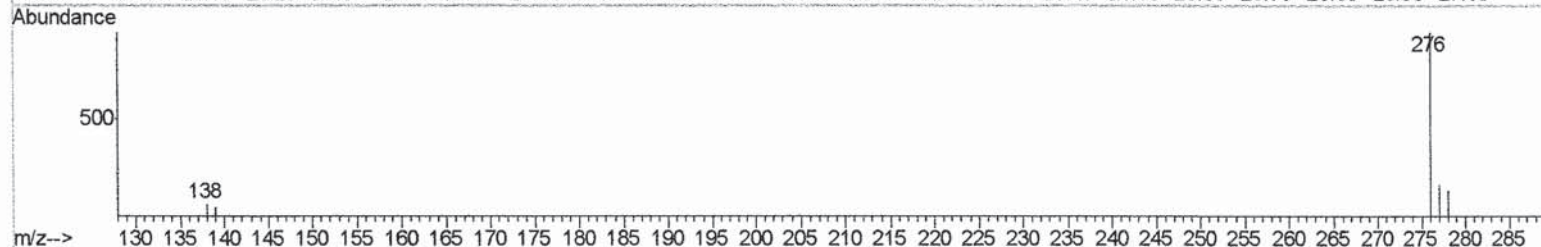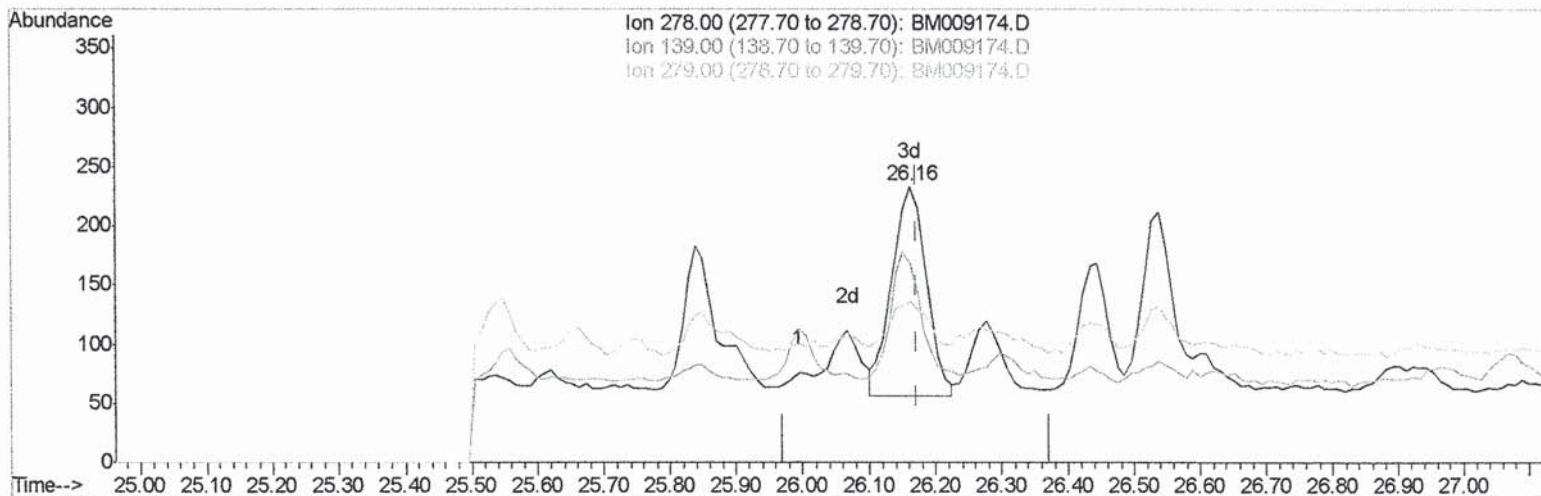

TIC: BM009174.D

(25) Dibenzo(a,h)anthracene

26.162min (-0.010) 0.16ng/ul m

response 640

Ion	Exp%	Act%
278.00	100	100
139.00	21.70	72.10#
279.00	32.40	58.80#
0.00	0.00	0.00

SJ
 03/13/17

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM031017\
 Data File : BM009174.D
 Acq On : 10 Mar 2017 13:58
 Operator : SJ/MA
 Sample : I2062-22
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AK8

Manual Integrations
 APPROVED

mohammad
 3/13/2017 2:13:28 PM

Quant Time: Mar 10 15:51:15 2017
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030317.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Mar 10 15:19:24 2017
 Response via : Initial Calibration

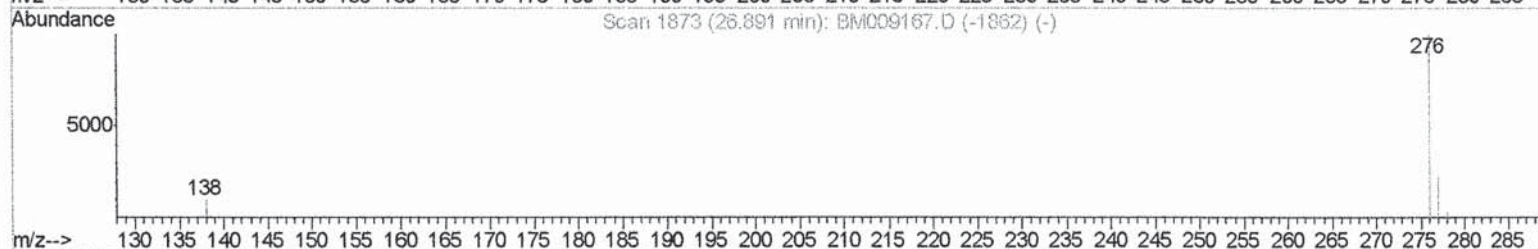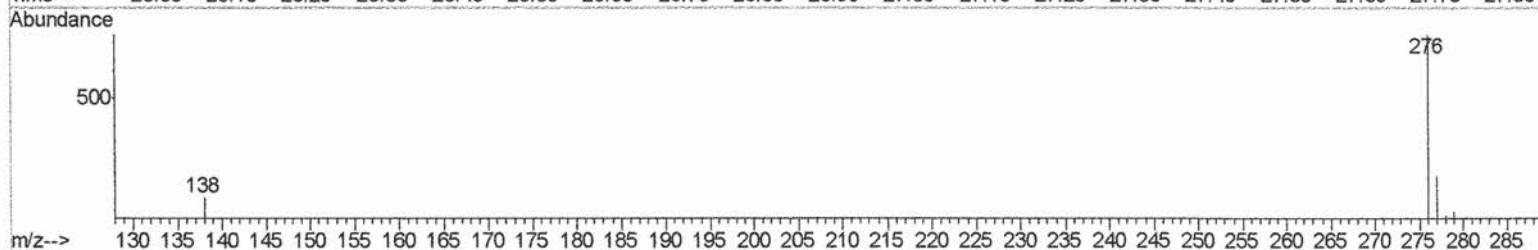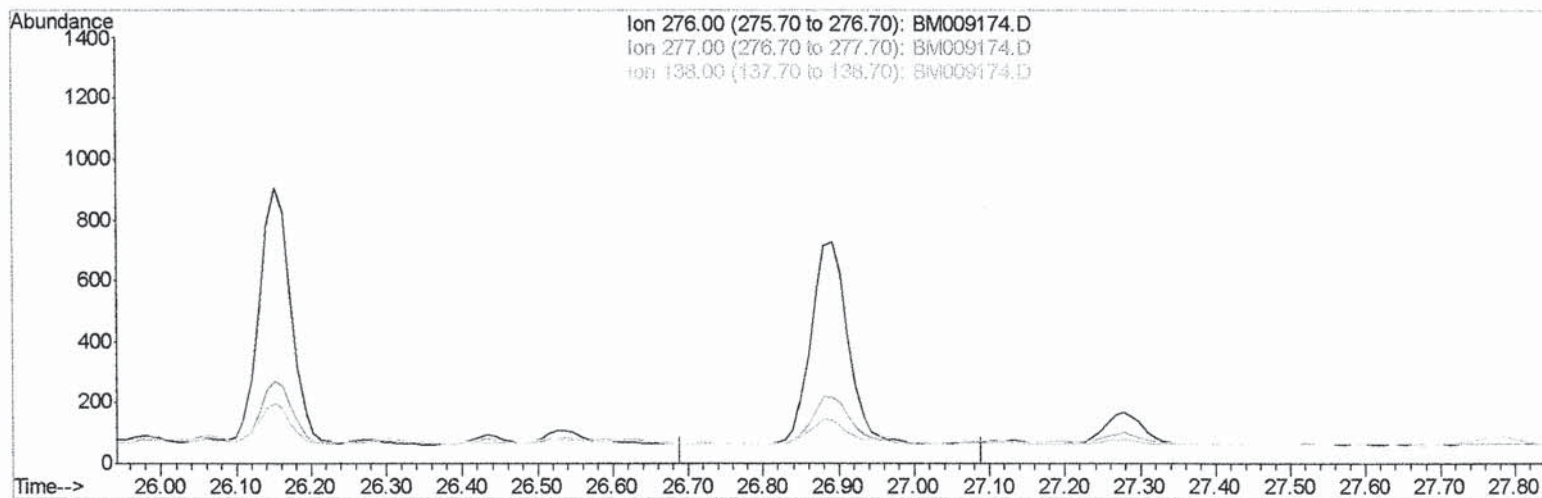

TIC: BM009174.D

(26) Benzo(g,h,i)perylene
 26.891min (-26.891) 0.00ng/ul
 response 0

Ion	Exp%	Act%
276.00	100	0.00
277.00	27.30	0.00#
138.00	25.60	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM031017\
 Data File : BM009174.D
 Acq On : 10 Mar 2017 13:58
 Operator : SJ/MA
 Sample : I2062-22
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AK8

Manual Integrations
 APPROVED

mohammad
 3/13/2017 2:13:28 PM

Quant Time: Mar 10 15:51:15 2017
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030317.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Mar 10 15:19:24 2017
 Response via : Initial Calibration

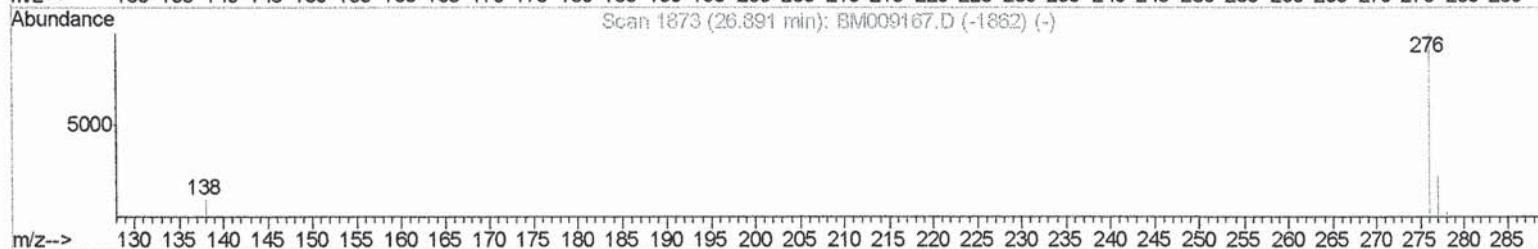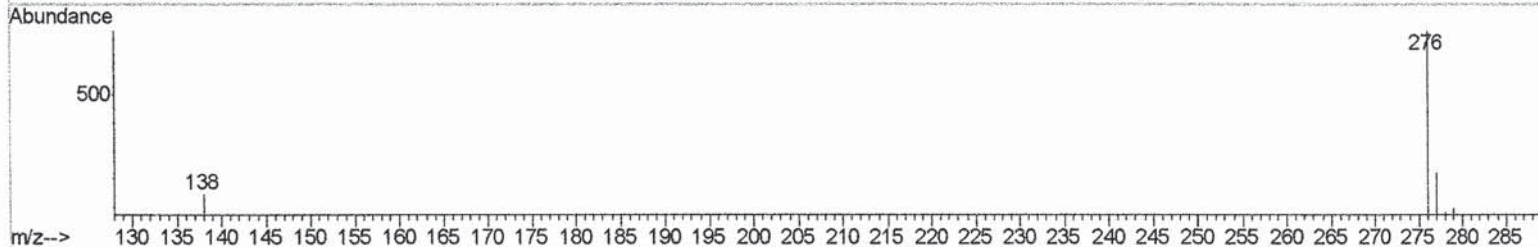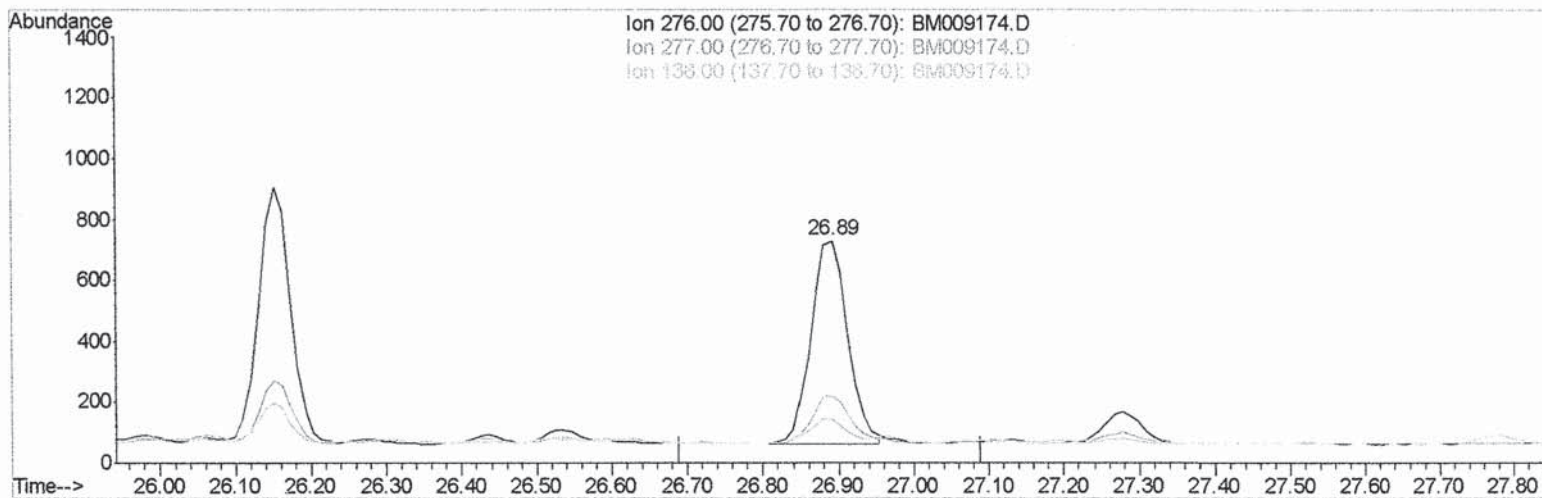

TIC: BM009174.D

(26) Benzo(g,h,i)perylene

26.891min (+0.000) 0.58ng/ul m

response 2278

Ion	Exp%	Act%
276.00	100	100
277.00	27.30	30.14
138.00	25.60	19.59#
0.00	0.00	0.00

SJ
 03/13/17

Data Path : Z:\HPCHEM1\BNA_M\Data\BM031017\
 Data File : BM009174.D
 Acq On : 10 Mar 2017 13:58
 Operator : SJ/MA
 Sample : I2062-22
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AK8

Manual Integrations
 APPROVED

mohammad
 3/13/2017 2:13:28 PM

Quant Time: Mar 10 15:54:13 2017
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM030317.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Mar 10 15:19:24 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.88	152	264	0.40	ng/ul	0.00
2) Naphthalene-d8	10.68	136	830	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.52	164	491	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.26	188	1098m	0.40	ng/ul	0.00
16) Chrysene-d12	21.44	240	1194	0.40	ng/ul	0.00
20) Perylene-d12	23.77	264	1028m	0.40	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	12.27	152	277	0.20	ng/ul	0.00
14) Fluoranthene-d10	19.29	212	769	0.22	ng/ul	0.00

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
3) Naphthalene	10.73	128	1315	0.55	ng/ul	96
5) 2-Methylnaphthalene	12.34	142	1256	0.73	ng/ul	100
7) Acenaphthylene	14.23	152	253	0.10	ng/ul#	41
8) Acenaphthene	14.57	153	70	0.04	ng/ul#	79
12) Phenanthrene	17.30	178	2444	0.71	ng/ul	98
13) Anthracene	17.40	178	262	0.08	ng/ul#	63
15) Fluoranthene	19.33	202	5804	1.29	ng/ul	94
17) Pyrene	19.69	202	5036	1.23	ng/ul	95
18) Benzo(a)anthracene	21.42	228	2557	0.64	ng/ul	94
19) Chrysene	21.47	228	3600m	0.96	ng/ul	
21) Benzo(b)fluoranthene	23.07	252	5627m	1.39	ng/ul	
22) Benzo(k)fluoranthene	23.11	252	1394m	0.39	ng/ul	
23) Benzo(a)pyrene	23.67	252	3276m	0.90	ng/ul	
24) Indeno(1,2,3-cd)pyrene	26.15	276	2449m	0.53	ng/ul	
25) Dibenzo(a,h)anthracene	26.16	278	640m	0.16	ng/ul	
26) Benzo(g,h,i)perylene	26.89	276	2278m	0.58	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed