


Data Path : Z:\HPCHEM1\BNA M\DATA\BM031017\
Data File : BM009190.D
Acq On : 11 Mar 2017 00:08
Operator : SJ/MA
Sample : I2072-03
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AK0

Manual Integrations
APPROVED

mohammad
3/13/2017 2:14:30 PM

Quant Time: Mar 11 03:44:51 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Mar 11 02:23:19 2017
Response via : Initial Calibration

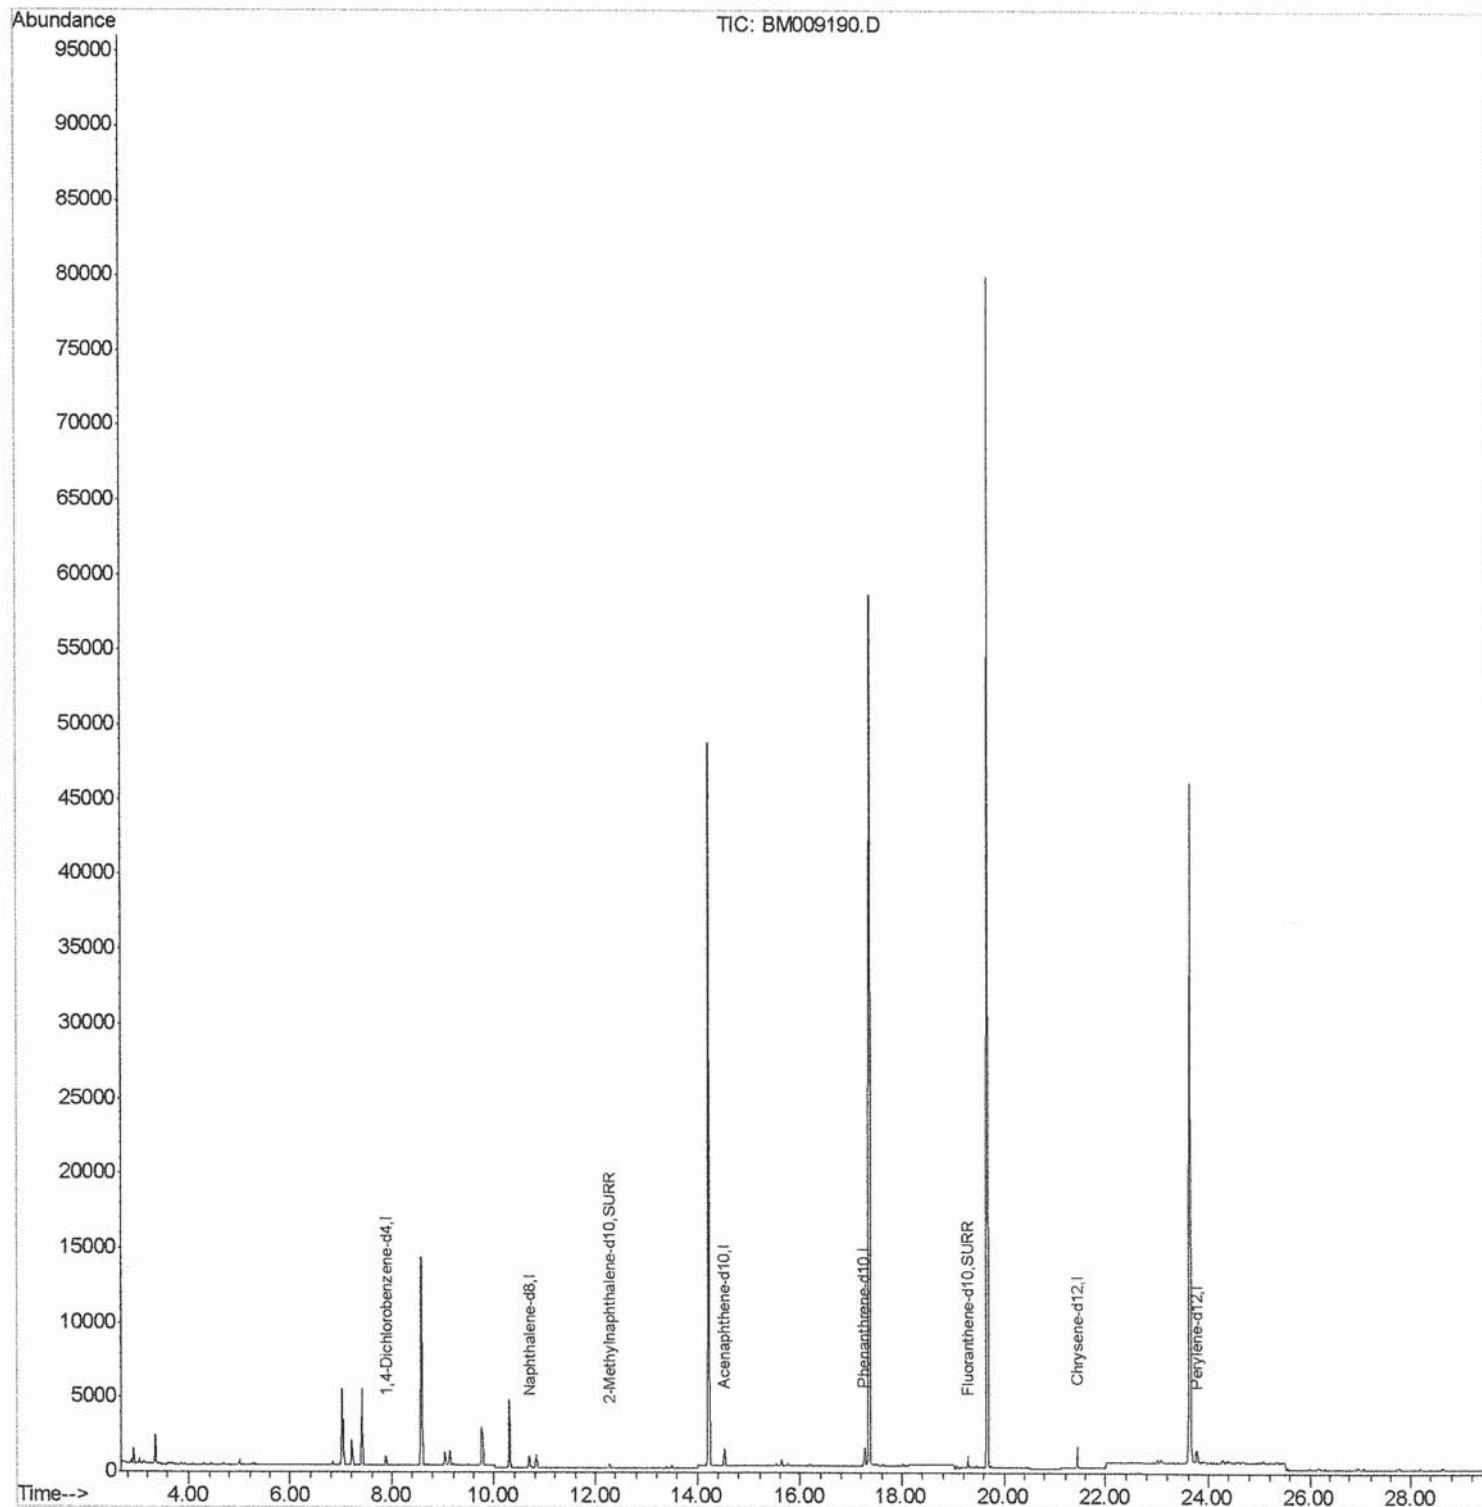




Data Path : Z:\HPCHEM1\BNA M\DATA\BM031017\
Data File : BM009190.D
Acq On : 11 Mar 2017 00:08
Operator : SJ/MA
Sample : I2072-03
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AK0

Manual Integrations
APPROVED

mohammad
3/13/2017 2:14:30 PM

Quant Time: Mar 11 03:41:22 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Mar 11 02:23:19 2017
Response via : Initial Calibration

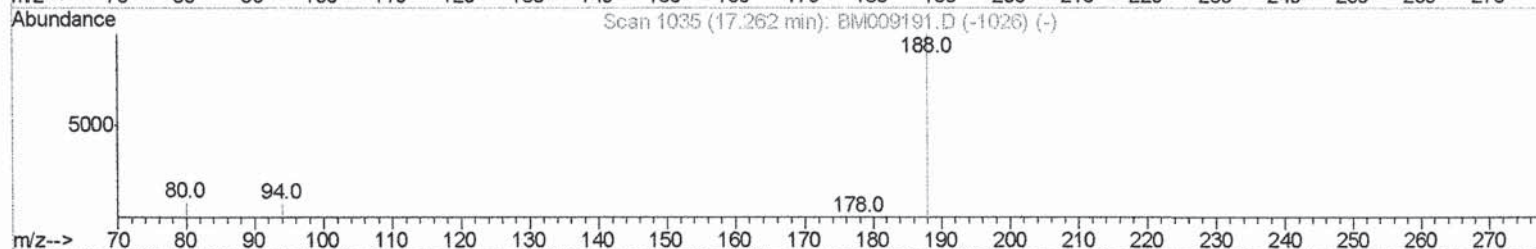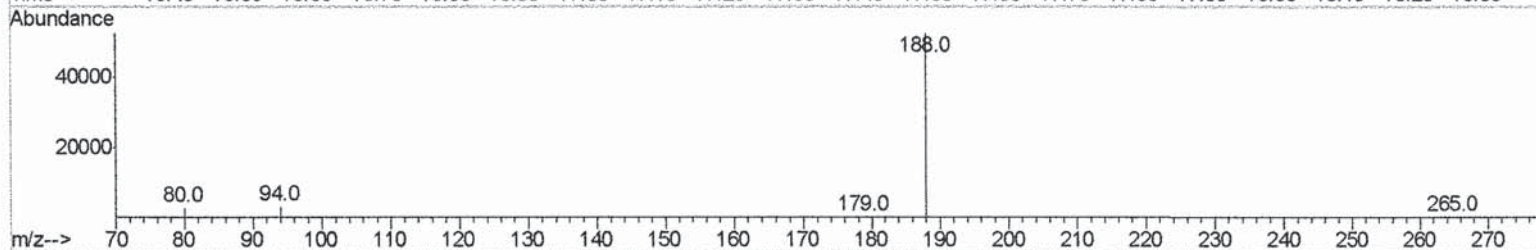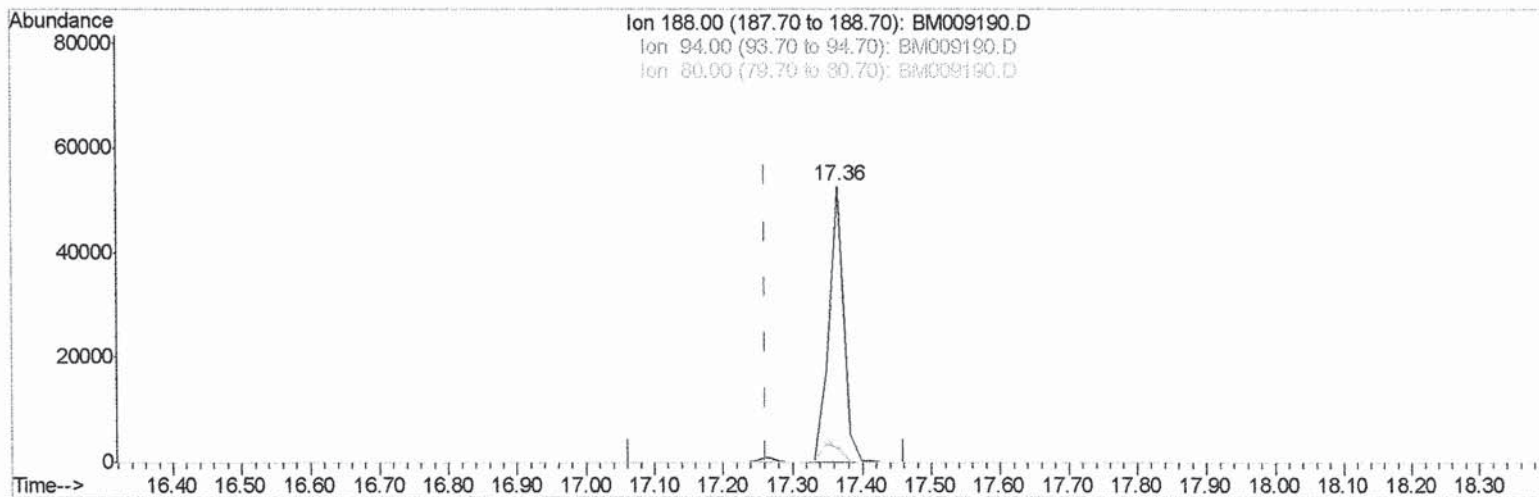

TIC: BM009190.D

(10) Phenanthrene-d10 (I)

17.365min (+0.103) 0.40ng/ul

response 77500

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	5.62#
80.00	11.80	5.13#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA M\DATA\BM031017\
 Data File : BM009190.D
 Acq On : 11 Mar 2017 00:08
 Operator : SJ/MA
 Sample : I2072-03
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AK0

Manual Integrations
 APPROVED

mohammad
 3/13/2017 2:14:30 PM

Quant Time: Mar 11 03:41:22 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030317.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Mar 11 02:23:19 2017
 Response via : Initial Calibration

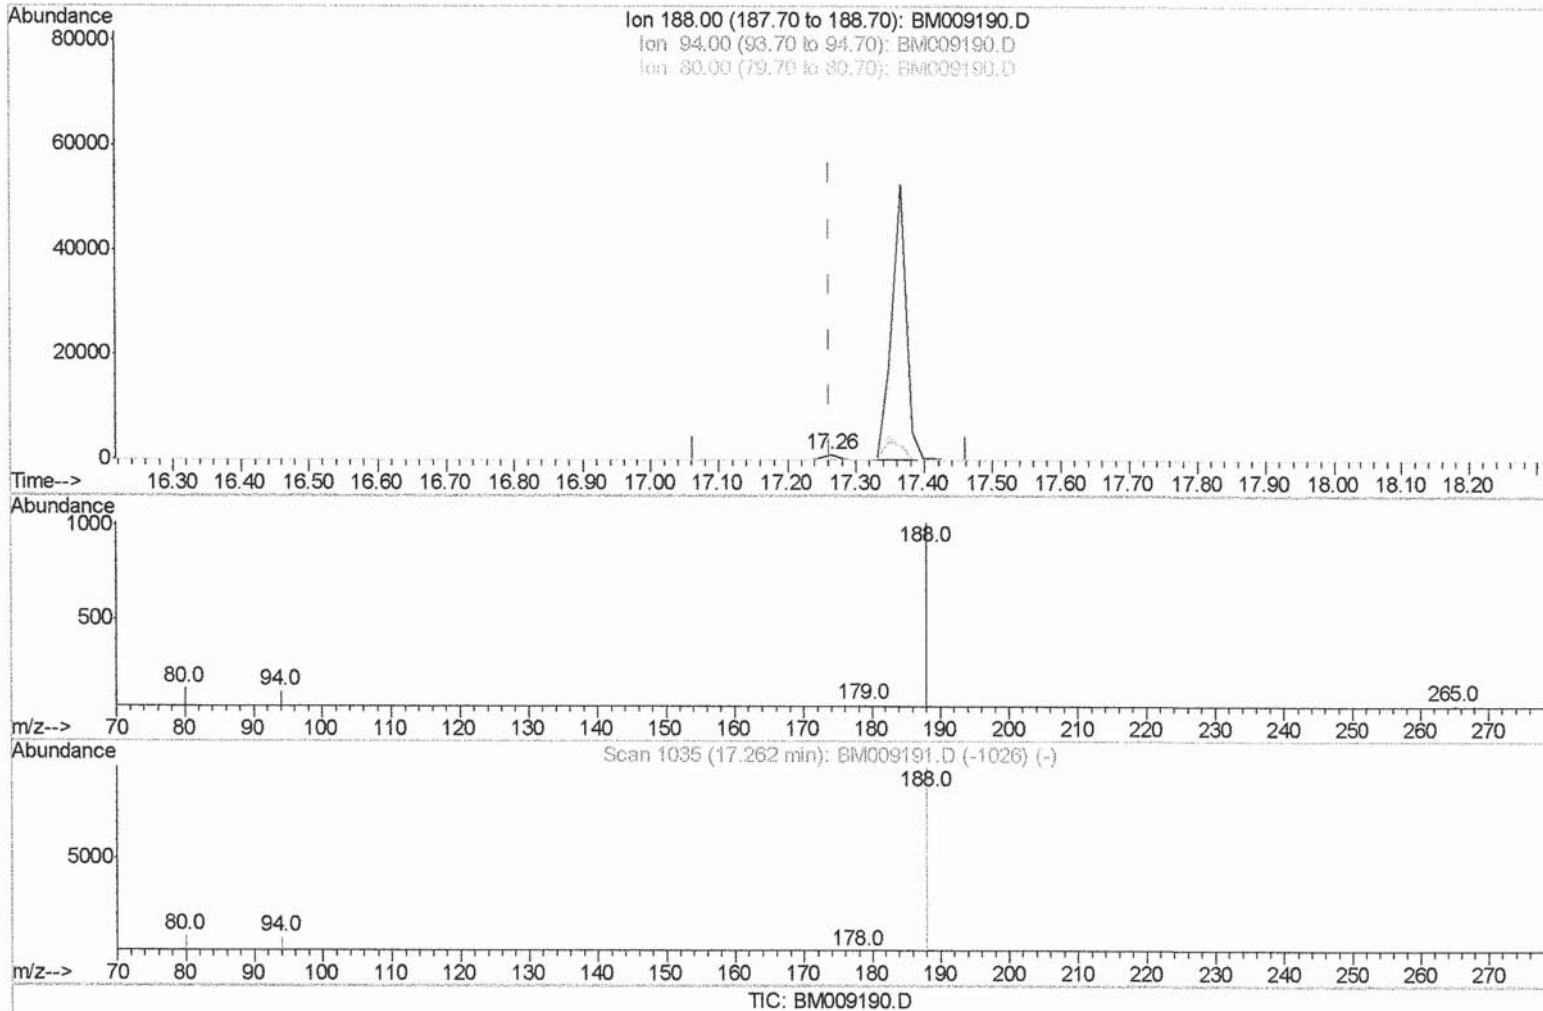

(10) Phenanthrene-d10 (I)

17.262min (+0.000) 0.40ng/ul m

response 1449

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	11.97
80.00	11.80	13.55
0.00	0.00	0.00

SJ
 03/13/17




Data Path : Z:\HPCHEM1\BNA M\DATA\BM031017\
Data File : BM009190.D
Acq On : 11 Mar 2017 00:08
Operator : SJ/MA
Sample : I2072-03
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AK0

Manual Integrations
APPROVED

mohammad
3/13/2017 2:14:30 PM

Quant Time: Mar 11 03:41:22 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Mar 11 02:23:19 2017
Response via : Initial Calibration

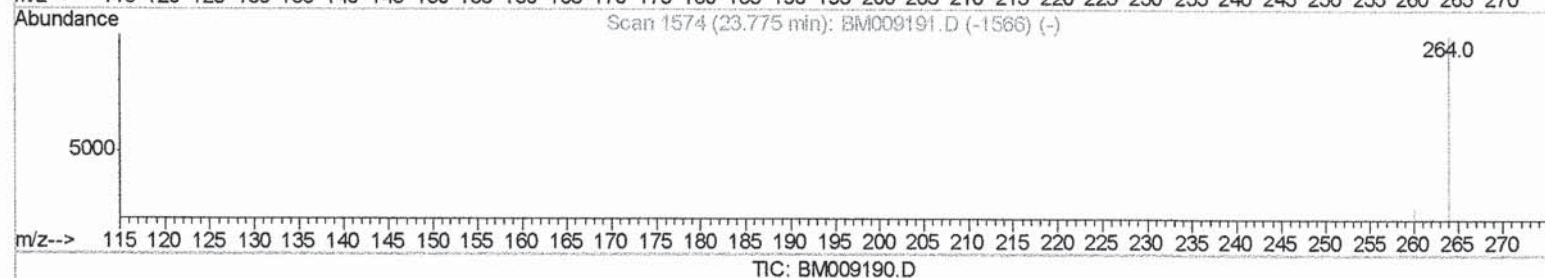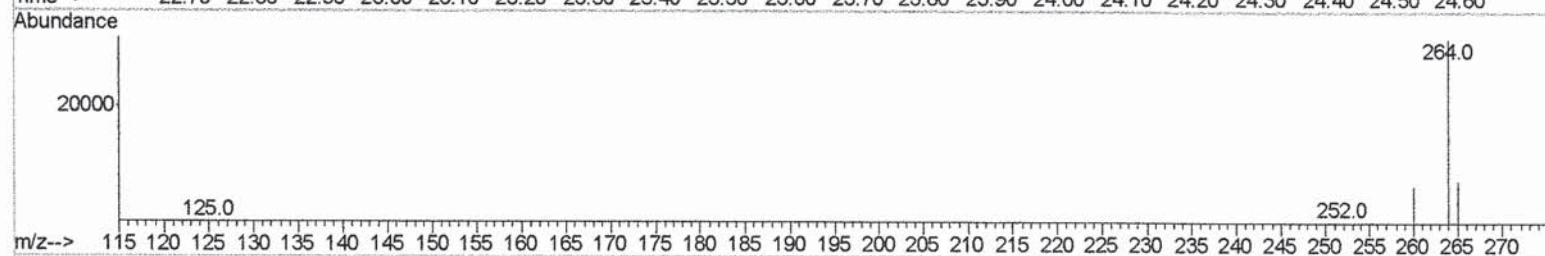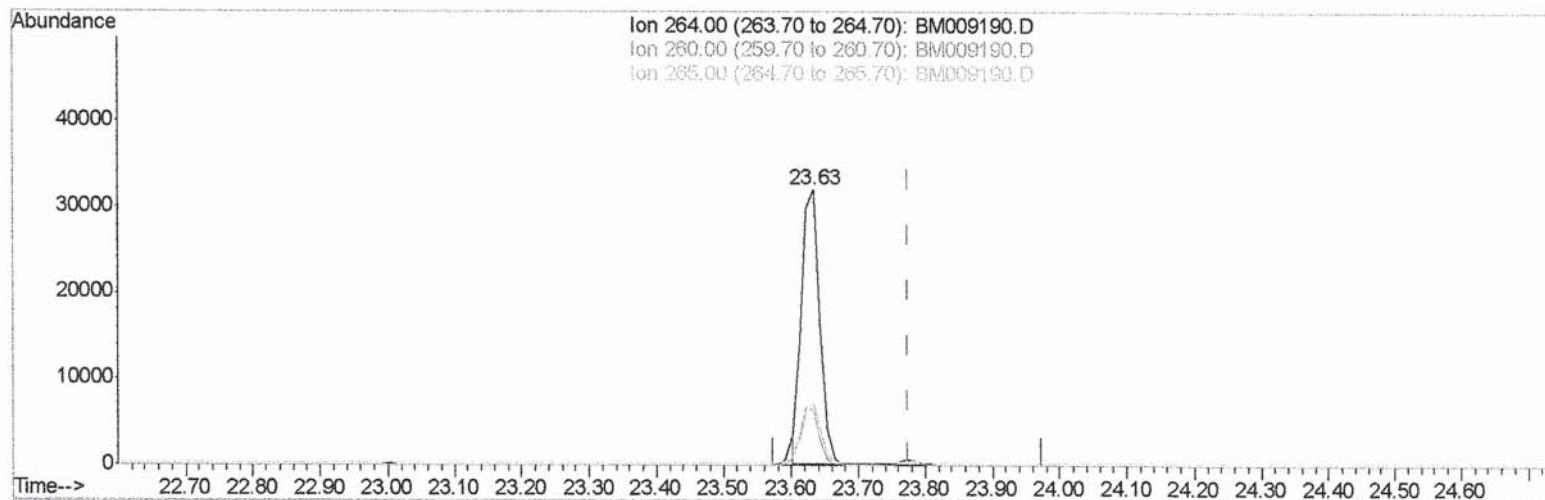

(20) Perylene-d12 (I)

23.632min (-0.142) 0.40ng/ul

response 60481

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	19.97#
265.00	103.50	22.75#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA M\DATA\BM031017\
 Data File : BM009190.D
 Acq On : 11 Mar 2017 00:08
 Operator : SJ/MA
 Sample : I2072-03
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AK0

Manual Integrations
 APPROVED

mohammad
 3/13/2017 2:14:30 PM

Quant Time: Mar 11 03:41:22 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030317.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Mar 11 02:23:19 2017
 Response via : Initial Calibration

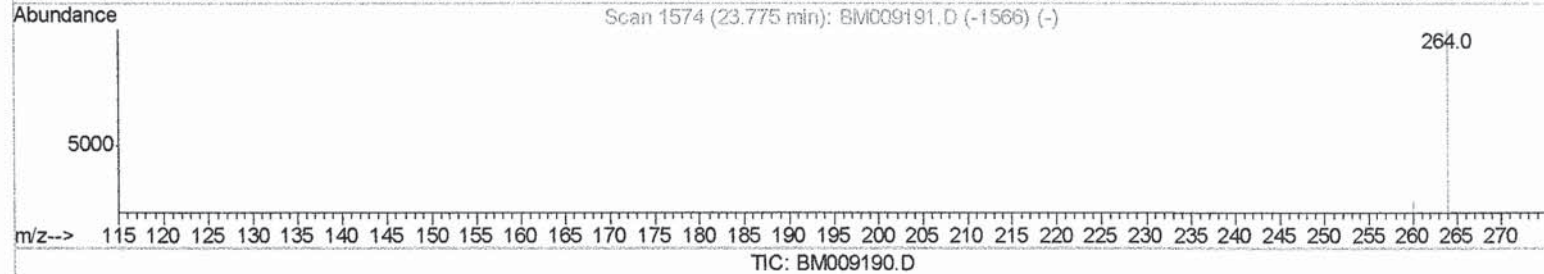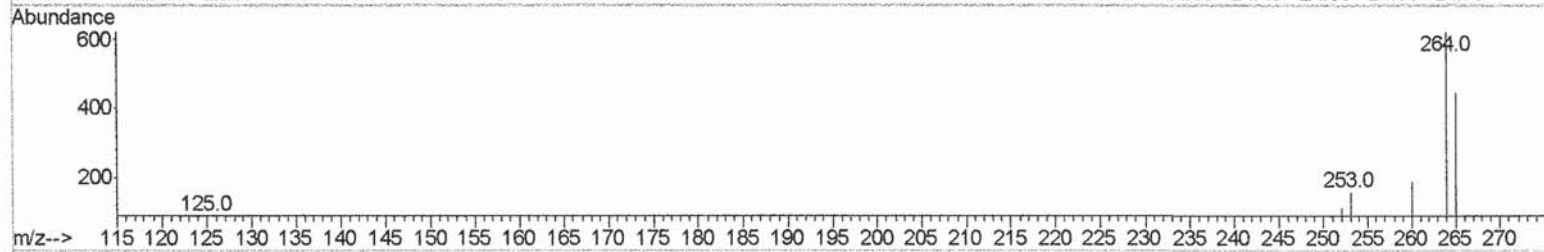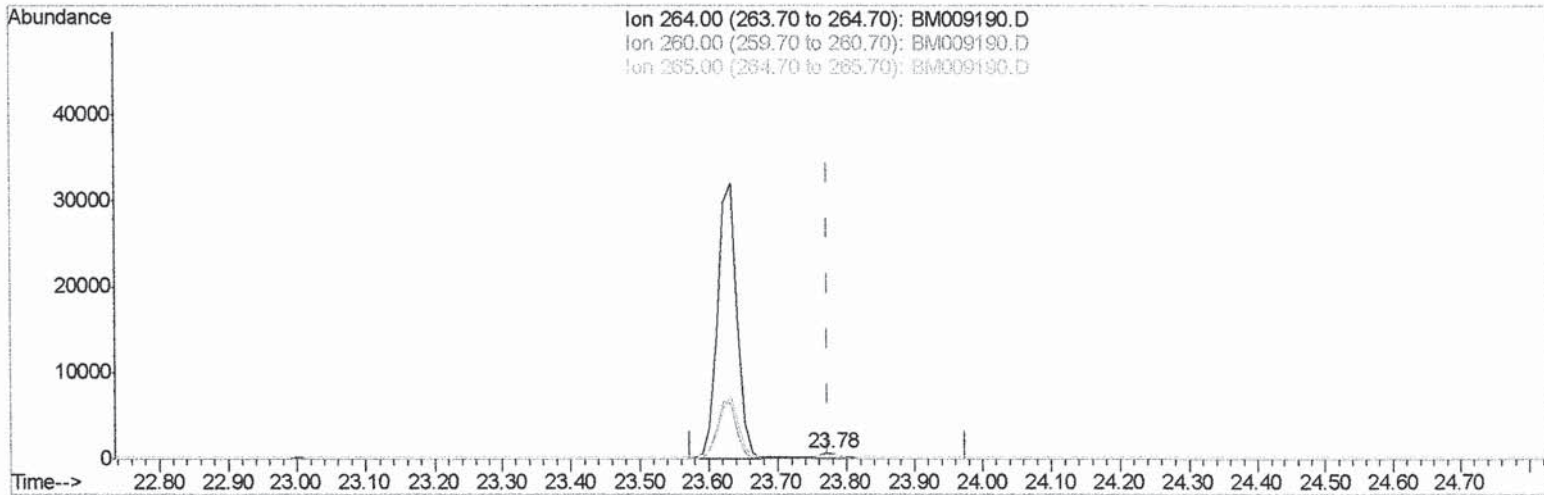

(20) Perylene-d12 (I)

23.778min (+0.003) 0.40ng/ul m

response 1214

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	30.60
265.00	103.50	71.18#
0.00	0.00	0.00

JJ
03/13/17

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA M\DATA\BM031017\
 Data File : BM009190.D
 Acq On : 11 Mar 2017 00:08
 Operator : SJ/MA
 Sample : I2072-03
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_M
ClientSampleId :
 C0AK0

Manual Integrations
APPROVED

mohammad
 3/13/2017 2:14:30 PM

Quant Time: Mar 11 03:42:53 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030317.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Mar 11 02:23:19 2017
 Response via : Initial Calibration

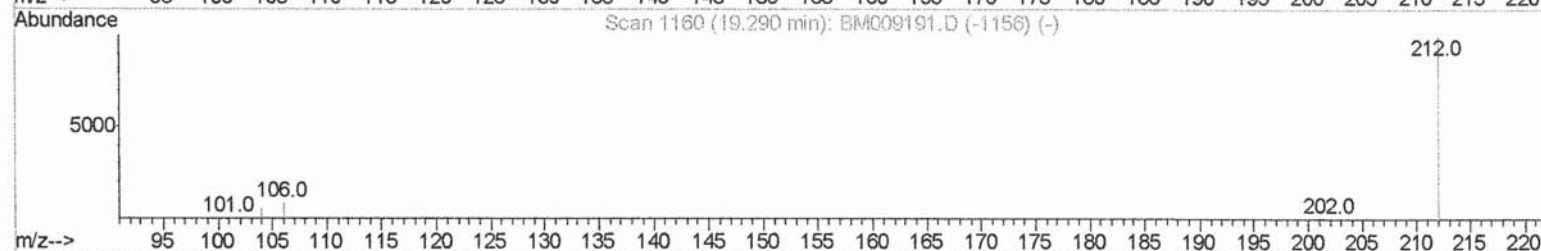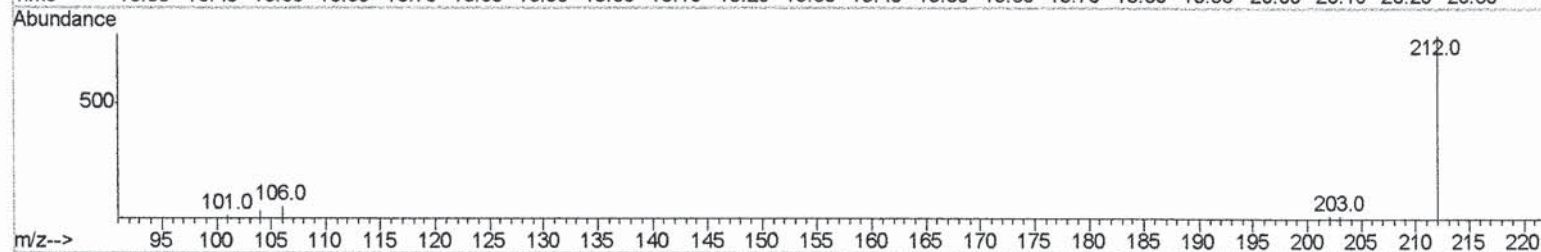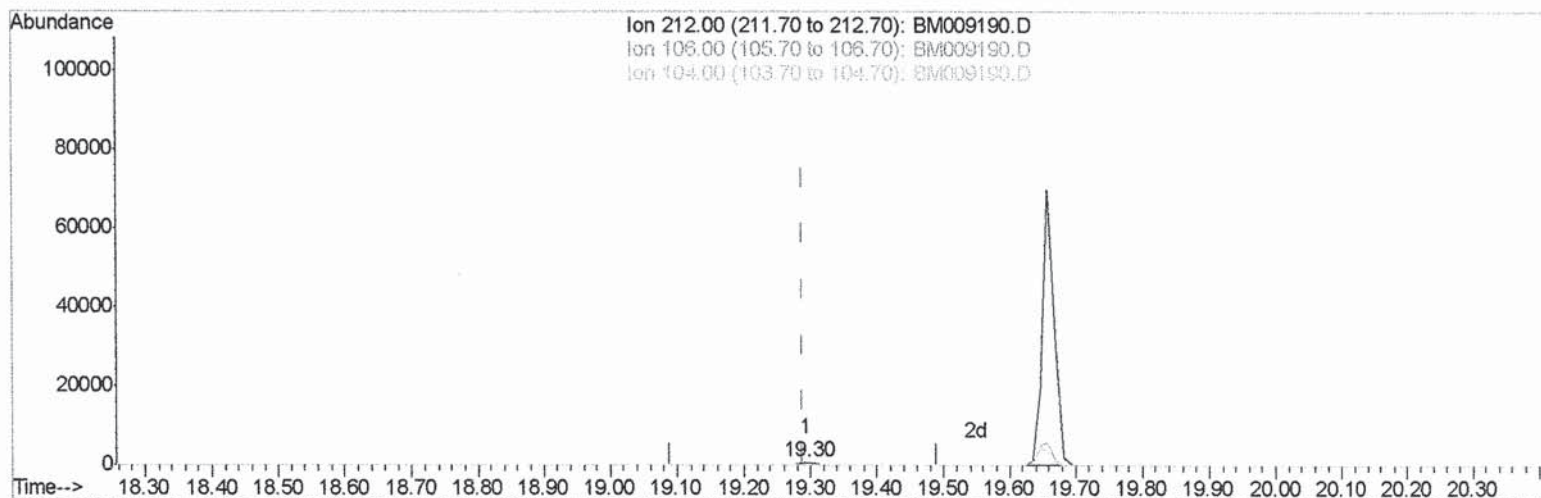

TIC: BM009190.D

(14) Fluoranthene-d10 (SURR)

19.295min (+0.005) 0.21ng/ul

response 961

Ion	Exp%	Act%
212.00	100	100
106.00	18.30	9.47#
104.00	15.60	5.72#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA M\DATA\BM031017\
 Data File : BM009190.D
 Acq On : 11 Mar 2017 00:08
 Operator : SJ/MA
 Sample : I2072-03
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AK0

Manual Integrations
 APPROVED

mohammad
 3/13/2017 2:14:30 PM

Quant Time: Mar 11 03:42:53 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030317.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Mar 11 02:23:19 2017
 Response via : Initial Calibration

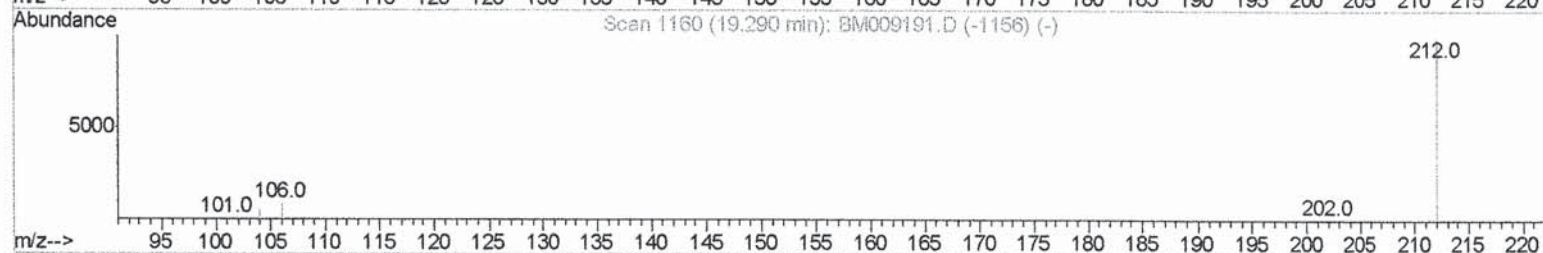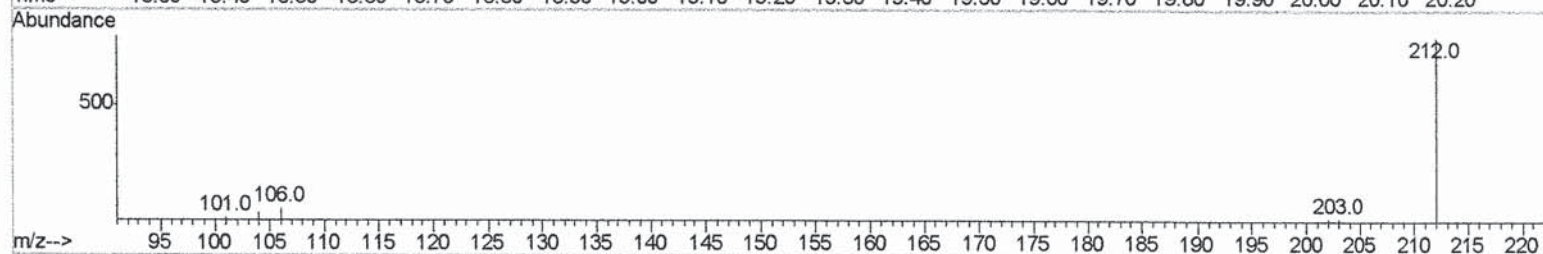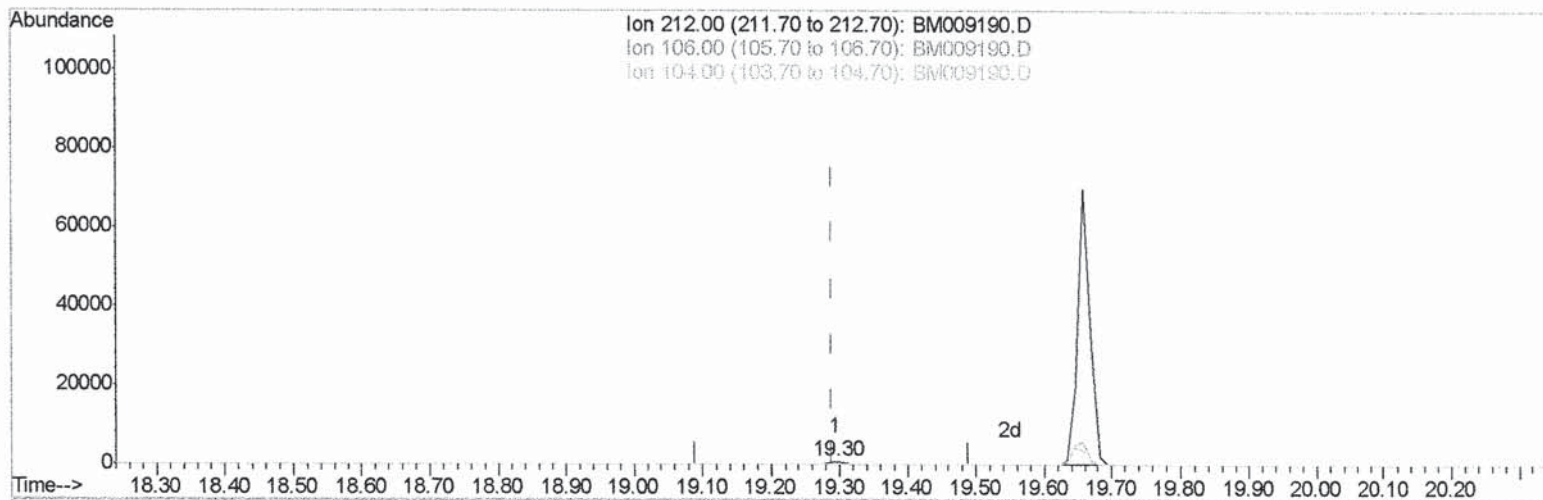

TIC: BM009190.D

(14) Fluoranthene-d10 (SURR)

19.295min (+0.005) 0.22ng/ul m

response 982

Ion	Exp%	Act%
212.00	100	100
106.00	18.30	9.27#
104.00	15.60	5.60#
0.00	0.00	0.00

SJ
03/13/17

Data Path : Z:\HPCHEM1\BNA M\DATA\BM031017\
Data File : BM009190.D
Acq On : 11 Mar 2017 00:08
Operator : SJ/MA
Sample : I2072-03
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AK0

Manual Integrations
APPROVED

mohammad
3/13/2017 2:14:30 PM

Quant Time: Mar 11 03:44:51 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Mar 11 02:23:19 2017
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Dichlorobenzene-d4	7.88	152	304	0.40	ng/ul	0.00
2) Naphthalene-d8	10.68	136	983	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.52	164	604	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.26	188	1449m	0.40	ng/ul	0.00
16) Chrysene-d12	21.44	240	1413	0.40	ng/ul	0.00
20) Perylene-d12	23.78	264	1214m	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.27	152	363	0.22	ng/ul	0.00
14) Fluoranthene-d10	19.30	212	982m	0.22	ng/ul	0.00

Target Compounds Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

SS
03/13/17
SS
03/13/17